
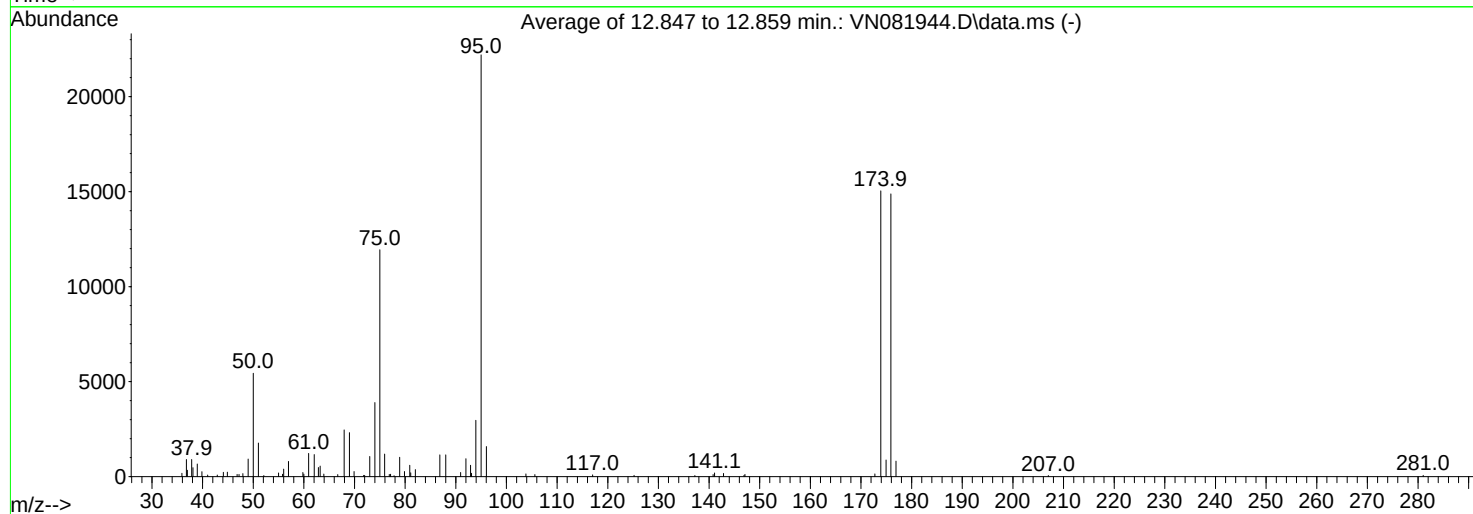


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050124\
Data File : VN081944.D
Acq On : 01 May 2024 09:04
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Title : SW846 8260
Last Update : Fri Apr 26 05:26:49 2024

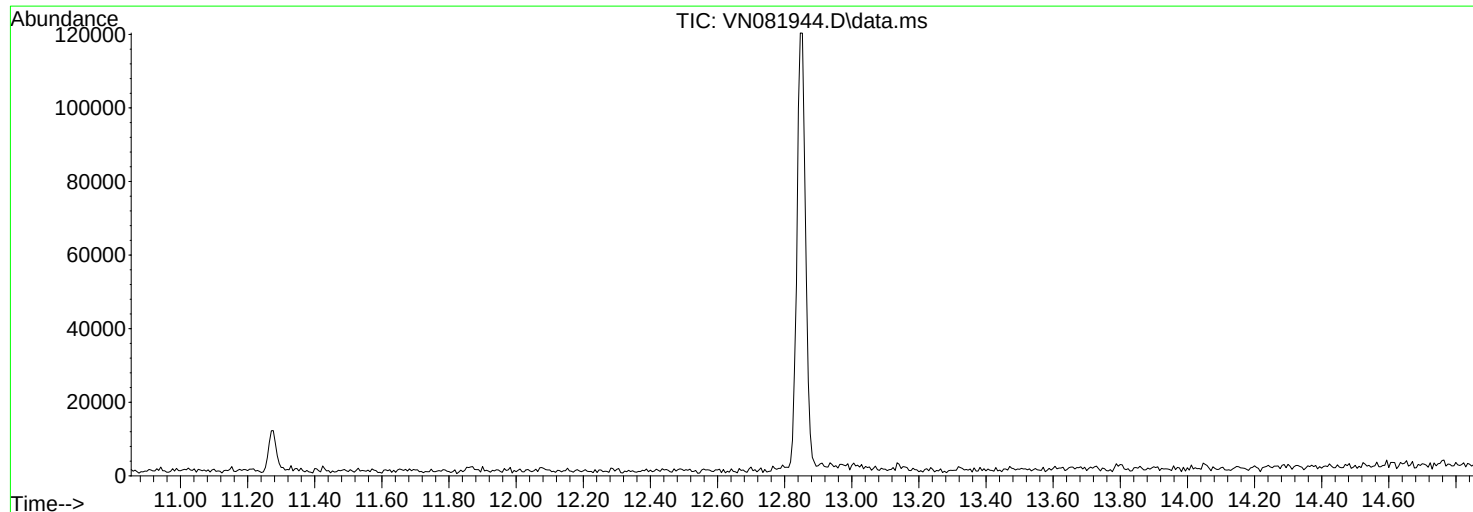

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1842

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.5	5440	PASS
75	95	30	60	53.8	11941	PASS
95	95	100	100	100.0	22200	PASS
96	95	5	9	7.1	1585	PASS
173	174	0.00	2	0.9	141	PASS
174	95	50	100	67.8	15044	PASS
175	174	5	9	5.8	877	PASS
176	174	95	101	98.9	14879	PASS
177	176	5	9	5.5	813	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	174	46.80	115	59.80	223	71.80	61
36.80	901	47.20	115	60.00	139	72.00	61
37.00	339	47.95	162	60.95	1221	73.00	106
37.85	903	49.00	924	62.05	1165	74.00	390
38.10	474	50.00	5440	62.85	483	75.00	11941
38.95	666	51.00	1771	63.20	552	75.95	1187
39.85	263	52.10	60	63.95	133	76.85	119
41.00	86	55.00	192	66.70	111	77.10	125
42.90	84	55.80	124	67.95	2456	77.80	54
44.10	225	56.00	398	69.00	2315	78.90	1021
44.90	239	56.95	801	69.90	271	79.85	266

Average of 12.847 to 12.859 min.: VN081944.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	596	96.05	1585	172.75	141		
81.10	203	103.85	140	173.90	15044		
82.00	373	105.60	111	174.95	877		
86.85	1147	117.00	93	175.90	14879		
88.00	1148	125.20	69	176.90	813		
90.95	219	137.20	59	207.00	61		
92.00	947	140.80	109	281.00	68		
92.90	595	141.10	191				
93.10	175	142.85	169				
93.95	2964	146.90	66				
95.00	22200	147.10	116				

Instrument :
MSVOA_N
ClientSampleId :
BFB