
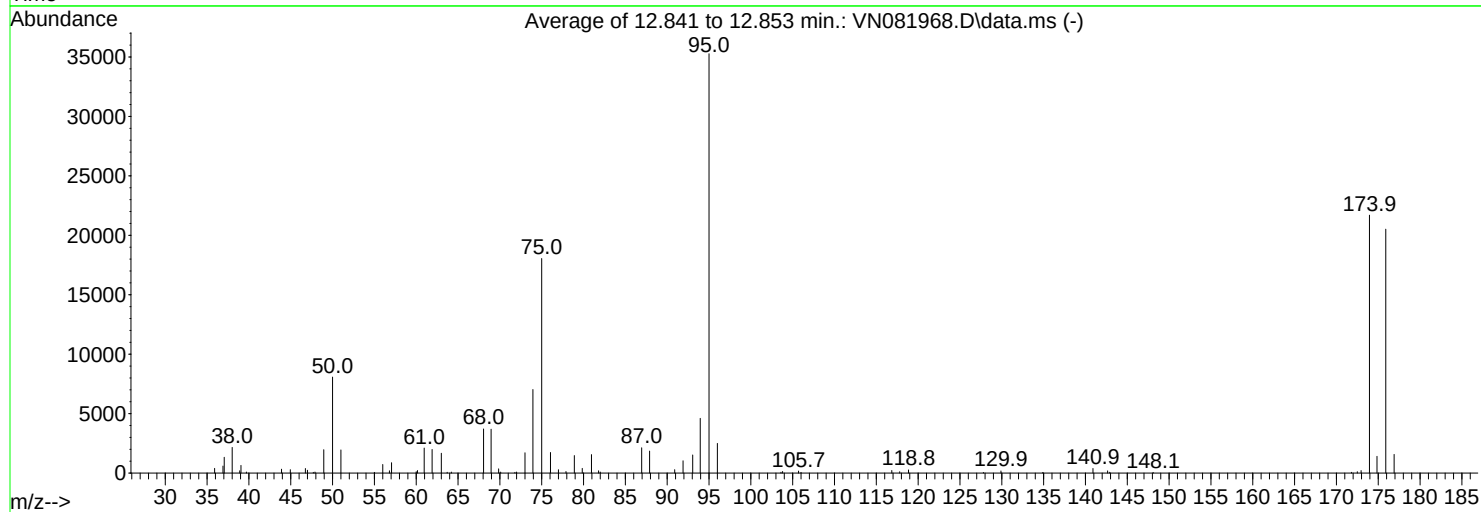


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050224\
Data File : VN081968.D
Acq On : 02 May 2024 08:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042624W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Apr 27 04:37:27 2024

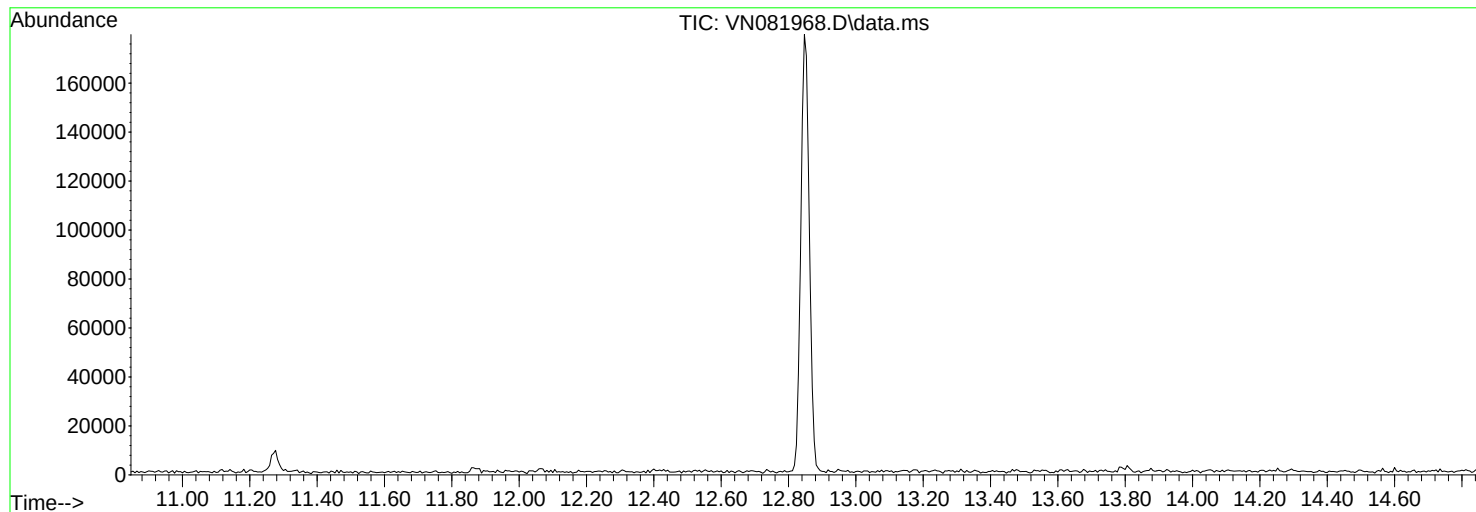

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	8076	PASS
75	95	30	60	51.2	18049	PASS
95	95	100	100	100.0	35275	PASS
96	95	5	9	7.1	2494	PASS
173	174	0.00	2	1.0	216	PASS
174	95	50	100	61.5	21696	PASS
175	174	5	9	6.5	1408	PASS
176	174	95	101	94.6	20517	FAIL*
177	176	5	9	7.7	1570	PASS