

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050225\
 Data File : VN086452.D
 Acq On : 02 May 2025 09:58
 Operator : JC\MD
 Sample : VN0502MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0502MBL01

Quant Time: May 02 23:14:11 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 16 04:19:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	152218	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	290230	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	265958	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	101992	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	108636	49.217	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	98.440%
35) Dibromofluoromethane	8.165	113	82323	61.116	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	122.240%
50) Toluene-d8	10.565	98	369820	51.371	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.740%
62) 4-Bromofluorobenzene	12.847	95	123889	47.182	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	94.360%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050225\
Data File : VN086452.D
Acq On : 02 May 2025 09:58
Operator : JC\MD
Sample : VN0502MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0502MBL01

Quant Time: May 02 23:14:11 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 16 04:19:23 2025
Response via : Initial Calibration




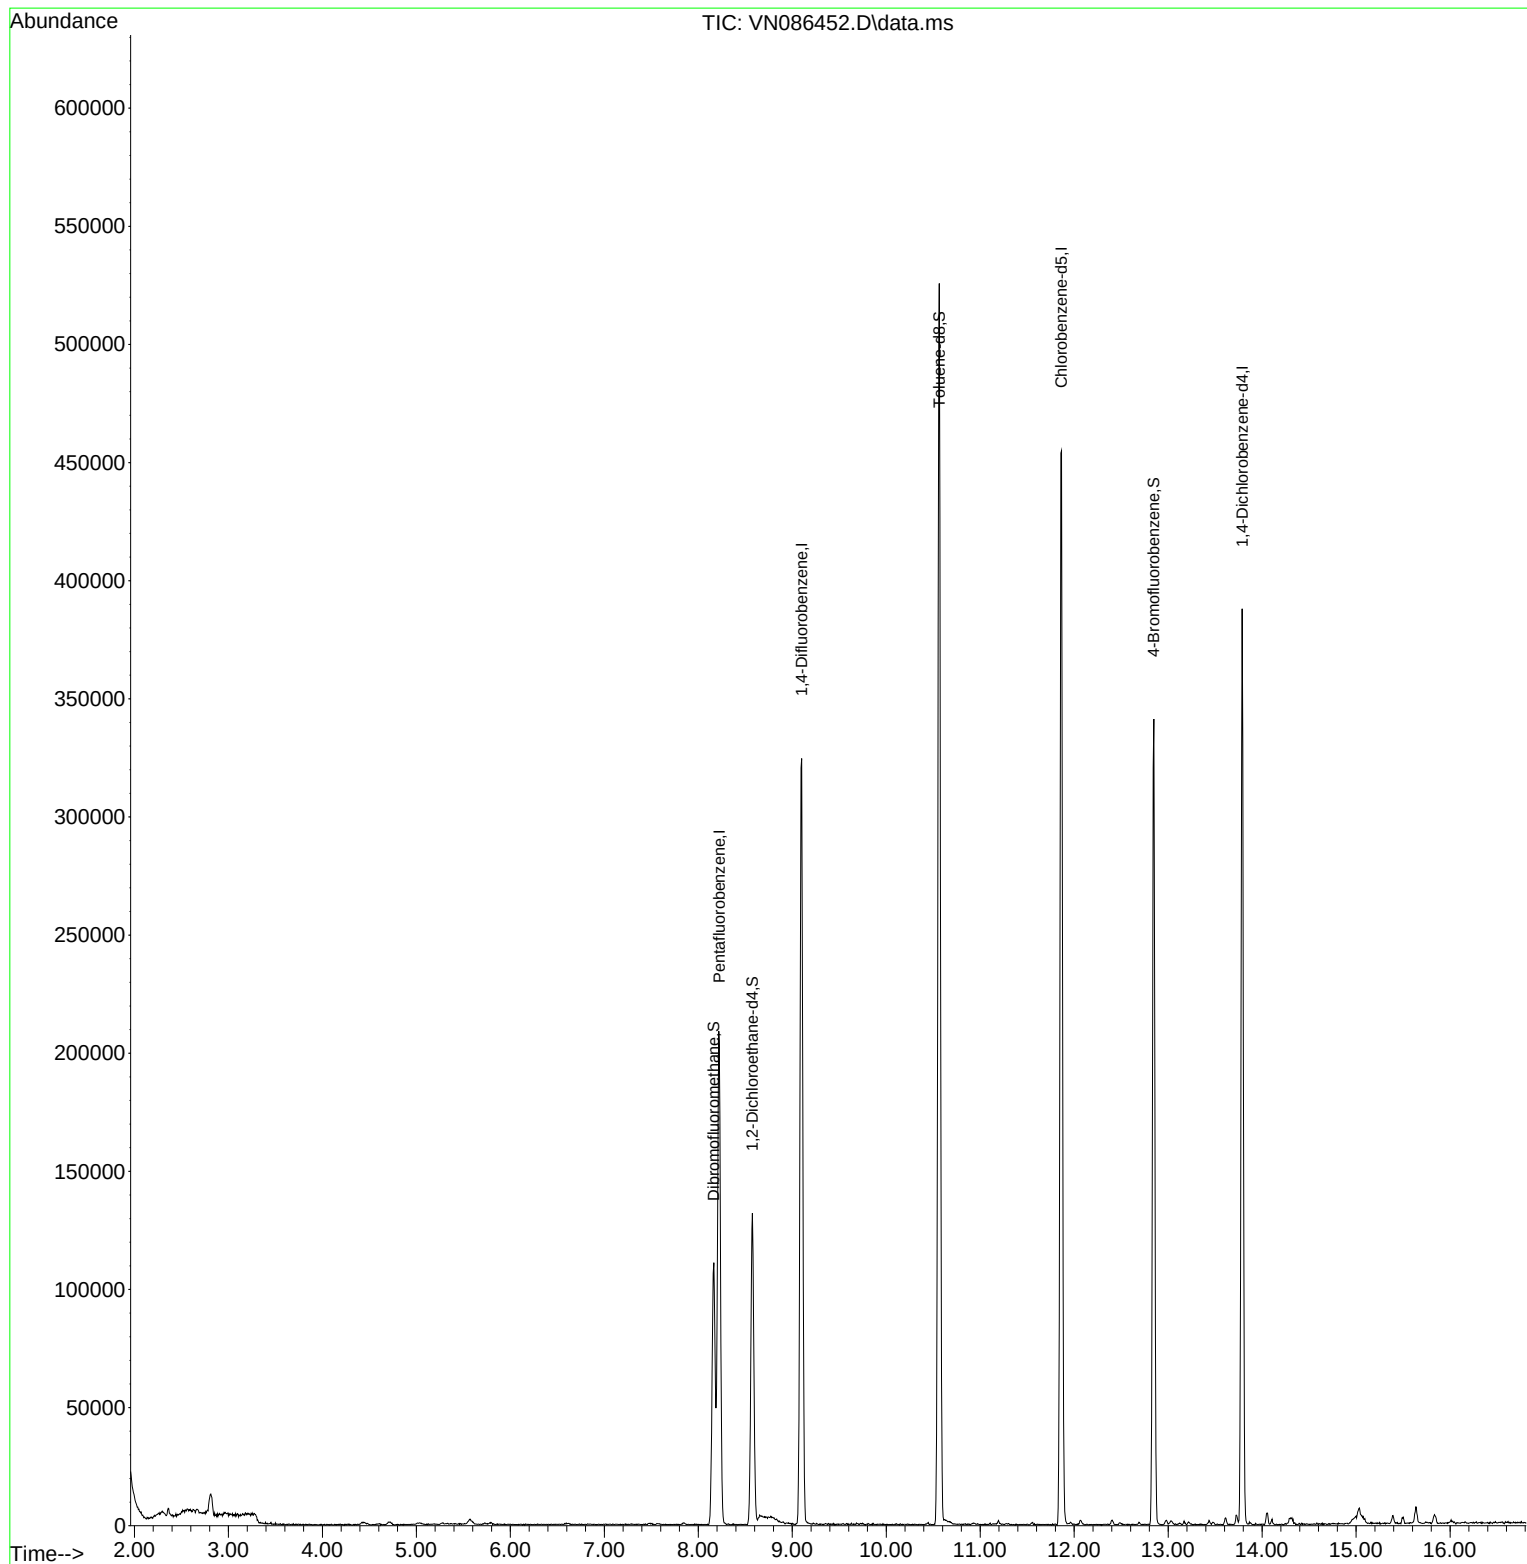


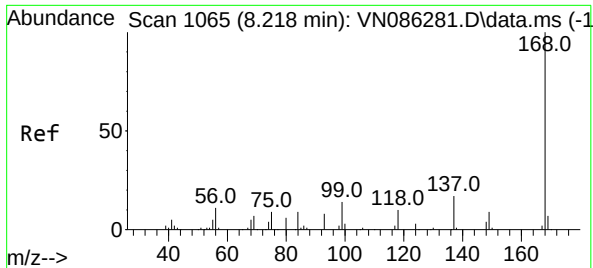

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN086452.D
Acq: 02 May 2025 09:58




Instrument :
MSVOA_N
ClientSampleId :
VN0502MBL01


Tgt Ion:168 Resp: 152218
Ion Ratio Lower Upper
168 100
99 60.1 52.5 78.7

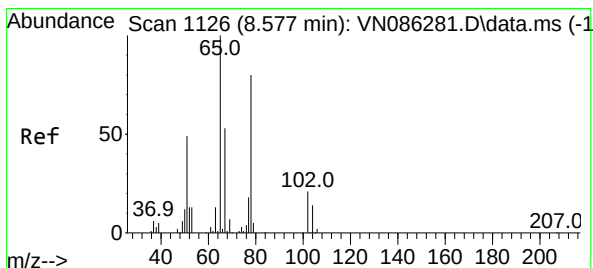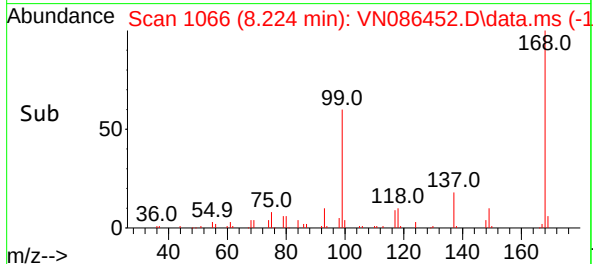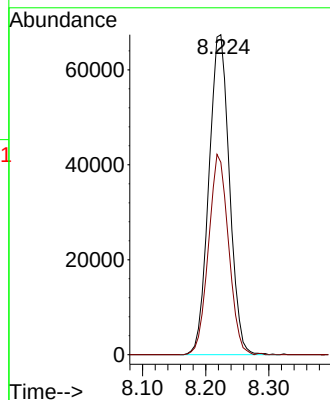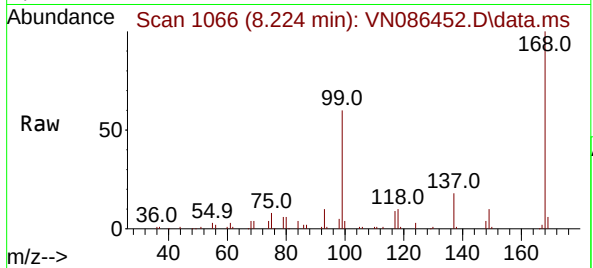

#33
1,2-Dichloroethane-d4
Concen: 49.217 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN086452.D
Acq: 02 May 2025 09:58

Tgt Ion: 65 Resp: 108636
Ion Ratio Lower Upper
65 100
67 52.0 0.0 106.0


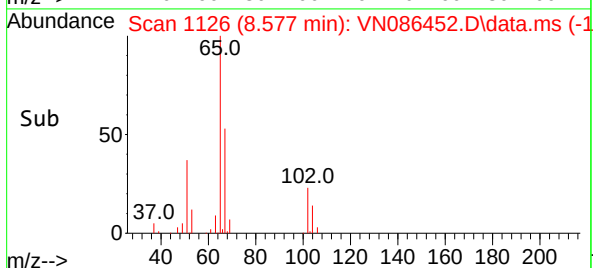
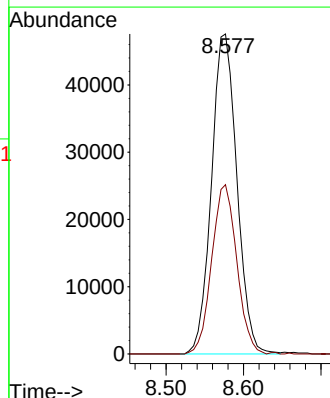
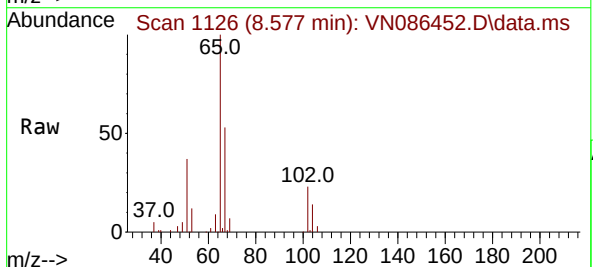


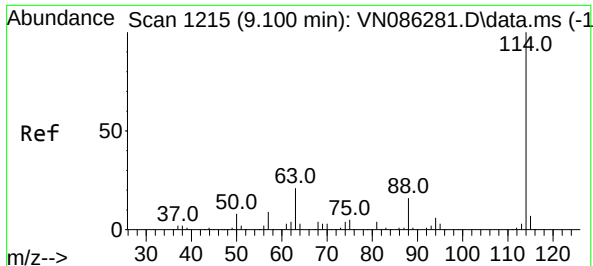

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN086452.D
Acq: 02 May 2025 09:58




Instrument :
MSVOA_N
ClientSampleId :
VN0502MBL01


Tgt Ion:114 Resp: 290230
Ion Ratio Lower Upper
114 100
63 21.1 0.0 42.6
88 15.2 0.0 31.8

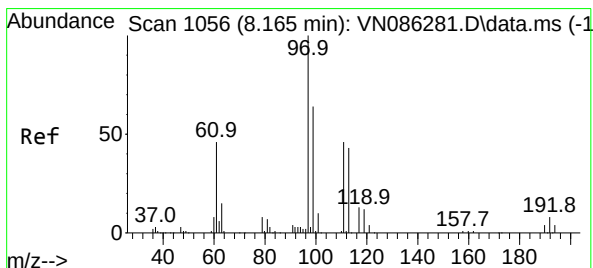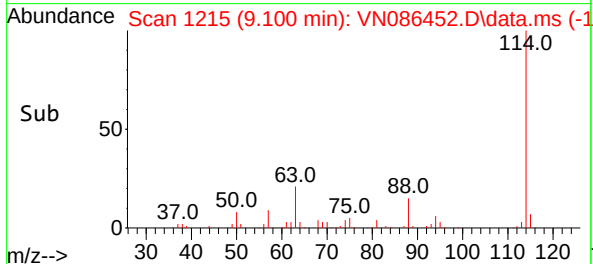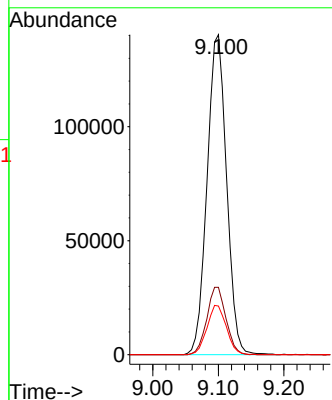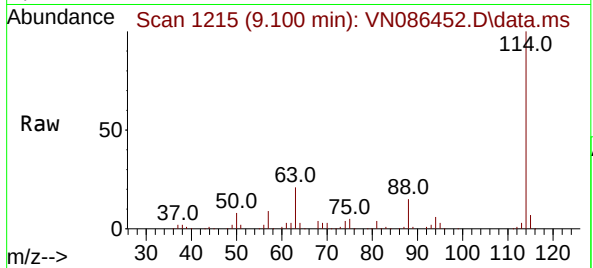

#35
Dibromofluoromethane
Concen: 61.116 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. 0.000 min
Lab File: VN086452.D
Acq: 02 May 2025 09:58

Tgt Ion:113 Resp: 82323
Ion Ratio Lower Upper
113 100
111 101.6 83.4 125.0
192 17.0 13.7 20.5


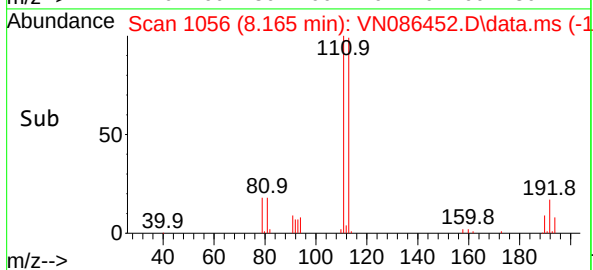
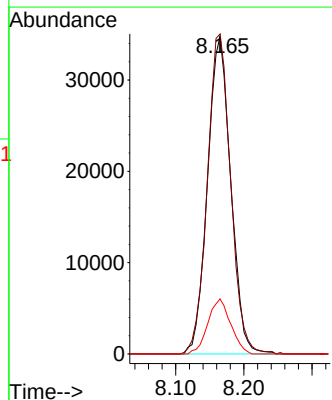
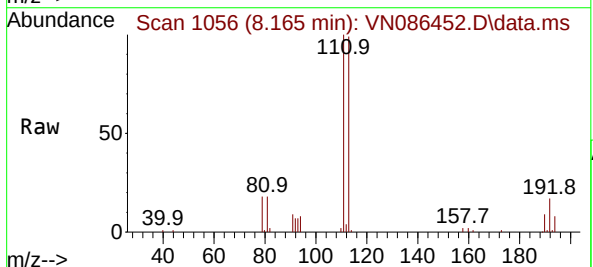


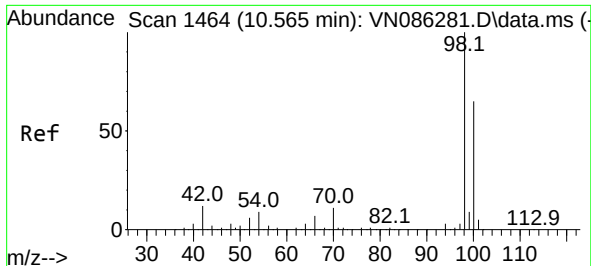

#50
Toluene-d8
Concen: 51.371 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN086452.D
Acq: 02 May 2025 09:58




Instrument :
MSVOA_N
ClientSampleId :
VN0502MBL01


Tgt Ion: 98 Resp: 369820
Ion Ratio Lower Upper
98 100
100 65.1 52.5 78.7

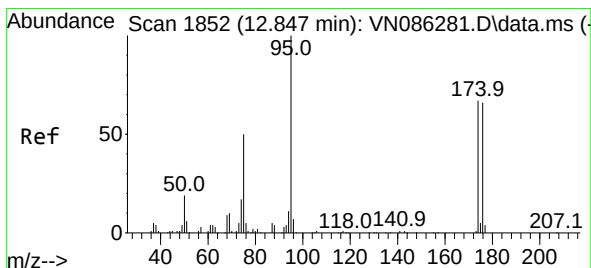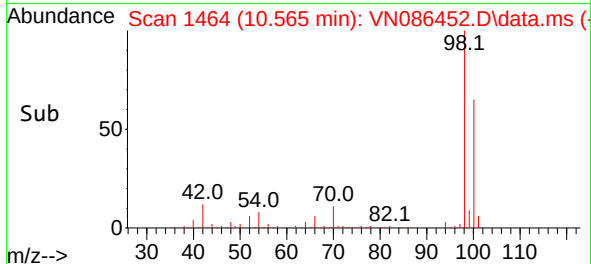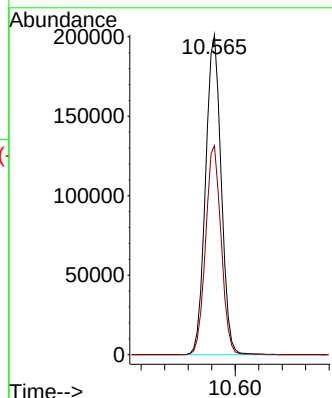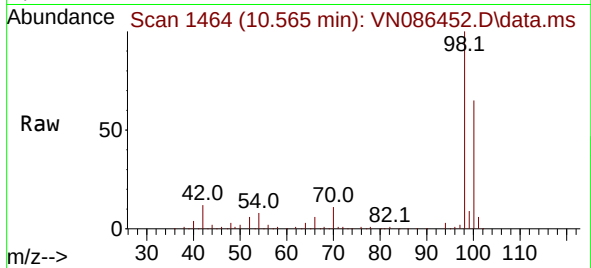

#62
4-Bromofluorobenzene
Concen: 47.182 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN086452.D
Acq: 02 May 2025 09:58

Tgt Ion: 95 Resp: 123889
Ion Ratio Lower Upper
95 100
174 73.5 0.0 133.4
176 69.3 0.0 129.2


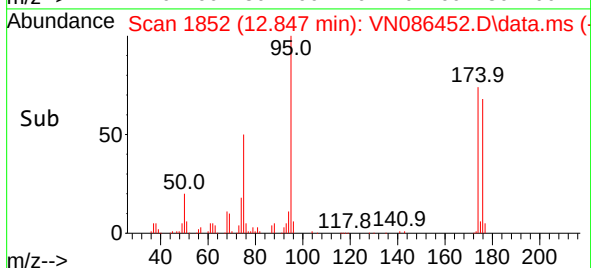
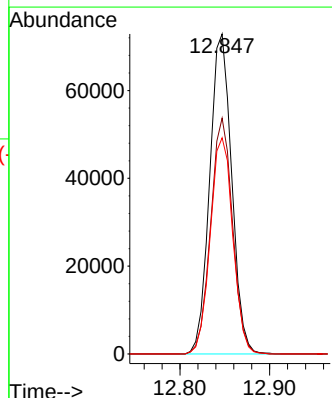
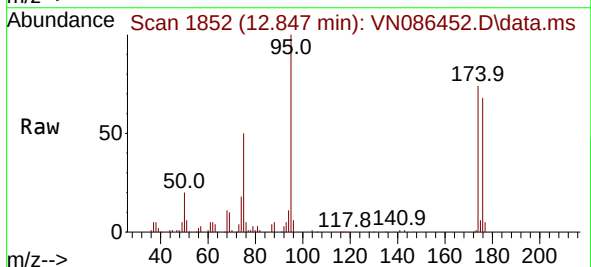


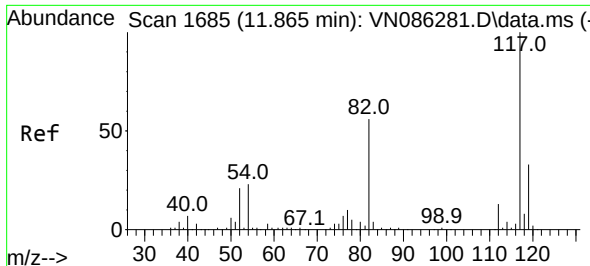

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN086452.D
Acq: 02 May 2025 09:58

Instrument :
MSVOA_N
ClientSampleId :
VN0502MBL01

Tgt Ion:117 Resp: 265958
Ion Ratio Lower Upper
117 100
82 56.7 44.7 67.1
119 31.8 26.4 39.6

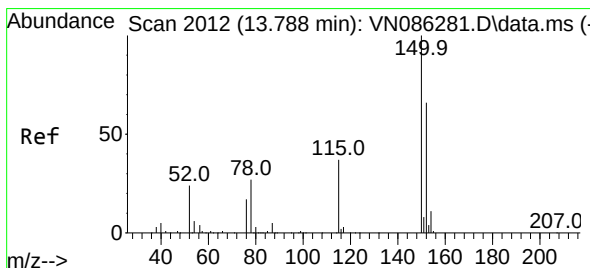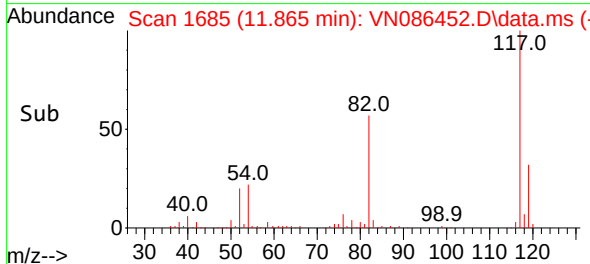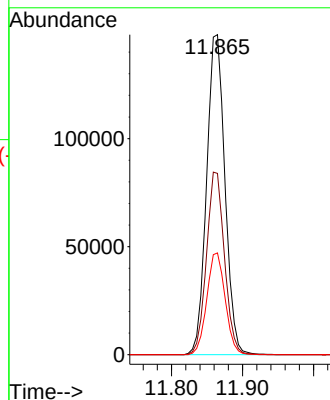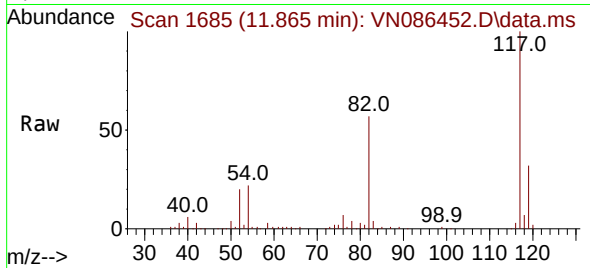

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. 0.000 min
Lab File: VN086452.D
Acq: 02 May 2025 09:58

Tgt Ion:152 Resp: 101992
Ion Ratio Lower Upper
152 100
115 60.4 31.9 95.9
150 160.0 0.0 352.0

