

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050225\
 Data File : VN086466.D
 Acq On : 02 May 2025 16:17
 Operator : JC\MD
 Sample : PB167816ZHE#11
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB167816ZHE#11

Manual Integrations
 APPROVED

Reviewed By : John Carlone 05/05/2025
 Supervised By : Semsettin Yesilyurt 05/05/2025

Quant Time: May 02 23:16:50 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 16 04:19:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	145140	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	273868	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	271268	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	118782	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	104857	49.821	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 99.640%			
35) Dibromofluoromethane	8.165	113	68052	53.540	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 107.080%			
50) Toluene-d8	10.565	98	356980	52.550	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 105.100%			
62) 4-Bromofluorobenzene	12.847	95	127445	51.436	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 102.880%			
Target Compounds					Qvalue	
16) Acetone	4.430	43	31888	39.006	ug/l	92
20) Methylene Chloride	5.271	84	8478	4.357	ug/l	93
43) Isopropyl Acetate	8.688	43	42348m	7.092	ug/l	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050225\
Data File : VN086466.D
Acq On : 02 May 2025 16:17
Operator : JC\MD
Sample : PB167816ZHE#11
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB167816ZHE#11

Manual Integrations
APPROVED

Reviewed By :John Carlone 05/05/2025
Supervised By :Semsettin Yesilyurt 05/05/2025


Quant Time: May 02 23:16:50 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 16 04:19:23 2025
Response via : Initial Calibration

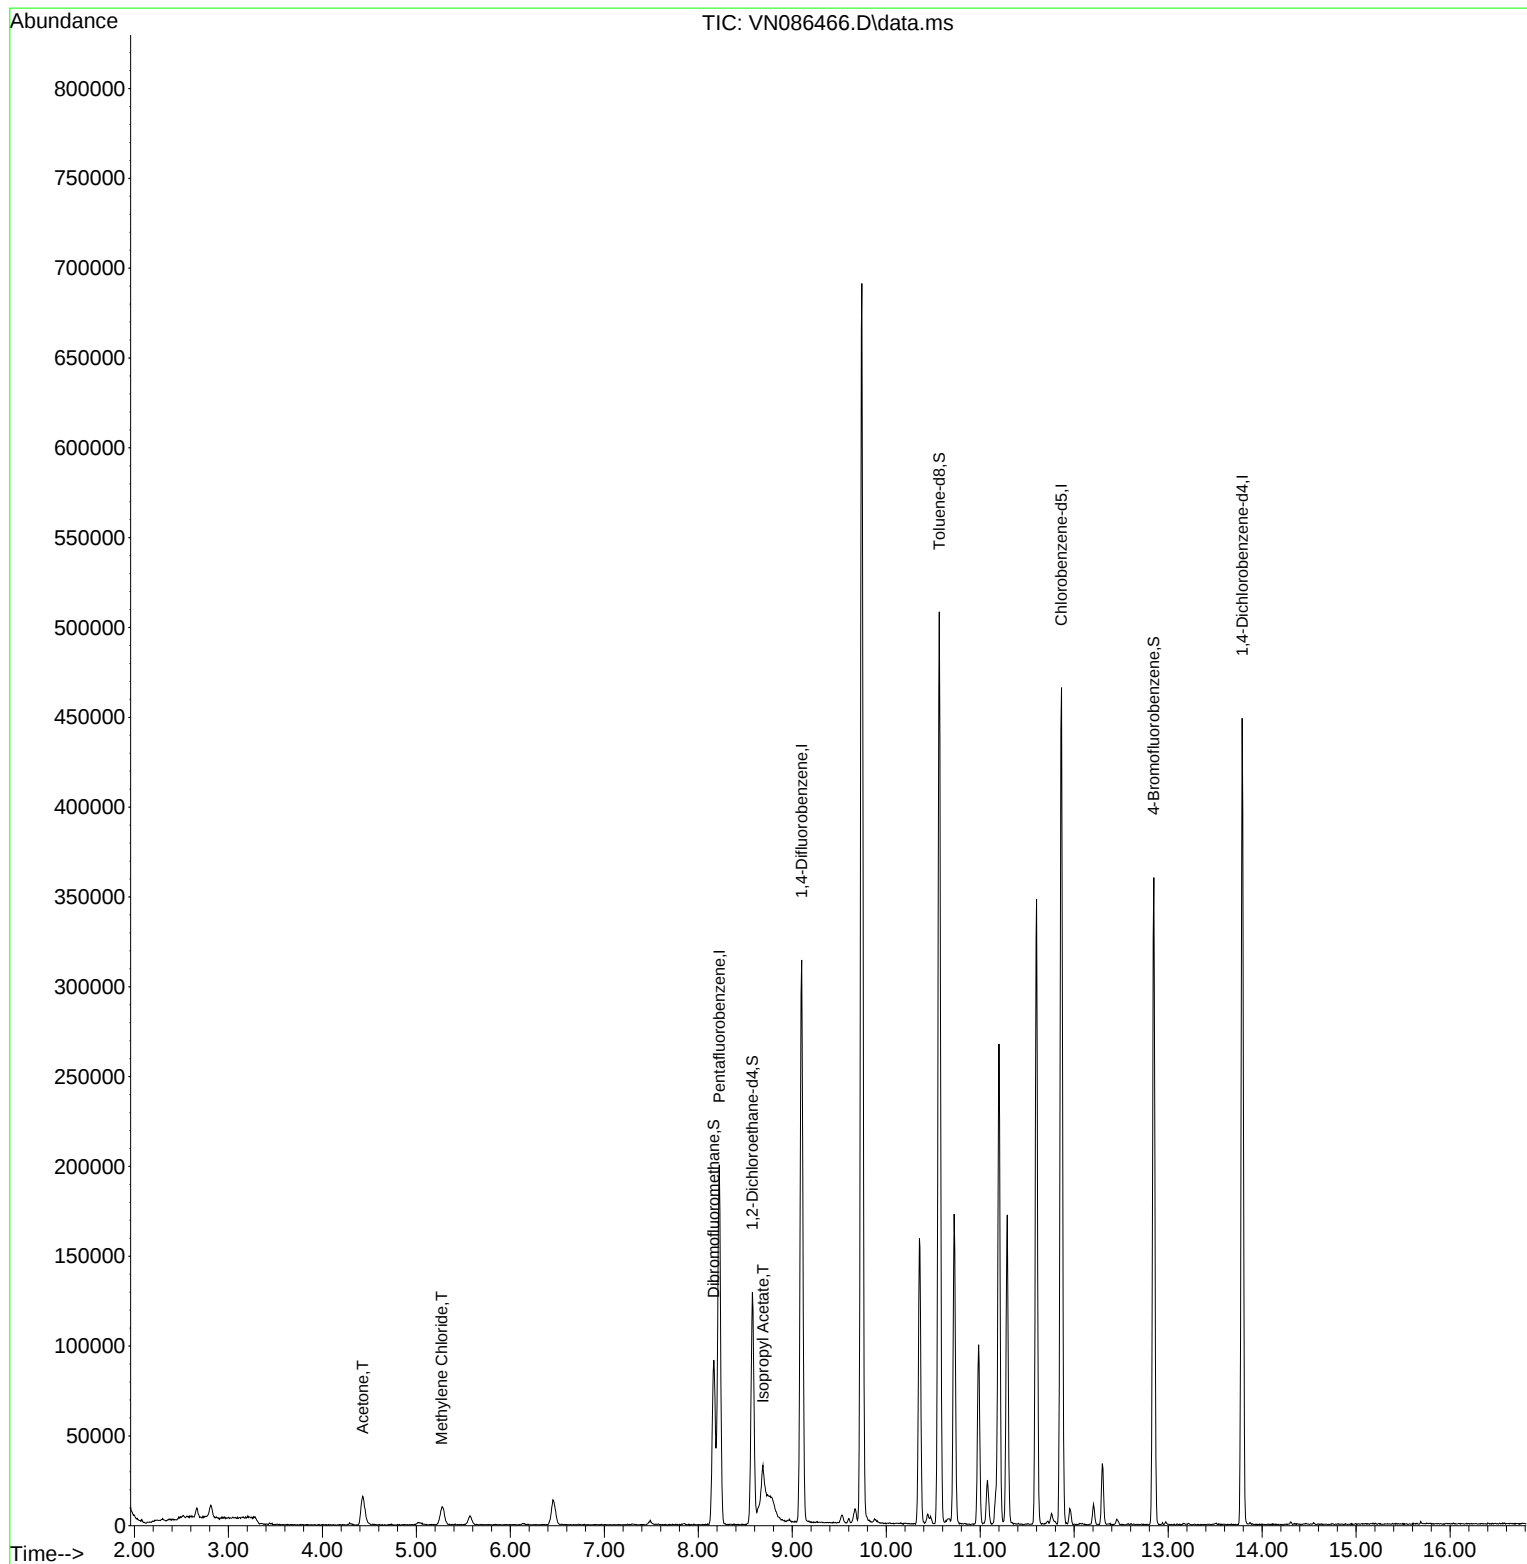



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN086466.D
Acq: 02 May 2025 16:17




Instrument :
MSVOA_N
ClientSampleId :
PB167816ZHE#11

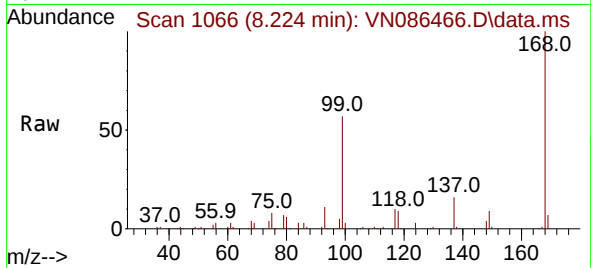


Tgt Ion:168 Resp: 145140
Ion Ratio Lower Upper
168 100
99 57.5 52.5 78.7

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/05/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

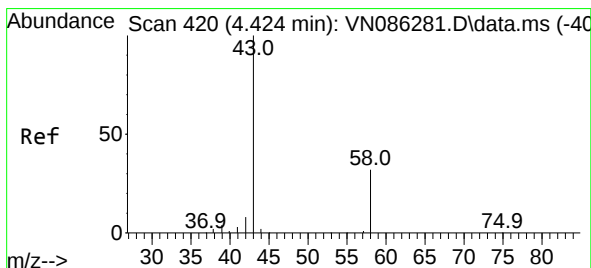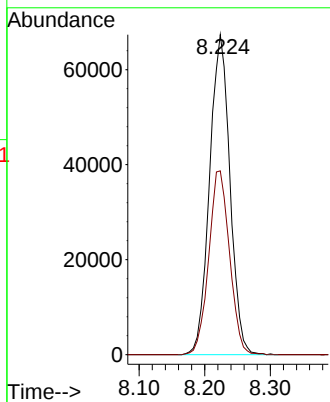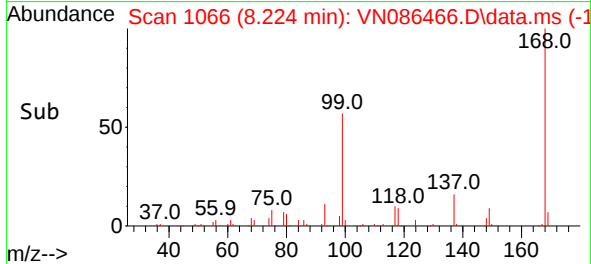

#16
Acetone
Concen: 39.006 ug/l
RT: 4.430 min Scan# 421
Delta R.T. 0.006 min
Lab File: VN086466.D
Acq: 02 May 2025 16:17

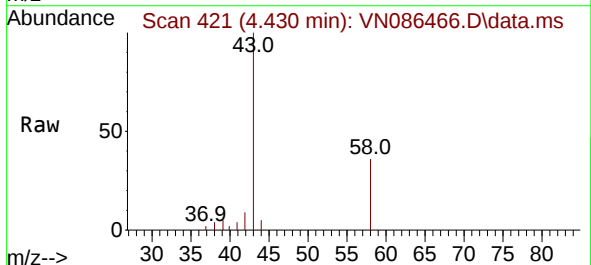


Tgt Ion: 43 Resp: 31888
Ion Ratio Lower Upper
43 100
58 35.8 25.3 37.9

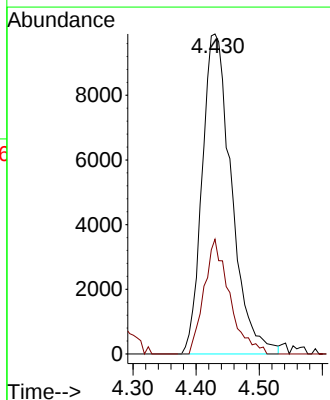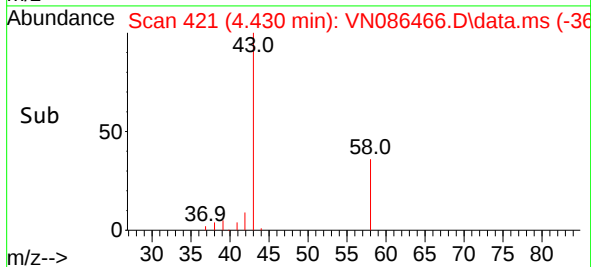



#20
Methylene Chloride
Concen: 4.357 ug/l
RT: 5.271 min Scan# 50
Delta R.T. 0.000 min
Lab File: VN086466.D
Acq: 02 May 2025 16:17




Instrument :
MSVOA_N
ClientSampleId :
PB167816ZHE#11

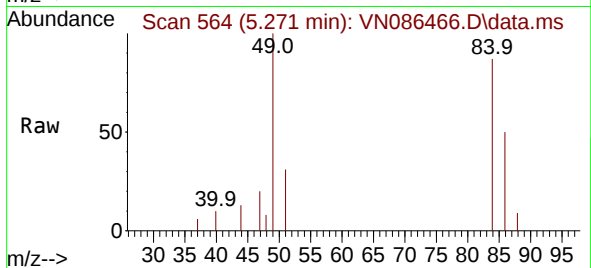

Tgt Ion: 84 Resp: 8478
Ion Ratio Lower Upper
84 100
49 114.7 98.2 147.2
51 35.7 29.8 44.6
86 57.9 52.0 78.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/05/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

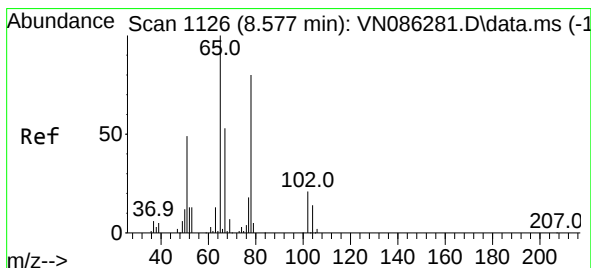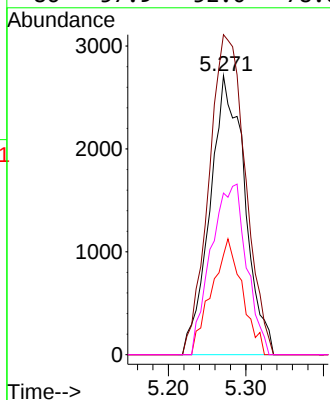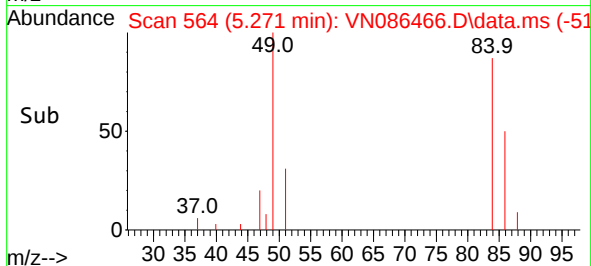

#33
1,2-Dichloroethane-d4
Concen: 49.821 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN086466.D
Acq: 02 May 2025 16:17

Tgt Ion: 65 Resp: 104857
Ion Ratio Lower Upper
65 100
67 52.7 0.0 106.0

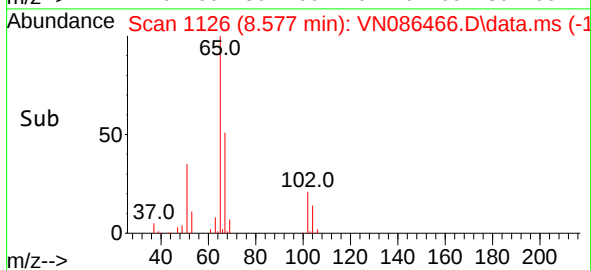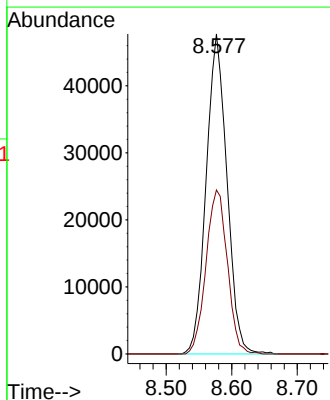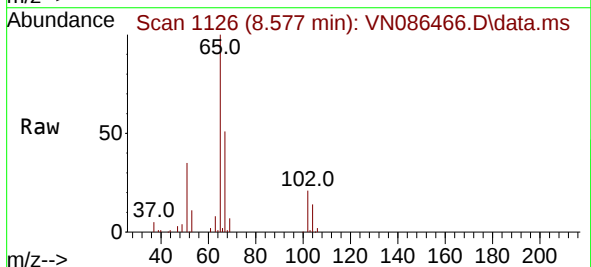

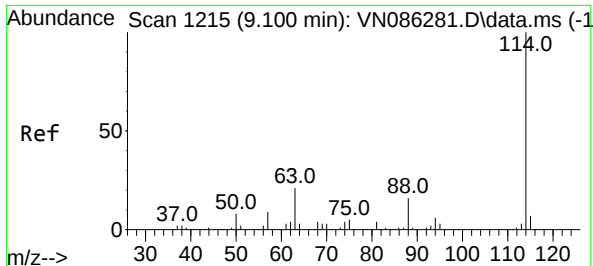

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN086466.D

Acq: 02 May 2025 16:17

Instrument :

MSVOA_N

ClientSampleId :

PB167816ZHE#11

Tgt Ion:114 Resp: 27386





Ion	Ratio	Lower	Upper
114	100		
63	19.4	0.0	42.6
88	15.6	0.0	31.8

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/05/2025

Supervised By :Semsettin Yesilyurt 05/05/2025

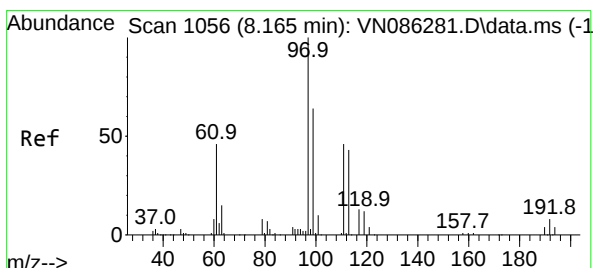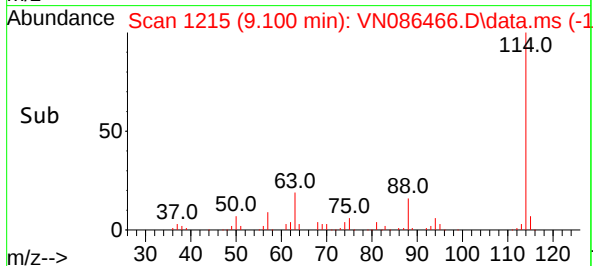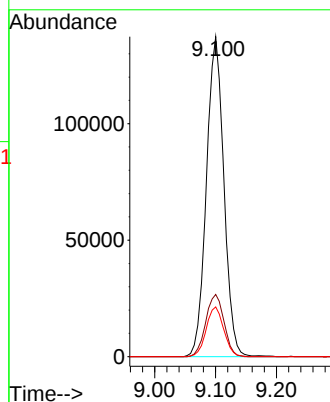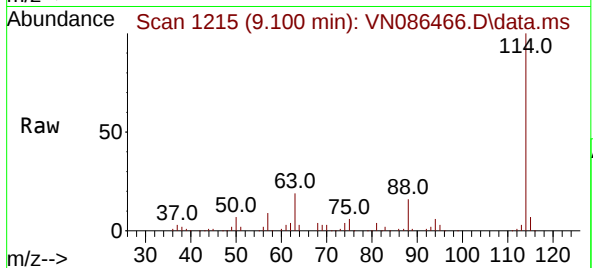

#35

Dibromofluoromethane

Concen: 53.540 ug/l

RT: 8.165 min Scan# 1056




Delta R.T. 0.000 min


Lab File: VN086466.D

Acq: 02 May 2025 16:17

Tgt Ion:113 Resp: 68052


Ion	Ratio	Lower	Upper
113	100		
111	102.9	83.4	125.0
192	18.0	13.7	20.5

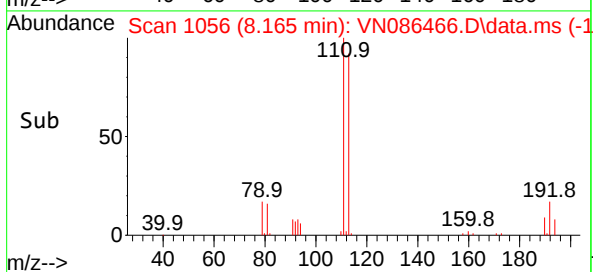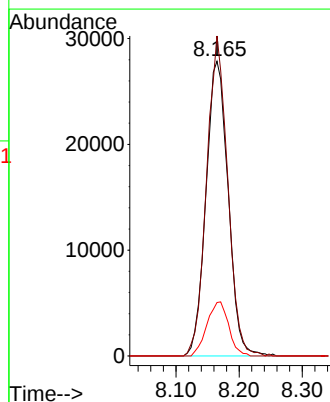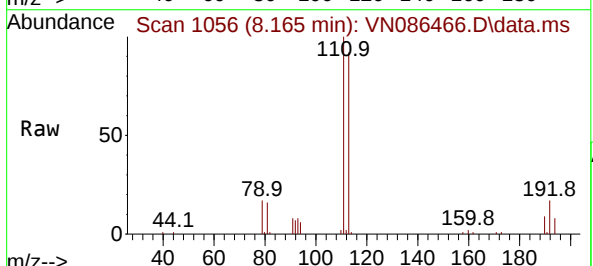

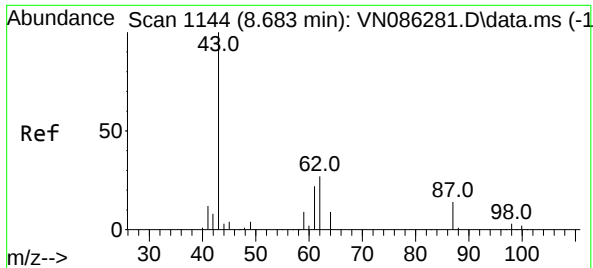

#43
Isopropyl Acetate
Concen: 7.092 ug/l m
RT: 8.688 min Scan# 1145
Delta R.T. 0.005 min
Lab File: VN086466.D
Acq: 02 May 2025 16:17




Instrument :
MSVOA_N
ClientSampleId :
PB167816ZHE#11

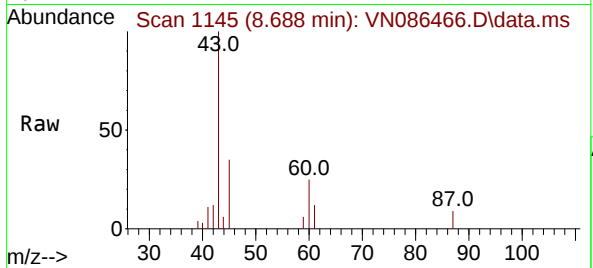


Tgt Ion: 43 Resp: 42348
Ion Ratio Lower Upper
43 100
61 10.3 20.5 30.7
87 6.3 10.5 15.7

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/05/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

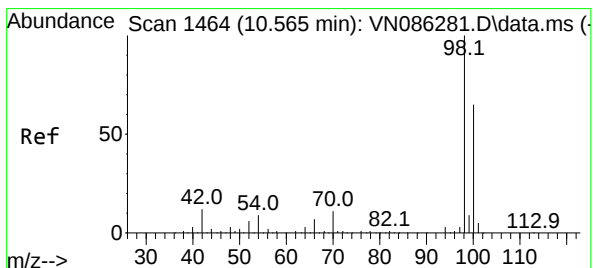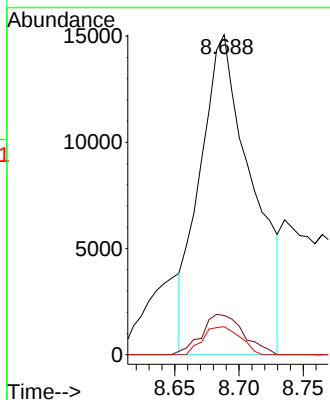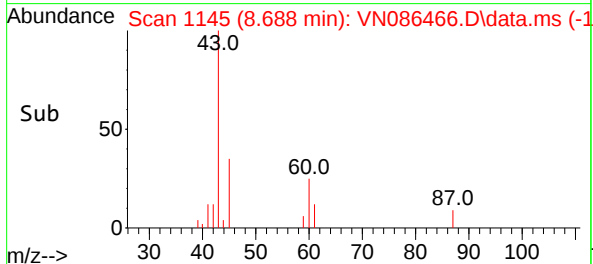


#50
Toluene-d8
Concen: 52.550 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN086466.D
Acq: 02 May 2025 16:17

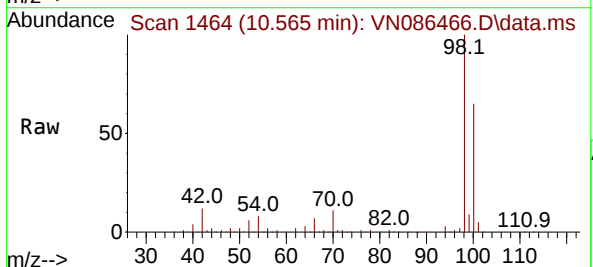


Tgt Ion: 98 Resp: 356980
Ion Ratio Lower Upper
98 100
100 65.0 52.5 78.7

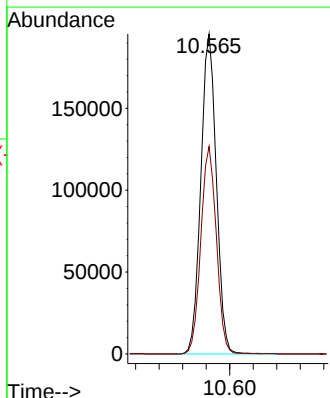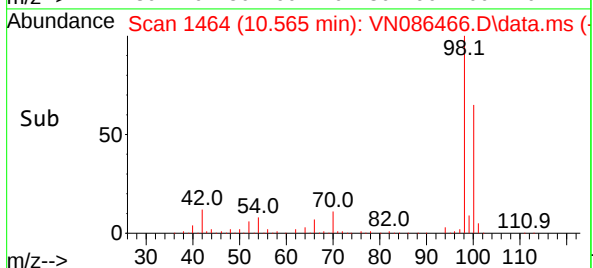

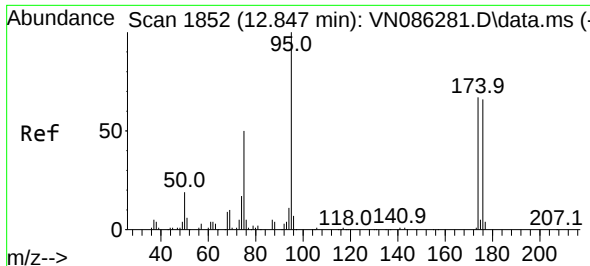

#62
4-Bromofluorobenzene
Concen: 51.436 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN086466.D
Acq: 02 May 2025 16:17




Instrument :
MSVOA_N
ClientSampleId :
PB167816ZHE#11

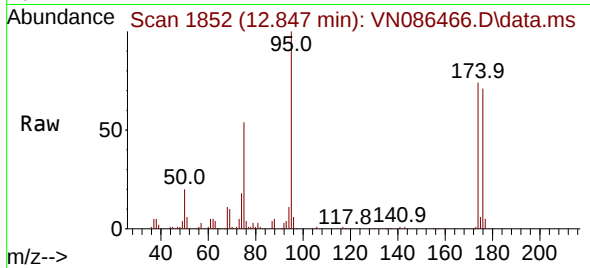


Tgt Ion: 95 Resp: 127449
Ion Ratio Lower Upper
95 100
174 74.0 0.0 133.4
176 70.1 0.0 129.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/05/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

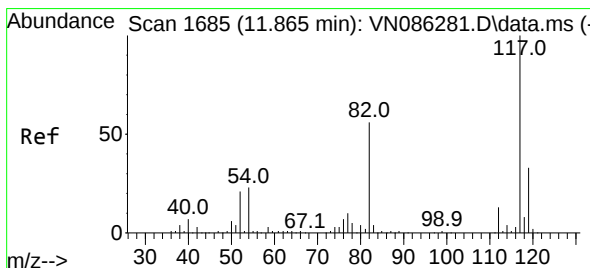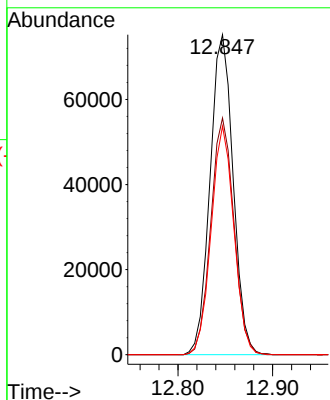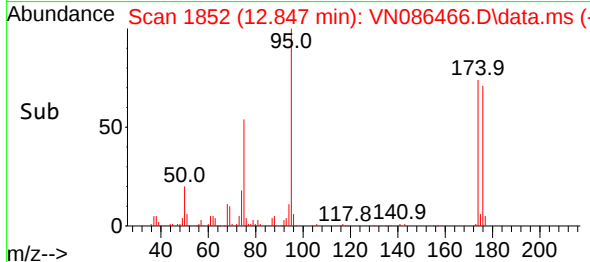


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VN086466.D
Acq: 02 May 2025 16:17

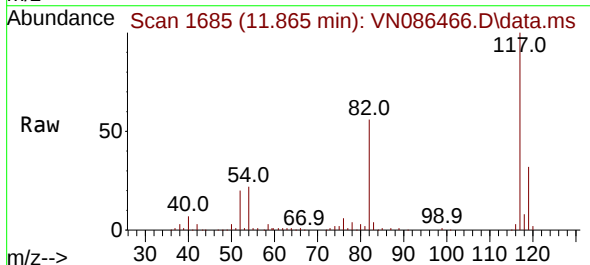


Tgt Ion:117 Resp: 271268
Ion Ratio Lower Upper
117 100
82 55.8 44.7 67.1
119 32.2 26.4 39.6

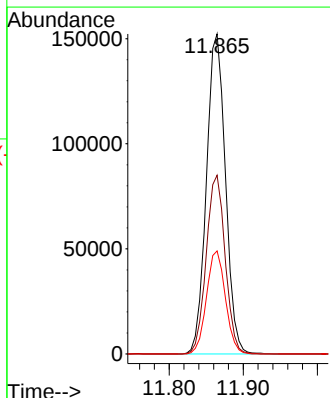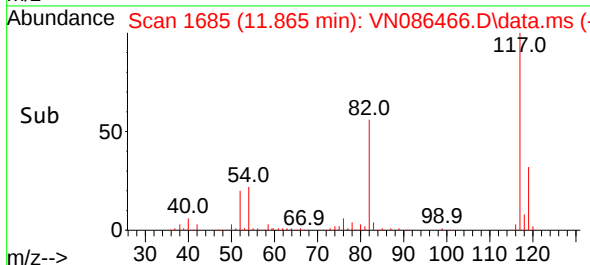

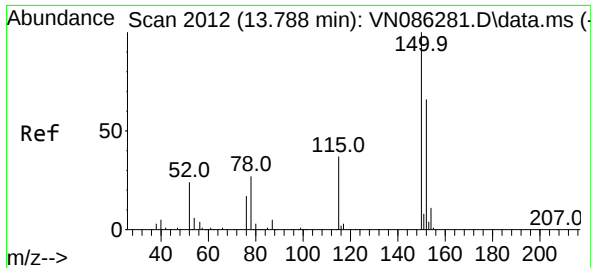

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 20
Delta R.T. 0.000 min
Lab File: VN086466.D
Acq: 02 May 2025 16:17

Instrument :
MSVOA_N
ClientSampleId :
PB167816ZHE#11

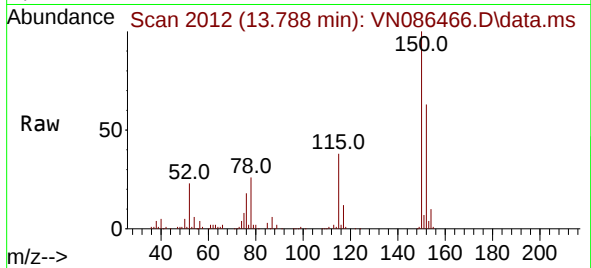

Tgt Ion:152 Resp: 11878
Ion Ratio Lower Upper
152 100
115 60.4 31.9 95.9
150 159.0 0.0 352.0

Manual Integrations
APPROVED

Reviewed By :John Carlone 05/05/2025
Supervised By :Semsettin Yesilyurt 05/05/2025

