

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050225\
 Data File : VN086475.D
 Acq On : 02 May 2025 19:56
 Operator : JC\MD
 Sample : Q1940-06
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-3

Quant Time: May 02 23:18:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 16 04:19:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	141230	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	272575	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	263663	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	115290	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	101597	49.609	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	99.220%
35) Dibromofluoromethane	8.165	113	75911	60.006	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	120.020%
50) Toluene-d8	10.565	98	347241	51.359	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.720%
62) 4-Bromofluorobenzene	12.847	95	123073	49.907	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	99.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050225\
Data File : VN086475.D
Acq On : 02 May 2025 19:56
Operator : JC\MD
Sample : Q1940-06
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-3


Quant Time: May 02 23:18:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 16 04:19:23 2025
Response via : Initial Calibration

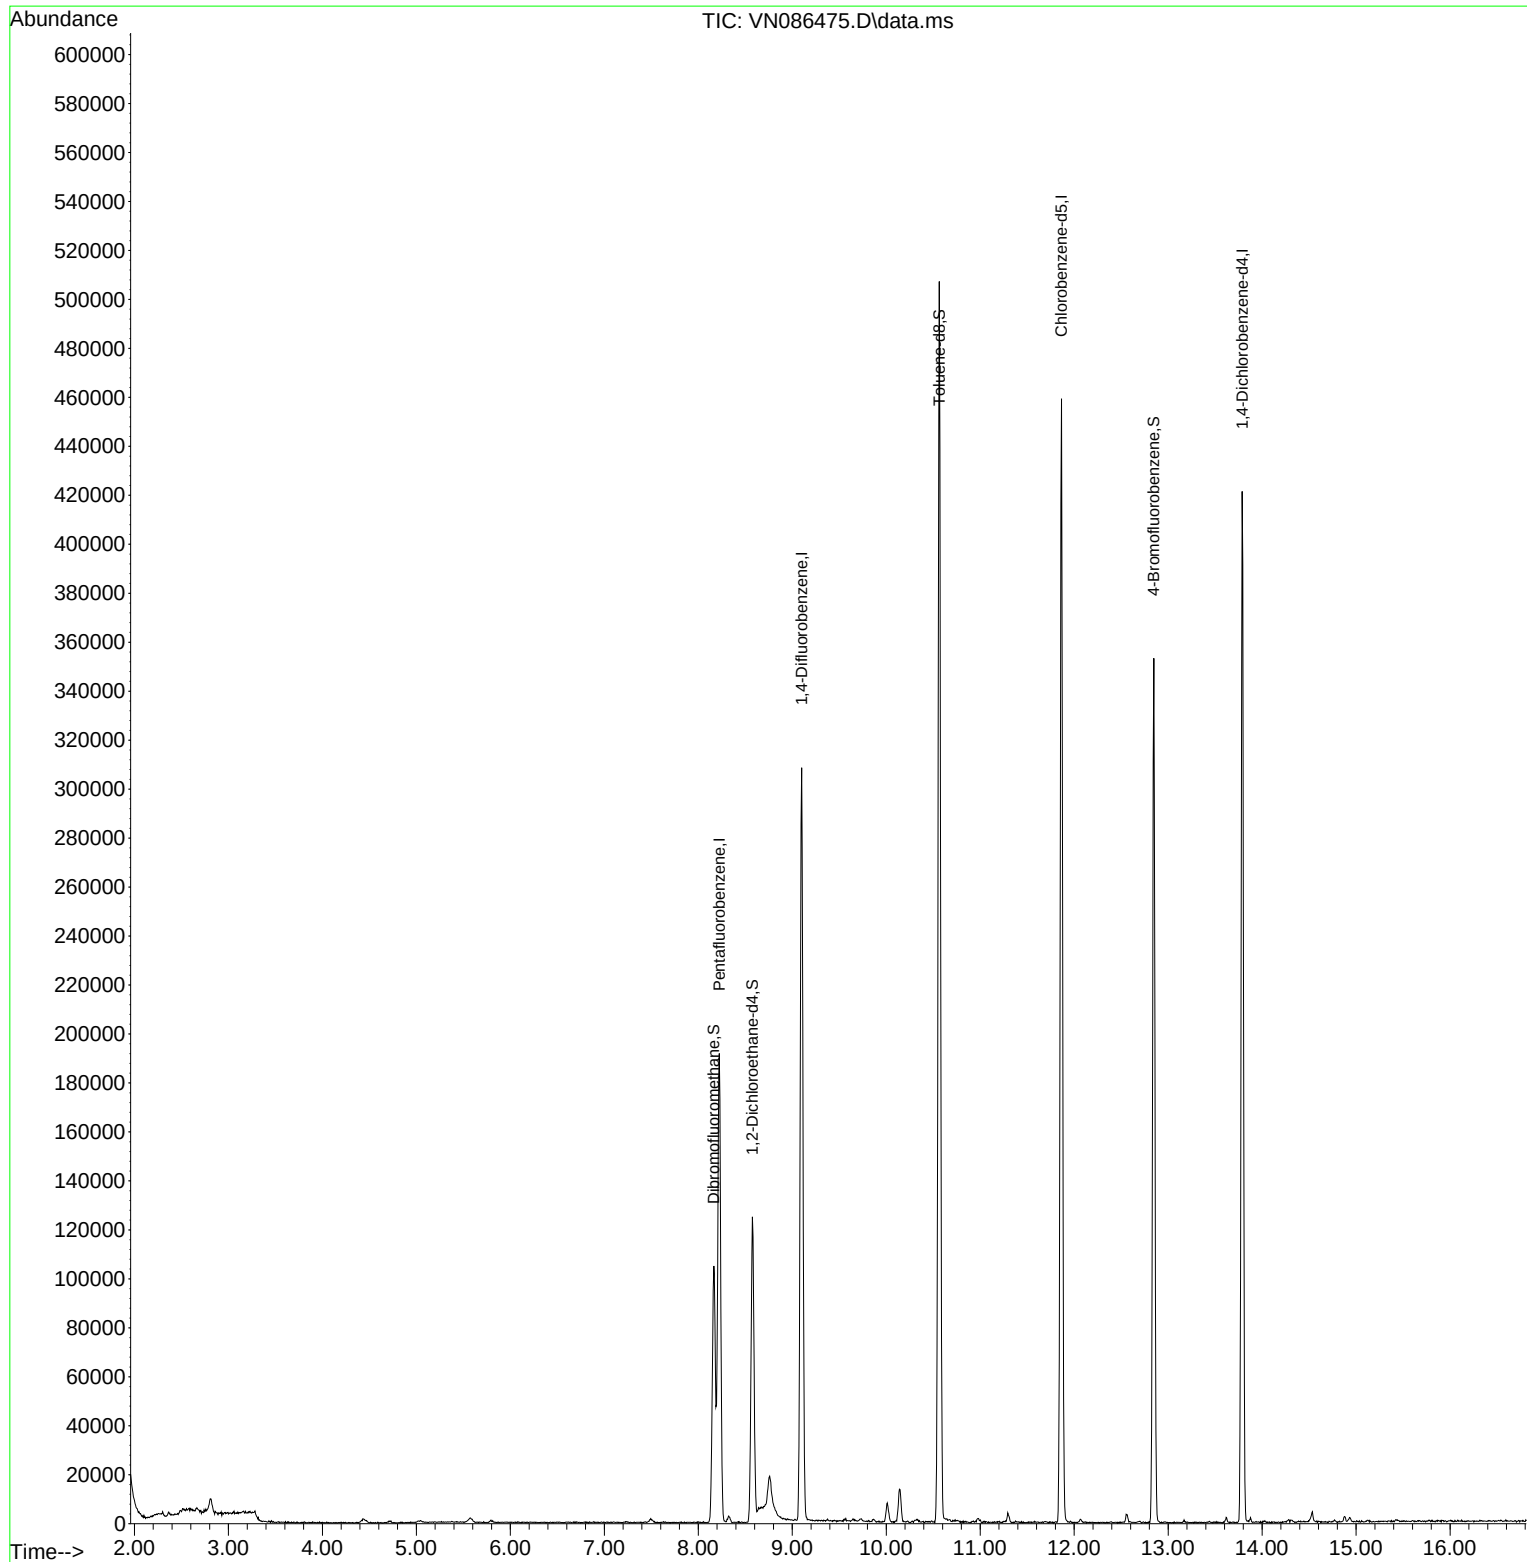



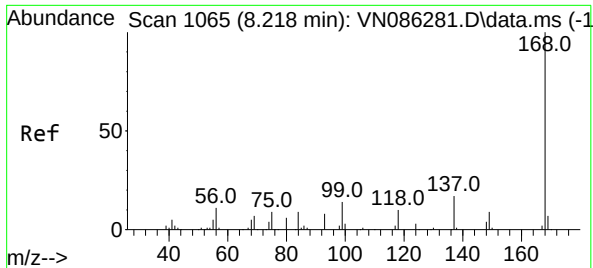


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN086475.D
Acq: 02 May 2025 19:56

Instrument :
MSVOA_N
ClientSampleId :
MW-3



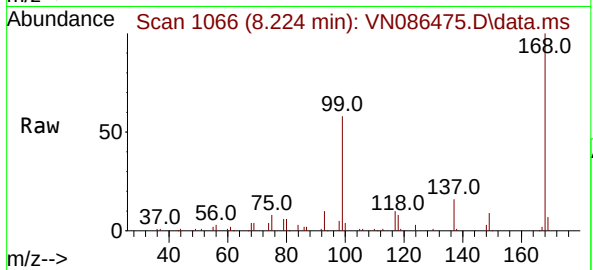



Tgt Ion:168 Resp: 141230
Ion Ratio Lower Upper
168 100
99 58.1 52.5 78.7

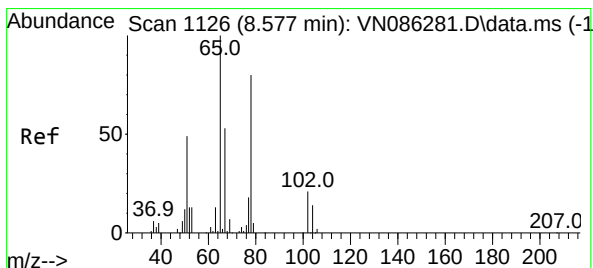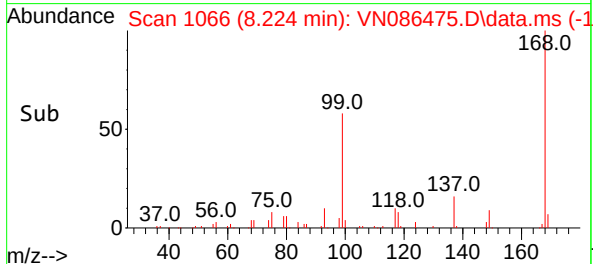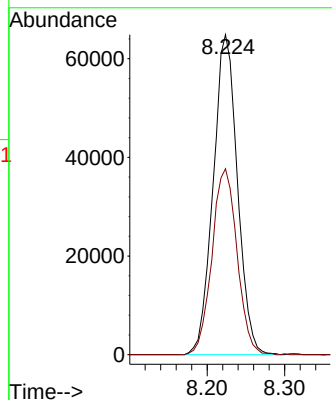

#33
1,2-Dichloroethane-d4
Concen: 49.609 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN086475.D
Acq: 02 May 2025 19:56

Tgt Ion: 65 Resp: 101597
Ion Ratio Lower Upper
65 100
67 52.3 0.0 106.0

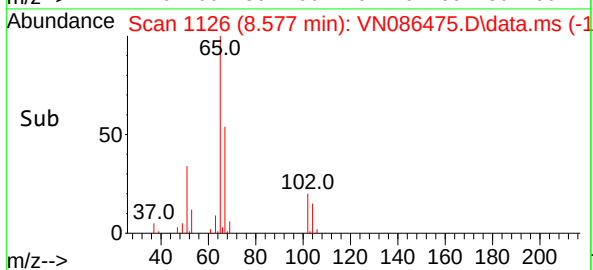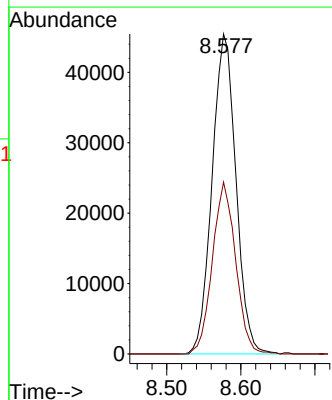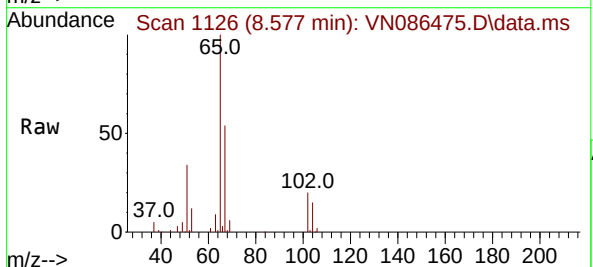

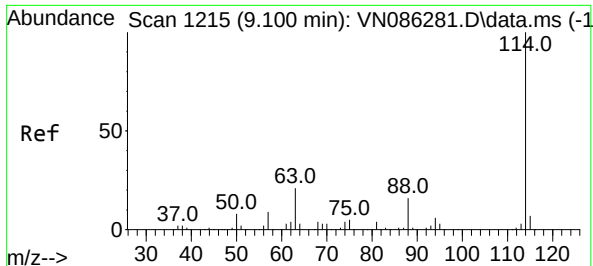

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN086475.D

Acq: 02 May 2025 19:56

Instrument :

MSVOA_N

ClientSampleId :

MW-3





Tgt Ion:114 Resp: 272575

Ion Ratio Lower Upper

114 100

63 19.4 0.0 42.6

88 15.4 0.0 31.8

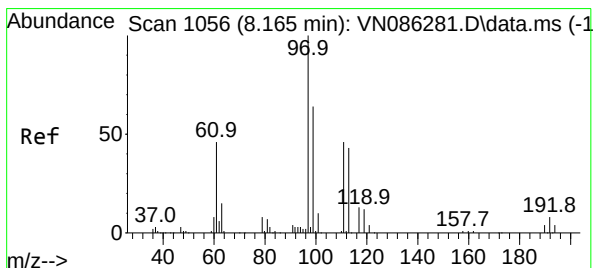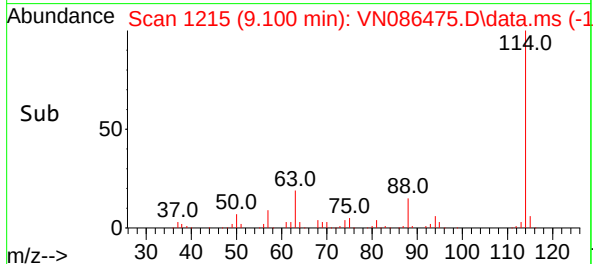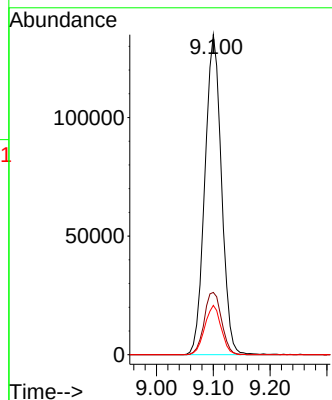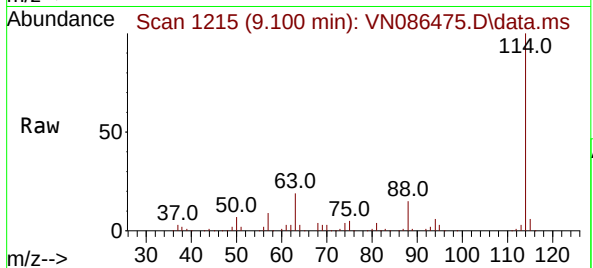

#35

Dibromofluoromethane

Concen: 60.006 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN086475.D

Acq: 02 May 2025 19:56




Tgt Ion:113 Resp: 75911


Ion Ratio Lower Upper

113 100

111 104.7 83.4 125.0

192 17.6 13.7 20.5


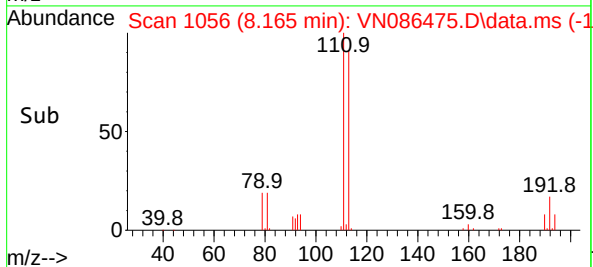
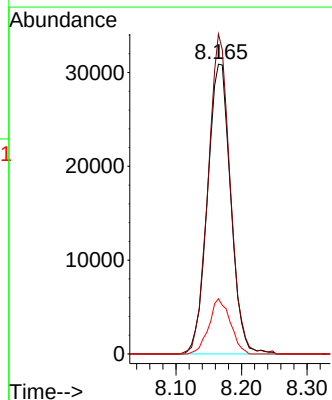
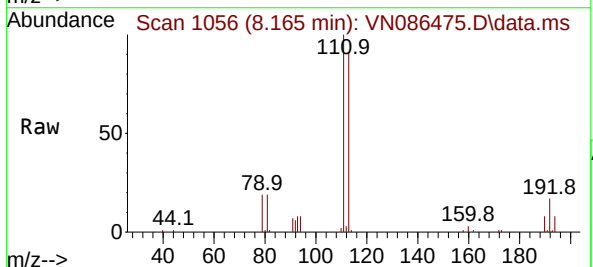


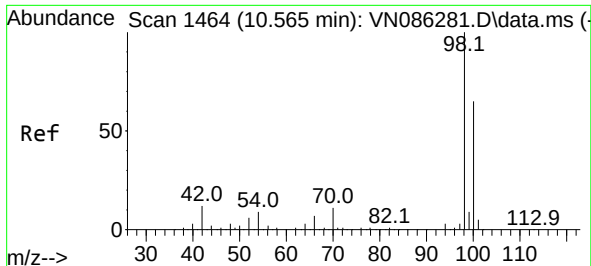

#50
Toluene-d8
Concen: 51.359 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN086475.D
Acq: 02 May 2025 19:56




Instrument :
MSVOA_N
ClientSampleId :
MW-3


Tgt Ion: 98 Resp: 347241
Ion Ratio Lower Upper
98 100
100 65.7 52.5 78.7

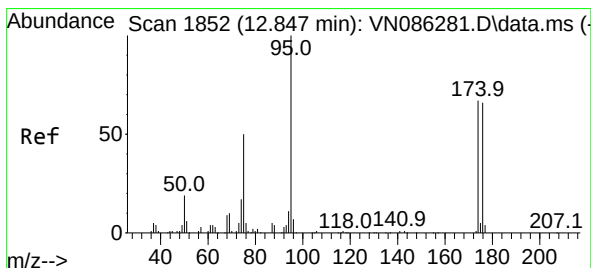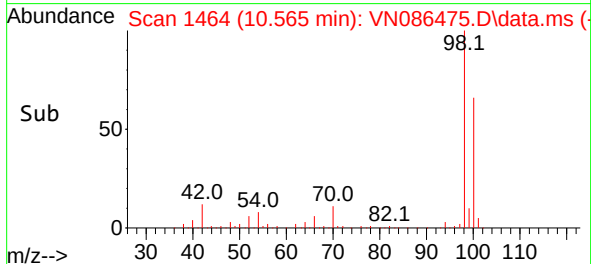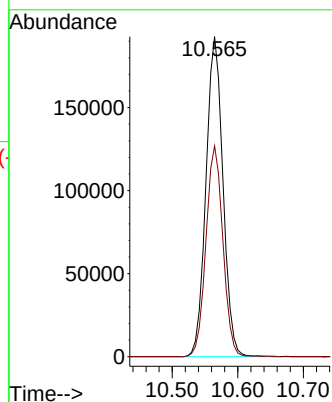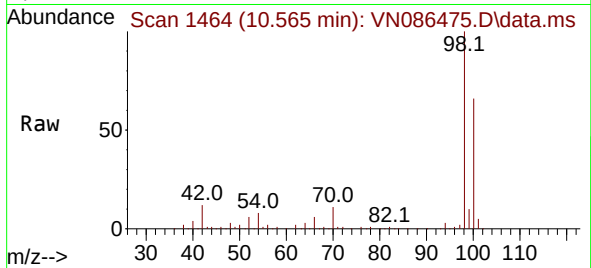

#62
4-Bromofluorobenzene
Concen: 49.907 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086475.D
Acq: 02 May 2025 19:56

Tgt Ion: 95 Resp: 123073
Ion Ratio Lower Upper
95 100
174 75.7 0.0 133.4
176 71.9 0.0 129.2


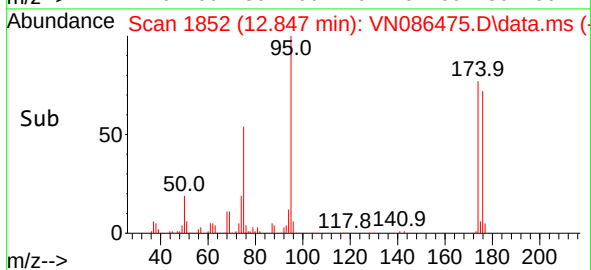
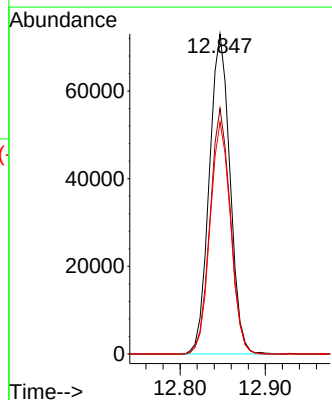
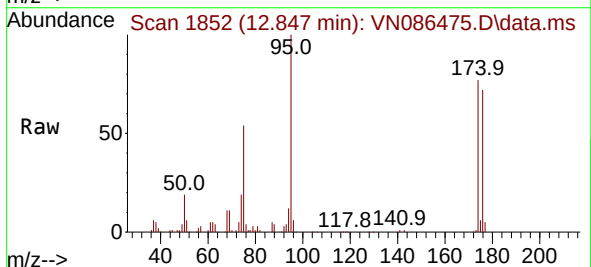


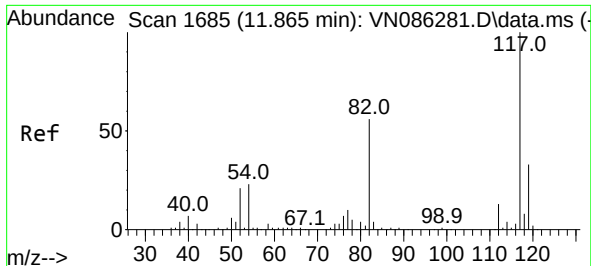

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086475.D
Acq: 02 May 2025 19:56

Instrument :
MSVOA_N
ClientSampleId :
MW-3

Tgt Ion:117 Resp: 263663
Ion Ratio Lower Upper
117 100
82 55.1 44.7 67.1
119 31.6 26.4 39.6

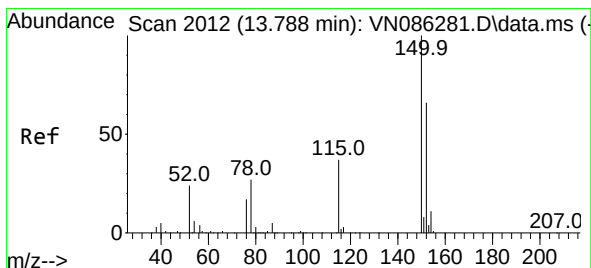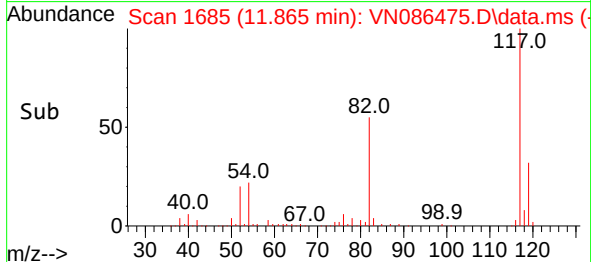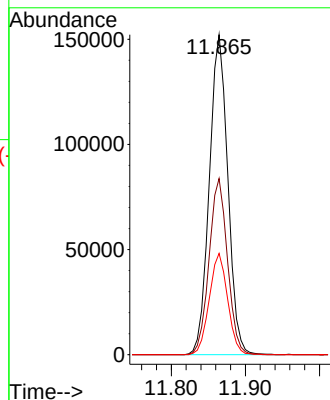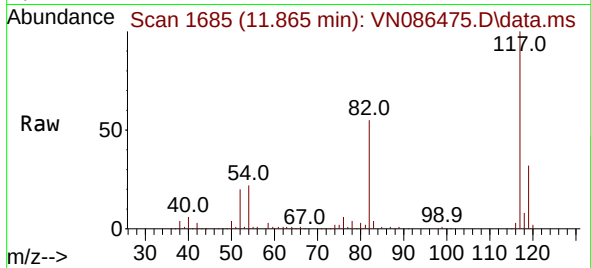

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN086475.D
Acq: 02 May 2025 19:56

Tgt Ion:152 Resp: 115290
Ion Ratio Lower Upper
152 100
115 61.2 31.9 95.9
150 157.8 0.0 352.0

