

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN050319\
 Data File : VN055400.D
 Acq On : 3 May 2019 19:33
 Operator : JC/SP
 Sample : K2674-02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FILTERBAG-RO

Quant Time: May 03 23:24:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 30 07:16:52 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	476678	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	827268	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	751707	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	229134	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	325854	52.25	ug/l	0.00
Spiked Amount			Recovery	=	104.50%	
35) Dibromofluoromethane	7.59	113	261546	48.17	ug/l	0.00
Spiked Amount			Recovery	=	96.34%	
50) Toluene-d8	10.09	98	1014715	51.75	ug/l	0.00
Spiked Amount			Recovery	=	103.50%	
62) 4-Bromofluorobenzene	12.40	95	331057	54.03	ug/l	0.00
Spiked Amount			Recovery	=	108.06%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.82	43	14101	7.257	ug/l	98
18) Methyl Acetate	4.35	43	3549	Below Cal	#	73
20) Methylene Chloride	4.56	84	4698	0.792	ug/l	97
25) 2-Butanone	6.85	43	2145	0.863	ug/l	96
29) Tetrahydrofuran	7.22	42	1171	0.736	ug/l #	84
30) Chloroform	7.37	83	2984	0.305	ug/l #	73
31) Cyclohexane	7.67	56	10229	1.043	ug/l #	6
36) 1,1-Dichloropropene	7.66	75	35642	4.498	ug/l #	50
38) Carbon Tetrachloride	7.67	117	44358	5.803	ug/l #	16
41) Methacrylonitrile	7.20	41	369	0.850	ug/l #	23
43) Isopropyl Acetate	8.17	43	15895	1.629	ug/l #	83
48) Methyl methacrylate	9.18	41	6954	1.449	ug/l #	31
51) 4-Methyl-2-Pentanone	10.02	43	7362	1.340	ug/l #	39
54) cis-1,3-Dichloropropene	9.90	75	49188	5.752	ug/l #	65
57) 1,3-Dichloropropane	10.76	76	8522	0.976	ug/l #	43
59) 2-Hexanone	10.76	43	138749	40.357	ug/l #	54
71) Bromoform	12.40	173	1878	0.588	ug/l #	1
73) Isopropylbenzene	12.24	105	117	Below Cal	#	49
75) 1,1,2,2-Tetrachloroethane	12.70	83	67	Below Cal	#	25
76) 1,2,3-Trichloropropane	12.40	75	170877	39.597	ug/l #	100
79) 2-Chlorotoluene	12.73	91	458	Below Cal	#	42
80) 1,3,5-Trimethylbenzene	12.73	105	5629	0.313	ug/l	93
81) trans-1,4-Dichloro-2-buten	12.40	75	170877	141.325	ug/l #	7
83) tert-Butylbenzene	13.05	119	190	Below Cal	#	25
95) Naphthalene	15.13	128	158	3.351	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN050319\
Data File : VN055400.D
Acq On : 3 May 2019 19:33
Operator : JC/SP
Sample : K2674-02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FILTERBAG-RO

Quant Time: May 03 23:24:42 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 30 07:16:52 2019
Response via : Initial Calibration

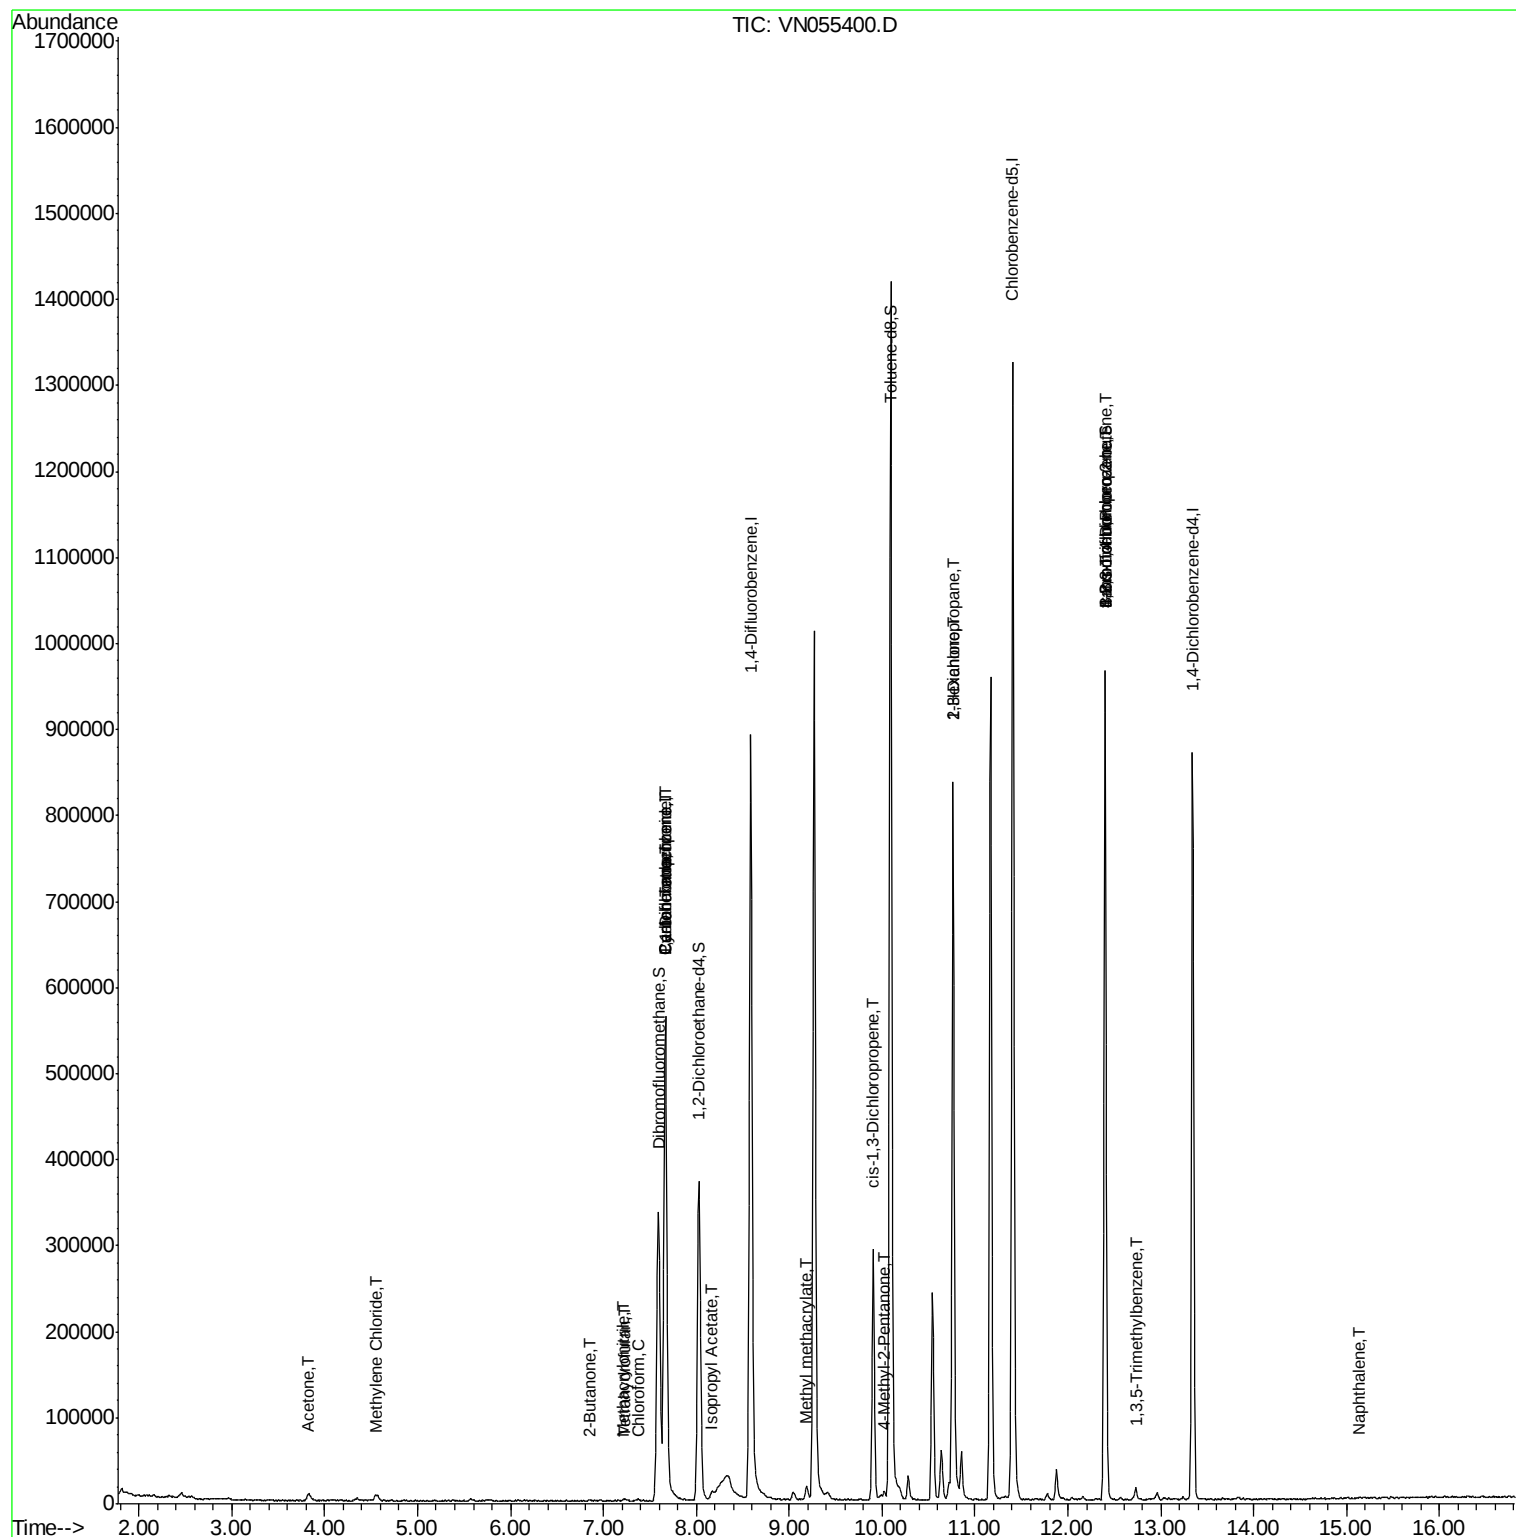

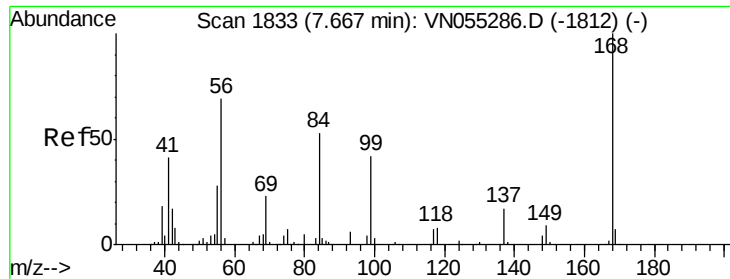

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33


Instrument :
MSVOA_N
ClientSampleId :
FILTERBAG-RO

Tot Ion:168 Resp: 476678

Ion Ratio Lower Upper




168 100

99 55.9 43.6 65.4

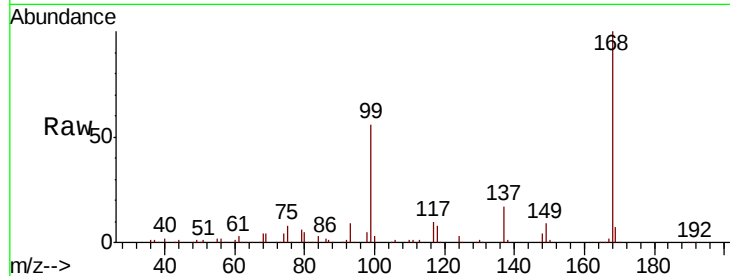

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

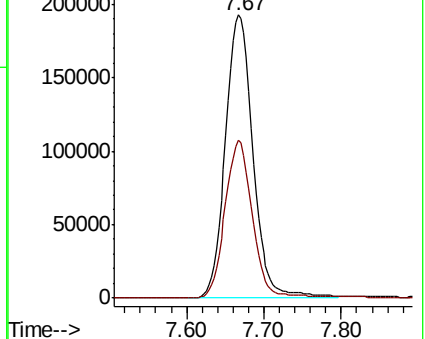

#16

Acetone

Concen: 7.257 ug/l

RT: 3.82 min Scan# 638

Delta R.T. 0.01 min

Lab File: VN055400.D


Acq: 3 May 2019 19:33

Tgt Ion: 43 Resp: 14101

Ion Ratio Lower Upper



43 100


58 28.4 23.6 35.4



Abundance Ion 43.00 (42.70 to 43.70): VN

Ion 58.00 (57.70 to 58.70): VN



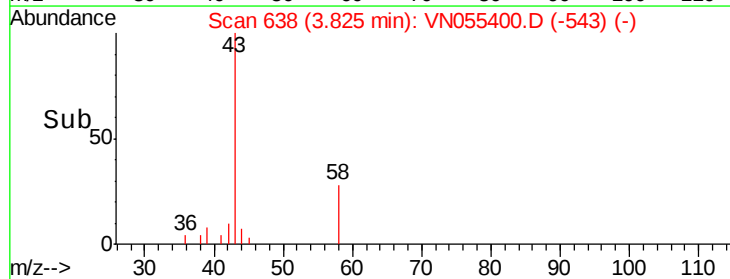
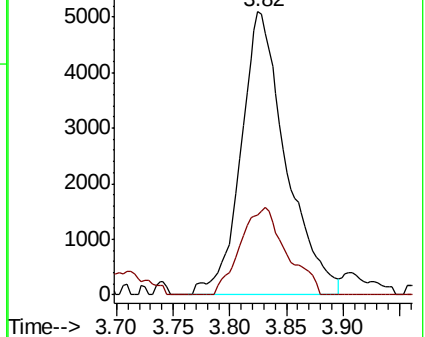




#18
Methyl Acetate
Concen: Below Cal
RT: 4.35 min Scan# 800
Delta R.T. 0.02 min
Lab File: VN055400.D
Acq: 3 May 2019 19:33




Instrument :
MSVOA_N
ClientSampleId :
FILTERBAG-RO


Tot Ion: 43 Resp: 3549
Ion Ratio Lower Upper
43 100
74 7.2 15.8 23.8#

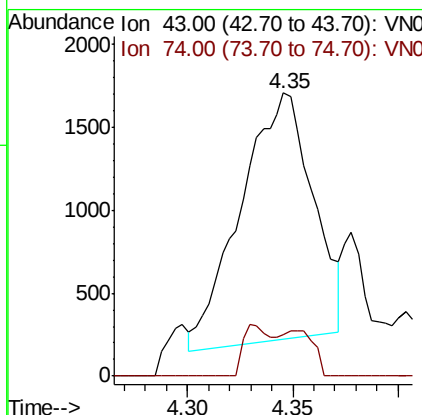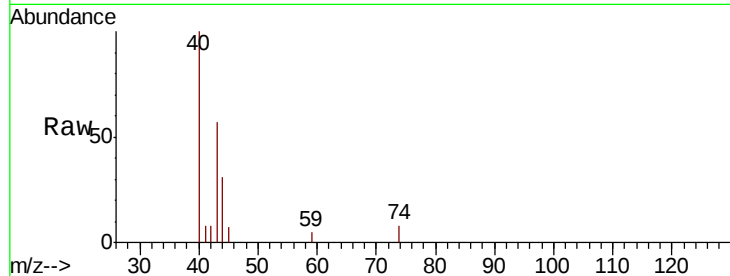

#20
Methylene Chloride
Concen: 0.792 ug/l
RT: 4.56 min Scan# 866
Delta R.T. 0.00 min
Lab File: VN055400.D
Acq: 3 May 2019 19:33

Tgt Ion: 84 Resp: 4698
Ion Ratio Lower Upper
84 100
49 136.6 112.4 168.6
51 43.8 34.6 51.8
86 67.7 51.9 77.9



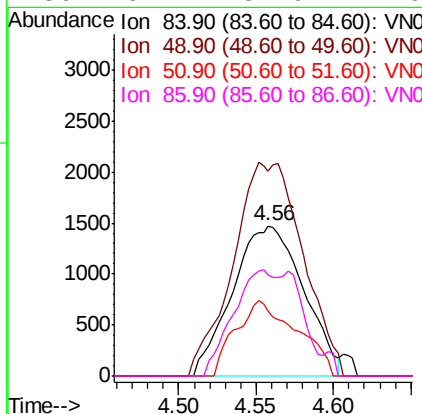





#25
 2-Butanone
 Concen: 0.863 ug/l
 RT: 6.85 min Scan# 1580
 Delta R.T. 0.02 min
 Lab File: VN055400.D
 Acq: 3 May 2019 19:33




Instrument :
 MSVOA_N
 ClientSampleId :
 FILTERBAG-RO


Tot Ion: 43 Resp: 2145
 Ion Ratio Lower Upper
 43 100
 72 20.8 18.0 27.0

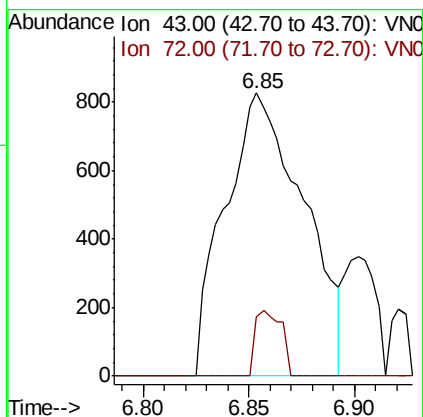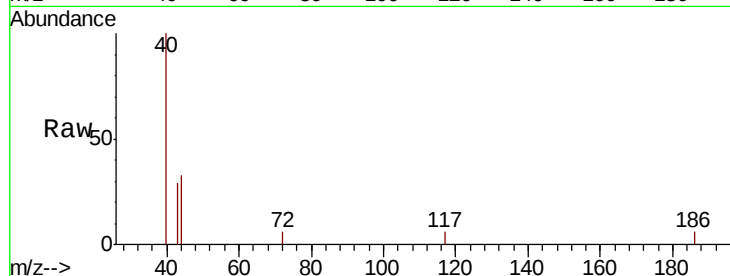

#29
 Tetrahydrofuran
 Concen: 0.736 ug/l
 RT: 7.22 min Scan# 1693
 Delta R.T. 0.01 min
 Lab File: VN055400.D
 Acq: 3 May 2019 19:33

Tgt Ion: 42 Resp: 1171
 Ion Ratio Lower Upper
 42 100
 72 45.0 29.0 43.6#
 71 43.9 27.1 40.7#

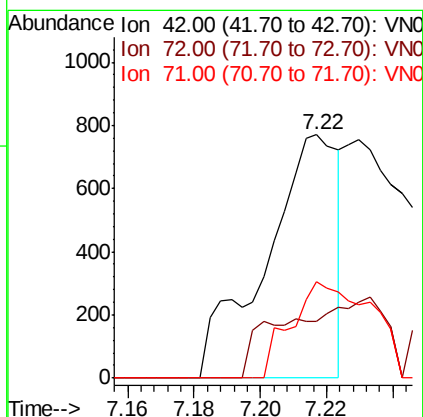

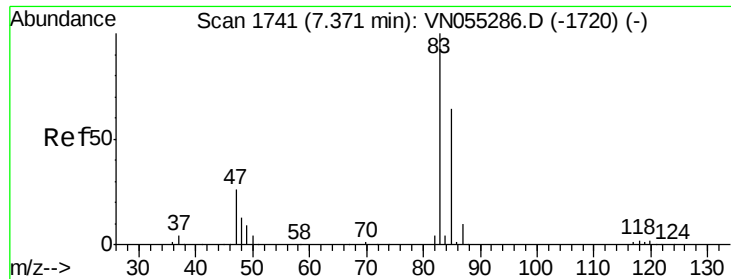

#30

Chloroform

Concen: 0.305 ug/l

RT: 7.37 min Scan# 1740

Delta R.T. -0.00 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33

Instrument :

MSVOA_N

ClientSampleId :





FILTERBAG-RO

Tot Ion: 83 Resp: 2984

Ion Ratio Lower Upper

83 100

85 43.3 51.4 77.2#

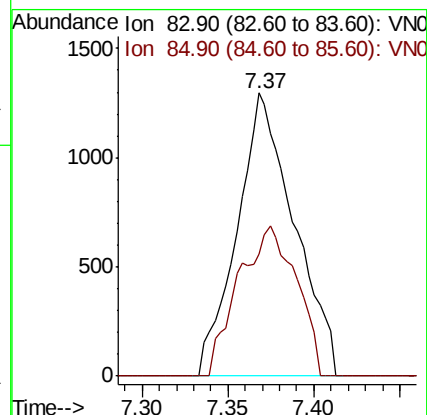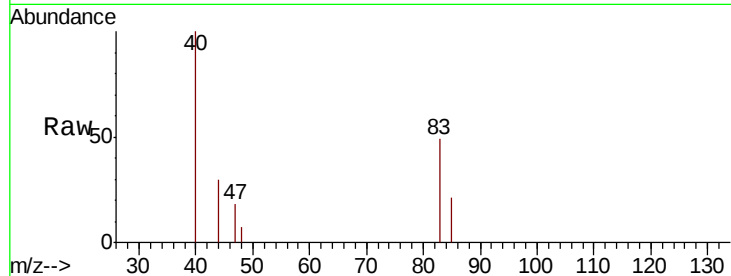

#31

Cyclohexane

Concen: 1.043 ug/l

RT: 7.67 min Scan# 1834

Delta R.T. 0.01 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33




Tgt Ion: 56 Resp: 10229


Ion Ratio Lower Upper

56 100

69 147.8 25.2 37.8#

84 116.1 61.1 91.7#



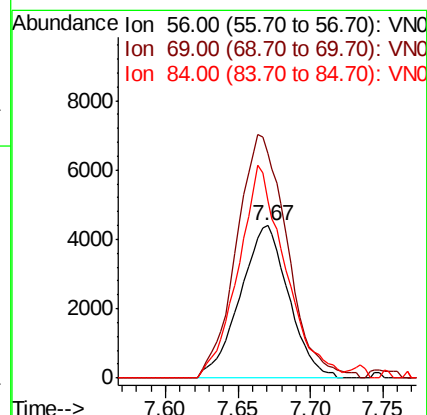



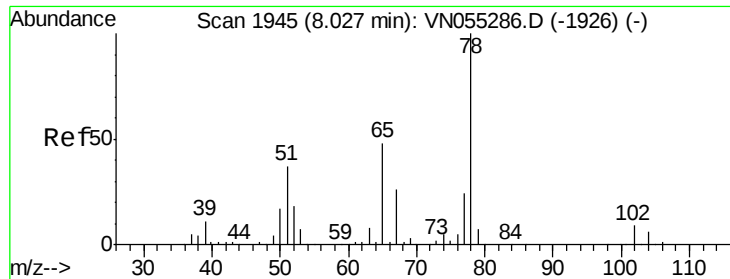

#33
 1,2-Dichloroethane-d4
 Concen: 52.253 ug/l
 RT: 8.03 min Scan# 1945
 Delta R.T. 0.00 min
 Lab File: VN055400.D
 Acq: 3 May 2019 19:33




Instrument :
 MSVOA_N
 ClientSampleId :
 FILTERBAG-RO


Tot Ion: 65 Resp: 325854
 Ion Ratio Lower Upper
 65 100
 67 53.3 0.0 106.8

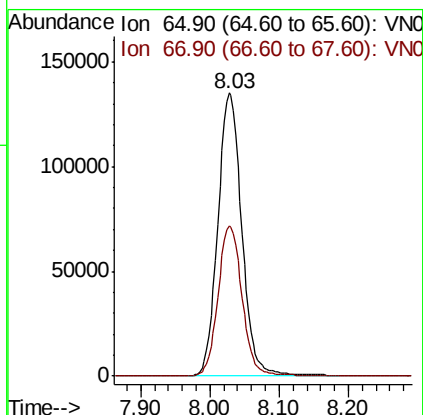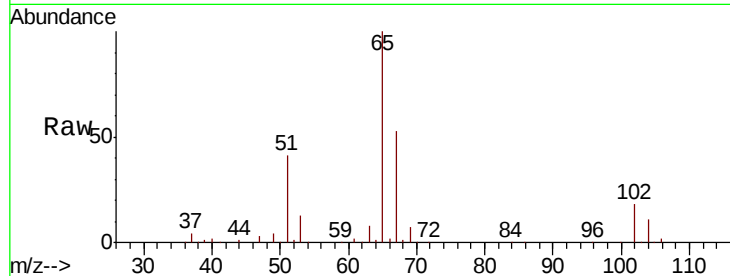

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN055400.D
 Acq: 3 May 2019 19:33

Tgt Ion: 114 Resp: 827268
 Ion Ratio Lower Upper
 114 100
 63 22.9 0.0 45.2
 88 16.1 0.0 31.6


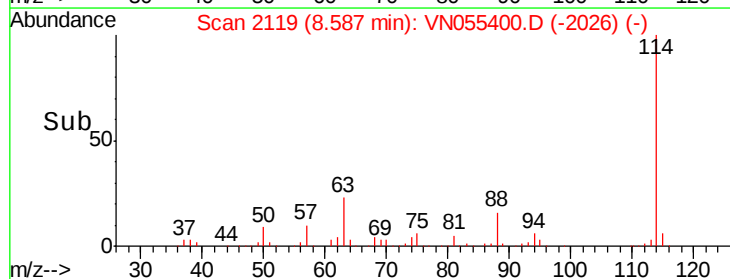
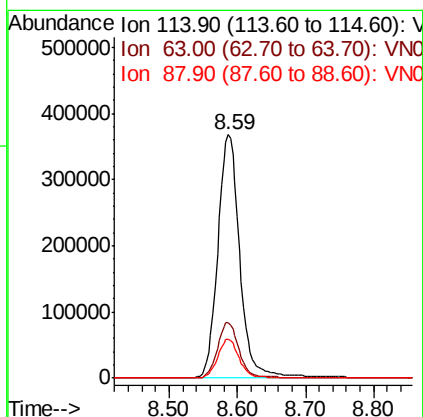





#35
 Dibromofluoromethane
 Concen: 48.168 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. 0.00 min
 Lab File: VN055400.D
 Acq: 3 May 2019 19:33




Instrument :
 MSVOA_N
 ClientSampleId :
 FILTERBAG-RO


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.0	82.3	123.5
192	21.1	17.0	25.6

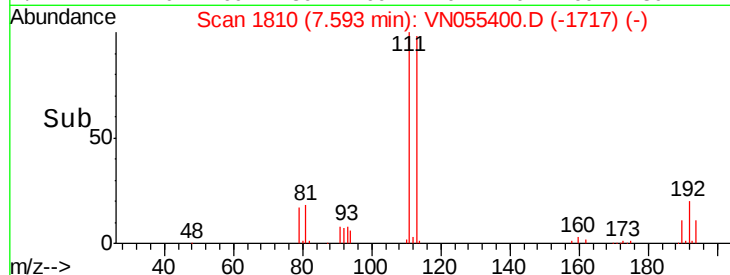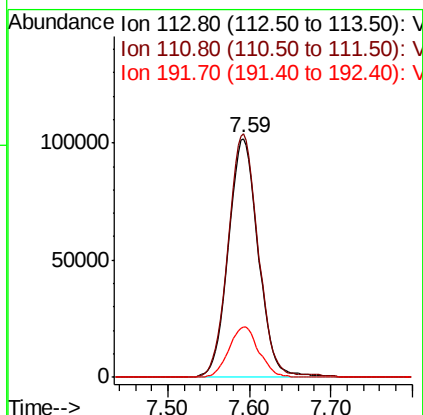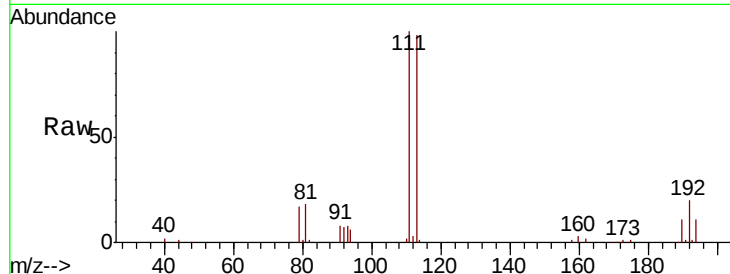

#36
 1,1-Dichloropropene
 Concen: 4.498 ug/l
 RT: 7.66 min Scan# 1832
 Delta R.T. -0.13 min
 Lab File: VN055400.D
 Acq: 3 May 2019 19:33

Tgt Ion	Ratio	Lower	Upper
75	100		
110	8.5	16.8	50.4#
77	0.0	25.0	37.6#

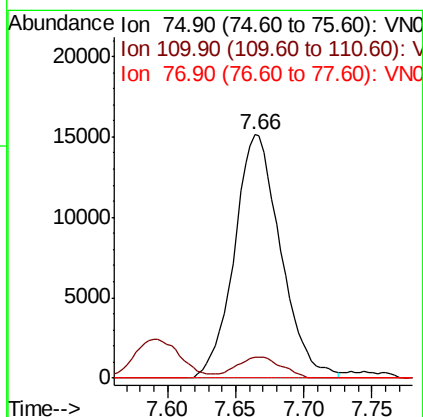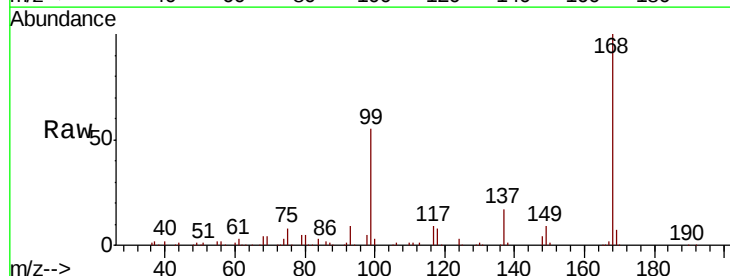

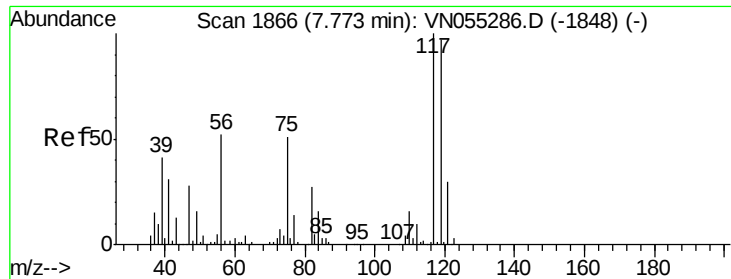

#38

Carbon Tetrachloride

Concen: 5.803 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.11 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33

Instrument :

MSVOA_N

ClientSampleId :

FILTERBAG-RO


Tot Ion:117 Resp: 44358

Ion Ratio Lower Upper

117 100

119 5.0 77.0 115.6#




121 0.0 23.8 35.8#

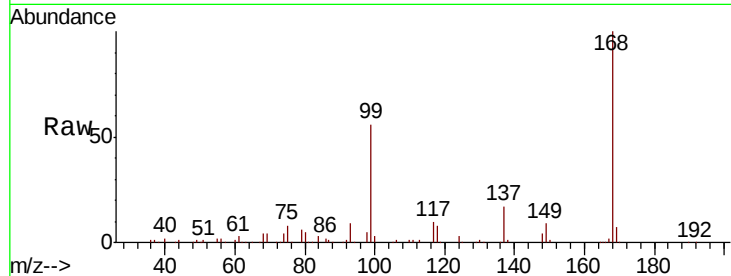

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

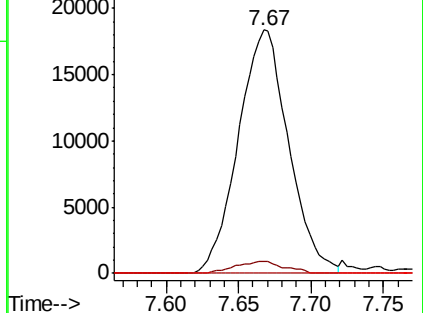

#41

Methacrylonitrile

Concen: 0.850 ug/l

RT: 7.20 min Scan# 1689

Delta R.T. 0.03 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33

Tgt Ion: 41 Resp: 369


Ion Ratio Lower Upper

41 100

39 0.0 48.5 72.7#

67 0.0 54.9 82.3#

52 0.0 24.9 37.3#






Abundance Ion 41.00 (40.70 to 41.70): VNO

Ion 39.00 (38.70 to 39.70): VNO

Ion 67.00 (66.70 to 67.70): VNO

Ion 52.00 (51.70 to 52.70): VNO

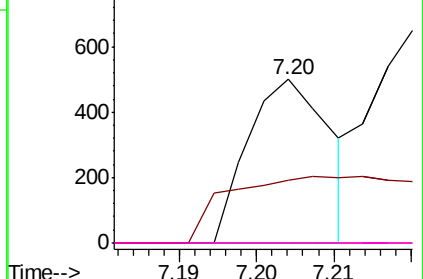



#43

Isopropyl Acetate

Concen: 1.629 ug/l

RT: 8.17 min Scan# 1988

Delta R.T. 0.00 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33

Instrument :

MSVOA_N

ClientSampleId :

FILTERBAG-RO


Tot Ion: 43 Resp: 15895

Ion Ratio Lower Upper

43 100

61 15.1 20.8 31.2#




87 8.8 8.5 12.7

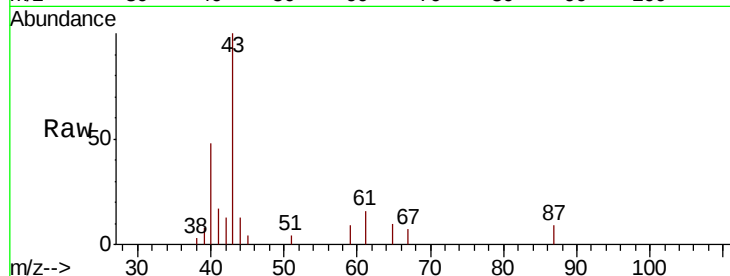

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

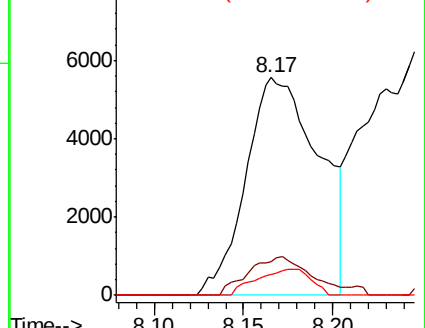

#48

Methyl methacrylate

Concen: 1.449 ug/l

RT: 9.18 min Scan# 2304

Delta R.T. -0.02 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33


Tgt Ion: 41 Resp: 6954

Ion Ratio Lower Upper

41 100

69 0.0 58.6 87.8#



39 22.2 43.8 65.6#




Abundance Ion 41.00 (40.70 to 41.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 39.00 (38.70 to 39.70): VN0

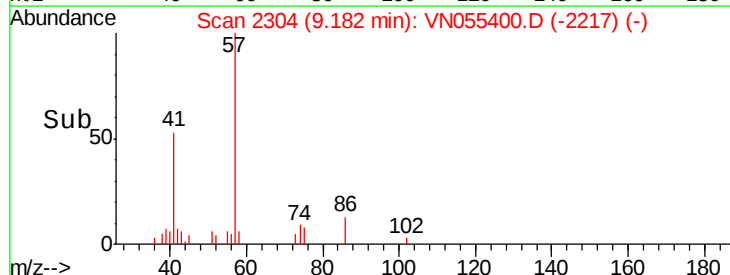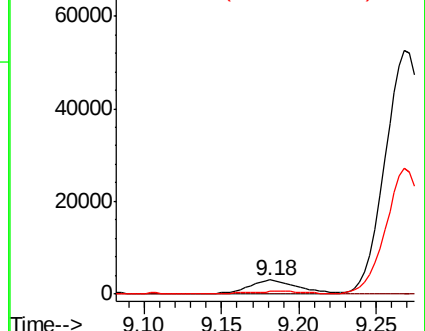

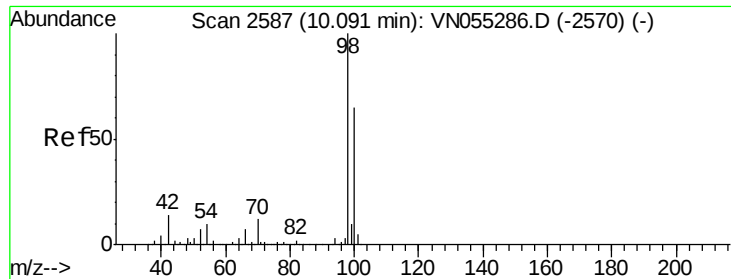

#50

Toluene-d8

Concen: 51.753 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33

Instrument :

MSVOA_N

ClientSampleId :





FILTERBAG-RO

Tot Ion: 98 Resp: 1014715

Ion Ratio Lower Upper

98 100

100 64.1 51.7 77.5

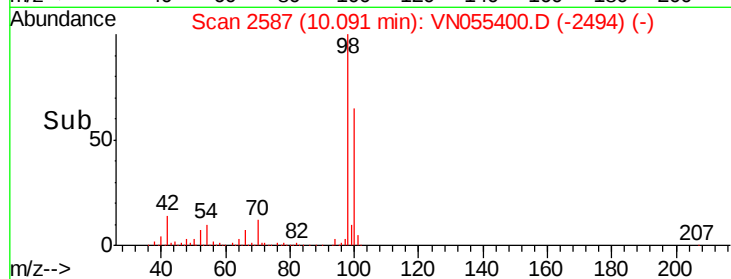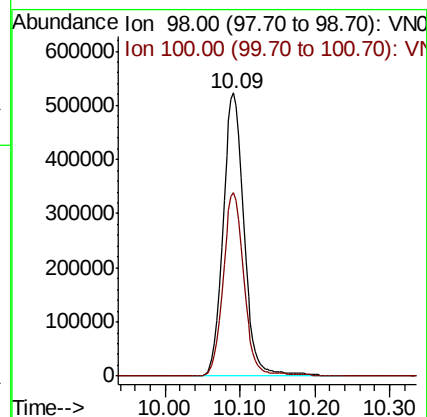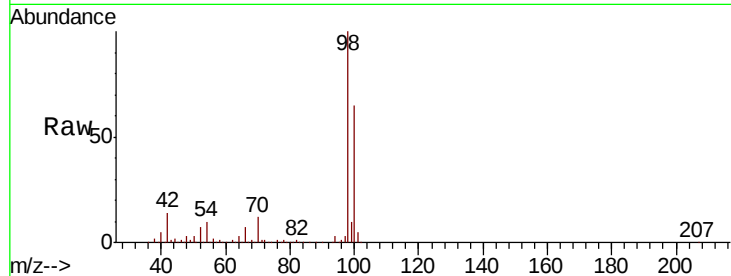

#51

4-Methyl-2-Pentanone

Concen: 1.340 ug/l

RT: 10.02 min Scan# 2566

Delta R.T. 0.04 min

Lab File: VN055400.D




Acq: 3 May 2019 19:33


Tgt Ion: 43 Resp: 7362

Ion Ratio Lower Upper

43 100

58 0.0 28.5 42.7#

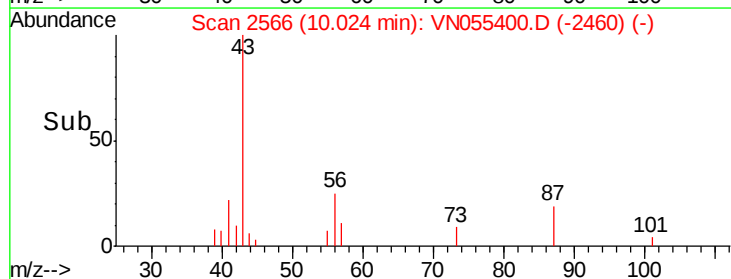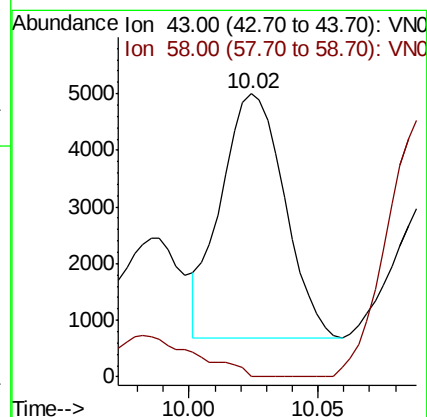

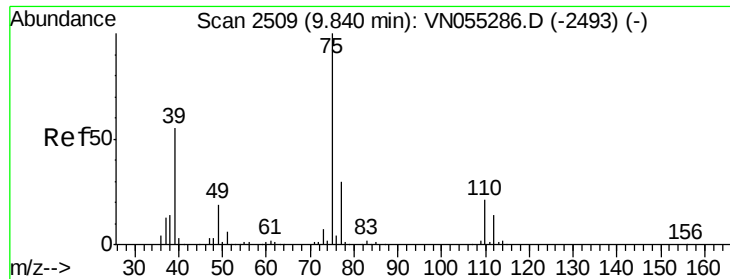

#54

cis-1,3-Dichloropropene

Concen: 5.752 ug/l

RT: 9.90 min Scan# 2529

Delta R.T. 0.06 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33

Instrument :

MSVOA_N

ClientSampleId :

FILTERBAG-RO


Tot Ion: 75 Resp: 49188

Ion Ratio Lower Upper

75 100

77 0.7 24.2 36.2#




39 37.7 44.2 66.2#

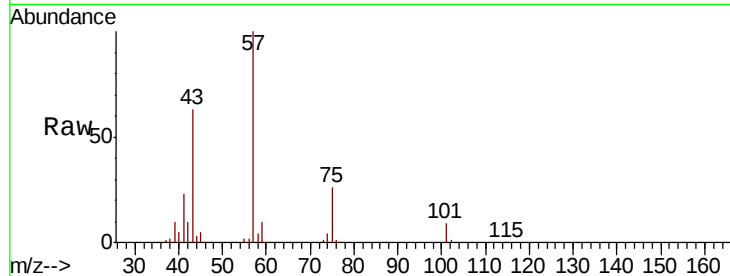

Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 76.90 (76.60 to 77.60): VN0

Ion 39.00 (38.70 to 39.70): VN0

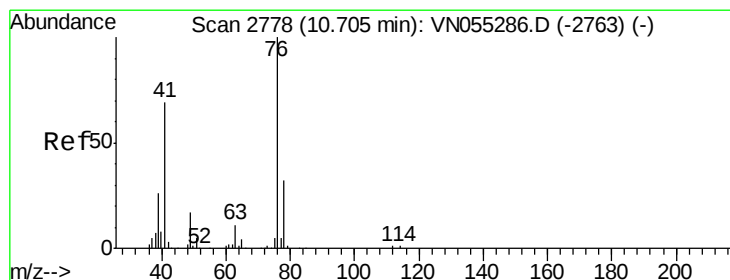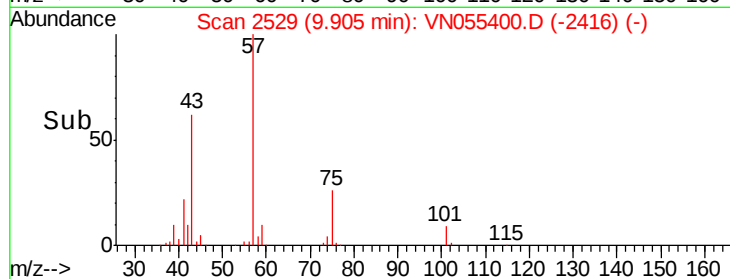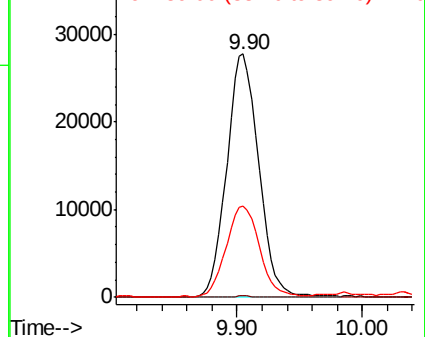

#57

1,3-Dichloropropane

Concen: 0.976 ug/l

RT: 10.76 min Scan# 2796

Delta R.T. 0.06 min

Lab File: VN055400.D


Acq: 3 May 2019 19:33

Tgt Ion: 76 Resp: 8522

Ion Ratio Lower Upper



76 100


78 0.0 25.6 38.4#



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0




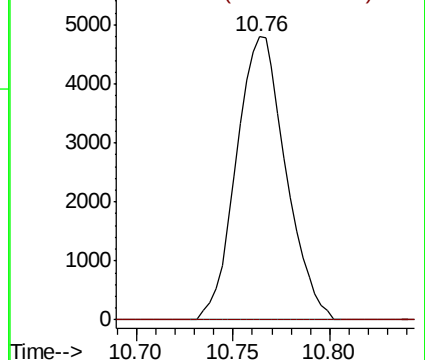




#59
2-Hexanone
Concen: 40.357 ug/l
RT: 10.76 min Scan# 2796
Delta R.T. 0.01 min
Lab File: VN055400.D
Acq: 3 May 2019 19:33




Instrument :
MSVOA_N
ClientSampleId :
FILTERBAG-RO


Tot Ion: 43 Resp: 138749
Ion Ratio Lower Upper
43 100
58 17.8 24.9 74.6#

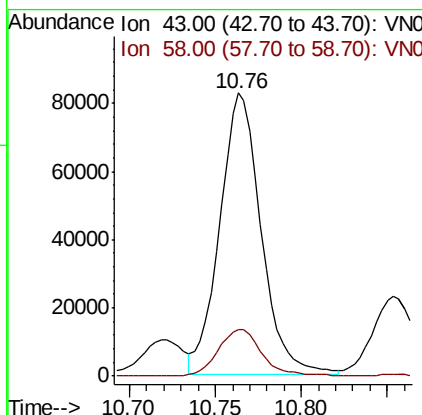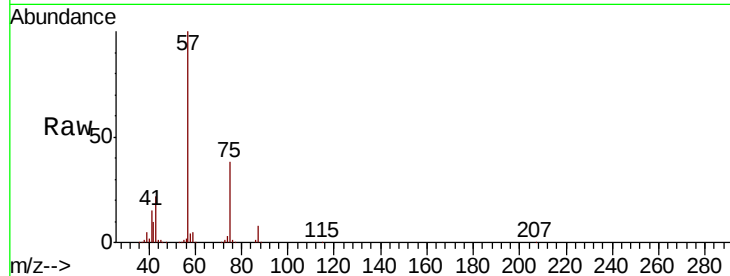

#62
4-Bromofluorobenzene
Concen: 54.025 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. 0.00 min
Lab File: VN055400.D
Acq: 3 May 2019 19:33

Tgt Ion: 95 Resp: 331057
Ion Ratio Lower Upper
95 100
174 83.4 0.0 166.6
176 80.2 0.0 157.8

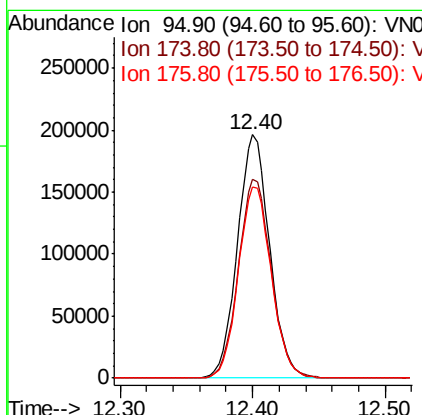


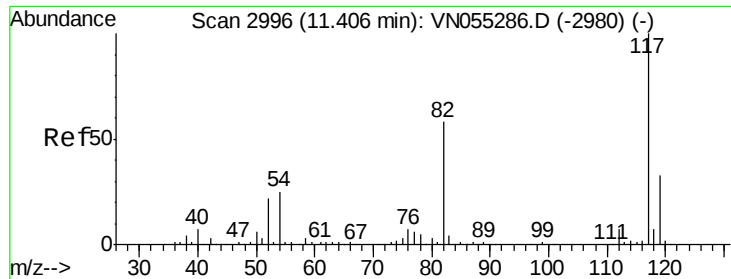




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN055400.D
Acq: 3 May 2019 19:33

Instrument :
MSVOA_N
ClientSampled :
FILTERBAG-RO

Tot Ion:117 Resp: 751707
Ion Ratio Lower Upper
117 100
82 57.8 46.2 69.4
119 32.3 26.6 40.0

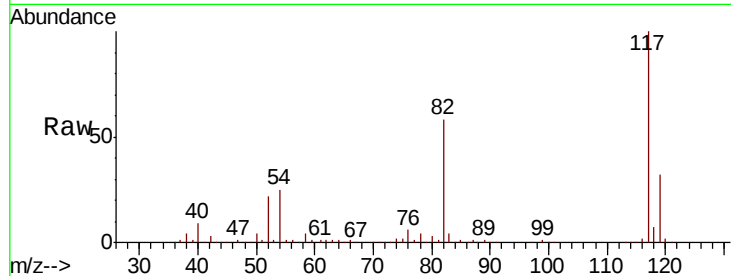


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

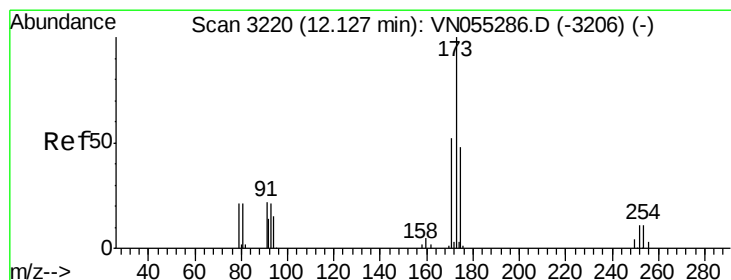
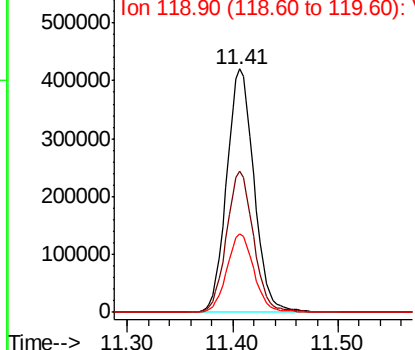



#71
Bromoform
Concen: 0.588 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. 0.27 min
Lab File: VN055400.D
Acq: 3 May 2019 19:33

Tgt Ion:173 Resp: 1878
Ion Ratio Lower Upper
173 100
175 956.4 23.6 71.0#
254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

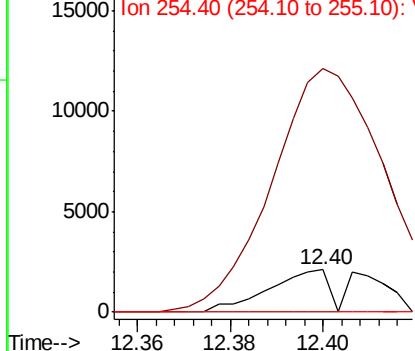

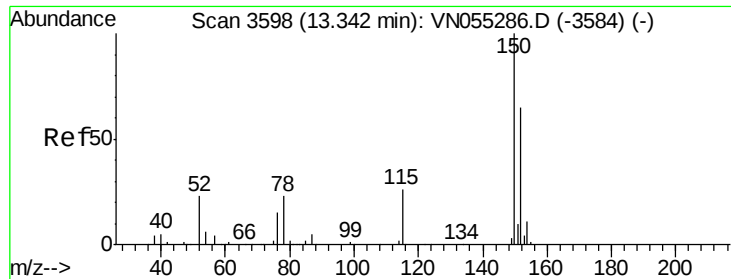

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. 0.00 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33

Instrument :

MSVOA_N

ClientSampled :

FILTERBAG-RO


Tot Ion:152 Resp: 229134

Ion Ratio Lower Upper

152 100

115 58.6 29.0 87.0




150 156.6 0.0 345.6

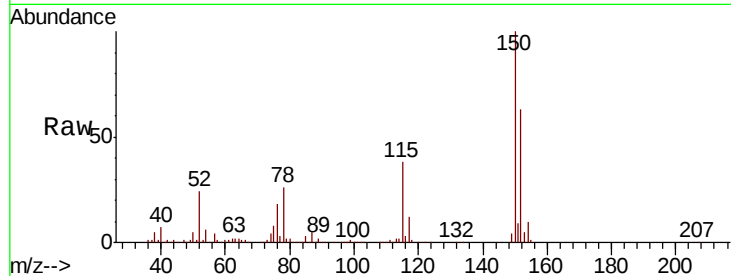

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

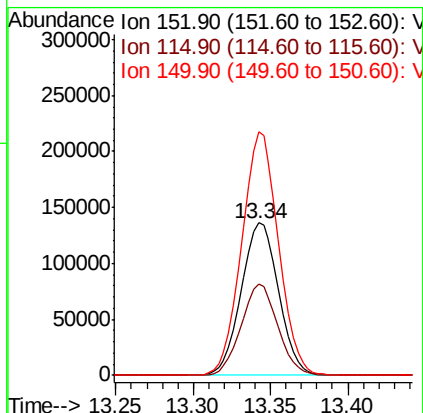

#73

Isopropylbenzene

Concen: Below Cal

RT: 12.24 min Scan# 3256

Delta R.T. -0.01 min

Lab File: VN055400.D


Acq: 3 May 2019 19:33

Tgt Ion:105 Resp: 117

Ion Ratio Lower Upper



105 100


120 0.0 12.9 38.7#



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

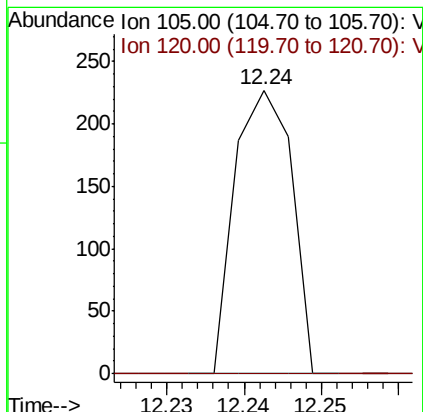



#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.70 min Scan# 3399

Delta R.T. 0.20 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33

Instrument :

MSVOA_N

ClientSampleId :

FILTERBAG-RO


Tot Ion: 83 Resp: 67

Ion Ratio Lower Upper

83 100

131 0.0 5.1 15.2#




85 0.0 32.3 96.8#

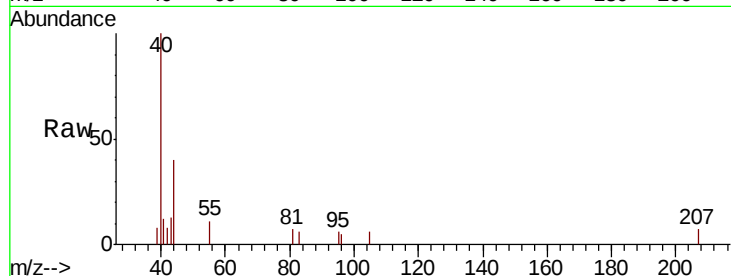

Abundance Ion 82.90 (82.60 to 83.60): VN055286.D (-3322) (-)

Ion 130.80 (130.50 to 131.50): VN055286.D (-3322) (-)

Ion 84.90 (84.60 to 85.60): VN055286.D (-3322) (-)

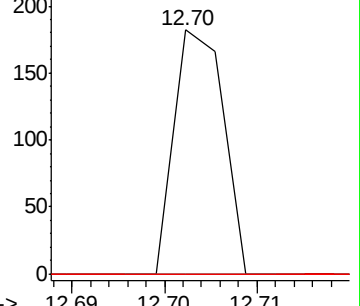

#76

1,2,3-Trichloropropane

Concen: 39.597 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.15 min

Lab File: VN055400.D


Acq: 3 May 2019 19:33

Tgt Ion: 75 Resp: 170877

Ion Ratio Lower Upper



75 100


77 1.2 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN055286.D (-3346) (-)

Ion 77.00 (76.70 to 77.70): VN055286.D (-3346) (-)




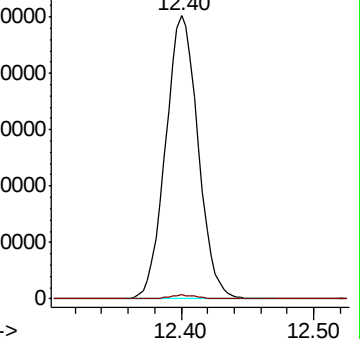




#79
 2-Chlorotoluene
 Concen: Below Cal
 RT: 12.73 min Scan# 3408
 Delta R.T. 0.06 min
 Lab File: VN055400.D
 Acq: 3 May 2019 19:33




Instrument :
 MSVOA_N
 ClientSampleId :
 FILTERBAG-RO


Tot Ion: 91 Resp: 458
 Ion Ratio Lower Upper
 91 100
 126 0.0 16.6 49.7#

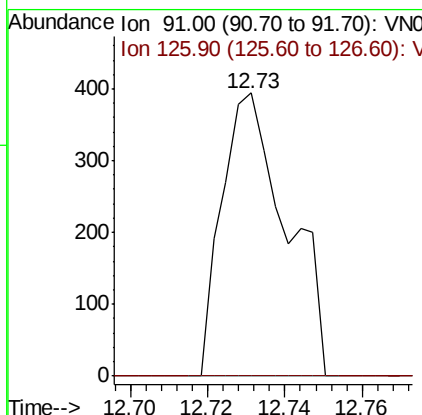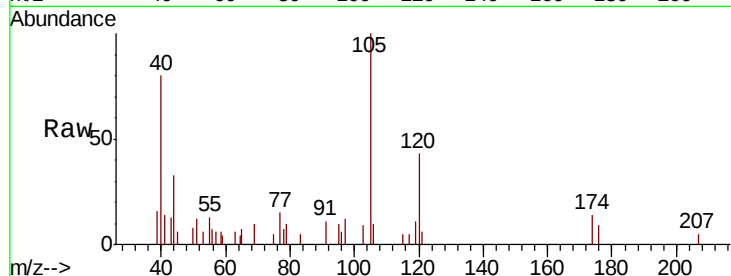

#80
 1,3,5-Trimethylbenzene
 Concen: 0.313 ug/l
 RT: 12.73 min Scan# 3408
 Delta R.T. 0.00 min
 Lab File: VN055400.D
 Acq: 3 May 2019 19:33

Tgt Ion: 105 Resp: 5629
 Ion Ratio Lower Upper
 105 100
 120 42.2 23.4 70.0

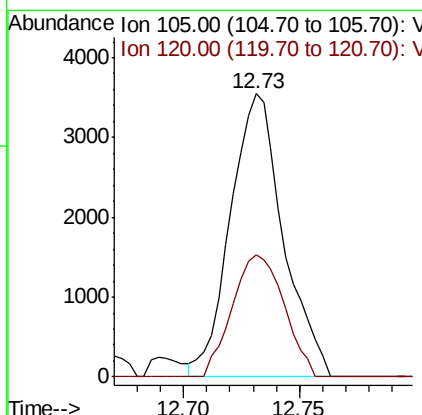



#81

trans-1,4-Dichloro-2-butene

Concen: 141.325 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.10 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33

Instrument :

MSVOA_N

ClientSampleId :

FILTERBAG-RO


Tot Ion: 75 Resp: 170877

Ion Ratio Lower Upper

75 100

53 0.0 86.3 129.5#




89 0.0 34.6 51.8#



Abundance Ion 74.90 (74.60 to 75.60): VN055400.D (-3305) (-)

Ion 53.00 (52.70 to 53.70): VN055400.D (-3305) (-)

Ion 88.90 (88.60 to 89.60): VN055400.D (-3305) (-)

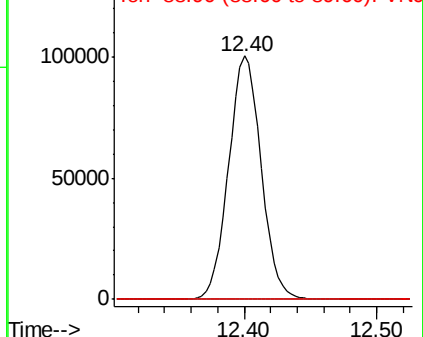

#83

tert-Butylbenzene

Concen: Below Cal

RT: 13.05 min Scan# 3507

Delta R.T. 0.06 min

Lab File: VN055400.D

Acq: 3 May 2019 19:33


Tgt Ion: 119 Resp: 190

Ion Ratio Lower Upper

119 100

91 0.0 34.3 102.9#



134 0.0 13.1 39.3#




Abundance Ion 119.00 (118.70 to 119.70): VN055400.D (-3507) (-)

Ion 91.00 (90.70 to 91.70): VN055400.D (-3507) (-)

Ion 134.00 (133.70 to 134.70): VN055400.D (-3507) (-)

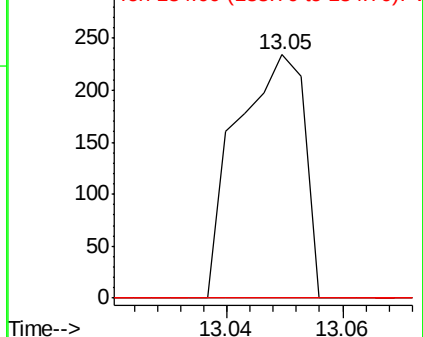

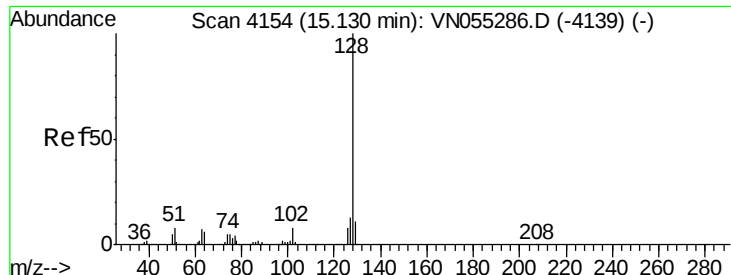

#95

Naphthalene

Concen: 3.351 ug/l

RT: 15.13 min Scan# 4153

Delta R.T. -0.00 min

Lab File: VN055400.D


Acq: 3 May 2019 19:33

Instrument :

MSVOA_N

ClientSampleId :

FILTERBAG-RO

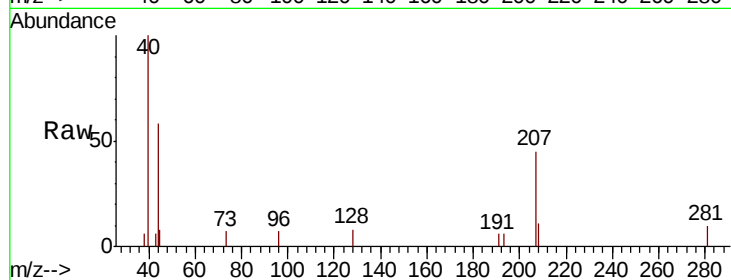


Tot Ion:128 Resp: 158

Ion Ratio Lower Upper

128 100

127 0.0 10.7 16.1#

129 0.0 8.6 13.0#

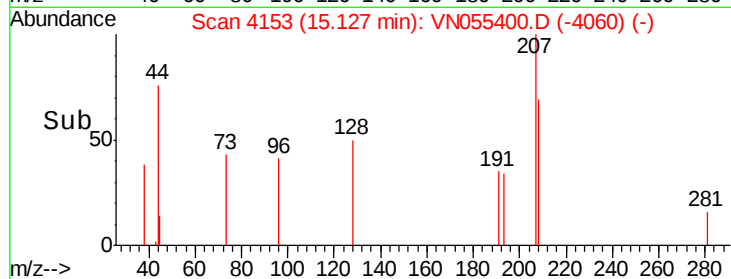

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

