


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN050319\
 Data File : VN055375.D
 Acq On : 3 May 2019 8:55
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
 Title : SW846 8260
 Last Update : Tue Apr 30 07:16:52 2019

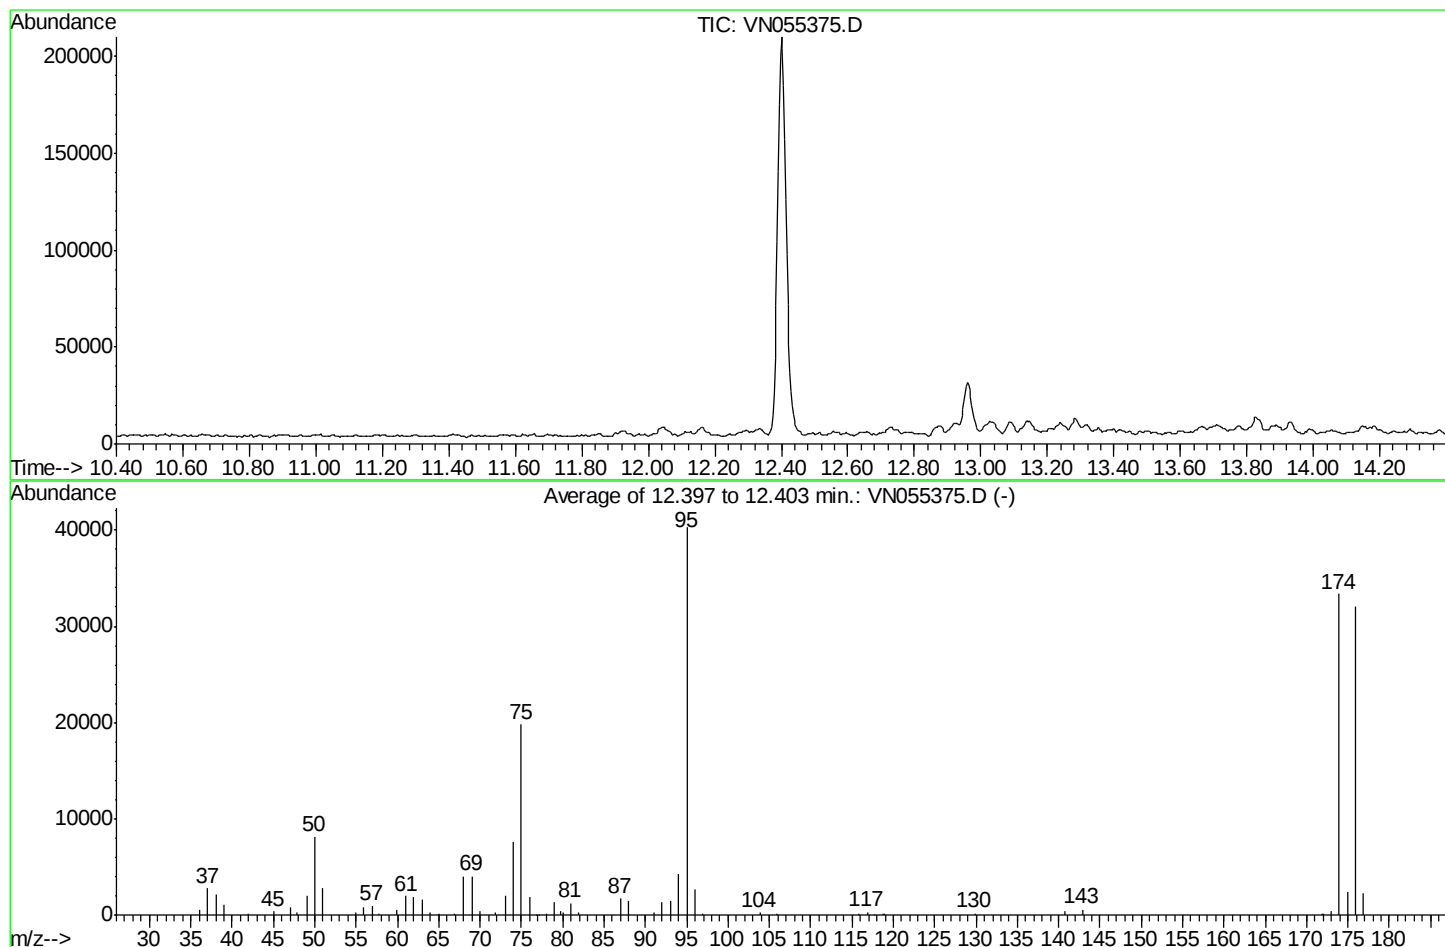

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	8170	PASS
75	95	30	60	49.2	19821	PASS
95	95	100	100	100.0	40290	PASS
96	95	5	9	6.6	2658	PASS
173	174	0.00	2	1.2	396	PASS
174	95	50	100	82.8	33378	PASS
175	174	5	9	7.2	2407	PASS
176	174	95	101	96.2	32117	PASS
177	176	5	9	6.9	2224	PASS