
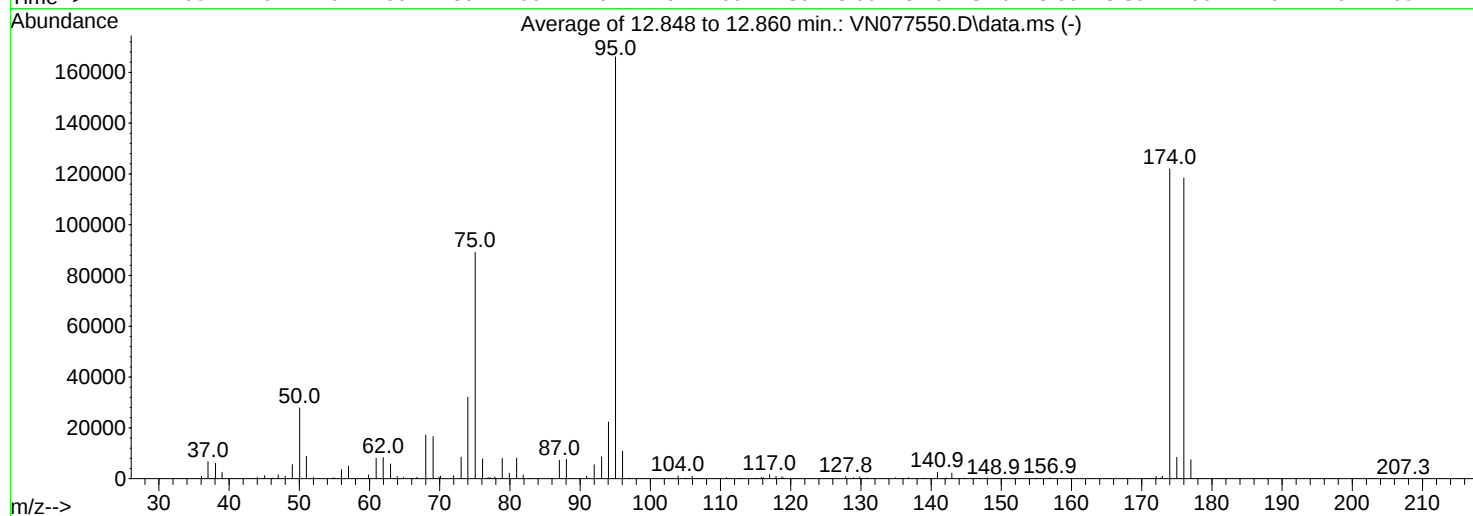


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050323\
Data File : VN077550.D
Acq On : 03 May 2023 09:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042423W.M
Title : SW846 8260
Last Update : Tue Apr 25 02:50:59 2023

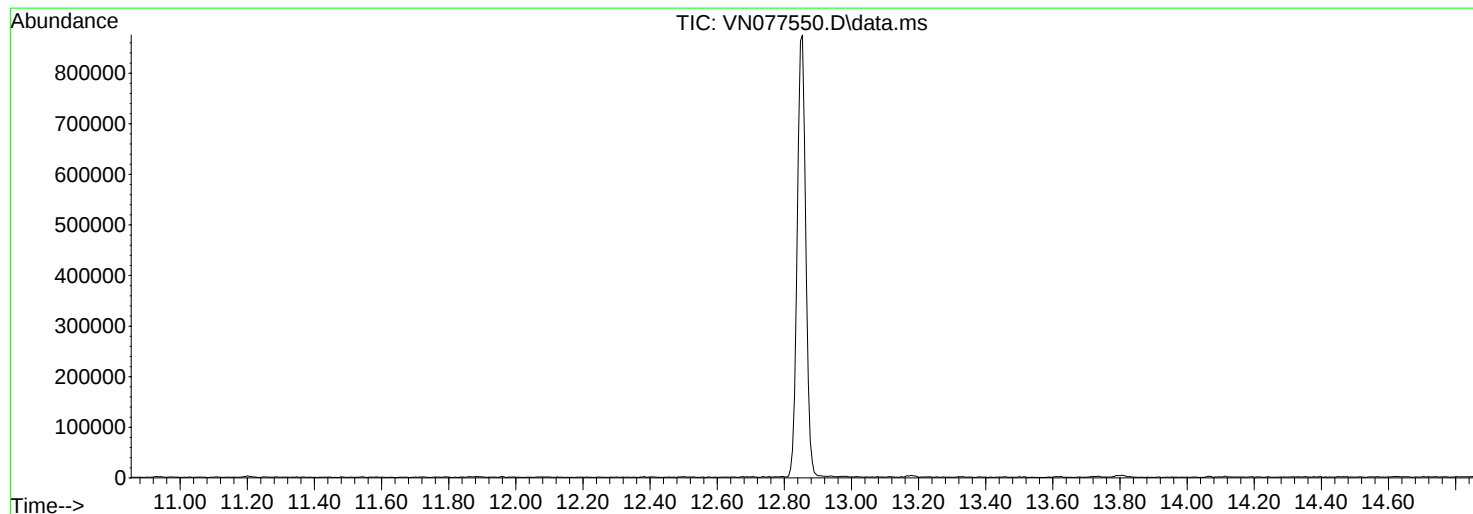

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	27837	PASS
75	95	30	60	53.7	89165	PASS
95	95	100	100	100.0	166123	PASS
96	95	5	9	6.5	10844	PASS
173	174	0.00	2	0.8	1005	PASS
174	95	50	100	73.4	122011	PASS
175	174	5	9	6.9	8387	PASS
176	174	95	101	97.1	118424	PASS
177	176	5	9	6.3	7450	PASS

Average of 12.848 to 12.860 min.: VN077550.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	957	50.05	27837	61.95	8320	73.05	843
37.00	6715	51.00	8786	63.00	5807	74.00	3209
38.05	6060	52.00	574	63.95	873	75.05	8916
39.00	2510	54.80	244	64.85	535	76.10	783
41.10	54	55.00	236	66.10	70	76.80	259
44.00	549	56.00	3548	66.75	487	77.00	404
45.05	1213	57.00	4950	68.00	17122	77.20	289
46.15	192	57.80	71	69.05	16579	77.85	686
47.00	1513	58.20	117	69.90	644	78.90	8039
48.00	985	59.85	1452	70.10	948	79.90	2126
49.00	5560	60.95	7978	71.95	1114	80.95	8145

Average of 12.848 to 12.860 min.: VN077550.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.90	1478	96.05	10844	115.80	451	134.90	366
82.70	51	97.00	211	116.10	425	135.70	76
82.90	122	103.95	1109	117.00	1608	136.80	368
86.00	178	105.00	173	117.90	891	138.90	187
87.05	7237	105.95	946	118.75	675	139.80	59
88.05	7633	106.80	123	119.00	315	140.90	2513
90.95	972	110.85	354	127.85	823	141.70	52
92.00	5502	112.10	70	128.95	425	142.15	226
93.05	8593	112.70	170	129.85	678	142.95	2209
94.05	22312	113.05	157	130.10	109	143.90	137
95.05	166123	114.95	212	130.95	260	144.80	214

Average of 12.848 to 12.860 min.: VN077550.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
145.70	128	161.00	90	207.30	61		
146.90	189	170.00	146				
147.60	56	171.10	100				
148.05	328	172.05	860				
148.90	61	172.70	295				
149.70	129	172.95	1005				
151.90	54	174.00	122011				
154.80	103	175.00	8387				
155.05	272	176.00	118424				
156.95	274	177.00	7450				
158.90	85	177.90	120				

Instrument :

MSVOA_N

ClientSampleId :

BFB