
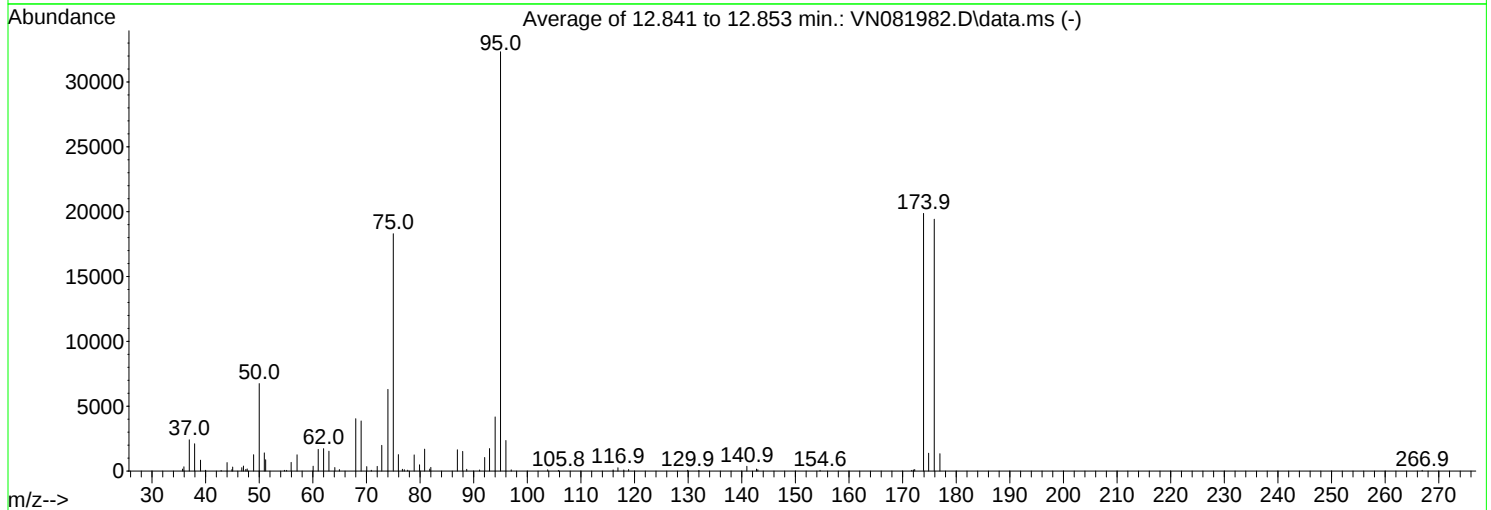


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050324\
Data File : VN081982.D
Acq On : 03 May 2024 08:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Title : SW846 8260
Last Update : Fri Apr 26 05:26:49 2024

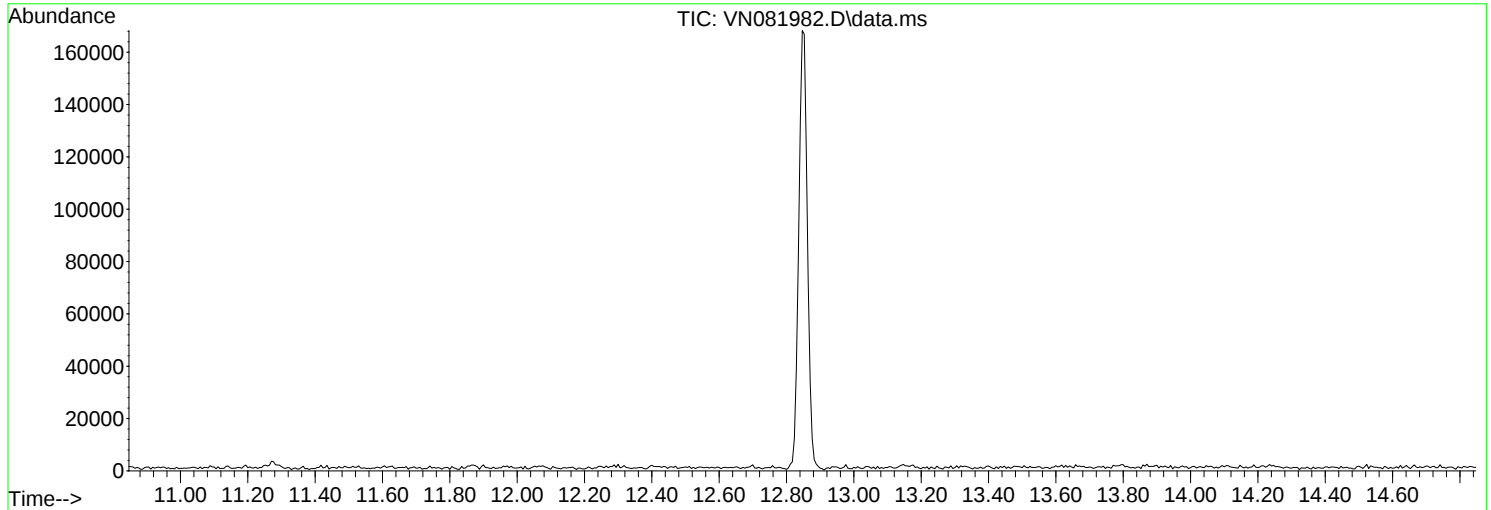

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	6747	PASS
75	95	30	60	56.6	18300	PASS
95	95	100	100	100.0	32331	PASS
96	95	5	9	7.3	2358	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	61.5	19868	PASS
175	174	5	9	6.9	1377	PASS
176	174	95	101	97.8	19421	PASS
177	176	5	9	6.9	1340	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.70	155	47.05	390	60.05	379	72.85	1983
35.95	329	47.50	131	61.00	1673	74.00	6300
36.95	2415	47.75	166	62.00	1729	75.00	18300
37.95	2106	48.95	1262	63.00	1535	75.95	1271
39.05	842	50.00	6747	64.10	275	76.70	141
40.00	65	50.95	1402	64.95	116	77.05	107
42.90	53	51.20	874	68.00	4038	77.70	73
44.00	655	54.70	61	69.00	3865	78.90	1246
44.90	112	55.10	57	70.05	344	79.90	486
45.05	310	55.95	671	70.90	64	80.85	1690
46.75	264	57.05	1256	72.00	363	81.80	155

Average of 12.841 to 12.853 min.: VN081982.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
82.00	285	103.80	101	154.60	59		
86.95	1644	105.80	53	171.70	57		
87.95	1518	116.00	91	172.00	90		
88.70	139	116.90	254	172.25	124		
91.10	87	118.00	91	173.90	19868		
92.05	1047	118.90	122	174.85	1377		
92.95	1737	129.90	62	175.90	19421		
94.00	4175	132.00	52	176.95	1340		
95.00	32331	140.95	370	266.90	61		
96.00	2358	142.75	155				
97.00	96	143.00	105				

Instrument :
MSVOA_N
ClientSampleId :
BFB