


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050421\
Data File : VN066925.D
Acq On : 4 May 2021 9:43
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N050421W.M
Title : SW846 8260
Last Update : Wed May 05 07:24:52 2021

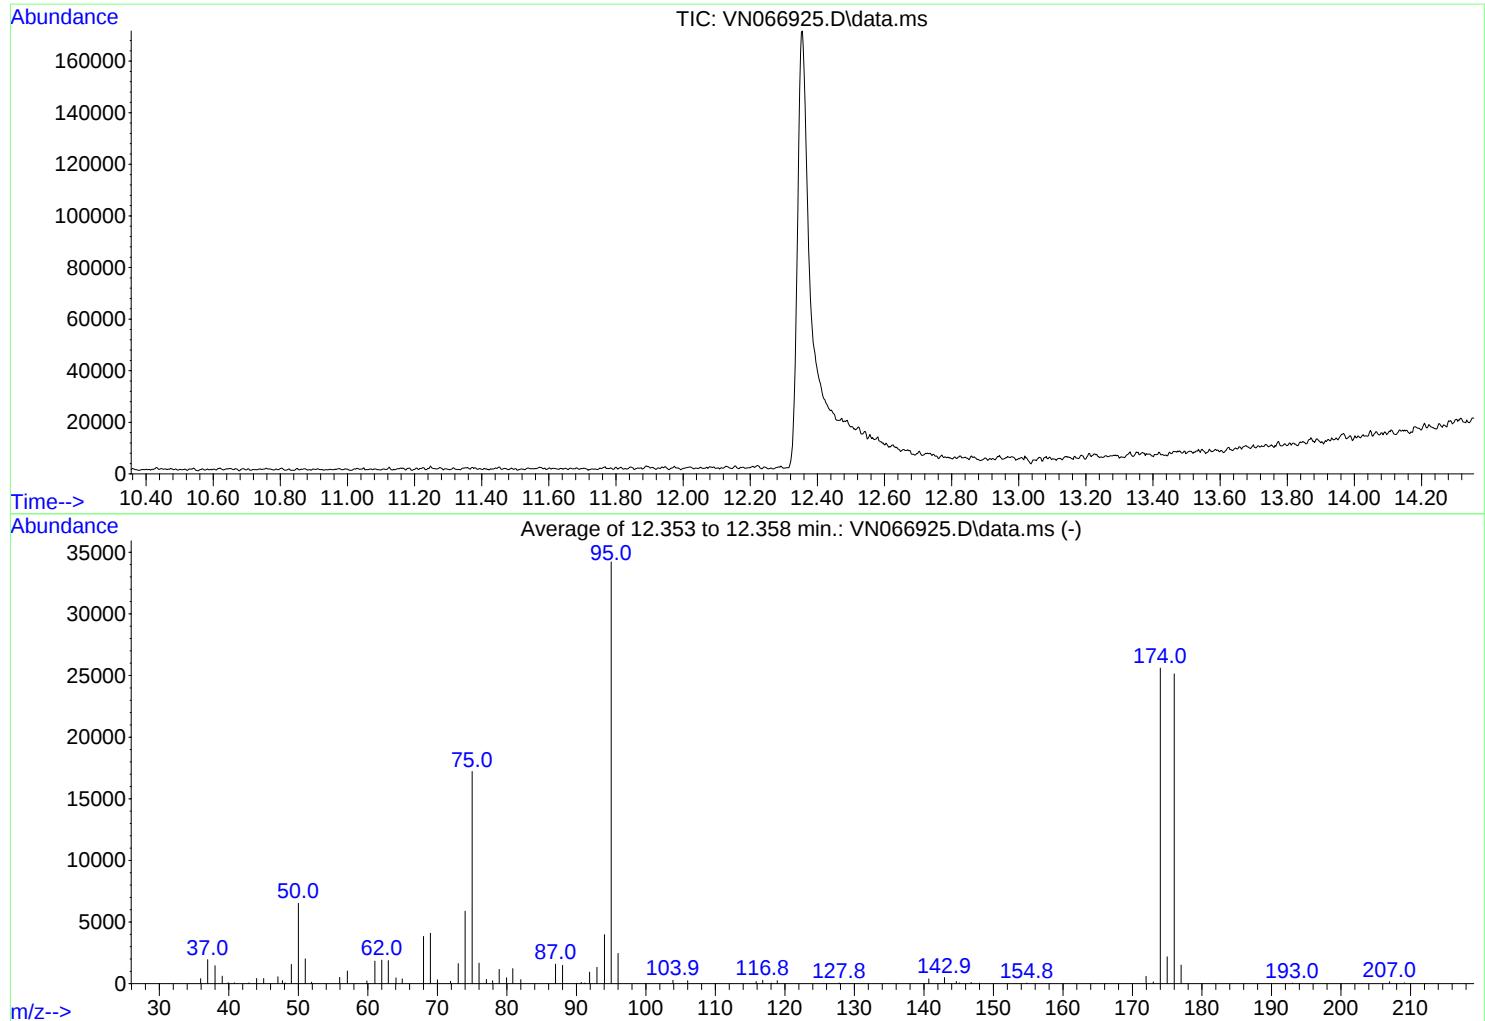

AutoFind: Scans 3951, 3952, 3953; Background Corrected with Scan 3935

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	6521	PASS
75	95	30	60	50.3	17216	PASS
95	95	100	100	100.0	34227	PASS
96	95	5	9	7.2	2450	PASS
173	174	0.00	2	0.6	149	PASS
174	95	50	100	74.8	25608	PASS
175	174	5	9	8.5	2183	PASS
176	174	95	101	98.2	25141	PASS
177	176	5	9	6.0	1504	PASS