
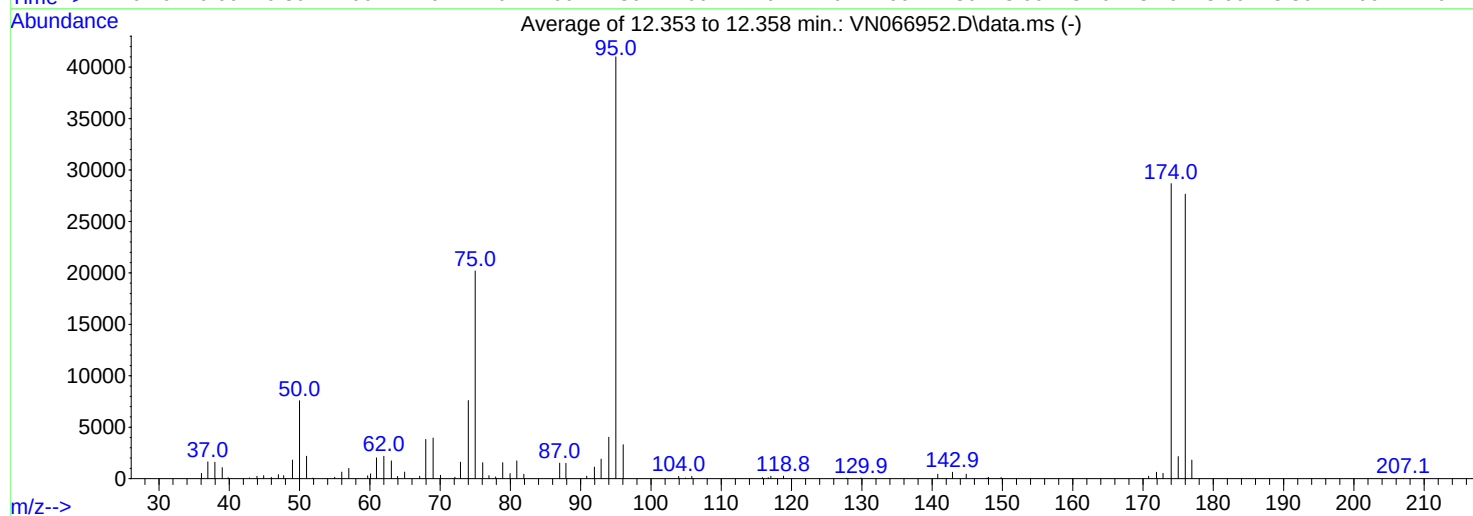


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050421\
Data File : VN066952.D
Acq On : 4 May 2021 21:55
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N050421W.M
Title : SW846 8260
Last Update : Wed May 05 07:24:52 2021

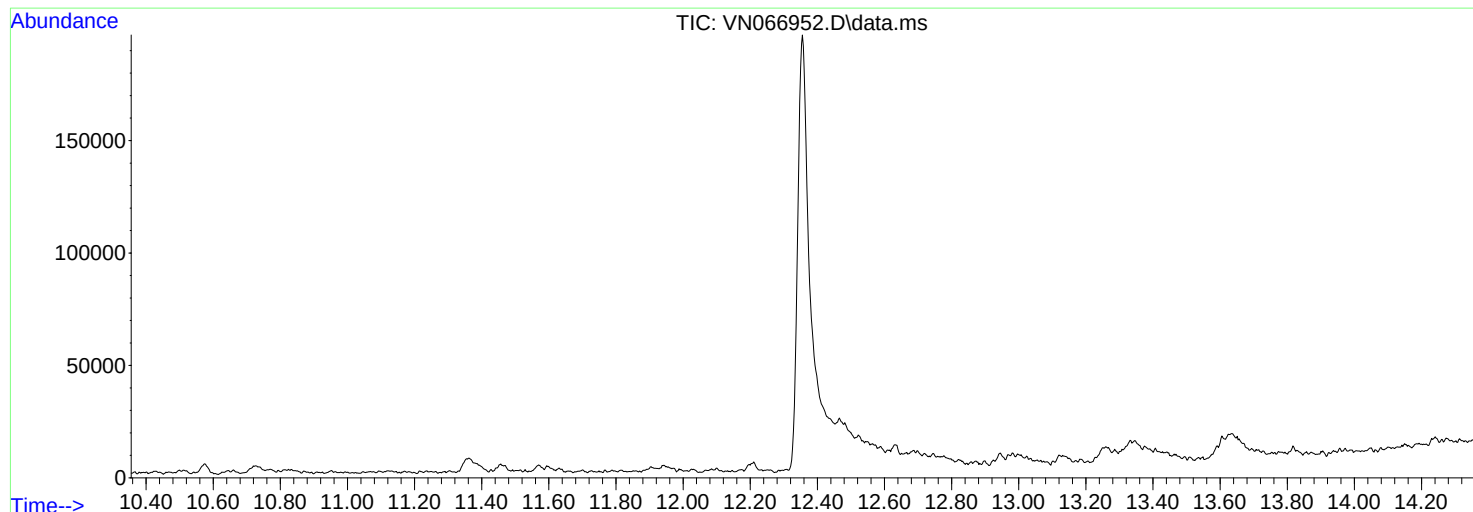

AutoFind: Scans 3951, 3952, 3953; Background Corrected with Scan 3934

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	7572	PASS
75	95	30	60	49.2	20187	PASS
95	95	100	100	100.0	41003	PASS
96	95	5	9	8.0	3294	PASS
173	174	0.00	2	1.8	506	PASS
174	95	50	100	69.9	28677	PASS
175	174	5	9	7.5	2148	PASS
176	174	95	101	96.4	27651	PASS
177	176	5	9	6.5	1801	PASS