
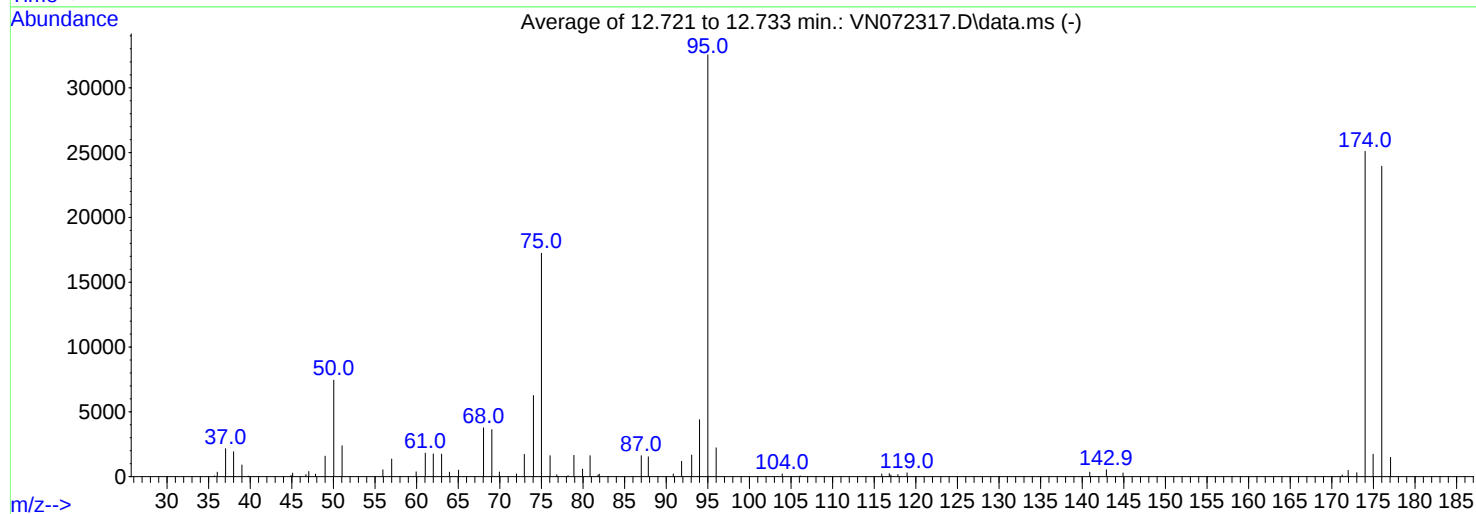


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050422\
Data File : VN072317.D
Acq On : 04 May 2022 10:04
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Title : SW846 8260
Last Update : Tue Apr 26 18:50:11 2022

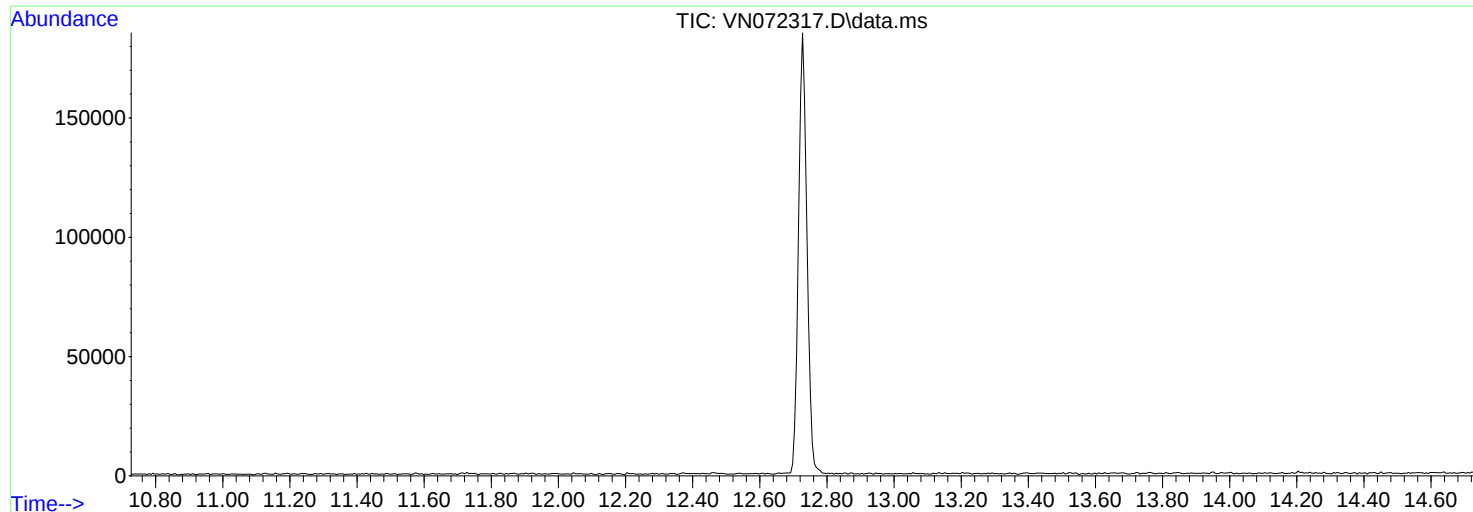

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.9	7440	PASS
75	95	30	60	53.0	17235	PASS
95	95	100	100	100.0	32539	PASS
96	95	5	9	6.8	2224	PASS
173	174	0.00	2	1.2	305	PASS
174	95	50	100	77.1	25093	PASS
175	174	5	9	6.9	1729	PASS
176	174	95	101	95.4	23944	PASS
177	176	5	9	6.3	1498	PASS