
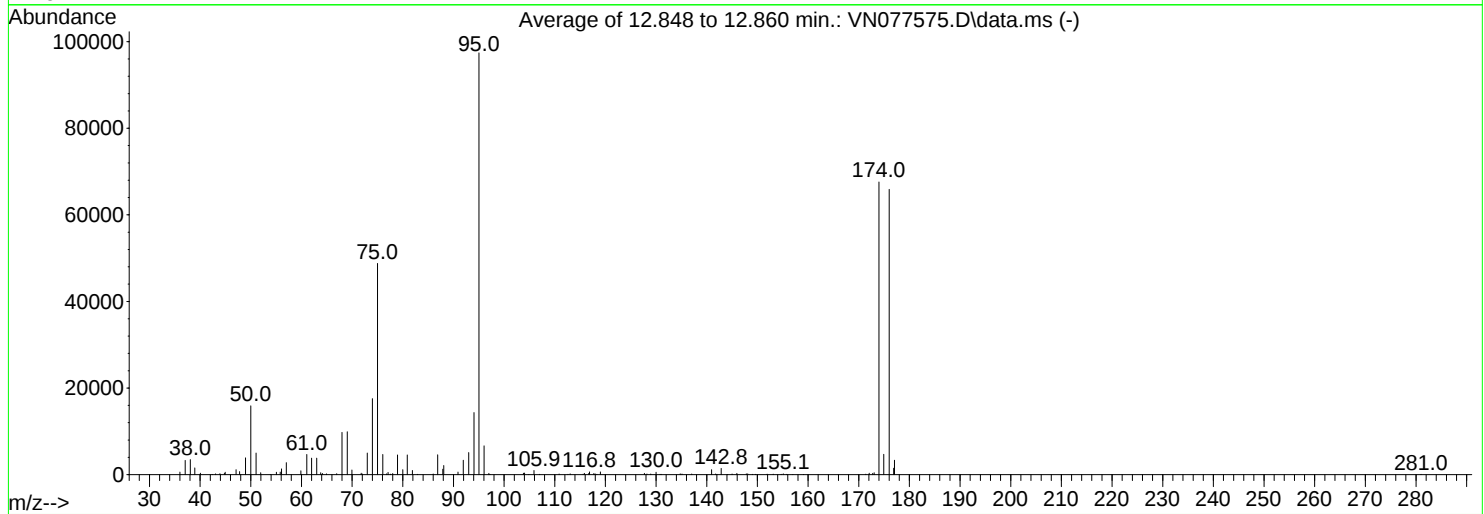


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050423\
Data File : VN077575.D
Acq On : 04 May 2023 09:00
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042423W.M
Title : SW846 8260
Last Update : Tue Apr 25 02:50:59 2023

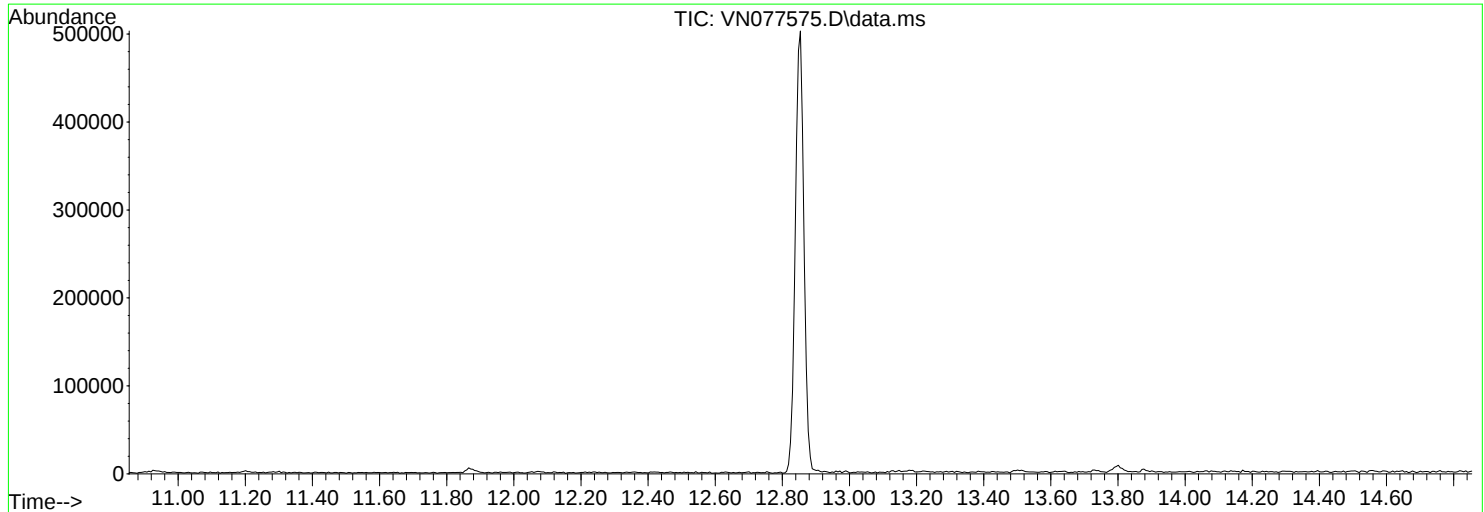

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	15895	PASS
75	95	30	60	50.1	48763	PASS
95	95	100	100	100.0	97413	PASS
96	95	5	9	6.8	6647	PASS
173	174	0.00	2	0.6	429	PASS
174	95	50	100	69.4	67605	PASS
175	174	5	9	7.0	4714	PASS
176	174	95	101	97.4	65880	PASS
177	176	5	9	5.1	3341	PASS

Average of 12.848 to 12.860 min.: VN077575.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	596	47.80	702	61.05	4655	72.00	131
37.05	3291	48.95	3887	62.00	3810	73.00	499
38.05	3481	50.00	15895	63.00	3826	74.00	1757
38.95	1546	51.05	4985	63.80	428	75.00	4876
40.05	352	51.95	437	64.15	253	76.05	4649
42.40	52	53.90	52	64.95	202	76.80	183
43.05	184	55.05	543	66.95	211	77.10	504
43.90	242	55.80	598	68.00	9753	77.60	98
44.80	282	56.05	1318	69.05	9908	78.00	258
44.95	559	57.00	2773	69.95	1073	78.95	4542
47.10	1134	59.90	904	71.80	322	80.00	1148

Average of 12.848 to 12.860 min.: VN077575.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	4550	95.05	97413	113.05	182	128.95	144
81.90	973	96.05	6647	115.60	121	130.00	575
82.90	60	97.00	291	115.85	294	130.80	88
86.00	152	97.20	54	116.70	276	131.00	65
86.90	4603	103.80	317	116.85	641	134.75	193
87.90	1242	104.05	361	117.70	274	135.10	159
88.10	2119	104.90	50	117.95	203	137.05	166
90.90	591	105.90	951	118.30	93	140.95	1133
91.95	3325	107.00	65	119.00	631	141.75	146
93.00	5113	110.85	134	127.70	312	142.00	68
94.05	14324	112.60	80	128.20	139	142.85	1438

Average of 12.848 to 12.860 min.: VN077575.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
144.10	55	155.80	61	177.05	3341		
145.00	161	157.00	57	281.00	67		
145.95	284	159.10	59				
147.80	196	171.40	130				
148.10	180	172.05	341				
149.00	60	172.75	312				
149.60	83	173.05	429				
151.90	112	174.00	67605				
153.10	109	174.95	4714				
154.70	75	176.00	65880				
155.10	199	176.90	1481				

Instrument :

MSVOA_N

ClientSampleId :

BFB