

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050523\
 Data File : VN077598.D
 Acq On : 05 May 2023 18:30
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: May 06 02:35:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042823W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Apr 28 16:20:59 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	7.819	128	50876	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.107	114	336119	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.866	117	316101	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.584	65	145658	32.114	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	107.033%
60) 4-Bromofluorobenzene	12.854	95	119013	21.490	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	71.633%
63) Toluene-d8	10.566	98	350582	31.475	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	104.900%
Target Compounds						
					Qvalue	
55) 2-Chloroethyl vinyl ether	10.166	63	4421	1.722	ug/l #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050523\
Data File : VN077598.D
Acq On : 05 May 2023 18:30
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: May 06 02:35:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042823W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Apr 28 16:20:59 2023
Response via : Initial Calibration

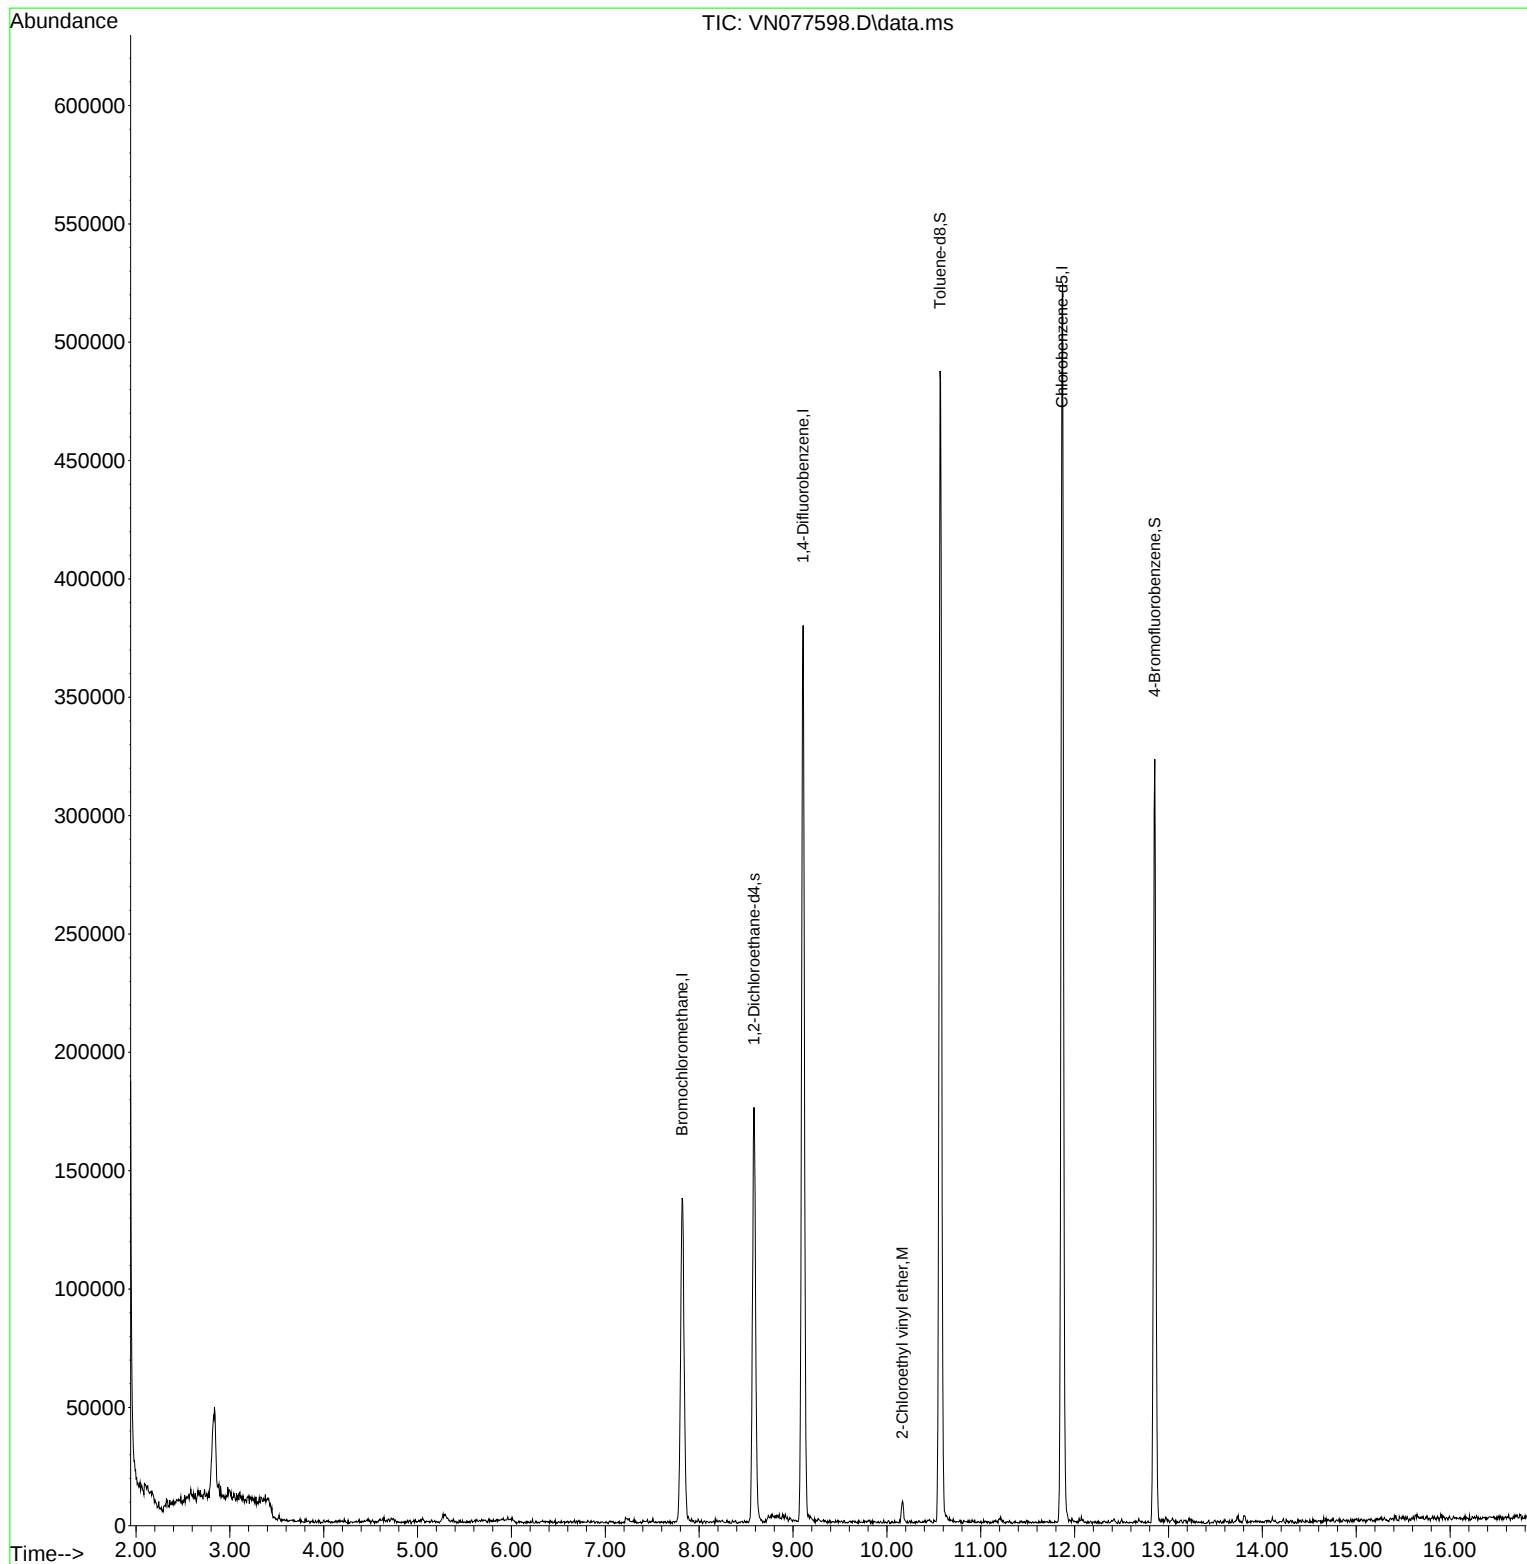

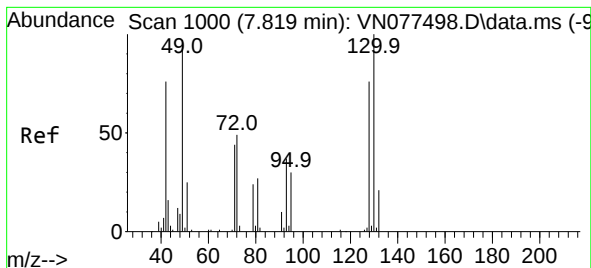

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 7.819 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN077598.D

Acq: 05 May 2023 18:30

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion:128 Resp: 50876

Ion Ratio Lower Upper

128 100

49 151.4 0.0 338.5

130 125.8 0.0 326.3

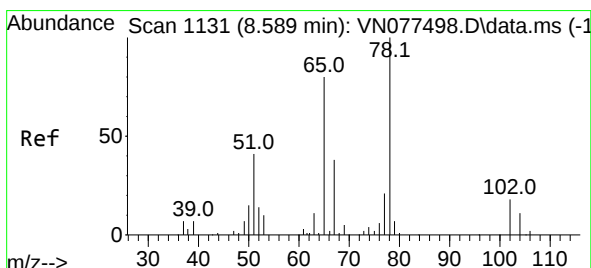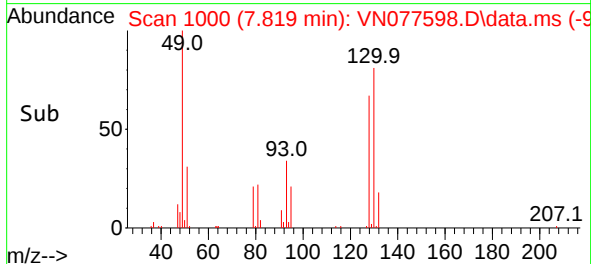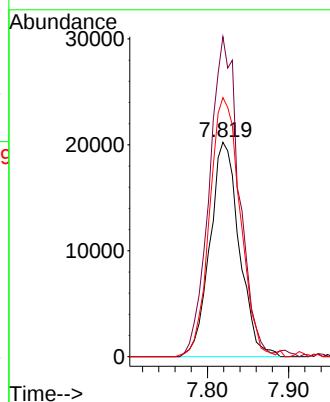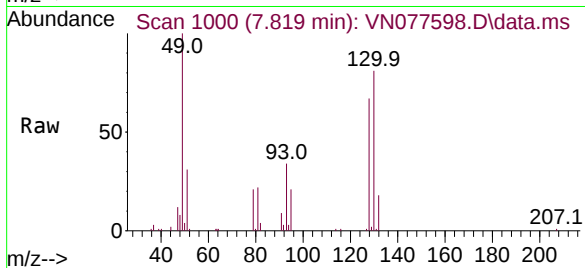

#27

1,2-Dichloroethane-d4

Concen: 32.114 ug/l

RT: 8.584 min Scan# 1130

Delta R.T. -0.005 min

Lab File: VN077598.D




Acq: 05 May 2023 18:30


Tgt Ion: 65 Resp: 145658

Ion Ratio Lower Upper

65 100

67 51.5 40.2 60.2


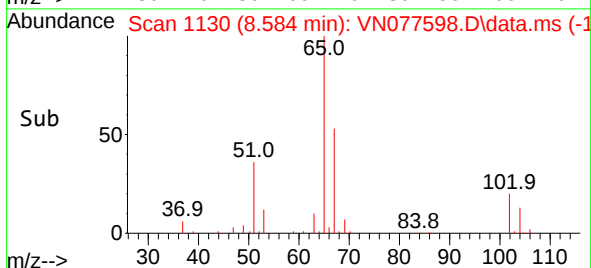
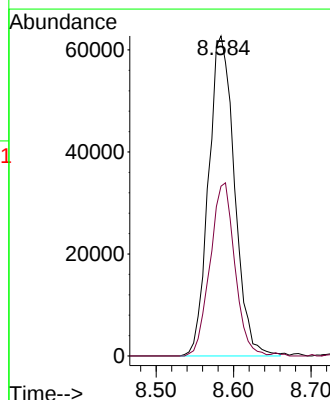
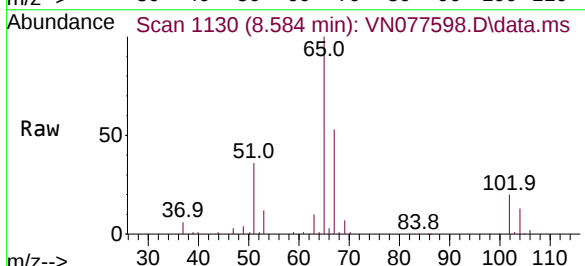


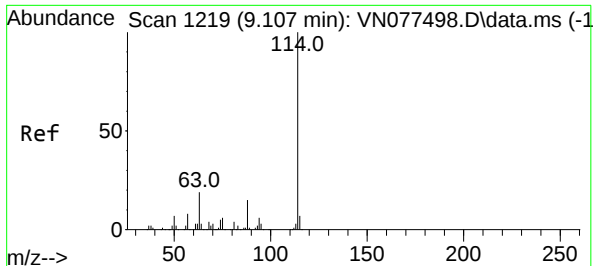

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 9.107 min Scan# 1219
Delta R.T. 0.000 min
Lab File: VN077598.D
Acq: 05 May 2023 18:30




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:114 Resp: 336119
Ion Ratio Lower Upper
114 100
63 19.5 14.1 21.1
88 15.7 12.3 18.5

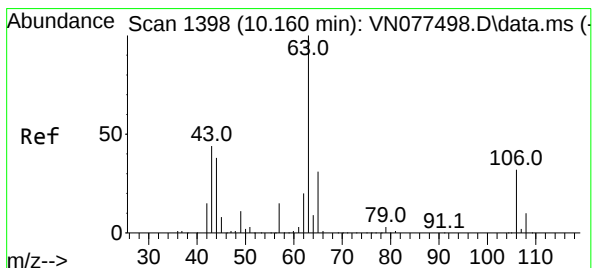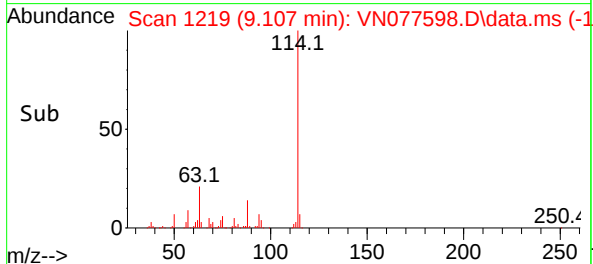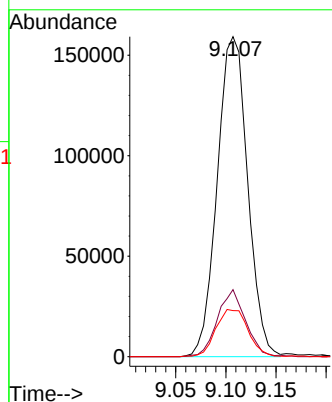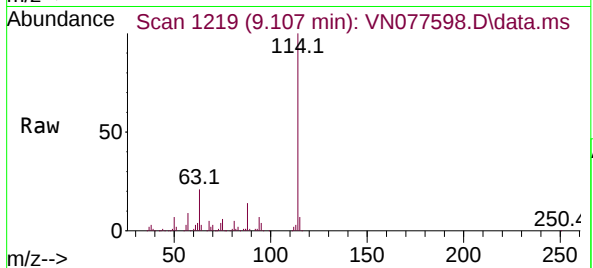

#55
2-Chloroethyl vinyl ether
Concen: 1.722 ug/l
RT: 10.166 min Scan# 1399
Delta R.T. 0.006 min
Lab File: VN077598.D
Acq: 05 May 2023 18:30

Tgt Ion: 63 Resp: 4421
Ion Ratio Lower Upper
63 100
65 23.2 25.8 38.6#
106 27.6 26.2 39.2


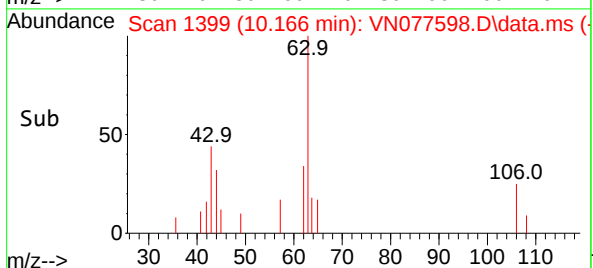
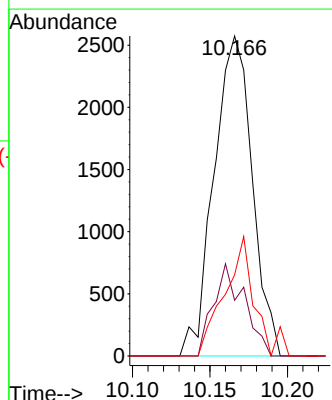
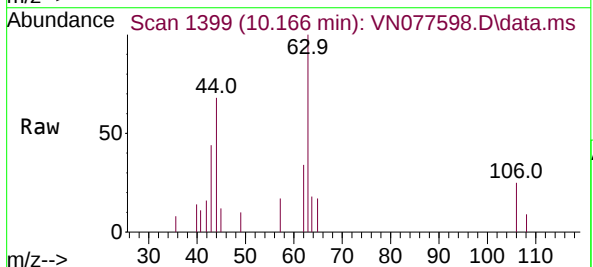


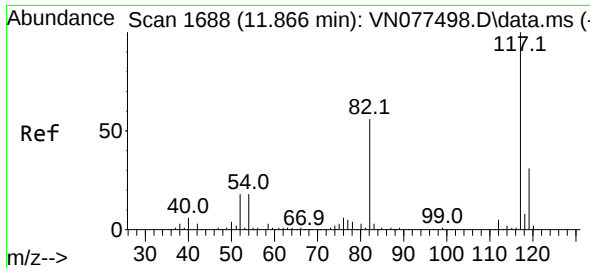

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.866 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN077598.D
Acq: 05 May 2023 18:30




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:117 Resp: 316101
Ion Ratio Lower Upper
117 100
82 58.4 44.2 66.2
119 31.4 25.4 38.2

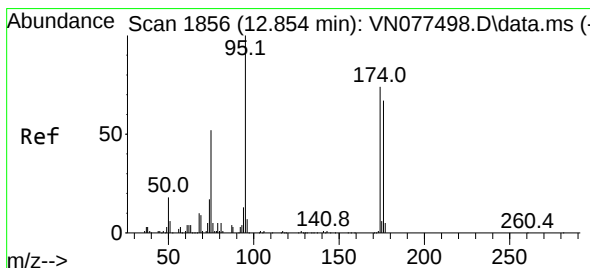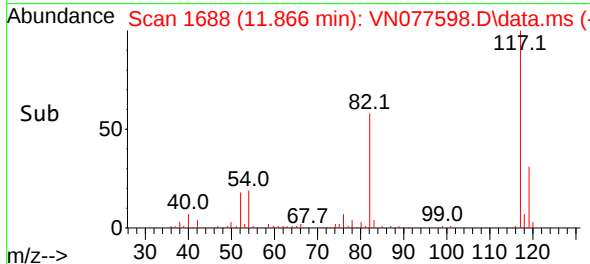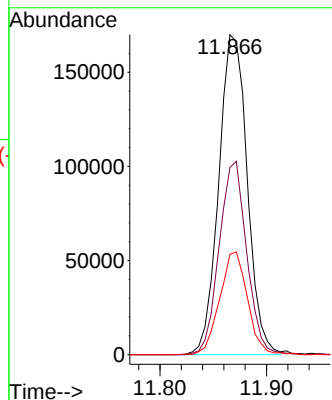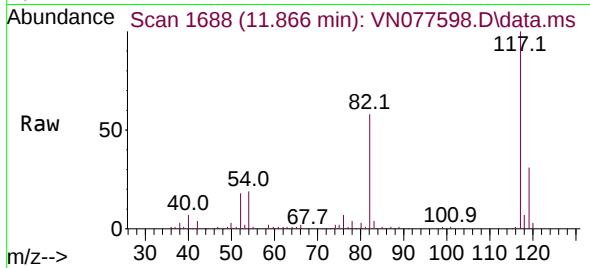

#60
4-Bromofluorobenzene
Concen: 21.490 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. -0.000 min
Lab File: VN077598.D
Acq: 05 May 2023 18:30

Tgt Ion: 95 Resp: 119013
Ion Ratio Lower Upper
95 100
174 67.1 55.9 83.9
176 62.6 53.9 80.9

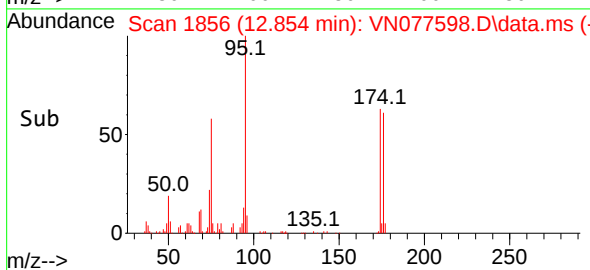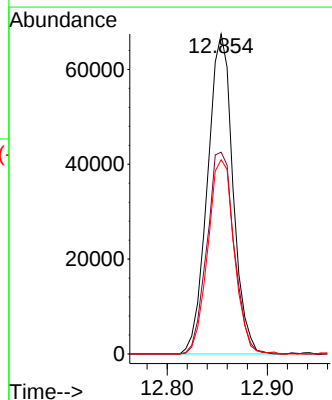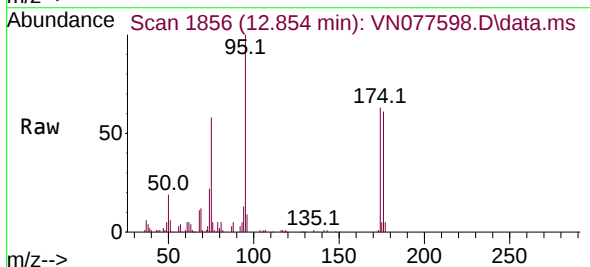

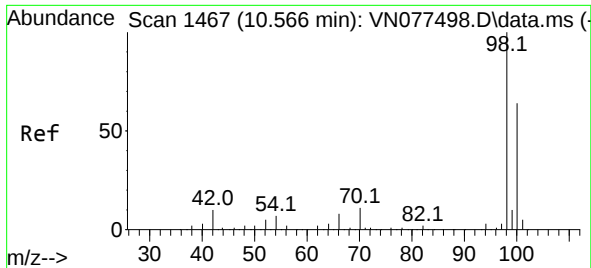

#63
Toluene-d8
Concen: 31.475 ug/l
RT: 10.566 min Scan# 14
Delta R.T. -0.000 min
Lab File: VN077598.D
Acq: 05 May 2023 18:30

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion: 98 Resp: 350582
Ion Ratio Lower Upper
98 100
100 65.3 51.0 76.4

