

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN050619\
 Data File : VN055422.D
 Acq On : 6 May 2019 17:54
 Operator : JC/SP
 Sample : K2680-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SSSI-0502-S-TCLP-8

Quant Time: May 07 02:25:18 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 30 07:16:52 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	492259	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	771442	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	621145	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	179822	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	315615	49.01	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.02%	
35) Dibromofluoromethane	7.59	113	246432	48.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.34%	
50) Toluene-d8	10.09	98	909739	49.76	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.52%	
62) 4-Bromofluorobenzene	12.40	95	265982	46.55	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.10%	
Target Compounds						
16) Acetone	3.83	43	7621	3.798	ug/l	99
20) Methylene Chloride	4.55	84	707785	115.562	ug/l	98
43) Isopropyl Acetate	8.17	43	10670	1.172	ug/l #	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN050619\
Data File : VN055422.D
Acq On : 6 May 2019 17:54
Operator : JC/SP
Sample : K2680-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SSSI-0502-S-TCLP-8

Quant Time: May 07 02:25:18 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 30 07:16:52 2019
Response via : Initial Calibration

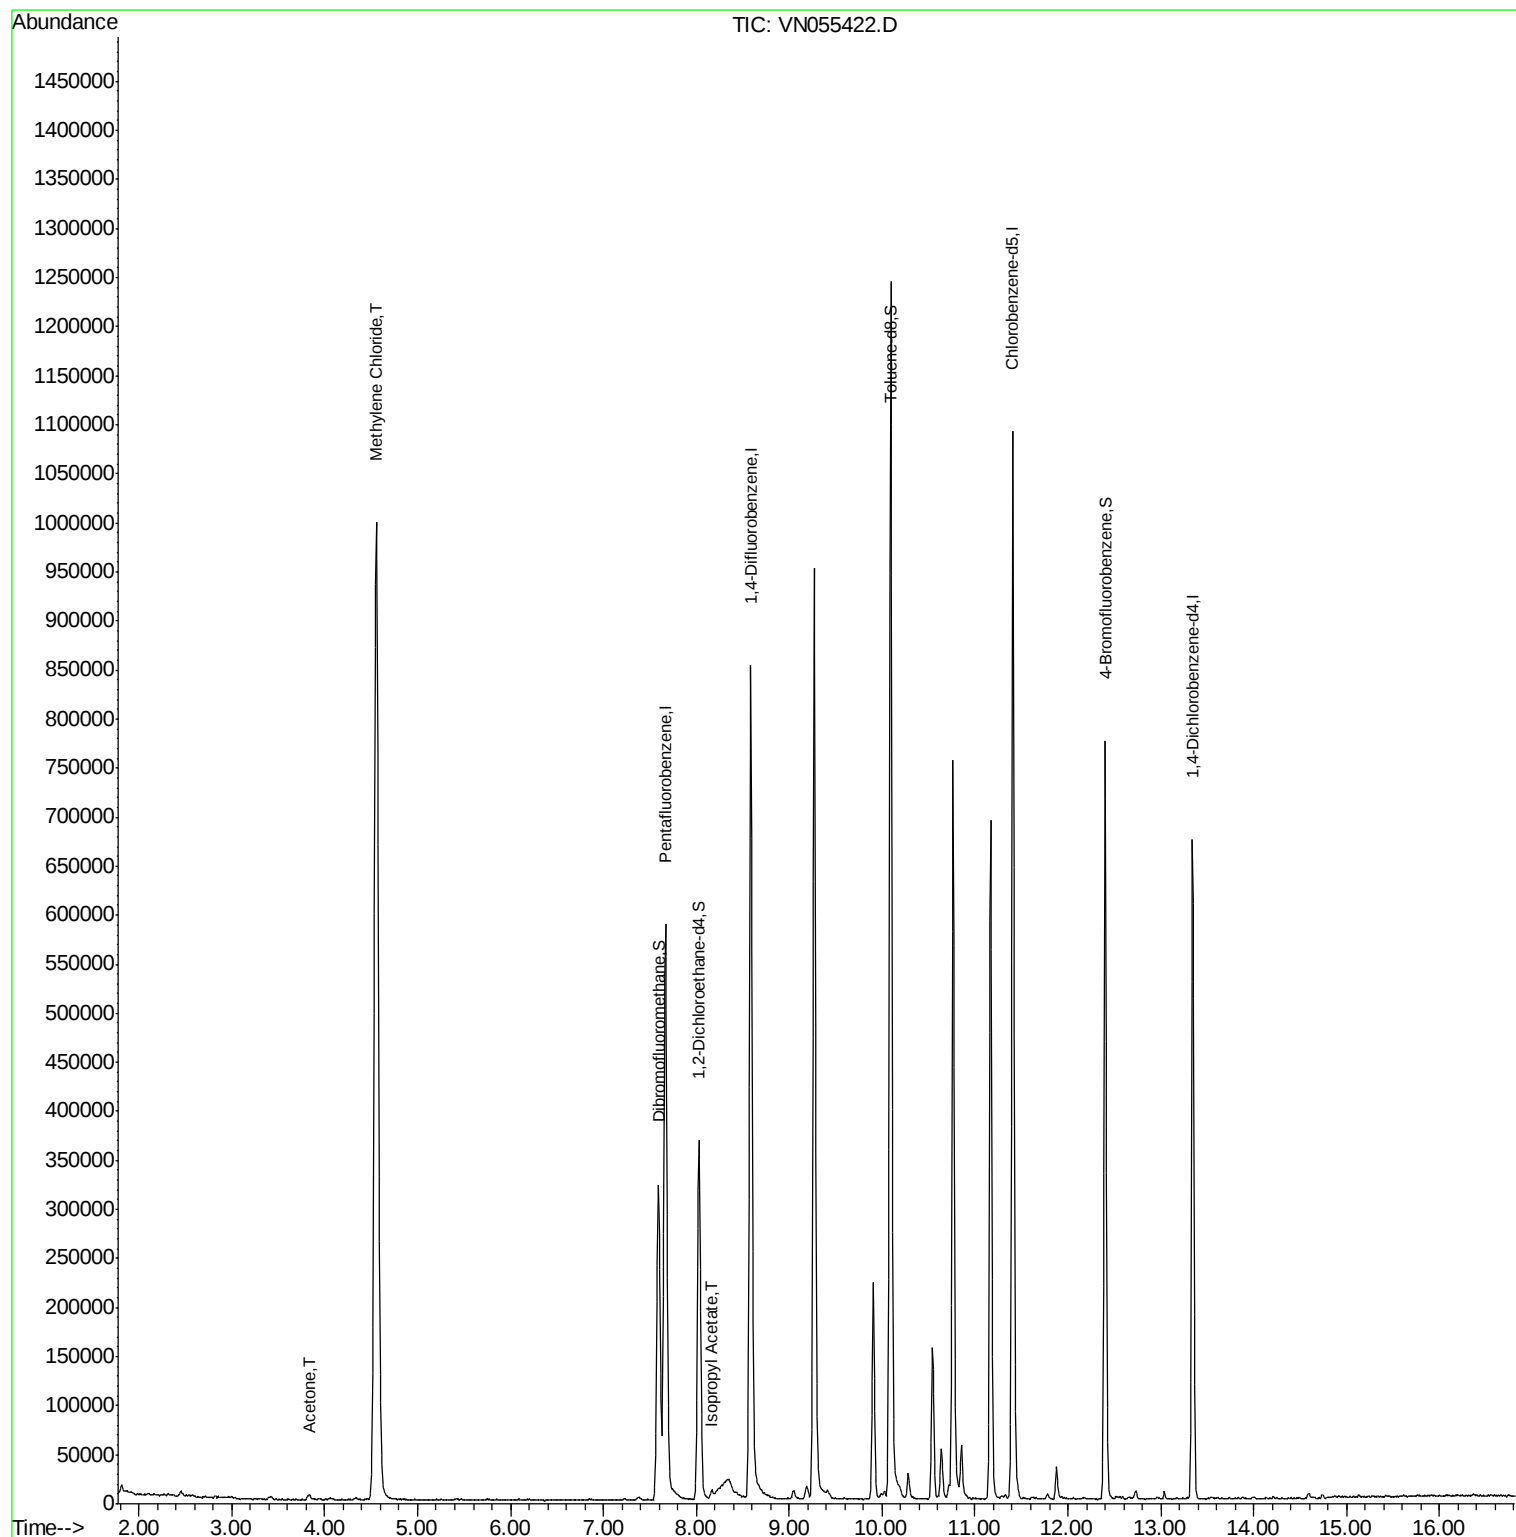

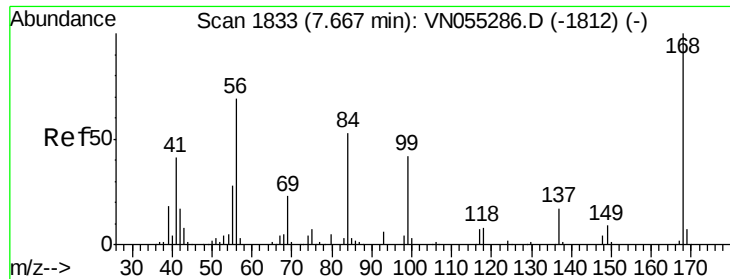

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1834

Delta R.T. 0.00 min

Lab File: VN055422.D

Acq: 6 May 2019 17:54

Instrument :

MSVOA_N

ClientSampleId :


SSSI-0502-S-TCLP-8

Tot Ion:168 Resp: 492259

Ion Ratio Lower Upper

168 100

99 56.0 43.6 65.4

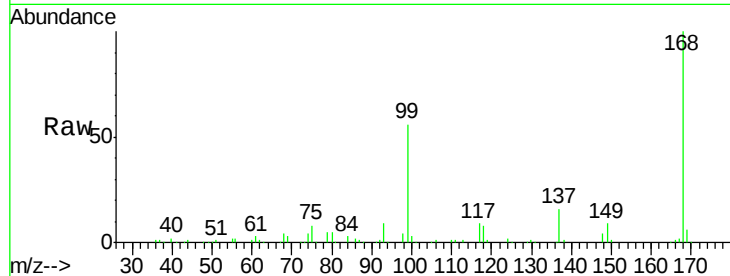

Abundance Ion 167.90 (167.60 to 168.60): VN055422.D (-1740) (-)

Ion 98.90 (98.60 to 99.60): VN055422.D (-1740) (-)

7.67

200000



150000

100000

50000

0

Time-->

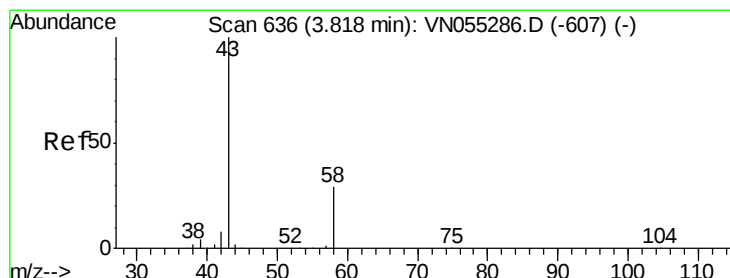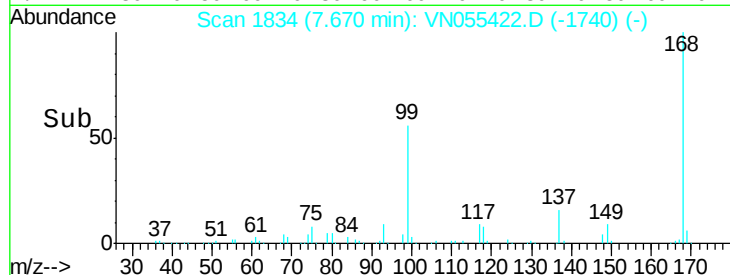

#16

Acetone

Concen: 3.798 ug/l

RT: 3.83 min Scan# 640

Delta R.T. 0.01 min

Lab File: VN055422.D


Acq: 6 May 2019 17:54

Tgt Ion: 43 Resp: 7621

Ion Ratio Lower Upper

43 100

58 28.7 23.6 35.4

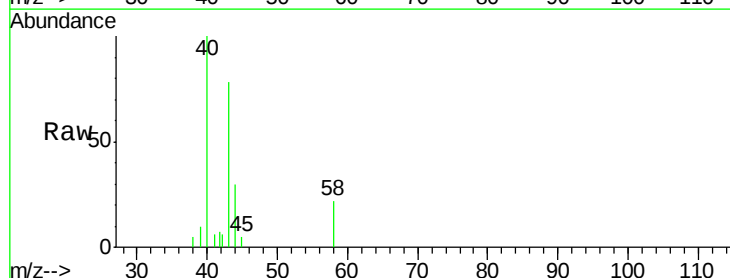

Abundance Ion 43.00 (42.70 to 43.70): VN055422.D (-543) (-)

Ion 58.00 (57.70 to 58.70): VN055422.D (-543) (-)

3.83

3000

2500

2000


1500


1000

500

0

Time-->




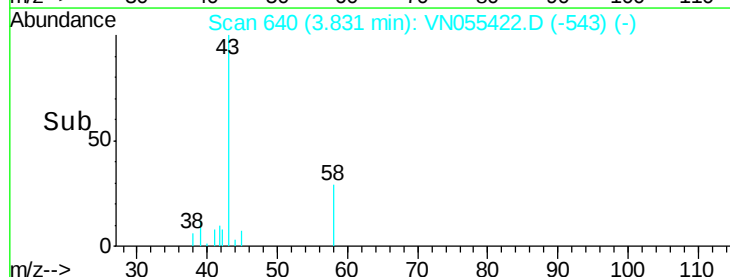


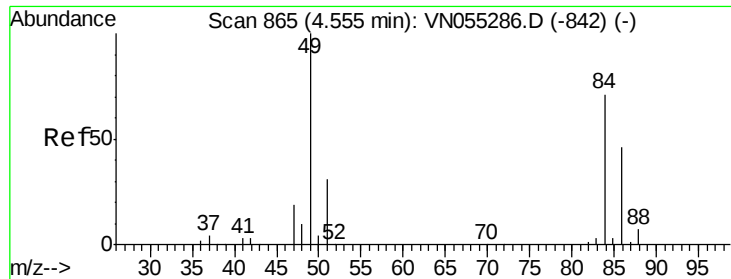

#20
Methvlene Chloride
Concen: 115.562 ug/l
RT: 4.55 min Scan# 865
Delta R.T. 0.00 min
Lab File: VN055422.D
Acq: 6 May 2019 17:54




Instrument :
MSVOA_N
ClientSampleId :
SSSI-0502-S-TCLP-8


Tot Ion: 84 Resp: 707785
Ion Ratio Lower Upper
84 100
49 144.9 112.4 168.6
51 44.2 34.6 51.8
86 64.8 51.9 77.9

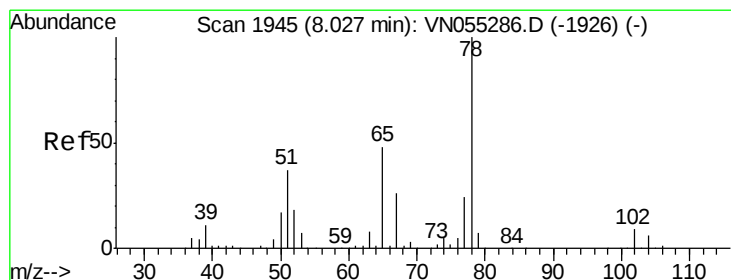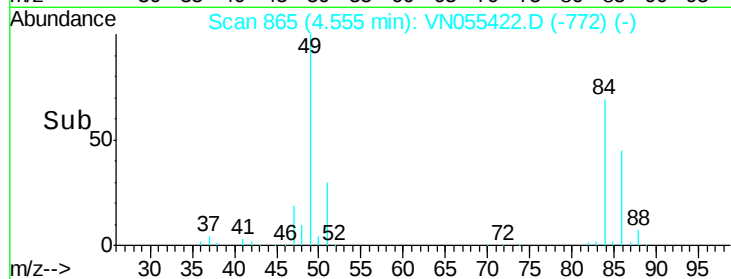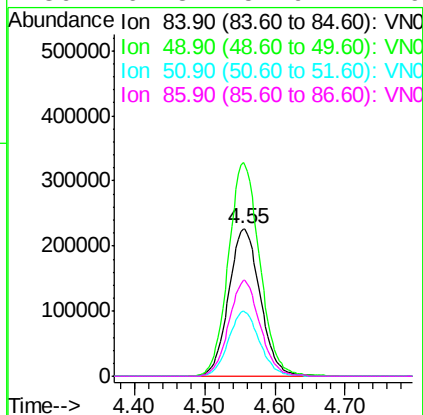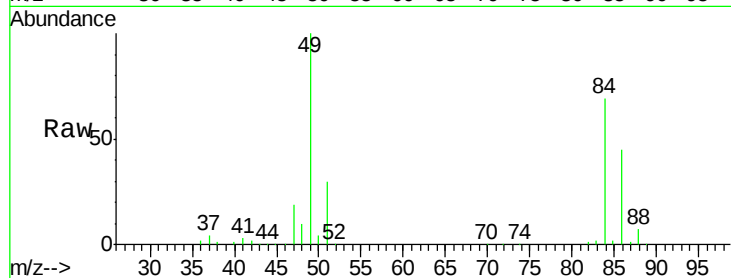

#33
1,2-Dichloroethane-d4
Concen: 49.010 ug/l
RT: 8.03 min Scan# 1945
Delta R.T. 0.00 min
Lab File: VN055422.D
Acq: 6 May 2019 17:54

Tgt Ion: 65 Resp: 315615
Ion Ratio Lower Upper
65 100
67 52.8 0.0 106.8

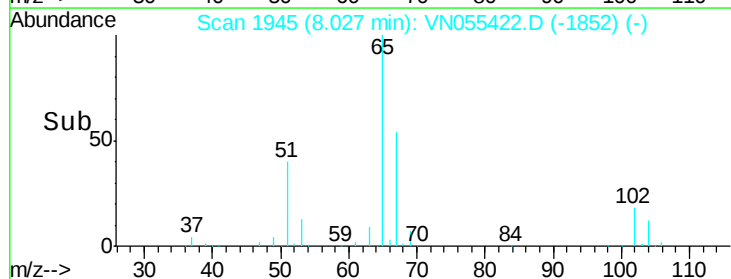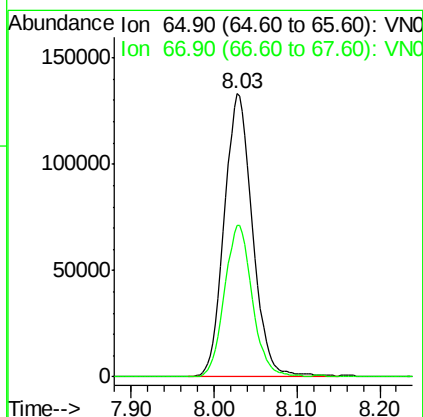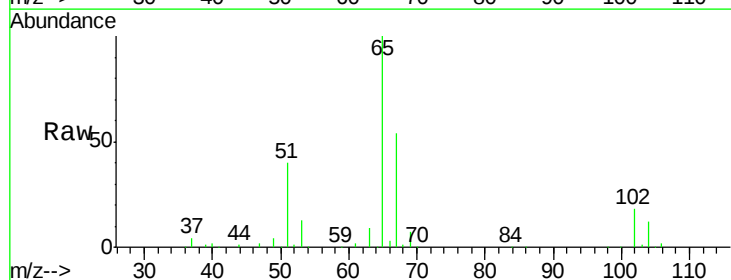

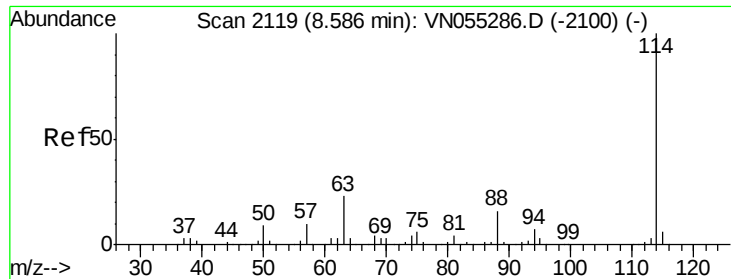

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. 0.00 min

Lab File: VN055422.D

Acq: 6 May 2019 17:54

Instrument :

MSVOA_N

ClientSampleId :

SSSI-0502-S-TCLP-8


Tot Ion:114 Resp: 771442

Ion Ratio Lower Upper

114 100

63 22.7 0.0 45.2




88 15.9 0.0 31.6

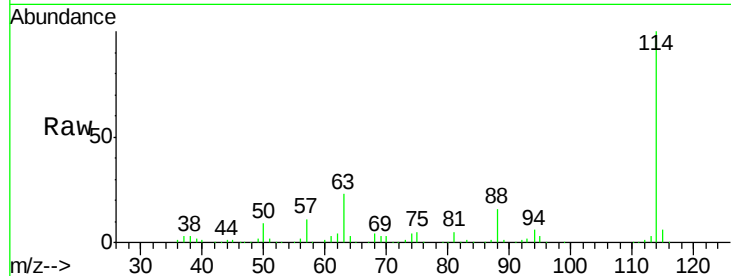

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

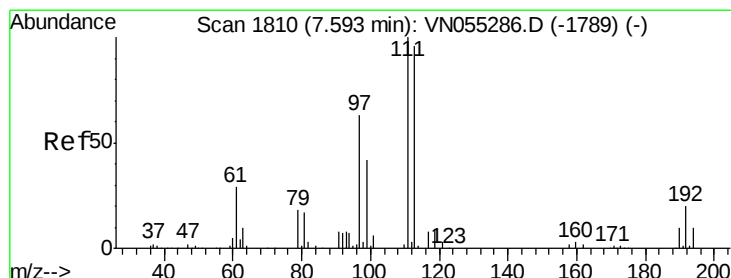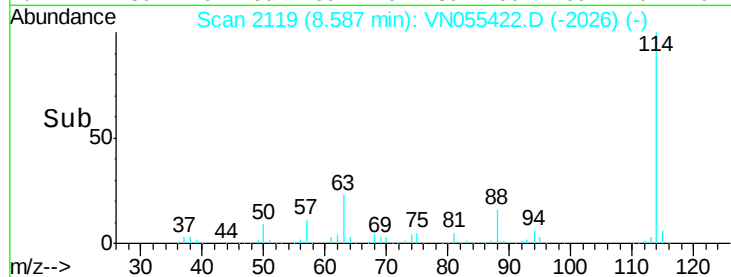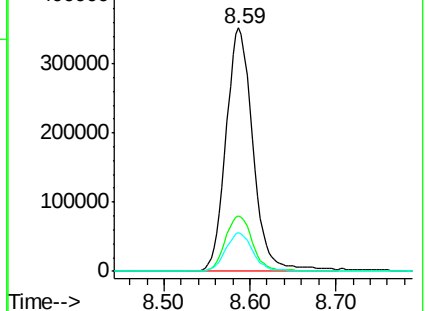

#35

Dibromofluoromethane

Concen: 48.668 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. 0.00 min

Lab File: VN055422.D

Acq: 6 May 2019 17:54


Tgt Ion:113 Resp: 246432

Ion Ratio Lower Upper

113 100

111 101.7 82.3 123.5



192 20.3 17.0 25.6

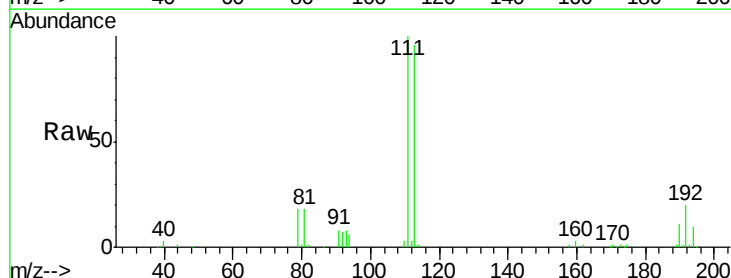


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

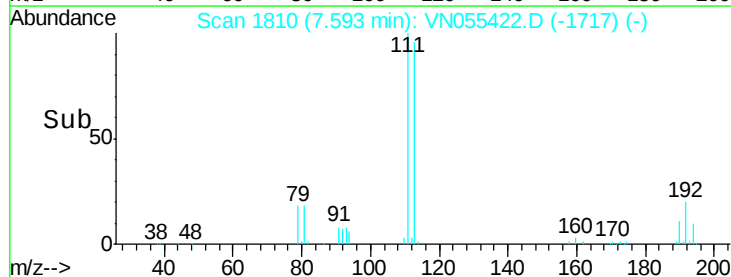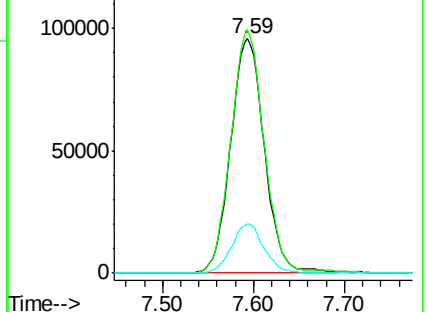

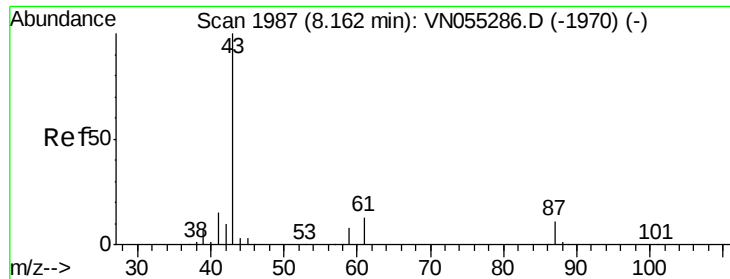

#43

Isopropyl Acetate

Concen: 1.172 ug/l

RT: 8.17 min Scan# 1988

Delta R.T. 0.00 min

Lab File: VN055422.D

Acq: 6 May 2019 17:54

Instrument :

MSVOA_N

ClientSampleId :

SSSI-0502-S-TCLP-8


Tot Ion: 43 Resp: 10670

Ion Ratio Lower Upper

43 100

61 17.6 20.8 31.2#




87 9.6 8.5 12.7

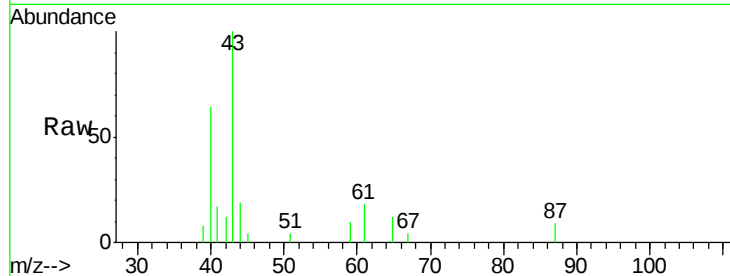

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

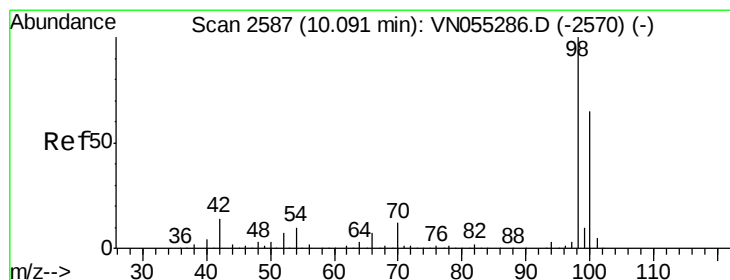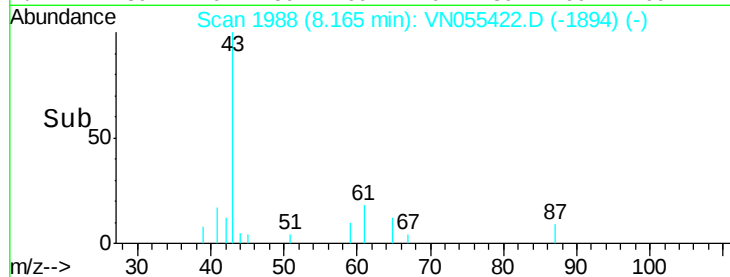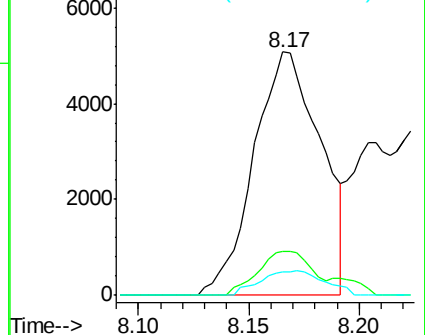

#50

Toluene-d8

Concen: 49.757 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN055422.D


Acq: 6 May 2019 17:54

Tgt Ion: 98 Resp: 909739

Ion Ratio Lower Upper



98 100


100 63.4 51.7 77.5

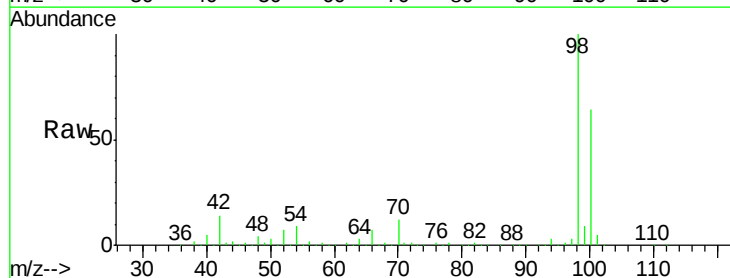

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0

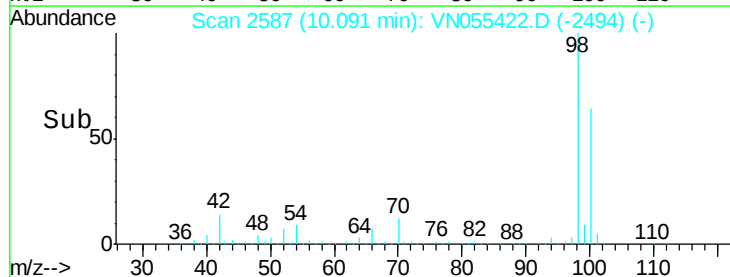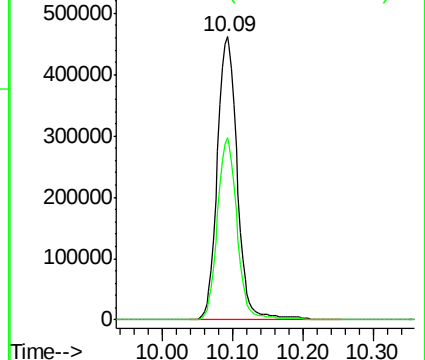

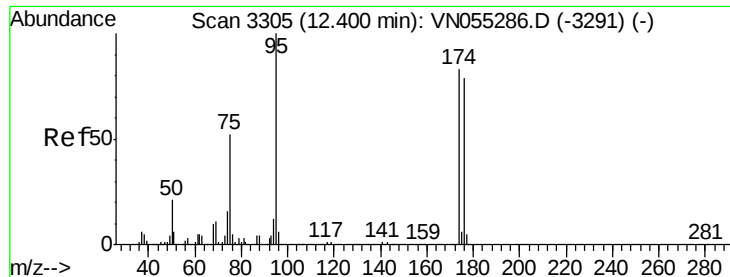

#62

4-Bromofluorobenzene

Concen: 46.547 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.00 min

Lab File: VN055422.D

Acq: 6 May 2019 17:54

Instrument :

MSVOA_N

ClientSampleId :

SSSI-0502-S-TCLP-8


Tot Ion: 95 Resp: 265982

Ion Ratio Lower Upper

95 100

174 82.9 0.0 166.6




176 78.9 0.0 157.8

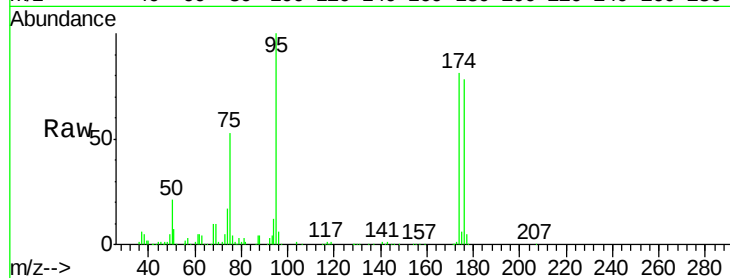

Abundance Ion 94.90 (94.60 to 95.60): VN055422.D (-2903) (-)

Ion 173.80 (173.50 to 174.50): VN055422.D (-2903) (-)

Ion 175.80 (175.50 to 176.50): VN055422.D (-2903) (-)

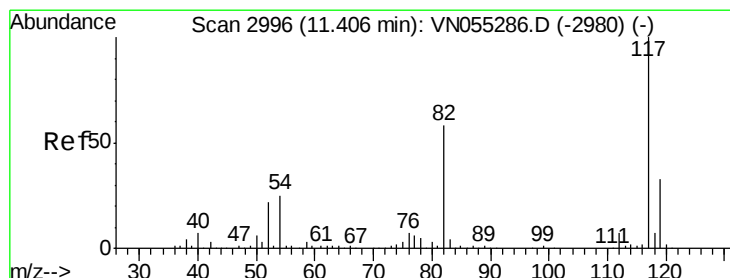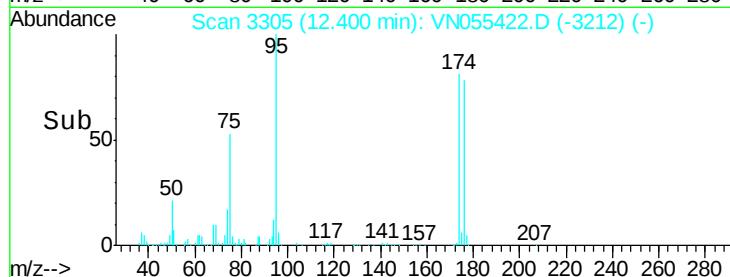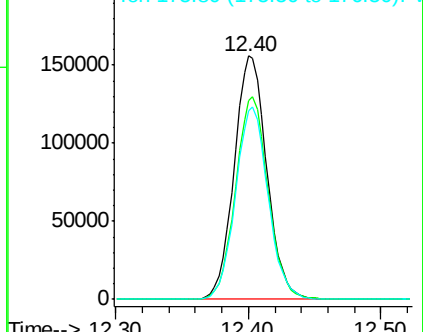

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. 0.00 min

Lab File: VN055422.D

Acq: 6 May 2019 17:54


Tgt Ion: 117 Resp: 621145

Ion Ratio Lower Upper

117 100

82 58.5 46.2 69.4



119 32.2 26.6 40.0

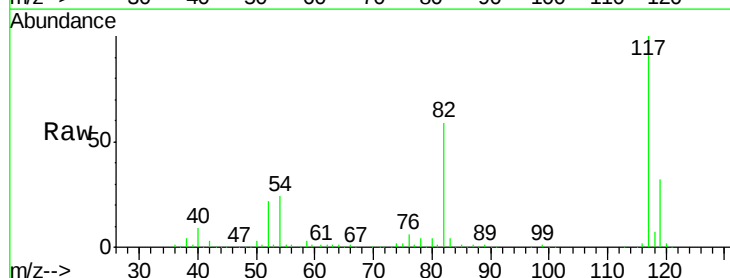


Abundance Ion 116.90 (116.60 to 117.60): VN055422.D (-2903) (-)

Ion 82.00 (81.70 to 82.70): VN055422.D (-2903) (-)

Ion 118.90 (118.60 to 119.60): VN055422.D (-2903) (-)

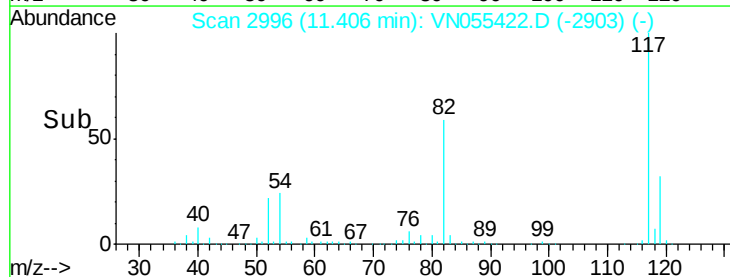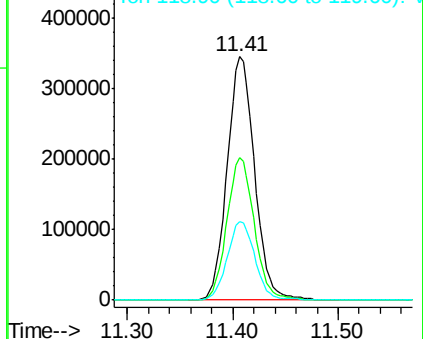

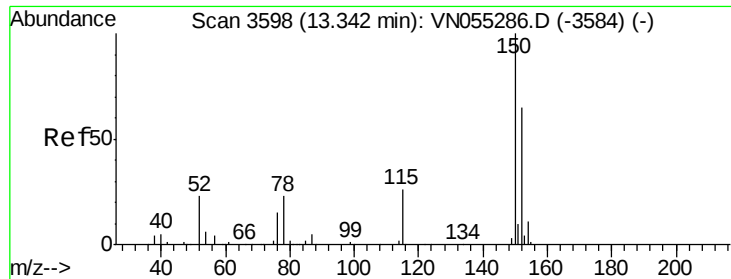

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. 0.00 min

Lab File: VN055422.D

Acq: 6 May 2019 17:54

Instrument :

MSVOA_N

ClientSampleId :

SSSI-0502-S-TCLP-8


Tot Ion:152 Resp: 179822

Ion Ratio Lower Upper

152 100

115 57.2 29.0 87.0

150 157.4 0.0 345.6

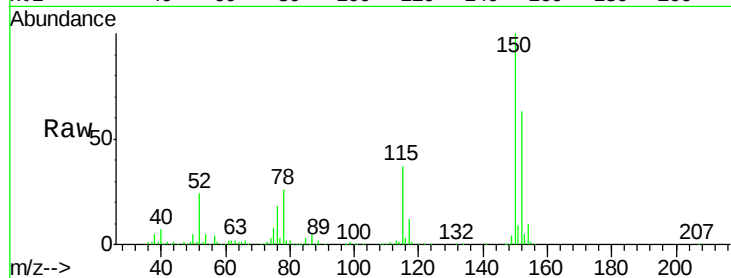

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

