

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
 Data File : VN072348.D
 Acq On : 06 May 2022 12:20
 Operator : JC\MD
 Sample : VN0506MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0506MBL01

Quant Time: May 09 03:11:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 26 18:50:11 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	206047	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.963	114	392369	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	418632	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	161017	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	161270	50.982	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery	= 101.960%		
35) Dibromofluoromethane	8.016	113	123597	49.215	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery	= 98.420%		
50) Toluene-d8	10.439	98	490177	49.672	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery	= 99.340%		
62) 4-Bromofluorobenzene	12.727	95	190271	58.090	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery	= 116.180%		
Target Compounds						Qvalue
3) Chloromethane	2.305	50	729	Below Cal		92
5) Bromomethane	2.869	94	367	Below Cal		86
6) Chloroethane	3.028	64	617	Below Cal	#	42
10) Methyl Iodide	4.428	142	663	0.257	ug/l #	54
11) Tert butyl alcohol	5.304	59	1076	2.070	ug/l #	72
15) Acrylonitrile	5.563	53	440	0.280	ug/l #	41
16) Acetone	4.293	43	1384	1.015	ug/l #	42
17) Carbon Disulfide	4.540	76	642	0.501	ug/l #	75
18) Methyl Acetate	4.828	43	96	Below Cal	#	48
20) Methylene Chloride	5.081	84	650	0.249	ug/l #	67
25) 2-Butanone	7.340	43	975	0.449	ug/l #	45
29) Tetrahydrofuran	7.716	42	631	0.443	ug/l #	40
31) Cyclohexane	8.081	56	4850	1.147	ug/l #	27
36) 1,1-Dichloropropene	8.081	75	16945	4.636	ug/l #	49
38) Carbon Tetrachloride	8.087	117	22184	5.666	ug/l #	18
43) Isopropyl Acetate	8.628	43	595	0.878	ug/l #	53
51) 4-Methyl-2-Pentanone	10.328	43	1998	0.436	ug/l #	86
56) Ethyl methacrylate	10.751	69	53	2.375	ug/l #	1
59) 2-Hexanone	11.081	43	4958	1.536	ug/l	79
74) N-amyl acetate	12.386	43	2321	0.436	ug/l	98
75) 1,1,2,2-Tetrachloroethane	12.816	83	680	Below Cal	#	66
76) 1,2,3-Trichloropropane	12.727	75	102750	28.411	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	102750	73.785	ug/l #	10
87) 1,3-Dichlorobenzene	13.610	146	1485	0.273	ug/l	87
88) 1,4-Dichlorobenzene	13.610	146	1485	0.281	ug/l	89
89) n-Butylbenzene	13.939	91	2828	0.349	ug/l	94
91) 1,2-Dichlorobenzene	13.986	146	1336	0.249	ug/l	78
92) 1,2-Dibromo-3-Chloropr...	14.604	75	326	0.331	ug/l #	46
93) 1,2,4-Trichlorobenzene	15.263	180	2119	3.233	ug/l	83
95) Naphthalene	15.510	128	7209	5.090	ug/l #	96
96) 1,2,3-Trichlorobenzene	15.698	180	2125	3.487	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
Data File : VN072348.D
Acq On : 06 May 2022 12:20
Operator : JC\MD
Sample : VN0506MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01

Quant Time: May 09 03:11:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 26 18:50:11 2022
Response via : Initial Calibration




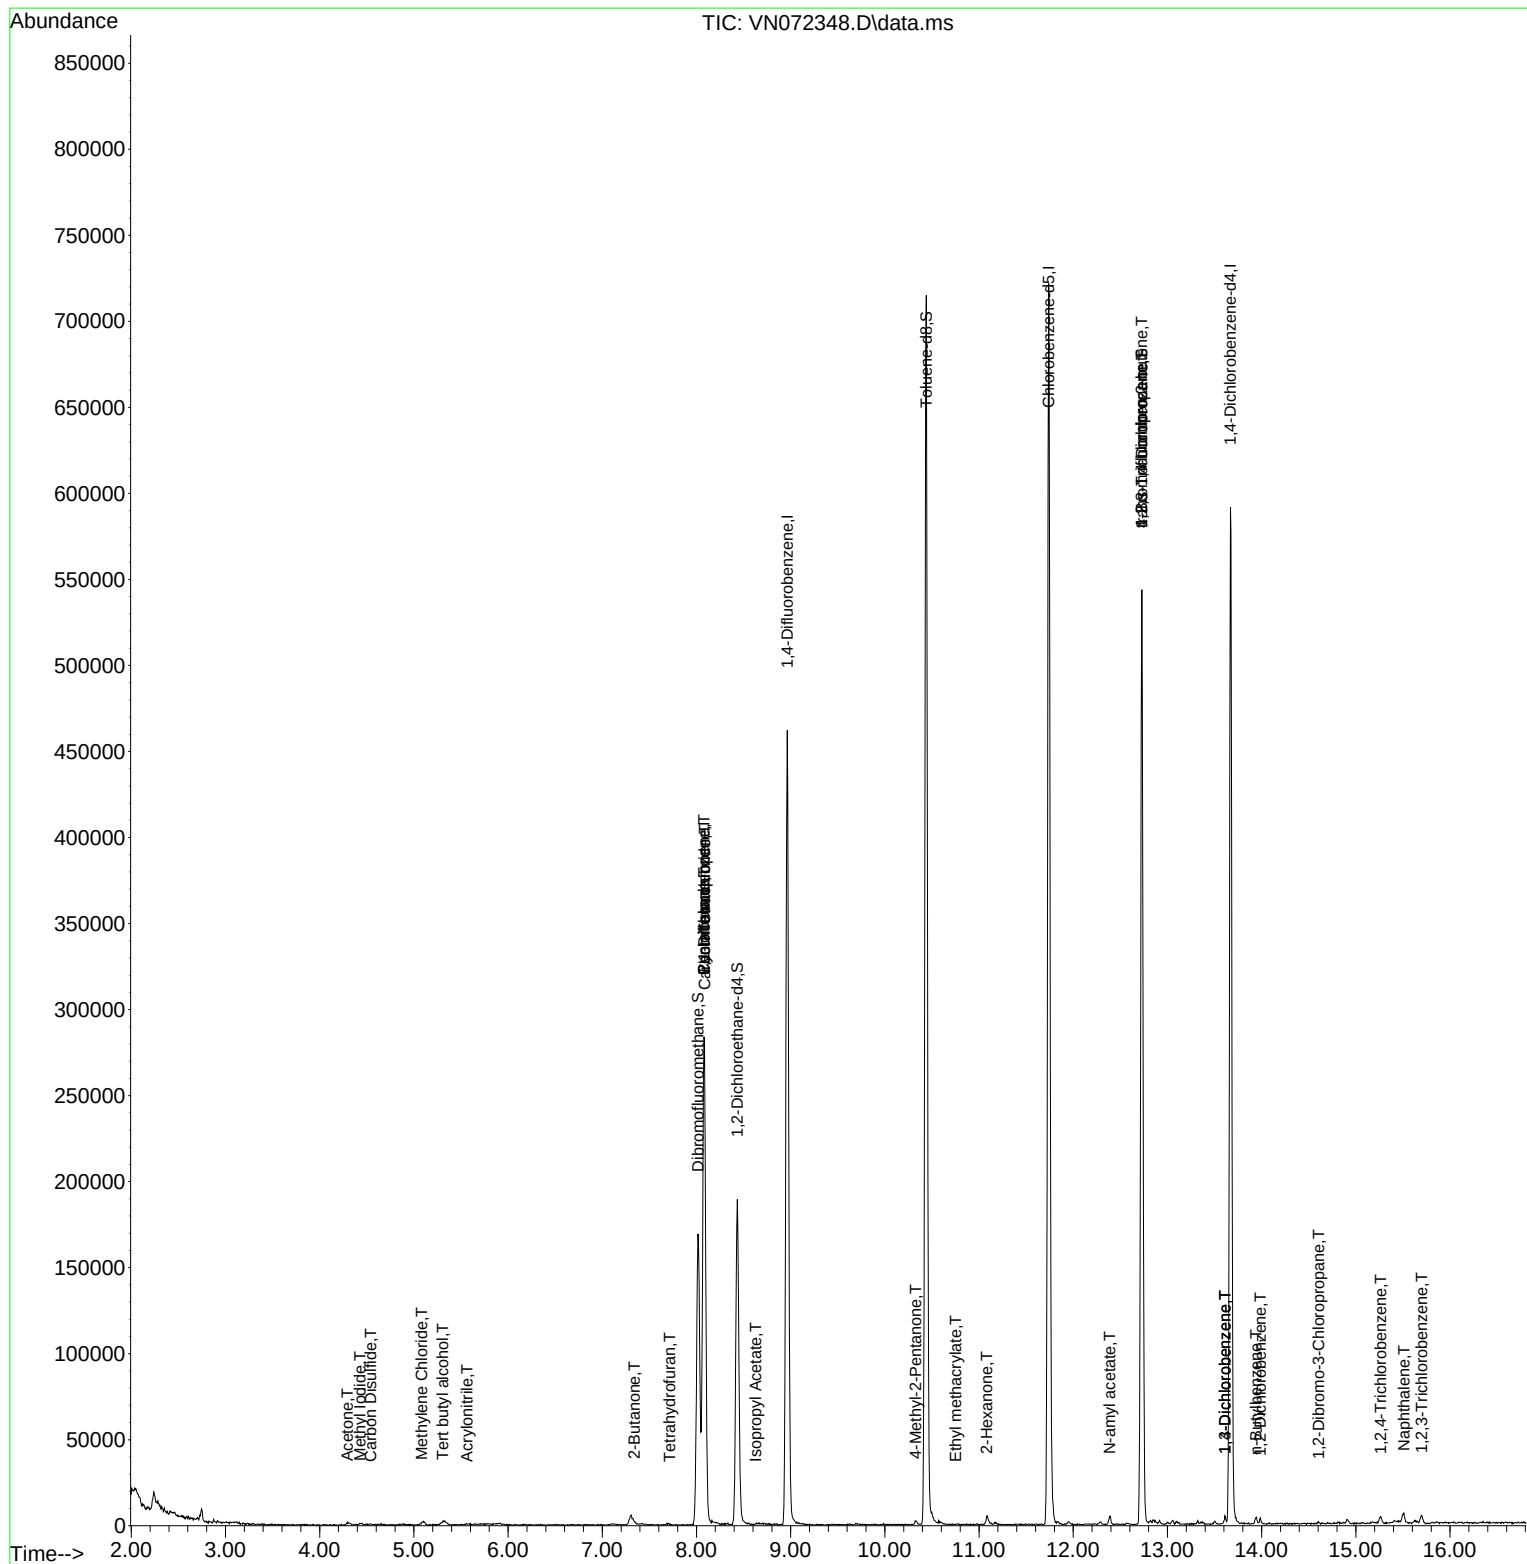


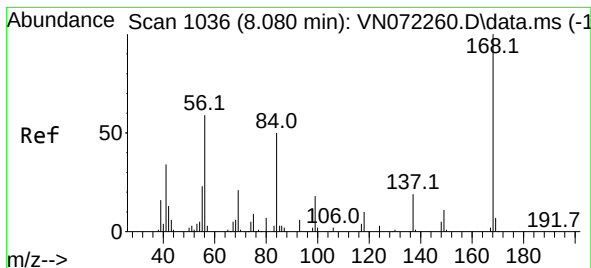

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1
Delta R.T. -0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion:168 Resp: 206047
Ion Ratio Lower Upper
168 100
99 69.2 42.3 63.5#

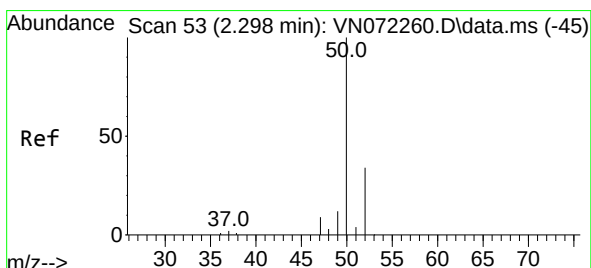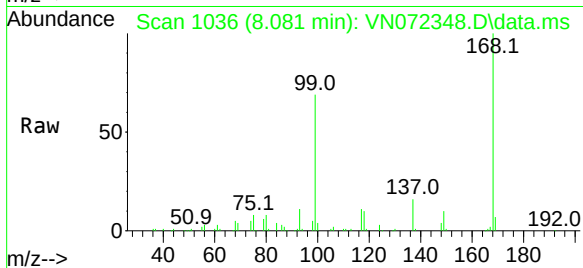

#3
Chloromethane
Concen: Below Cal
RT: 2.305 min Scan# 54
Delta R.T. 0.006 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion: 50 Resp: 729
Ion Ratio Lower Upper
50 100
52 27.7 25.7 38.5

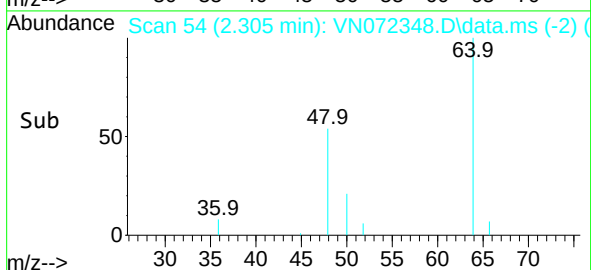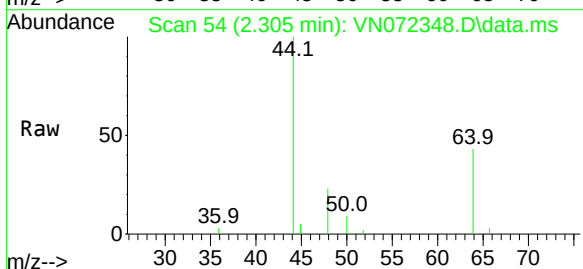



#5

Bromomethane

Concen: Below Cal

RT: 2.869 min Scan# 11

Delta R.T. 0.035 min

Lab File: VN072348.D

Acq: 06 May 2022 12:20

Instrument :

MSVOA_N

ClientSampleId :





VN0506MBL01

Tgt Ion: 94 Resp: 367

Ion Ratio Lower Upper

94 100

96 81.6 76.0 114.0

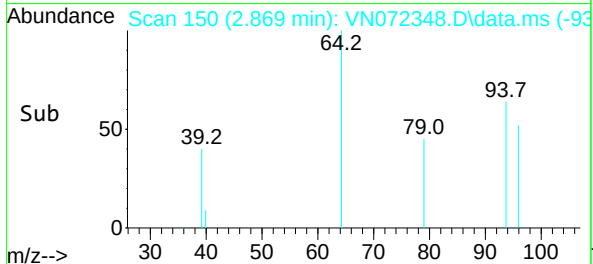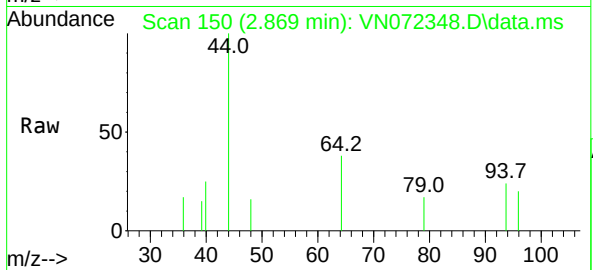

#6

Chloroethane

Concen: Below Cal

RT: 3.028 min Scan# 177

Delta R.T. 0.023 min

Lab File: VN072348.D




Acq: 06 May 2022 12:20


Tgt Ion: 64 Resp: 617

Ion Ratio Lower Upper

64 100

66 0.0 26.2 39.4#


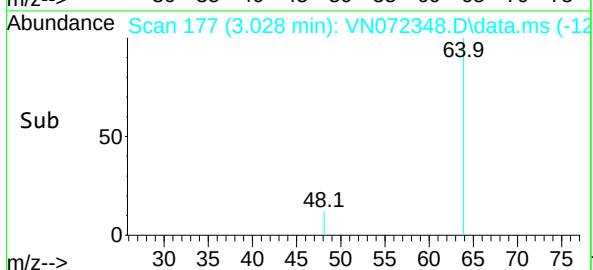

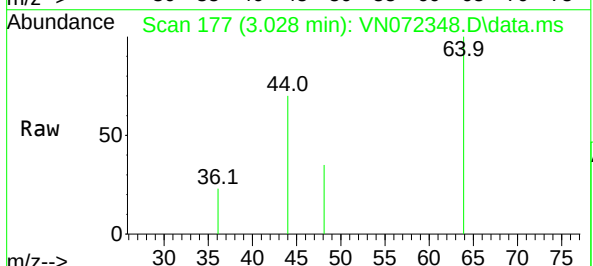




#10
Methyl Iodide
Concen: 0.257 ug/l
RT: 4.428 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion:142 Resp: 663
Ion Ratio Lower Upper
142 100
127 69.8 31.3 46.9#
141 0.0 11.2 16.8#

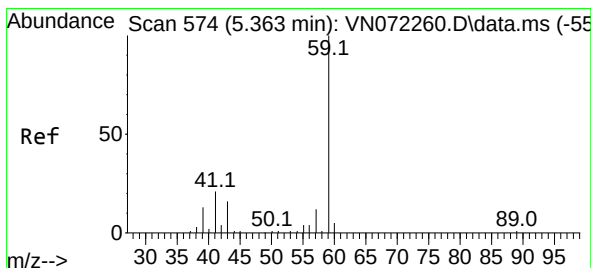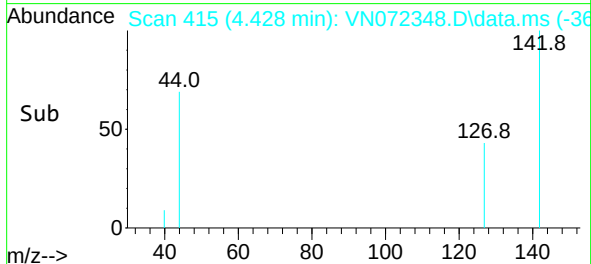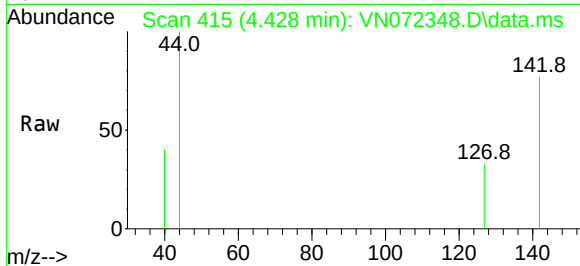

#11
Tert butyl alcohol
Concen: 2.070 ug/l
RT: 5.304 min Scan# 564
Delta R.T. -0.059 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion: 59 Resp: 1076
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


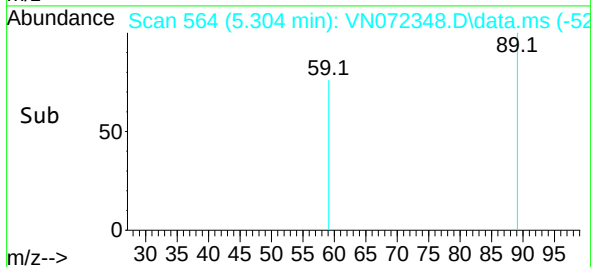

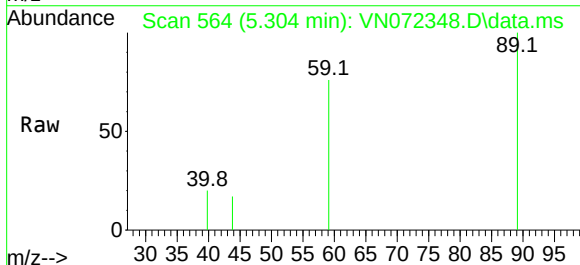


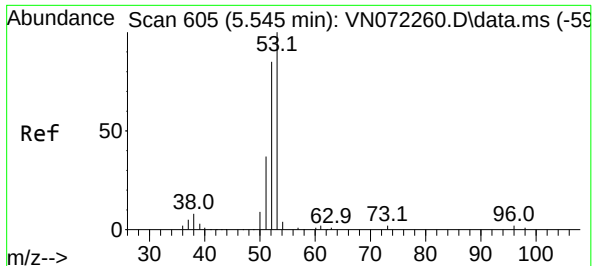

#15
Acrylonitrile
Concen: 0.280 ug/l
RT: 5.563 min Scan# 605
Delta R.T. 0.017 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion: 53 Resp: 440
Ion Ratio Lower Upper
53 100
52 30.9 66.4 99.6#
51 0.0 28.5 42.7#

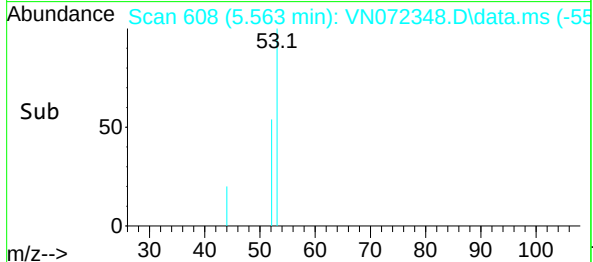

#16
Acetone
Concen: 1.015 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.012 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion: 43 Resp: 1384
Ion Ratio Lower Upper
43 100
58 0.0 26.0 39.0#

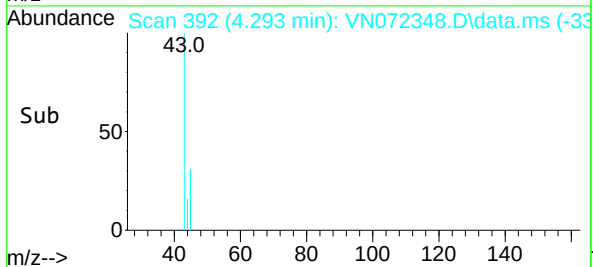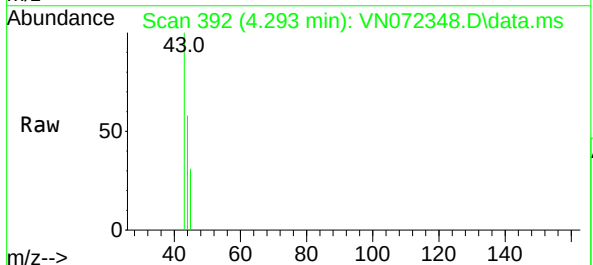

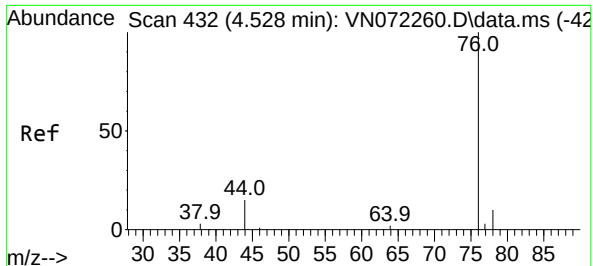

#17

Carbon Disulfide

Concen: 0.501 ug/l

RT: 4.540 min Scan# 41

Delta R.T. 0.006 min

Lab File: VN072348.D

Acq: 06 May 2022 12:20

Instrument :

MSVOA_N

ClientSampleId :





VN0506MBL01

Tgt Ion: 76 Resp: 642

Ion Ratio Lower Upper

76 100

78 0.0 7.2 10.8#

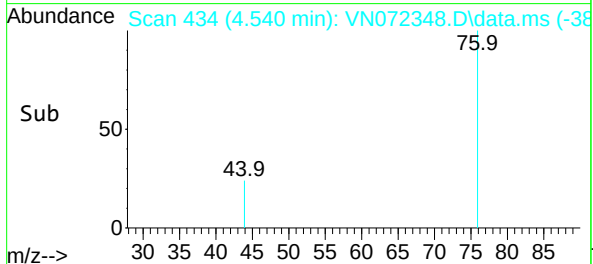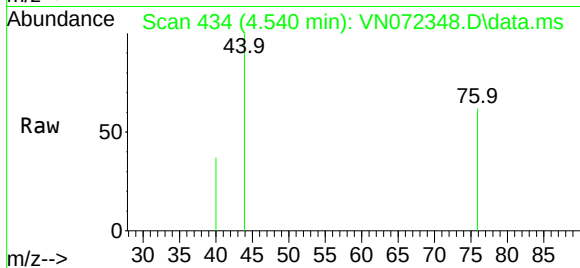

#20

Methylene Chloride

Concen: 0.249 ug/l

RT: 5.081 min Scan# 526

Delta R.T. -0.006 min

Lab File: VN072348.D

Acq: 06 May 2022 12:20

Tgt Ion: 84 Resp: 650




Ion Ratio Lower Upper


84 100

49 58.8 88.3 132.5#

51 42.2 28.2 42.2#

86 50.4 50.6 76.0#


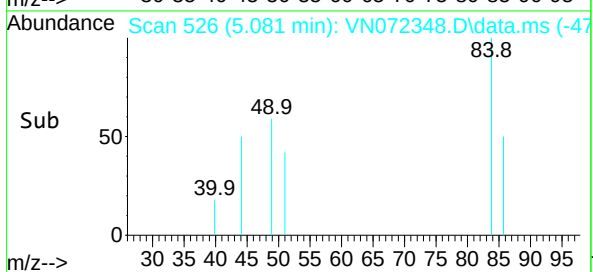

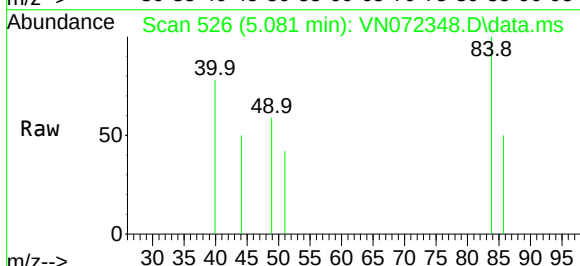




#25
2-Butanone
Concen: 0.449 ug/l
RT: 7.340 min Scan# 910
Delta R.T. 0.012 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion: 43 Resp: 975
Ion Ratio Lower Upper
43 100
72 0.0 23.7 35.5#

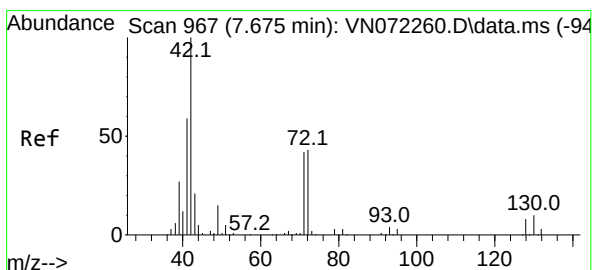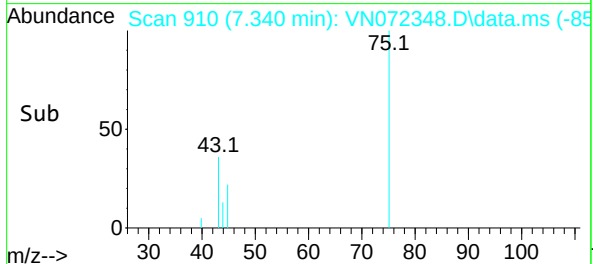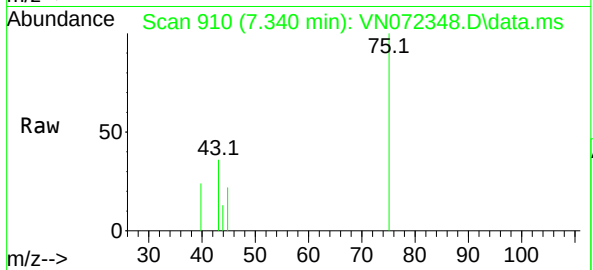

#29
Tetrahydrofuran
Concen: 0.443 ug/l
RT: 7.716 min Scan# 974
Delta R.T. 0.035 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20


Tgt Ion: 42 Resp: 631
Ion Ratio Lower Upper
42 100
72 0.0 39.7 59.5#
71 14.9 36.6 55.0#

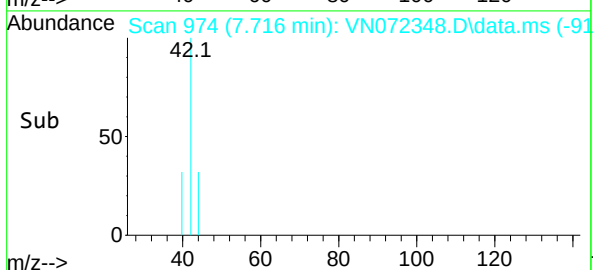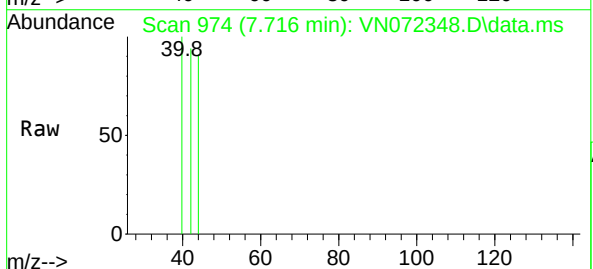






#31
Cyclohexane
Concen: 1.147 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.011 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20


Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01

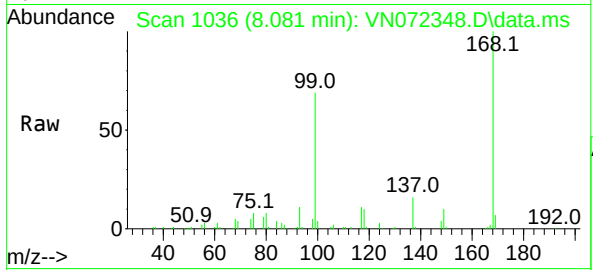



Tgt Ion: 56 Resp: 4850
Ion Ratio Lower Upper
56 100
69 127.6 27.8 41.8#
84 136.1 76.9 115.3#

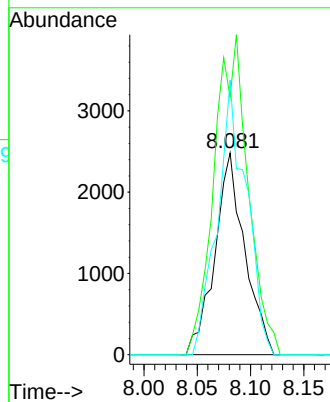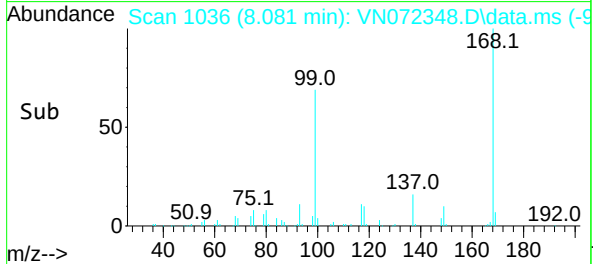


#33
1,2-Dichloroethane-d4
Concen: 50.982 ug/l
RT: 8.434 min Scan# 1096
Delta R.T. -0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

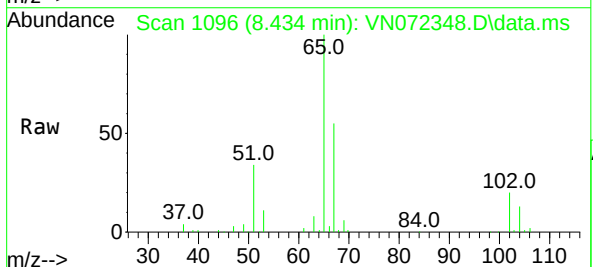

Tgt Ion: 65 Resp: 161270
Ion Ratio Lower Upper
65 100
67 51.5 0.0 104.8



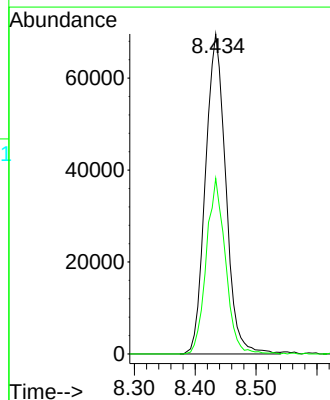
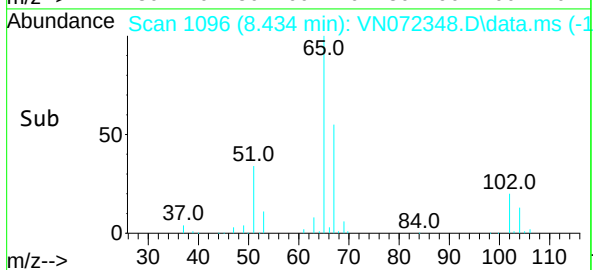




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. 0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion:	114	Resp:	392369
Ion	Ratio	Lower	Upper
114	100		
63	21.6	0.0	40.0
88	16.0	0.0	32.6

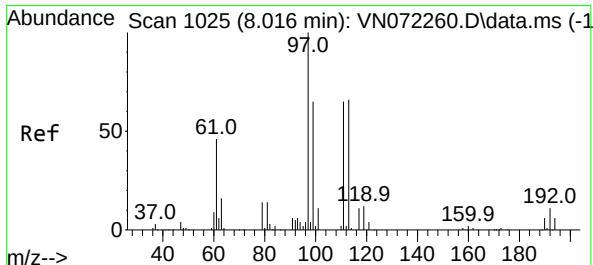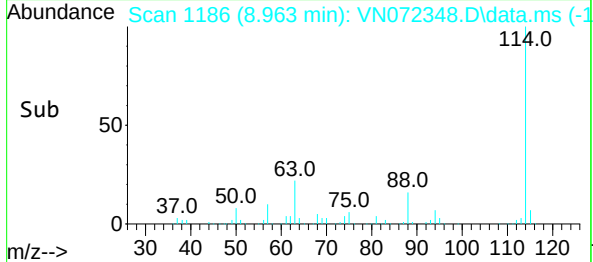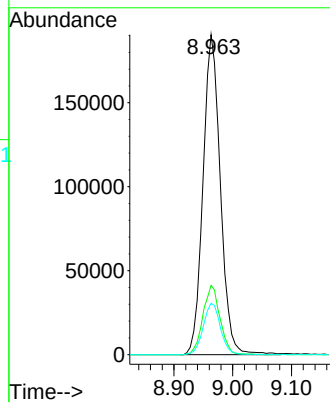

#35
Dibromofluoromethane
Concen: 49.215 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. 0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion:	113	Resp:	123597
Ion	Ratio	Lower	Upper
113	100		
111	105.3	81.4	122.0
192	18.8	17.0	25.6

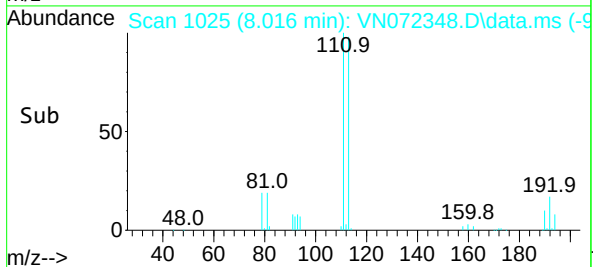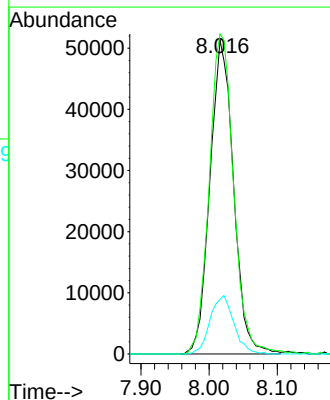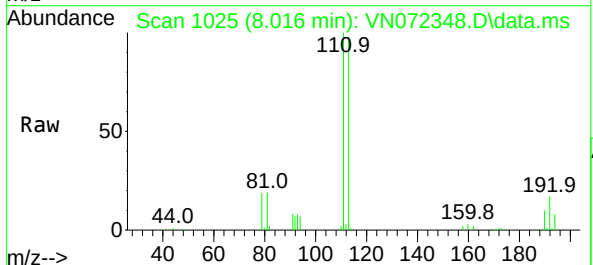

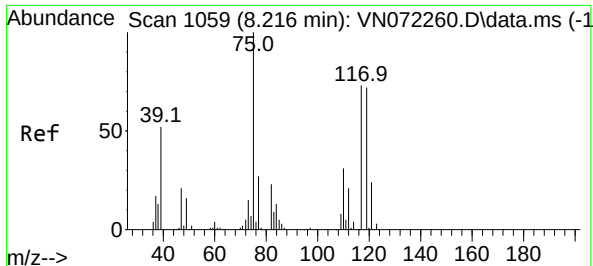

#36

1,1-Dichloropropene

Concen: 4.636 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.135 min

Lab File: VN072348.D

Acq: 06 May 2022 12:20

Instrument :

MSVOA_N

ClientSampleId :

VN0506MBL01





Tgt Ion: 75 Resp: 16945

Ion Ratio Lower Upper

75 100

110 9.8 18.3 54.8#

77 0.0 25.1 37.7#

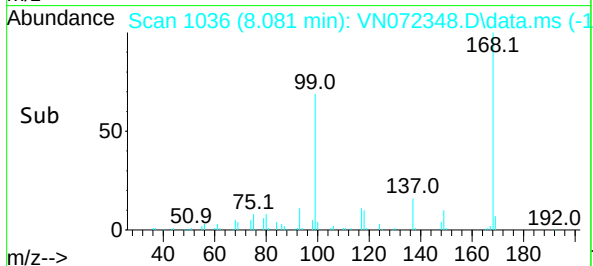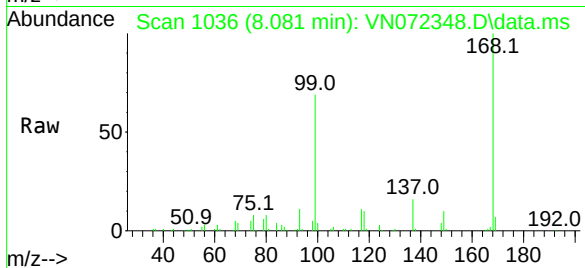

#38

Carbon Tetrachloride

Concen: 5.666 ug/l

RT: 8.087 min Scan# 1037

Delta R.T. -0.117 min

Lab File: VN072348.D

Acq: 06 May 2022 12:20




Tgt Ion: 117 Resp: 22184


Ion Ratio Lower Upper

117 100

119 6.6 75.8 113.8#

121 0.0 24.6 37.0#


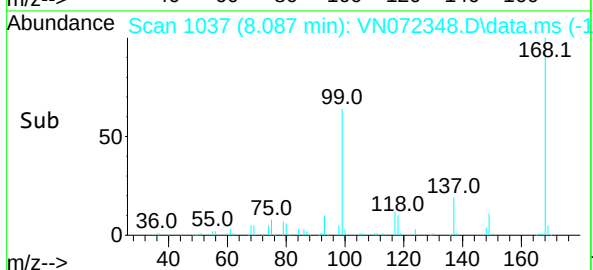

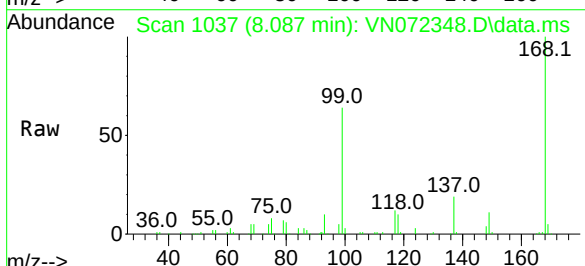




#43
Isopropyl Acetate
Concen: 0.878 ug/l
RT: 8.628 min Scan# 1117
Delta R.T. 0.071 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion: 43 Resp: 595
Ion Ratio Lower Upper
43 100
61 0.0 21.9 32.9#
87 0.0 12.0 18.0#

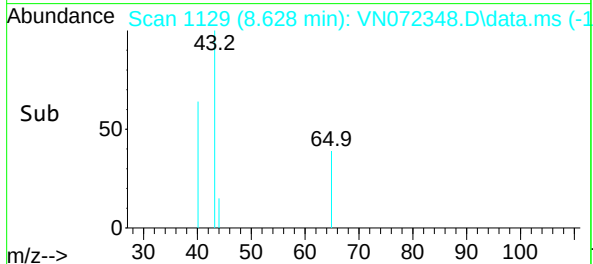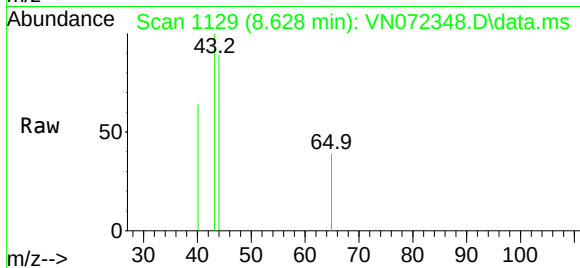

#50
Toluene-d8
Concen: 49.672 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion: 98 Resp: 490177
Ion Ratio Lower Upper
98 100
100 65.3 52.6 78.8


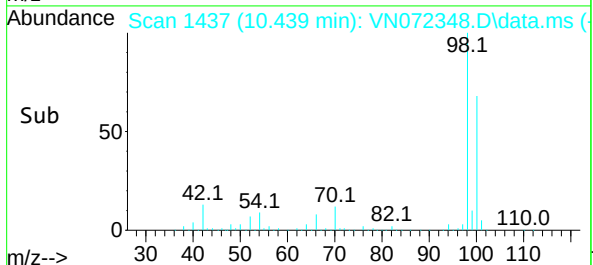

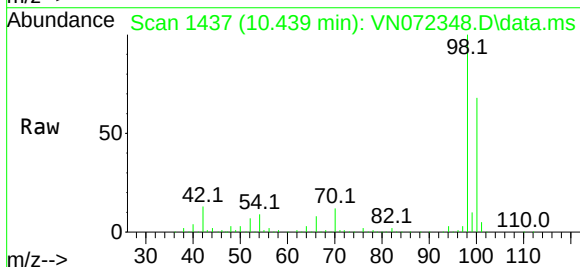


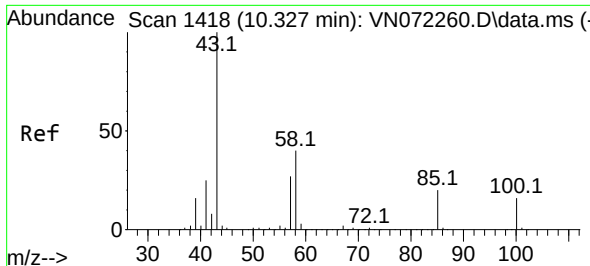

#51
4-Methyl-2-Pentanone
Concen: 0.436 ug/l
RT: 10.328 min Scan# 1418
Delta R.T. -0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion: 43 Resp: 1998
Ion Ratio Lower Upper
43 100
58 34.0 34.1 51.1#

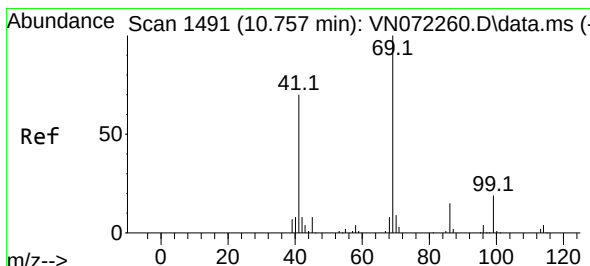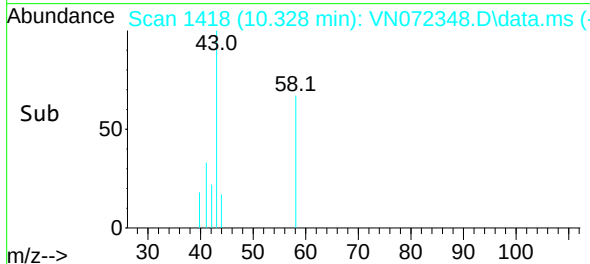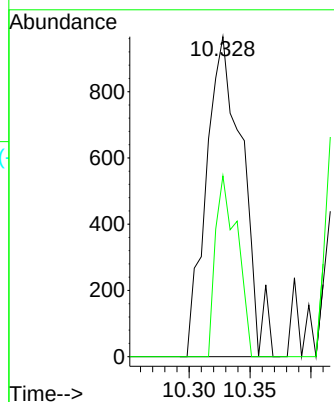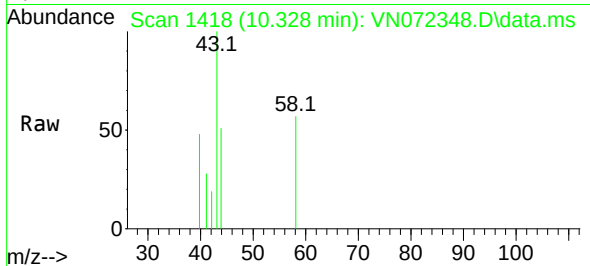

#56
Ethyl methacrylate
Concen: 2.375 ug/l
RT: 10.751 min Scan# 1490
Delta R.T. -0.006 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion: 69 Resp: 53
Ion Ratio Lower Upper
69 100
41 262.3 47.8 71.6#
39 0.0 27.3 40.9#


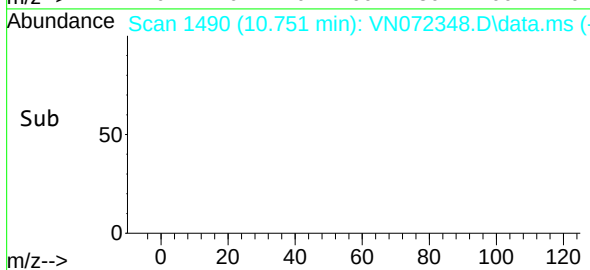
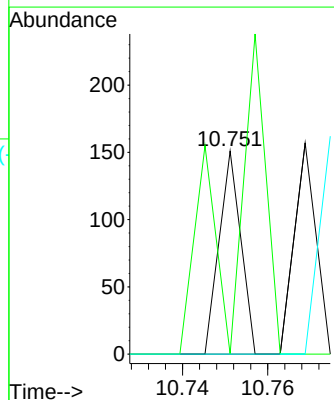
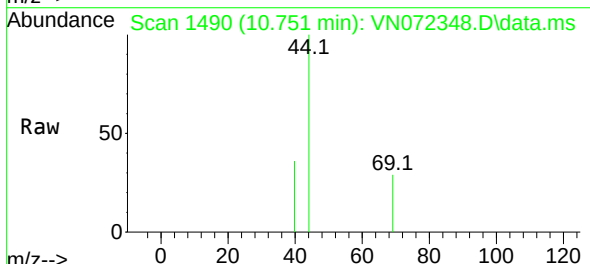


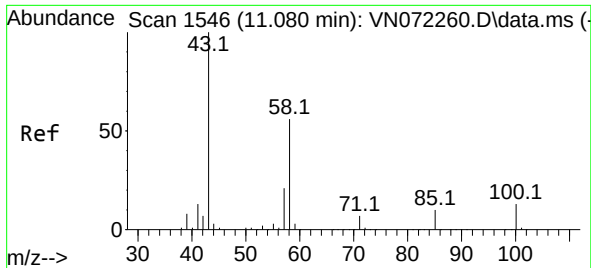

#59
2-Hexanone
Concen: 1.536 ug/l
RT: 11.081 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion: 43 Resp: 4958
Ion Ratio Lower Upper
43 100
58 43.8 29.7 89.1

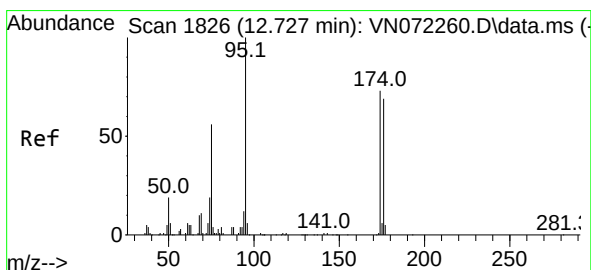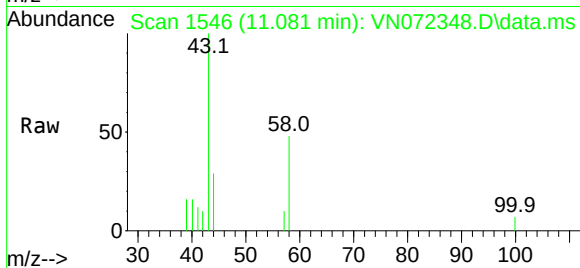

#62
4-Bromofluorobenzene
Concen: 58.090 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion: 95 Resp: 190271
Ion Ratio Lower Upper
95 100
174 77.8 0.0 167.6
176 74.1 0.0 163.4


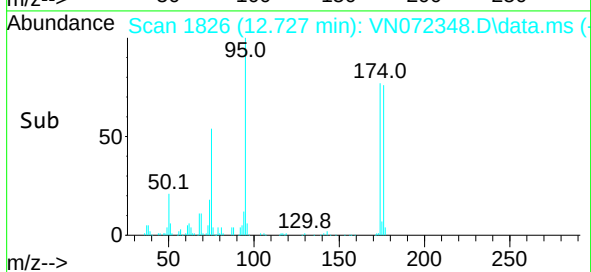

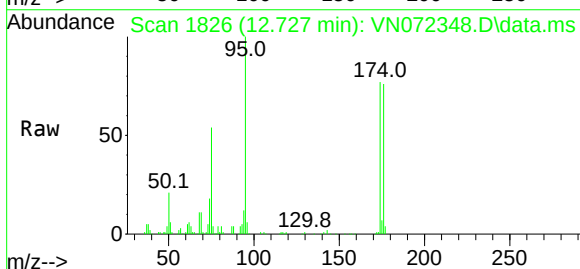




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1
Delta R.T. 0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion:117 Resp: 418632
Ion Ratio Lower Upper
117 100
82 55.1 44.2 66.2
119 32.0 25.4 38.0

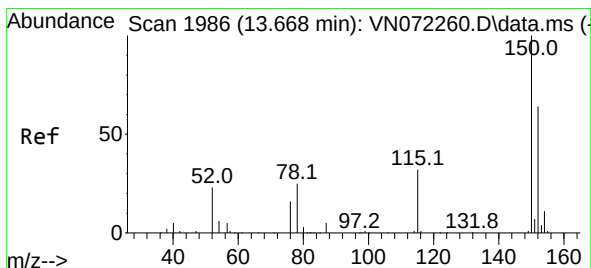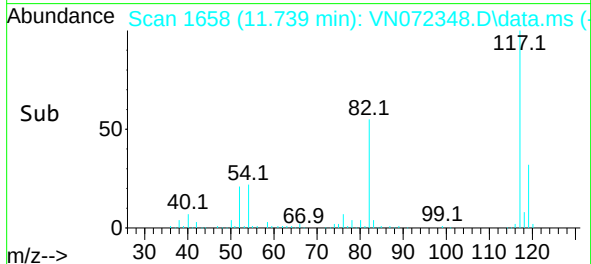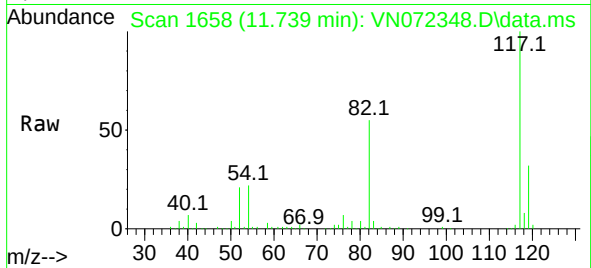

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. -0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion:152 Resp: 161017
Ion Ratio Lower Upper
152 100
115 60.6 28.9 86.7
150 155.3 0.0 356.2


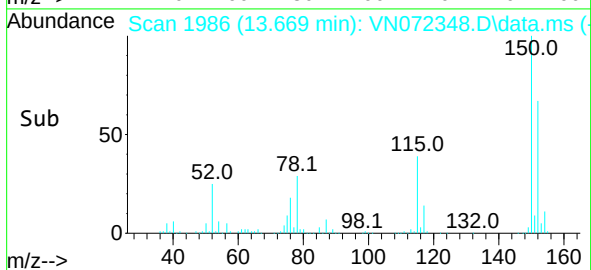

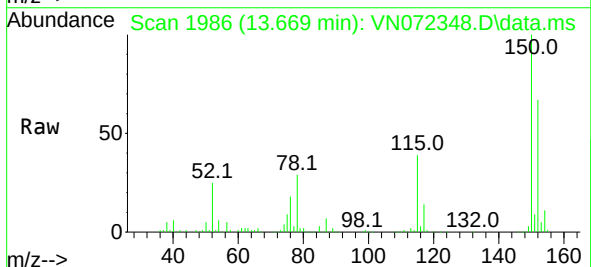




#74
N-amy1 acetate
Concen: 0.436 ug/l
RT: 12.386 min Scan# 1768
Delta R.T. 0.006 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion: 43	Resp:	2321	
Ion	Ratio	Lower	Upper
43	100		
70	47.3	39.0	58.4
55	26.5	21.1	31.7
61	28.7	21.1	31.7

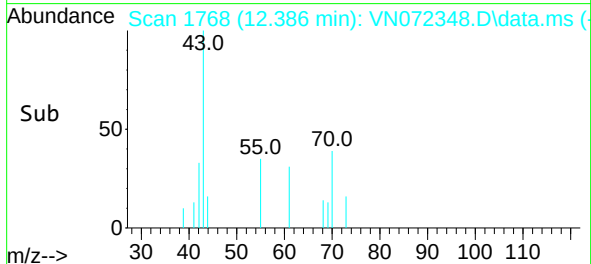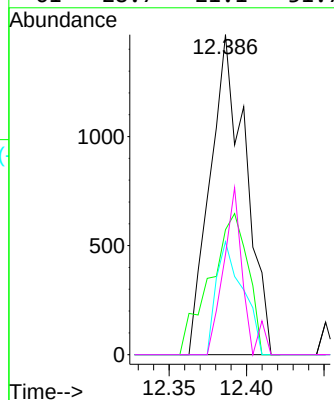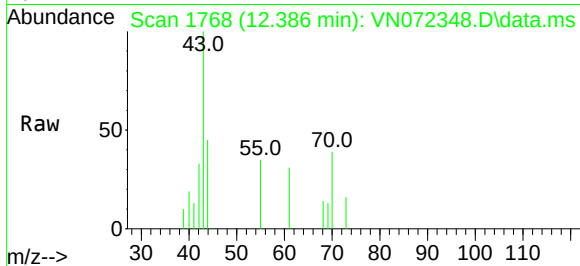

#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.816 min Scan# 1841
Delta R.T. -0.006 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion: 83	Resp:	680	
Ion Ratio	Lower	Upper	
83 100			
131 0.0	5.3	15.9#	
85 37.1	32.3	96.9	


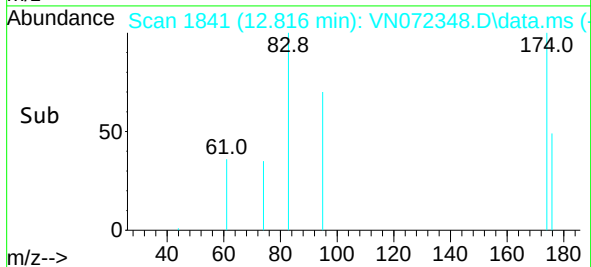
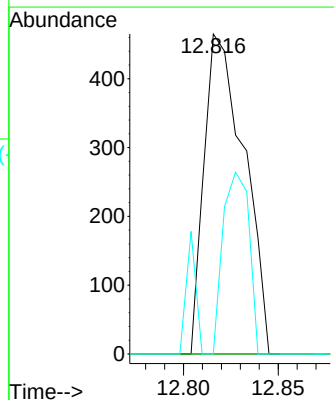
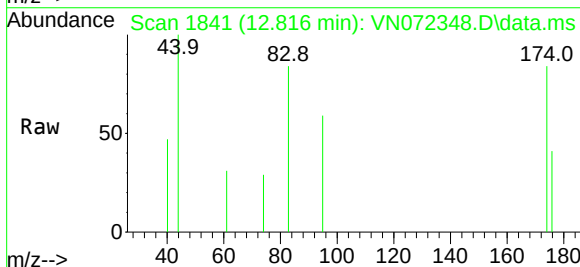


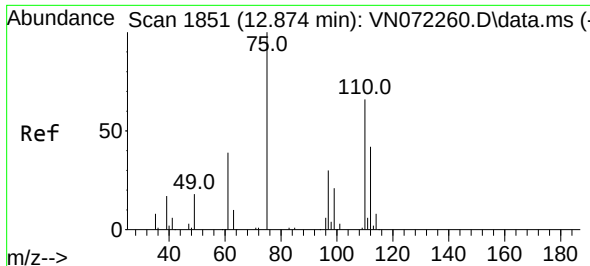

#76
1,2,3-Trichloropropane
Concen: 28.411 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion: 75 Resp: 102750
Ion Ratio Lower Upper
75 100
77 0.7 98.5 295.5#

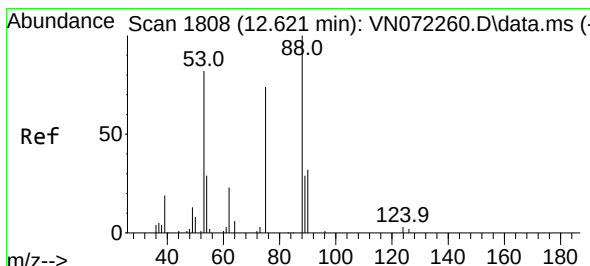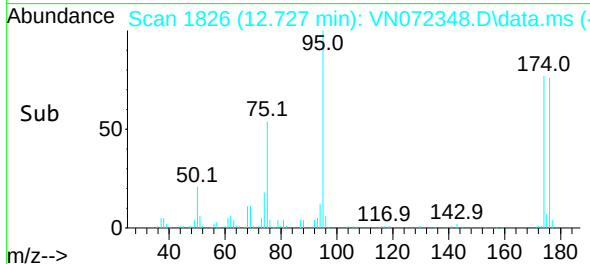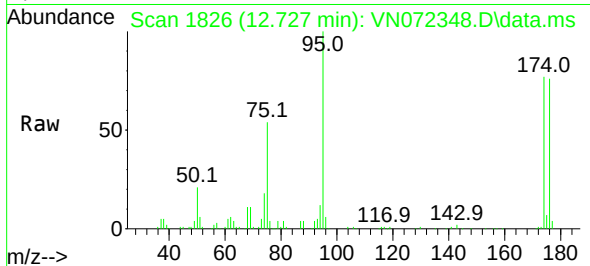

#81
trans-1,4-Dichloro-2-butene
Concen: 73.785 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.105 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion: 75 Resp: 102750
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#


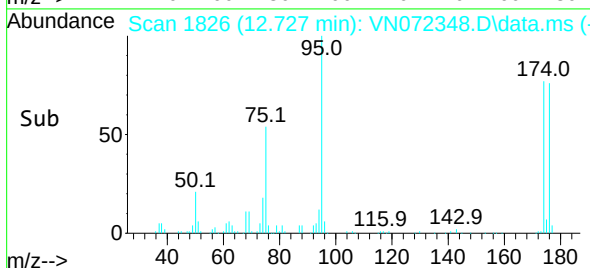

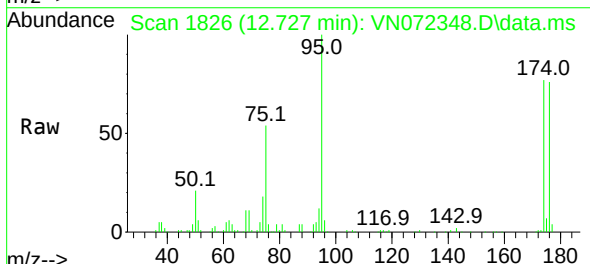




#87
1,3-Dichlorobenzene
Concen: 0.273 ug/l
RT: 13.610 min Scan# 1976
Delta R.T. -0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion:146 Resp: 1485
Ion Ratio Lower Upper
146 100
111 34.9 20.0 60.0
148 51.6 32.0 96.0

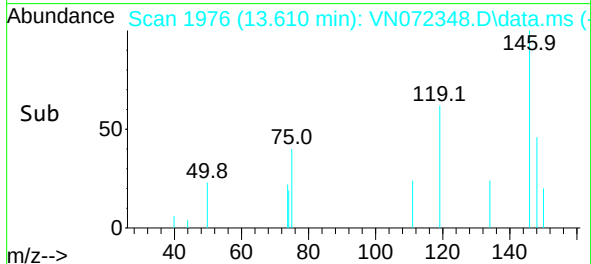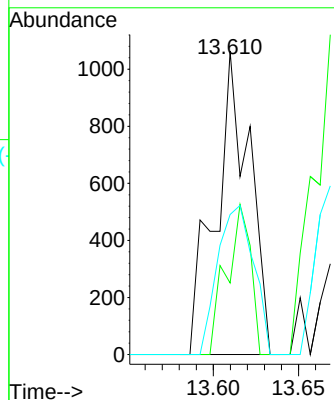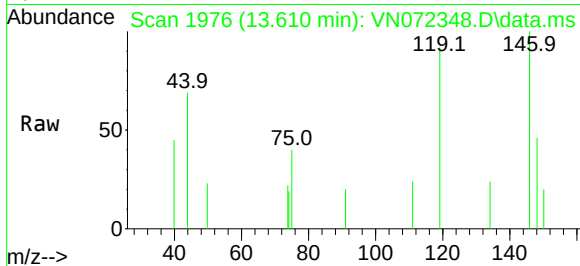

#88
1,4-Dichlorobenzene
Concen: 0.281 ug/l
RT: 13.610 min Scan# 1976
Delta R.T. -0.082 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion:146 Resp: 1485
Ion Ratio Lower Upper
146 100
111 34.9 19.1 57.1
148 51.6 31.4 94.3


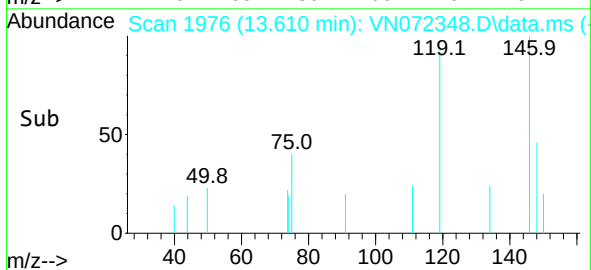
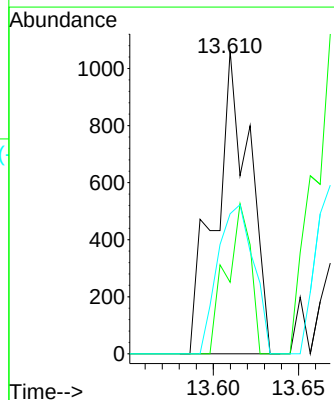
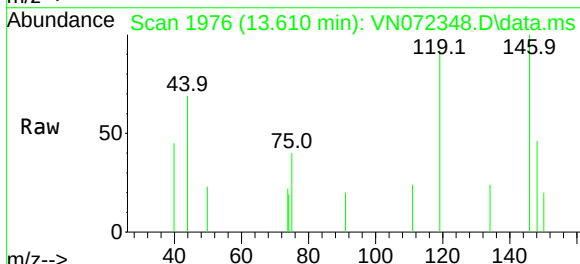




#89
n-Butylbenzene
Concen: 0.349 ug/l
RT: 13.939 min Scan# 2032
Delta R.T. 0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20




Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01


Tgt Ion: 91 Resp: 2828
Ion Ratio Lower Upper
91 100
92 53.1 26.9 80.7
134 19.2 13.6 40.8

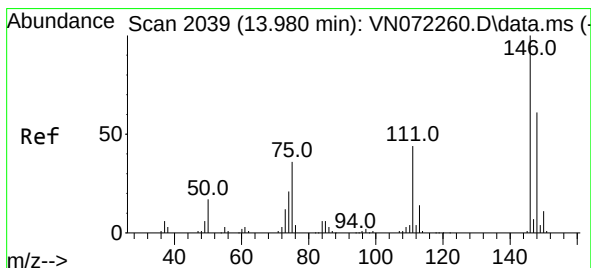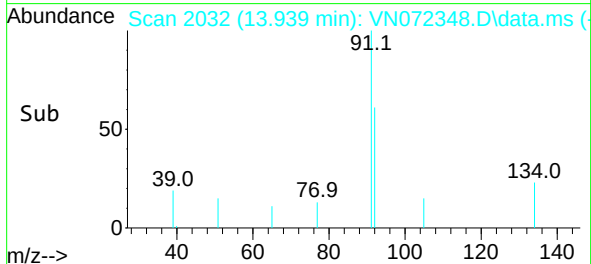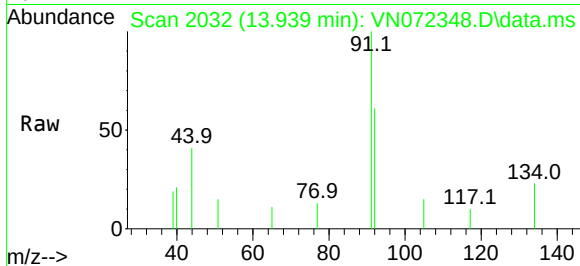

#91
1,2-Dichlorobenzene
Concen: 0.249 ug/l
RT: 13.986 min Scan# 2040
Delta R.T. 0.000 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion: 146 Resp: 1336
Ion Ratio Lower Upper
146 100
111 28.2 20.9 62.8
148 81.1 32.1 96.3


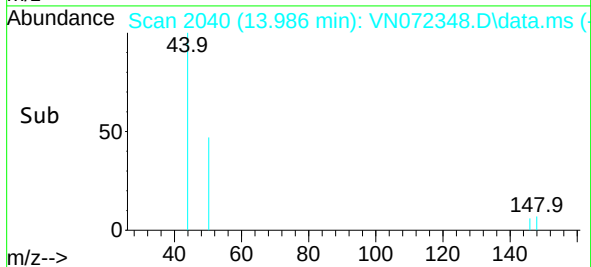

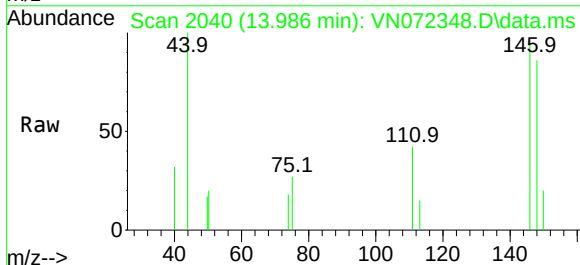




#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.331 ug/l
 RT: 14.604 min Scan# 2145
 Delta R.T. 0.006 min
 Lab File: VN072348.D
 Acq: 06 May 2022 12:20




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0506MBL01


Tgt Ion: 75 Resp: 326
 Ion Ratio Lower Upper
 75 100
 155 19.9 44.9 134.5#
 157 75.8 59.0 176.8

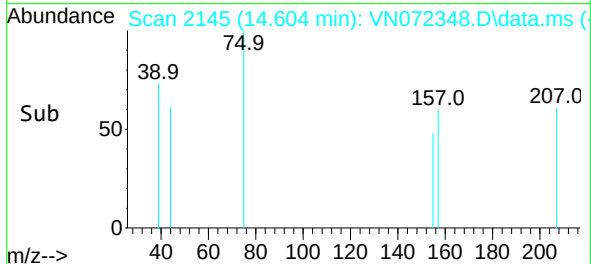

#93
 1,2,4-Trichlorobenzene
 Concen: 3.233 ug/l
 RT: 15.263 min Scan# 2257
 Delta R.T. 0.006 min
 Lab File: VN072348.D
 Acq: 06 May 2022 12:20

Tgt Ion: 180 Resp: 2119
 Ion Ratio Lower Upper
 180 100
 182 77.3 47.5 142.5
 145 21.5 14.5 43.5


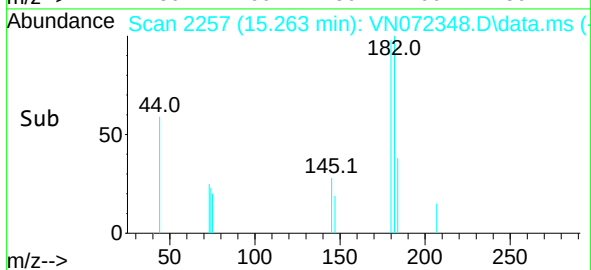

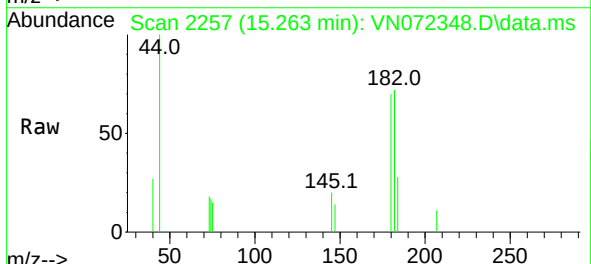


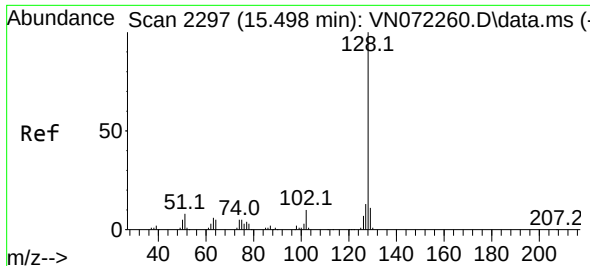

#95
Naphthalene
Concen: 5.090 ug/l
RT: 15.510 min Scan# 2299
Delta R.T. 0.012 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Instrument :
MSVOA_N
ClientSampleId :
VN0506MBL01

Tgt Ion:128 Resp: 7209
Ion Ratio Lower Upper
128 100
127 13.6 10.3 15.5
129 8.4 8.6 13.0#

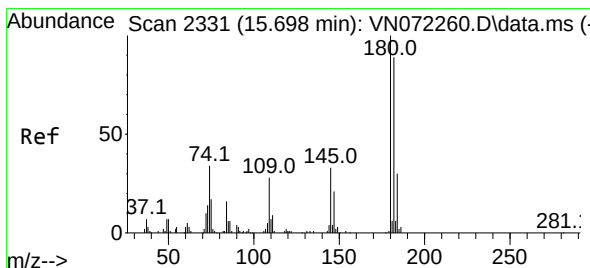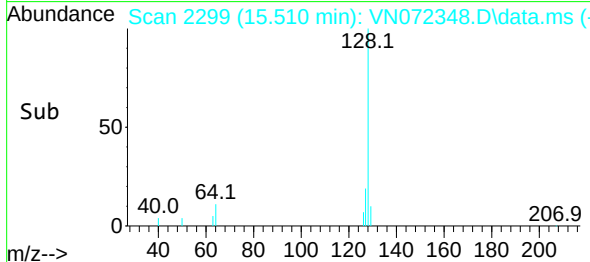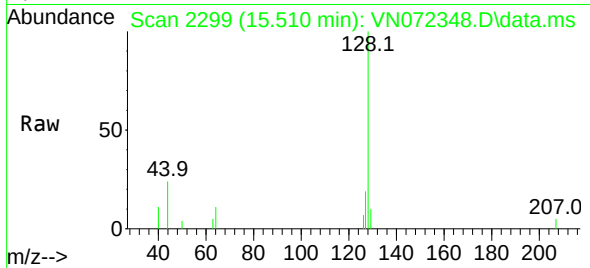

#96
1,2,3-Trichlorobenzene
Concen: 3.487 ug/l
RT: 15.698 min Scan# 2331
Delta R.T. 0.006 min
Lab File: VN072348.D
Acq: 06 May 2022 12:20

Tgt Ion:180 Resp: 2125
Ion Ratio Lower Upper
180 100
182 95.6 47.8 143.3
145 34.2 15.5 46.5

