

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
 Data File : VN072354.D
 Acq On : 06 May 2022 14:59
 Operator : JC\MD
 Sample : N2725-05 20X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TRE-1278

Quant Time: May 09 03:13:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 26 18:50:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	251103	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	471284	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	536808	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	212161	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	190673	49.461	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	98.920%		
35) Dibromofluoromethane	8.016	113	145531	48.245	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	96.500%		
50) Toluene-d8	10.439	98	612337	51.661	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	103.320%		
62) 4-Bromofluorobenzene	12.727	95	250412	63.650	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	127.300%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.304	50	752	Below Cal	#	43
5) Bromomethane	2.810	94	418	Below Cal		98
6) Chloroethane	2.998	64	574	Below Cal	#	42
11) Tert butyl alcohol	5.316	59	10320	16.290	ug/l #	72
13) Acrolein	4.057	56	133	0.209	ug/l #	74
14) Allyl chloride	4.581	41	14103	2.832	ug/l #	60
16) Acetone	4.281	43	442888	266.472	ug/l	95
17) Carbon Disulfide	4.534	76	506	0.452	ug/l #	75
18) Methyl Acetate	4.863	43	3159	0.641	ug/l #	68
20) Methylene Chloride	5.087	84	1837	0.577	ug/l #	81
25) 2-Butanone	7.333	43	47397	17.906	ug/l #	85
29) Tetrahydrofuran	7.710	42	1425	0.820	ug/l #	29
31) Cyclohexane	8.075	56	5469	1.062	ug/l #	6
36) 1,1-Dichloropropene	8.081	75	20727	4.721	ug/l #	49
37) Ethyl Acetate	7.410	43	60467	10.370	ug/l	98
38) Carbon Tetrachloride	8.081	117	27359	5.818	ug/l #	16
41) Methacrylonitrile	7.675	41	2221	0.753	ug/l #	28
43) Isopropyl Acetate	8.557	43	625	0.868	ug/l #	53
51) 4-Methyl-2-Pentanone	10.327	43	11359	2.065	ug/l #	82
52) Toluene	10.498	92	15078	1.852	ug/l	95
56) Ethyl methacrylate	10.763	69	135	2.387	ug/l #	1
59) 2-Hexanone	11.086	43	1614	0.416	ug/l	81
68) m/p-Xylenes	11.945	106	2391	0.340	ug/l	93
74) N-amyl acetate	12.351	43	4168	0.594	ug/l #	39
75) 1,1,2,2-Tetrachloroethane	12.833	83	68	Below Cal	#	25
76) 1,2,3-Trichloropropane	12.727	75	136377	28.620	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	136377	74.325	ug/l #	11
93) 1,2,4-Trichlorobenzene	15.262	180	402	2.537	ug/l	58
95) Naphthalene	15.498	128	4732	4.693	ug/l #	79
96) 1,2,3-Trichlorobenzene	15.692	180	287	2.757	ug/l #	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
Data File : VN072354.D
Acq On : 06 May 2022 14:59
Operator : JC\MD
Sample : N2725-05 20X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TRE-1278

Quant Time: May 09 03:13:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 26 18:50:11 2022
Response via : Initial Calibration




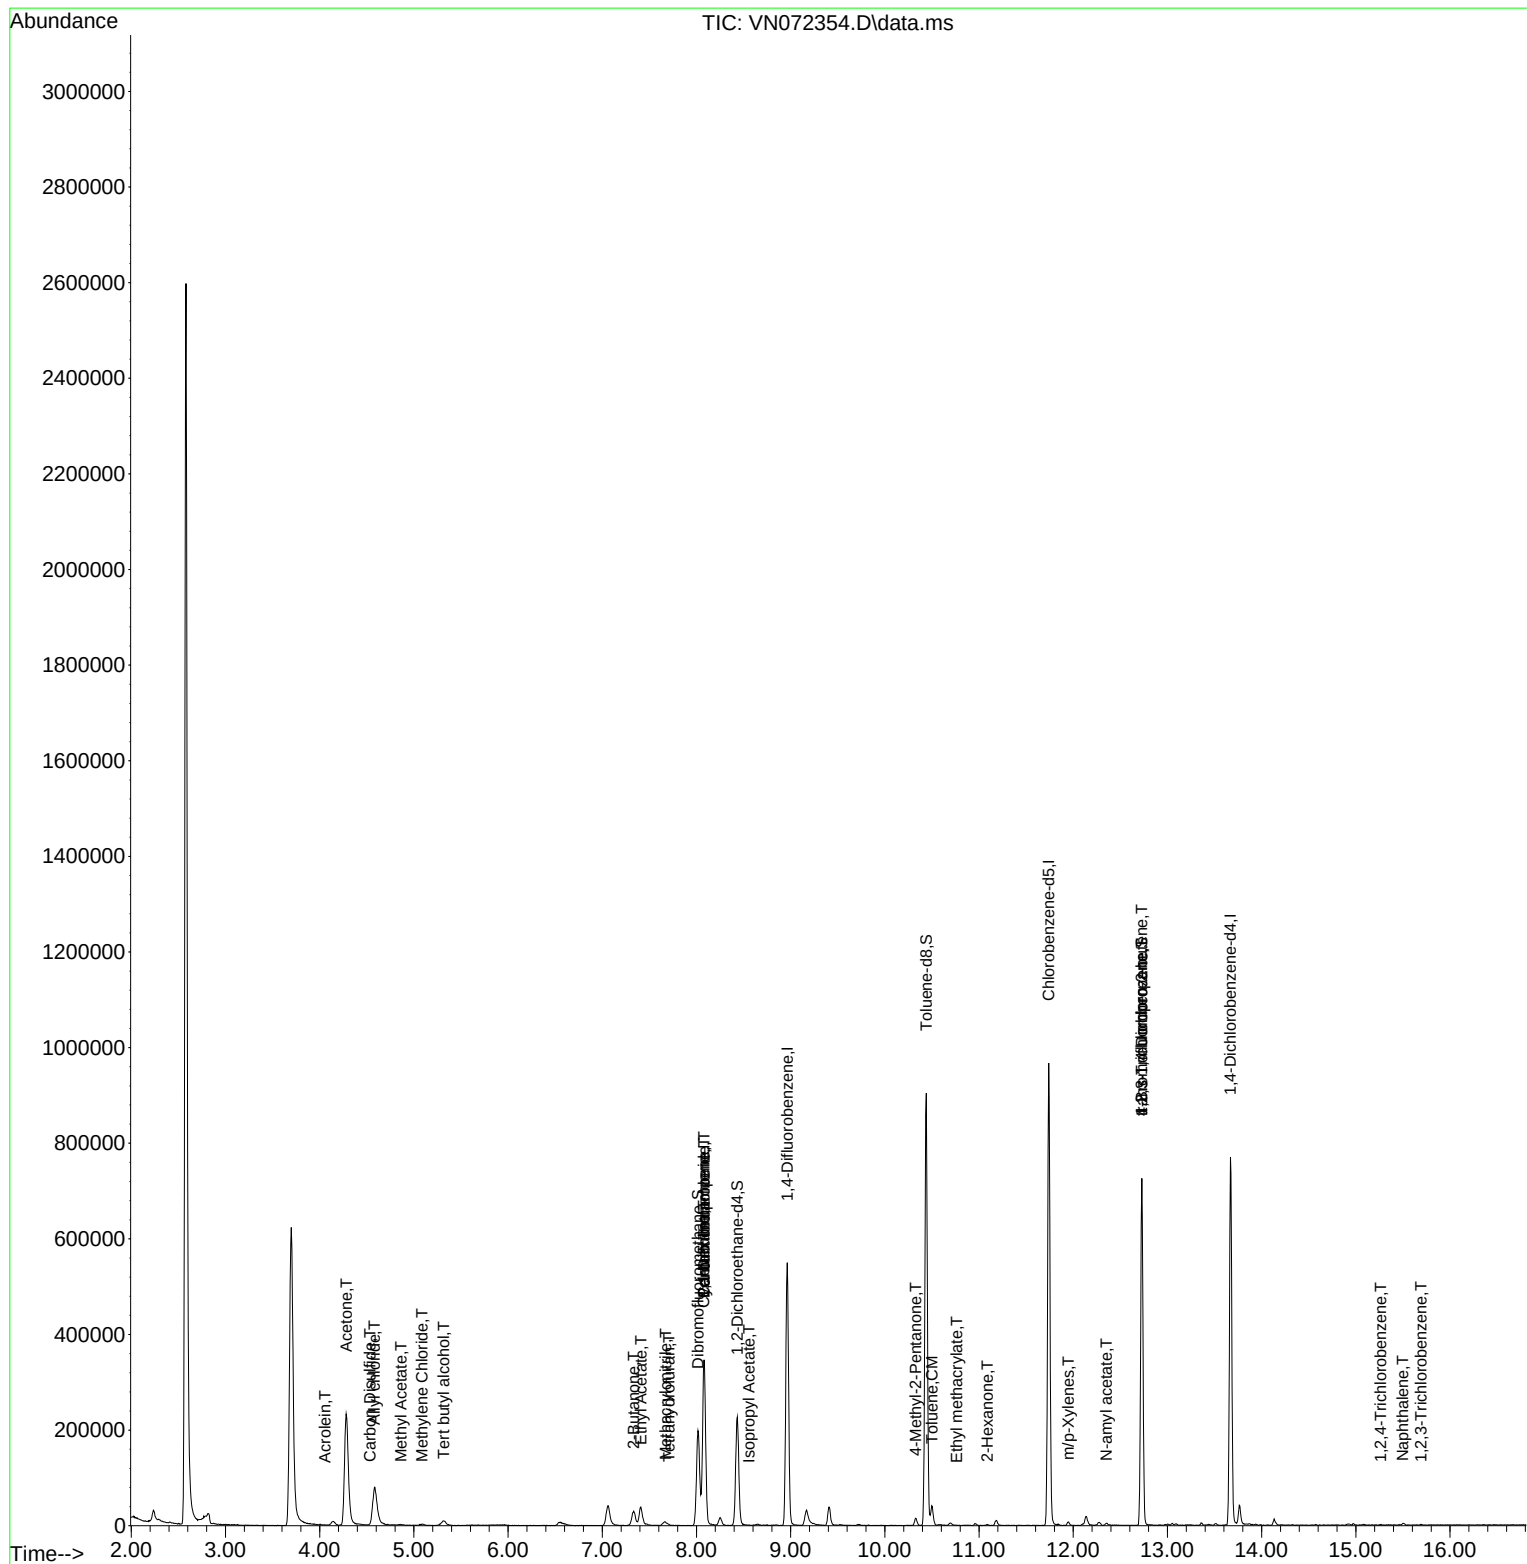




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59




Instrument :
MSVOA_N
ClientSampleId :
TRE-1278


Tgt Ion:168 Resp: 251103
Ion Ratio Lower Upper
168 100
99 60.0 42.3 63.5

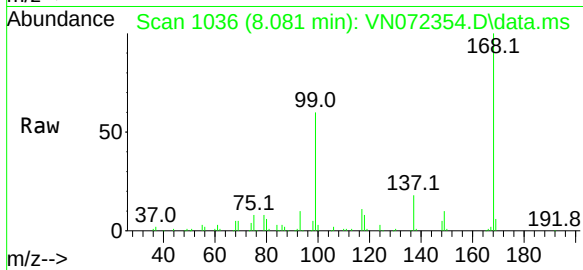

#3
Chloromethane
Concen: Below Cal
RT: 2.304 min Scan# 54
Delta R.T. 0.005 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion: 50 Resp: 752
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5#




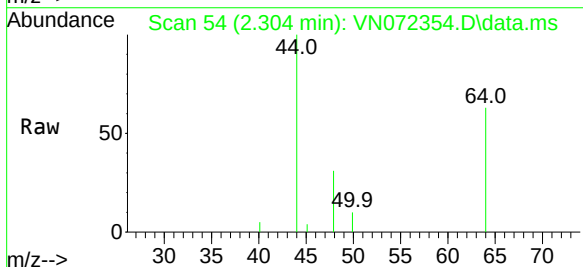


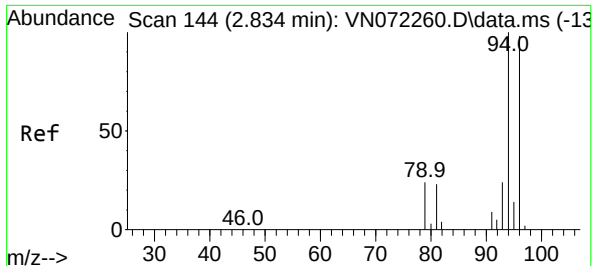

#5
Bromomethane
Concen: Below Cal
RT: 2.810 min Scan# 144
Delta R.T. -0.024 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59




Instrument :
MSVOA_N
ClientSampleId :
TRE-1278


Tgt Ion: 94 Resp: 418
Ion Ratio Lower Upper
94 100
96 97.3 76.0 114.0

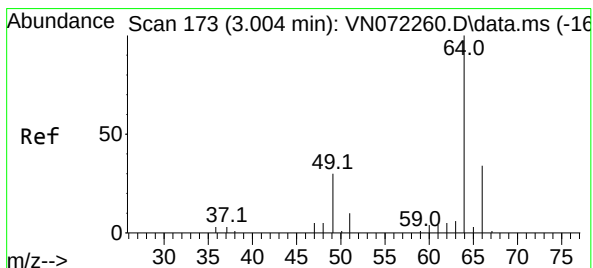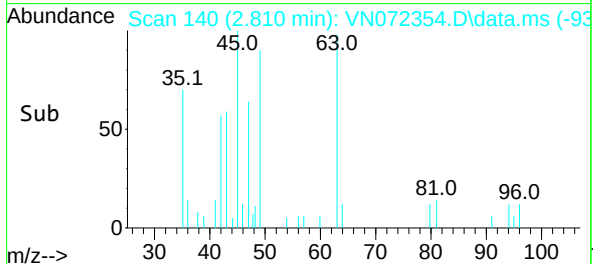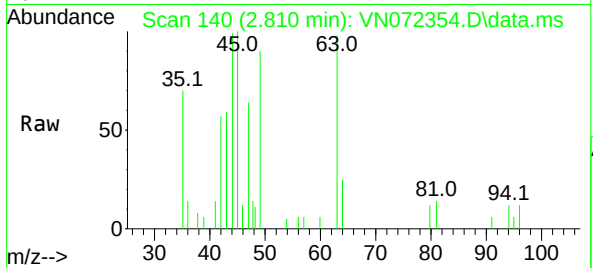

#6
Chloroethane
Concen: Below Cal
RT: 2.998 min Scan# 172
Delta R.T. -0.007 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion: 64 Resp: 574
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#


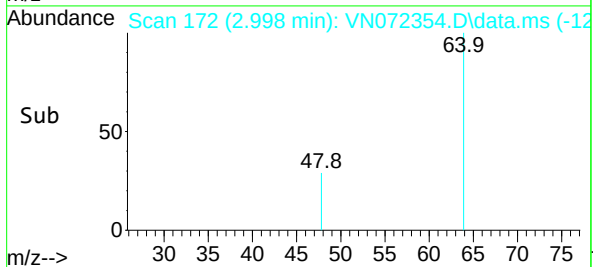

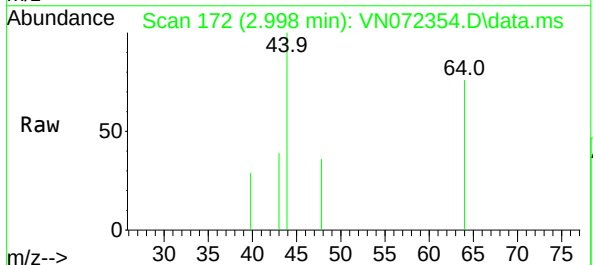




#11
Tert butyl alcohol
Concen: 16.290 ug/l
RT: 5.316 min Scan# 50
Delta R.T. -0.047 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59




Instrument :
MSVOA_N
ClientSampleId :
TRE-1278


Tgt Ion: 59 Resp: 10320
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

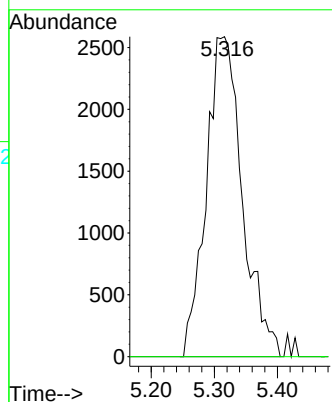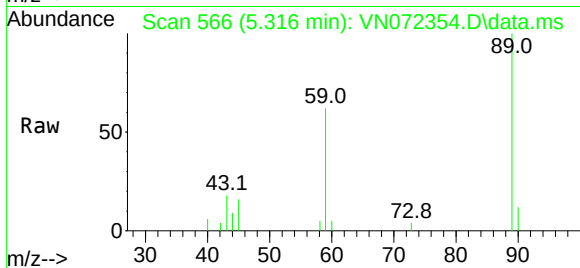

#13
Acrolein
Concen: 0.209 ug/l
RT: 4.057 min Scan# 352
Delta R.T. 0.017 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion: 56 Resp: 133
Ion Ratio Lower Upper
56 100
55 47.4 54.8 82.2#

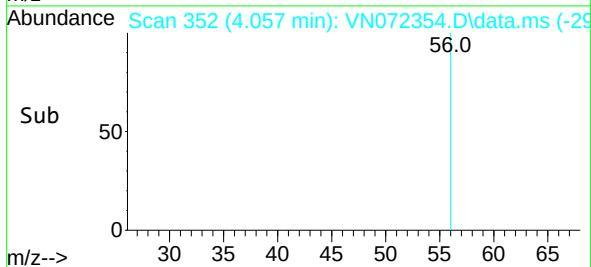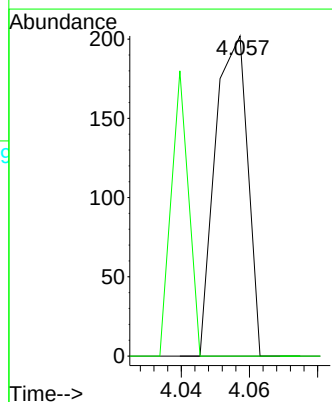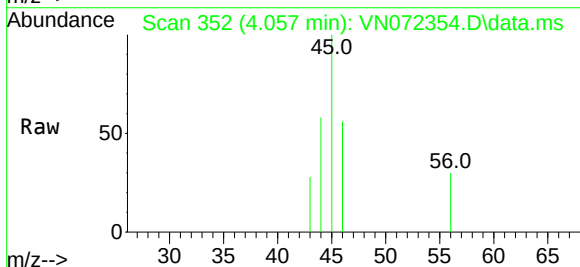



#14

Allyl chloride

Concen: 2.832 ug/l

RT: 4.581 min Scan# 441

Delta R.T. -0.259 min

Lab File: VN072354.D

Acq: 06 May 2022 14:59

Instrument :

MSVOA_N

ClientSampleId :

TRE-1278





Tgt Ion: 41 Resp: 14103

Ion Ratio Lower Upper

41 100

39 88.6 53.2 79.8#

76 0.0 29.9 44.9#

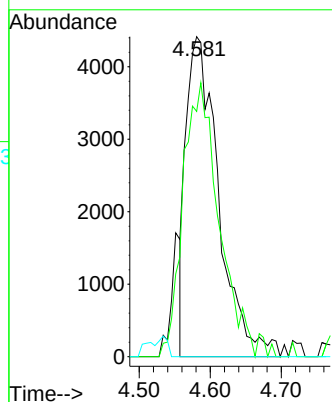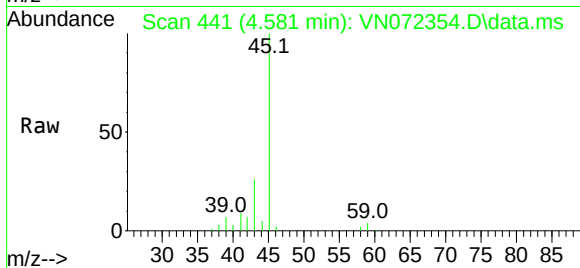

#16

Acetone

Concen: 266.472 ug/l

RT: 4.281 min Scan# 390

Delta R.T. -0.000 min

Lab File: VN072354.D




Acq: 06 May 2022 14:59


Tgt Ion: 43 Resp: 442888

Ion Ratio Lower Upper

43 100

58 29.6 26.0 39.0

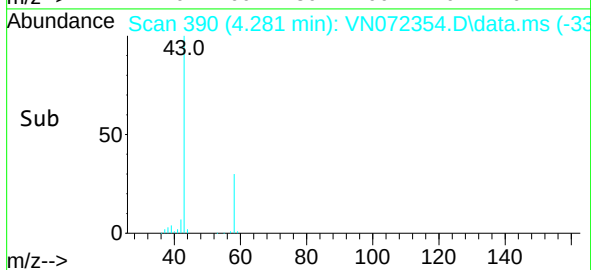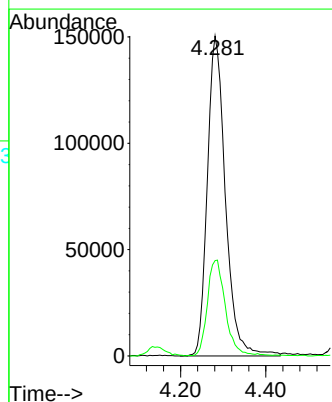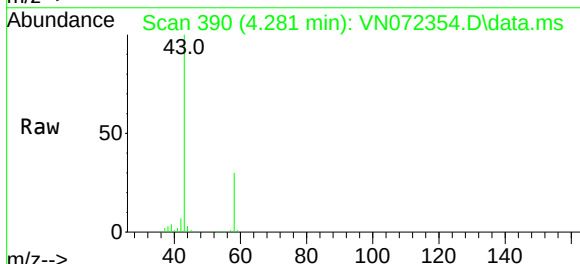



#17

Carbon Disulfide

Concen: 0.452 ug/l

RT: 4.534 min Scan# 41

Delta R.T. -0.000 min

Lab File: VN072354.D

Acq: 06 May 2022 14:59

Instrument :

MSVOA_N

ClientSampleId :





TRE-1278

Tgt Ion: 76 Resp: 506

Ion Ratio Lower Upper

76 100

78 0.0 7.2 10.8#

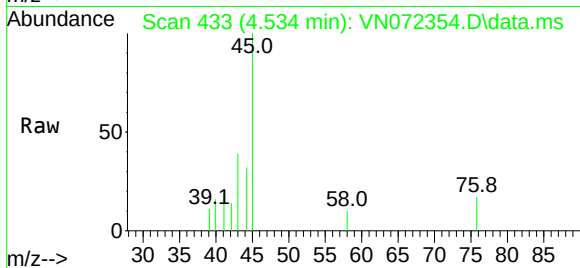

#18

Methyl Acetate

Concen: 0.641 ug/l

RT: 4.863 min Scan# 489

Delta R.T. 0.012 min

Lab File: VN072354.D




Acq: 06 May 2022 14:59


Tgt Ion: 43 Resp: 3159

Ion Ratio Lower Upper

43 100


74 10.5 21.6 32.4#

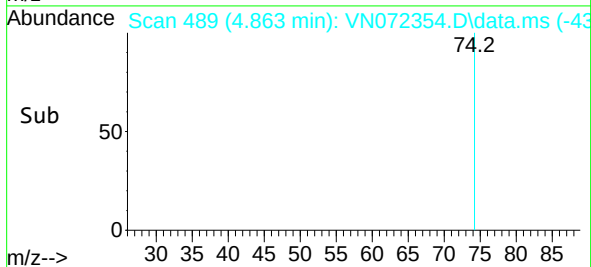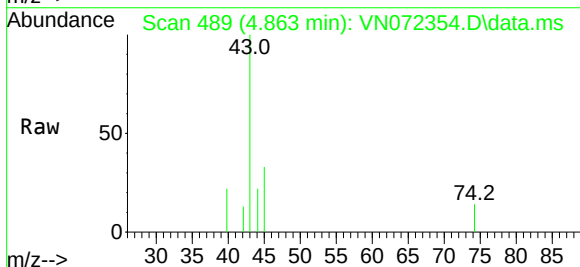





#20
Methylene Chloride
Concen: 0.577 ug/l
RT: 5.087 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Instrument :
MSVOA_N
ClientSampleId :
TRE-1278







Tgt Ion: 84	Resp: 1837
Ion Ratio	Lower Upper
84 100	
49 117.1	88.3 132.5
51 49.4	28.2 42.2#
86 93.7	50.6 76.0#



#25
2-Butanone
Concen: 17.906 ug/l
RT: 7.333 min Scan# 909
Delta R.T. 0.005 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion: 43	Resp: 47397
Ion Ratio	Lower Upper
43 100	
72 21.7	23.7 35.5#

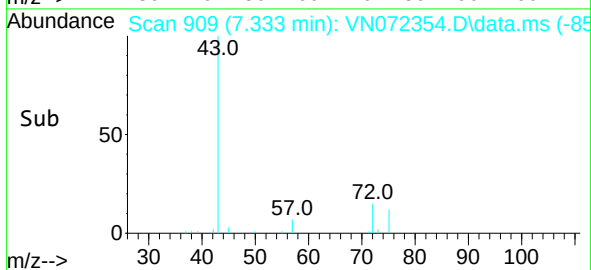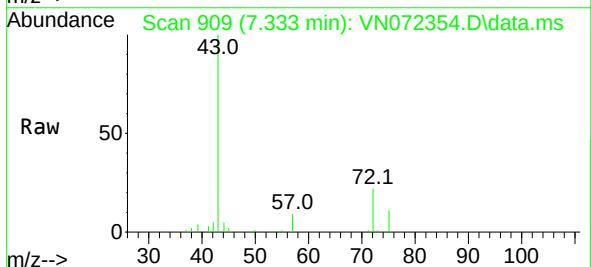



#29

Tetrahydrofuran

Concen: 0.820 ug/l

RT: 7.710 min Scan# 91

Delta R.T. 0.029 min

Lab File: VN072354.D

Acq: 06 May 2022 14:59

Instrument :

MSVOA_N

ClientSampleId :

TRE-1278





Tgt Ion: 42 Resp: 1425

Ion Ratio Lower Upper

42 100

72 0.0 39.7 59.5#

71 0.0 36.6 55.0#

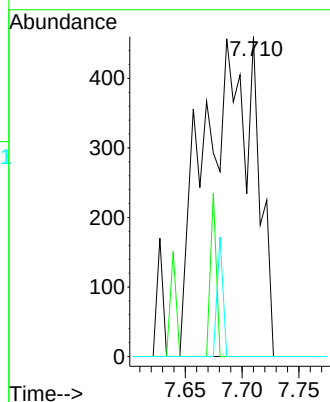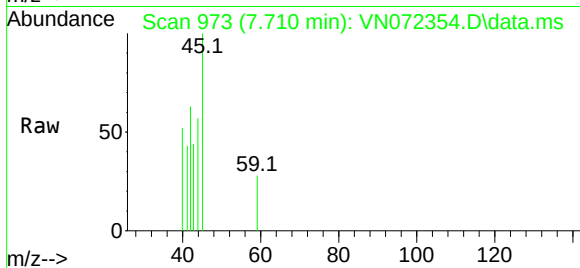

#31

Cyclohexane

Concen: 1.062 ug/l

RT: 8.075 min Scan# 1035

Delta R.T. -0.017 min

Lab File: VN072354.D

Acq: 06 May 2022 14:59




Tgt Ion: 56 Resp: 5469


Ion Ratio Lower Upper

56 100

69 151.3 27.8 41.8#

84 150.4 76.9 115.3#

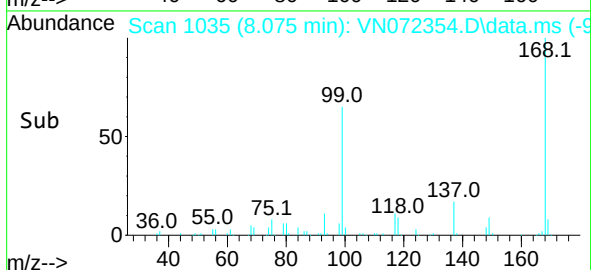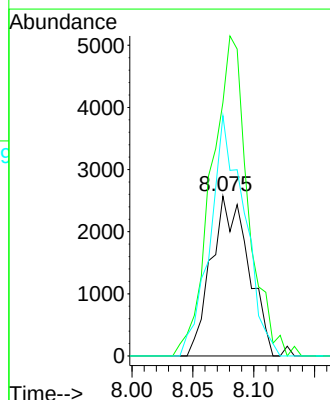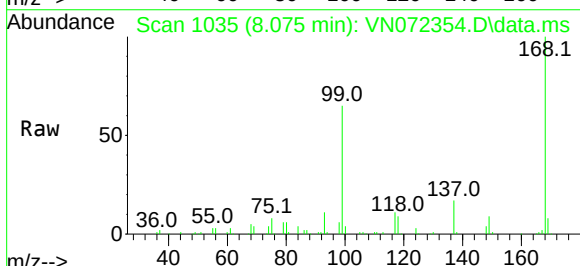

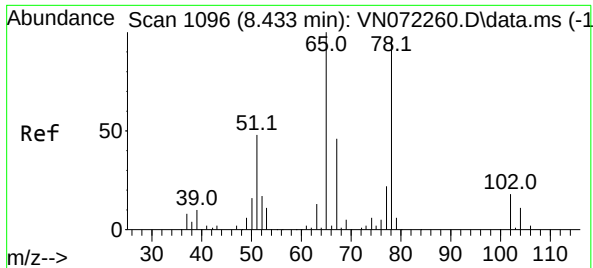

#33

1,2-Dichloroethane-d4

Concen: 49.461 ug/l

RT: 8.433 min Scan# 1096

Delta R.T. -0.001 min

Lab File: VN072354.D

Acq: 06 May 2022 14:59

Instrument :

MSVOA_N

ClientSampleId :





TRE-1278

Tgt Ion: 65 Resp: 190673

Ion Ratio Lower Upper

65 100

67 51.0 0.0 104.8

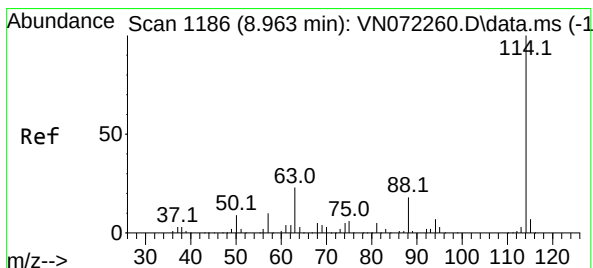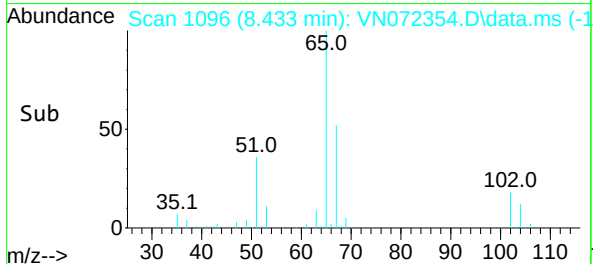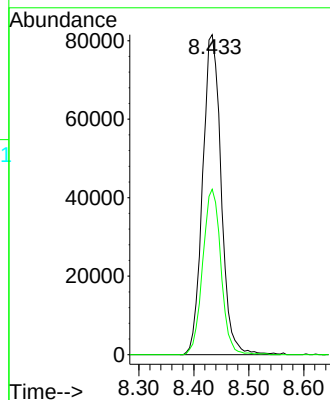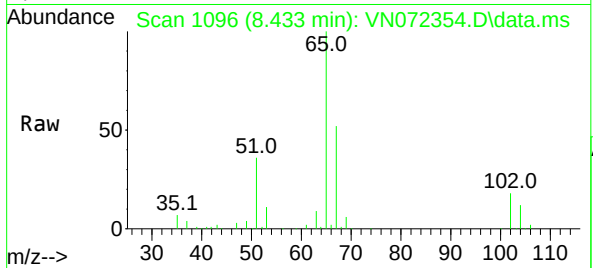

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072354.D

Acq: 06 May 2022 14:59




Tgt Ion: 114 Resp: 471284


Ion Ratio Lower Upper

114 100

63 22.0 0.0 40.0

88 17.4 0.0 32.6

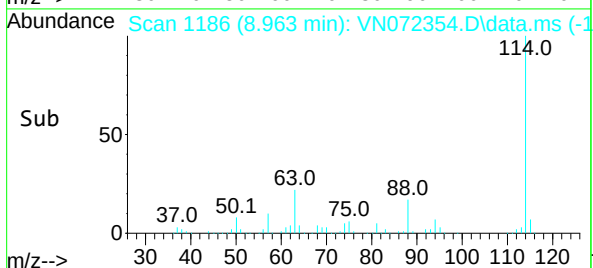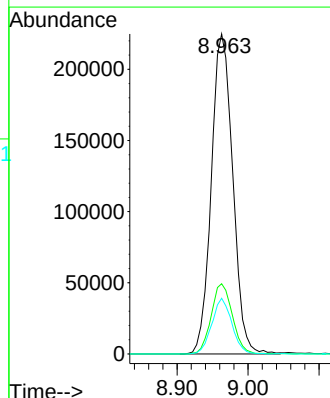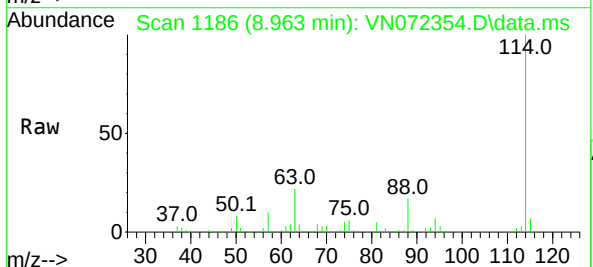

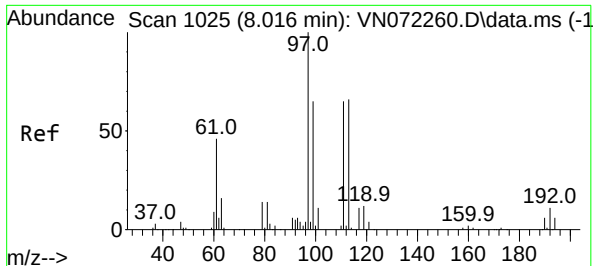

#35

Dibromofluoromethane

Concen: 48.245 ug/l

RT: 8.016 min Scan# 1035

Delta R.T. -0.000 min

Lab File: VN072354.D

Acq: 06 May 2022 14:59

Instrument :

MSVOA_N

ClientSampleId :

TRE-1278





Tgt Ion:113 Resp: 145531

Ion Ratio Lower Upper

113 100

111 103.9 81.4 122.0

192 19.3 17.0 25.6

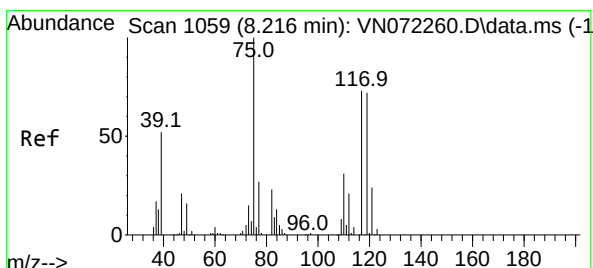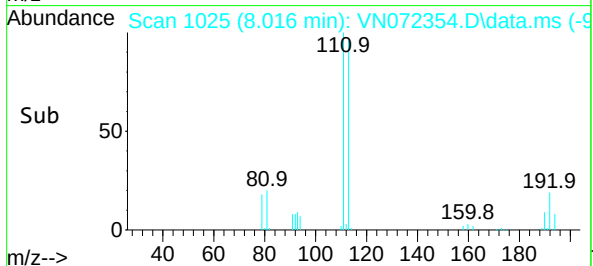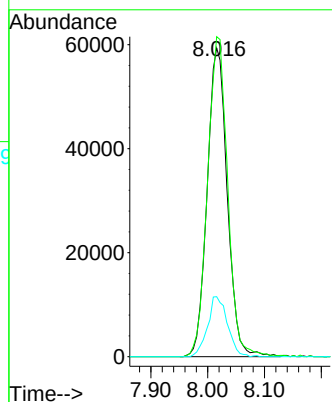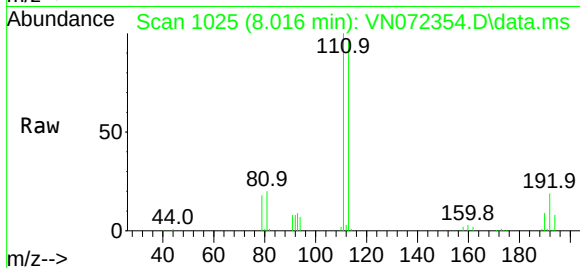

#36

1,1-Dichloropropene

Concen: 4.721 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.135 min

Lab File: VN072354.D

Acq: 06 May 2022 14:59




Tgt Ion: 75 Resp: 20727


Ion Ratio Lower Upper

75 100

110 9.6 18.3 54.8#

77 0.0 25.1 37.7#


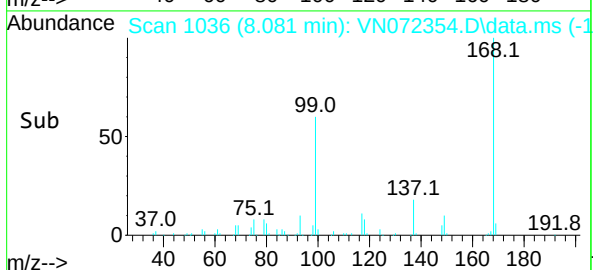

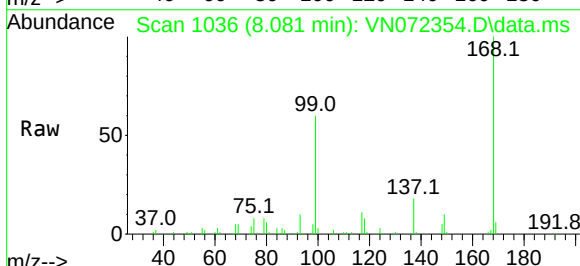




#37
Ethyl Acetate
Concen: 10.370 ug/l
RT: 7.410 min Scan# 91
Delta R.T. -0.000 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59




Instrument :
MSVOA_N
ClientSampleId :
TRE-1278


Tgt Ion: 43 Resp: 60467
Ion Ratio Lower Upper
43 100
61 14.7 11.8 17.6
70 9.8 9.3 13.9



#38
Carbon Tetrachloride
Concen: 5.818 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.123 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion: 117 Resp: 27359
Ion Ratio Lower Upper
117 100
119 4.8 75.8 113.8#
121 0.0 24.6 37.0#



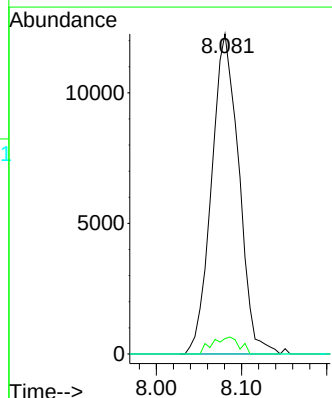





#41
Methacrylonitrile
Concen: 0.753 ug/l
RT: 7.675 min Scan# 90
Delta R.T. 0.041 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59




Instrument :
MSVOA_N
ClientSampleId :
TRE-1278


Tgt Ion: 41 Resp: 2221
Ion Ratio Lower Upper
41 100
39 28.1 48.6 73.0#
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#

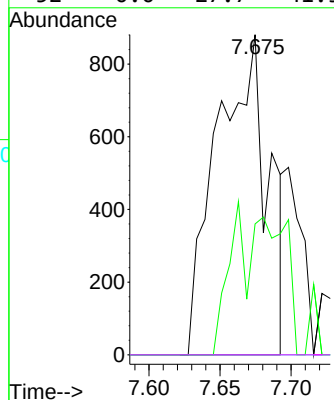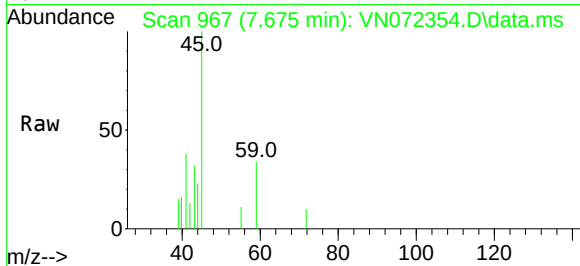

#43
Isopropyl Acetate
Concen: 0.868 ug/l
RT: 8.557 min Scan# 1117
Delta R.T. -0.000 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion: 43 Resp: 625
Ion Ratio Lower Upper
43 100
61 0.0 21.9 32.9#
87 0.0 12.0 18.0#


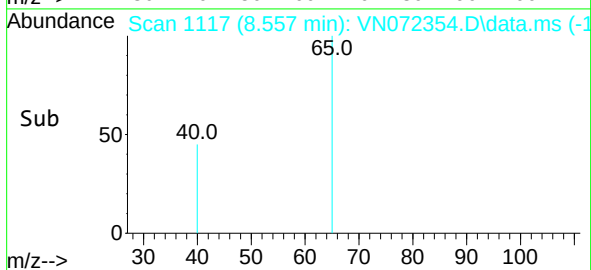
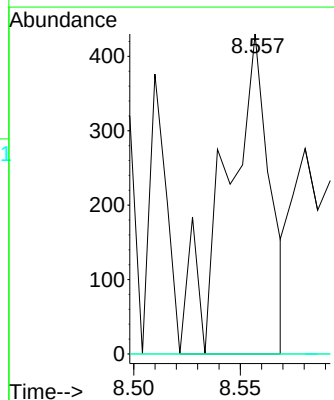
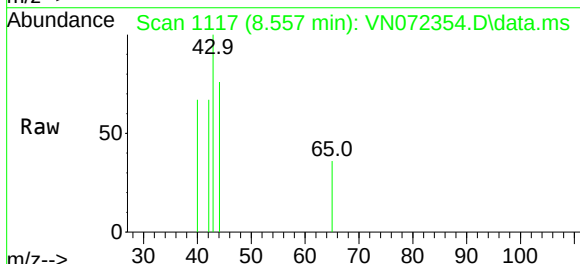




#50
Toluene-d8
Concen: 51.661 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59




Instrument :
MSVOA_N
ClientSampleId :
TRE-1278


Tgt Ion: 98 Resp: 612337
Ion Ratio Lower Upper
98 100
100 64.9 52.6 78.8

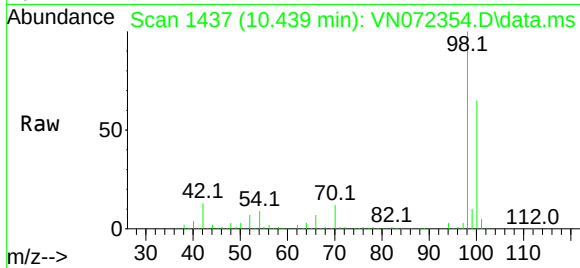

#51
4-Methyl-2-Pentanone
Concen: 2.065 ug/l
RT: 10.327 min Scan# 1418
Delta R.T. -0.001 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion: 43 Resp: 11359
Ion Ratio Lower Upper
43 100
58 31.3 34.1 51.1#


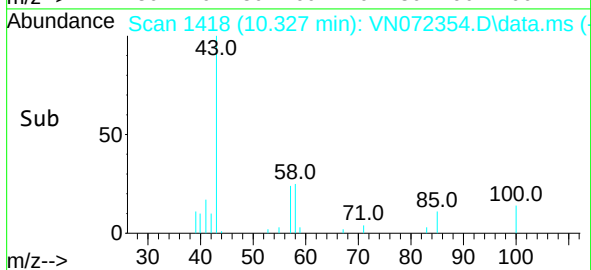
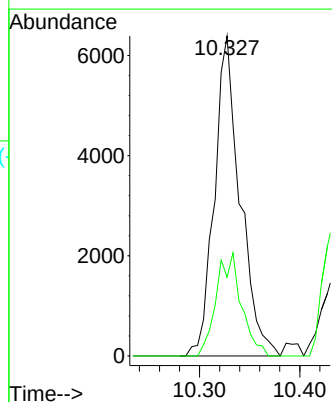
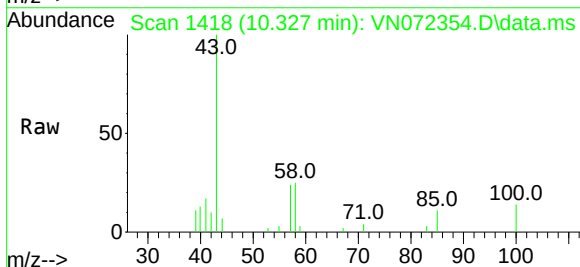




#52
Toluene
Concen: 1.852 ug/l
RT: 10.498 min Scan# 1447
Delta R.T. -0.006 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59




Instrument :
MSVOA_N
ClientSampleId :
TRE-1278


Tgt Ion: 92 Resp: 15078
Ion Ratio Lower Upper
92 100
91 166.2 138.6 207.8

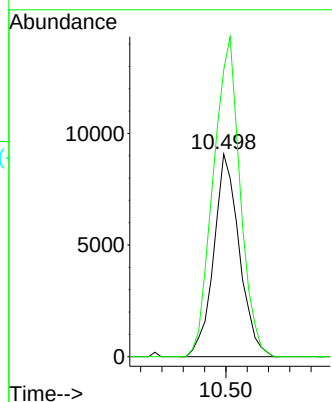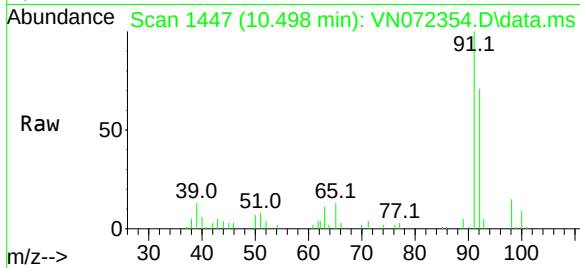

#56
Ethyl methacrylate
Concen: 2.387 ug/l
RT: 10.763 min Scan# 1492
Delta R.T. 0.006 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion: 69 Resp: 135
Ion Ratio Lower Upper
69 100
41 155.6 47.8 71.6#
39 0.0 27.3 40.9#


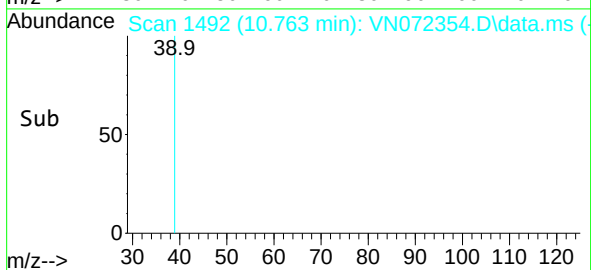

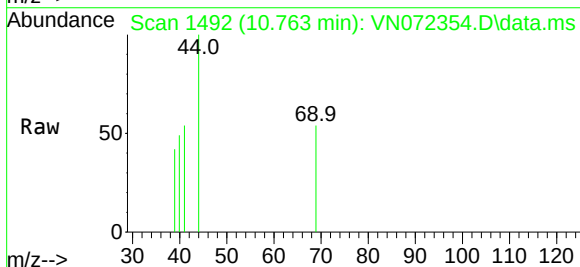




#59
2-Hexanone
Concen: 0.416 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59




Instrument :
MSVOA_N
ClientSampleId :
TRE-1278


Tgt Ion: 43 Resp: 1614
Ion Ratio Lower Upper
43 100
58 45.0 29.7 89.1

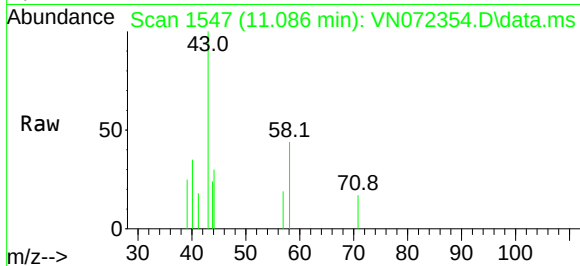

#62
4-Bromofluorobenzene
Concen: 63.650 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion: 95 Resp: 250412
Ion Ratio Lower Upper
95 100
174 76.1 0.0 167.6
176 74.6 0.0 163.4


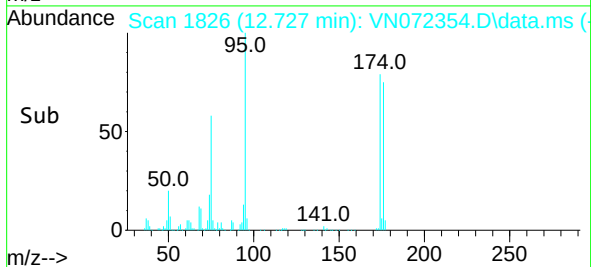

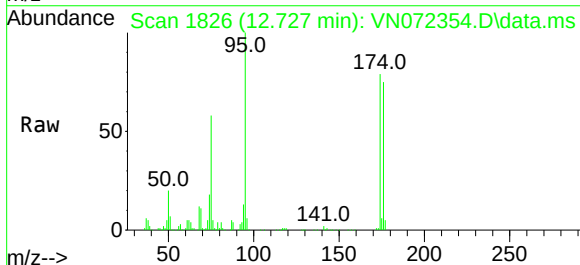




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59




Instrument :
MSVOA_N
ClientSampleId :
TRE-1278


Tgt Ion:117 Resp: 536808
Ion Ratio Lower Upper
117 100
82 57.0 44.2 66.2
119 31.7 25.4 38.0

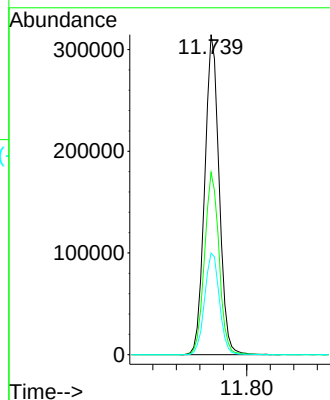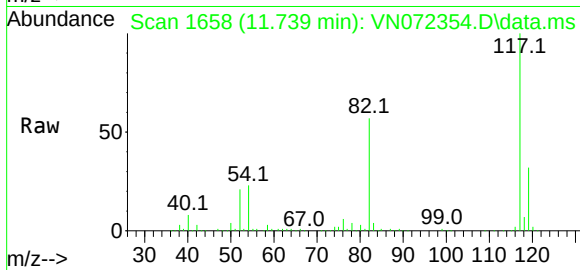

#68
m/p-Xylenes
Concen: 0.340 ug/l
RT: 11.945 min Scan# 1693
Delta R.T. -0.006 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion:106 Resp: 2391
Ion Ratio Lower Upper
106 100
91 209.4 158.9 238.3



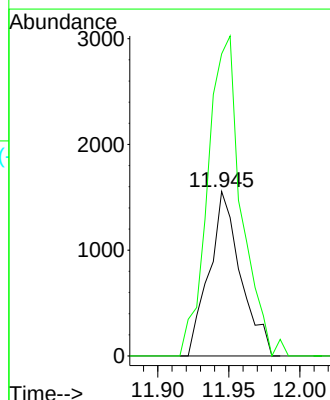
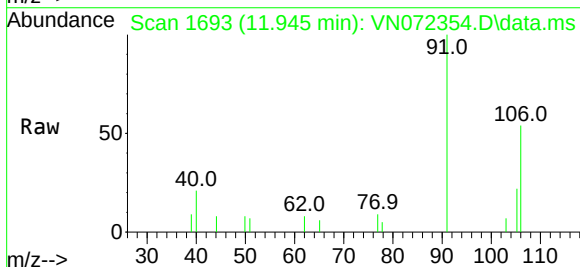


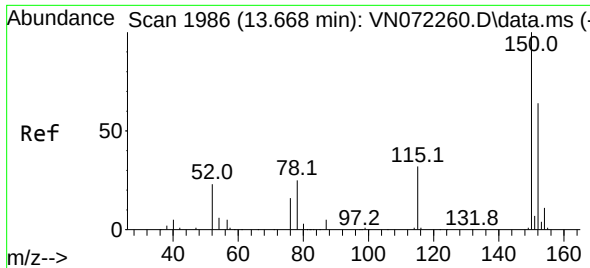

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.668 min Scan# 1986
 Delta R.T. -0.001 min
 Lab File: VN072354.D
 Acq: 06 May 2022 14:59




Instrument :
 MSVOA_N
 ClientSampleId :
 TRE-1278


Tgt Ion:152 Resp: 212161
 Ion Ratio Lower Upper
 152 100
 115 59.3 28.9 86.7
 150 154.4 0.0 356.2

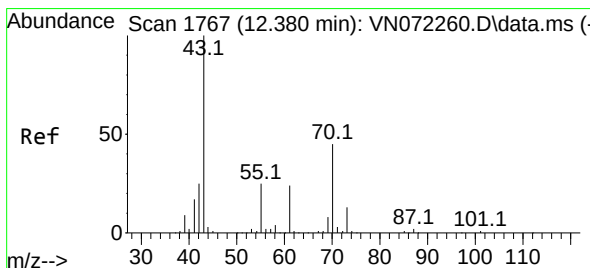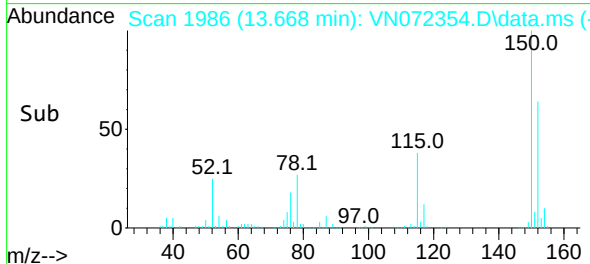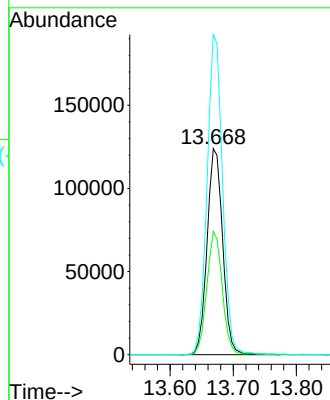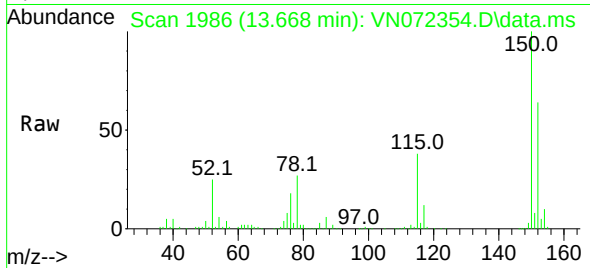

#74
 N-ethyl acetate
 Concen: 0.594 ug/l
 RT: 12.351 min Scan# 1762
 Delta R.T. -0.029 min
 Lab File: VN072354.D
 Acq: 06 May 2022 14:59

Tgt Ion: 43 Resp: 4168
 Ion Ratio Lower Upper
 43 100
 70 0.0 39.0 58.4#
 55 0.0 21.1 31.7#
 61 0.0 21.1 31.7#


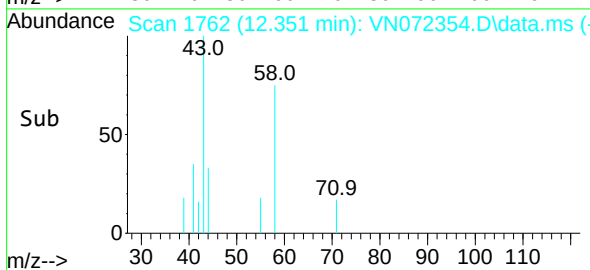
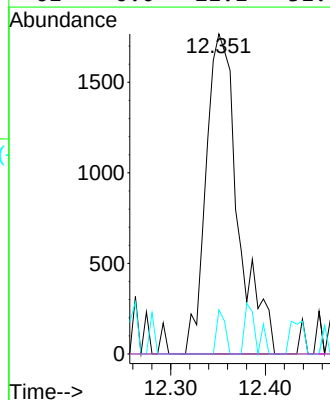
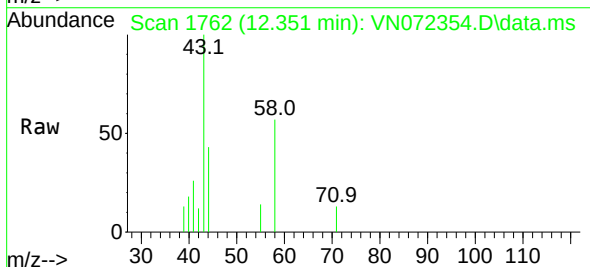




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.833 min Scan# 1844
Delta R.T. 0.011 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59




Instrument :
MSVOA_N
ClientSampleId :
TRE-1278


Tgt Ion: 83 Resp: 68
Ion Ratio Lower Upper
83 100
131 0.0 5.3 15.9#
85 0.0 32.3 96.9#



#76
1,2,3-Trichloropropane
Concen: 28.620 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN072354.D
Acq: 06 May 2022 14:59

Tgt Ion: 75 Resp: 136377
Ion Ratio Lower Upper
75 100
77 1.5 98.5 295.5#


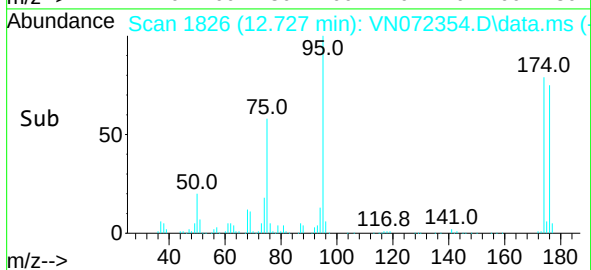




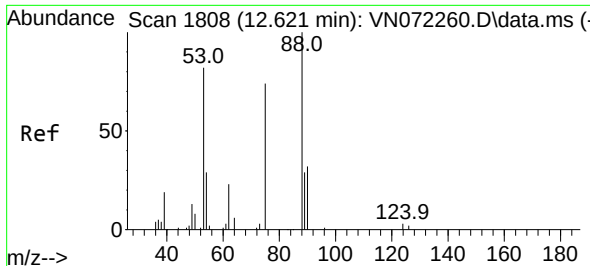

#81
 trans-1,4-Dichloro-2-butene
 Concen: 74.325 ug/l
 RT: 12.727 min Scan# 11
 Delta R.T. 0.105 min
 Lab File: VN072354.D
 Acq: 06 May 2022 14:59




Instrument :
 MSVOA_N
 ClientSampleId :
 TRE-1278


Tgt Ion: 75 Resp: 136377
 Ion Ratio Lower Upper
 75 100
 53 0.1 78.0 117.0#
 89 0.0 37.2 55.8#

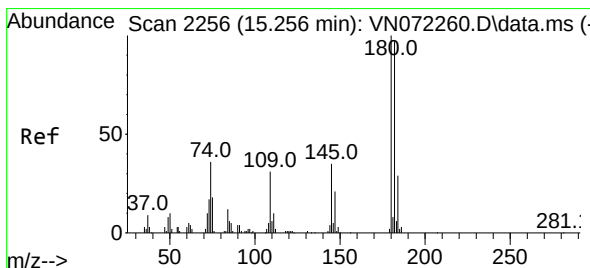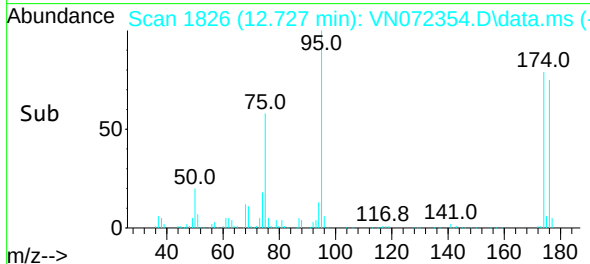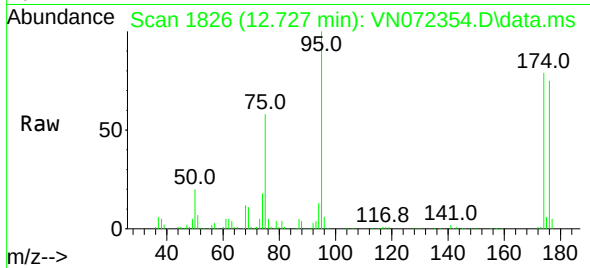

#93
 1,2,4-Trichlorobenzene
 Concen: 2.537 ug/l
 RT: 15.262 min Scan# 2257
 Delta R.T. 0.005 min
 Lab File: VN072354.D
 Acq: 06 May 2022 14:59

Tgt Ion: 180 Resp: 402
 Ion Ratio Lower Upper
 180 100
 182 48.3 47.5 142.5
 145 17.4 14.5 43.5

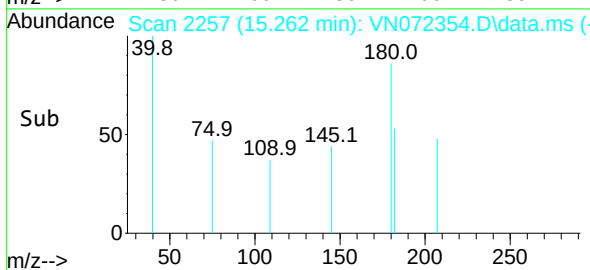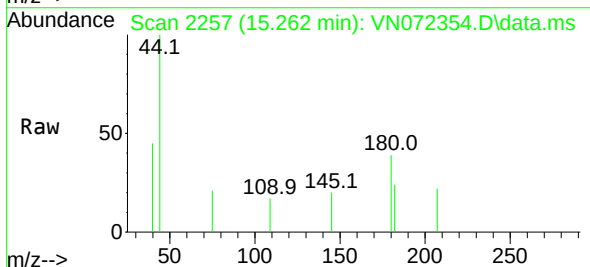



#95

Naphthalene

Concen: 4.693 ug/l

RT: 15.498 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN072354.D

Acq: 06 May 2022 14:59

Instrument :

MSVOA_N

ClientSampleId :

TRE-1278





Tgt Ion:128 Resp: 4732

Ion Ratio Lower Upper

128 100

127 7.2 10.3 15.5#

129 0.0 8.6 13.0#

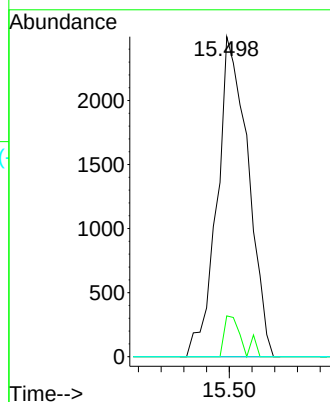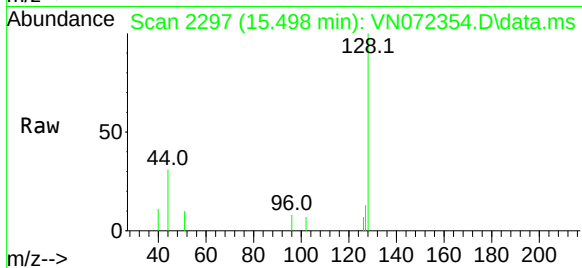

#96

1,2,3-Trichlorobenzene

Concen: 2.757 ug/l

RT: 15.692 min Scan# 2330

Delta R.T. -0.000 min

Lab File: VN072354.D

Acq: 06 May 2022 14:59

Tgt Ion:180 Resp: 287

Ion Ratio Lower Upper

180 100

182 133.4 47.8 143.3

145 0.0 15.5 46.5#

