

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
 Data File : VN072369.D
 Acq On : 06 May 2022 21:02
 Operator : JC\MD
 Sample : N2726-01RE
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FLOOR-DRAINING-TOTERE

Quant Time: May 09 03:17:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 26 18:50:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	294909	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.963	114	567499	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	615694	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	266287	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	218224	48.200	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	96.400%
35) Dibromofluoromethane	8.016	113	168172	46.299	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	92.600%
50) Toluene-d8	10.439	98	731877	51.278	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	102.560%
62) 4-Bromofluorobenzene	12.727	95	300229	63.374	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	126.740%

Target Compounds				Qvalue		
3) Chloromethane	2.299	50	2431	Below Cal	#	43
5) Bromomethane	2.834	94	60	Below Cal	#	2
6) Chloroethane	3.010	64	626	Below Cal	#	44
11) Tert butyl alcohol	5.387	59	685	0.921	ug/l	# 72
16) Acetone	4.281	43	829155	424.774	ug/l	95
17) Carbon Disulfide	4.522	76	1784	0.630	ug/l	# 75
18) Methyl Acetate	4.846	43	15573	2.816	ug/l	# 69
20) Methylene Chloride	5.093	84	9326	2.492	ug/l	87
24) 1,1-Dichloroethane	6.387	63	4081	0.606	ug/l	# 82
25) 2-Butanone	7.340	43	45419	14.610	ug/l	97
30) Chloroform	7.834	83	4678	0.691	ug/l	# 58
31) Cyclohexane	8.081	56	6688	1.106	ug/l	# 1
32) 1,1,1-Trichloroethane	8.004	97	2231	0.388	ug/l	# 44
36) 1,1-Dichloropropene	8.081	75	24953	4.720	ug/l	# 50
37) Ethyl Acetate	7.410	43	58510	8.333	ug/l	97
38) Carbon Tetrachloride	8.081	117	31642	5.588	ug/l	# 15
40) Benzene	8.457	78	7171	0.437	ug/l	# 82
41) Methacrylonitrile	7.645	41	849	0.239	ug/l	# 19
42) 1,2-Dichloroethane	8.528	62	1470	0.234	ug/l	# 74
43) Isopropyl Acetate	8.410	43	36548	4.063	ug/l	# 53
51) 4-Methyl-2-Pentanone	10.328	43	51277	7.740	ug/l	94
52) Toluene	10.498	92	19472	1.986	ug/l	94
56) Ethyl methacrylate	10.763	69	646	2.451	ug/l	# 42
58) 2-Chloroethyl Vinyl ether	9.910	63	72	17.768	ug/l	# 44
59) 2-Hexanone	11.086	43	2472	0.530	ug/l	87
67) Ethyl Benzene	11.839	91	14605	0.673	ug/l	94
68) m/p-Xylenes	11.945	106	18144	2.252	ug/l	89
69) o-Xylene	12.274	106	12716	1.628	ug/l	92
74) N-amyl acetate	12.351	43	13571	1.540	ug/l	# 43
75) 1,1,2,2-Tetrachloroethane	12.574	83	764	Below Cal		94
76) 1,2,3-Trichloropropane	12.727	75	158608	26.487	ug/l	# 1
78) n-propylbenzene	12.916	91	8671	0.335	ug/l	94
80) 1,3,5-Trimethylbenzene	13.051	105	14596	0.745	ug/l	90
81) trans-1,4-Dichloro-2-b...	12.727	75	158608	68.870	ug/l	# 11
84) 1,2,4-Trimethylbenzene	13.363	105	50855	2.684	ug/l	94
86) p-Isopropyltoluene	13.557	119	4354	0.249	ug/l	94


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
 Data File : VN072369.D
 Acq On : 06 May 2022 21:02
 Operator : JC\MD
 Sample : N2726-01RE
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FLOOR-DRAINING-TOTERE

Quant Time: May 09 03:17:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 26 18:50:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
93) 1,2,4-Trichlorobenzene	15.251	180	271	2.483	ug/l #	10
95) Naphthalene	15.498	128	73314	9.158	ug/l	98
96) 1,2,3-Trichlorobenzene	15.686	180	64	2.688	ug/l #	1





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion:168 Resp: 294909
Ion Ratio Lower Upper
168 100
99 63.8 42.3 63.5#



#5
Bromomethane
Concen: Below Cal
RT: 2.834 min Scan# 144
Delta R.T. -0.000 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 94 Resp: 60
Ion Ratio Lower Upper
94 100
96 0.0 76.0 114.0#




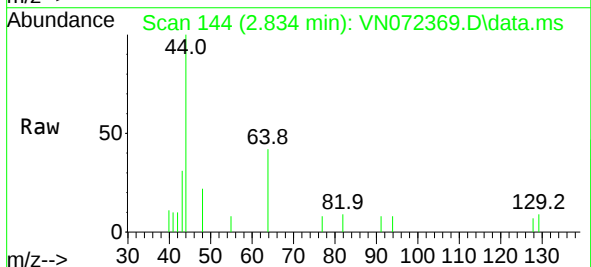




#6
Chloroethane
Concen: Below Cal
RT: 3.010 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion: 64 Resp: 626
Ion Ratio Lower Upper
64 100
66 64.6 26.2 39.4#

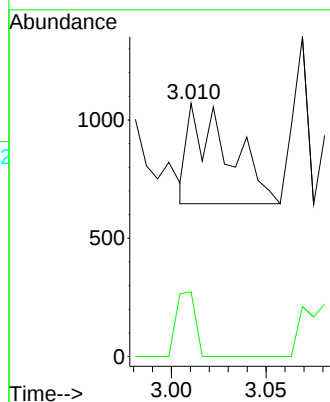

#11
Tert butyl alcohol
Concen: 0.921 ug/l
RT: 5.387 min Scan# 578
Delta R.T. 0.024 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 59 Resp: 685
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

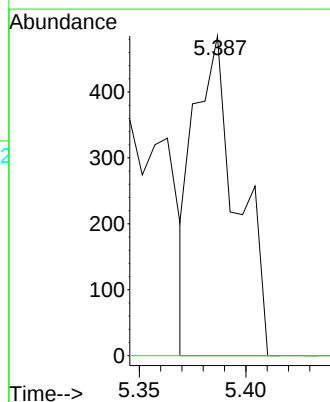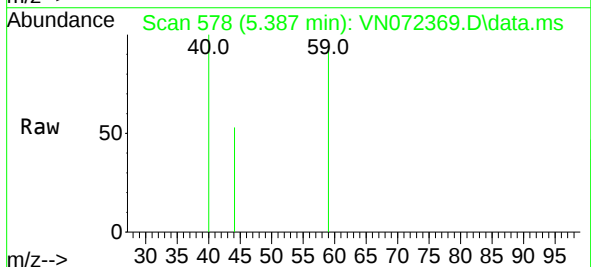



#16

Acetone

Concen: 424.774 ug/l

RT: 4.281 min Scan# 390

Delta R.T. -0.000 min

Lab File: VN072369.D


Acq: 06 May 2022 21:02

Instrument :

MSVOA_N

ClientSampleId :

FLOOR-DRAINING-TOTERE



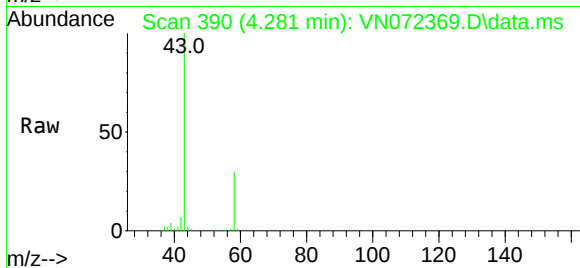


Tgt Ion: 43 Resp: 829155

Ion Ratio Lower Upper

43 100

58 29.8 26.0 39.0



#17

Carbon Disulfide

Concen: 0.630 ug/l

RT: 4.522 min Scan# 431

Delta R.T. -0.012 min

Lab File: VN072369.D




Acq: 06 May 2022 21:02


Tgt Ion: 76 Resp: 1784

Ion Ratio Lower Upper

76 100

78 0.0 7.2 10.8#









#18
Methyl Acetate
Concen: 2.816 ug/l
RT: 4.846 min Scan# 41
Delta R.T. -0.005 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion: 43 Resp: 15573
Ion Ratio Lower Upper
43 100
74 10.7 21.6 32.4#

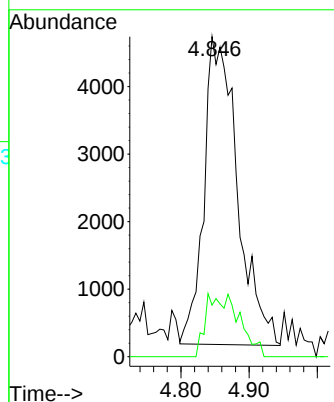

#20
Methylene Chloride
Concen: 2.492 ug/l
RT: 5.093 min Scan# 528
Delta R.T. 0.006 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 84 Resp: 9326
Ion Ratio Lower Upper
84 100
49 129.9 88.3 132.5
51 33.5 28.2 42.2
86 56.4 50.6 76.0



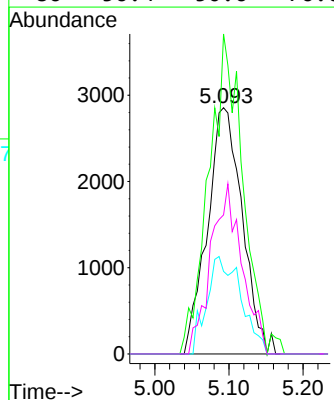





#24
1,1-Dichloroethane
Concen: 0.606 ug/l
RT: 6.387 min Scan# 74
Delta R.T. -0.000 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion: 63 Resp: 4081
Ion Ratio Lower Upper
63 100
98 0.0 3.5 10.4#
100 0.0 2.3 6.8#



#25
2-Butanone
Concen: 14.610 ug/l
RT: 7.340 min Scan# 910
Delta R.T. 0.011 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 43 Resp: 45419
Ion Ratio Lower Upper
43 100
72 28.2 23.7 35.5



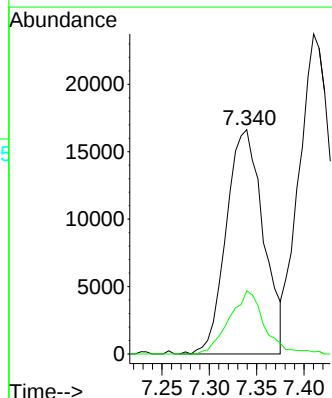





#30
Chloroform
Concen: 0.691 ug/l
RT: 7.834 min Scan# 991
Delta R.T. 0.018 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion: 83 Resp: 4678
Ion Ratio Lower Upper
83 100
85 31.7 51.8 77.8#



#31
Cyclohexane
Concen: 1.106 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.011 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 56 Resp: 6688
Ion Ratio Lower Upper
56 100
69 200.8 27.8 41.8#
84 136.8 76.9 115.3#

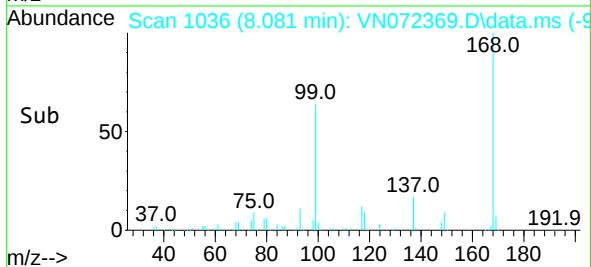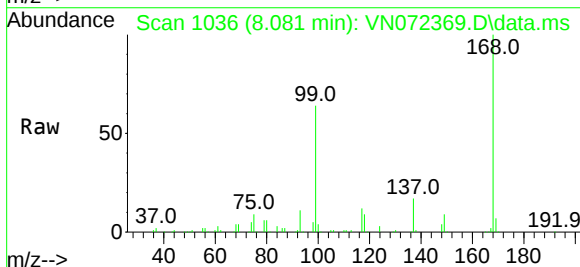



#32

1,1,1-Trichloroethane

Concen: 0.388 ug/l

RT: 8.004 min Scan# 1023

Delta R.T. -0.006 min

Lab File: VN072369.D


Acq: 06 May 2022 21:02

Instrument :

MSVOA_N

ClientSampleId :

FLOOR-DRAINING-TOTERE

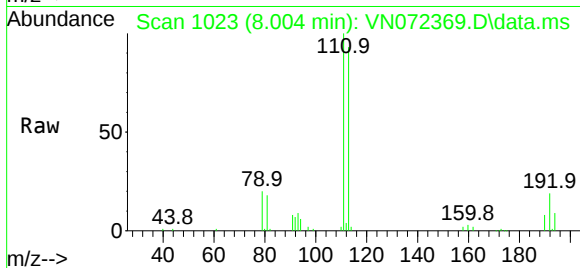




Tgt Ion: 97 Resp: 2231

Ion Ratio Lower Upper

97 100

99 0.0 50.6 76.0#

61 32.1 36.0 54.0#

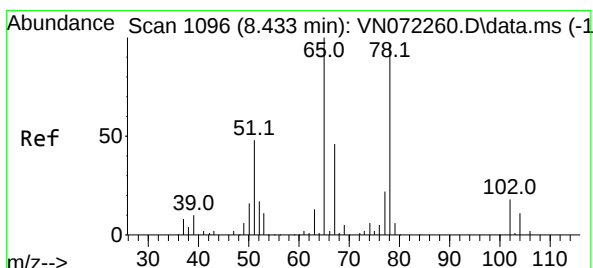

#33

1,2-Dichloroethane-d4

Concen: 48.200 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.000 min

Lab File: VN072369.D




Acq: 06 May 2022 21:02


Tgt Ion: 65 Resp: 218224

Ion Ratio Lower Upper

65 100

67 50.6 0.0 104.8

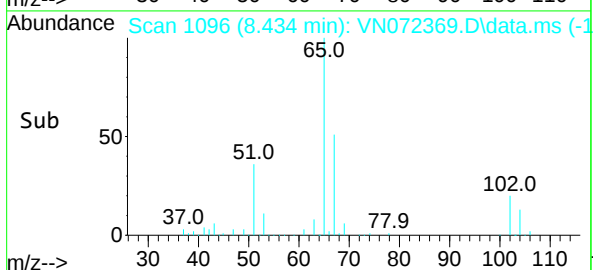



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072369.D

Acq: 06 May 2022 21:02

Instrument :

MSVOA_N

ClientSampleId :

FLOOR-DRAINING-TOTERE





Tgt Ion:114 Resp: 567499

Ion Ratio Lower Upper

114 100

63 21.4 0.0 40.0

88 16.0 0.0 32.6

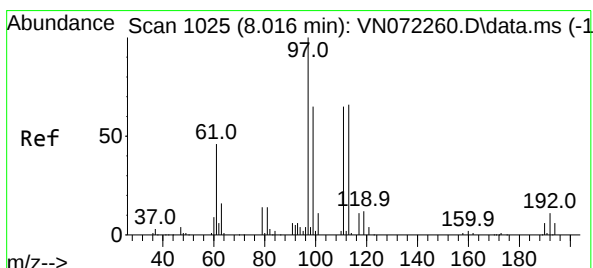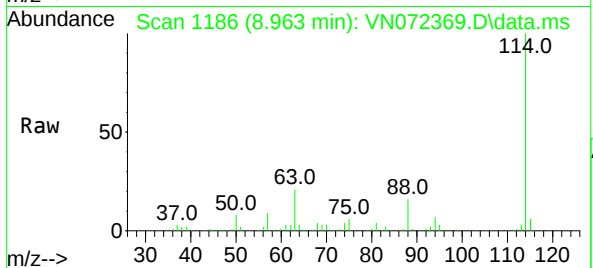

#35

Dibromofluoromethane

Concen: 46.299 ug/l

RT: 8.016 min Scan# 1025

Delta R.T. -0.000 min

Lab File: VN072369.D

Acq: 06 May 2022 21:02




Tgt Ion:113 Resp: 168172


Ion Ratio Lower Upper

113 100

111 102.8 81.4 122.0

192 18.2 17.0 25.6

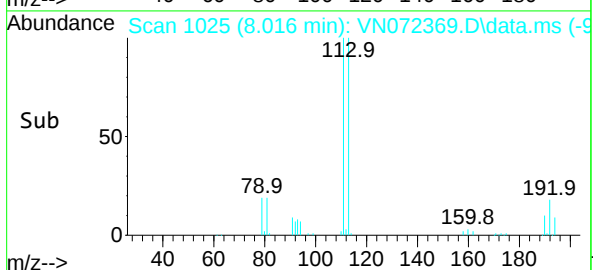



#36

1,1-Dichloropropene

Concen: 4.720 ug/l

RT: 8.081 min Scan# 1

Delta R.T. -0.135 min

Lab File: VN072369.D


Acq: 06 May 2022 21:02

Instrument :

MSVOA_N

ClientSampleId :

FLOOR-DRAINING-TOTERE

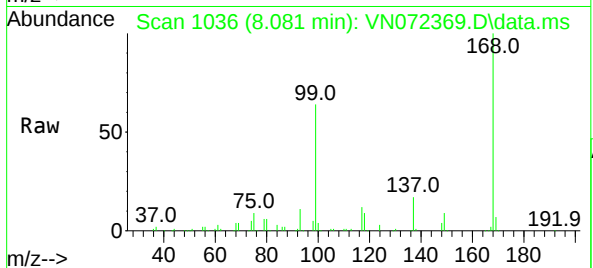




Tgt Ion: 75 Resp: 24953

Ion Ratio Lower Upper

75 100

110 10.3 18.3 54.8#

77 0.0 25.1 37.7#

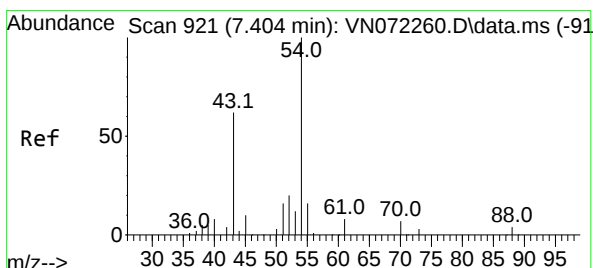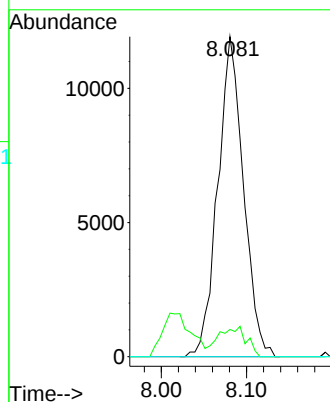

#37

Ethyl Acetate

Concen: 8.333 ug/l

RT: 7.410 min Scan# 922

Delta R.T. 0.000 min

Lab File: VN072369.D

Acq: 06 May 2022 21:02




Tgt Ion: 43 Resp: 58510


Ion Ratio Lower Upper

43 100

61 13.9 11.8 17.6

70 10.2 9.3 13.9

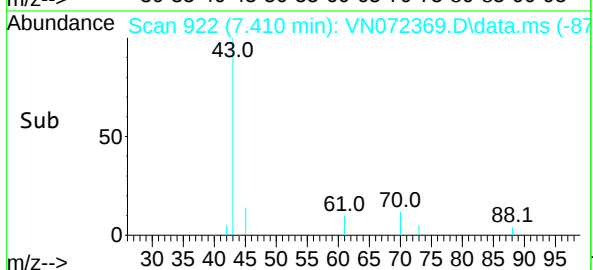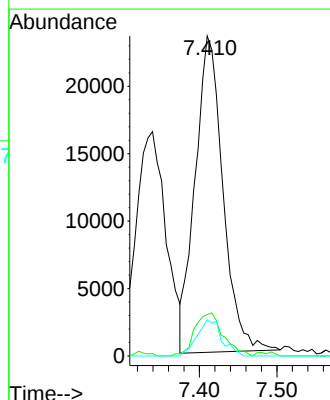



#38

Carbon Tetrachloride

Concen: 5.588 ug/l

RT: 8.081 min Scan# 1100

Delta R.T. -0.123 min

Lab File: VN072369.D


Acq: 06 May 2022 21:02

Instrument :

MSVOA_N

ClientSampleId :

FLOOR-DRAINING-TOTERE

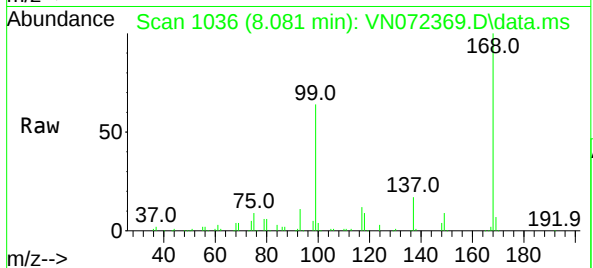




Tgt Ion:117 Resp: 31642

Ion Ratio Lower Upper

117 100

119 3.8 75.8 113.8#

121 0.0 24.6 37.0#

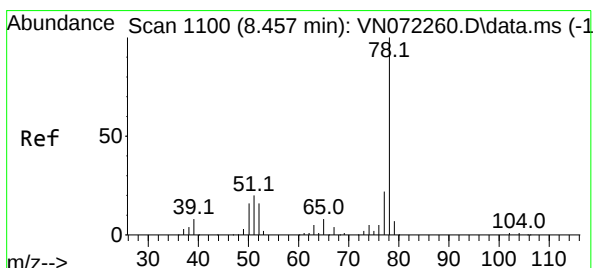

#40

Benzene

Concen: 0.437 ug/l

RT: 8.457 min Scan# 1100

Delta R.T. 0.000 min

Lab File: VN072369.D




Acq: 06 May 2022 21:02


Tgt Ion: 78 Resp: 7171

Ion Ratio Lower Upper

78 100

77 15.2 19.4 29.0#


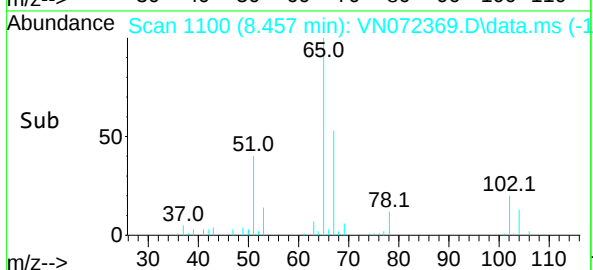






#41
Methacrylonitrile
Concen: 0.239 ug/l
RT: 7.645 min Scan# 91
Delta R.T. 0.011 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion: 41 Resp: 849
Ion Ratio Lower Upper
41 100
39 6.6 48.6 73.0#
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#



#42
1,2-Dichloroethane
Concen: 0.234 ug/l
RT: 8.528 min Scan# 1112
Delta R.T. -0.000 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 62 Resp: 1470
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.4




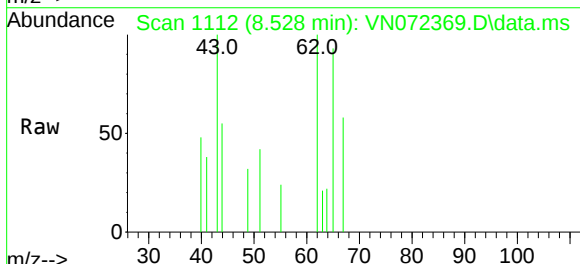




#43
Isopropyl Acetate
Concen: 4.063 ug/l
RT: 8.410 min Scan# 1092
Delta R.T. -0.147 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument : MSVOA_N
ClientSampleId : FLOOR-DRAINING-TOTERE


Tgt Ion: 43 Resp: 36548
Ion Ratio Lower Upper
43 100
61 0.0 21.9 32.9#
87 0.0 12.0 18.0#

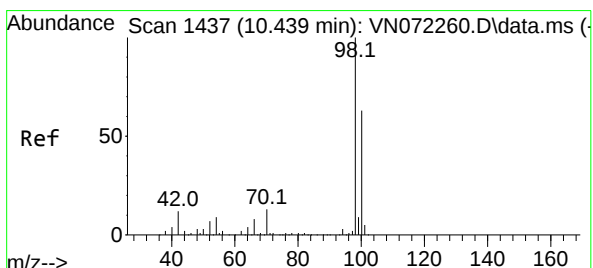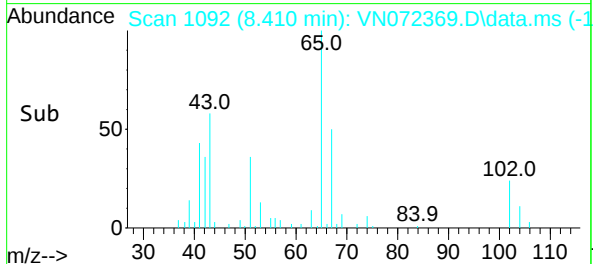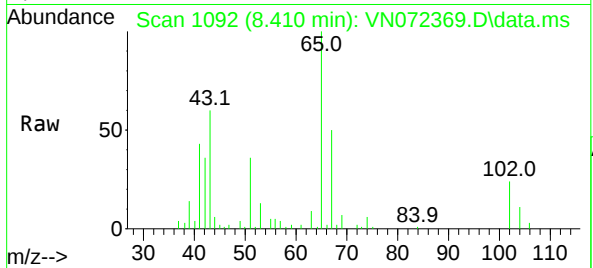

#50
Toluene-d8
Concen: 51.278 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 98 Resp: 731877
Ion Ratio Lower Upper
98 100
100 64.9 52.6 78.8


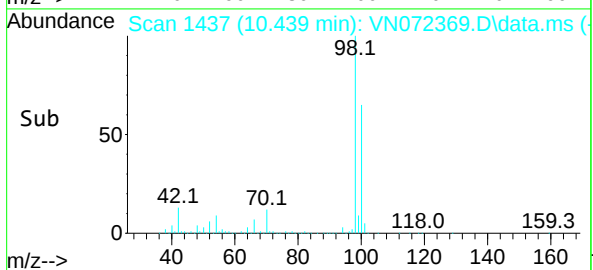

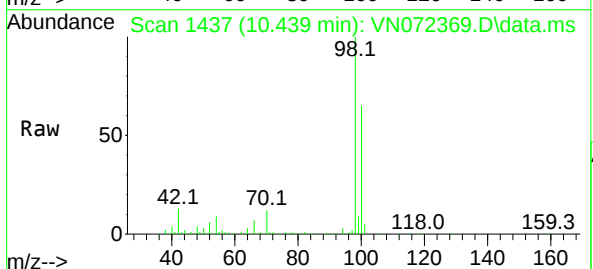




#51
4-Methyl-2-Pentanone
Concen: 7.740 ug/l
RT: 10.328 min Scan# 1418
Delta R.T. -0.000 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion: 43 Resp: 51277
Ion Ratio Lower Upper
43 100
58 38.6 34.1 51.1



#52
Toluene
Concen: 1.986 ug/l
RT: 10.498 min Scan# 1447
Delta R.T. -0.006 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 92 Resp: 19472
Ion Ratio Lower Upper
92 100
91 181.7 138.6 207.8


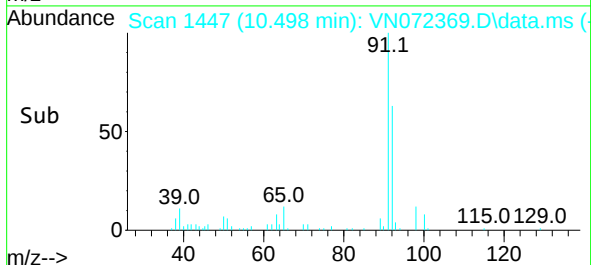

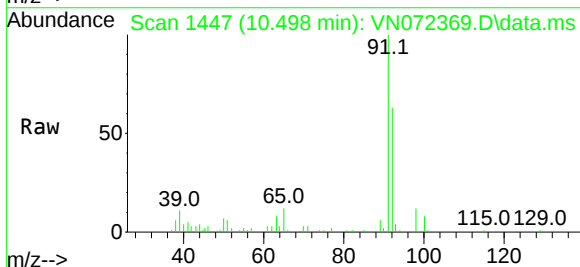




#56
Ethyl methacrylate
Concen: 2.451 ug/l
RT: 10.763 min Scan# 1491
Delta R.T. 0.006 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion: 69 Resp: 646
Ion Ratio Lower Upper
69 100
41 0.0 47.8 71.6#
39 21.5 27.3 40.9#



#58
2-Chloroethyl Vinyl ether
Concen: 17.768 ug/l
RT: 9.910 min Scan# 1347
Delta R.T. -0.129 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 63 Resp: 72
Ion Ratio Lower Upper
63 100
106 0.0 24.6 36.8#


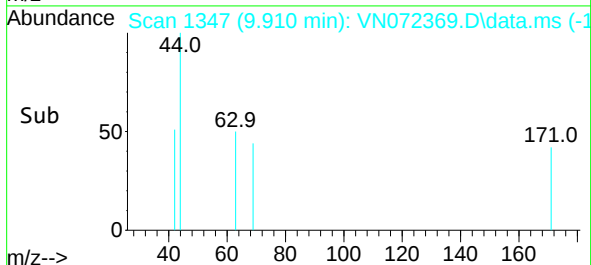

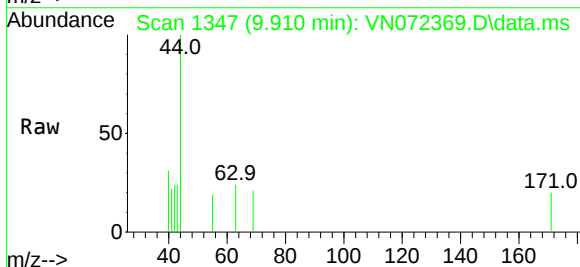




#59
2-Hexanone
Concen: 0.530 ug/l
RT: 11.086 min Scan# 11
Delta R.T. 0.005 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion: 43 Resp: 2472
Ion Ratio Lower Upper
43 100
58 49.5 29.7 89.1



#62
4-Bromofluorobenzene
Concen: 63.374 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 95 Resp: 300229
Ion Ratio Lower Upper
95 100
174 75.1 0.0 167.6
176 71.5 0.0 163.4

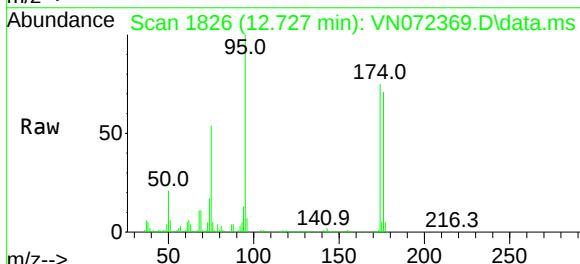



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.739 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN072369.D


Acq: 06 May 2022 21:02

Instrument :

MSVOA_N

ClientSampleId :

FLOOR-DRAINING-TOTERE

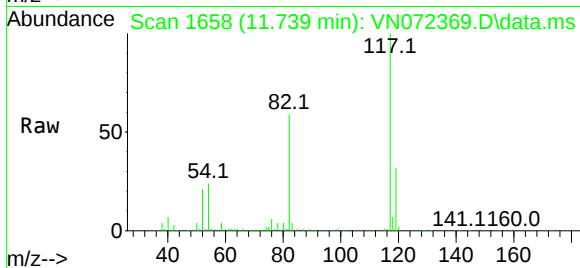




Tgt Ion:117 Resp: 615694

Ion Ratio Lower Upper

117 100

82 59.2 44.2 66.2

119 31.7 25.4 38.0



#67

Ethyl Benzene

Concen: 0.673 ug/l

RT: 11.839 min Scan# 1675

Delta R.T. 0.000 min

Lab File: VN072369.D




Acq: 06 May 2022 21:02


Tgt Ion: 91 Resp: 14605

Ion Ratio Lower Upper

91 100

106 34.2 24.9 37.3


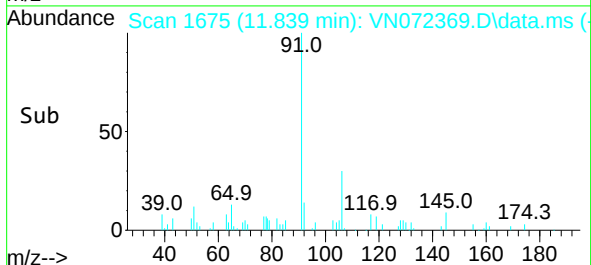
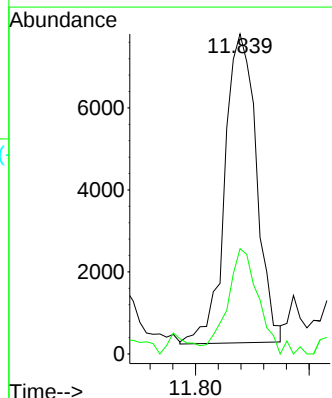
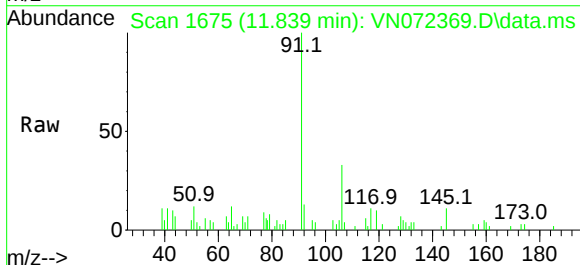




#68
m/p-Xylenes
Concen: 2.252 ug/l
RT: 11.945 min Scan# 1693
Delta R.T. -0.006 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion:106 Resp: 18144
Ion Ratio Lower Upper
106 100
91 214.9 158.9 238.3

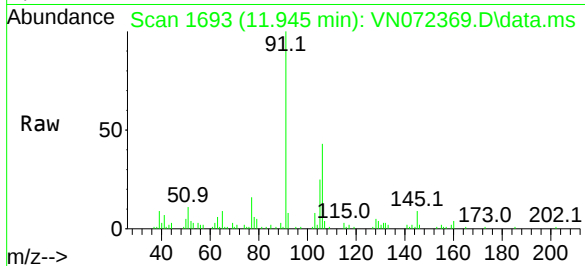

#69
o-Xylene
Concen: 1.628 ug/l
RT: 12.274 min Scan# 1749
Delta R.T. -0.001 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion:106 Resp: 12716
Ion Ratio Lower Upper
106 100
91 224.7 106.0 318.0

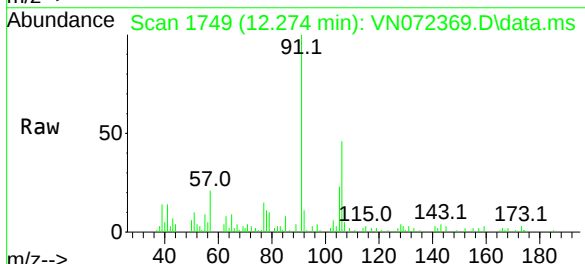

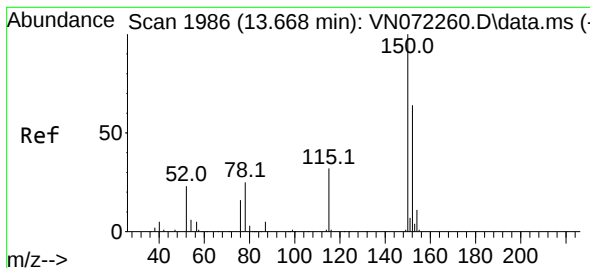

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.669 min Scan# 1986

Delta R.T. -0.001 min

Lab File: VN072369.D


Acq: 06 May 2022 21:02

Instrument :

MSVOA_N

ClientSampleId :

FLOOR-DRAINING-TOTERE

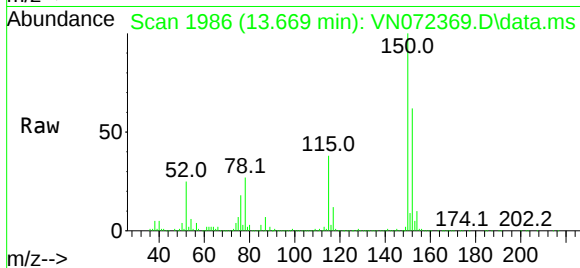




Tgt Ion:152 Resp: 266287

Ion Ratio Lower Upper

152 100

115 62.9 28.9 86.7

150 157.4 0.0 356.2

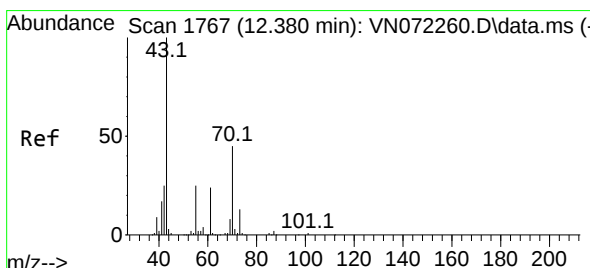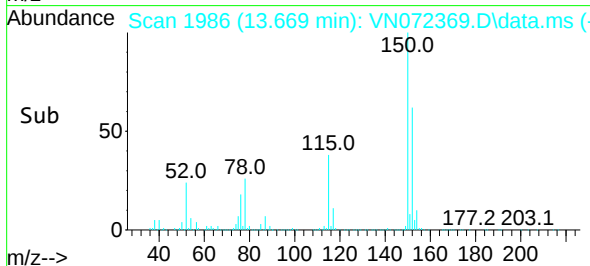

#74

N-ethyl acetate

Concen: 1.540 ug/l

RT: 12.351 min Scan# 1762

Delta R.T. -0.029 min

Lab File: VN072369.D

Acq: 06 May 2022 21:02

Tgt Ion: 43 Resp: 13571




Ion Ratio Lower Upper


43 100

70 5.4 39.0 58.4#

55 0.0 21.1 31.7#

61 0.0 21.1 31.7#


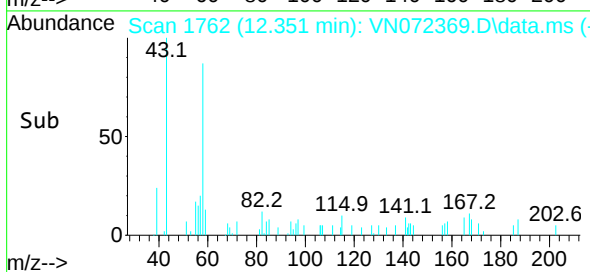

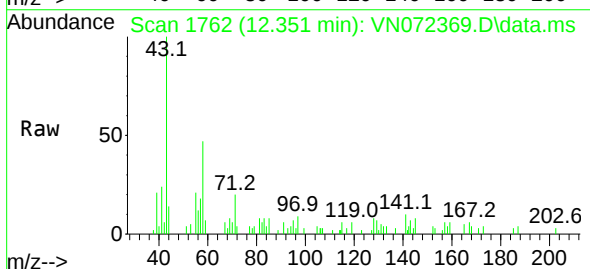




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.574 min Scan# 1800
Delta R.T. -0.248 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion: 83 Resp: 764
Ion Ratio Lower Upper
83 100
131 6.9 5.3 15.9
85 69.0 32.3 96.9



#76
1,2,3-Trichloropropane
Concen: 26.487 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 75 Resp: 158608
Ion Ratio Lower Upper
75 100
77 1.3 98.5 295.5#

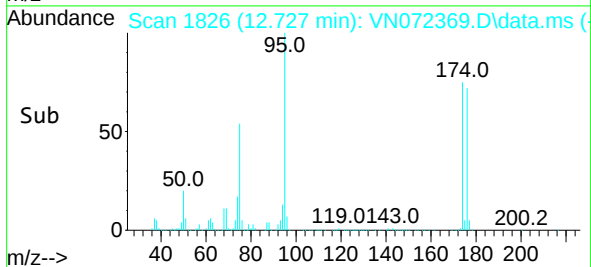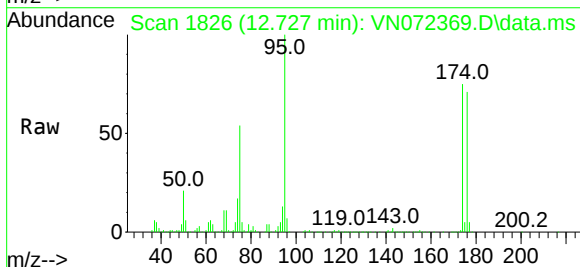



#78

n-propylbenzene

Concen: 0.335 ug/l

RT: 12.916 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN072369.D

Acq: 06 May 2022 21:02

Instrument :

MSVOA_N

ClientSampleId :





FLOOR-DRAINING-TOTERE

Tgt Ion: 91 Resp: 8671

Ion Ratio Lower Upper

91 100

120 20.9 11.9 35.5

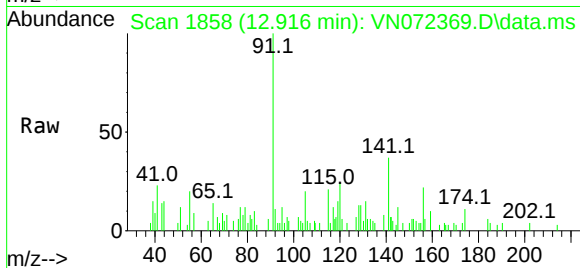

#80

1,3,5-Trimethylbenzene

Concen: 0.745 ug/l

RT: 13.051 min Scan# 1881

Delta R.T. -0.000 min

Lab File: VN072369.D




Acq: 06 May 2022 21:02


Tgt Ion: 105 Resp: 14596

Ion Ratio Lower Upper

105 100

120 43.0 24.9 74.7









#81
trans-1,4-Dichloro-2-butene
Concen: 68.870 ug/l
RT: 12.727 min Scan# 1808
Delta R.T. 0.105 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion: 75 Resp: 158608
Ion Ratio Lower Upper
75 100
53 0.3 78.0 117.0#
89 0.1 37.2 55.8#



#84
1,2,4-Trimethylbenzene
Concen: 2.684 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion: 105 Resp: 50855
Ion Ratio Lower Upper
105 100
120 42.8 23.3 69.8




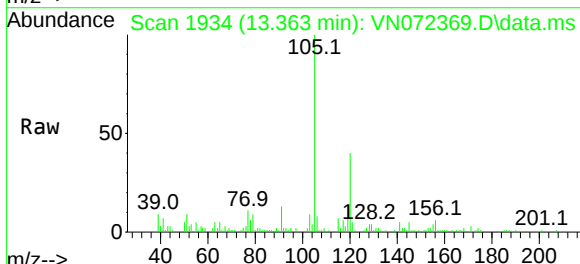




#86
p-Isopropyltoluene
Concen: 0.249 ug/l
RT: 13.557 min Scan# 1976
Delta R.T. -0.053 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02




Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE


Tgt Ion:119 Resp: 4354
Ion Ratio Lower Upper
119 100
134 26.1 13.3 39.8
91 17.2 11.3 33.9



#93
1,2,4-Trichlorobenzene
Concen: 2.483 ug/l
RT: 15.251 min Scan# 2255
Delta R.T. -0.006 min
Lab File: VN072369.D
Acq: 06 May 2022 21:02

Tgt Ion:180 Resp: 271
Ion Ratio Lower Upper
180 100
182 193.4 47.5 142.5#
145 0.0 14.5 43.5#

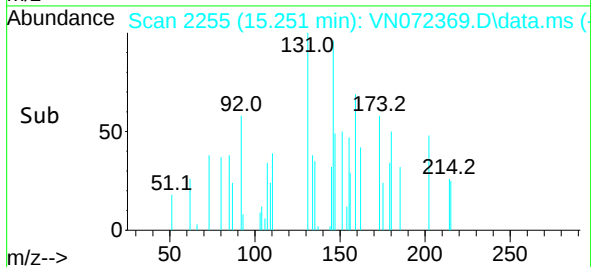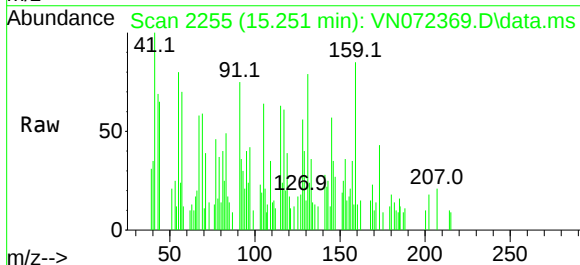



#95

Naphthalene

Concen: 9.158 ug/l

RT: 15.498 min Scan# 21

Delta R.T. -0.000 min

Lab File: VN072369.D

Acq: 06 May 2022 21:02

Instrument :

MSVOA_N

ClientSampleId :

FLOOR-DRAINING-TOTERE





Tgt Ion:128 Resp: 73314

Ion Ratio Lower Upper

128 100

127 14.0 10.3 15.5

129 11.5 8.6 13.0

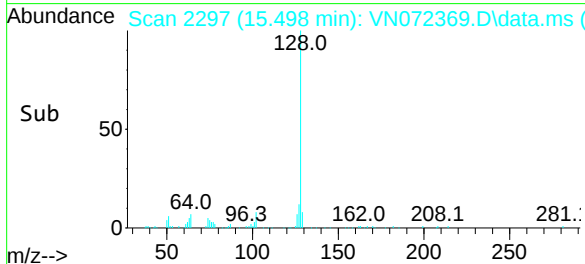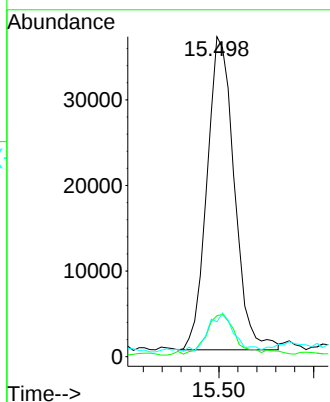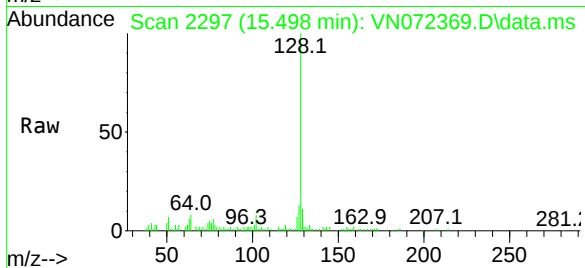

#96

1,2,3-Trichlorobenzene

Concen: 2.688 ug/l

RT: 15.686 min Scan# 2329

Delta R.T. -0.006 min

Lab File: VN072369.D

Acq: 06 May 2022 21:02

Tgt Ion:180 Resp: 64

Ion Ratio Lower Upper

180 100

182 300.0 47.8 143.3#

145 1673.4 15.5 46.5#

