

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
 Data File : VN072369.D
 Acq On : 06 May 2022 21:02
 Operator : JC\MD
 Sample : N2726-01RE
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FLOOR-DRAINING-TOTERE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
 Title : SW846 8260

Signal : TIC: VN072369.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.234	36	42	48	rBV3	40061	97930	1.68%	0.408%
2	2.581	94	101	120	rBV	1704636	2997649	51.35%	12.482%
3	3.693	276	290	320	rBV	2195423	5837683	100.00%	24.308%
4	4.281	380	390	413	rBV	421850	1261093	21.60%	5.251%
5	4.575	430	440	455	rBV2	42813	142970	2.45%	0.595%
6	7.063	855	863	873	rBV4	20713	60838	1.04%	0.253%
7	7.340	897	910	916	rBV	27166	75479	1.29%	0.314%
8	7.410	916	922	932	rVB	36740	91004	1.56%	0.379%
9	8.016	1014	1025	1030	rBV	229881	539231	9.24%	2.245%
10	8.081	1030	1036	1048	rVB	408569	922438	15.80%	3.841%
11	8.434	1083	1096	1108	rBV2	278208	721506	12.36%	3.004%
12	8.963	1177	1186	1198	rBV	670703	1351690	23.15%	5.628%
13	9.151	1211	1218	1235	rBV2	98401	263836	4.52%	1.099%
14	10.328	1411	1418	1426	rBV2	69875	135116	2.31%	0.563%
15	10.439	1428	1437	1444	rVV	1064644	1979758	33.91%	8.244%
16	10.504	1444	1448	1453	rVB	46289	82744	1.42%	0.345%
17	11.739	1651	1658	1670	rBV	1079089	1899827	32.54%	7.911%
18	11.945	1688	1693	1702	rVB	59982	118144	2.02%	0.492%
19	12.133	1714	1725	1736	rBV2	157979	357226	6.12%	1.487%
20	12.274	1743	1749	1758	rBV2	53157	102782	1.76%	0.428%
21	12.727	1820	1826	1836	rVB	843906	1433480	24.56%	5.969%
22	12.974	1864	1868	1872	rBV	39685	67264	1.15%	0.280%
23	13.051	1877	1881	1889	rVB4	30554	58766	1.01%	0.245%
24	13.363	1929	1934	1941	rVB	84006	146108	2.50%	0.608%
25	13.669	1979	1986	1997	rBV	1026702	1834009	31.42%	7.637%
26	13.763	1997	2002	2012	rBV	309367	549964	9.42%	2.290%
27	14.133	2061	2065	2074	rBV9	35314	78670	1.35%	0.328%
28	14.804	2175	2179	2183	rBV	38835	73841	1.26%	0.307%
29	14.927	2193	2200	2204	rBV3	87730	184717	3.16%	0.769%
30	14.974	2205	2208	2214	rVB2	46231	78347	1.34%	0.326%
31	15.080	2222	2226	2234	rVB2	46616	85434	1.46%	0.356%
32	15.504	2293	2298	2303	rVV	69449	130740	2.24%	0.544%
33	15.692	2327	2330	2340	rVB4	37496	76446	1.31%	0.318%
34	16.010	2381	2384	2392	rVB8	32406	65768	1.13%	0.274%
35	16.615	2480	2487	2492	rBV	52362	113361	1.94%	0.472%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
Data File : VN072369.D
Acq On : 06 May 2022 21:02
Operator : JC\MD
Sample : N2726-01RE
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Title : SW846 8260




Sum of corrected areas: 24015859

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
Data File : VN072369.D
Acq On : 06 May 2022 21:02
Operator : JC\MD
Sample : N2726-01RE
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

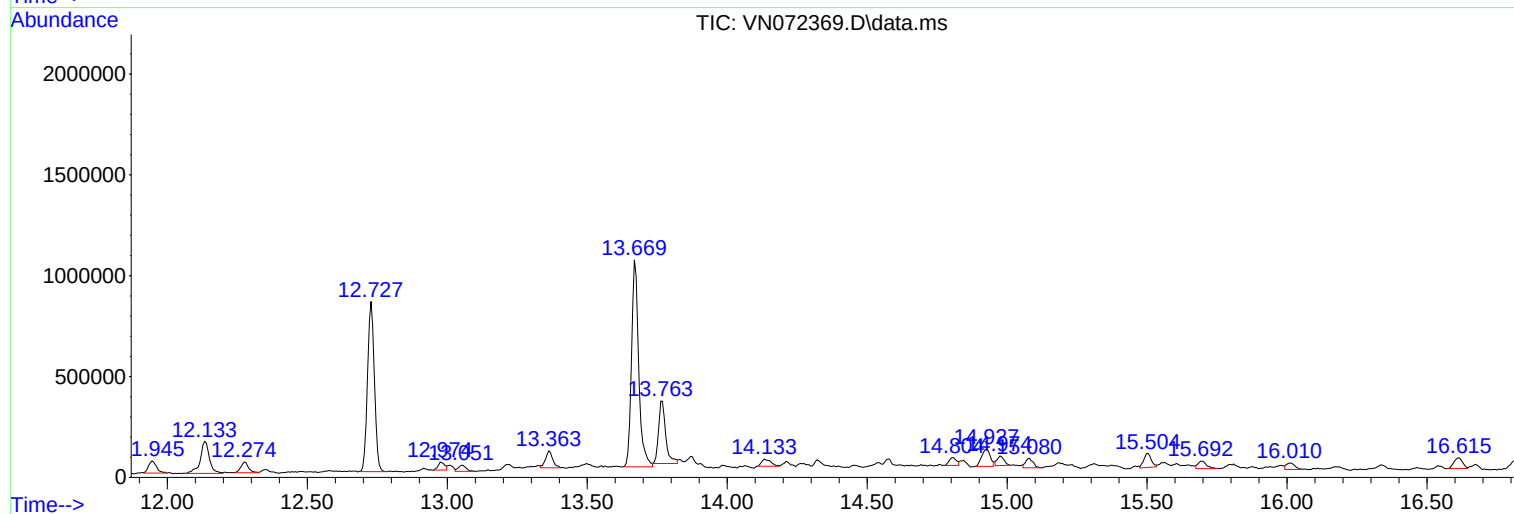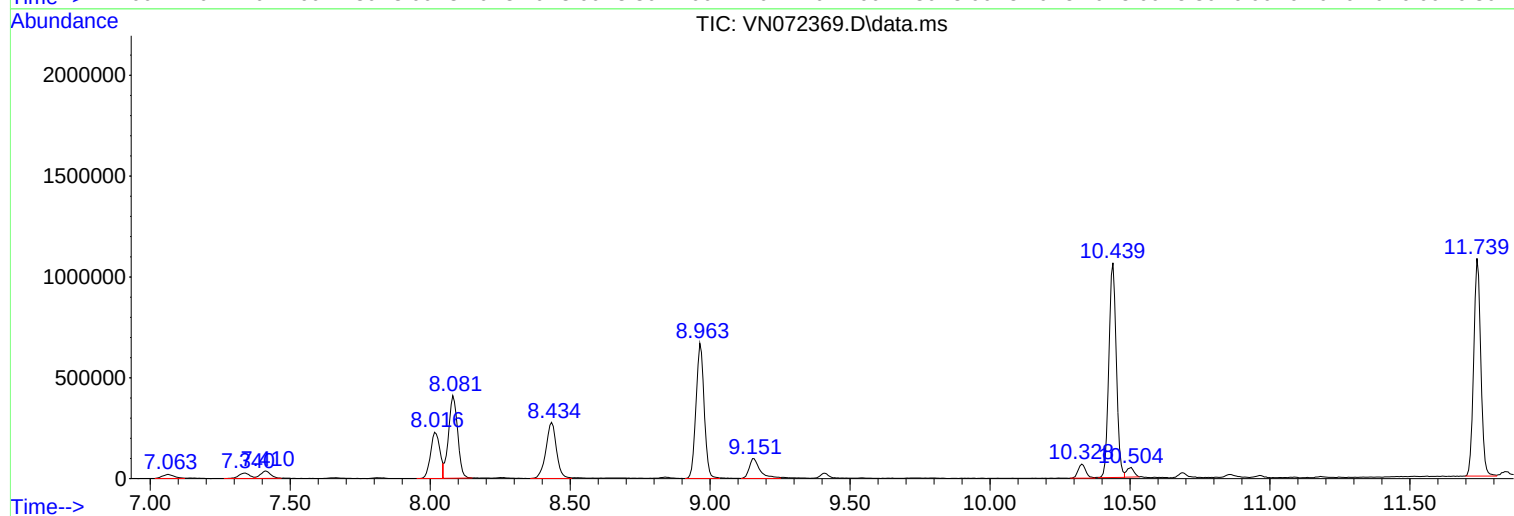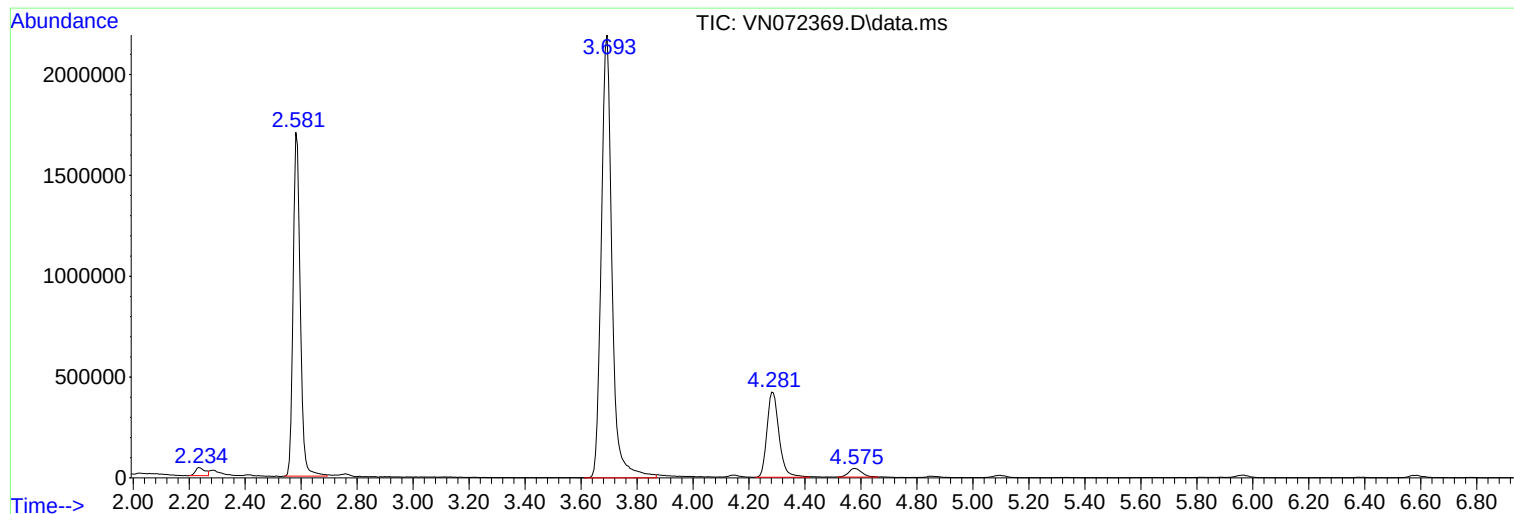

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
Data File : VN072369.D
Acq On : 06 May 2022 21:02
Operator : JC\MD
Sample : N2726-01RE
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050622\
Data File : VN072369.D
Acq On : 06 May 2022 21:02
Operator : JC\MD
Sample : N2726-01RE
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FLOOR-DRAINING-TOTERE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc