


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050625\
Data File : VN086503.D
Acq On : 06 May 2025 09:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

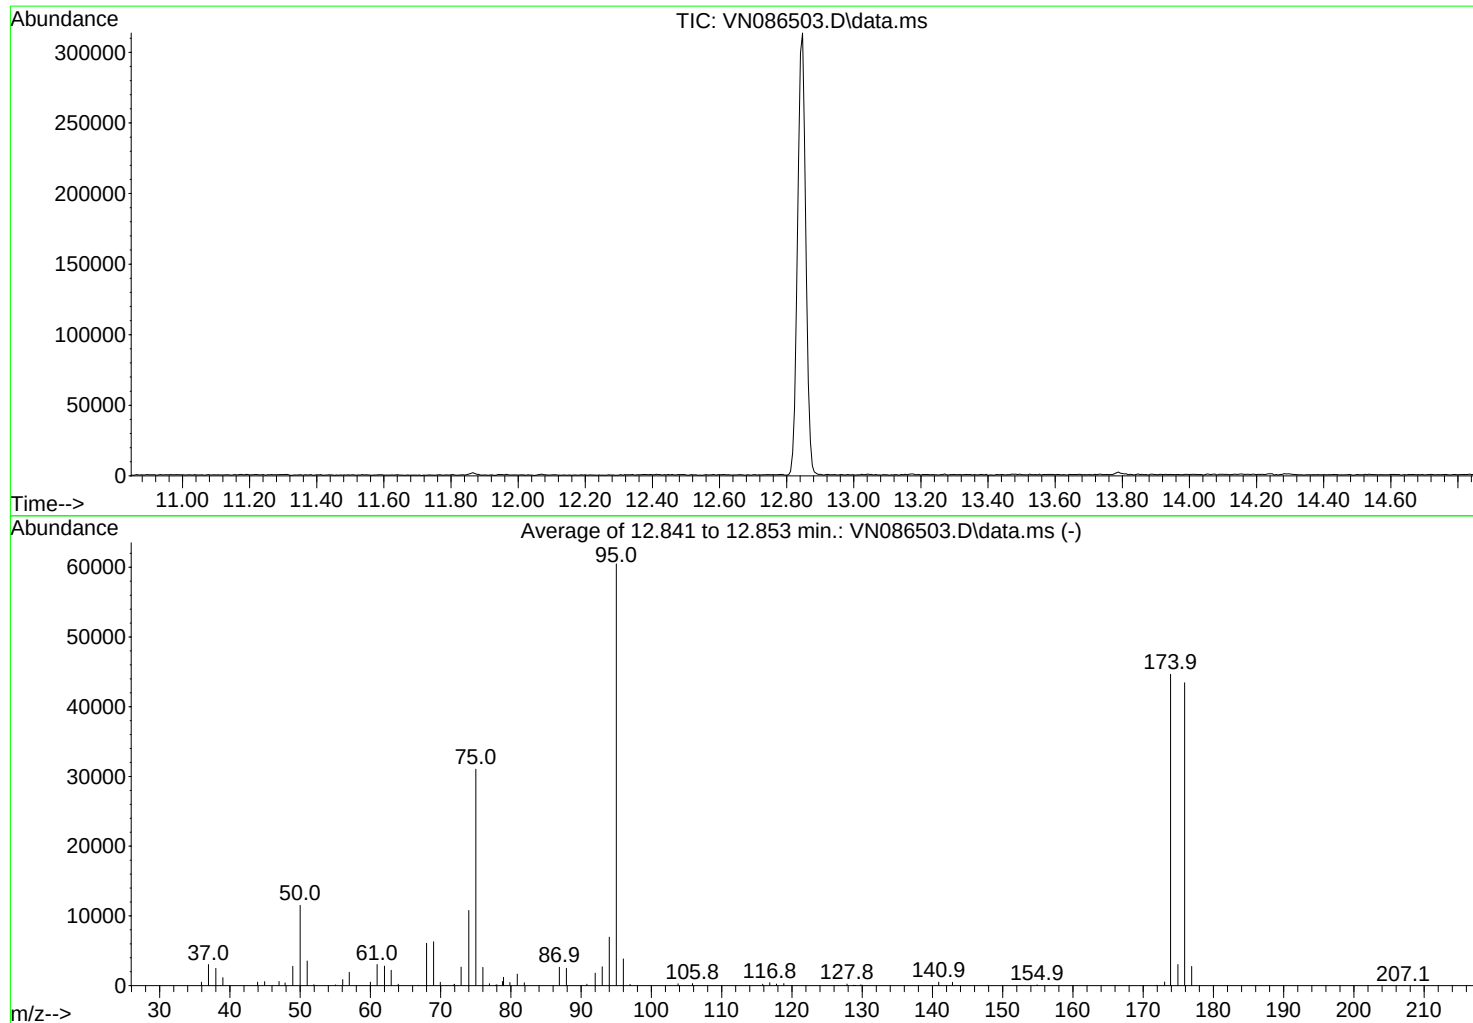

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	11520	PASS
75	95	30	60	51.3	31056	PASS
95	95	100	100	100.0	60491	PASS
96	95	5	9	6.3	3832	PASS
173	174	0.00	2	1.2	539	PASS
174	95	50	100	73.8	44659	PASS
175	174	5	9	6.8	3021	PASS
176	174	95	101	97.3	43437	PASS
177	176	5	9	6.3	2756	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	507	51.95	135	69.00	6299	78.80	591
36.95	3031	55.00	127	69.95	481	78.95	1191
38.00	2483	56.05	885	71.80	101	79.85	46
39.00	1154	57.00	1899	71.95	215	80.90	166
43.95	496	60.00	516	72.90	2665	81.90	414
44.95	564	60.95	3027	74.00	10779	86.90	2649
47.00	597	62.00	2808	75.00	31056	87.90	2490
47.85	403	62.95	2206	76.00	2621	90.80	207
48.95	2772	63.95	205	76.95	272	92.00	1786
50.00	11520	66.80	51	77.80	63	93.00	2708
51.00	3534	68.00	6084	78.00	136	94.00	6954

Average of 12.841 to 12.853 min.: VN086503.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	60491	129.00	53	175.90	43437		
96.00	3832	129.80	124	176.90	2756		
96.95	181	130.00	76	207.05	20		
103.80	273	140.90	498				
105.85	290	142.85	477				
115.85	197	147.80	56				
116.85	419	154.90	118				
117.80	227	171.90	50				
118.85	291	173.05	539				
127.85	222	173.90	44659				
128.80	66	174.95	3021				

Instrument :

MSVOA_N

ClientSampleId :

BFB