


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN050719\
Data File : VN055449.D
Acq On : 7 May 2019 20:32
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042919W.M
Title : SW846 8260
Last Update : Tue Apr 30 07:16:52 2019

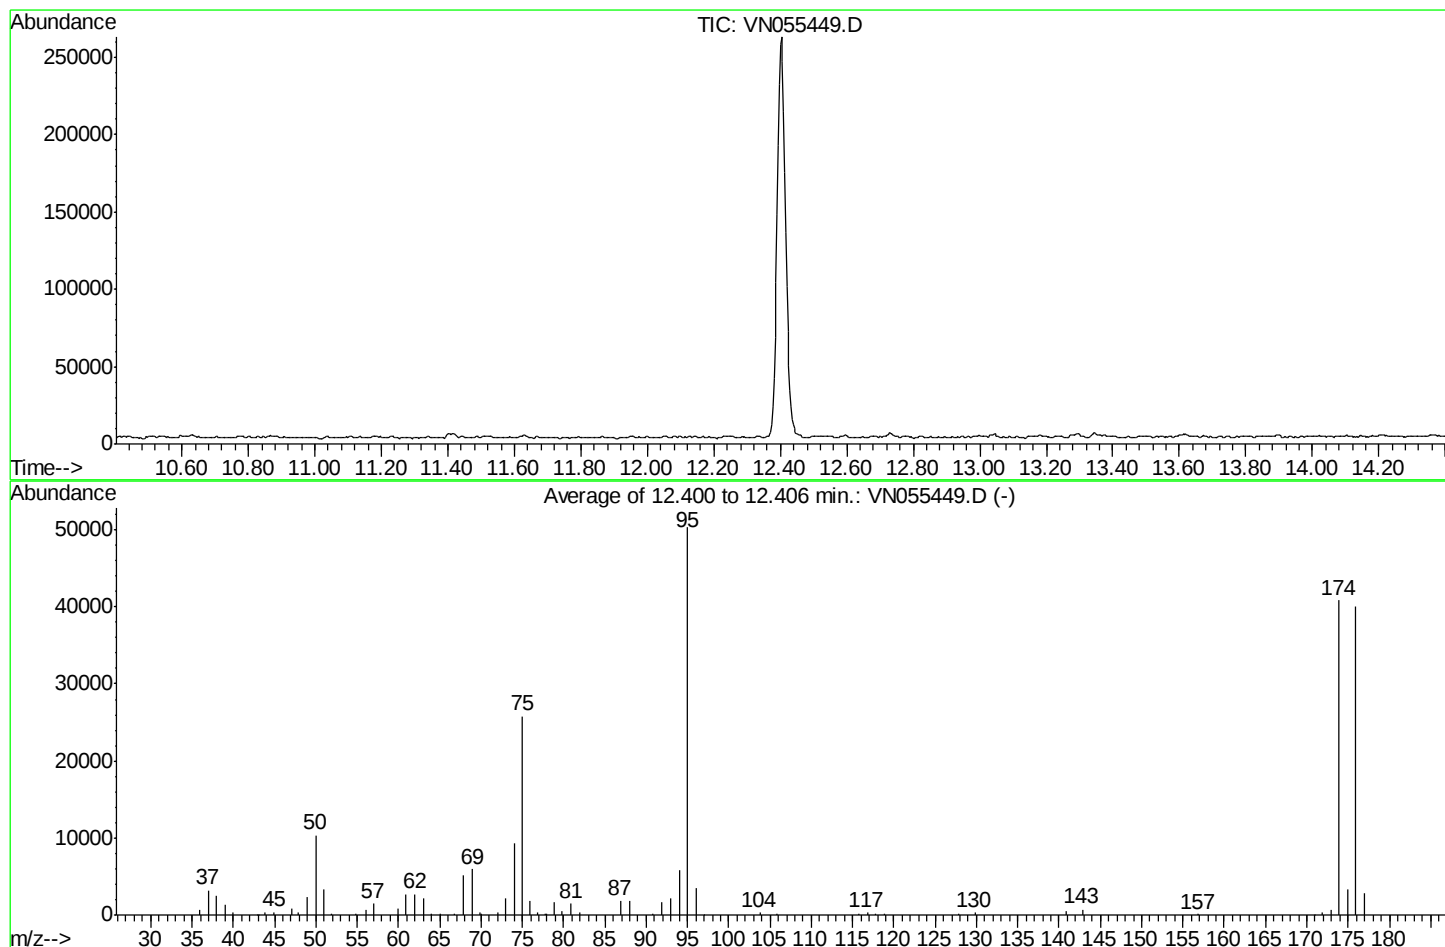

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	10352	PASS
75	95	30	60	51.3	25832	PASS
95	95	100	100	100.0	50328	PASS
96	95	5	9	7.1	3551	PASS
173	174	0.00	2	1.5	616	PASS
174	95	50	100	81.2	40869	PASS
175	174	5	9	8.0	3273	PASS
176	174	95	101	98.0	40058	PASS
177	176	5	9	7.1	2859	PASS