

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN050720\
 Data File : VN061326.D
 Acq On : 7 May 2020 12:15
 Operator : JC/MD
 Sample : PB128697TB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: May 08 01:27:30 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 05 07:01:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.62	168	89417	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	161766	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	158495	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	64468	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	7.98	65	74396	52.58	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.16%	
35) Dibromofluoromethane	7.54	113	44771	46.80	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.60%	
50) Toluene-d8	10.06	98	204873	52.54	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.08%	
62) 4-Bromofluorobenzene	12.38	95	74526	50.79	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.58%	

Target Compounds


						Qvalue
16) Acetone	3.77	43	7554	8.467	ug/l	96
18) Methyl Acetate	4.28	43	1267	1.379	ug/l #	55
20) Methylene Chloride	4.50	84	1384	1.254	ug/l #	91
25) 2-Butanone	6.78	43	1856	2.217	ug/l #	53
31) Cyclohexane	7.63	56	2553	1.240	ug/l #	15
36) 1,1-Dichloropropene	7.62	75	8280	5.113	ug/l #	49
37) Ethyl Acetate	6.78	43	1856	0.978	ug/l #	71
38) Carbon Tetrachloride	7.62	117	9549	8.454	ug/l #	18
43) Isopropyl Acetate	8.12	43	37861	12.017	ug/l #	90
45) 1,2-Dichloropropane	9.24	63	671	0.521	ug/l #	44
48) Methyl methacrylate	9.14	41	2022	1.422	ug/l #	16
51) 4-Methyl-2-Pentanone	9.95	43	3708	1.999	ug/l	95
54) cis-1,3-Dichloropropene	9.87	75	14124	6.922	ug/l #	65
56) Ethyl methacrylate	10.51	69	503	2.962	ug/l #	1
57) 1,3-Dichloropropane	10.73	76	2578	1.265	ug/l #	43
59) 2-Hexanone	10.73	43	43327	32.113	ug/l #	52
71) Bromoform	12.38	173	190	0.230	ug/l #	1
74) N-amyl acetate	12.00	43	1483	0.618	ug/l #	46
76) 1,2,3-Trichloropropane	12.38	75	42038	30.929	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.71	105	2890	0.737	ug/l	95
81) trans-1,4-Dichloro-2-buten	12.38	75	42038	78.545	ug/l #	8
88) 1,4-Dichlorobenzene	13.34	146	502	0.244	ug/l #	25
93) 1,2,4-Trichlorobenzene	14.88	180	485	0.412	ug/l #	75
94) Hexachlorobutadiene	14.98	225	239	0.486	ug/l #	18
95) Naphthalene	15.11	128	2066	0.539	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.29	180	426	0.367	ug/l #	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN050720\
Data File : VN061326.D
Acq On : 7 May 2020 12:15
Operator : JC/MD
Sample : PB128697TB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: May 08 01:27:30 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
Quant Title : SW846 8260
QLast Update : Tue May 05 07:01:08 2020
Response via : Initial Calibration

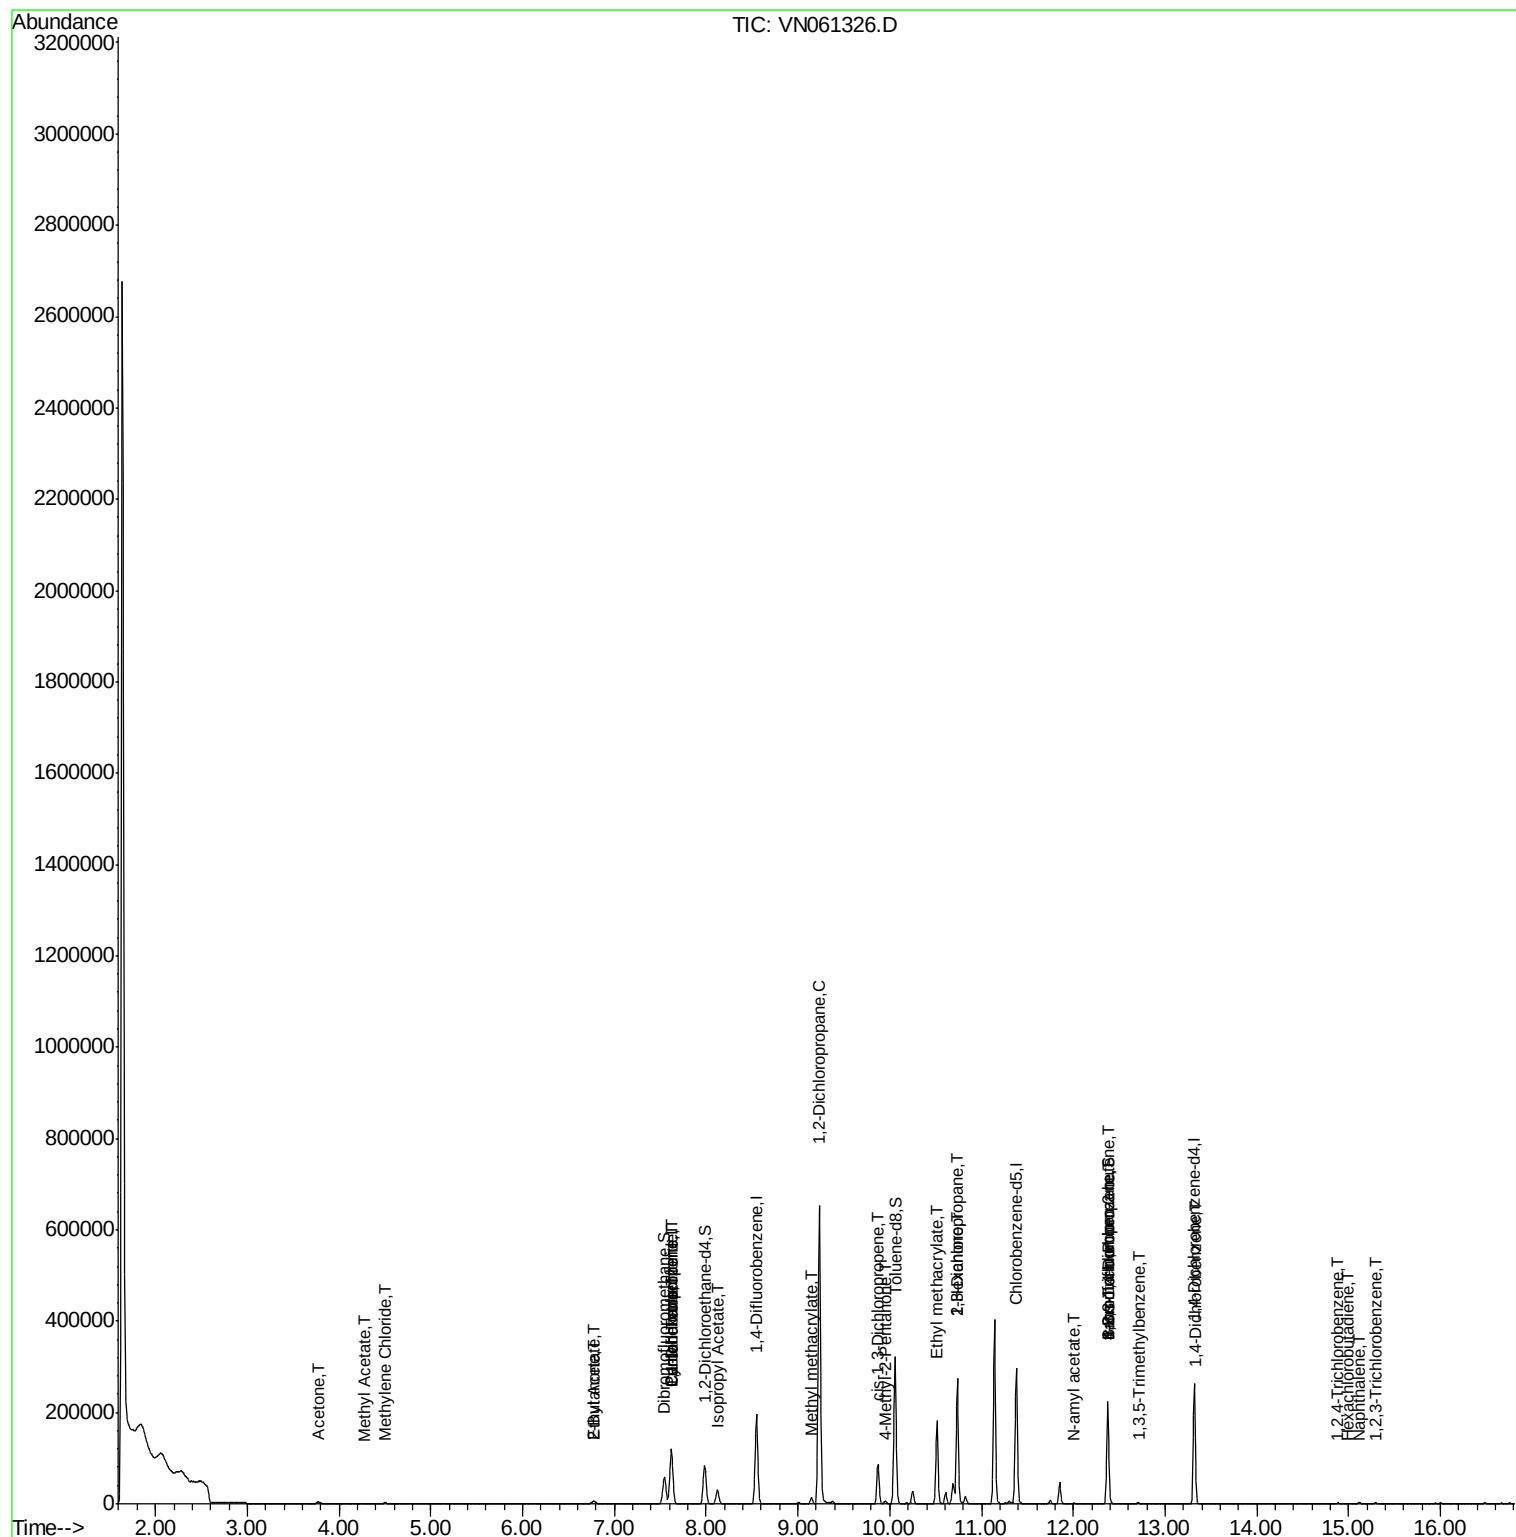



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.62 min Scan# 1876

Delta R.T. -0.00 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion:168 Resp: 89417

Ion Ratio Lower Upper




168 100

99 63.4 51.2 76.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

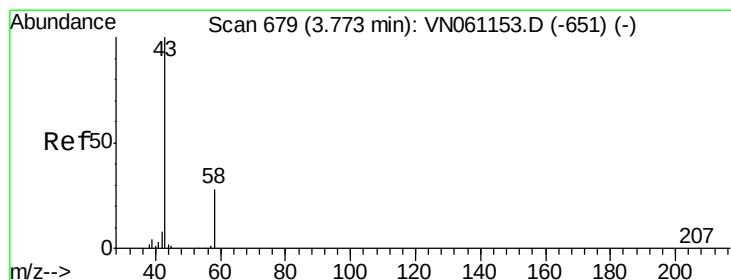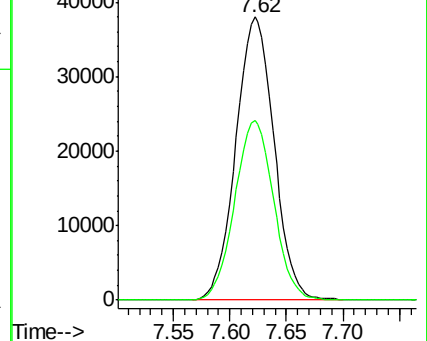

#16

Acetone

Concen: 8.467 ug/l

RT: 3.77 min Scan# 679

Delta R.T. 0.00 min

Lab File: VN061326.D


Acq: 7 May 2020 12:15

Tgt Ion: 43 Resp: 7554

Ion Ratio Lower Upper



43 100


58 29.5 22.2 33.2

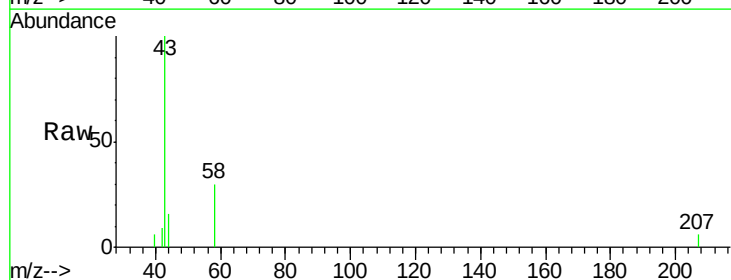

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0



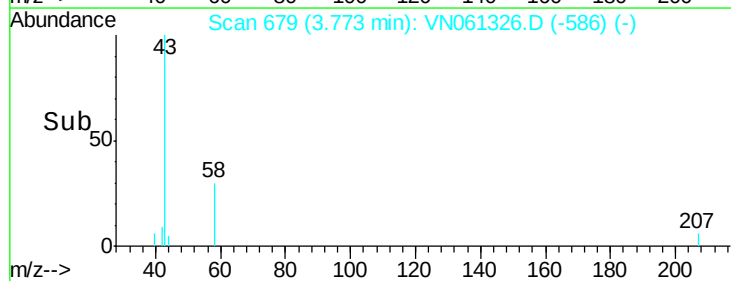
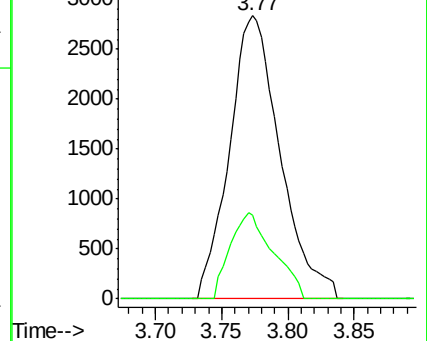


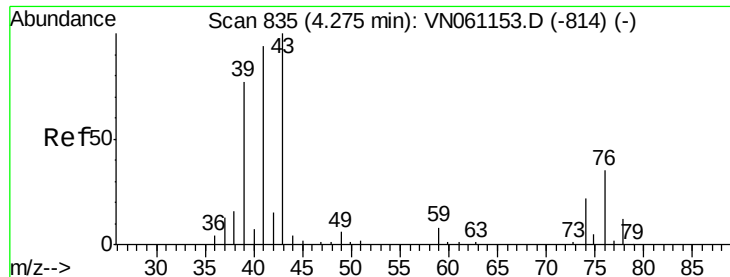

#18
Methvl Acetate
Concen: 1.379 ug/l
RT: 4.28 min Scan# 837
Delta R.T. 0.01 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 43 Resp: 1267
Ion Ratio Lower Upper
43 100
74 0.0 17.0 25.4#

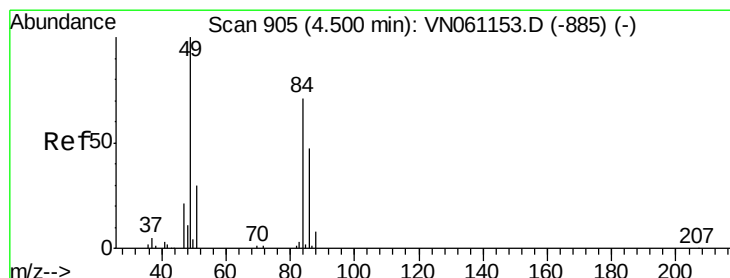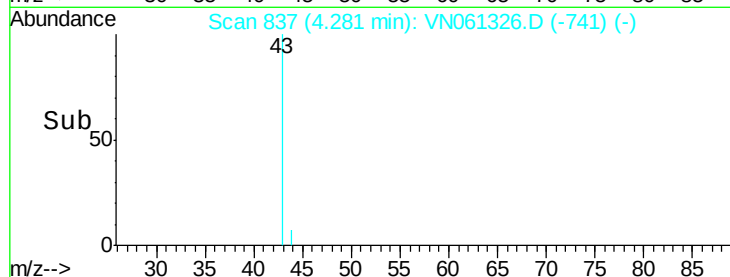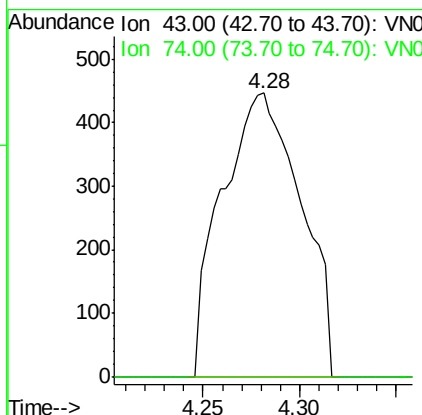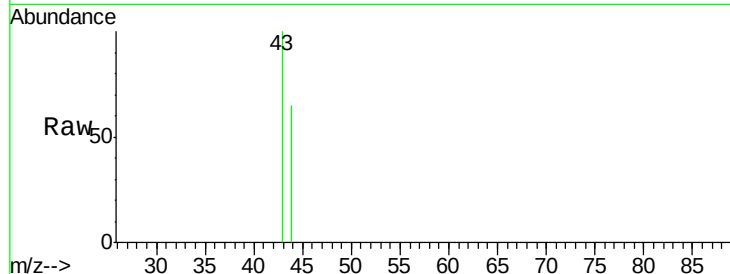

#20
Methylene Chloride
Concen: 1.254 ug/l
RT: 4.50 min Scan# 905
Delta R.T. 0.00 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15

Tgt Ion: 84 Resp: 1384
Ion Ratio Lower Upper
84 100
49 132.3 112.0 168.0
51 60.2 33.6 50.4#
86 67.7 52.1 78.1

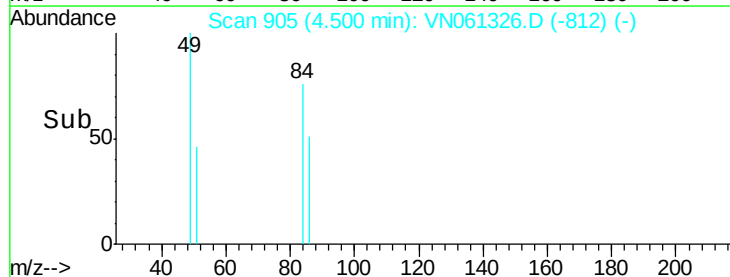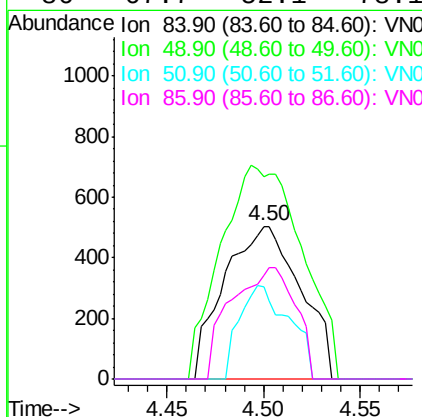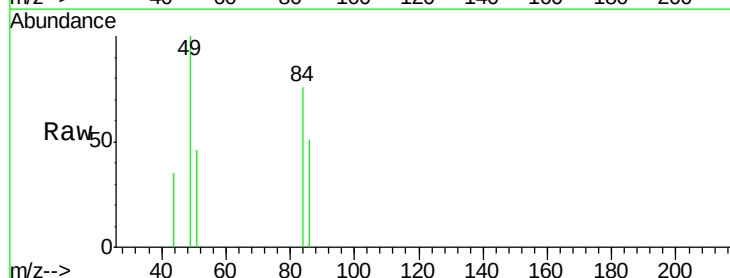



#25

2-Butanone

Concen: 2.217 ug/l

RT: 6.78 min Scan# 1614

Delta R.T. -0.00 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15





Instrument :
MSVOA_N
ClientSampleId :

Tot Ion: 43 Resp: 1856

Ion Ratio Lower Upper

43 100

72 0.0 18.2 27.4#

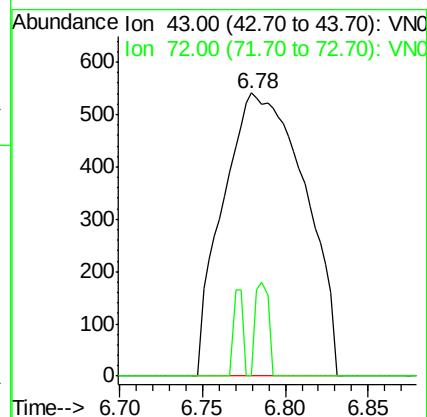

#31

Cyclohexane

Concen: 1.240 ug/l

RT: 7.63 min Scan# 1877

Delta R.T. 0.01 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15




Tgt Ion: 56 Resp: 2553


Ion Ratio Lower Upper

56 100

69 146.8 25.7 38.5#

84 114.1 64.6 97.0#



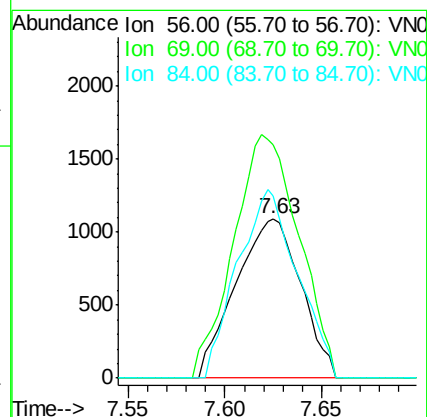





#33
 1,2-Dichloroethane-d4
 Concen: 52.582 ug/l
 RT: 7.98 min Scan# 1988
 Delta R.T. -0.00 min
 Lab File: VN061326.D
 Acq: 7 May 2020 12:15




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion: 65 Resp: 74396
 Ion Ratio Lower Upper
 65 100
 67 49.7 0.0 101.6

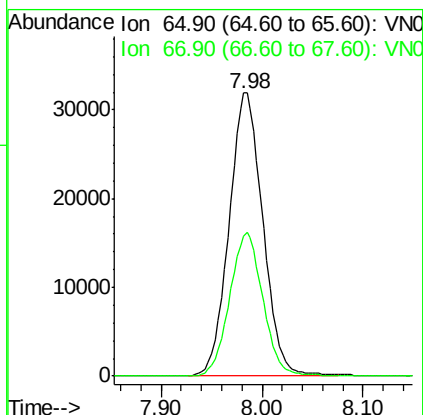

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2164
 Delta R.T. -0.00 min
 Lab File: VN061326.D
 Acq: 7 May 2020 12:15

Tgt Ion: 114 Resp: 161766
 Ion Ratio Lower Upper
 114 100
 63 24.6 0.0 46.6
 88 16.6 0.0 33.4

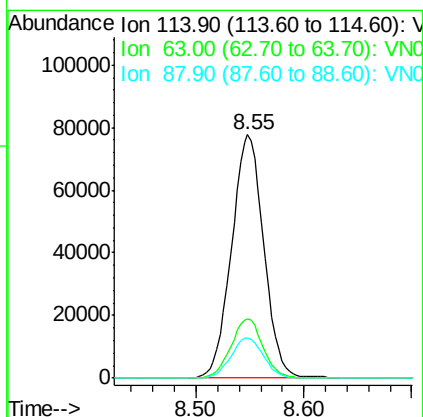


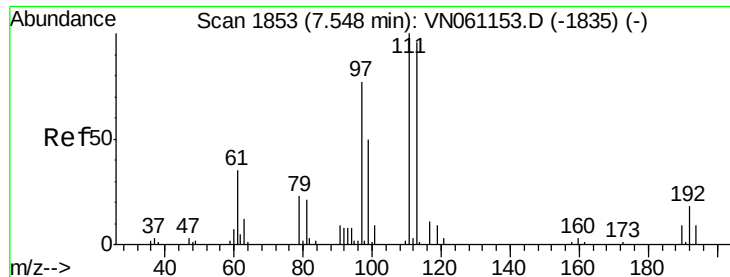




#35
 Dibromofluoromethane
 Concen: 46.804 ug/l
 RT: 7.54 min Scan# 1852
 Delta R.T. -0.00 min
 Lab File: VN061326.D
 Acq: 7 May 2020 12:15

Instrument :
 MSVOA_N
 ClientSampled :

Tot Ion:113 Resp: 44771
 Ion Ratio Lower Upper
 113 100
 111 105.3 82.9 124.3
 192 18.4 14.7 22.1

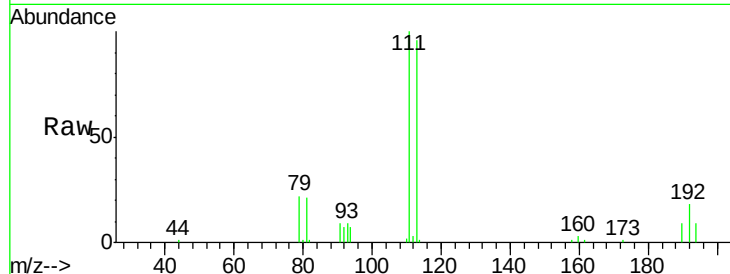


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

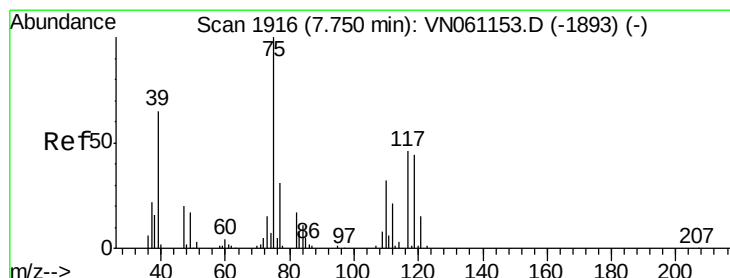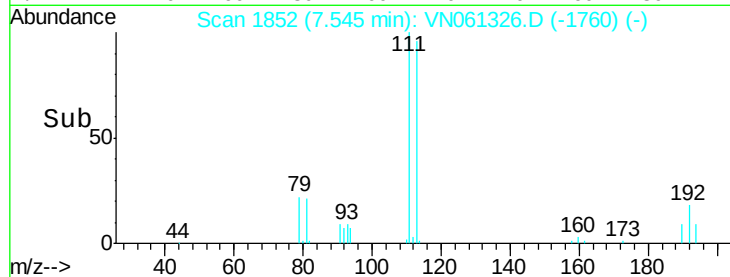
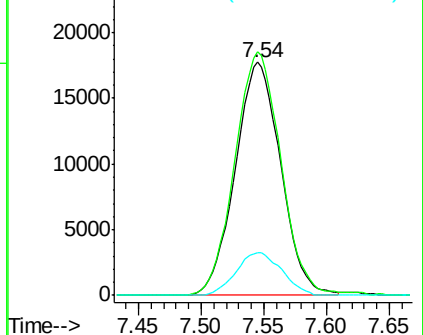



#36
 1,1-Dichloropropene
 Concen: 5.113 ug/l
 RT: 7.62 min Scan# 1876
 Delta R.T. -0.13 min
 Lab File: VN061326.D
 Acq: 7 May 2020 12:15

Tgt Ion: 75 Resp: 8280
 Ion Ratio Lower Upper
 75 100
 110 6.2 16.0 48.0#
 77 0.0 24.6 37.0#

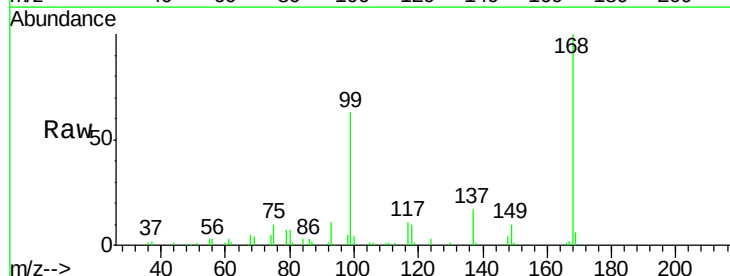

Abundance Ion 74.90 (74.60 to 75.60): V
 Ion 109.90 (109.60 to 110.60): V
 Ion 76.90 (76.60 to 77.60): V



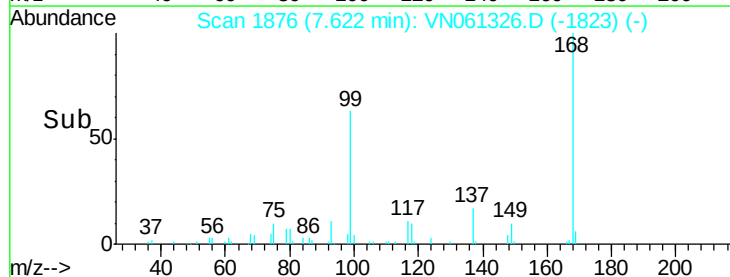
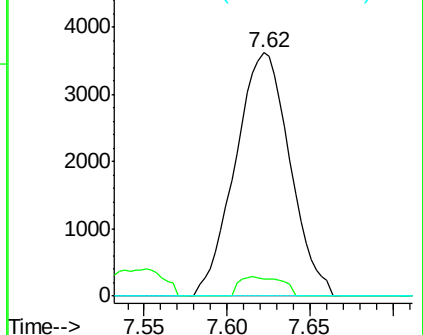




#37
Ethyl Acetate
Concen: 0.978 ug/l
RT: 6.78 min Scan# 1614
Delta R.T. -0.10 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 43 Resp: 1856
Ion Ratio Lower Upper
43 100
61 0.0 10.2 15.2#
70 0.0 7.2 10.8#

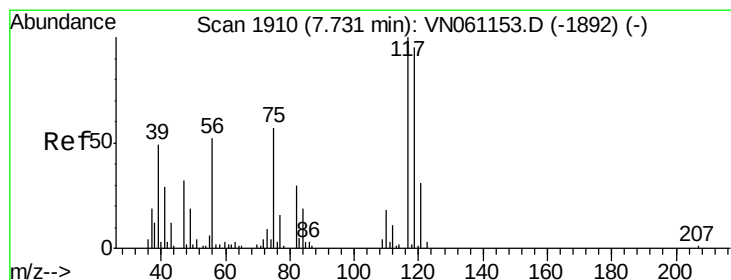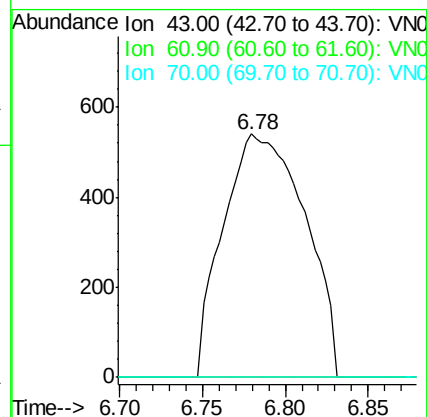

#38
Carbon Tetrachloride
Concen: 8.454 ug/l
RT: 7.62 min Scan# 1876
Delta R.T. -0.11 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15

Tgt Ion: 117 Resp: 9549
Ion Ratio Lower Upper
117 100
119 6.7 75.8 113.6#
121 0.0 24.7 37.1#

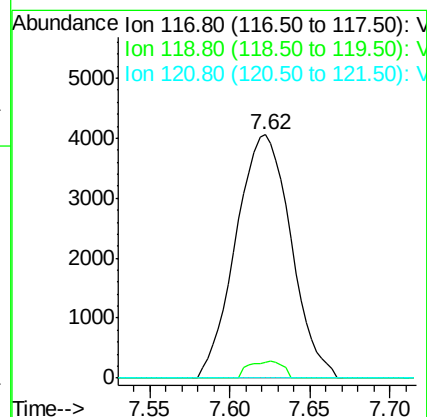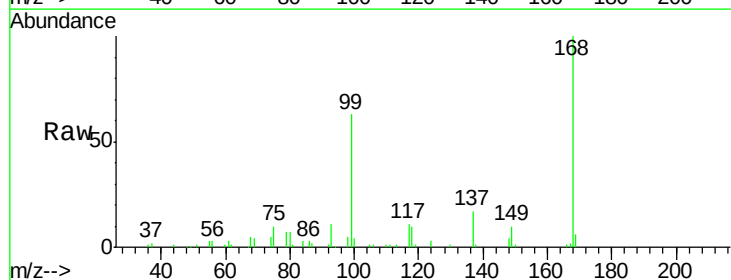



#43

Isopropyl Acetate

Concen: 12.017 ug/l

RT: 8.12 min Scan# 2032

Delta R.T. 0.00 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15

Instrument :

MSVOA_N

ClientSampled :


Tot Ion: 43 Resp: 37861

Ion Ratio Lower Upper

43 100

61 17.4 19.5 29.3#




87 11.0 8.9 13.3



Abundance Ion 43.00 (42.70 to 43.70): VN061153.D (-2014) (-)

Ion 61.00 (60.70 to 61.70): VN061153.D (-2014) (-)

Ion 87.00 (86.70 to 87.70): VN061153.D (-2014) (-)

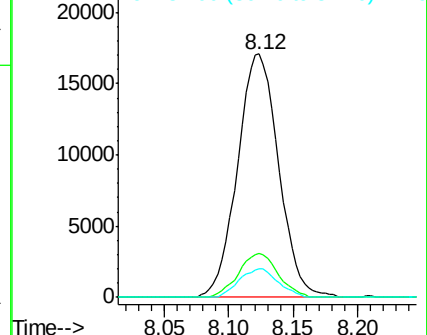

#45

1,2-Dichloropropane

Concen: 0.521 ug/l

RT: 9.24 min Scan# 2378

Delta R.T. 0.15 min

Lab File: VN061326.D


Acq: 7 May 2020 12:15

Tgt Ion: 63 Resp: 671

Ion Ratio Lower Upper



63 100


65 0.0 24.7 37.1#



Abundance Ion 62.90 (62.60 to 63.60): VN061153.D (-2310) (-)

Ion 64.90 (64.60 to 65.60): VN061153.D (-2310) (-)




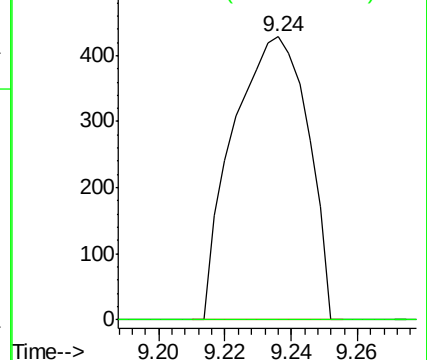




#48
Methvl methacrylate
Concen: 1.422 ug/l
RT: 9.14 min Scan# 2349
Delta R.T. -0.02 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 41 Resp: 2022
Ion Ratio Lower Upper
41 100
69 0.0 60.3 90.5#
39 0.0 47.4 71.0#

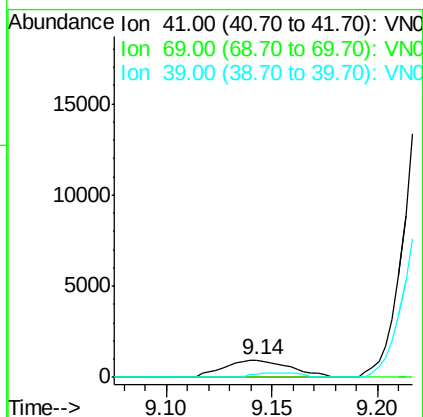

#50
Toluene-d8
Concen: 52.539 ug/l
RT: 10.06 min Scan# 2634
Delta R.T. 0.00 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15

Tgt Ion: 98 Resp: 204873
Ion Ratio Lower Upper
98 100
100 66.2 53.4 80.0

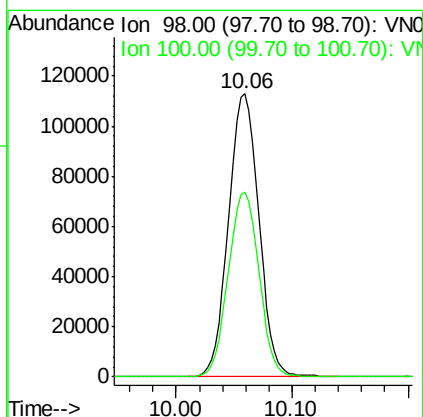



#51

4-Methyl-2-Pentanone

Concen: 1.999 ug/l

RT: 9.95 min Scan# 2600

Delta R.T. -0.00 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 43 Resp: 3708




Ion Ratio Lower Upper

43 100

58 39.5 29.1 43.7



Abundance Ion 43.00 (42.70 to 43.70): VN061326.D (-2508) (-)

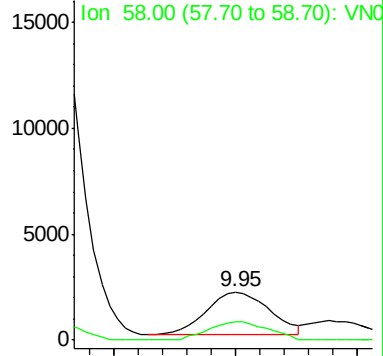

#54

cis-1,3-Dichloropropene

Concen: 6.922 ug/l

RT: 9.87 min Scan# 2576

Delta R.T. 0.06 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15


Tgt Ion: 75 Resp: 14124

Ion Ratio Lower Upper



75 100


77 0.0 25.0 37.4#

39 43.0 48.7 73.1#



Abundance Ion 74.90 (74.60 to 75.60): VN061326.D (-2463) (-)




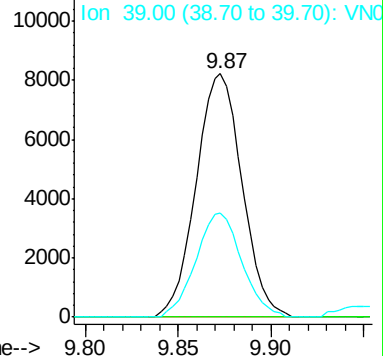




#56
Ethyl methacrylate
Concen: 2.962 ug/l
RT: 10.51 min Scan# 2774
Delta R.T. 0.11 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15




Instrument :
MSVOA_N
ClientSampled :


Tot Ion: 69 Resp: 503
Ion Ratio Lower Upper
69 100
41 7343.3 60.3 90.5#
39 3178.1 35.9 53.9#

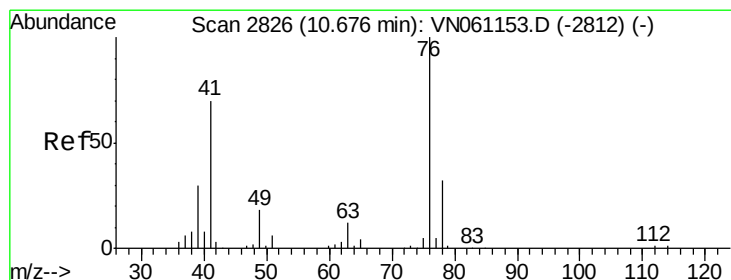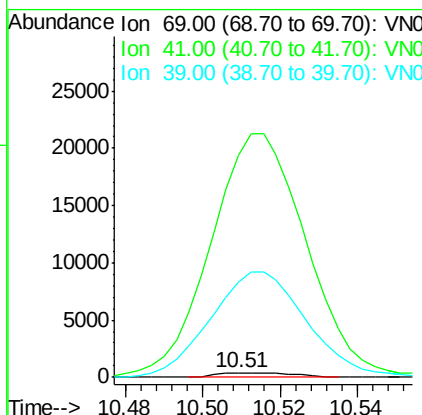

#57
1,3-Dichloropropane
Concen: 1.265 ug/l
RT: 10.73 min Scan# 2844
Delta R.T. 0.06 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15

Tgt Ion: 76 Resp: 2578
Ion Ratio Lower Upper
76 100
78 0.0 25.5 38.3#



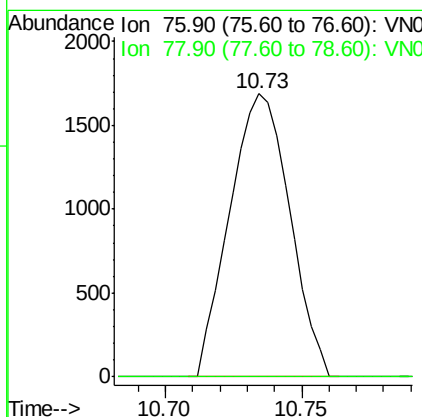
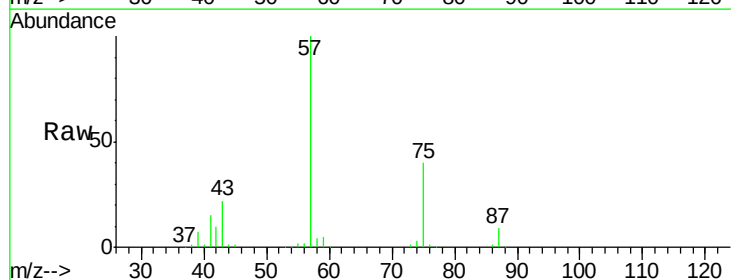




#59
2-Hexanone
Concen: 32.113 ug/l
RT: 10.73 min Scan# 2844
Delta R.T. 0.01 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 43 Resp: 43327
Ion Ratio Lower Upper
43 100
58 17.7 25.4 76.4#

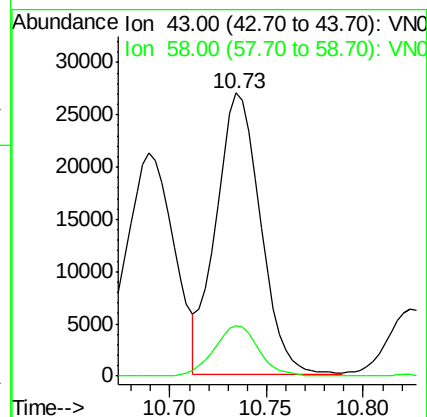

#62
4-Bromofluorobenzene
Concen: 50.787 ug/l
RT: 12.38 min Scan# 3355
Delta R.T. 0.00 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15

Tgt Ion: 95 Resp: 74526
Ion Ratio Lower Upper
95 100
174 73.6 0.0 149.4
176 69.9 0.0 144.8

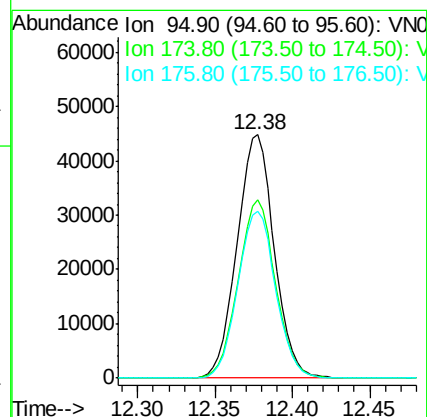


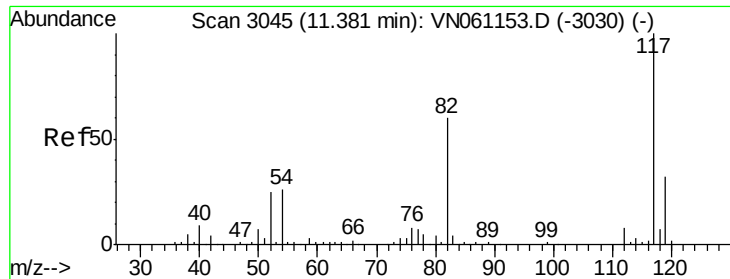




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 3045
Delta R.T. 0.00 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15

Instrument :
MSVOA_N
ClientSampled :

Tot Ion:117 Resp: 158495
Ion Ratio Lower Upper
117 100
82 59.5 47.8 71.8
119 31.9 25.8 38.6

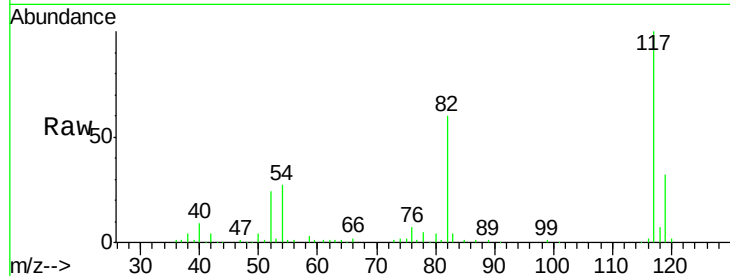


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

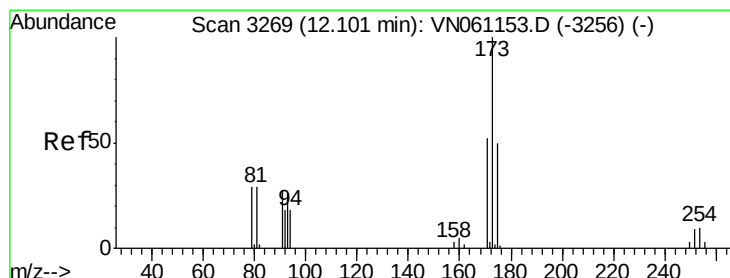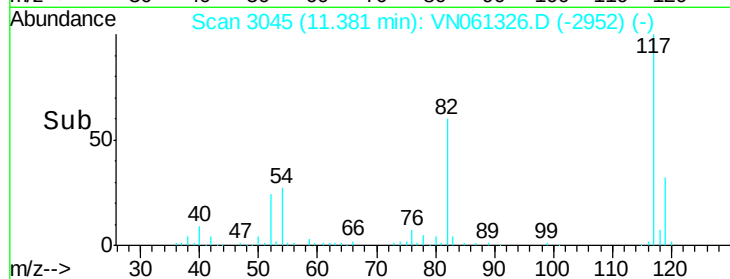
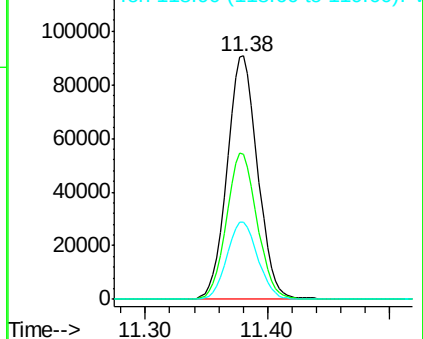



#71
Bromoform
Concen: 0.230 ug/l
RT: 12.38 min Scan# 3355
Delta R.T. 0.28 min
Lab File: VN061326.D
Acq: 7 May 2020 12:15

Tgt Ion:173 Resp: 190
Ion Ratio Lower Upper
173 100
175 1930.5 24.1 72.4#
254 0.0 0.0 0.0

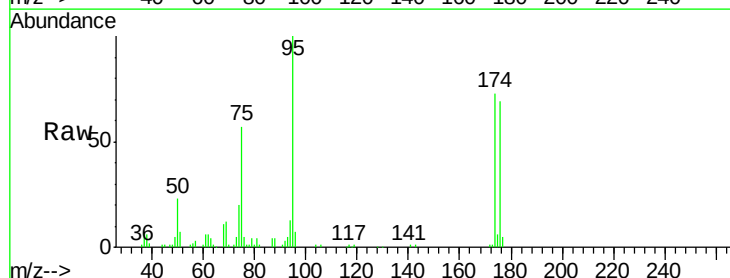

Abundance Ion 172.70 (172.40 to 173.40): V
Ion 174.70 (174.40 to 175.40): V
Ion 254.40 (254.10 to 255.10): V

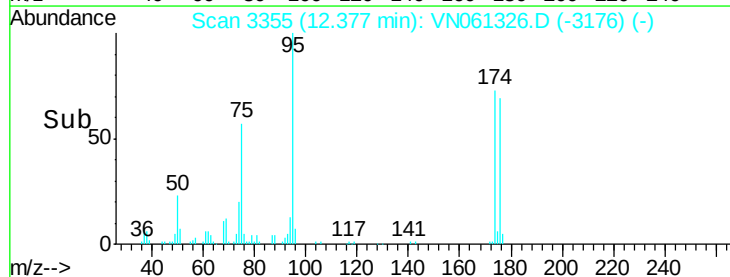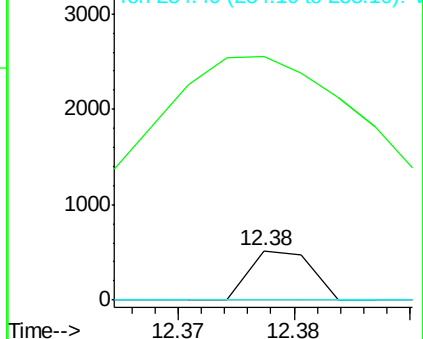



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3648

Delta R.T. 0.00 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:152 Resp: 64468

Ion Ratio Lower Upper

152 100

115 63.2 31.0 93.0




150 158.0 0.0 351.8



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

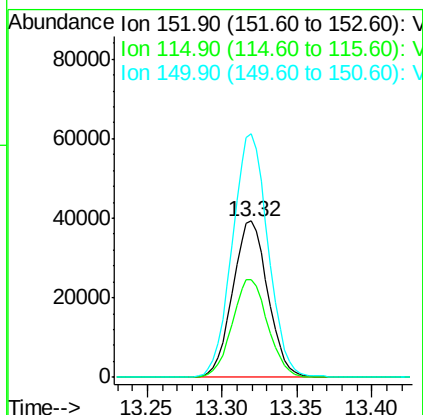

#74

N-ethyl acetate

Concen: 0.618 ug/l

RT: 12.00 min Scan# 3238

Delta R.T. -0.04 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15

Tgt Ion: 43 Resp: 1483


Ion Ratio Lower Upper

43 100

70 0.0 30.6 46.0#

55 0.0 18.5 27.7#

61 0.0 17.9 26.9#






Abundance Ion 43.00 (42.70 to 43.70): V

Ion 70.00 (69.70 to 70.70): V

Ion 55.00 (54.70 to 55.70): V

Ion 61.00 (60.70 to 61.70): V



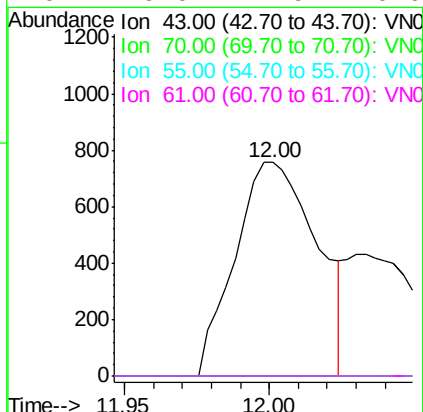





#76
 1,2,3-Trichloropropane
 Concen: 30.929 ug/l
 RT: 12.38 min Scan# 3355
 Delta R.T. -0.15 min
 Lab File: VN061326.D
 Acq: 7 May 2020 12:15




Instrument :
 MSVOA_N
 ClientSampled :


Tot Ion: 75 Resp: 42038
 Ion Ratio Lower Upper
 75 100
 77 0.8 0.0 0.0#

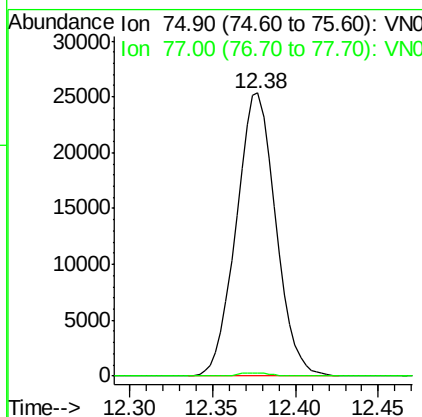

#80
 1,3,5-Trimethylbenzene
 Concen: 0.737 ug/l
 RT: 12.71 min Scan# 3459
 Delta R.T. 0.00 min
 Lab File: VN061326.D
 Acq: 7 May 2020 12:15

Tgt Ion: 105 Resp: 2890
 Ion Ratio Lower Upper
 105 100
 120 44.7 23.9 71.7

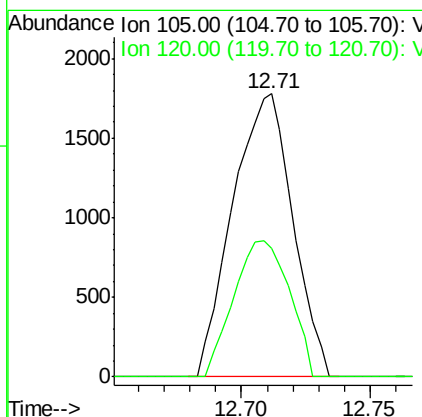



#81

trans-1,4-Dichloro-2-butene

Concen: 78.545 ug/l

RT: 12.38 min Scan# 3355

Delta R.T. 0.10 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion: 75 Resp: 42038

Ion Ratio Lower Upper

75 100

53 0.0 84.1 126.1#




89 0.0 35.2 52.8#



Abundance Ion 74.90 (74.60 to 75.60): VN061153.D (-3313) (-)

Ion 53.00 (52.70 to 53.70): VN061153.D (-3313) (-)

Ion 88.90 (88.60 to 89.60): VN061153.D (-3313) (-)

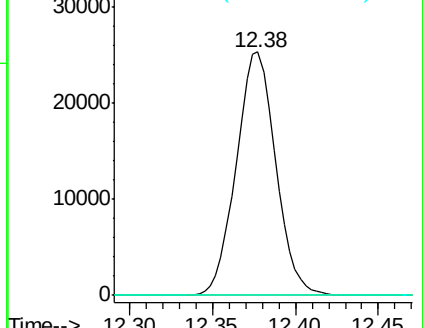

#88

1,4-Dichlorobenzene

Concen: 0.244 ug/l

RT: 13.34 min Scan# 3654

Delta R.T. 0.00 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15


Tgt Ion: 146 Resp: 502

Ion Ratio Lower Upper

146 100

111 0.0 20.4 61.3#



148 0.0 31.9 95.7#




Abundance Ion 145.90 (145.60 to 146.60): VN061153.D (-3641) (-)

Ion 110.90 (110.60 to 111.60): VN061153.D (-3641) (-)

Ion 147.90 (147.60 to 148.60): VN061153.D (-3641) (-)




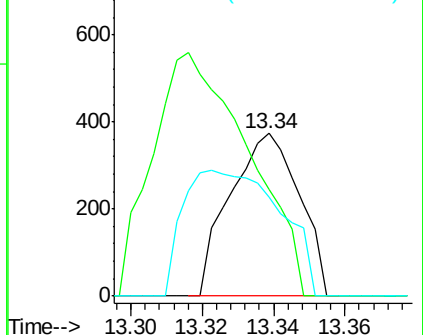


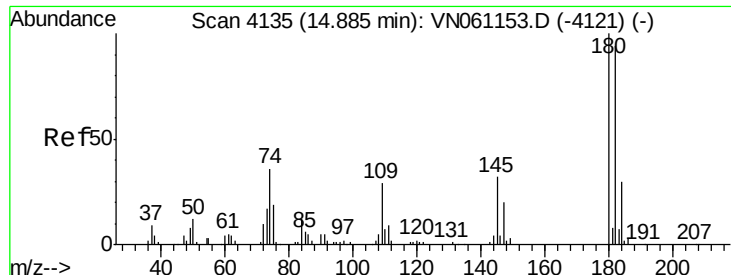

#93
 1,2,4-Trichlorobenzene
 Concen: 0.412 ug/l
 RT: 14.88 min Scan# 4134
 Delta R.T. -0.00 min
 Lab File: VN061326.D
 Acq: 7 May 2020 12:15




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion:180 Resp: 485
 Ion Ratio Lower Upper
 180 100
 182 80.6 47.3 141.9
 145 0.0 16.0 47.9#

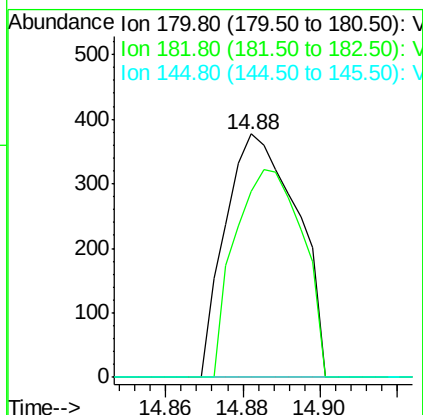

#94
 Hexachlorobutadiene
 Concen: 0.486 ug/l
 RT: 14.98 min Scan# 4166
 Delta R.T. 0.00 min
 Lab File: VN061326.D
 Acq: 7 May 2020 12:15

Tgt Ion:225 Resp: 239
 Ion Ratio Lower Upper
 225 100
 223 0.0 32.4 97.0#
 227 0.0 32.4 97.0#

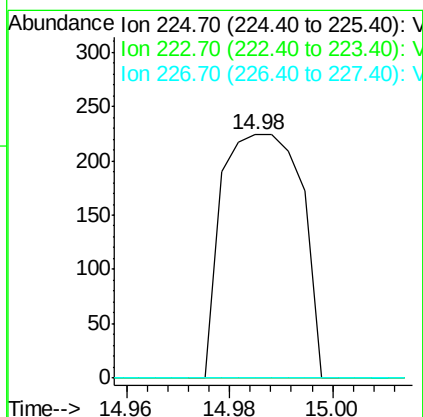

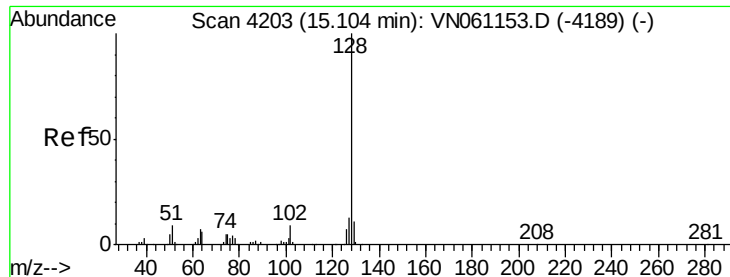

#95

Naphthalene

Concen: 0.539 ug/l

RT: 15.11 min Scan# 4204

Delta R.T. 0.00 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15

Instrument :

MSVOA_N

ClientSampled :


Tot Ion:128 Resp: 2066

Ion Ratio Lower Upper

128 100

127 0.0 10.4 15.6#




129 0.0 8.7 13.1#

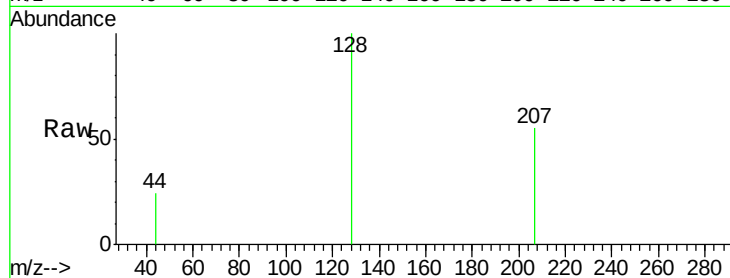

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

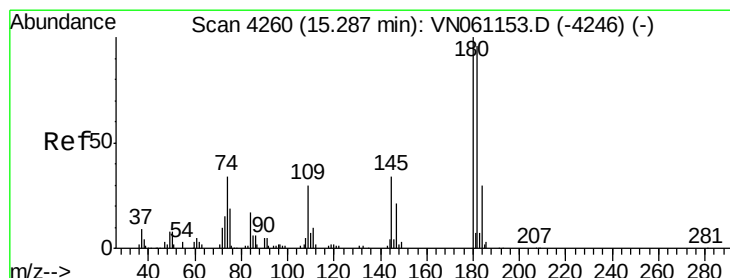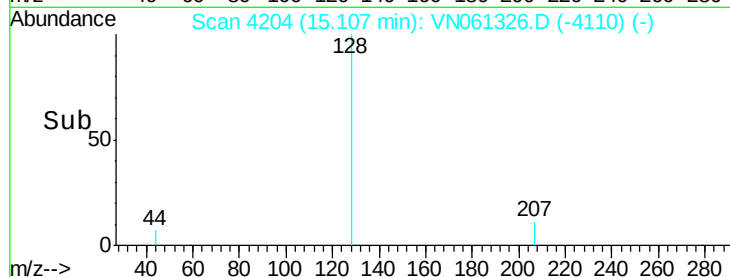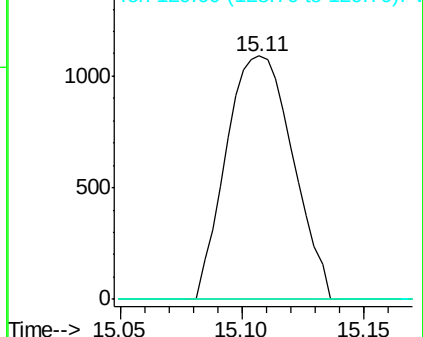

#96

1,2,3-Trichlorobenzene

Concen: 0.367 ug/l

RT: 15.29 min Scan# 4260

Delta R.T. 0.00 min

Lab File: VN061326.D

Acq: 7 May 2020 12:15


Tgt Ion:180 Resp: 426

Ion Ratio Lower Upper

180 100

182 116.7 47.5 142.5

145 0.0 16.9 50.7#

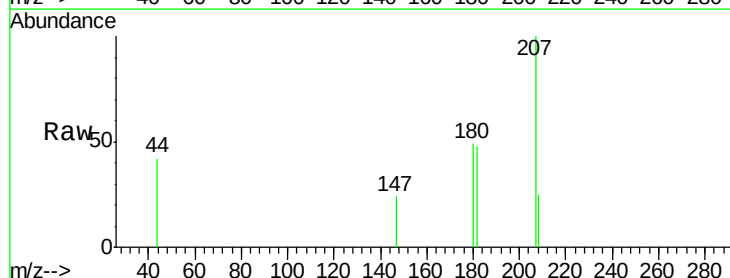

Abundance Ion 179.80 (179.50 to 180.50): V

Ion 181.80 (181.50 to 182.50): V

Ion 144.90 (144.60 to 145.60): V

