

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN050720\
 Data File : VN061344.D
 Acq On : 7 May 2020 19:12
 Operator : JC/MD
 Sample : L2544-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: May 08 02:56:59 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 05 07:01:08 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	92951	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	170928	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	166494	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	74610	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	7.99	65	79022	53.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.46%	
35) Dibromofluoromethane	7.55	113	51892	51.34	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.68%	
50) Toluene-d8	10.06	98	216950	52.65	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.30%	
62) 4-Bromofluorobenzene	12.38	95	81306	52.44	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.88%	

Target Compounds


					Qvalue	
11) Tert butyl alcohol	4.73	59	315	1.599	ug/l #	72
16) Acetone	3.78	43	1364	Below Cal	#	47
18) Methyl Acetate	4.48	43	2096	1.793	ug/l #	55
31) Cyclohexane	7.63	56	3003	1.404	ug/l #	45
36) 1,1-Dichloropropene	7.62	75	8394	4.906	ug/l #	49
38) Carbon Tetrachloride	7.63	117	9847	8.306	ug/l #	16
39) Methylcyclohexane	9.01	83	2612	1.361	ug/l #	31
40) Benzene	8.00	78	2254	0.442	ug/l #	88
47) Bromodichloromethane	9.49	83	481	0.266	ug/l #	25
48) Methyl methacrylate	9.19	41	2966	1.974	ug/l #	33
51) 4-Methyl-2-Pentanone	9.99	43	1050	0.536	ug/l #	38
55) 1,1,2-Trichloroethane	10.50	97	1622	1.324	ug/l #	14
56) Ethyl methacrylate	10.40	69	918	3.134	ug/l #	1
59) 2-Hexanone	10.68	43	333	0.234	ug/l #	27
65) Chlorobenzene	11.41	112	981822	297.279	ug/l	100
73) Isopropylbenzene	12.22	105	8574	1.563	ug/l	100
76) 1,2,3-Trichloropropane	12.37	75	46122	29.321	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.37	75	46122	74.461	ug/l #	8
83) tert-Butylbenzene	12.97	119	16865	4.406	ug/l	92
84) 1,2,4-Trimethylbenzene	13.15	105	18921	4.045	ug/l #	32
85) sec-Butylbenzene	13.15	105	18921	3.626	ug/l #	54
86) p-Isopropyltoluene	13.42	119	71275	15.158	ug/l	97
87) 1,3-Dichlorobenzene	13.26	146	701	0.301	ug/l	79
88) 1,4-Dichlorobenzene	13.26	146	701	0.294	ug/l	79
89) n-Butylbenzene	13.57	91	1270	0.295	ug/l #	23
90) Hexachloroethane	13.92	117	23902	48.927	ug/l #	14
92) 1,2-Dibromo-3-Chloropropan	14.18	75	134	0.371	ug/l #	7

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN050720\
Data File : VN061344.D
Acq On : 7 May 2020 19:12
Operator : JC/MD
Sample : L2544-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: May 08 02:56:59 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
Quant Title : SW846 8260
QLast Update : Tue May 05 07:01:08 2020
Response via : Initial Calibration

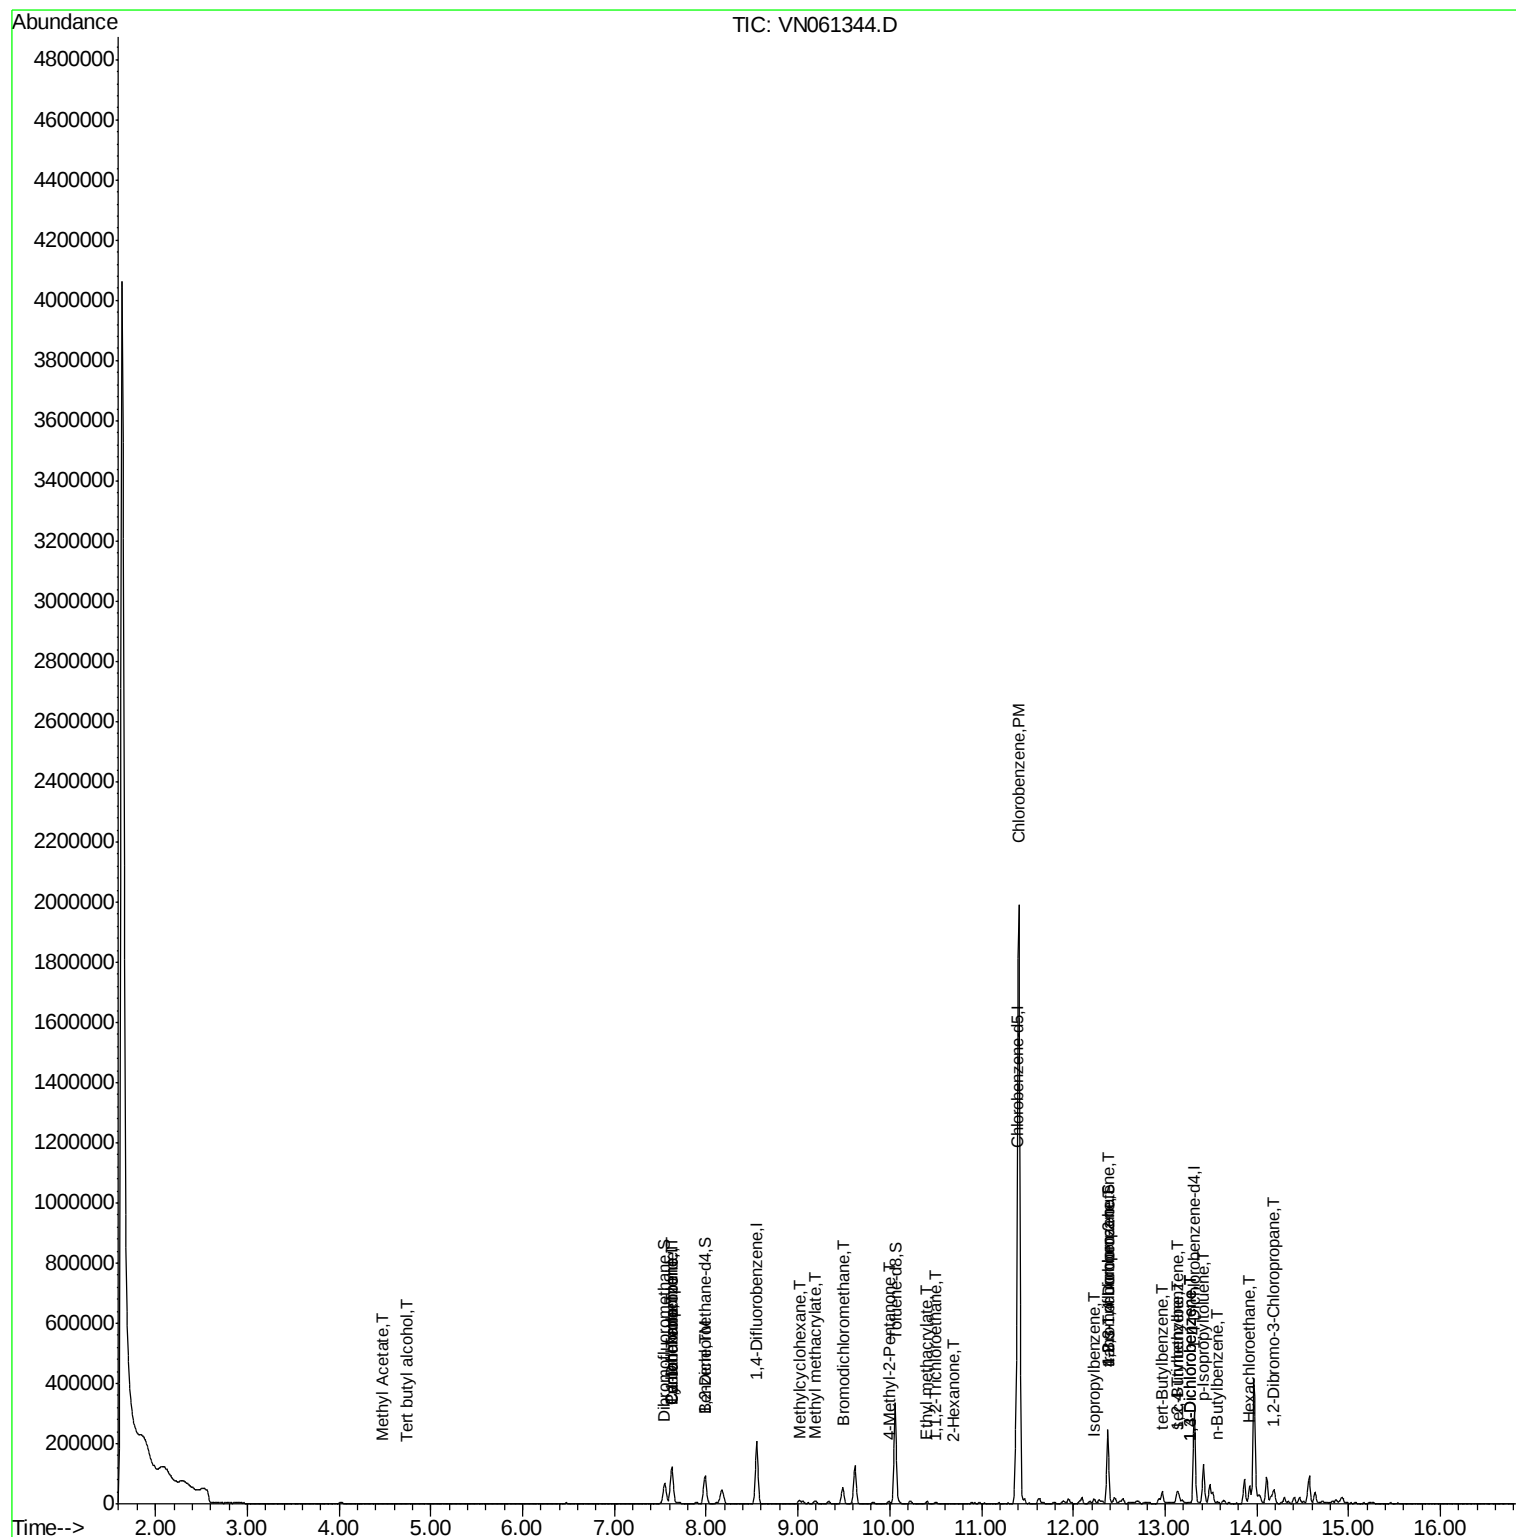



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1877

Delta R.T. 0.00 min

Lab File: VN061344.D

Acq: 7 May 2020 19:12

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion:168 Resp: 92951

Ion Ratio Lower Upper




168 100

99 62.5 51.2 76.8

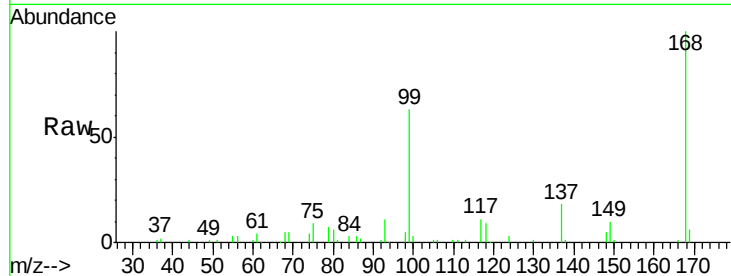

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

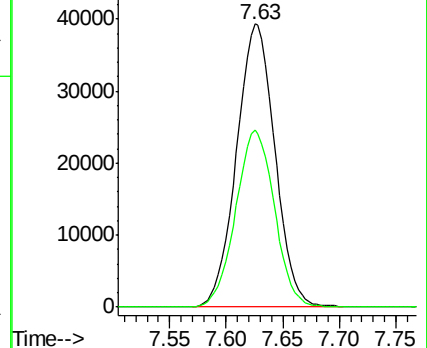

#11

Tert butyl alcohol

Concen: 1.599 ug/l

RT: 4.73 min Scan# 977

Delta R.T. 0.00 min

Lab File: VN061344.D


Acq: 7 May 2020 19:12

Tgt Ion: 59 Resp: 315

Ion Ratio Lower Upper



59 100


57 0.0 8.3 12.5#



Abundance Ion 59.00 (58.70 to 59.70): VNO

Ion 57.00 (56.70 to 57.70): VNO

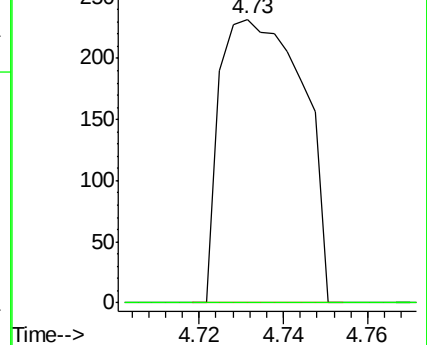



#16

Acetone

Concen: Below Cal

RT: 3.78 min Scan# 682

Delta R.T. 0.01 min

Lab File: VN061344.D

Acq: 7 May 2020 19:12

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 43 Resp: 1364




Ion Ratio Lower Upper

43 100

58 0.0 22.2 33.2#

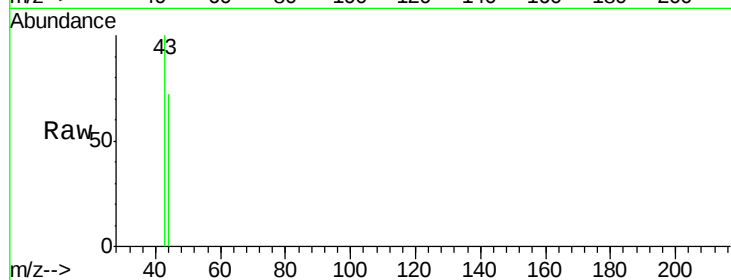

Abundance Ion 43.00 (42.70 to 43.70): VN061153.D (-651) (-)

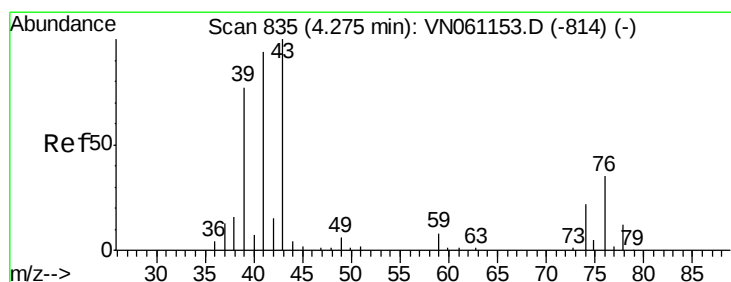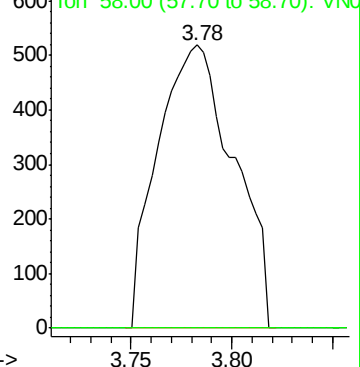

#18

Methyl Acetate

Concen: 1.793 ug/l

RT: 4.48 min Scan# 899

Delta R.T. 0.21 min

Lab File: VN061344.D


Acq: 7 May 2020 19:12

Tgt Ion: 43 Resp: 2096



Ion Ratio Lower Upper


43 100

74 0.0 17.0 25.4#

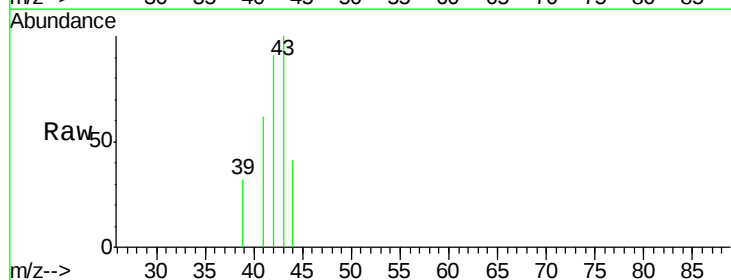

Abundance Ion 43.00 (42.70 to 43.70): VN061153.D (-814) (-)




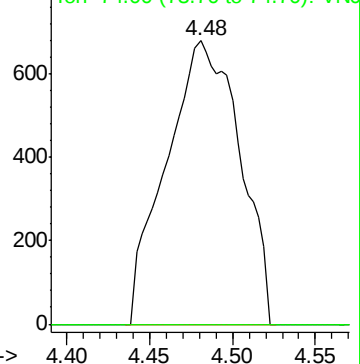


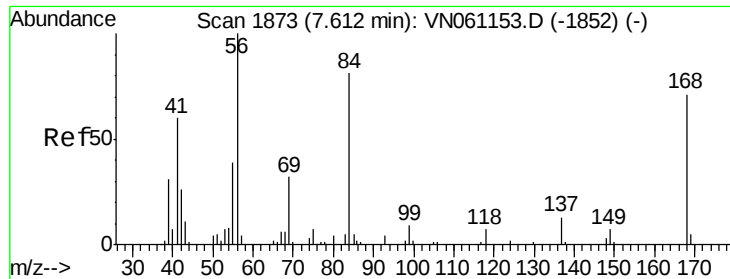

#31
Cyclohexane
Concen: 1.404 ug/l
RT: 7.63 min Scan# 1877
Delta R.T. 0.01 min
Lab File: VN061344.D
Acq: 7 May 2020 19:12




Instrument :
MSVOA_N
ClientSampled :


Tot Ion: 56 Resp: 3003
Ion Ratio Lower Upper
56 100
69 136.5 25.7 38.5#
84 83.1 64.6 97.0

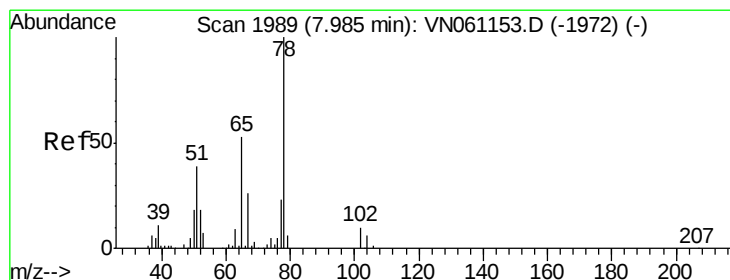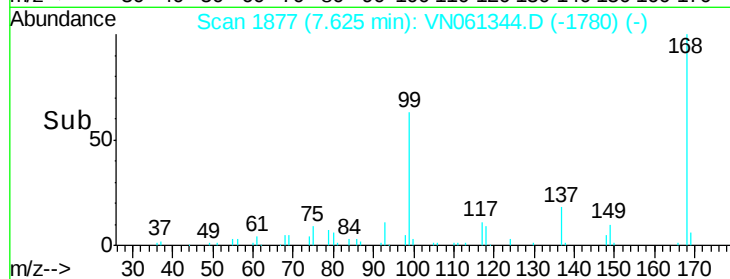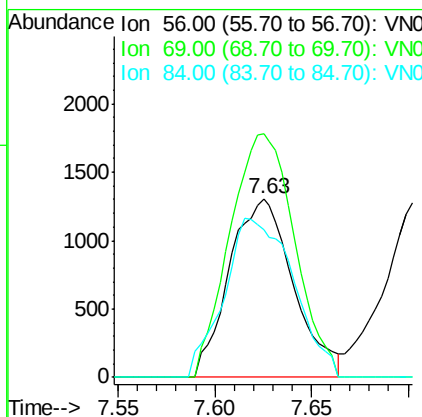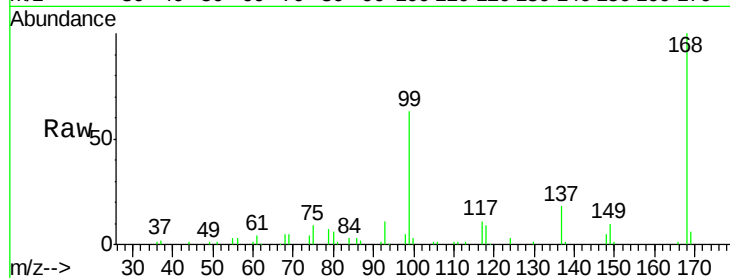

#33
1,2-Dichloroethane-d4
Concen: 53.728 ug/l
RT: 7.99 min Scan# 1990
Delta R.T. 0.00 min
Lab File: VN061344.D
Acq: 7 May 2020 19:12

Tgt Ion: 65 Resp: 79022
Ion Ratio Lower Upper
65 100
67 50.8 0.0 101.6

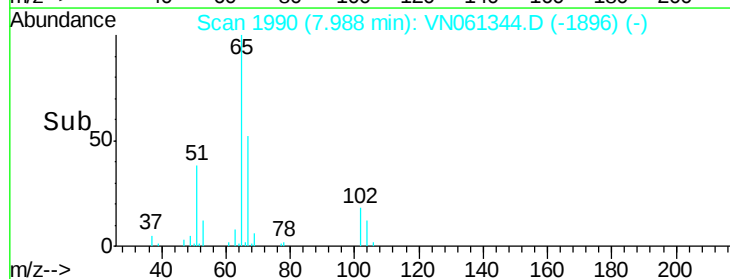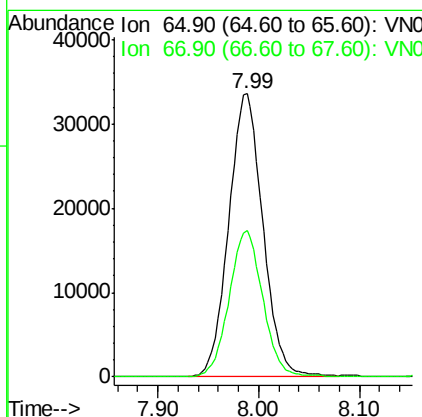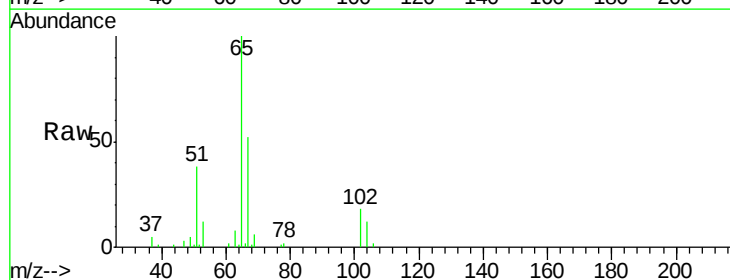


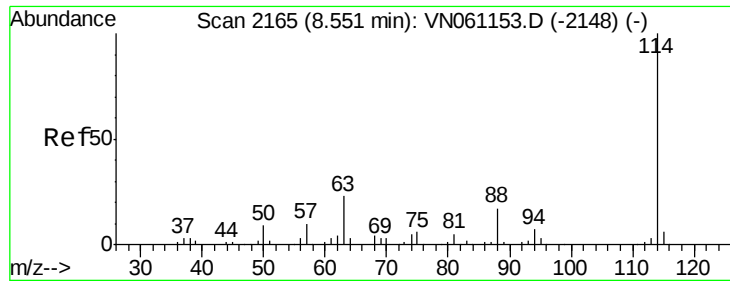




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2165
 Delta R.T. 0.00 min
 Lab File: VN061344.D
 Acq: 7 May 2020 19:12

Instrument :
 MSVOA_N
 ClientSampleId :

Tot Ion:114 Resp: 170928
 Ion Ratio Lower Upper
 114 100
 63 23.9 0.0 46.6
 88 16.5 0.0 33.4

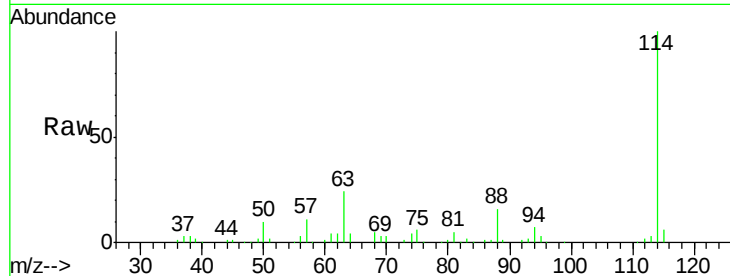


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): V
 Ion 87.90 (87.60 to 88.60): V

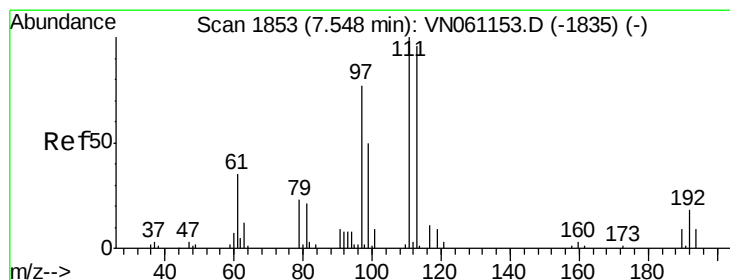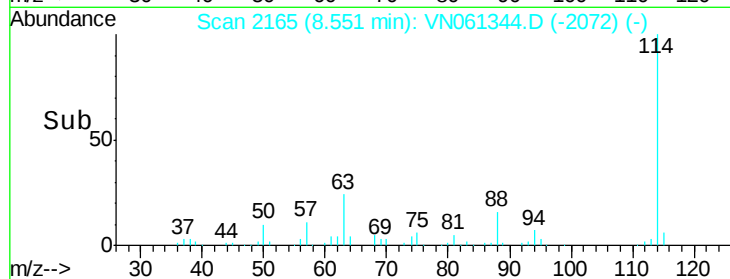
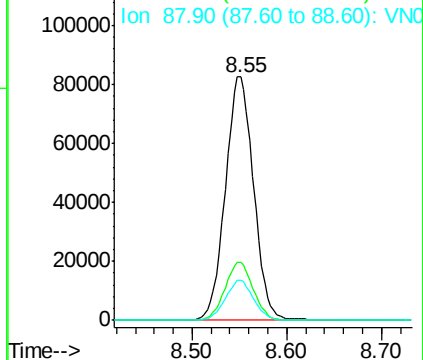



#35
 Dibromofluoromethane
 Concen: 51.341 ug/l
 RT: 7.55 min Scan# 1853
 Delta R.T. 0.00 min
 Lab File: VN061344.D
 Acq: 7 May 2020 19:12

Tgt Ion:113 Resp: 51892
 Ion Ratio Lower Upper
 113 100
 111 104.0 82.9 124.3
 192 18.4 14.7 22.1

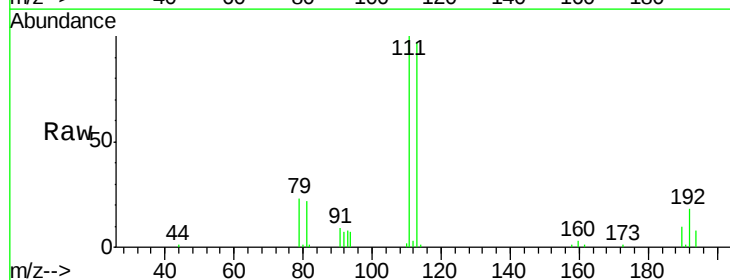

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



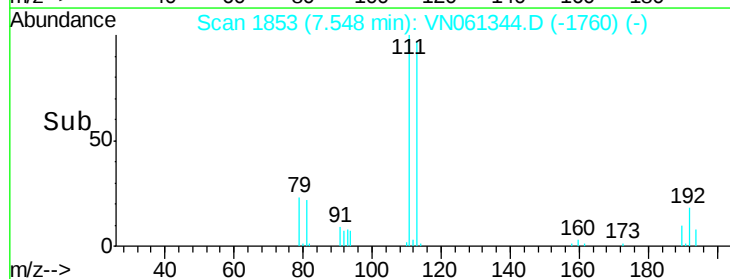
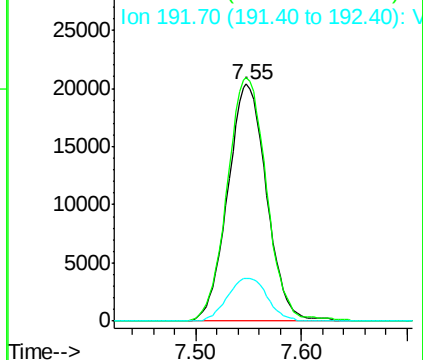


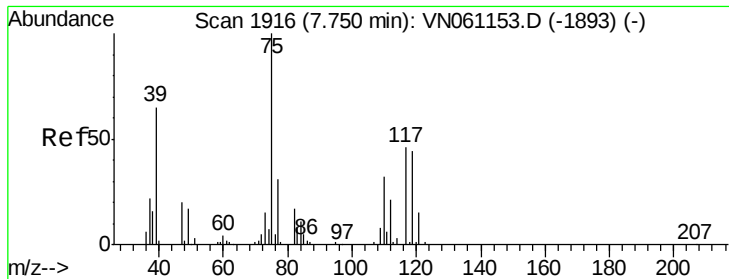

#36
 1,1-Dichloropropene
 Concen: 4.906 ug/l
 RT: 7.62 min Scan# 1876
 Delta R.T. -0.13 min
 Lab File: VN061344.D
 Acq: 7 May 2020 19:12




Instrument :
 MSVOA_N
 ClientSampled :


Tot Ion: 75 Resp: 8394
 Ion Ratio Lower Upper
 75 100
 110 6.5 16.0 48.0#
 77 0.0 24.6 37.0#

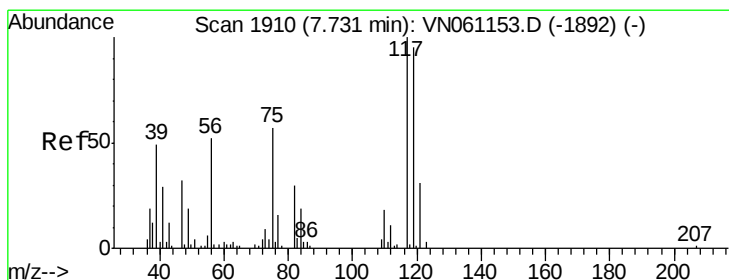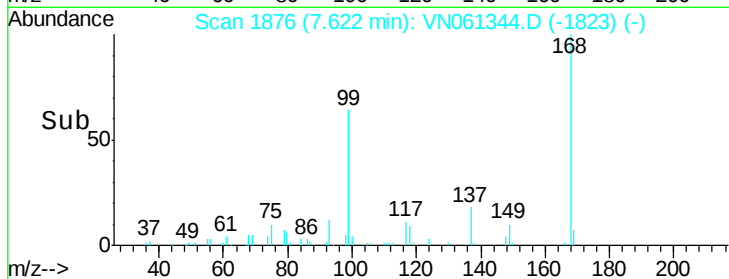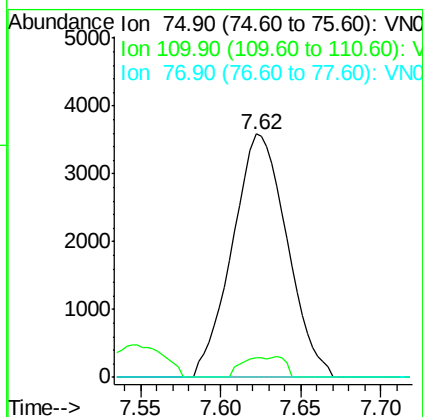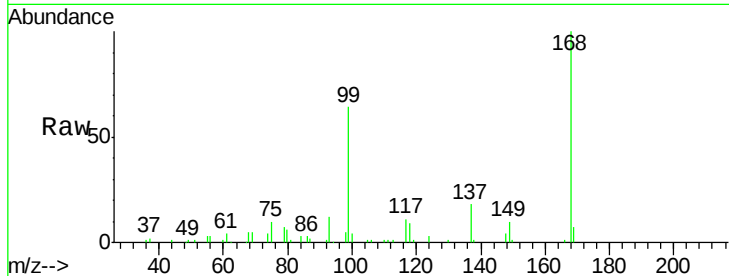

#38
 Carbon Tetrachloride
 Concen: 8.306 ug/l
 RT: 7.63 min Scan# 1877
 Delta R.T. -0.11 min
 Lab File: VN061344.D
 Acq: 7 May 2020 19:12

Tgt Ion: 117 Resp: 9847
 Ion Ratio Lower Upper
 117 100
 119 4.6 75.8 113.6#
 121 0.0 24.7 37.1#


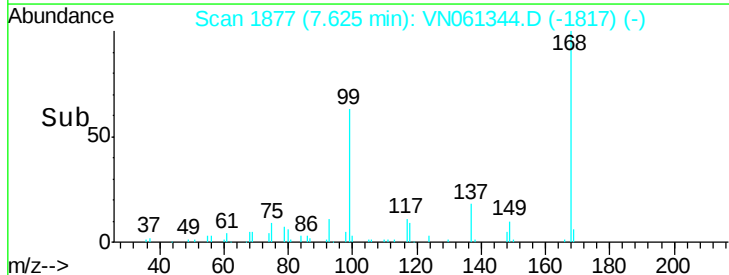
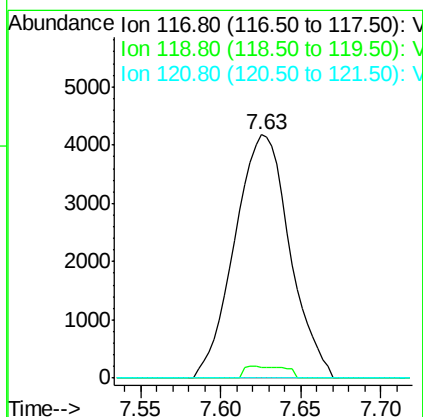
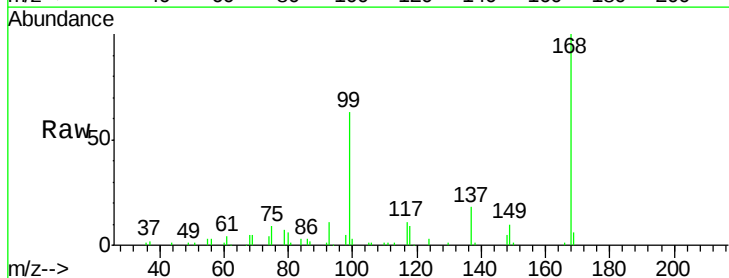




#39
Methvlcvclohexane
Concen: 1.361 ug/l
RT: 9.01 min Scan# 2309
Delta R.T. -0.03 min
Lab File: VN061344.D
Acq: 7 May 2020 19:12




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 83 Resp: 2612
Ion Ratio Lower Upper
83 100
55 146.3 67.3 100.9#
98 0.0 37.7 56.5#

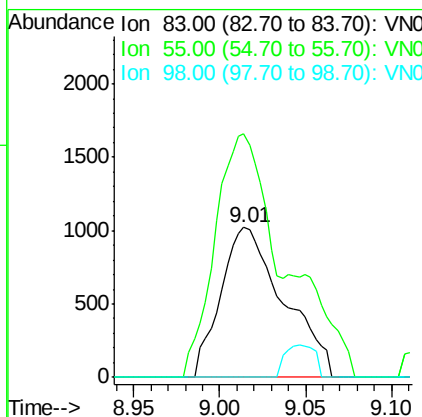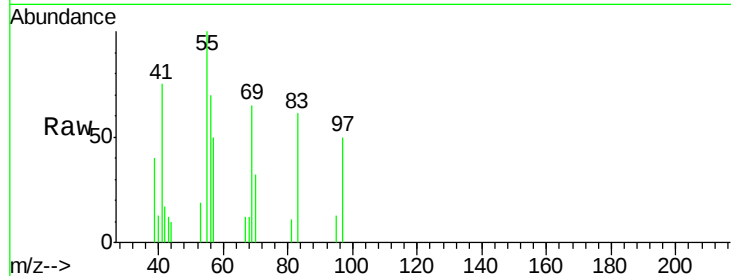

#40
Benzene
Concen: 0.442 ug/l
RT: 8.00 min Scan# 1993
Delta R.T. -0.00 min
Lab File: VN061344.D
Acq: 7 May 2020 19:12

Tgt Ion: 78 Resp: 2254
Ion Ratio Lower Upper
78 100
77 29.5 19.0 28.6#

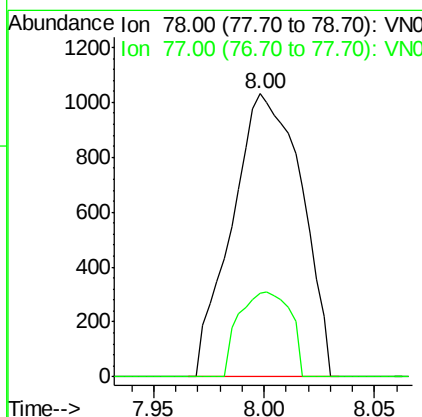

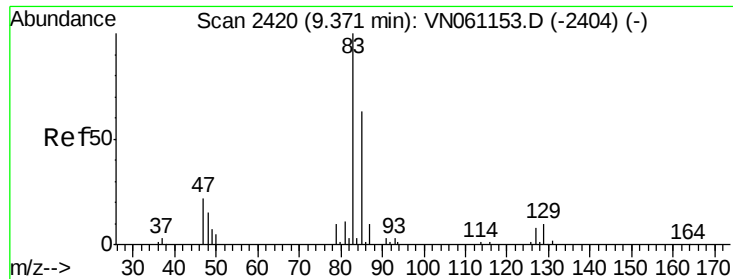

#47

Bromodichloromethane

Concen: 0.266 ug/l

RT: 9.49 min Scan# 2456

Delta R.T. 0.12 min

Lab File: VN061344.D

Acq: 7 May 2020 19:12

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion: 83 Resp: 481

Ion Ratio Lower Upper

83 100

85 0.0 50.4 75.6#




127 0.0 6.2 9.2#

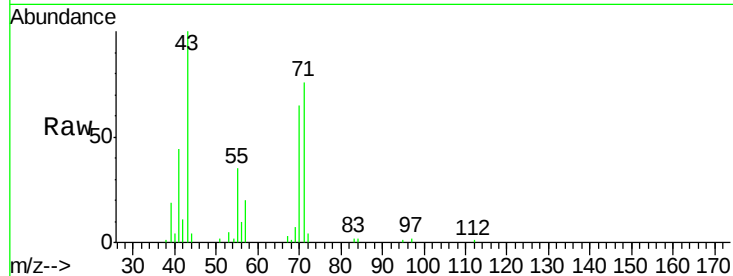

Abundance Ion 82.90 (82.60 to 83.60): VN061153.D (-2404) (-)

Ion 84.90 (84.60 to 85.60): VN061153.D (-2404) (-)

Ion 126.80 (126.50 to 127.50): VN061153.D (-2404) (-)

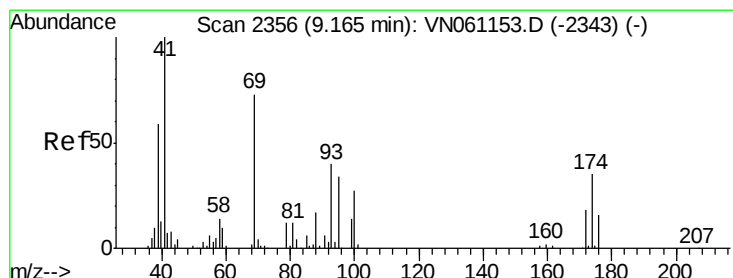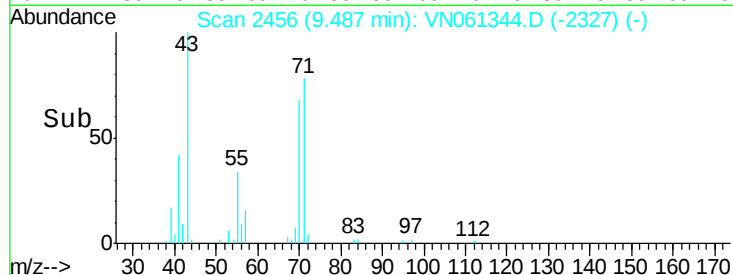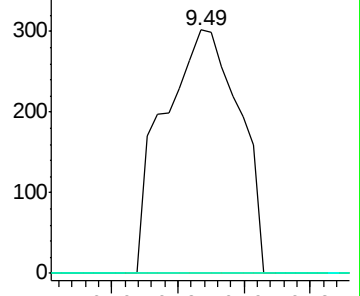

#48

Methyl methacrylate

Concen: 1.974 ug/l

RT: 9.19 min Scan# 2364

Delta R.T. 0.03 min

Lab File: VN061344.D

Acq: 7 May 2020 19:12


Tgt Ion: 41 Resp: 2966

Ion Ratio Lower Upper

41 100

69 0.0 60.3 90.5#



39 29.4 47.4 71.0#

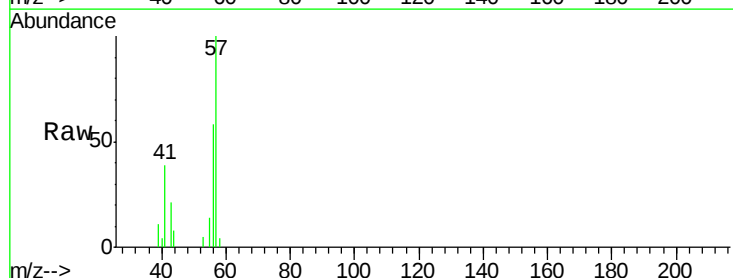


Abundance Ion 41.00 (40.70 to 41.70): VN061153.D (-2343) (-)

Ion 69.00 (68.70 to 69.70): VN061153.D (-2343) (-)

Ion 39.00 (38.70 to 39.70): VN061153.D (-2343) (-)



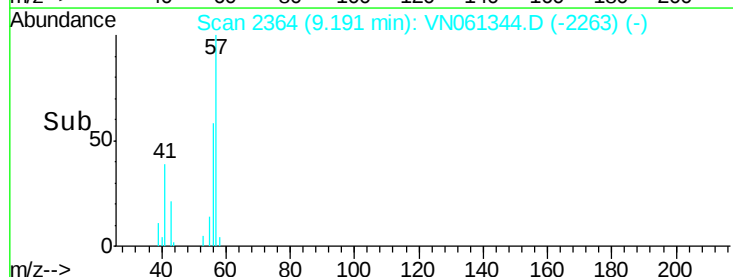
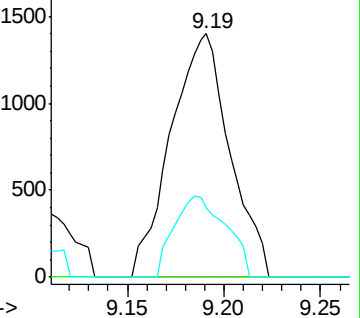


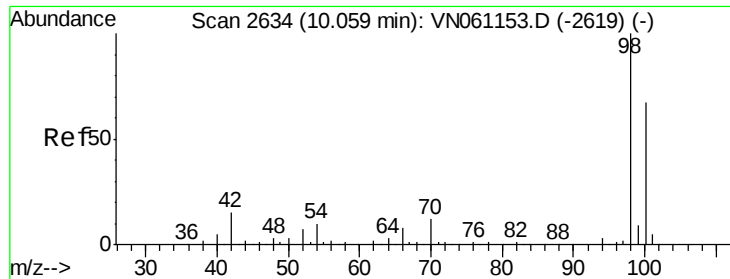

#50
Toluene-d8
Concen: 52.654 ug/l
RT: 10.06 min Scan# 2634
Delta R.T. 0.00 min
Lab File: VN061344.D
Acq: 7 May 2020 19:12




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 98 Resp: 216950
Ion Ratio Lower Upper
98 100
100 65.3 53.4 80.0

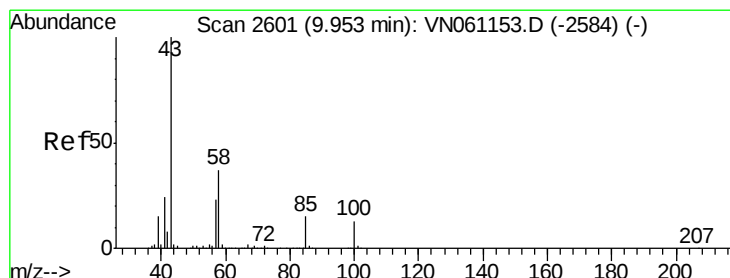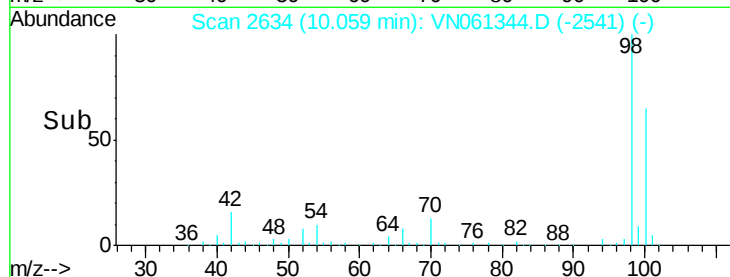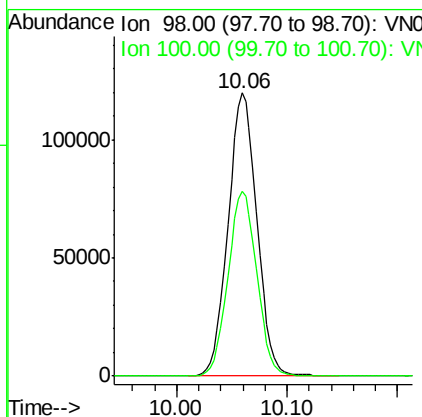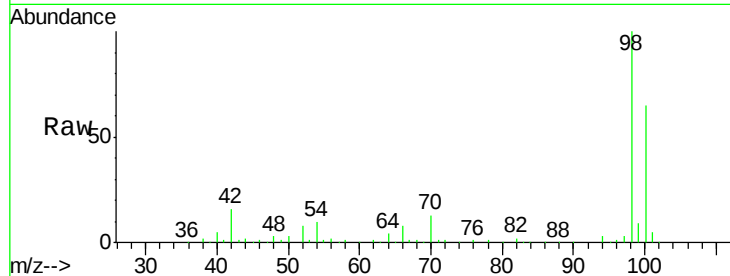

#51
4-Methyl-2-Pentanone
Concen: 0.536 ug/l
RT: 9.99 min Scan# 2613
Delta R.T. 0.04 min
Lab File: VN061344.D
Acq: 7 May 2020 19:12

Tgt Ion: 43 Resp: 1050
Ion Ratio Lower Upper
43 100
58 0.0 29.1 43.7#

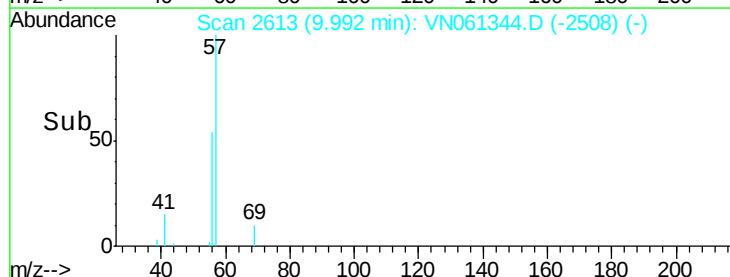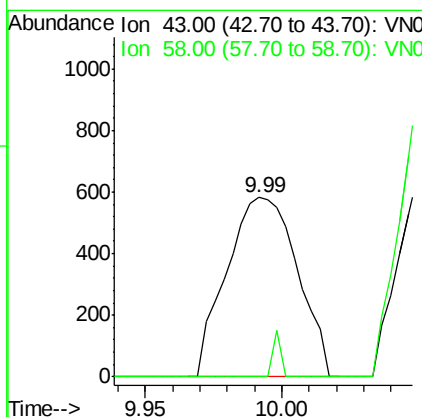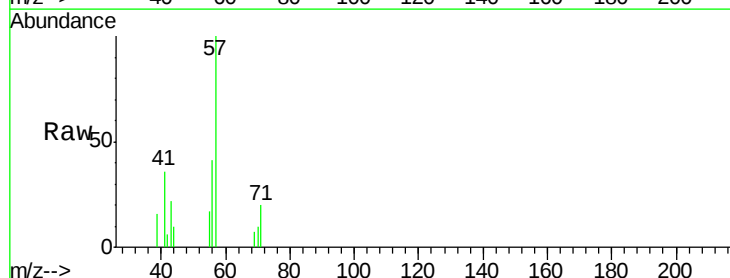







#55
 1,1,2-Trichloroethane
 Concen: 1.324 ug/l
 RT: 10.50 min Scan# 2771
 Delta R.T. -0.03 min
 Lab File: VN061344.D
 Acq: 7 May 2020 19:12

Instrument :
 MSVOA_N
 ClientSampled :

Tot Ion: 97 Resp: 1622
 Ion Ratio Lower Upper
 97 100
 83 0.0 70.6 106.0#
 85 0.0 46.4 69.6#
 99 0.0 50.6 75.8#

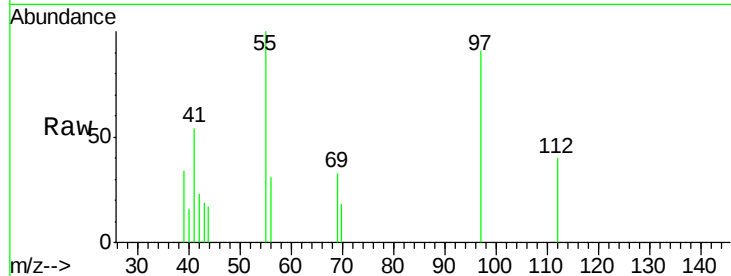


Abundance Ion 96.90 (96.60 to 97.60): VN0
 Ion 82.90 (82.60 to 83.60): VN0
 Ion 84.90 (84.60 to 85.60): VN0
 Ion 98.90 (98.60 to 99.60): VN0

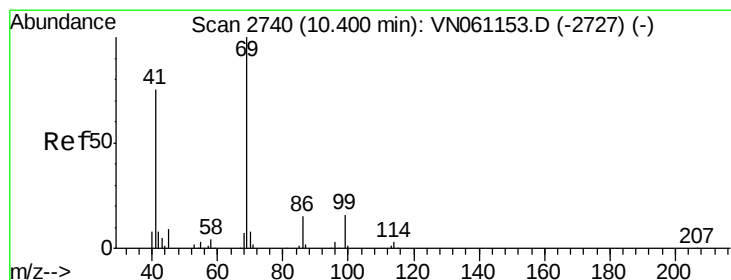
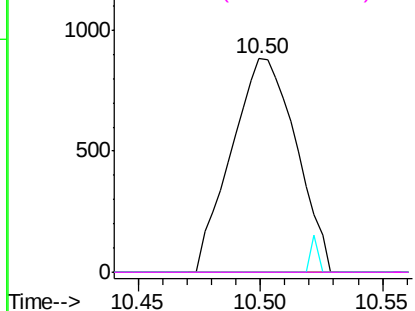



#56
 Ethyl methacrylate
 Concen: 3.134 ug/l
 RT: 10.40 min Scan# 2741
 Delta R.T. 0.00 min
 Lab File: VN061344.D
 Acq: 7 May 2020 19:12

Tgt Ion: 69 Resp: 918
 Ion Ratio Lower Upper
 69 100
 41 201.0 60.3 90.5#
 39 110.7 35.9 53.9#



Abundance Ion 69.00 (68.70 to 69.70): VN0
 Ion 41.00 (40.70 to 41.70): VN0
 Ion 39.00 (38.70 to 39.70): VN0



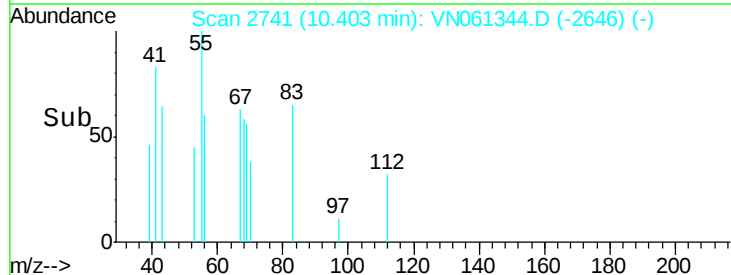
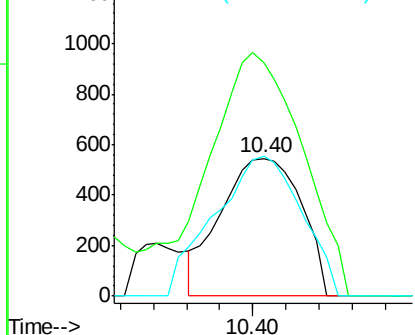




#59
2-Hexanone
Concen: 0.234 ug/l
RT: 10.68 min Scan# 2828
Delta R.T. -0.04 min
Lab File: VN061344.D
Acq: 7 May 2020 19:12




Instrument :
MSVOA_N
ClientSampleId :


Tot Ion: 43 Resp: 333
Ion Ratio Lower Upper
43 100
58 0.0 25.4 76.4#

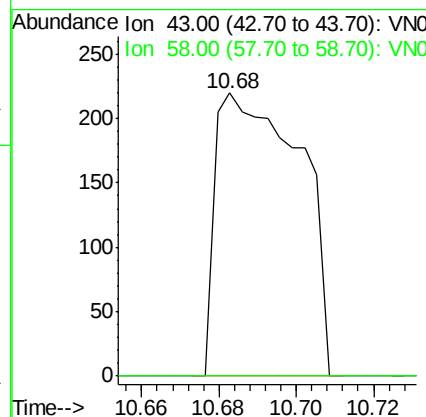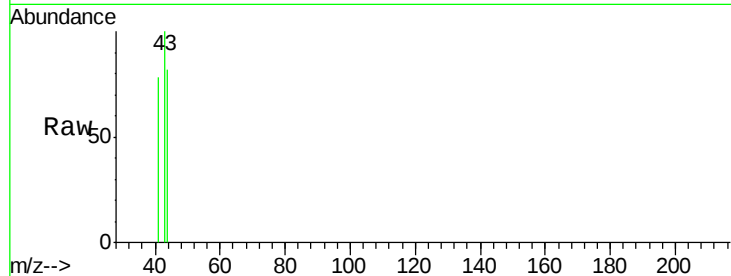

#62
4-Bromofluorobenzene
Concen: 52.437 ug/l
RT: 12.38 min Scan# 3355
Delta R.T. 0.00 min
Lab File: VN061344.D
Acq: 7 May 2020 19:12

Tgt Ion: 95 Resp: 81306
Ion Ratio Lower Upper
95 100
174 73.9 0.0 149.4
176 71.2 0.0 144.8

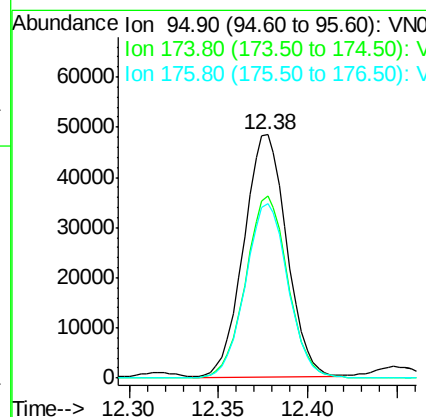

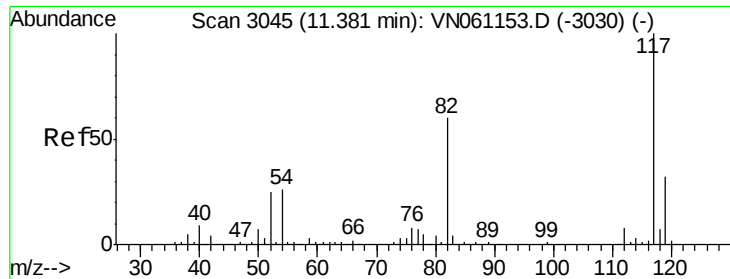

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 3045

Delta R.T. 0.00 min

Lab File: VN061344.D

Acq: 7 May 2020 19:12

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:117 Resp: 166494

Ion Ratio Lower Upper

117 100

82 59.5 47.8 71.8




119 31.8 25.8 38.6

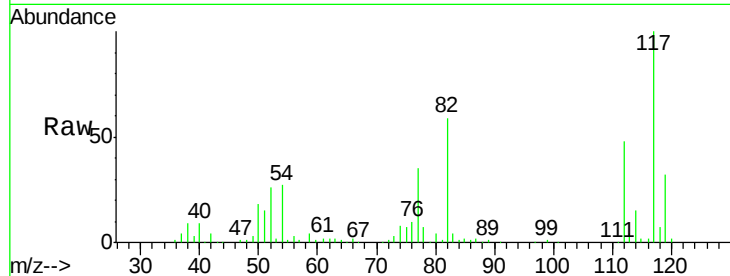

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 82.00 (81.70 to 82.70): VN

Ion 118.90 (118.60 to 119.60): V

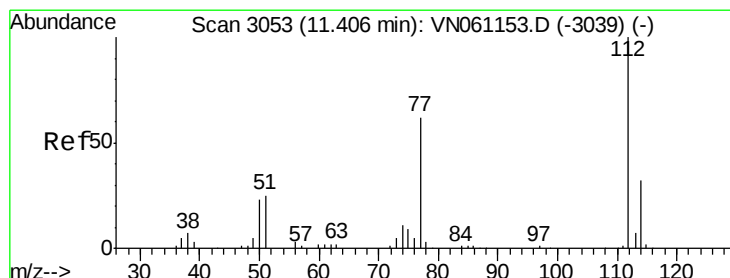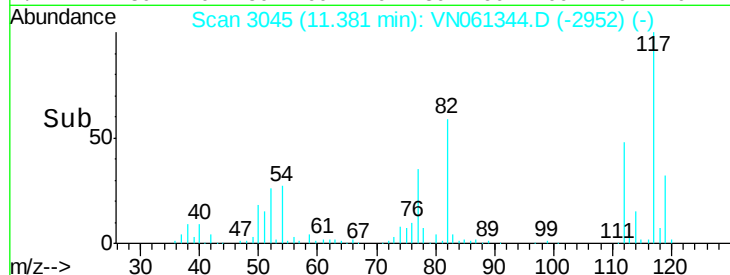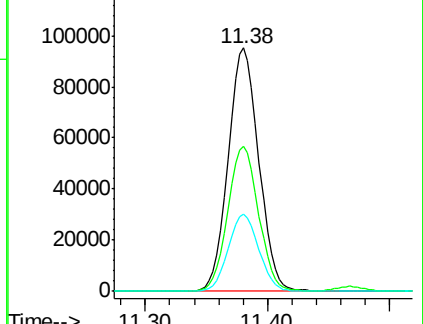

#65

Chlorobenzene

Concen: 297.279 ug/l

RT: 11.41 min Scan# 3053

Delta R.T. 0.00 min

Lab File: VN061344.D


Acq: 7 May 2020 19:12

Tgt Ion:112 Resp: 981822

Ion Ratio Lower Upper



112 100


114 32.0 25.4 38.2

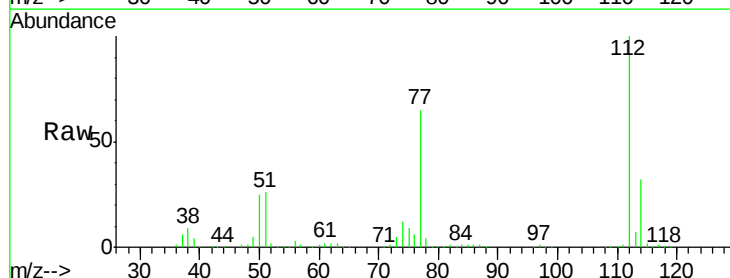

Abundance Ion 111.90 (111.60 to 112.60): V

Ion 113.90 (113.60 to 114.60): V

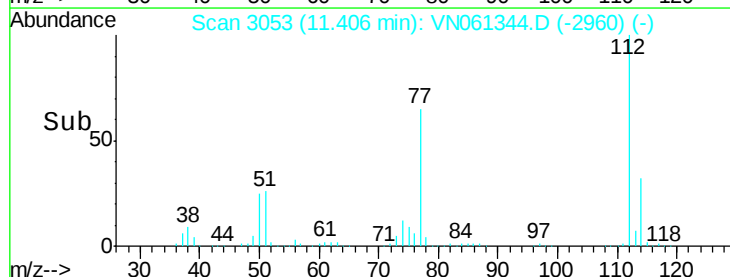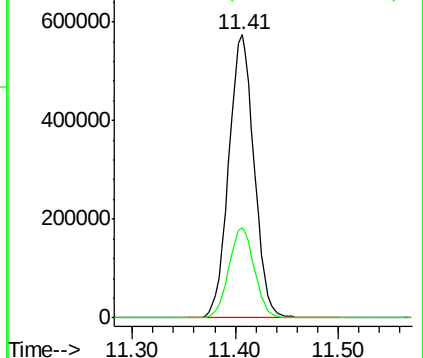



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3648

Delta R.T. 0.00 min

Lab File: VN061344.D

Acq: 7 May 2020 19:12

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:152 Resp: 74610

Ion Ratio Lower Upper

152 100

115 63.2 31.0 93.0




150 158.4 0.0 351.8



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

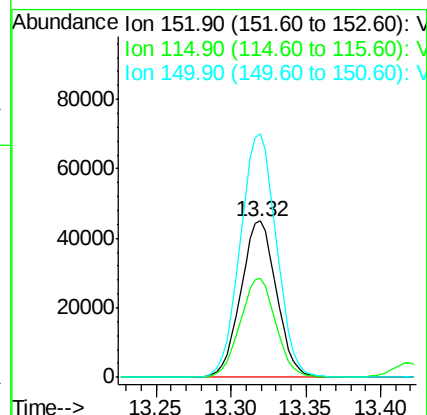

#73

Isopropylbenzene

Concen: 1.563 ug/l

RT: 12.22 min Scan# 3307

Delta R.T. 0.00 min

Lab File: VN061344.D


Acq: 7 May 2020 19:12

Tgt Ion:105 Resp: 8574

Ion Ratio Lower Upper



105 100


120 25.3 12.6 37.8



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V



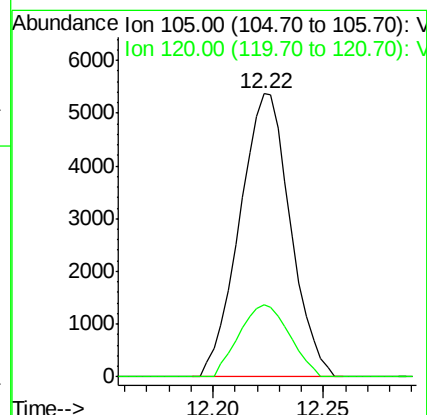





#76
 1,2,3-Trichloropropane
 Concen: 29.321 ug/l
 RT: 12.37 min Scan# 3354
 Delta R.T. -0.15 min
 Lab File: VN061344.D
 Acq: 7 May 2020 19:12




Instrument :
 MSVOA_N
 ClientSampled :


Tot Ion: 75 Resp: 46122
 Ion Ratio Lower Upper
 75 100
 77 1.3 0.0 0.0#

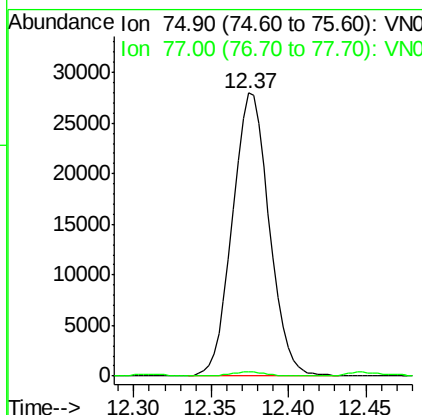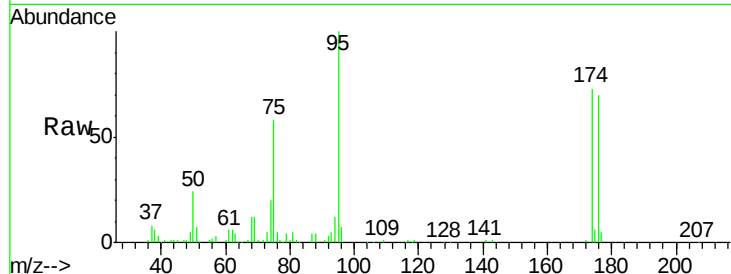

#81
 trans-1,4-Dichloro-2-butene
 Concen: 74.461 ug/l
 RT: 12.37 min Scan# 3354
 Delta R.T. 0.10 min
 Lab File: VN061344.D
 Acq: 7 May 2020 19:12

Tgt Ion: 75 Resp: 46122
 Ion Ratio Lower Upper
 75 100
 53 0.0 84.1 126.1#
 89 0.0 35.2 52.8#



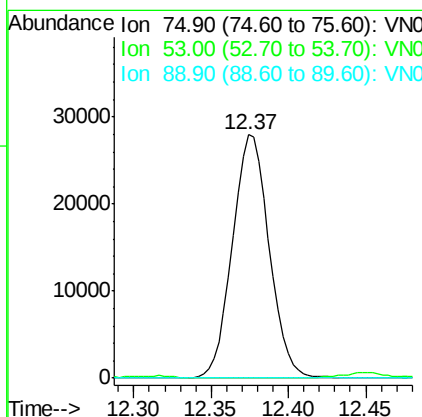
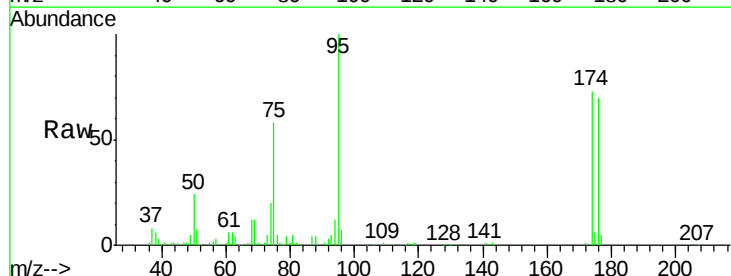




#83
tert-Butylbenzene
Concen: 4.406 ug/l
RT: 12.97 min Scan# 3539
Delta R.T. 0.00 min
Lab File: VN061344.D
Acq: 7 May 2020 19:12




Instrument :
MSVOA_N
ClientSampled :


Tot Ion:119 Resp: 16865
Ion Ratio Lower Upper
119 100
91 77.3 34.8 104.4
134 24.4 12.9 38.7

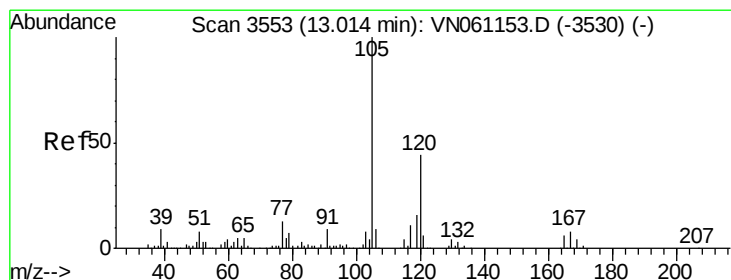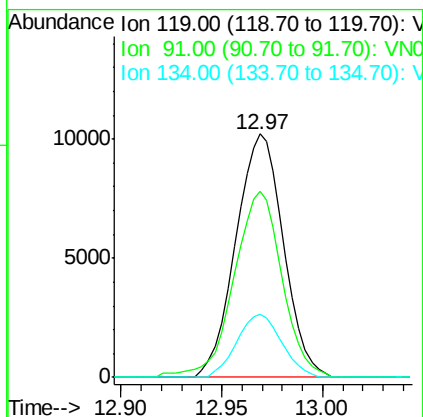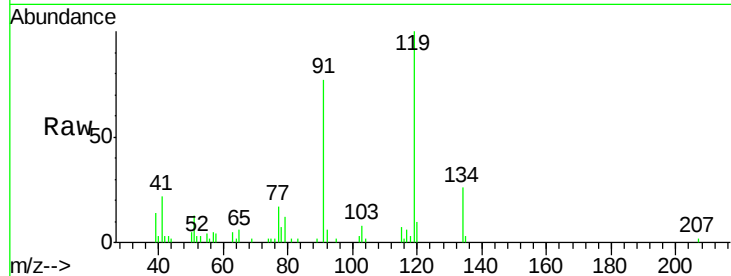

#84
1,2,4-Trimethylbenzene
Concen: 4.045 ug/l
RT: 13.15 min Scan# 3595
Delta R.T. 0.14 min
Lab File: VN061344.D
Acq: 7 May 2020 19:12

Tgt Ion:105 Resp: 18921
Ion Ratio Lower Upper
105 100
120 0.0 22.2 66.6#


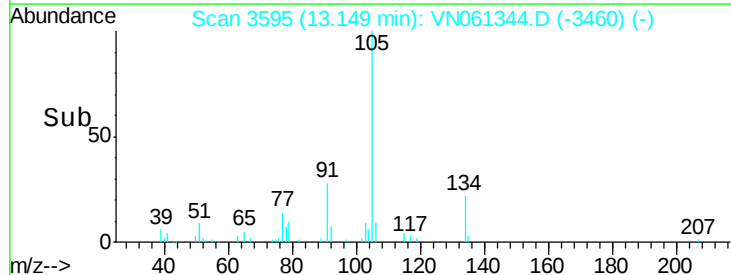
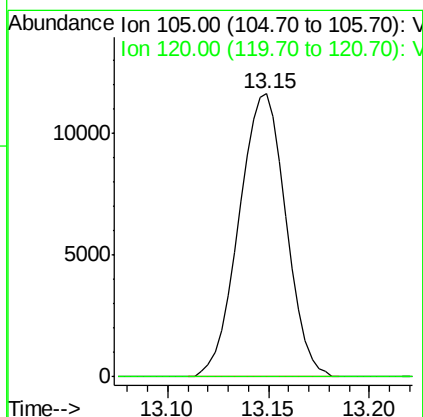





#85
 sec-Butylbenzene
 Concen: 3.626 ug/l
 RT: 13.15 min Scan# 3595
 Delta R.T. 0.00 min
 Lab File: VN061344.D
 Acq: 7 May 2020 19:12




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion:105 Resp: 18921
 Ion Ratio Lower Upper
 105 100
 134 40.0 9.6 28.8#

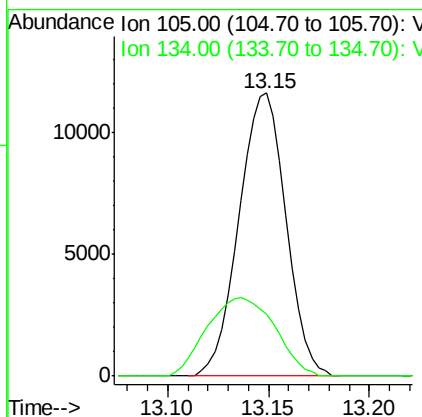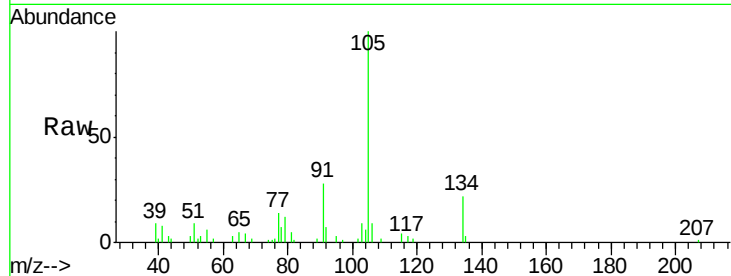

#86
 p-Isopropyltoluene
 Concen: 15.158 ug/l
 RT: 13.42 min Scan# 3679
 Delta R.T. 0.15 min
 Lab File: VN061344.D
 Acq: 7 May 2020 19:12

Tgt Ion:119 Resp: 71275
 Ion Ratio Lower Upper
 119 100
 134 26.3 12.6 37.6
 91 27.2 12.7 38.0

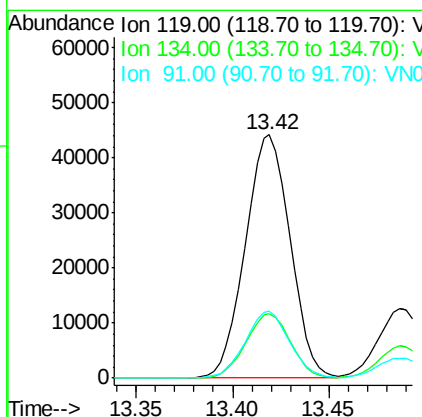



#87

1,3-Dichlorobenzene

Concen: 0.301 ug/l

RT: 13.26 min Scan# 3630

Delta R.T. 0.00 min


Lab File: VN061344.D

Acq: 7 May 2020 19:12

Instrument :

MSVOA_N

ClientSampled :

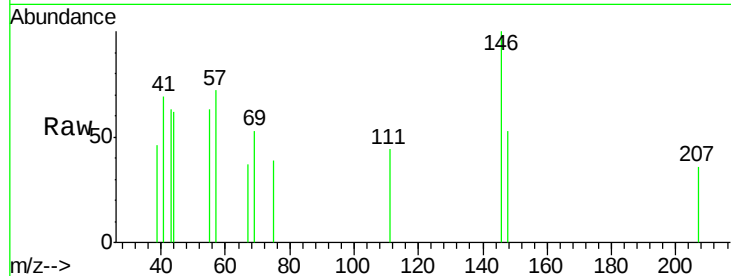




Tot Ion:146 Resp: 701

Ion Ratio Lower Upper

146 100

111 59.3 20.7 62.1

148 51.4 31.8 95.3

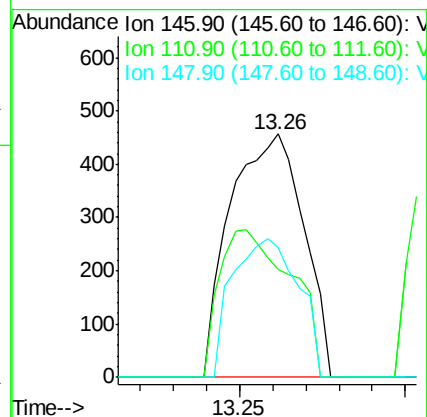

#88

1,4-Dichlorobenzene

Concen: 0.294 ug/l

RT: 13.26 min Scan# 3630

Delta R.T. -0.08 min

Lab File: VN061344.D

Acq: 7 May 2020 19:12




Tgt Ion:146 Resp: 701


Ion Ratio Lower Upper

146 100

111 59.3 20.4 61.3

148 51.4 31.9 95.7

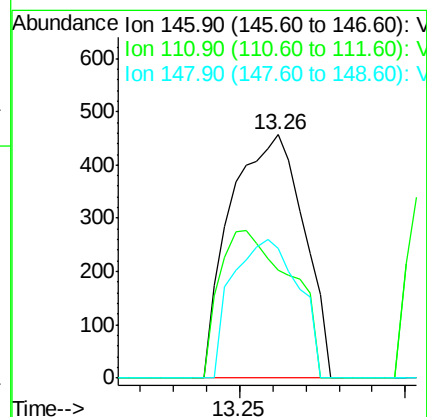



#89

n-Butylbenzene

Concen: 0.295 ug/l

RT: 13.57 min Scan# 3725

Delta R.T. -0.02 min

Lab File: VN061344.D

Acq: 7 May 2020 19:12

Instrument :

MSVOA_N

ClientSampled :





Tot Ion: 91 Resp: 1270

Ion Ratio Lower Upper

91 100

92 5.0 26.8 80.3#

134 71.7 11.9 35.5#

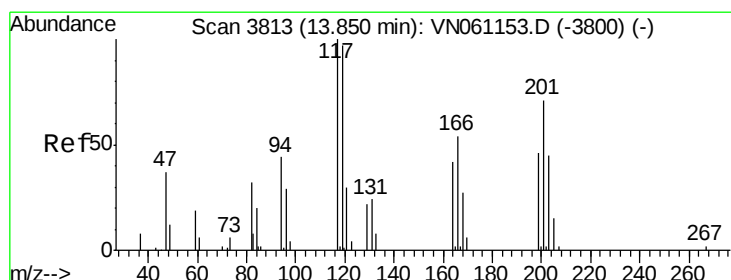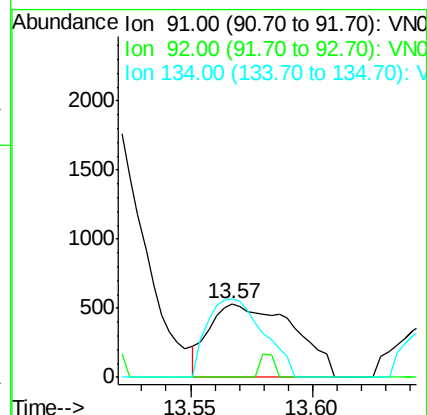

#90

Hexachloroethane

Concen: 48.927 ug/l

RT: 13.92 min Scan# 3835

Delta R.T. 0.07 min

Lab File: VN061344.D




Acq: 7 May 2020 19:12


Tgt Ion: 117 Resp: 23902

Ion Ratio Lower Upper

117 100

201 0.0 35.5 106.7#

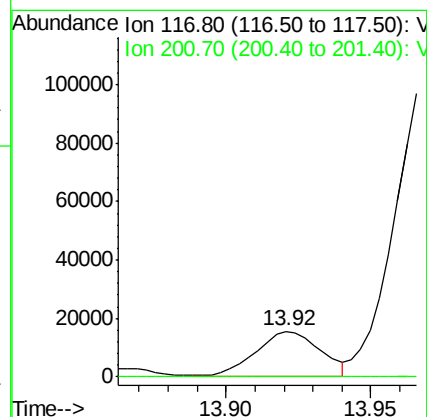



#92

1,2-Dibromo-3-Chloropropane

Concen: 0.371 ug/l

RT: 14.18 min Scan# 3916

Delta R.T. -0.06 min


Lab File: VN061344.D

Acq: 7 May 2020 19:12

Instrument :

MSVOA_N

ClientSampleId :



Tot Ion: 75 Resp: 134

Ion Ratio Lower Upper

75 100

155 0.0 36.5 109.7#

157 0.0 46.6 139.7#

Abundance Ion 74.90 (74.60 to 75.60): VN061344.D (-3843) (-)

Ion 154.80 (154.50 to 155.50): VN061344.D (-3843) (-)

Ion 156.80 (156.50 to 157.50): VN061344.D (-3843) (-)

