

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
 Data File : VN067024.D
 Acq On : 6 May 2021 21:12
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: May 07 06:59:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri May 07 06:53:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	7.115	128	79995	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.520	114	405190	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.352	117	326037	30.00	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	7.954	65	206869	29.51	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	98.37%
60) 4-Bromofluorobenzene	12.355	95	96595	17.81	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	59.37%#
63) Toluene-d8	10.030	98	518447	32.10	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	107.00%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	1.834	85	1203	0.22	ug/l	93
3) Chloromethane	2.035	50	3092	0.37	ug/l	96
5) Bromomethane	2.523	94	2743	0.61	ug/l	87
13) Acrolein	3.545	56	1121	1.06	ug/l #	40
15) Acetone	3.760	58	185	0.25	ug/l #	1
16) Carbon Disulfide	3.988	76	13799	0.92	ug/l #	92
23) tert-Butyl Alcohol	4.709	59	341	0.33	ug/l #	100
37) Trichloroethene	8.770	130	1767	0.36	ug/l #	74
38) Methylcyclohexane	9.016	83	1745	0.25	ug/l	68
45) 1,4-Dioxane	9.129	88	169	2.18	ug/l #	83
46) Methyl methacrylate	9.148	41	1107	0.22	ug/l #	57
47) n-amyl Acetate	11.792	43	62	2.57	ug/l #	49
50) 1,1,2-Trichloroethane	10.499	97	1180	0.22	ug/l #	77
58) 4-Methyl-2-Pentanone	9.931	43	10267	1.68	ug/l #	94
61) Tetrachloroethene	10.575	164	1890	0.51	ug/l #	81
62) Toluene	10.097	91	4658	0.23	ug/l	96
64) Chlorobenzene	11.379	112	4185	0.36	ug/l	99
66) Ethyl Benzene	11.468	91	4401	0.22	ug/l	100
70) Isopropylbenzene	12.205	105	5212	0.27	ug/l	96
72) 1,2,3-Trichloropropane	12.358	75	55948	8.64	ug/l	1
73) Bromobenzene	12.473	156	955	0.20	ug/l	8
77) t-1,4-Dichloro-2-butene	12.200	75	93	7.41	ug/l #	16
79) tert-butylbenzene	12.943	119	5961	0.41	ug/l	84
81) sec-Butylbenzene	13.128	105	7114	0.37	ug/l	81
82) p-Isopropyltoluene	13.251	119	6257	0.40	ug/l #	57
85) n-Butylbenzene	13.589	91	6438	0.52	ug/l	90
86) Hexachloroethane	13.814	117	1198	0.35	ug/l	85
88) 1,2-Dibromo-3-Chloropr...	14.230	75	363	0.26	ug/l #	34
89) 1,2,4-Trichlorobenzene	14.866	180	26098	6.34	ug/l	94
90) Hexachlorobutadiene	14.957	225	4195	1.51	ug/l	86
91) Naphthalene	15.080	128	147022	13.03	ug/l	98
92) 1,2,3-Trichlorobenzene	15.260	180	32180	7.47	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
Data File : VN067024.D
Acq On : 6 May 2021 21:12
Operator : JC/MD
Sample : IBLK
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: May 07 06:59:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri May 07 06:53:40 2021
Response via : Initial Calibration




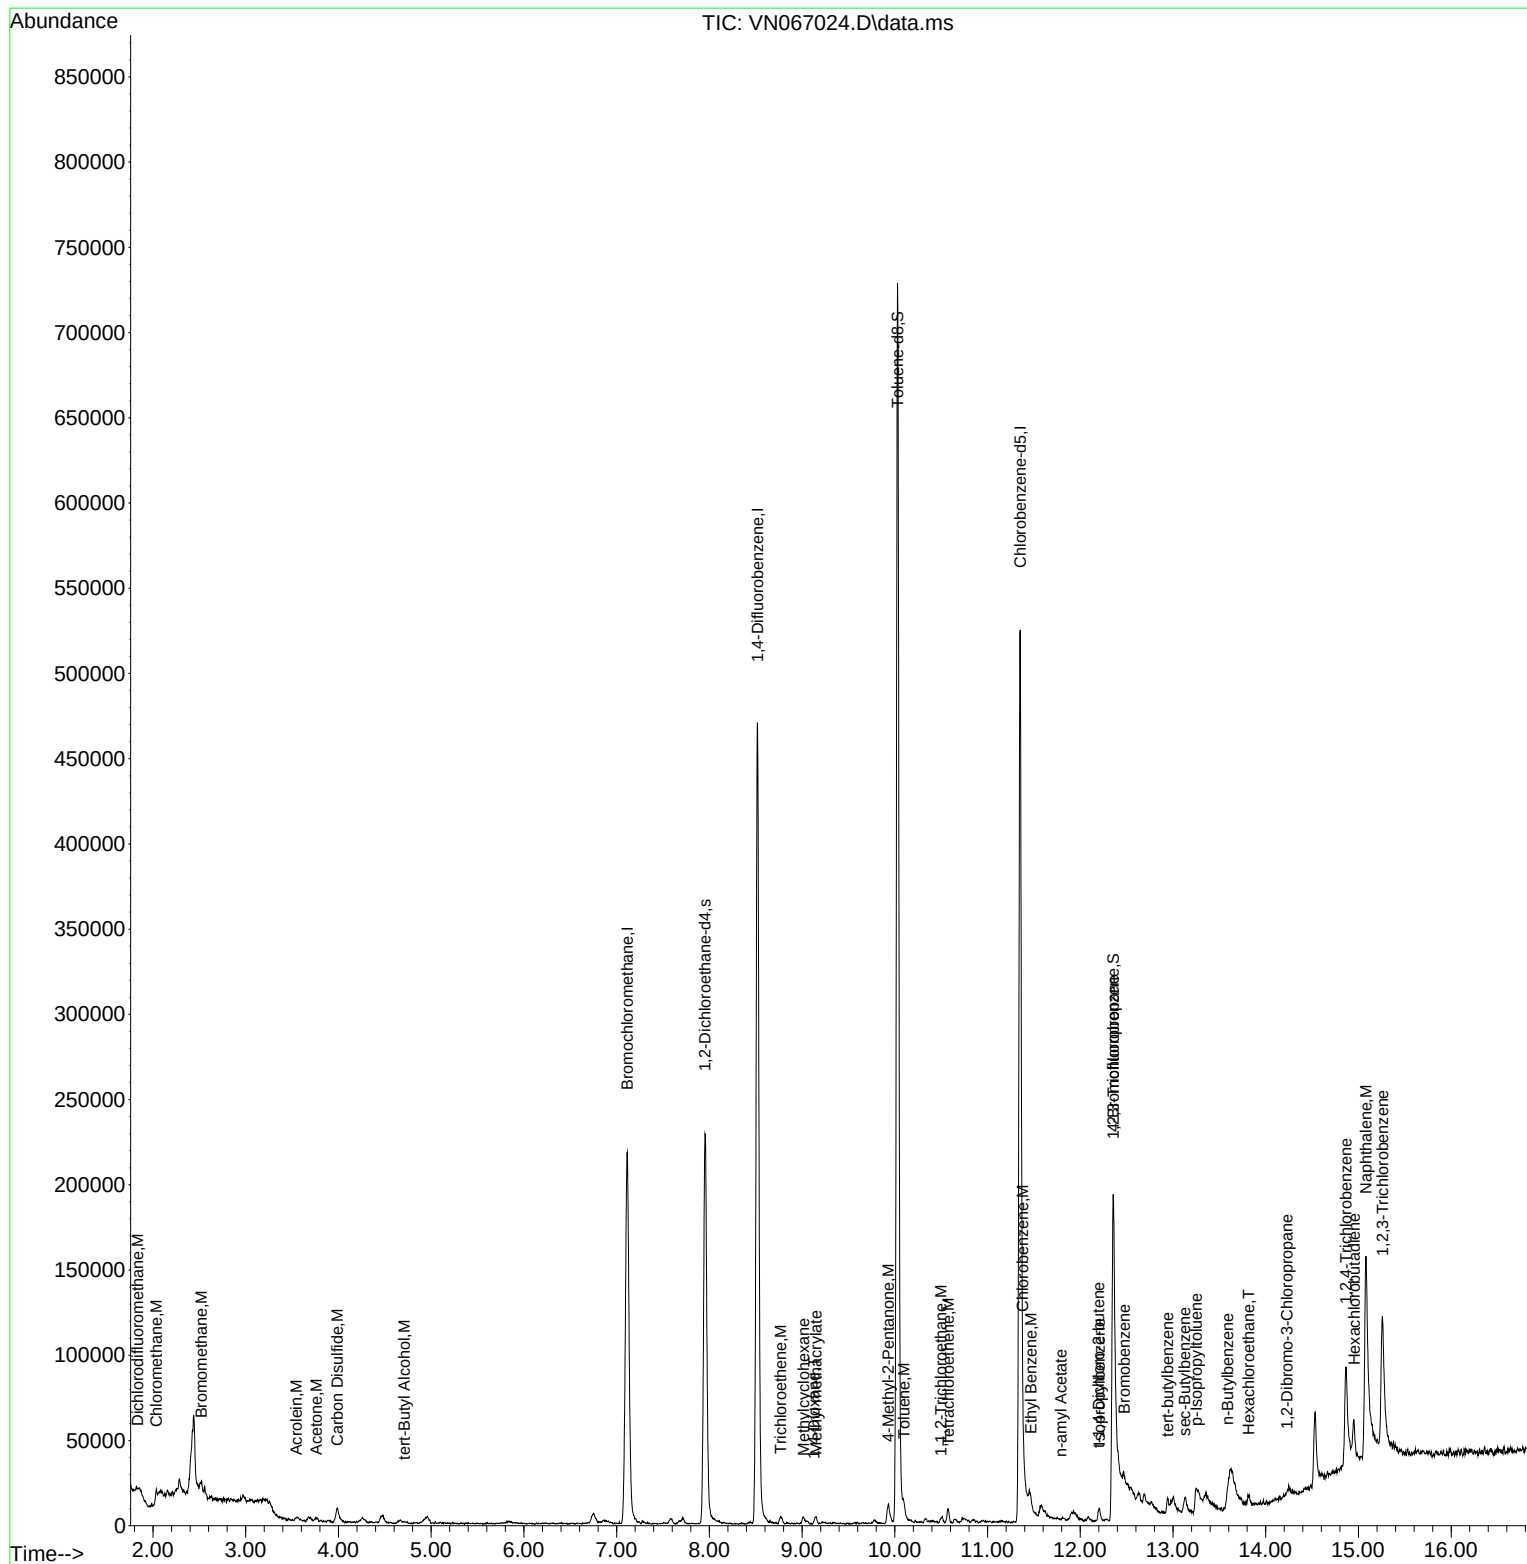




#1
Bromochloromethane
Concen: 30.00 ug/l
RT: 7.115 min Scan# 1998
Delta R.T. 0.003 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:128 Resp: 79995
Ion Ratio Lower Upper
128 100
49 192.4 0.0 486.3
130 127.7 0.0 326.0

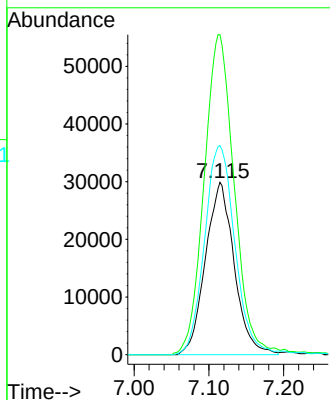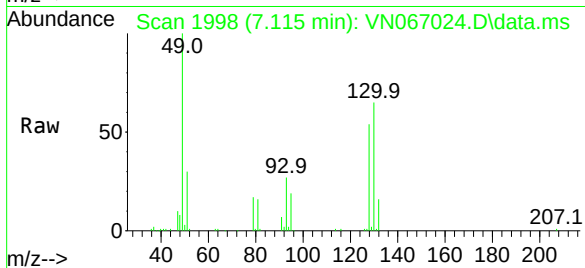

#2
Dichlorodifluoromethane
Concen: 0.22 ug/l
RT: 1.834 min Scan# 29
Delta R.T. 0.000 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion: 85 Resp: 1203
Ion Ratio Lower Upper
85 100
87 28.5 16.1 48.3


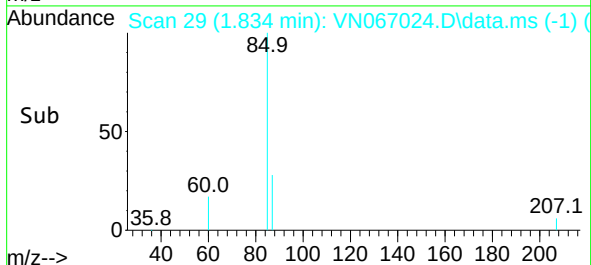
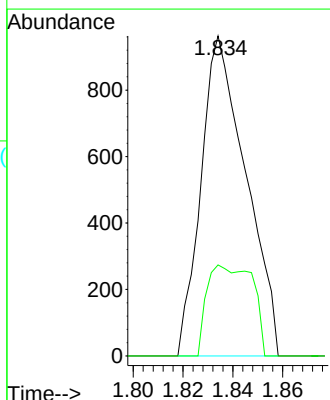
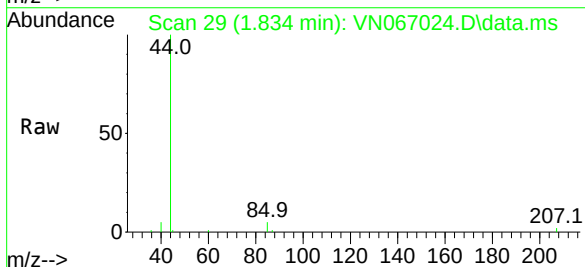




#3
Chloromethane
Concen: 0.37 ug/l
RT: 2.035 min Scan# 104
Delta R.T. 0.000 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampled :
IBLK


Tgt Ion: 50 Resp: 3092
Ion Ratio Lower Upper
50 100
52 30.0 25.9 38.9

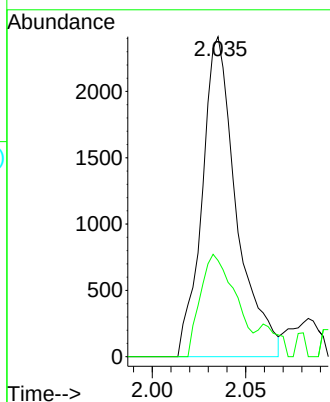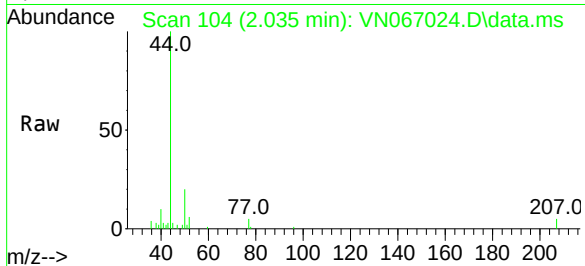

#5
Bromomethane
Concen: 0.61 ug/l
RT: 2.523 min Scan# 286
Delta R.T. 0.022 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12


Tgt Ion: 94 Resp: 2743
Ion Ratio Lower Upper
94 100
96 106.9 75.4 113.2

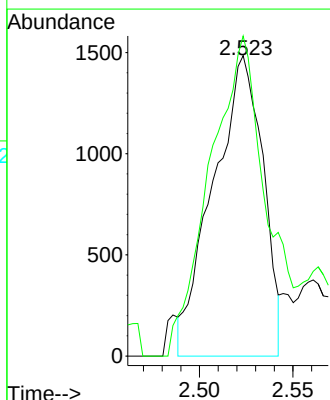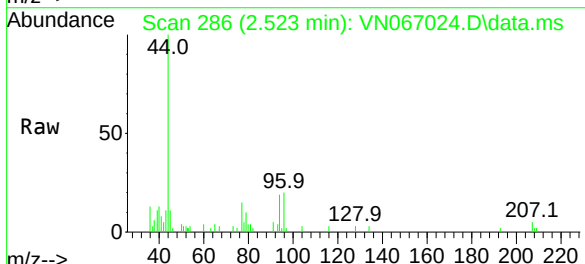






#13
Acrolein
Concen: 1.06 ug/l
RT: 3.545 min Scan# 667
Delta R.T. 0.000 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Instrument :
MSVOA_N
ClientSampled :
IBLK







Tgt Ion: 56 Resp: 1121
Ion Ratio Lower Upper
56 100
55 120.4 56.6 84.8#



#15
Acetone
Concen: 0.25 ug/l
RT: 3.760 min Scan# 747
Delta R.T. 0.006 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12


Tgt Ion: 58 Resp: 185
Ion Ratio Lower Upper
58 100
43 57.5 235.0 352.6#

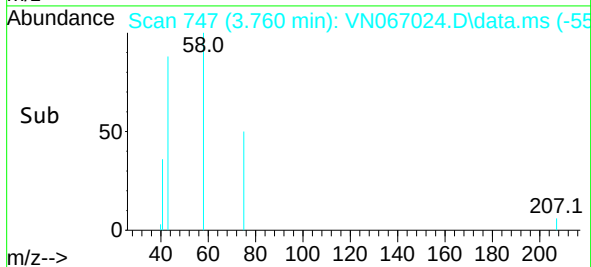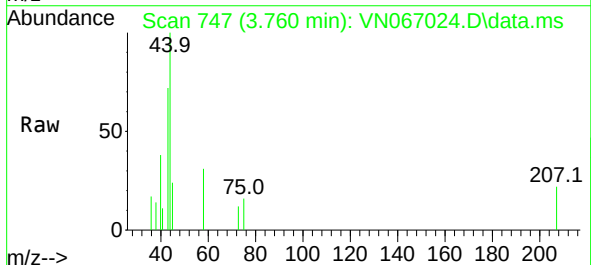






#16
Carbon Disulfide
Concen: 0.92 ug/l
RT: 3.988 min Scan# 832
Delta R.T. 0.008 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Instrument :
MSVOA_N
ClientSampleId :
IBLK



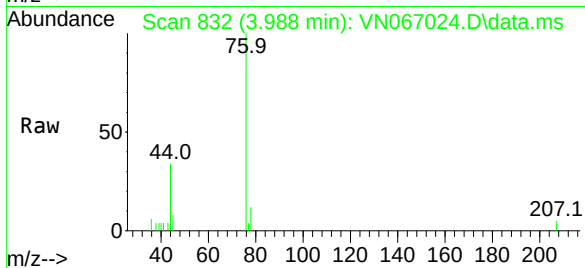



Tgt Ion: 76 Resp: 13799
Ion Ratio Lower Upper
76 100
78 12.3 7.5 11.3#

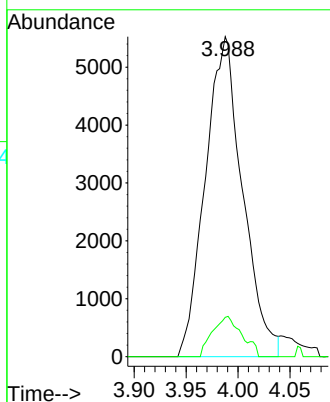

#23
tert-Butyl Alcohol
Concen: 0.33 ug/l
RT: 4.709 min Scan# 1101
Delta R.T. -0.002 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion: 59 Resp: 341
Ion Ratio Lower Upper
59 100
52 0.0 0.0 0.0

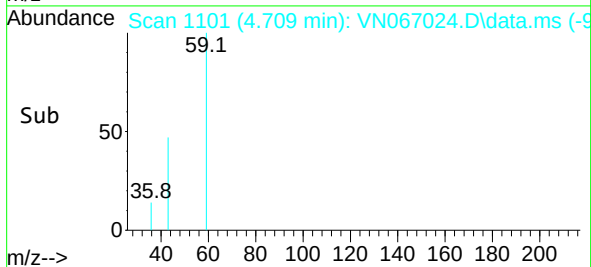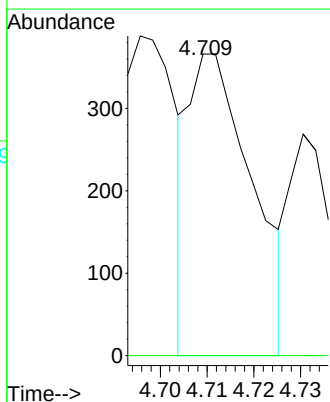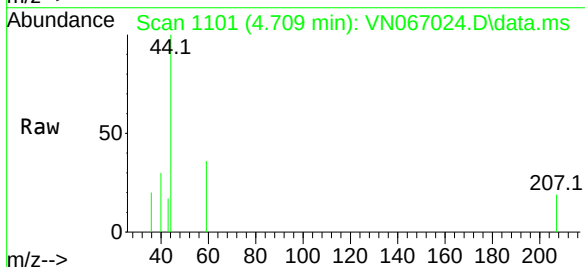



#27

1,2-Dichloroethane-d4

Concen: 29.51 ug/l

RT: 7.954 min Scan# 2311

Delta R.T. 0.000 min

Lab File: VN067024.D





Acq: 6 May 2021 21:12

Tgt Ion: 65 Resp: 206869

Ion Ratio Lower Upper

65 100

67 52.7 41.6 62.4

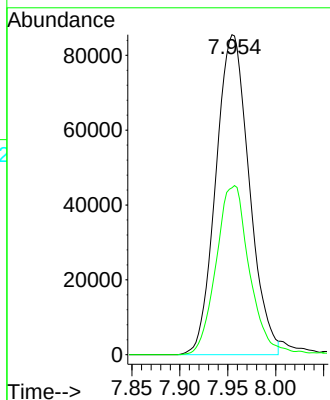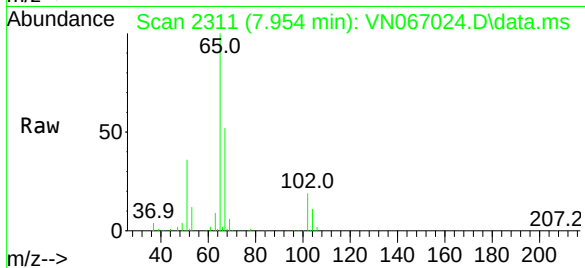

#28

1,4-Difluorobenzene

Concen: 30.00 ug/l

RT: 8.520 min Scan# 2522

Delta R.T. 0.000 min

Lab File: VN067024.D

Acq: 6 May 2021 21:12




Tgt Ion: 114 Resp: 405190


Ion Ratio Lower Upper

114 100

63 23.3 18.8 28.2

88 16.8 13.8 20.6

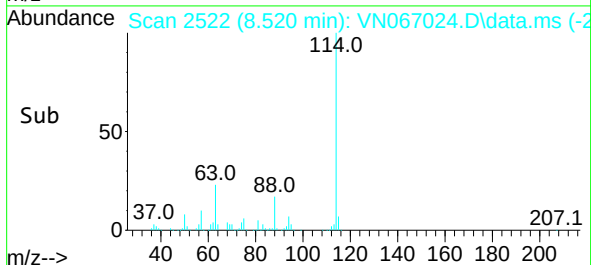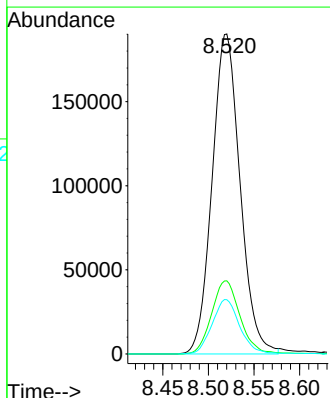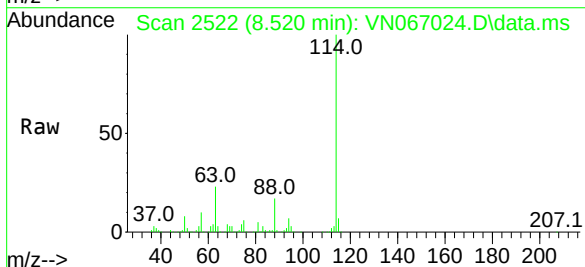

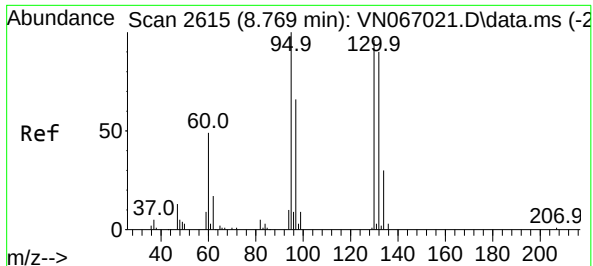

#37

Trichloroethene

Concen: 0.36 ug/l

RT: 8.770 min Scan# 2615

Delta R.T. 0.000 min

Lab File: VN067024.D

Acq: 6 May 2021 21:12

Instrument :

MSVOA_N

ClientSampled :





IBLK

Tgt Ion:130 Resp: 1767

Ion Ratio Lower Upper

130 100

95 78.1 83.5 125.3#

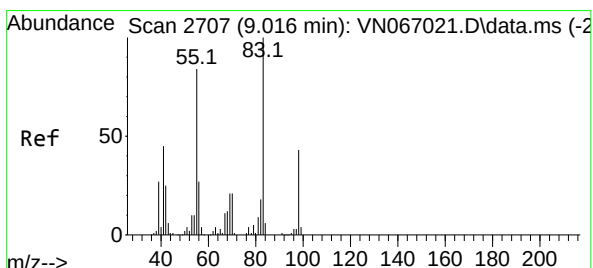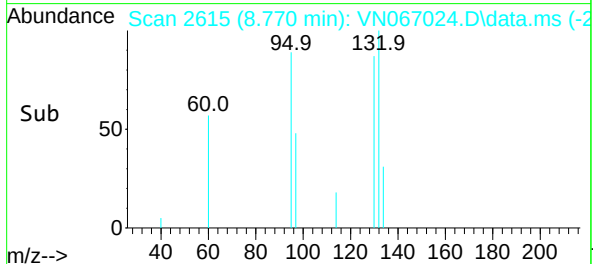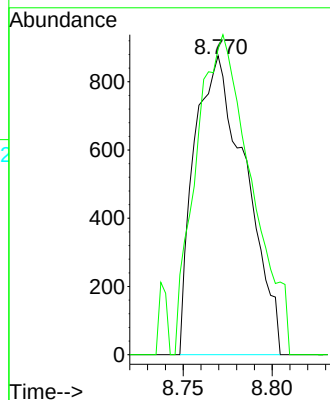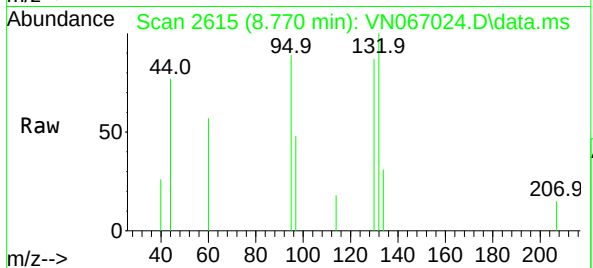

#38

Methylcyclohexane

Concen: 0.25 ug/l

RT: 9.016 min Scan# 2707

Delta R.T. 0.000 min

Lab File: VN067024.D

Acq: 6 May 2021 21:12




Tgt Ion: 83 Resp: 1745


Ion Ratio Lower Upper

83 100

55 57.5 43.1 129.3

98 22.2 22.0 66.0

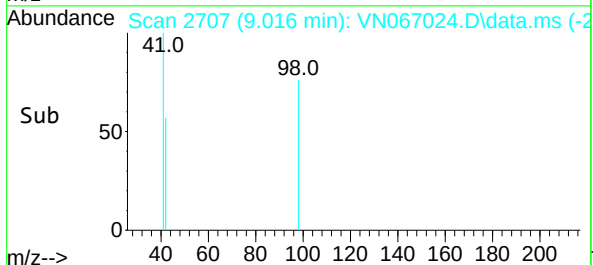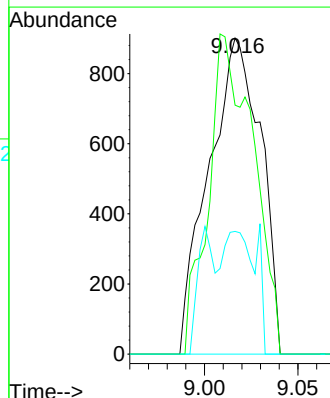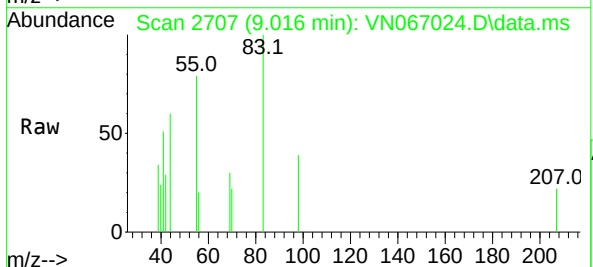

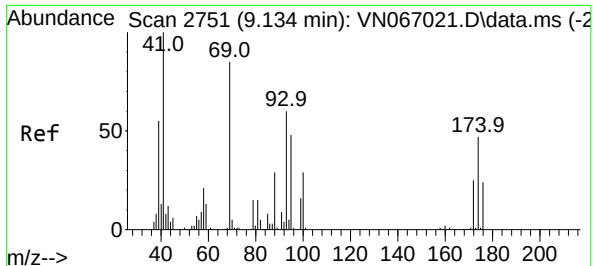

#45

1,4-Dioxane

Concen: 2.18 ug/l

RT: 9.129 min Scan# 2749





Delta R.T. -0.005 min

Lab File: VN067024.D

Acq: 6 May 2021 21:12

Tgt Ion: 88	Resp: 169
Ion Ratio	Lower Upper
88 100	
43 52.1	28.0 42.0#
58 88.8	62.8 94.2

Instrument :
MSVOA_N
ClientSampled :
IBLK

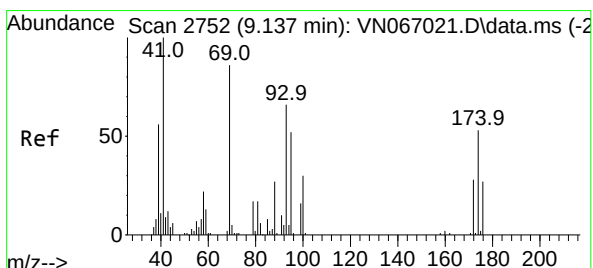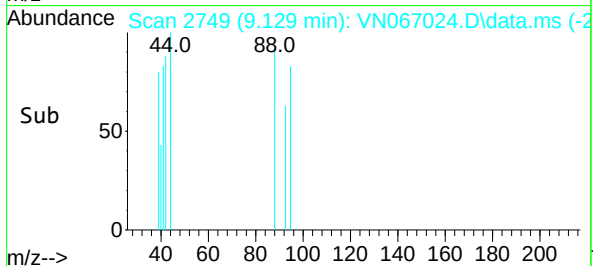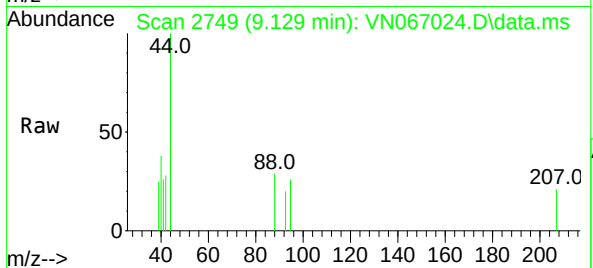

#46

Methyl methacrylate

Concen: 0.22 ug/l




RT: 9.148 min Scan# 2756


Delta R.T. 0.011 min

Lab File: VN067024.D

Acq: 6 May 2021 21:12

Tgt Ion: 41	Resp: 1107
Ion Ratio	Lower Upper
41 100	
69 59.2	42.7 128.1
39 8.1	28.1 84.2#


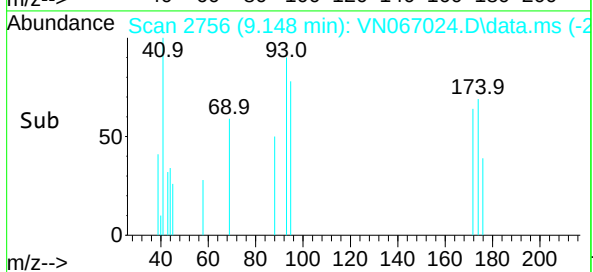

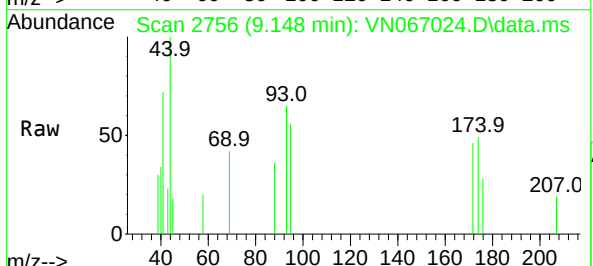




#47
n-amy1 Acetate
Concen: 2.57 ug/l
RT: 11.792 min Scan# 3742
Delta R.T. 0.006 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampled :
IBLK


Tgt Ion: 43 Resp: 62
Ion Ratio Lower Upper
43 100
55 0.0 21.1 31.7#



#50
1,1,2-Trichloroethane
Concen: 0.22 ug/l
RT: 10.499 min Scan# 3260
Delta R.T. -0.005 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion: 97 Resp: 1180
Ion Ratio Lower Upper
97 100
83 66.6 70.6 106.0#
85 73.1 45.6 68.4#
99 42.9 48.4 72.6#


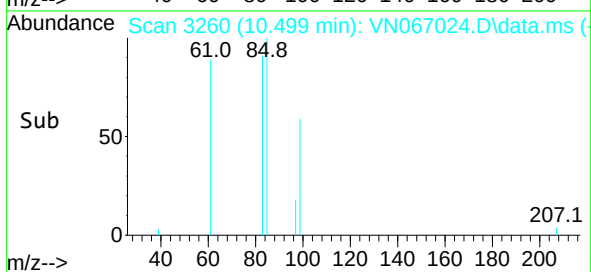






#57
Chlorobenzene-d5
Concen: 30.00 ug/l
RT: 11.352 min Scan# 3578
Delta R.T. 0.003 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:	117	Resp:	326037
Ion	Ratio	Lower	Upper
117	100		
82	61.2	49.3	73.9
119	31.6	25.5	38.3

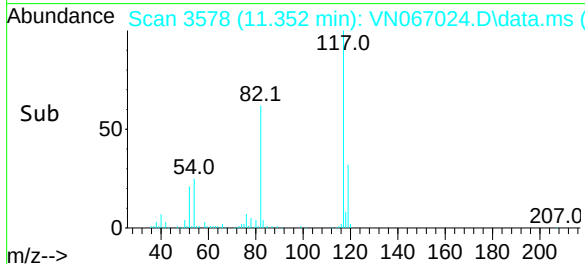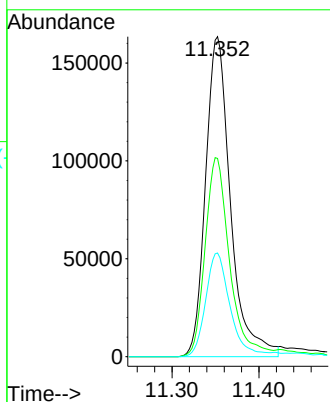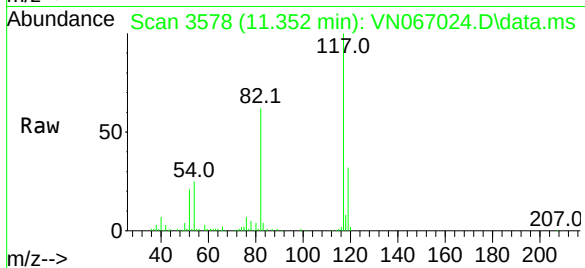

#58
4-Methyl-2-Pentanone
Concen: 1.68 ug/l
RT: 9.931 min Scan# 3048
Delta R.T. 0.008 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12


Tgt Ion:	43	Resp:	10267
Ion	Ratio	Lower	Upper
43	100		
58	35.3	30.4	45.6
85	12.1	13.4	20.0#

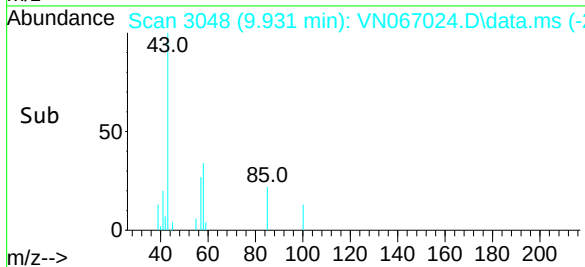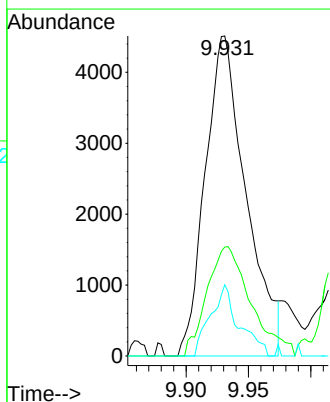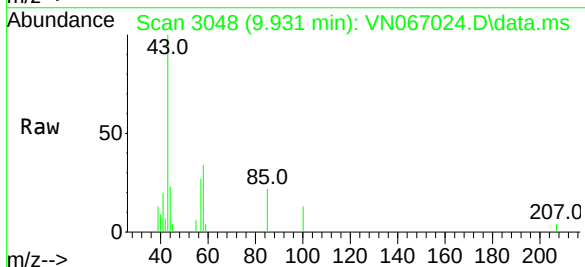



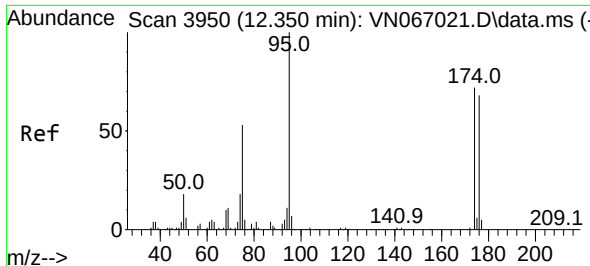


#60
4-Bromofluorobenzene
Concen: 17.81 ug/l
RT: 12.355 min Scan# 3952
Delta R.T. 0.005 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Instrument :
MSVOA_N
ClientSampled :
IBLK



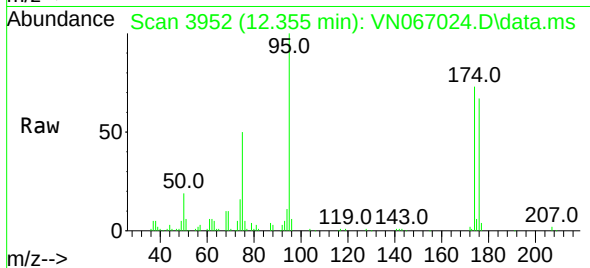



Tgt Ion: 95 Resp: 96595
Ion Ratio Lower Upper
95 100
174 80.1 57.2 85.8
176 75.9 54.5 81.7

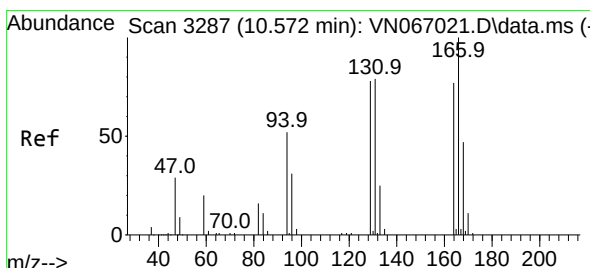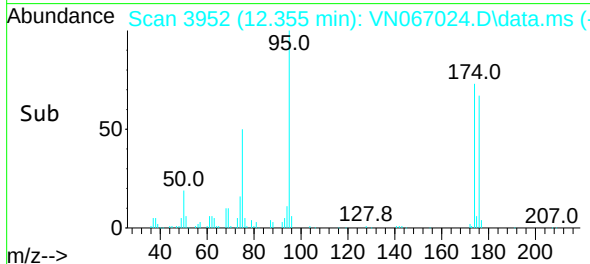

#61
Tetrachloroethene
Concen: 0.51 ug/l
RT: 10.575 min Scan# 3288
Delta R.T. 0.003 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion: 164 Resp: 1890
Ion Ratio Lower Upper
164 100
166 111.4 103.4 155.0
129 74.8 80.6 120.8#
131 84.7 81.9 122.9

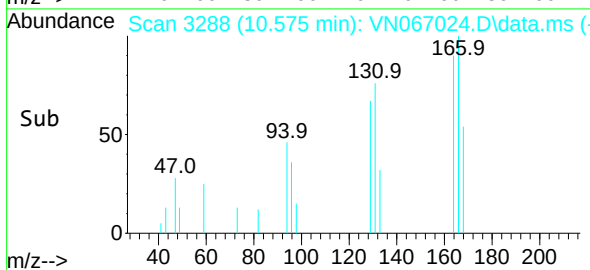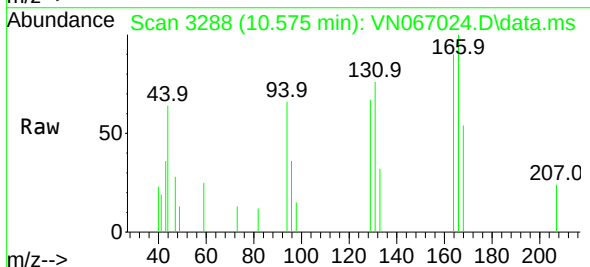

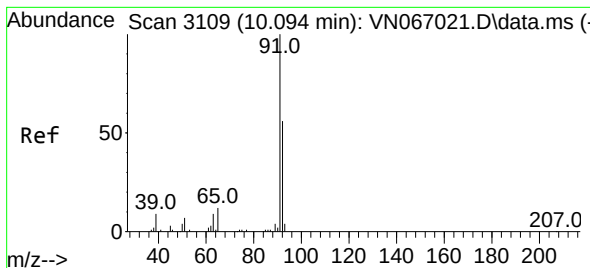

#62

Toluene

Concen: 0.23 ug/l

RT: 10.097 min Scan# 3110

Delta R.T. 0.003 min





Lab File: VN067024.D

Acq: 6 May 2021 21:12

Tgt Ion: 91 Resp: 4658

Ion	Ratio	Lower	Upper
91	100		
92	54.5	46.2	69.2

Instrument :
MSVOA_N
ClientSampled :
IBLK

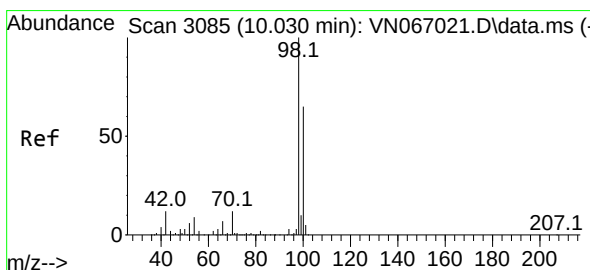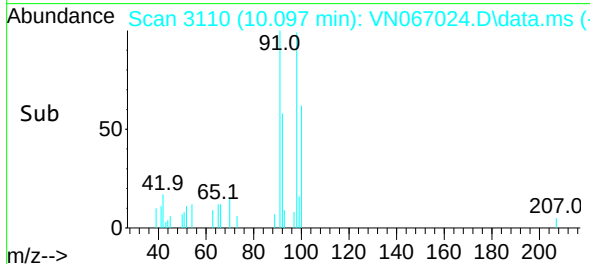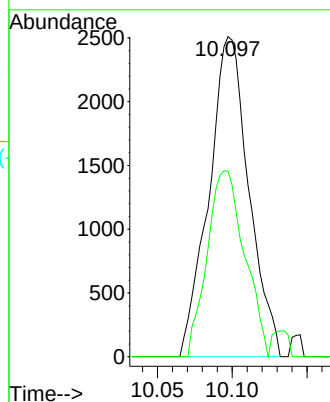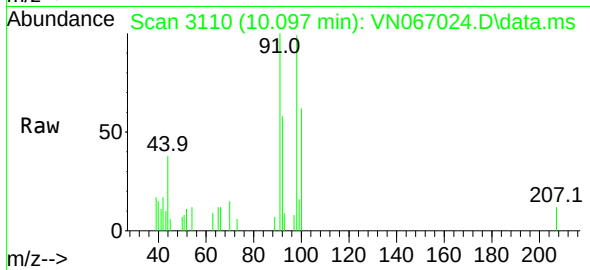

#63

Toluene-d8

Concen: 32.10 ug/l

RT: 10.030 min Scan# 3085




Delta R.T. 0.000 min


Lab File: VN067024.D

Acq: 6 May 2021 21:12

Tgt Ion: 98 Resp: 518447

Ion	Ratio	Lower	Upper
98	100		
100	63.5	51.1	76.7


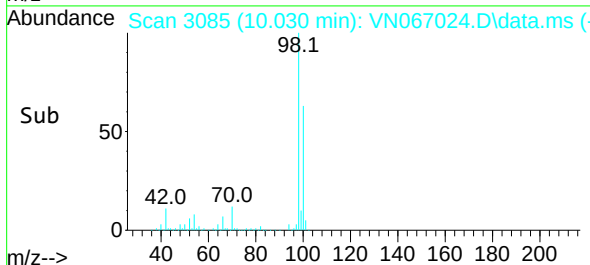
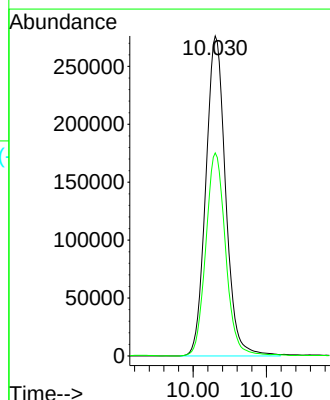
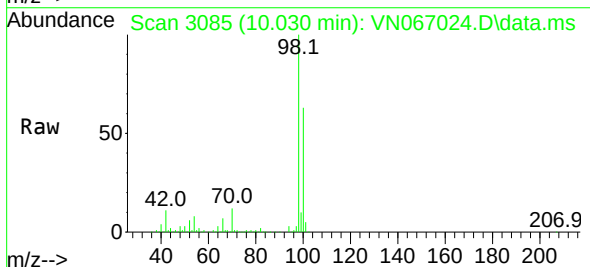


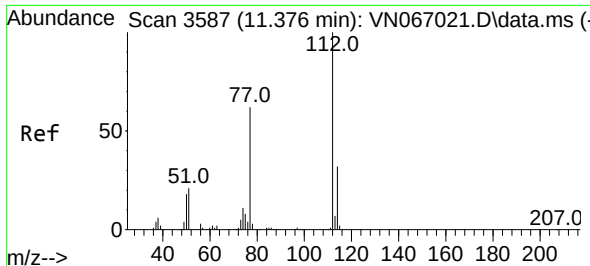

#64
Chlorobenzene
Concen: 0.36 ug/l
RT: 11.379 min Scan# 3588
Delta R.T. 0.003 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampled :
IBLK


Tgt Ion:112 Resp: 4185
Ion Ratio Lower Upper
112 100
114 31.2 25.2 37.8

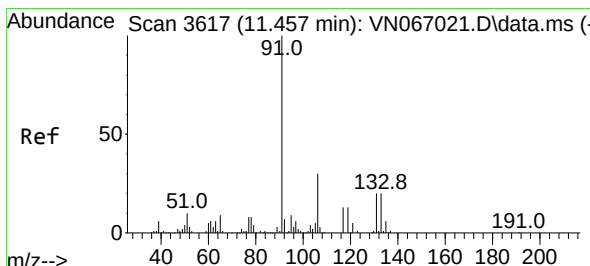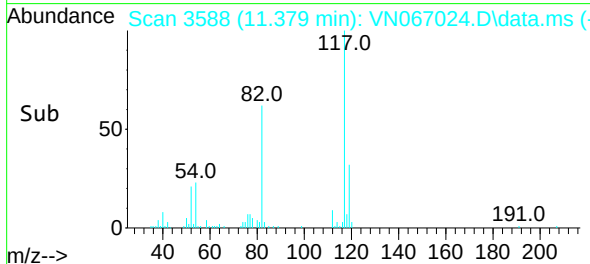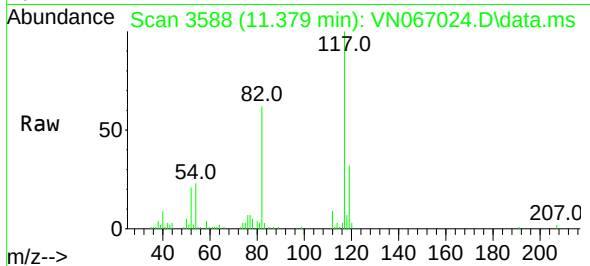

#66
Ethyl Benzene
Concen: 0.22 ug/l
RT: 11.468 min Scan# 3621
Delta R.T. 0.011 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion: 91 Resp: 4401
Ion Ratio Lower Upper
91 100
106 30.2 24.1 36.1


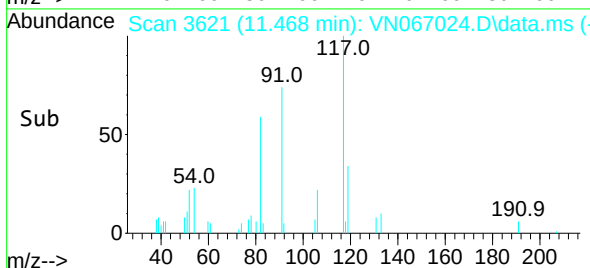

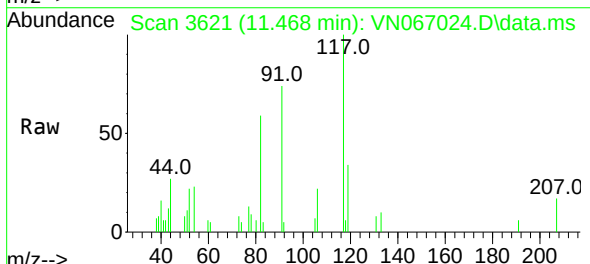




#70
Isopropylbenzene
Concen: 0.27 ug/l
RT: 12.205 min Scan# 3896
Delta R.T. 0.008 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampled :
IBLK


Tgt Ion:105 Resp: 5212
Ion Ratio Lower Upper
105 100
120 24.0 18.2 33.8



#72
1,2,3-Trichloropropane
Concen: 8.64 ug/l
RT: 12.358 min Scan# 3953
Delta R.T. -0.145 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion: 75 Resp: 55948
Ion Ratio Lower Upper
75 100
77 1.3 0.0 329.6


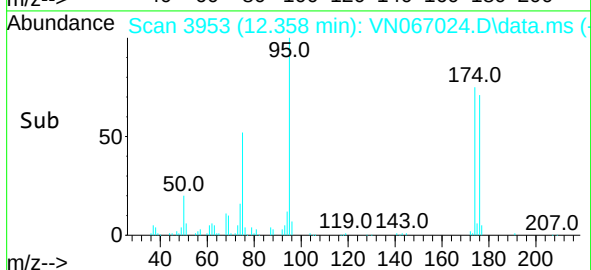






#73
Bromobenzene
Concen: 0.20 ug/l
RT: 12.473 min Scan# 3996
Delta R.T. 0.003 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampled :
IBLK


Tgt Ion:156 Resp: 955
Ion Ratio Lower Upper
156 100
77 36.5 0.0 448.2
158 57.9 0.0 192.4



#77
t-1,4-Dichloro-2-butene
Concen: 7.41 ug/l
RT: 12.200 min Scan# 3894
Delta R.T. -0.056 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion: 75 Resp: 93
Ion Ratio Lower Upper
75 100
53 0.0 43.1 129.4#
89 0.0 18.8 56.4#


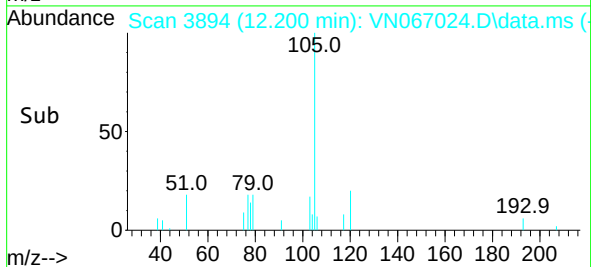

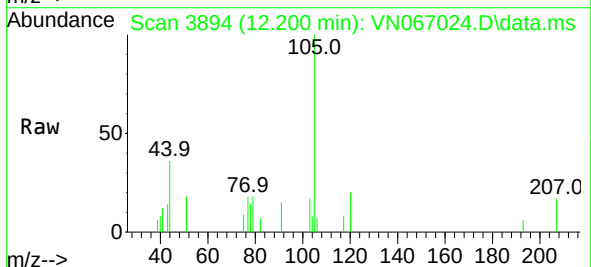




#79
tert-butylbenzene
Concen: 0.41 ug/l
RT: 12.943 min Scan# 4171
Delta R.T. 0.003 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampled :
IBLK


Tgt Ion:119 Resp: 5961
Ion Ratio Lower Upper
119 100
91 58.8 0.0 140.2
134 13.0 0.0 46.6

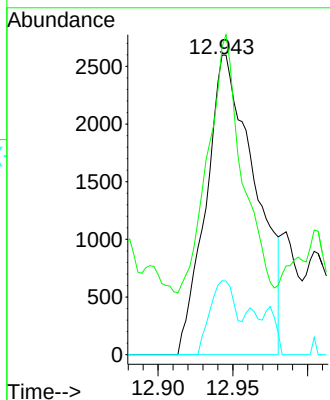

#81
sec-Butylbenzene
Concen: 0.37 ug/l
RT: 13.128 min Scan# 4240
Delta R.T. 0.008 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion:105 Resp: 7114
Ion Ratio Lower Upper
105 100
134 10.8 0.0 38.8


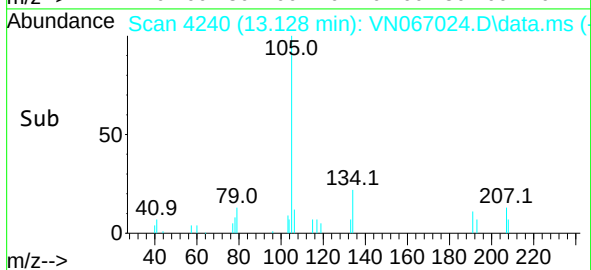
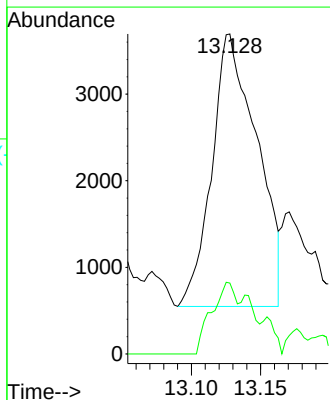



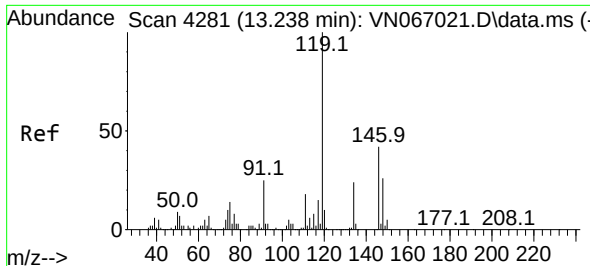

#82
p-Isopropyltoluene
Concen: 0.40 ug/l
RT: 13.251 min Scan# 4286
Delta R.T. 0.014 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampled :
IBLK


Tgt Ion:119 Resp: 6257
Ion Ratio Lower Upper
119 100
134 6.7 0.0 49.8
91 0.0 0.0 49.6

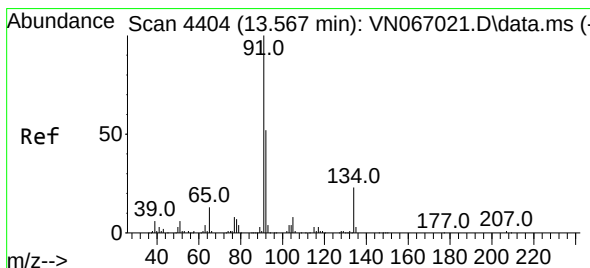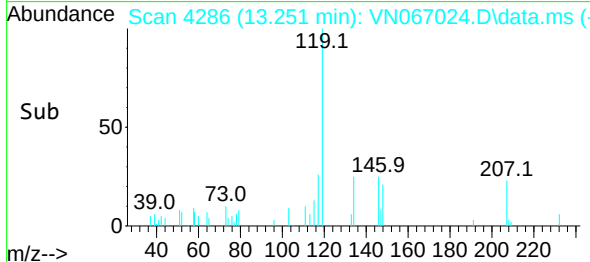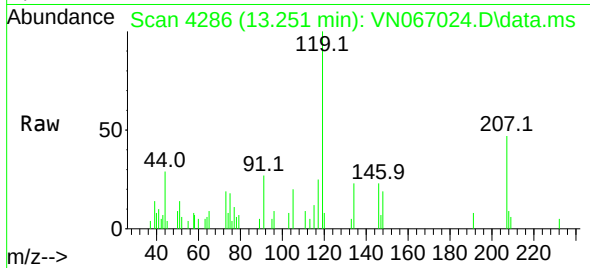

#85
n-Butylbenzene
Concen: 0.52 ug/l
RT: 13.589 min Scan# 4412
Delta R.T. 0.022 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion: 91 Resp: 6438
Ion Ratio Lower Upper
91 100
92 37.6 0.0 95.4
134 22.0 0.0 44.0


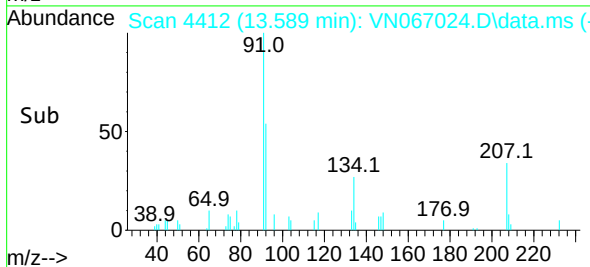

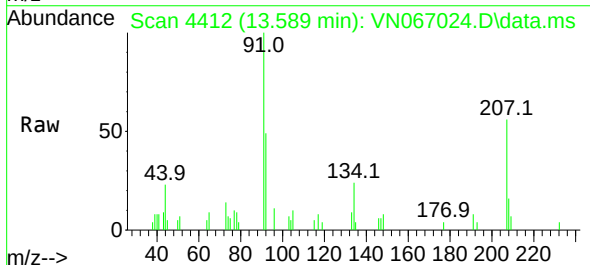




#86
Hexachloroethane
Concen: 0.35 ug/l
RT: 13.814 min Scan# 4496
Delta R.T. -0.002 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampled :
IBLK


Tgt Ion:117 Resp: 1198
Ion Ratio Lower Upper
117 100
201 62.6 37.8 113.4



#88
1,2-Dibromo-3-Chloropropane
Concen: 0.26 ug/l
RT: 14.230 min Scan# 4651
Delta R.T. 0.006 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion: 75 Resp: 363
Ion Ratio Lower Upper
75 100
155 43.5 53.4 80.2#
157 0.0 69.8 104.8#


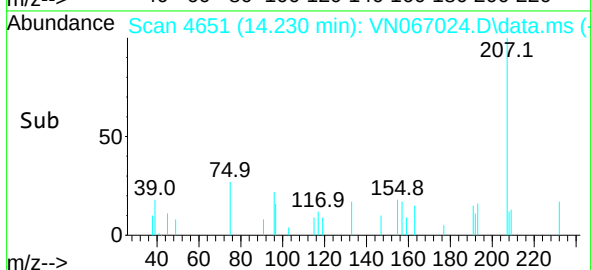






#89
1,2,4-Trichlorobenzene
Concen: 6.34 ug/l
RT: 14.866 min Scan# 4888
Delta R.T. 0.008 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12




Instrument :
MSVOA_N
ClientSampled :
IBLK


Tgt Ion:180 Resp: 26098
Ion Ratio Lower Upper
180 100
182 90.5 78.6 117.8
145 30.8 25.0 37.4



#90
Hexachlorobutadiene
Concen: 1.51 ug/l
RT: 14.957 min Scan# 4922
Delta R.T. 0.006 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion:225 Resp: 4195
Ion Ratio Lower Upper
225 100
223 47.4 0.0 137.2
227 62.8 0.0 127.8



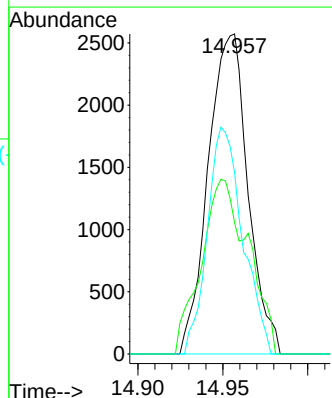



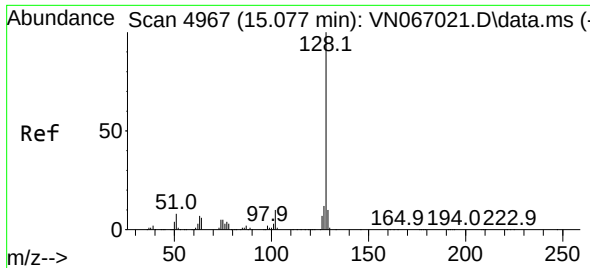

#91
Naphthalene
Concen: 13.03 ug/l
RT: 15.080 min Scan# 4968
Delta R.T. 0.003 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Instrument :
MSVOA_N
ClientSampled :
IBLK

Tgt Ion:128 Resp: 147022
Ion Ratio Lower Upper
128 100
127 11.0 9.8 14.6
129 9.6 7.8 11.8

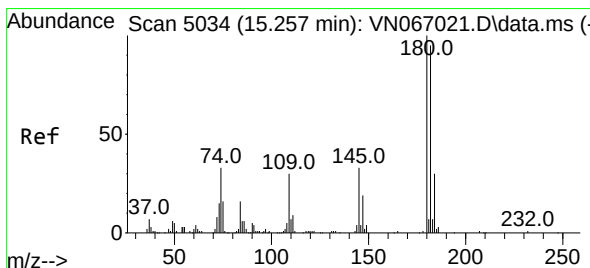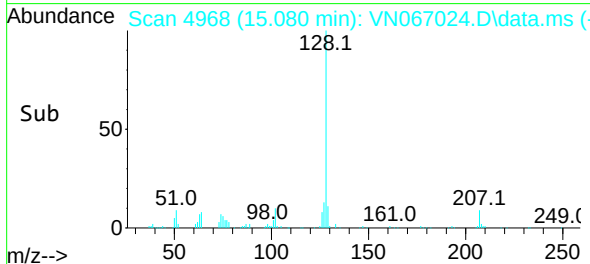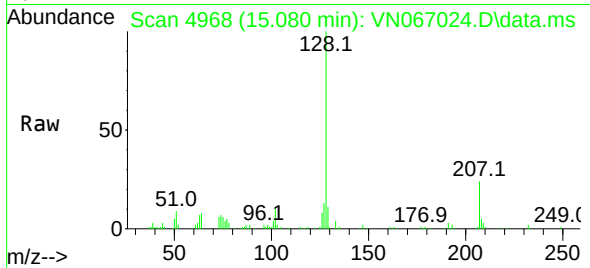

#92
1,2,3-Trichlorobenzene
Concen: 7.47 ug/l
RT: 15.260 min Scan# 5035
Delta R.T. 0.003 min
Lab File: VN067024.D
Acq: 6 May 2021 21:12

Tgt Ion:180 Resp: 32180
Ion Ratio Lower Upper
180 100
182 102.2 0.0 184.4
145 33.1 0.0 67.6

