

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
 Data File : VN067031.D
 Acq On : 7 May 2021 00:47
 Operator : JC/MD
 Sample : M2307-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-05

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VN067031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.997	81	90	99	rBV	44604	57702	1.06%	0.187%
2	2.158	132	150	167	rBV	515530	779647	14.31%	2.530%
3	2.247	173	183	194	rBV2	68797	96793	1.78%	0.314%
4	2.432	239	252	264	rVB5	36128	86967	1.60%	0.282%
5	2.762	358	375	406	rBV	973704	1970549	36.17%	6.393%
6	3.092	481	498	523	rBV3	342724	855229	15.70%	2.775%
7	3.507	633	653	676	rBV2	233605	558962	10.26%	1.814%
8	3.735	713	738	765	rBV3	54503	172739	3.17%	0.560%
9	4.355	944	969	984	rBV4	50829	160178	2.94%	0.520%
10	4.454	985	1006	1017	rBV4	118252	374264	6.87%	1.214%
11	4.704	1085	1099	1131	rVB2	56769	191489	3.52%	0.621%
12	4.961	1164	1195	1236	rBV4	186754	687657	12.62%	2.231%
13	5.291	1288	1318	1339	rBV2	32003	103354	1.90%	0.335%
14	5.481	1364	1389	1416	rBV5	32673	105468	1.94%	0.342%
15	5.846	1491	1525	1554	rBV5	126855	484920	8.90%	1.573%
16	5.978	1554	1574	1597	rBV4	67479	212696	3.90%	0.690%
17	6.283	1666	1688	1721	rVB3	77632	234781	4.31%	0.762%
18	6.541	1762	1784	1803	rBV3	231720	719339	13.20%	2.334%
19	7.112	1972	1997	2024	rBV2	214104	615578	11.30%	1.997%
20	7.313	2054	2072	2096	rVB2	199332	523146	9.60%	1.697%
21	7.579	2147	2171	2188	rBV4	194821	554455	10.18%	1.799%
22	7.670	2193	2205	2236	rVB4	100611	287163	5.27%	0.932%
23	7.860	2266	2276	2292	rVB5	30136	72153	1.32%	0.234%
24	7.968	2292	2316	2342	rBV2	2199057	5447629	100.00%	17.675%
25	8.233	2405	2415	2442	rVB5	100235	247542	4.54%	0.803%
26	8.343	2442	2456	2478	rVB7	23063	58833	1.08%	0.191%
27	8.517	2500	2521	2549	rBV	640572	1562019	28.67%	5.068%
28	8.759	2596	2611	2614	rBV5	40577	67856	1.25%	0.220%
29	8.799	2617	2626	2647	rVB3	113759	232736	4.27%	0.755%
30	8.981	2673	2694	2700	rBV4	96015	206598	3.79%	0.670%
31	9.370	2824	2839	2844	rBV4	50861	94831	1.74%	0.308%
32	9.456	2861	2871	2886	rVB5	58833	112077	2.06%	0.364%
33	9.553	2892	2907	2918	rBV2	252754	489216	8.98%	1.587%
34	9.794	2983	2997	3006	rBV7	33545	73903	1.36%	0.240%
35	9.907	3026	3039	3068	rVB3	200987	391680	7.19%	1.271%
36	10.030	3068	3085	3101	rBV	766353	1494537	27.43%	4.849%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
 Data File : VN067031.D
 Acq On : 7 May 2021 00:47
 Operator : JC/MD
 Sample : M2307-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-05

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

37	10.094	3104	3109	3123	rVB2	74282	116023	2.13%	0.376%
38	10.242	3153	3164	3177	rVB6	71254	135385	2.49%	0.439%
39	10.322	3184	3194	3205	rVB4	53504	85828	1.58%	0.278%
40	10.459	3233	3245	3268	rVB5	94437	195441	3.59%	0.634%
41	10.735	3329	3348	3359	rBV2	100503	204725	3.76%	0.664%
42	10.859	3387	3394	3406	rVB4	38310	61027	1.12%	0.198%
43	11.352	3563	3578	3607	rBV	582817	1346143	24.71%	4.368%
44	11.575	3648	3661	3686	rVB2	78019	191160	3.51%	0.620%
45	11.698	3697	3707	3723	rVB7	38835	77019	1.41%	0.250%
46	12.194	3879	3892	3907	rBV	166120	305847	5.61%	0.992%
47	12.353	3936	3951	3981	rBV	310970	728871	13.38%	2.365%
48	12.540	4010	4021	4041	rBV	185982	363296	6.67%	1.179%
49	12.841	4123	4133	4147	rBV2	64060	114182	2.10%	0.370%
50	13.487	4353	4374	4388	rBV	2019821	3690215	67.74%	11.973%
51	13.747	4464	4471	4490	rVB3	72156	125417	2.30%	0.407%
52	13.836	4493	4504	4515	rBV	259636	424268	7.79%	1.377%
53	13.889	4517	4524	4531	rVV3	95932	148978	2.73%	0.483%
54	13.938	4532	4542	4563	rVB	646216	1099305	20.18%	3.567%
55	14.155	4612	4623	4631	rBV	208983	341110	6.26%	1.107%
56	14.192	4632	4637	4649	rVB2	124752	181737	3.34%	0.590%
57	14.423	4715	4723	4733	rBV2	81134	125411	2.30%	0.407%
58	14.536	4754	4765	4781	rVB4	116870	236221	4.34%	0.766%
59	14.683	4814	4820	4834	rVB6	49022	76218	1.40%	0.247%
60	14.793	4855	4861	4869	rBV7	47190	63081	1.16%	0.205%


Sum of corrected areas: 30821594

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
Data File : VN067031.D
Acq On : 7 May 2021 00:47
Operator : JC/MD
Sample : M2307-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

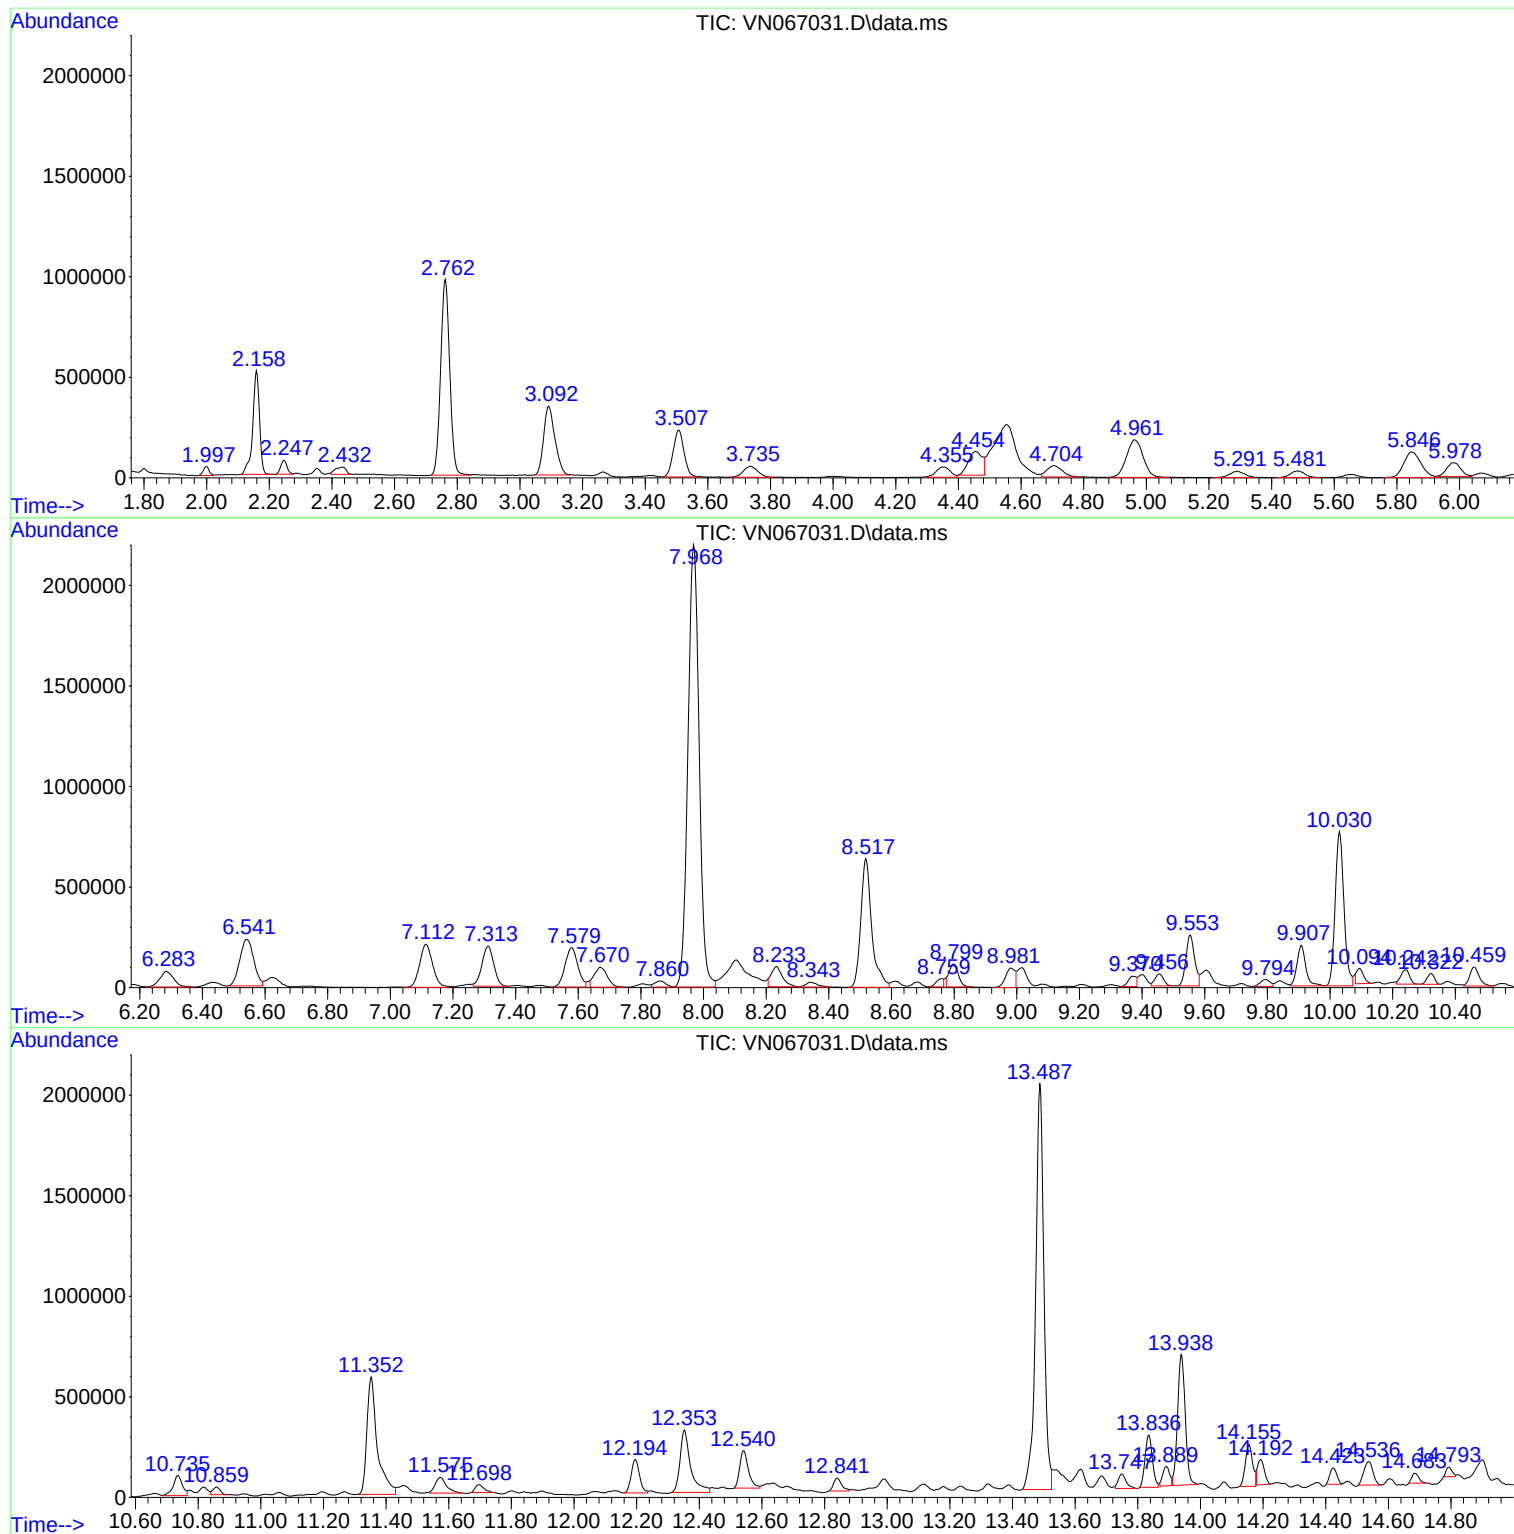

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
Data File : VN067031.D
Acq On : 7 May 2021 00:47
Operator : JC/MD
Sample : M2307-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
Data File : VN067031.D
Acq On : 7 May 2021 00:47
Operator : JC/MD
Sample : M2307-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-05

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
