

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
 Data File : VN067044.D
 Acq On : 7 May 2021 5:58
 Operator : JC/MD
 Sample : M2313-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 210505078-02-VOA

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VN067044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.979	75	83	115	rVB2	252228	531658	4.63%	1.421%
2	2.437	241	254	285	rBV3	86515	343213	2.99%	0.917%
3	3.754	722	745	795	rBV	769083	2136087	18.62%	5.708%
4	4.001	818	837	861	rBV	115419	331493	2.89%	0.886%
5	4.706	1063	1100	1159	rBV	1697635	6102989	53.19%	16.307%
6	6.745	1830	1860	1943	rBV2	3603849	11473177	100.00%	30.657%
7	7.128	1976	2003	2049	rBV3	1740559	5209219	45.40%	13.919%
8	7.957	2283	2312	2338	rBV3	250924	717043	6.25%	1.916%
9	8.520	2503	2522	2548	rBV	432411	915763	7.98%	2.447%
10	10.030	3069	3085	3101	rBV	699800	1325964	11.56%	3.543%
11	10.094	3102	3109	3117	rVV2	67315	119755	1.04%	0.320%
12	10.663	3305	3321	3340	rBV	149439	271804	2.37%	0.726%
13	11.352	3563	3578	3605	rBV	560164	1080776	9.42%	2.888%
14	11.457	3606	3617	3641	rVV	151167	300129	2.62%	0.802%
15	11.564	3645	3657	3691	rVB	125242	282892	2.47%	0.756%
16	11.894	3768	3780	3804	rBV2	74106	154559	1.35%	0.413%
17	12.353	3937	3951	3977	rBV	291824	669541	5.84%	1.789%
18	13.350	4306	4323	4343	rVB4	160335	314946	2.75%	0.842%
19	13.825	4491	4500	4515	rVB	140903	242334	2.11%	0.648%
20	14.163	4612	4626	4655	rBV	779570	1417954	12.36%	3.789%
21	14.592	4775	4786	4800	rBV	202612	364374	3.18%	0.974%
22	14.745	4832	4843	4845	rBV8	92291	126732	1.10%	0.339%
23	14.785	4847	4858	4870	rVV	1439191	2417098	21.07%	6.459%
24	14.839	4870	4878	4898	rVB5	288871	575050	5.01%	1.537%




Sum of corrected areas: 37424550

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
Data File : VN067044.D
Acq On : 7 May 2021 5:58
Operator : JC/MD
Sample : M2313-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
210505078-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

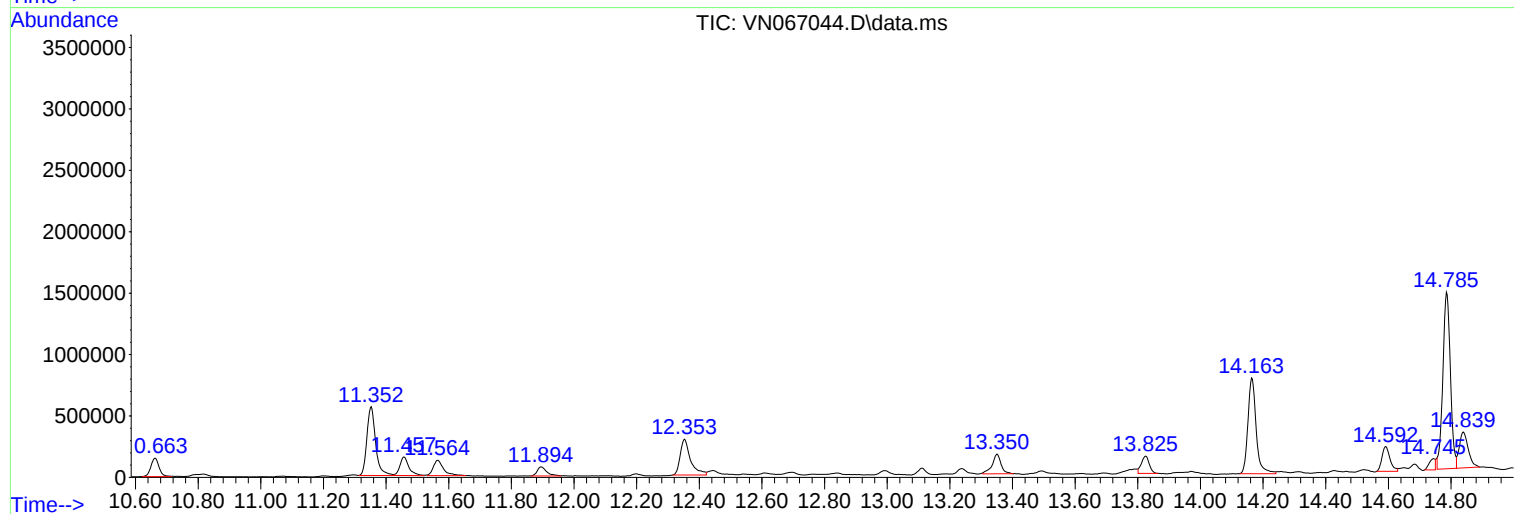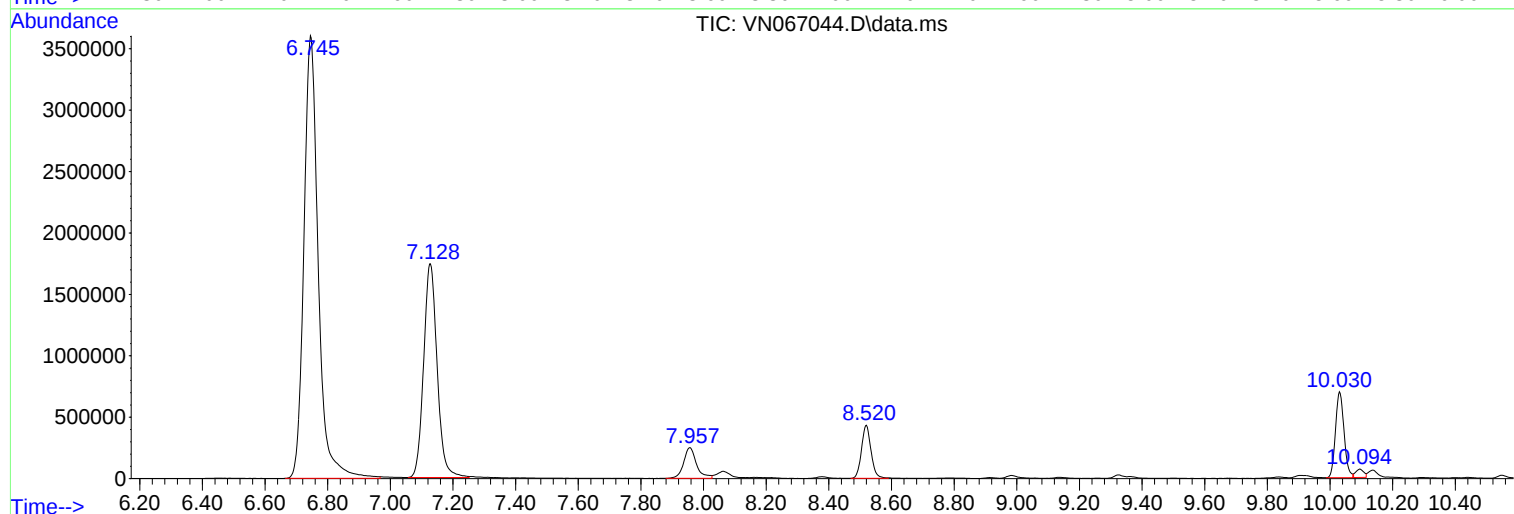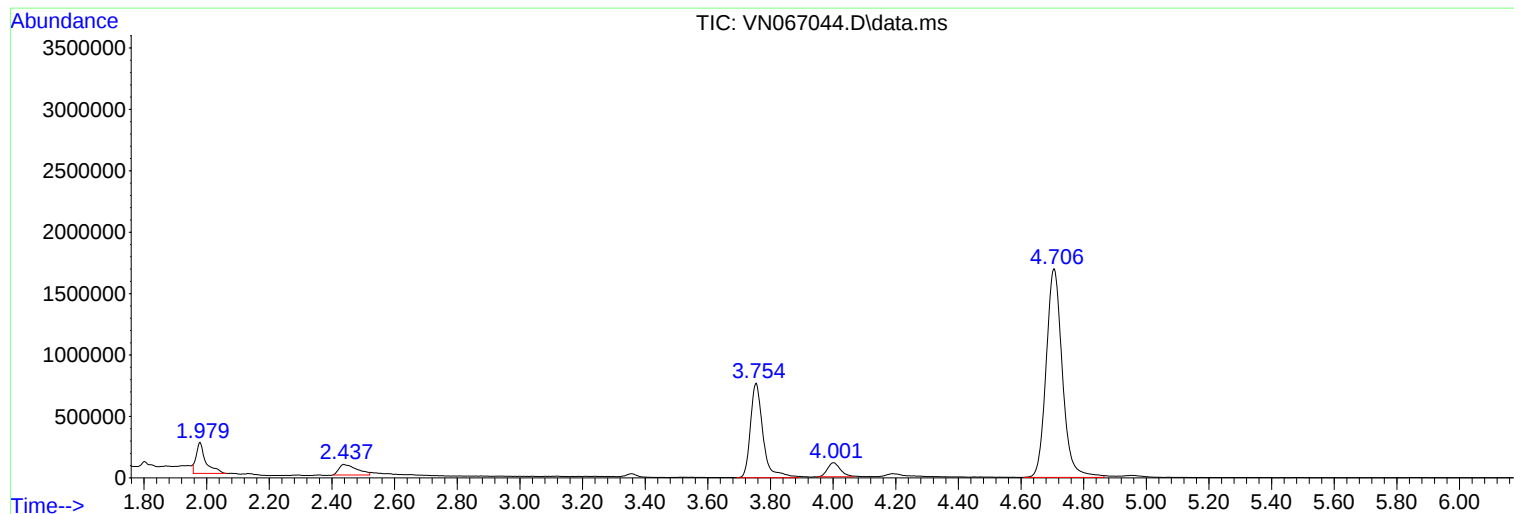

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
Data File : VN067044.D
Acq On : 7 May 2021 5:58
Operator : JC/MD
Sample : M2313-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
210505078-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050721\
Data File : VN067044.D
Acq On : 7 May 2021 5:58
Operator : JC/MD
Sample : M2313-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
210505078-02-VOA

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
