

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050725\
 Data File : VN086532.D
 Acq On : 07 May 2025 13:20
 Operator : JC\MD
 Sample : Q1949-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 001-WILLETS-PT-BLVD(MAY)

Quant Time: May 08 03:25:36 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042325W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu Apr 24 04:42:24 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	7.812	128	45740	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.095	114	271916	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.865	117	243077	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.577	65	126733	28.738	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	95.800%
60) 4-Bromofluorobenzene	12.847	95	134917	28.240	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	94.133%
63) Toluene-d8	10.565	98	395947	29.608	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	98.700%
Target Compounds						
					Qvalue	
3) Chloromethane	2.360	50	1074	0.239	ug/l	94
12) Methyl Acetate	5.018	43	1346	0.298	ug/l	92
13) Acrolein	4.177	56	210	Below Cal		85
15) Acetone	4.418	58	214983	463.481	ug/l	98
16) Carbon Disulfide	4.724	76	34827	4.142	ug/l	95
18) Methylene Chloride	5.271	84	1422	0.391	ug/l	94
23) tert-Butyl Alcohol	5.506	59	4067	6.237	ug/l #	100
25) Chloroform	7.959	83	6424	0.956	ug/l	96
30) 2-Butanone	7.477	43	120575	51.822	ug/l	97
35) Methacrylonitrile	7.777	41	8032	3.026	ug/l #	47
36) 1,2-Dichloroethane	9.095	62	9077	1.834	ug/l #	74
43) Ethyl Acetate	7.559	43	13521	2.936	ug/l	95
44) Isopropyl Acetate	8.677	43	2108	0.241	ug/l #	49
45) 1,4-Dioxane	9.342	88	740	10.853	ug/l #	37
46) Methyl methacrylate	9.653	41	1819	0.451	ug/l #	42
48) t-1,3-Dichloropropene	10.624	75	3198	0.537	ug/l #	1
49) cis-1,3-Dichloropropene	10.624	75	3198	0.509	ug/l #	1
51) Ethyl methacrylate	10.789	69	2398	0.391	ug/l	74
56) Bromoform	12.841	173	867	0.338	ug/l #	1
58) 4-Methyl-2-Pentanone	10.441	43	22889	4.866	ug/l	98
59) 2-Hexanone	11.194	43	1662	0.479	ug/l #	74
62) Toluene	10.624	91	487357	29.953	ug/l	100
66) Ethyl Benzene	11.965	91	13831	0.755	ug/l	100
67) m/p-Xylenes	12.065	106	23972	3.450	ug/l	96
68) o-Xylene	12.394	106	9682	1.423	ug/l	94
72) 1,2,3-Trichloropropane	12.847	75	68187	17.489	ug/l	1
77) t-1,4-Dichloro-2-butene	12.847	75	68187	34.460	ug/l #	13
79) tert-butylbenzene	13.724	119	5048	0.423	ug/l	57
80) 1,2,4-Trimethylbenzene	13.477	105	9973	0.701	ug/l	80
82) p-Isopropyltoluene	13.724	119	5048	0.354	ug/l	98
90) Hexachlorobutadiene	15.506	225	514	0.399	ug/l	65
91) Naphthalene	15.635	128	5170	0.451	ug/l #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050725\
Data File : VN086532.D
Acq On : 07 May 2025 13:20
Operator : JC\MD
Sample : Q1949-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)

Quant Time: May 08 03:25:36 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N042325W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu Apr 24 04:42:24 2025
Response via : Initial Calibration




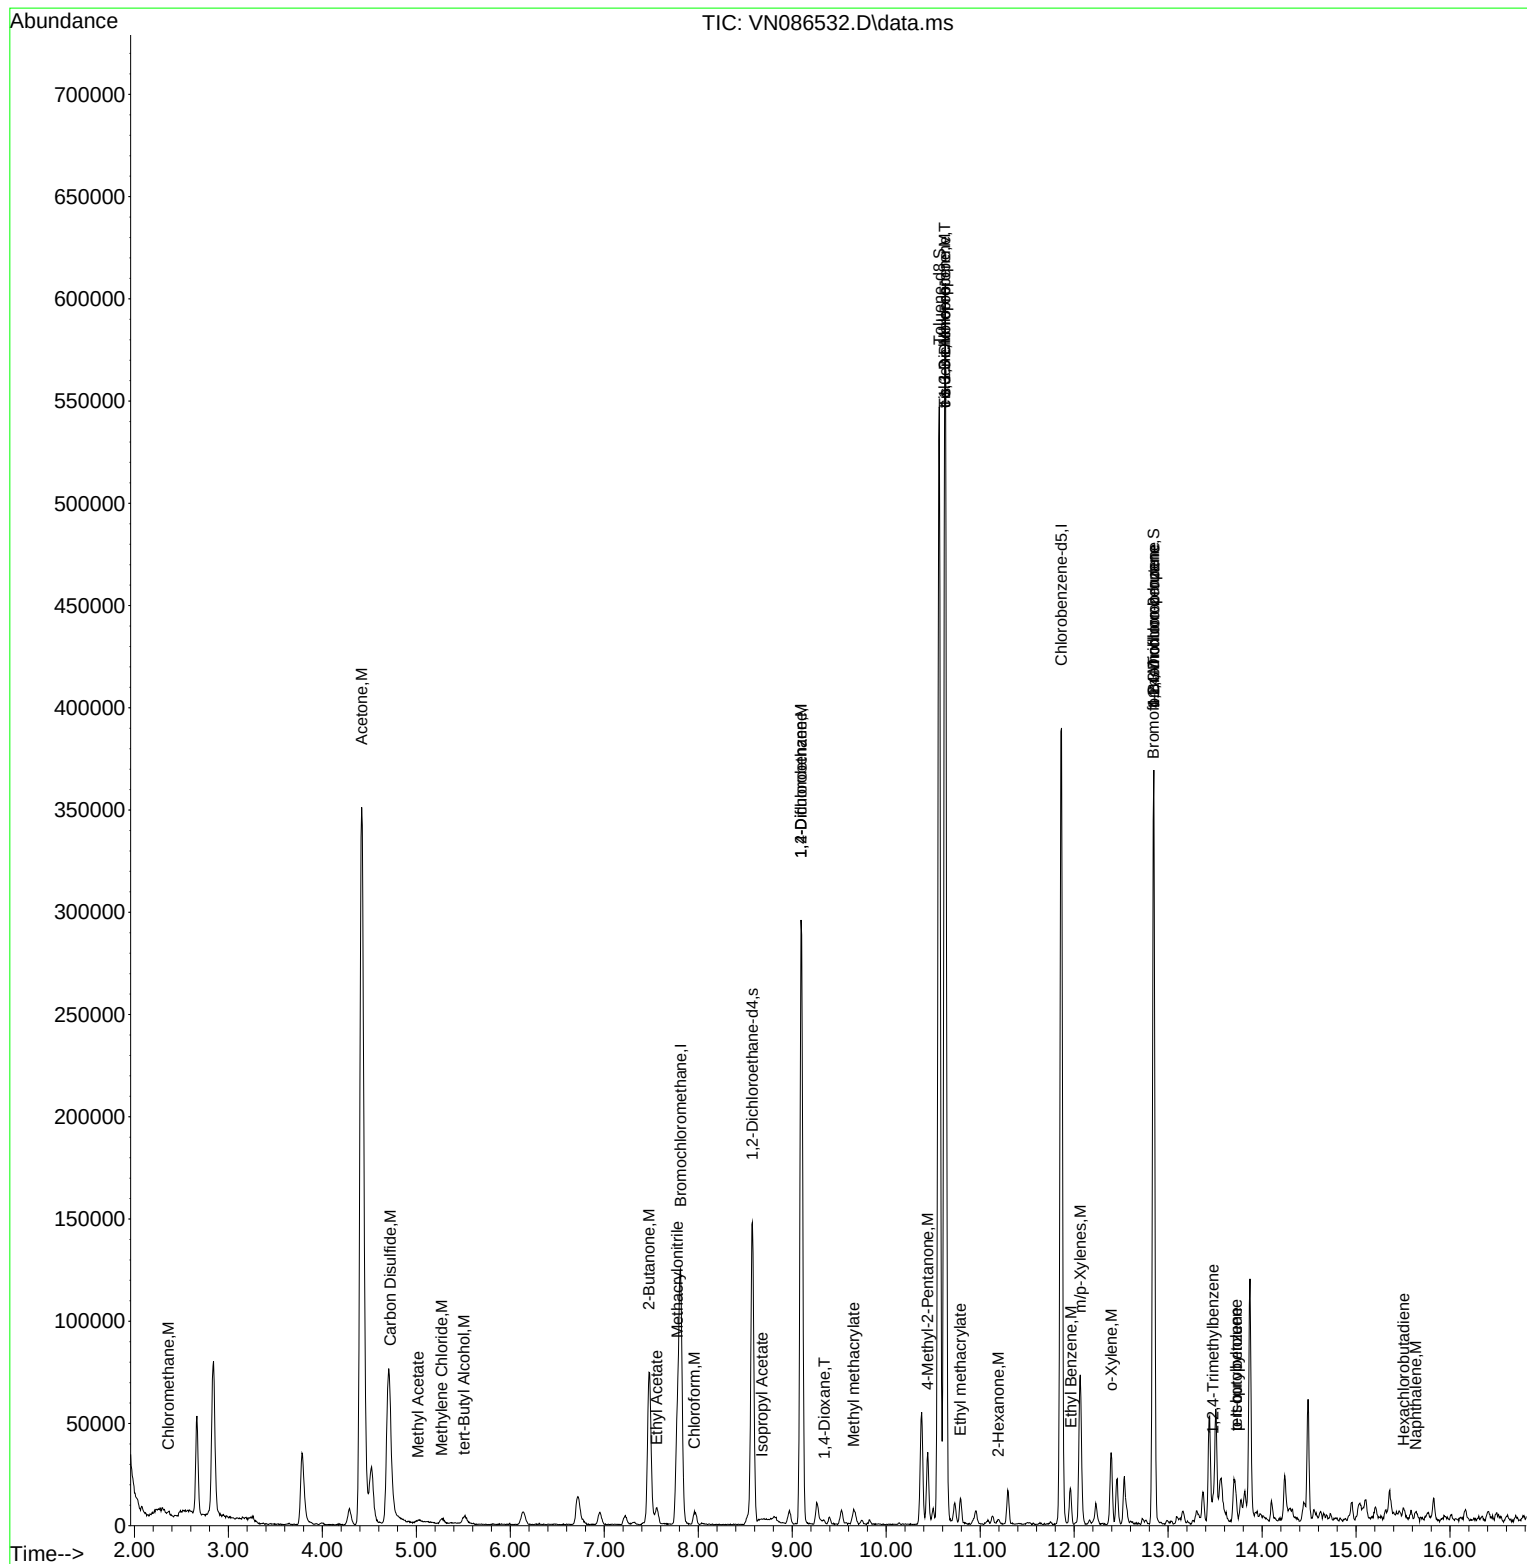




#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.812 min Scan# 996
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion:128 Resp: 45740
Ion Ratio Lower Upper
128 100
49 144.7 0.0 433.8
130 128.3 0.0 325.0

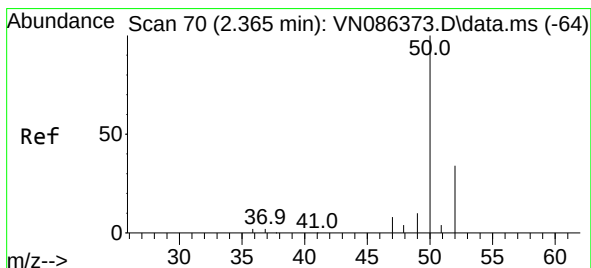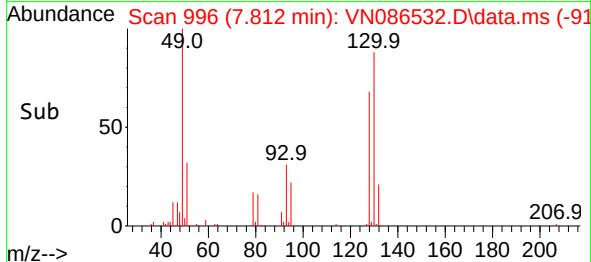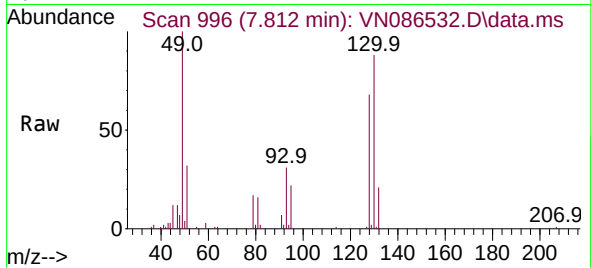

#3
Chloromethane
Concen: 0.239 ug/l
RT: 2.360 min Scan# 69
Delta R.T. -0.006 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion: 50 Resp: 1074
Ion Ratio Lower Upper
50 100
52 37.6 27.3 40.9

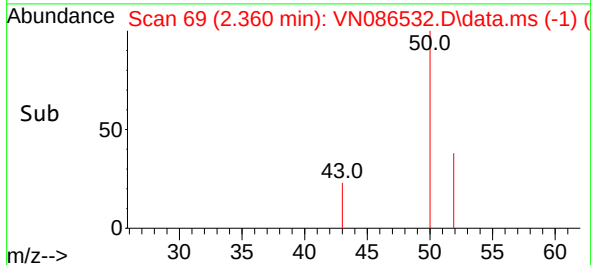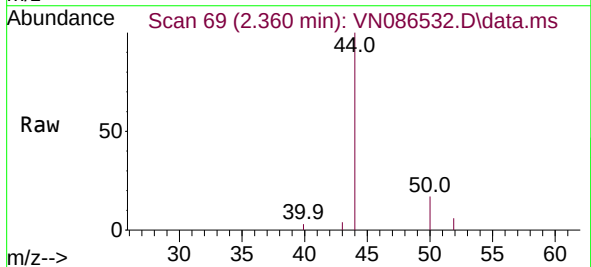



#12

Methyl Acetate

Concen: 0.298 ug/l

RT: 5.018 min Scan# 51

Delta R.T. 0.000 min

Lab File: VN086532.D

Acq: 07 May 2025 13:20

Instrument :

MSVOA_N

ClientSampleId :





001-WILLETS-PT-BLVD(MAY)

Tgt Ion: 43 Resp: 1346

Ion Ratio Lower Upper

43 100

74 21.9 20.8 31.2

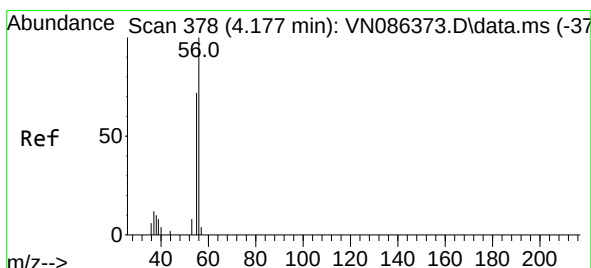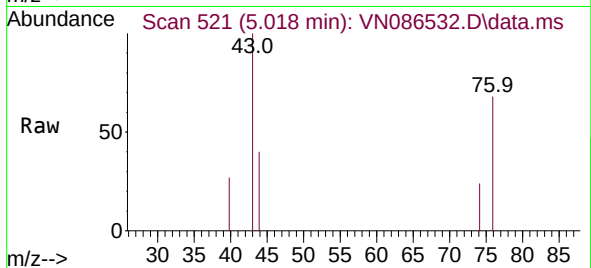

#13

Acrolein

Concen: Below Cal

RT: 4.177 min Scan# 378

Delta R.T. 0.000 min

Lab File: VN086532.D




Acq: 07 May 2025 13:20


Tgt Ion: 56 Resp: 210

Ion Ratio Lower Upper

56 100

55 58.1 56.1 84.1

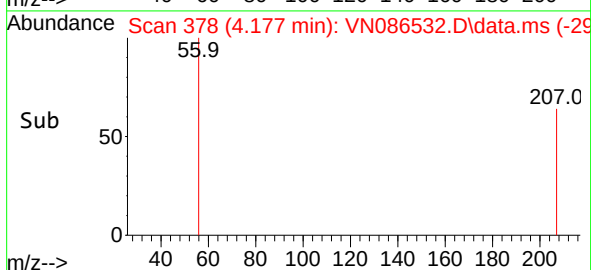

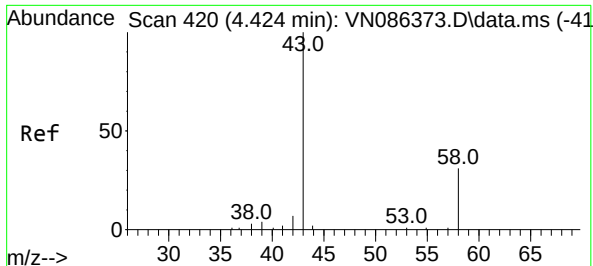

#15

Acetone

Concen: 463.481 ug/l

RT: 4.418 min Scan# 41

Delta R.T. -0.006 min

Lab File: VN086532.D

Acq: 07 May 2025 13:20

Instrument :

MSVOA_N

ClientSampleId :





001-WILLETS-PT-BLVD(MAY)

Tgt Ion: 58 Resp: 214983

Ion Ratio Lower Upper

58 100

43 314.3 255.1 382.7

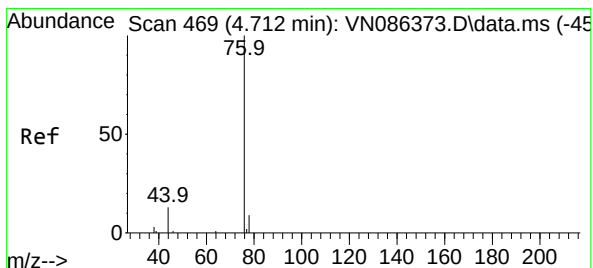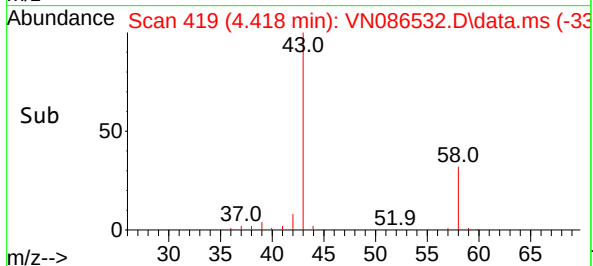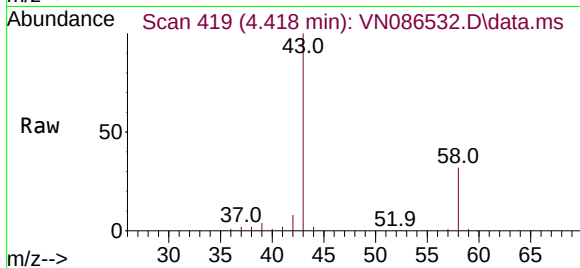

#16

Carbon Disulfide

Concen: 4.142 ug/l

RT: 4.724 min Scan# 471

Delta R.T. 0.012 min

Lab File: VN086532.D




Acq: 07 May 2025 13:20


Tgt Ion: 76 Resp: 34827

Ion Ratio Lower Upper

76 100

78 7.2 7.1 10.7

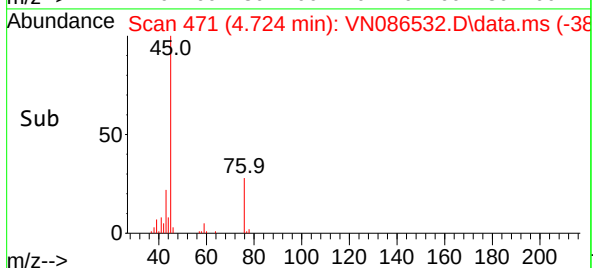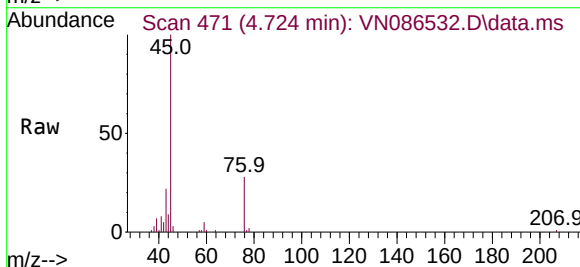







#18
Methylene Chloride
Concen: 0.391 ug/l
RT: 5.271 min Scan# 501
Delta R.T. -0.006 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)

Tgt Ion: 84 Resp: 1422




Ion	Ratio	Lower	Upper
84	100		
49	114.7	95.4	143.0
51	45.0	32.8	49.2
86	59.4	53.0	79.4

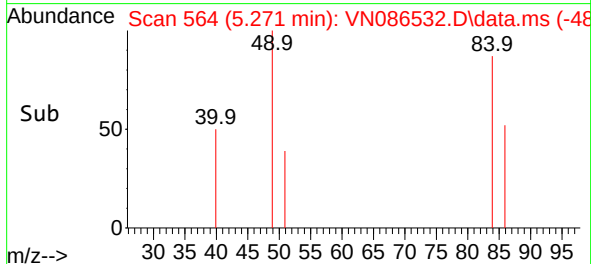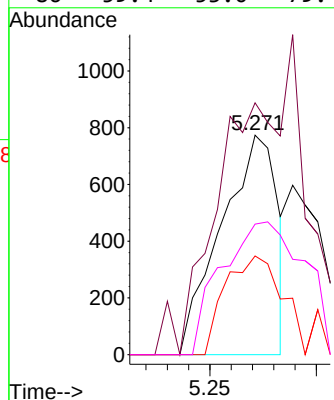


#23
tert-Butyl Alcohol
Concen: 6.237 ug/l
RT: 5.506 min Scan# 604
Delta R.T. -0.006 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion: 59 Resp: 4067

Ion	Ratio	Lower	Upper
59	100		
52	0.0	0.1	0.1

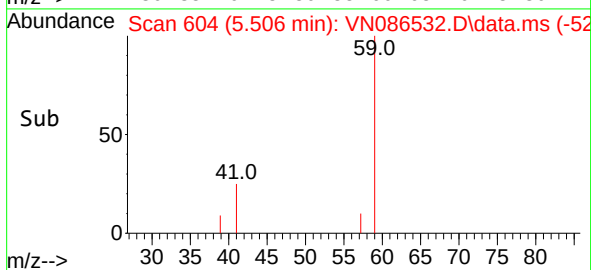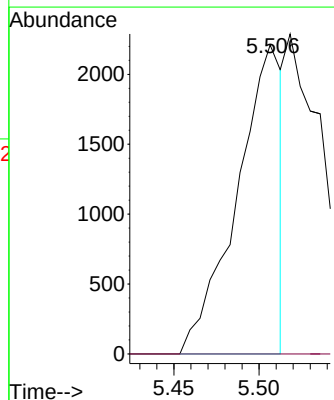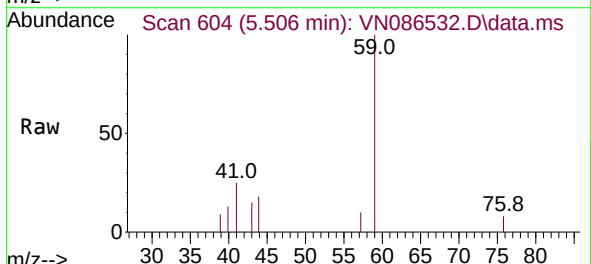

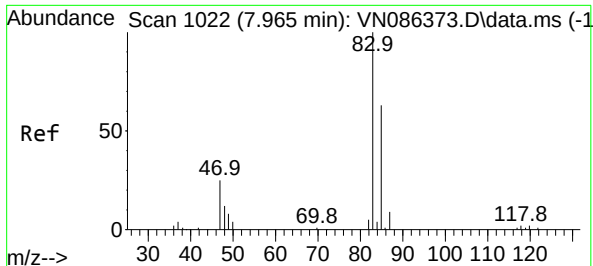

#25

Chloroform

Concen: 0.956 ug/l

RT: 7.959 min Scan# 110

Delta R.T. -0.006 min

Lab File: VN086532.D

Acq: 07 May 2025 13:20

Instrument :

MSVOA_N

ClientSampleId :





001-WILLETS-PT-BLVD(MAY)

Tgt Ion: 83 Resp: 6424

Ion Ratio Lower Upper

83 100

85 59.3 50.2 75.2

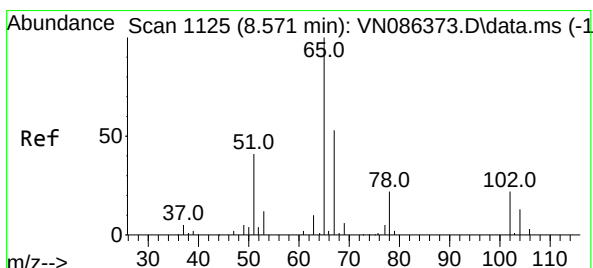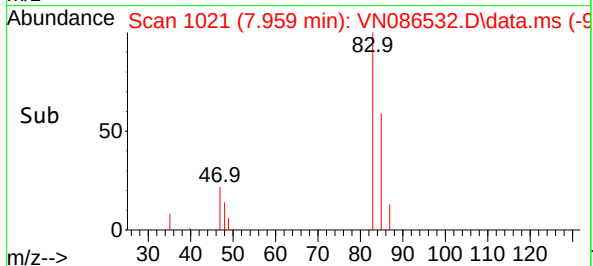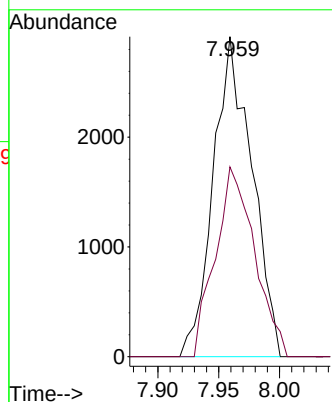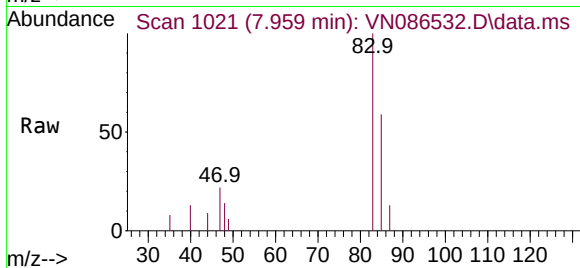

#27

1,2-Dichloroethane-d4

Concen: 28.738 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. 0.006 min

Lab File: VN086532.D




Acq: 07 May 2025 13:20


Tgt Ion: 65 Resp: 126733

Ion Ratio Lower Upper

65 100

67 51.3 42.5 63.7


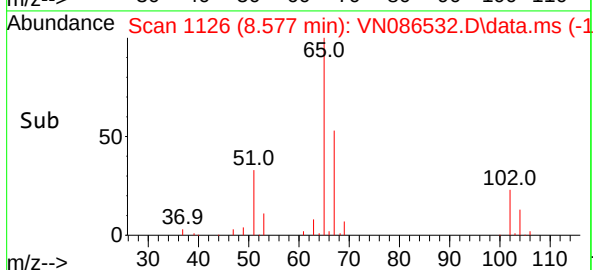

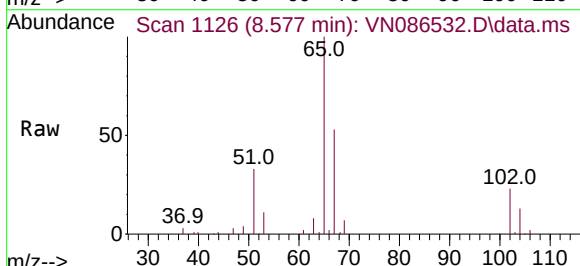


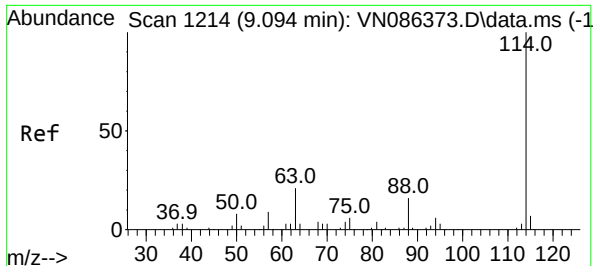

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 9.095 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion:114 Resp: 271916
Ion Ratio Lower Upper
114 100
63 19.3 16.7 25.1
88 15.7 12.6 19.0

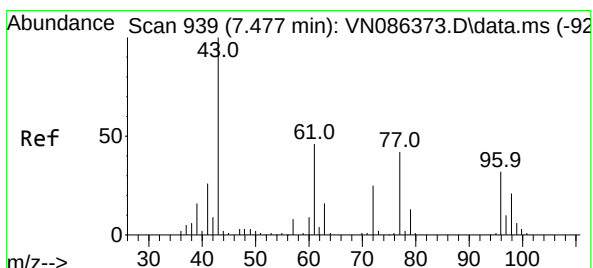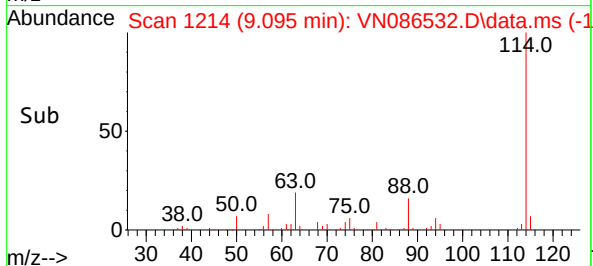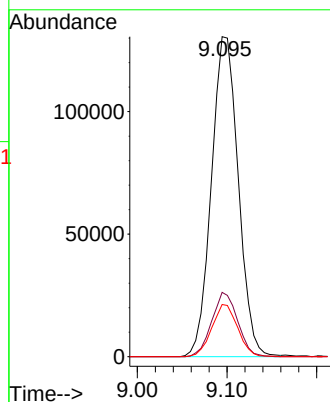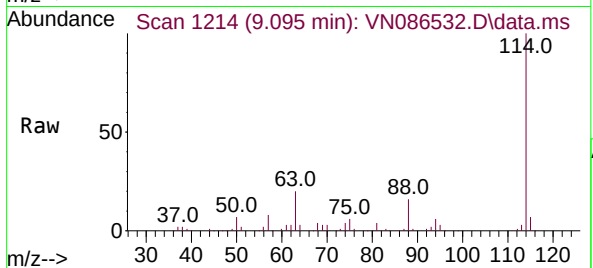

#30
2-Butanone
Concen: 51.822 ug/l
RT: 7.477 min Scan# 939
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion: 43 Resp: 120575
Ion Ratio Lower Upper
43 100
57 9.0 6.6 10.0
72 29.7 22.2 33.4


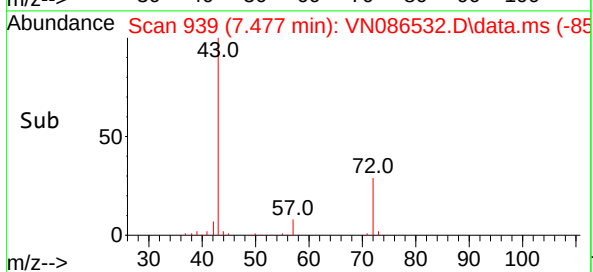
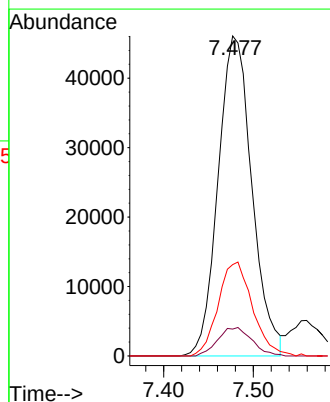
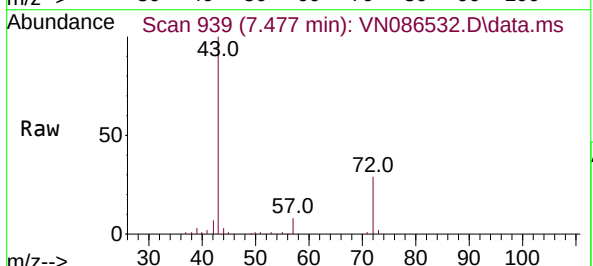




#35
Methacrylonitrile
Concen: 3.026 ug/l
RT: 7.777 min Scan# 990
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion:	41	Resp:	8032
Ion	Ratio	Lower	Upper
41	100		
39	49.3	27.0	80.8
67	0.0	35.8	107.3#
52	0.0	15.2	45.5#

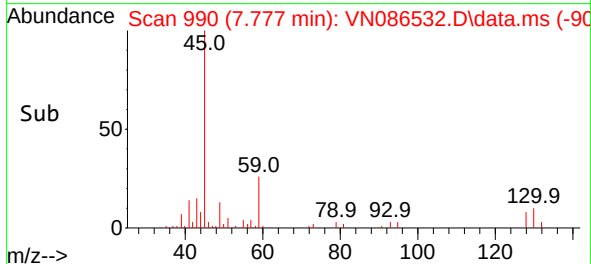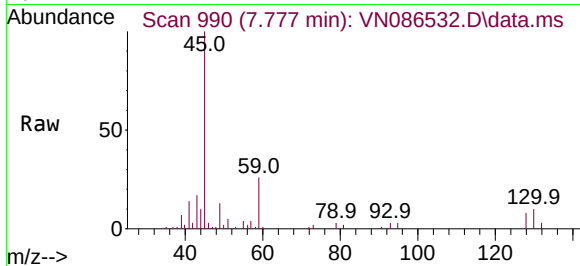

#36
1,2-Dichloroethane
Concen: 1.834 ug/l
RT: 9.095 min Scan# 1214
Delta R.T. 0.430 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion:	62	Resp:	9077
Ion	Ratio	Lower	Upper
62	100		
98	0.0	7.6	11.4#


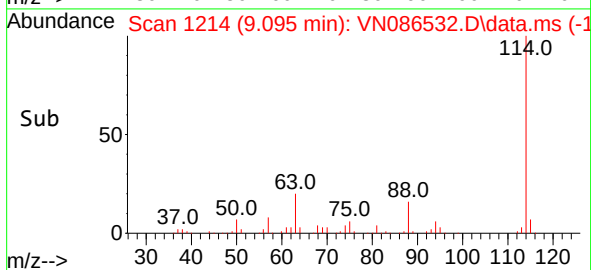

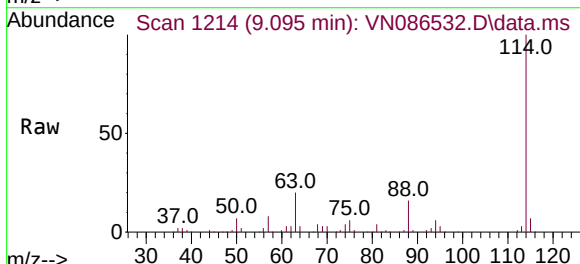




#43
Ethyl Acetate
Concen: 2.936 ug/l
RT: 7.559 min Scan# 91
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion: 43 Resp: 13521
Ion Ratio Lower Upper
43 100
45 12.4 11.4 17.2

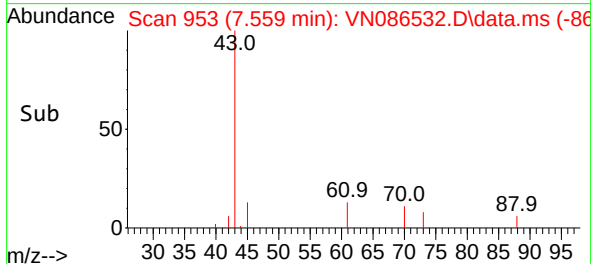

#44
Isopropyl Acetate
Concen: 0.241 ug/l
RT: 8.677 min Scan# 1143
Delta R.T. -0.006 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion: 43 Resp: 2108
Ion Ratio Lower Upper
43 100
61 0.0 21.0 31.4#


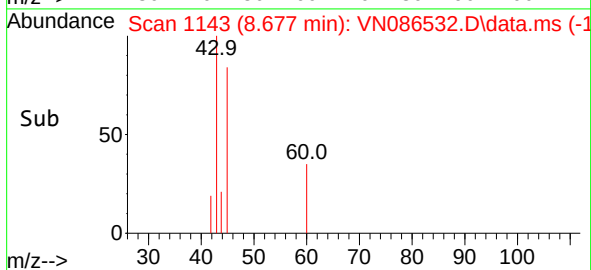

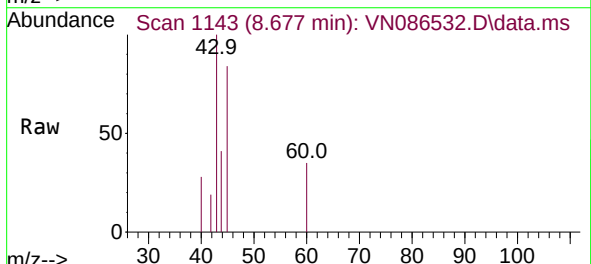


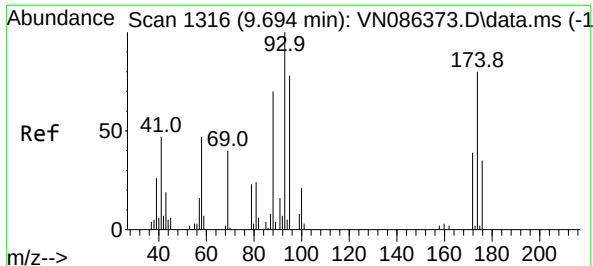

#45
1,4-Dioxane
Concen: 10.853 ug/l
RT: 9.342 min Scan# 11
Delta R.T. -0.353 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion: 88 Resp: 740
Ion Ratio Lower Upper
88 100
43 27.2 24.9 37.3
58 0.0 57.8 86.8#

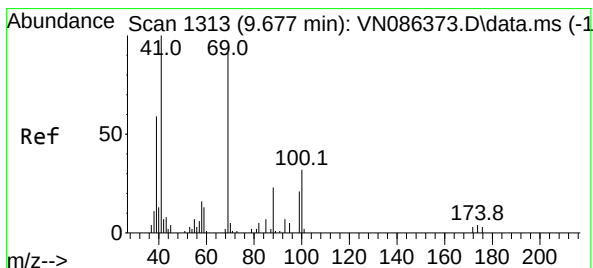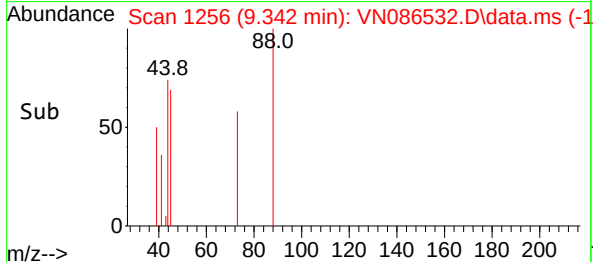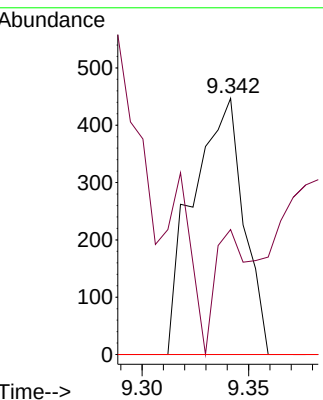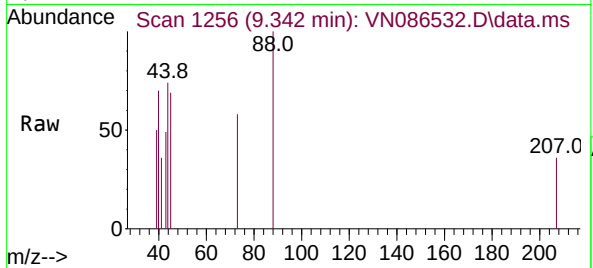

#46
Methyl methacrylate
Concen: 0.451 ug/l
RT: 9.653 min Scan# 1309
Delta R.T. -0.023 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion: 41 Resp: 1819
Ion Ratio Lower Upper
41 100
69 0.0 44.1 132.3#
39 56.9 30.0 90.1


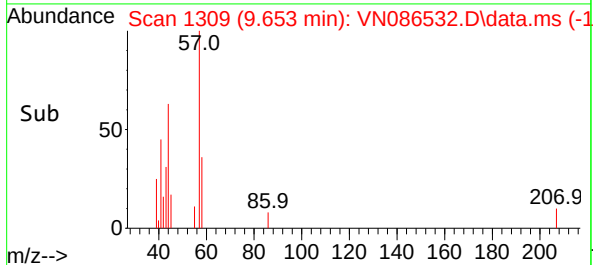
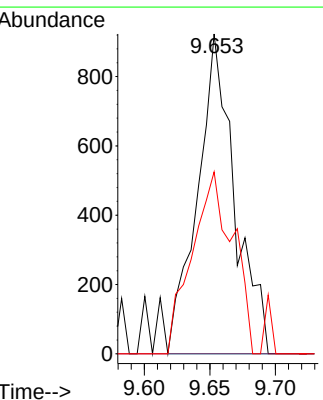
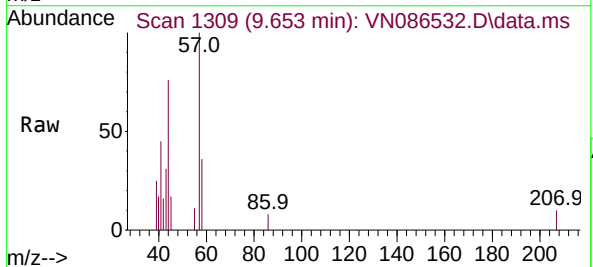


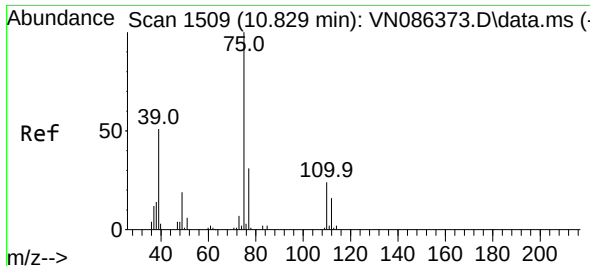

#48
t-1,3-Dichloropropene
Concen: 0.537 ug/l
RT: 10.624 min Scan# 1474
Delta R.T. -0.206 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion: 75 Resp: 3198
Ion Ratio Lower Upper
75 100
77 179.1 24.4 36.6#

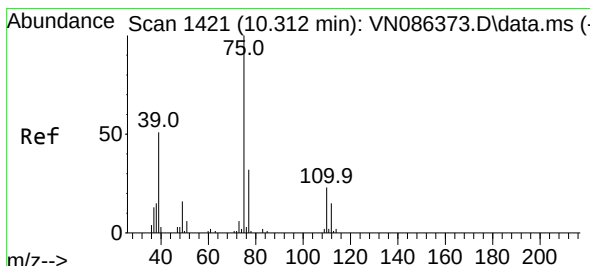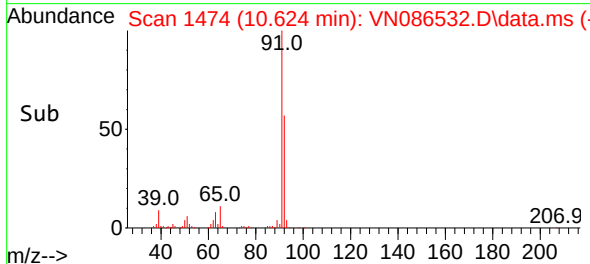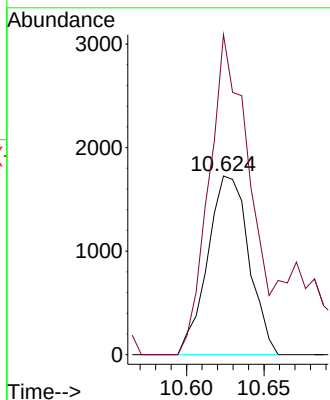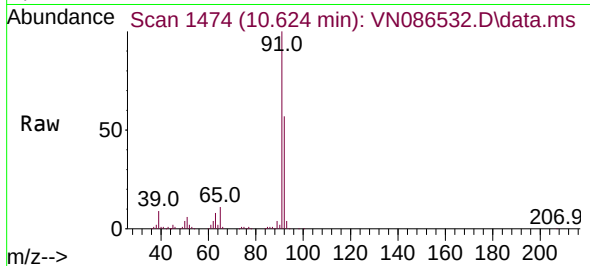

#49
cis-1,3-Dichloropropene
Concen: 0.509 ug/l
RT: 10.624 min Scan# 1474
Delta R.T. 0.312 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion: 75 Resp: 3198
Ion Ratio Lower Upper
75 100
77 179.1 25.6 38.4#
39 1284.0 40.6 60.8#


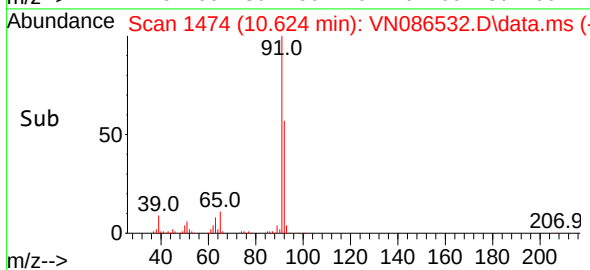
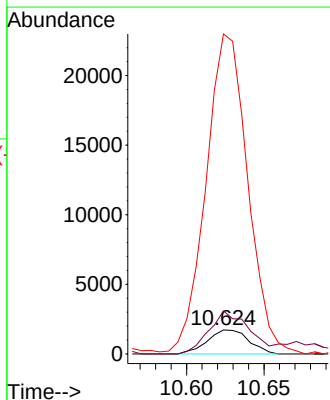
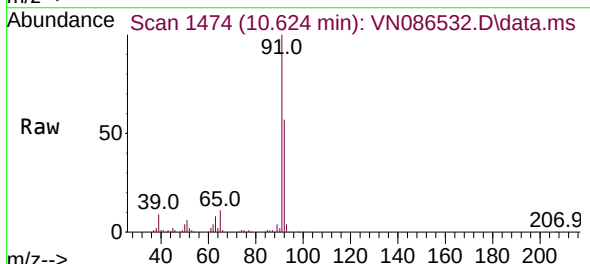




#51
Ethyl methacrylate
Concen: 0.391 ug/l
RT: 10.789 min Scan# 11
Delta R.T. -0.082 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion: 69 Resp: 2398
Ion Ratio Lower Upper
69 100
41 92.1 32.3 96.8
39 45.1 19.1 57.1

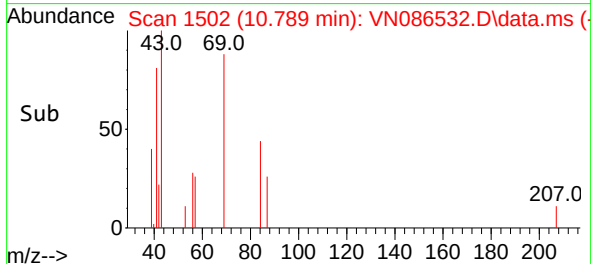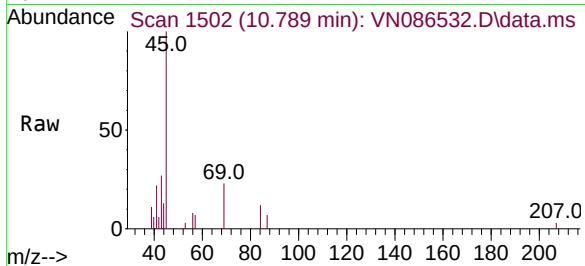

#56
Bromoform
Concen: 0.338 ug/l
RT: 12.841 min Scan# 1851
Delta R.T. 0.265 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion:173 Resp: 867
Ion Ratio Lower Upper
173 100
175 873.9 39.0 58.6#
254 0.0 3.8 5.6#


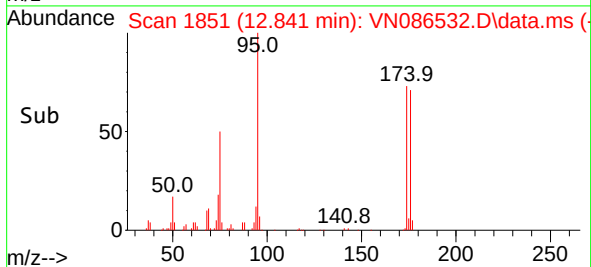

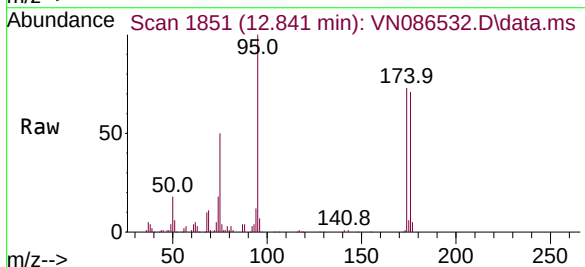


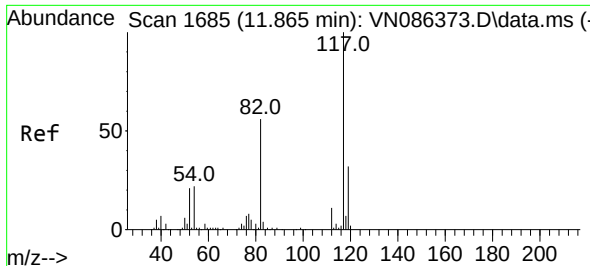

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.865 min Scan# 1186
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion:117 Resp: 243077
Ion Ratio Lower Upper
117 100
82 53.7 45.5 68.3
119 32.2 25.9 38.9

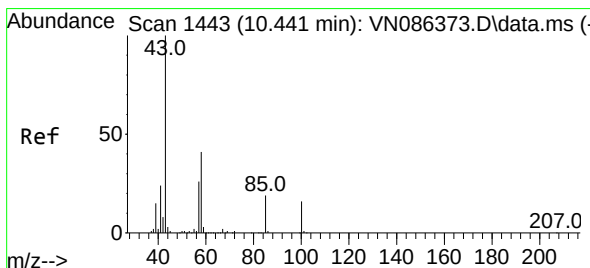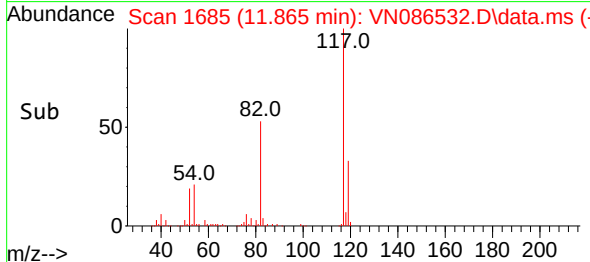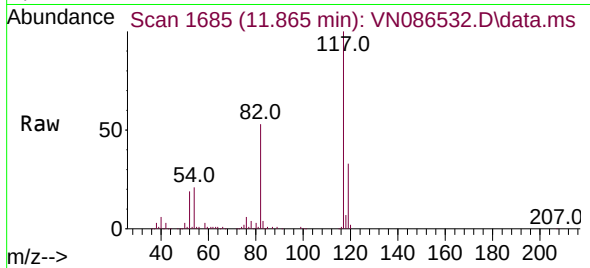

#58
4-Methyl-2-Pentanone
Concen: 4.866 ug/l
RT: 10.441 min Scan# 1443
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion: 43 Resp: 22889
Ion Ratio Lower Upper
43 100
58 41.2 33.0 49.6
85 21.2 14.9 22.3


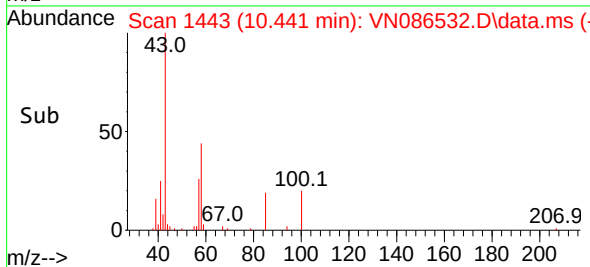

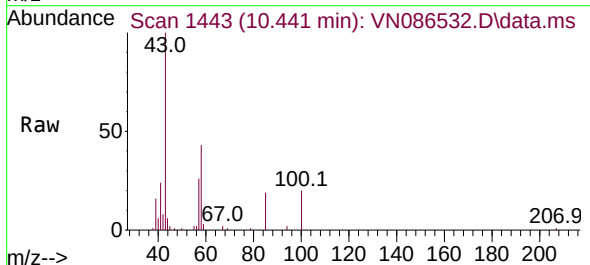




#59
2-Hexanone
Concen: 0.479 ug/l
RT: 11.194 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion: 43 Resp: 1662
Ion Ratio Lower Upper
43 100
58 42.2 45.0 67.6#
57 39.8 15.5 23.3#

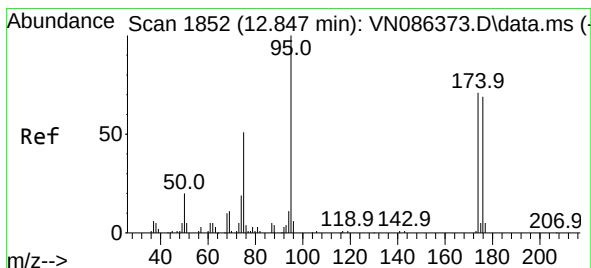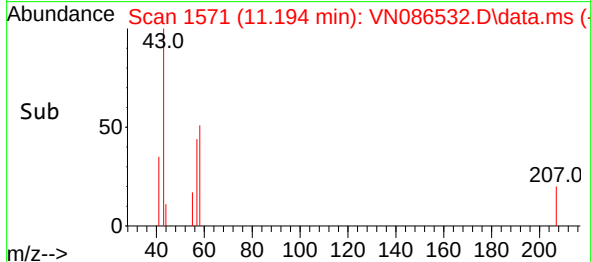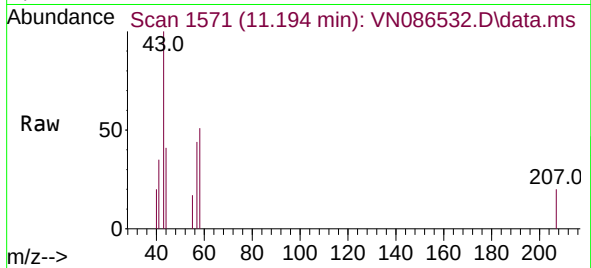

#60
4-Bromofluorobenzene
Concen: 28.240 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion: 95 Resp: 134917
Ion Ratio Lower Upper
95 100
174 75.2 56.6 84.8
176 72.5 53.3 79.9


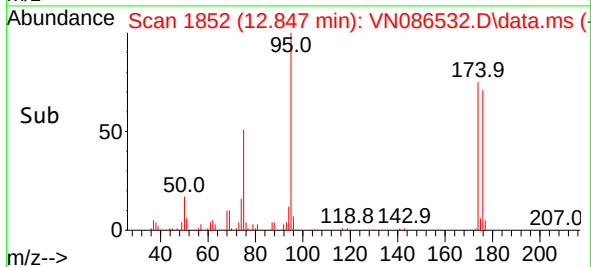

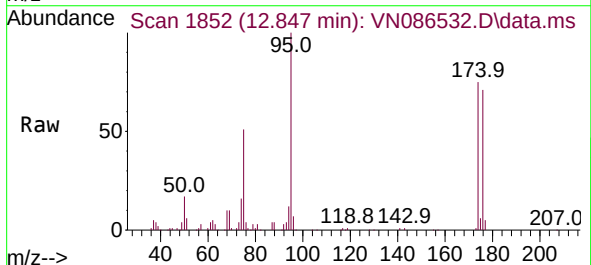


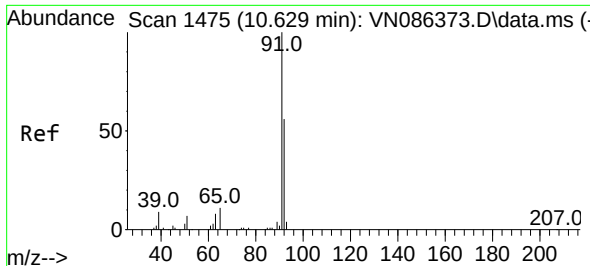

#62
Toluene
Concen: 29.953 ug/l
RT: 10.624 min Scan# 1475
Delta R.T. -0.006 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion: 91 Resp: 487357
Ion Ratio Lower Upper
91 100
92 57.3 45.7 68.5

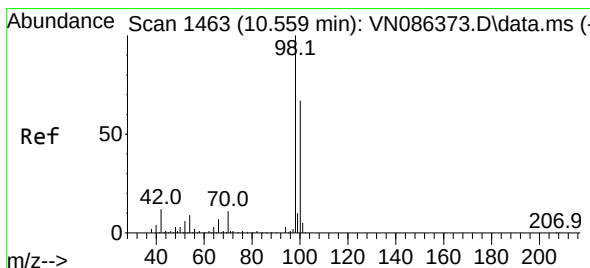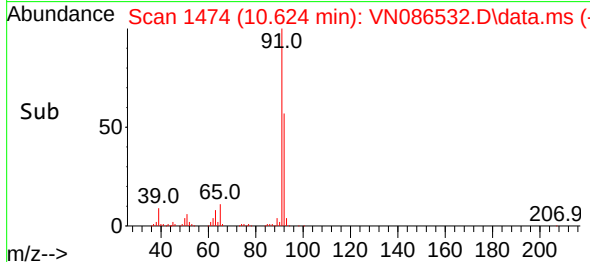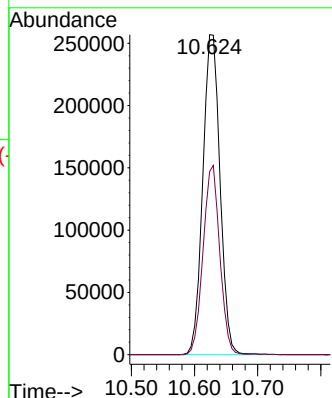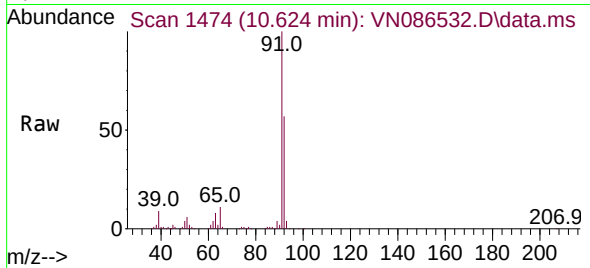

#63
Toluene-d8
Concen: 29.608 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.006 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion: 98 Resp: 395947
Ion Ratio Lower Upper
98 100
100 65.6 53.1 79.7


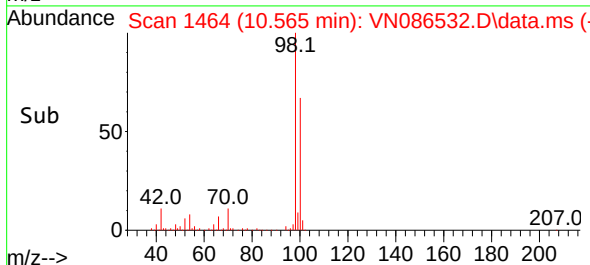
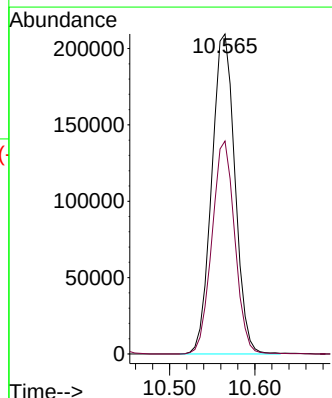
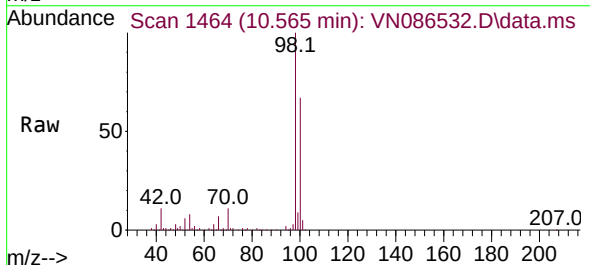


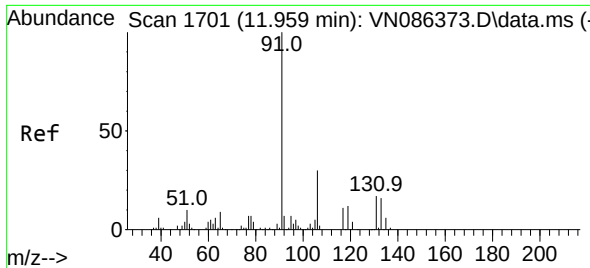

#66
Ethyl Benzene
Concen: 0.755 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. 0.006 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion: 91 Resp: 13831
Ion Ratio Lower Upper
91 100
106 30.6 24.3 36.5

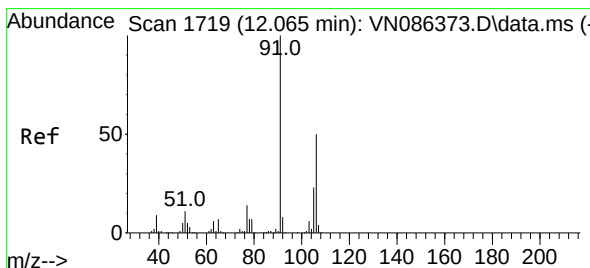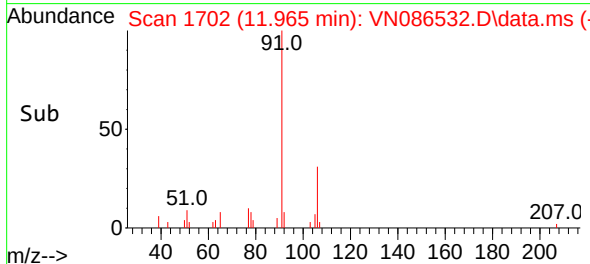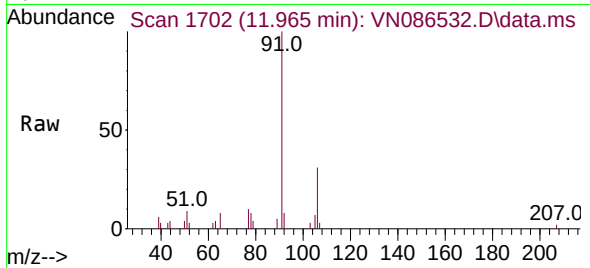

#67
m/p-Xylenes
Concen: 3.450 ug/l
RT: 12.065 min Scan# 1719
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion:106 Resp: 23972
Ion Ratio Lower Upper
106 100
91 197.8 162.6 243.8


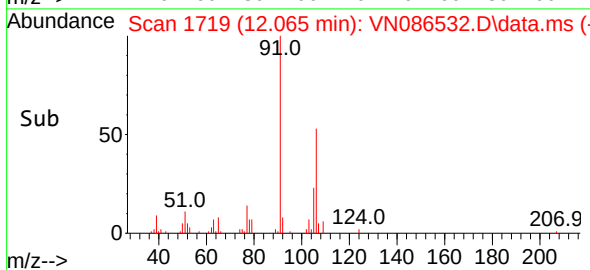

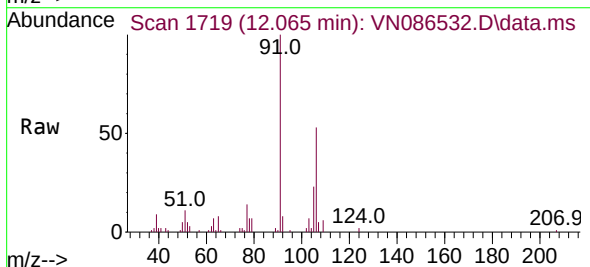




#68
o-Xylene
Concen: 1.423 ug/l
RT: 12.394 min Scan# 11
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)


Tgt Ion:106 Resp: 9682
Ion Ratio Lower Upper
106 100
91 231.5 110.6 331.6

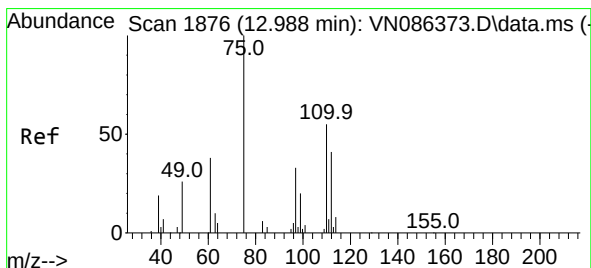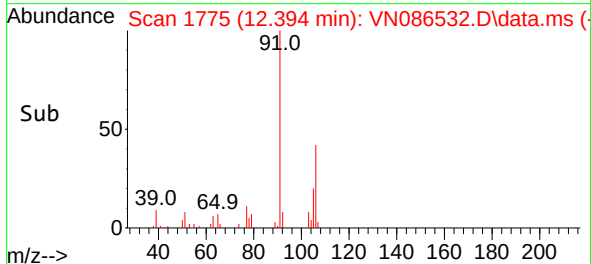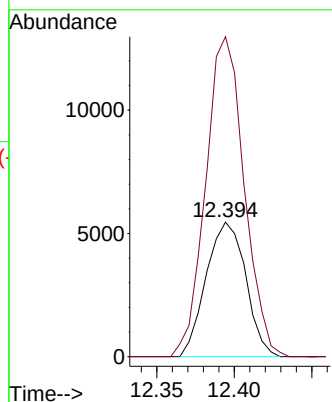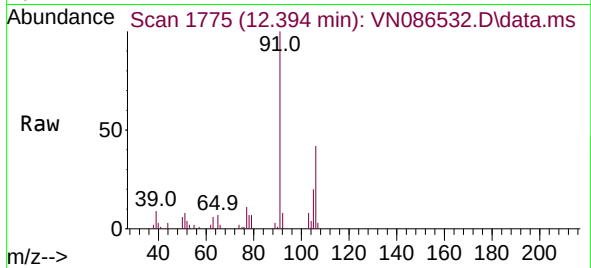

#72
1,2,3-Trichloropropane
Concen: 17.489 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.141 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion: 75 Resp: 68187
Ion Ratio Lower Upper
75 100
77 1.0 0.0 464.4


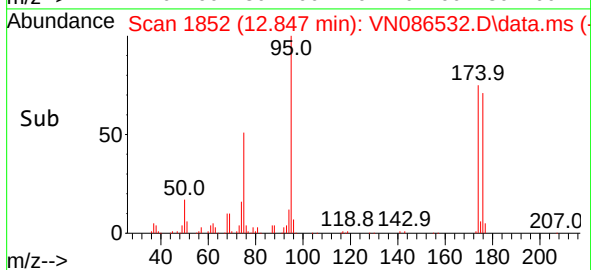
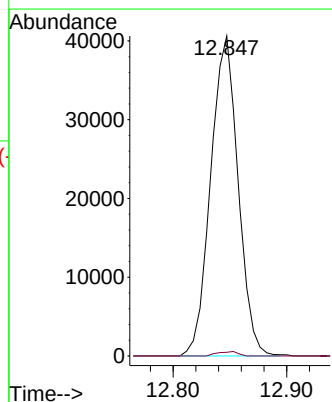
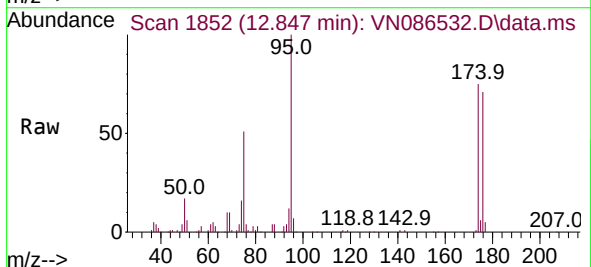




#77
 t-1,4-Dichloro-2-butene
 Concen: 34.460 ug/l
 RT: 12.847 min Scan# 11
 Delta R.T. 0.112 min
 Lab File: VN086532.D
 Acq: 07 May 2025 13:20




Instrument :
 MSVOA_N
 ClientSampleId :
 001-WILLETS-PT-BLVD(MAY)


Tgt Ion: 75 Resp: 68187
 Ion Ratio Lower Upper
 75 100
 53 0.0 46.0 138.0#
 89 0.0 21.6 64.6#

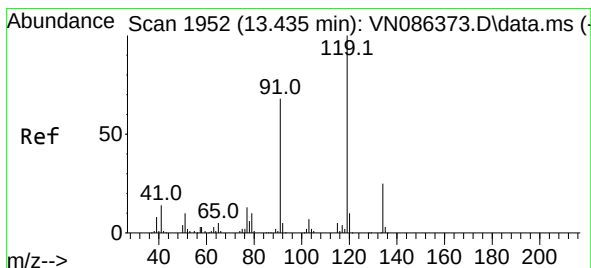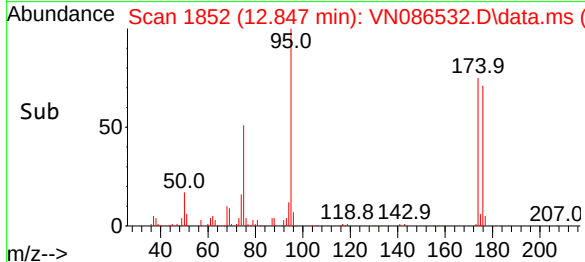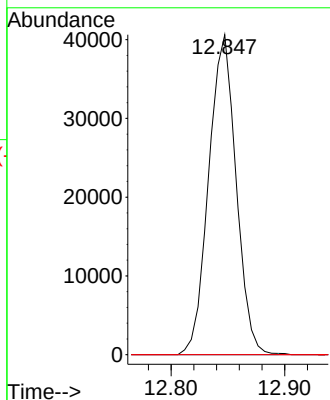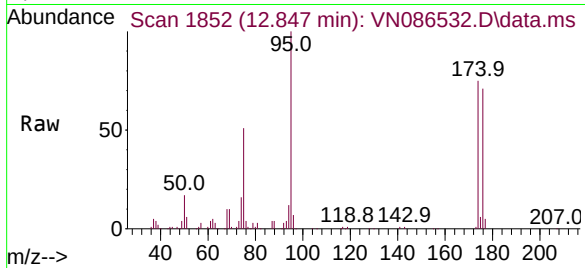

#79
 tert-butylbenzene
 Concen: 0.423 ug/l
 RT: 13.724 min Scan# 2001
 Delta R.T. 0.288 min
 Lab File: VN086532.D
 Acq: 07 May 2025 13:20

Tgt Ion: 119 Resp: 5048
 Ion Ratio Lower Upper
 119 100
 91 23.6 0.0 137.4
 134 27.8 0.0 49.2


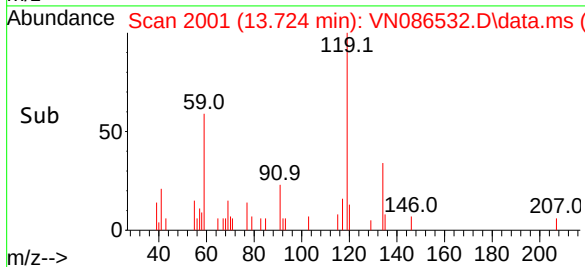
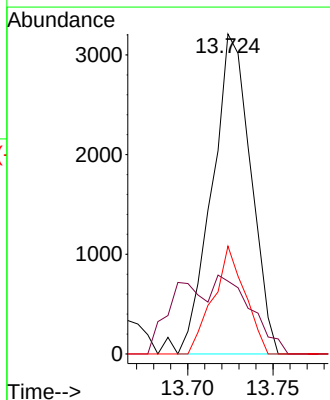
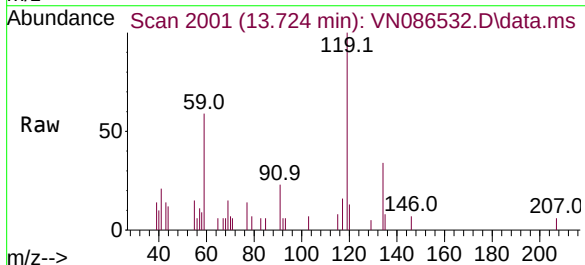


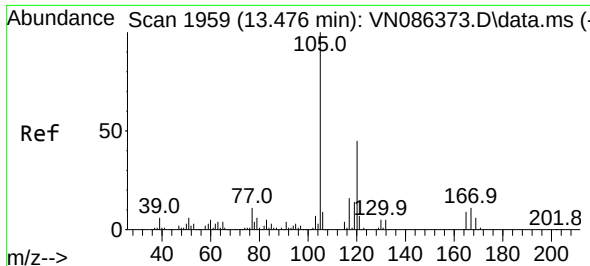

#80
1,2,4-Trimethylbenzene
Concen: 0.701 ug/l
RT: 13.477 min Scan# 1959
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20




Instrument : MSVOA_N
ClientSampleId : 001-WILLETS-PT-BLVD(MAY)


Tgt Ion:105 Resp: 9973
Ion Ratio Lower Upper
105 100
120 30.7 0.0 87.6

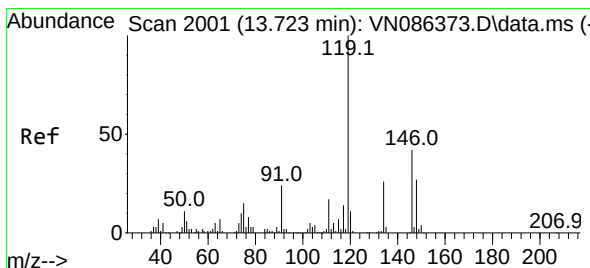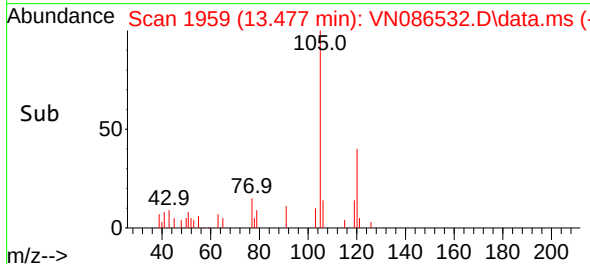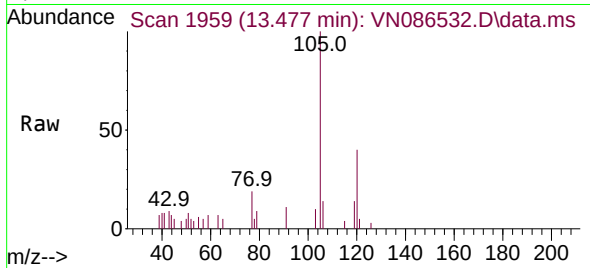

#82
p-Isopropyltoluene
Concen: 0.354 ug/l
RT: 13.724 min Scan# 2001
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion:119 Resp: 5048
Ion Ratio Lower Upper
119 100
134 27.8 0.0 52.2
91 23.6 0.0 47.6


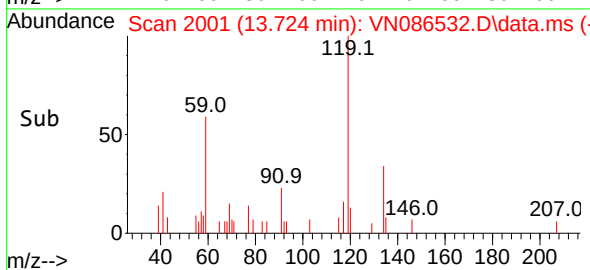

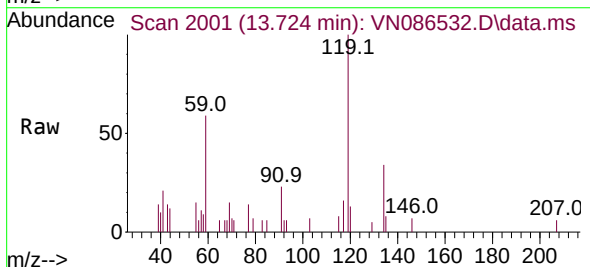




#90
Hexachlorobutadiene
Concen: 0.399 ug/l
RT: 15.506 min Scan# 2304
Delta R.T. 0.012 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Instrument :
MSVOA_N
ClientSampleId :
001-WILLETS-PT-BLVD(MAY)

Tgt Ion:225	Resp:	514
Ion Ratio	Lower	Upper
225	100	
223	34.4	0.0 128.8
227	35.4	0.0 120.2

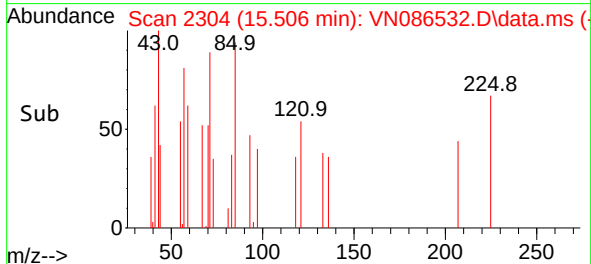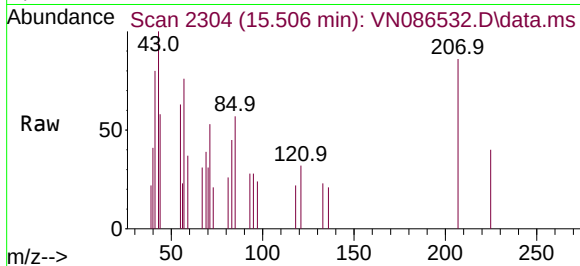

#91
Naphthalene
Concen: 0.451 ug/l
RT: 15.635 min Scan# 2326
Delta R.T. 0.000 min
Lab File: VN086532.D
Acq: 07 May 2025 13:20

Tgt Ion:128	Resp:	5170
Ion Ratio	Lower	Upper
128	100	
127	7.0	10.6 15.8#
129	5.2	8.7 13.1#

