



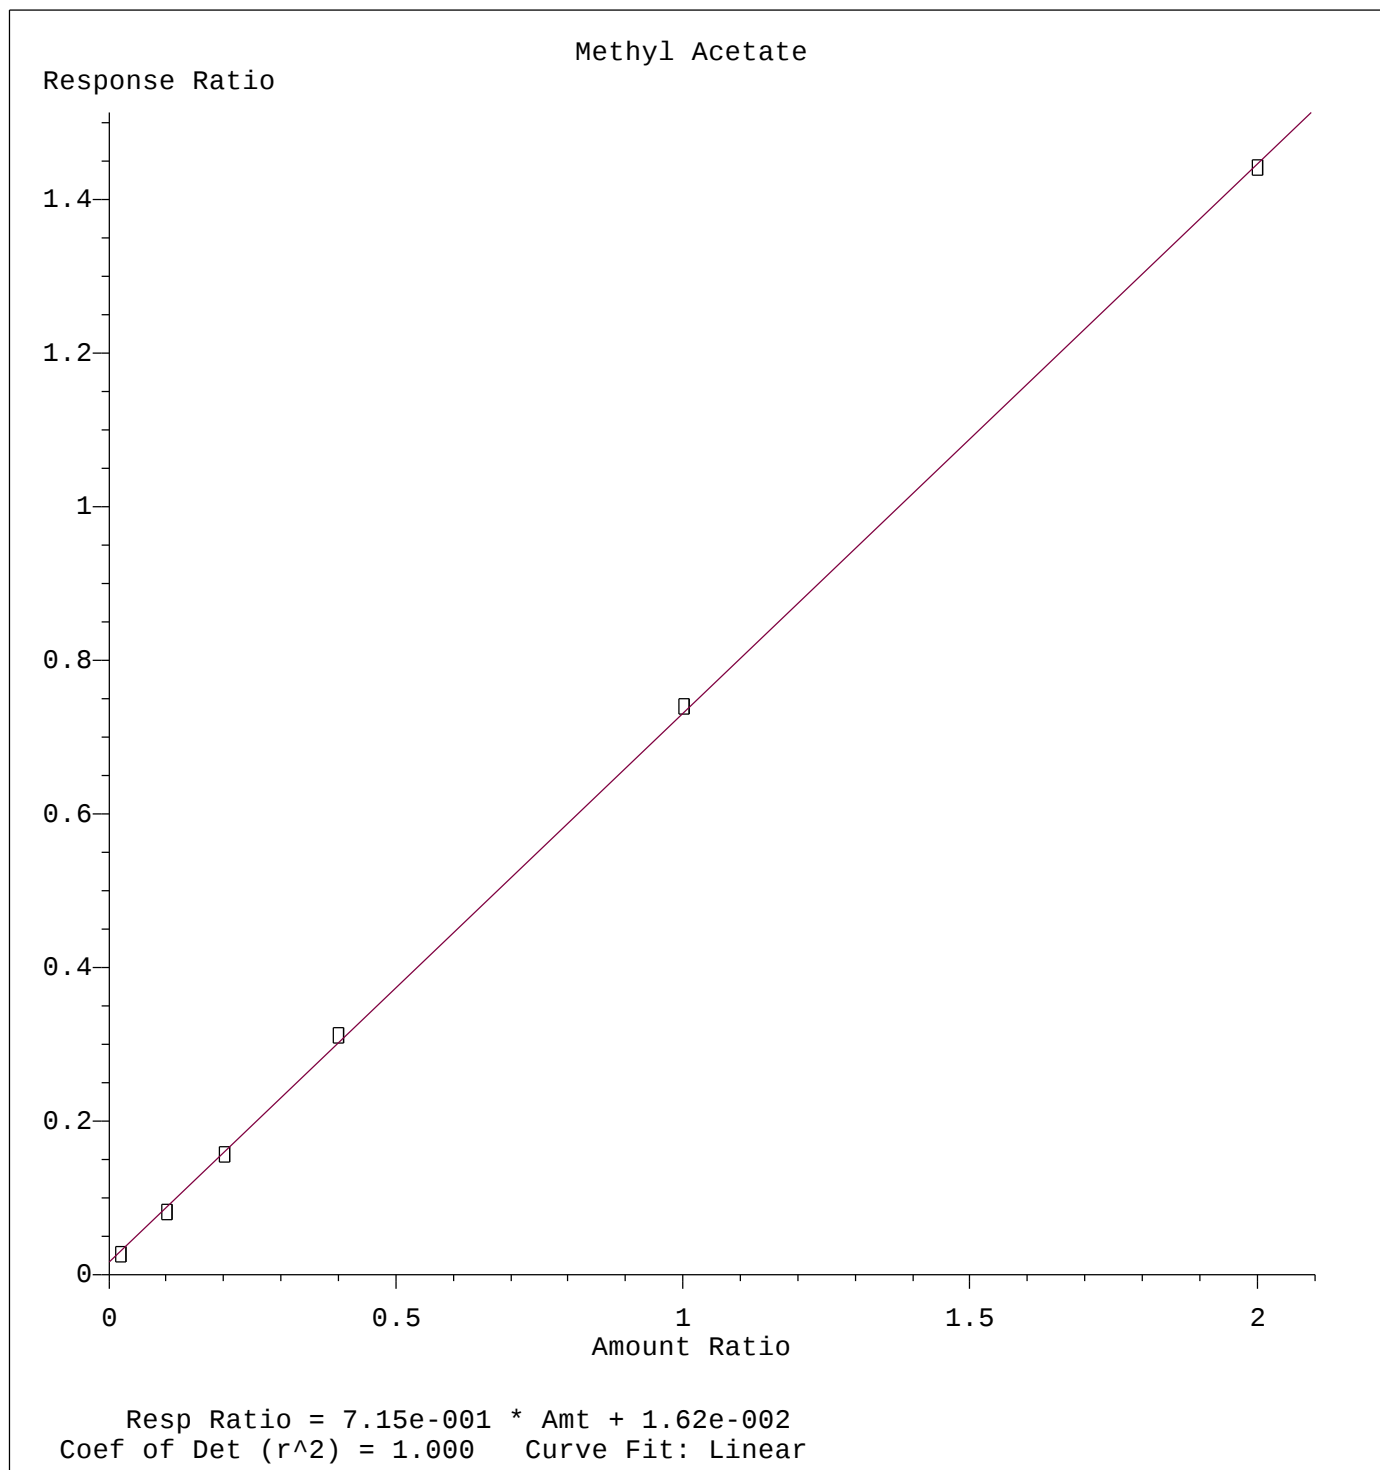

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Calibration Table Last Updated: Fri May 10 06:48:32 2019

2-Chloroethyl Vinyl ether

Response Ratio

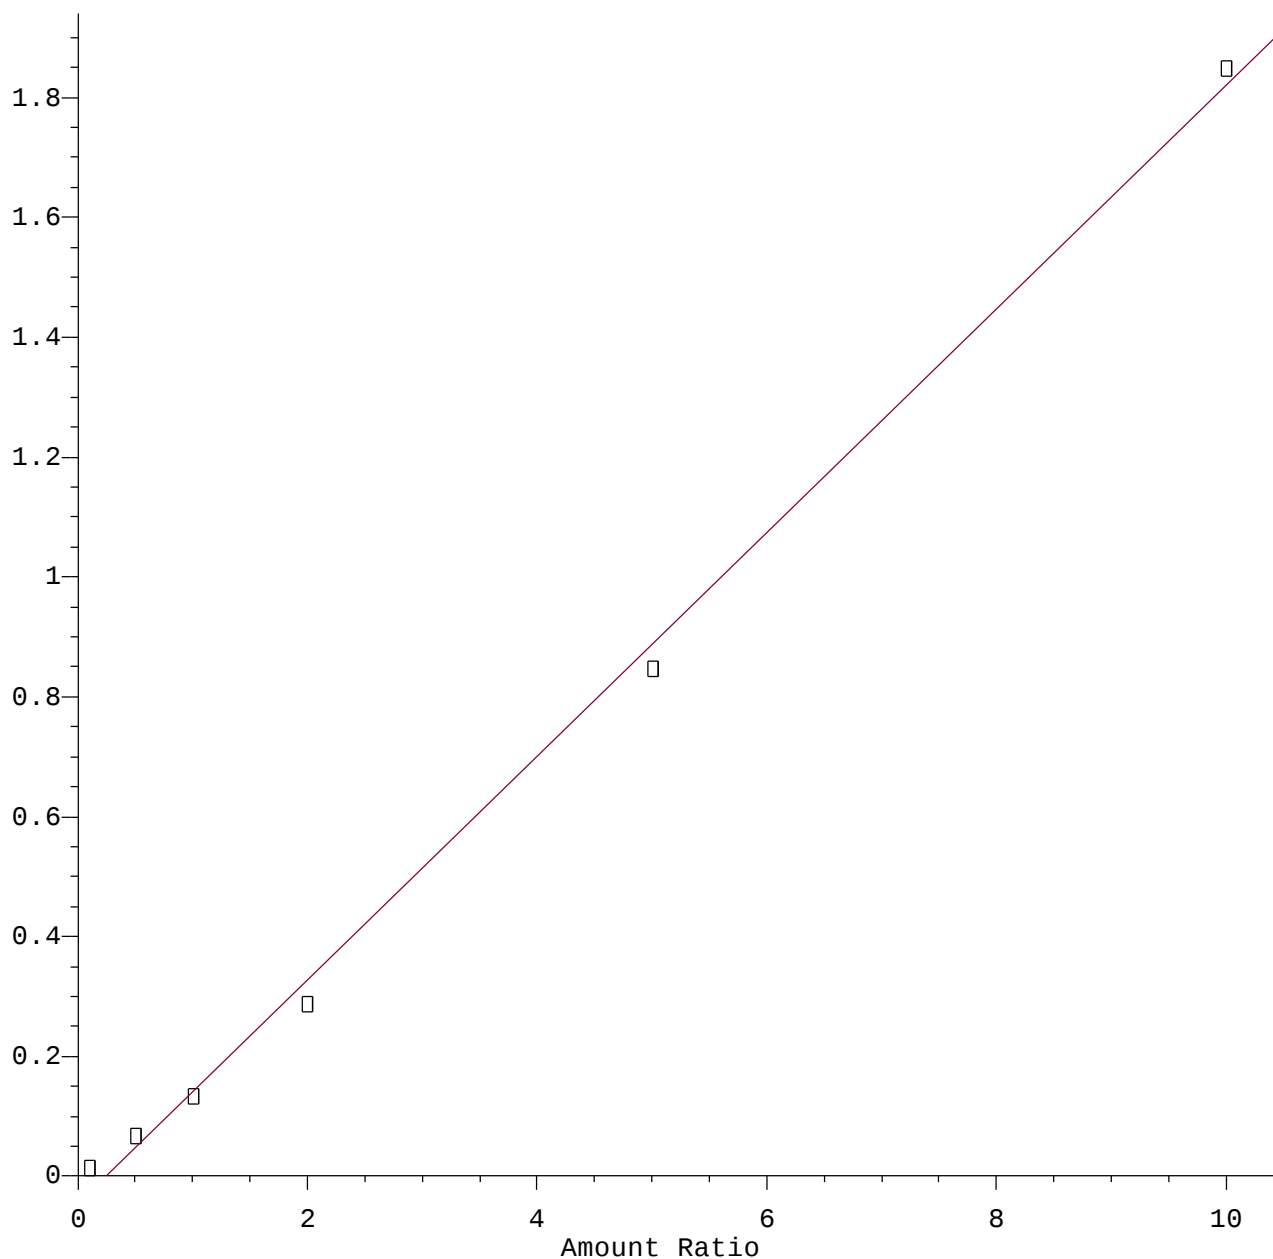


Resp Ratio = $1.87 \times 10^{-1} \times \text{Amt} - 4.67 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Calibration Table Last Updated: Fri May 10 06:48:32 2019

Isopropylbenzene

Response Ratio

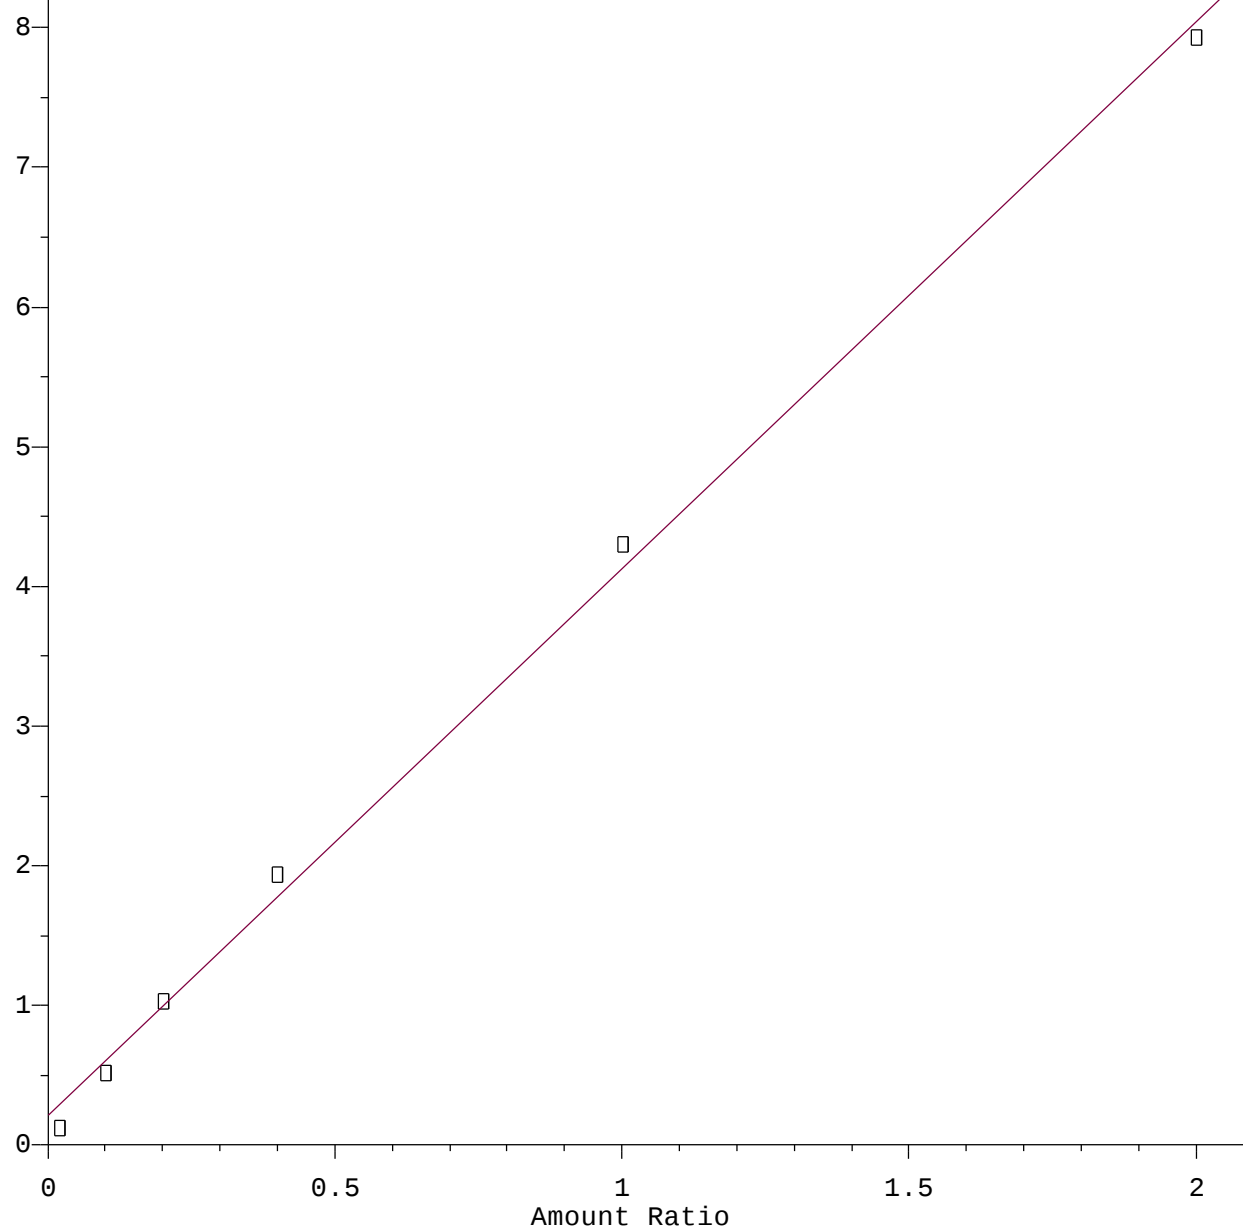


Resp Ratio = $3.92 \times 10^0 \times \text{Amt} + 2.07 \times 10^{-1}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Calibration Table Last Updated: Fri May 10 06:48:32 2019

1,1,2,2-Tetrachloroethane

Response Ratio

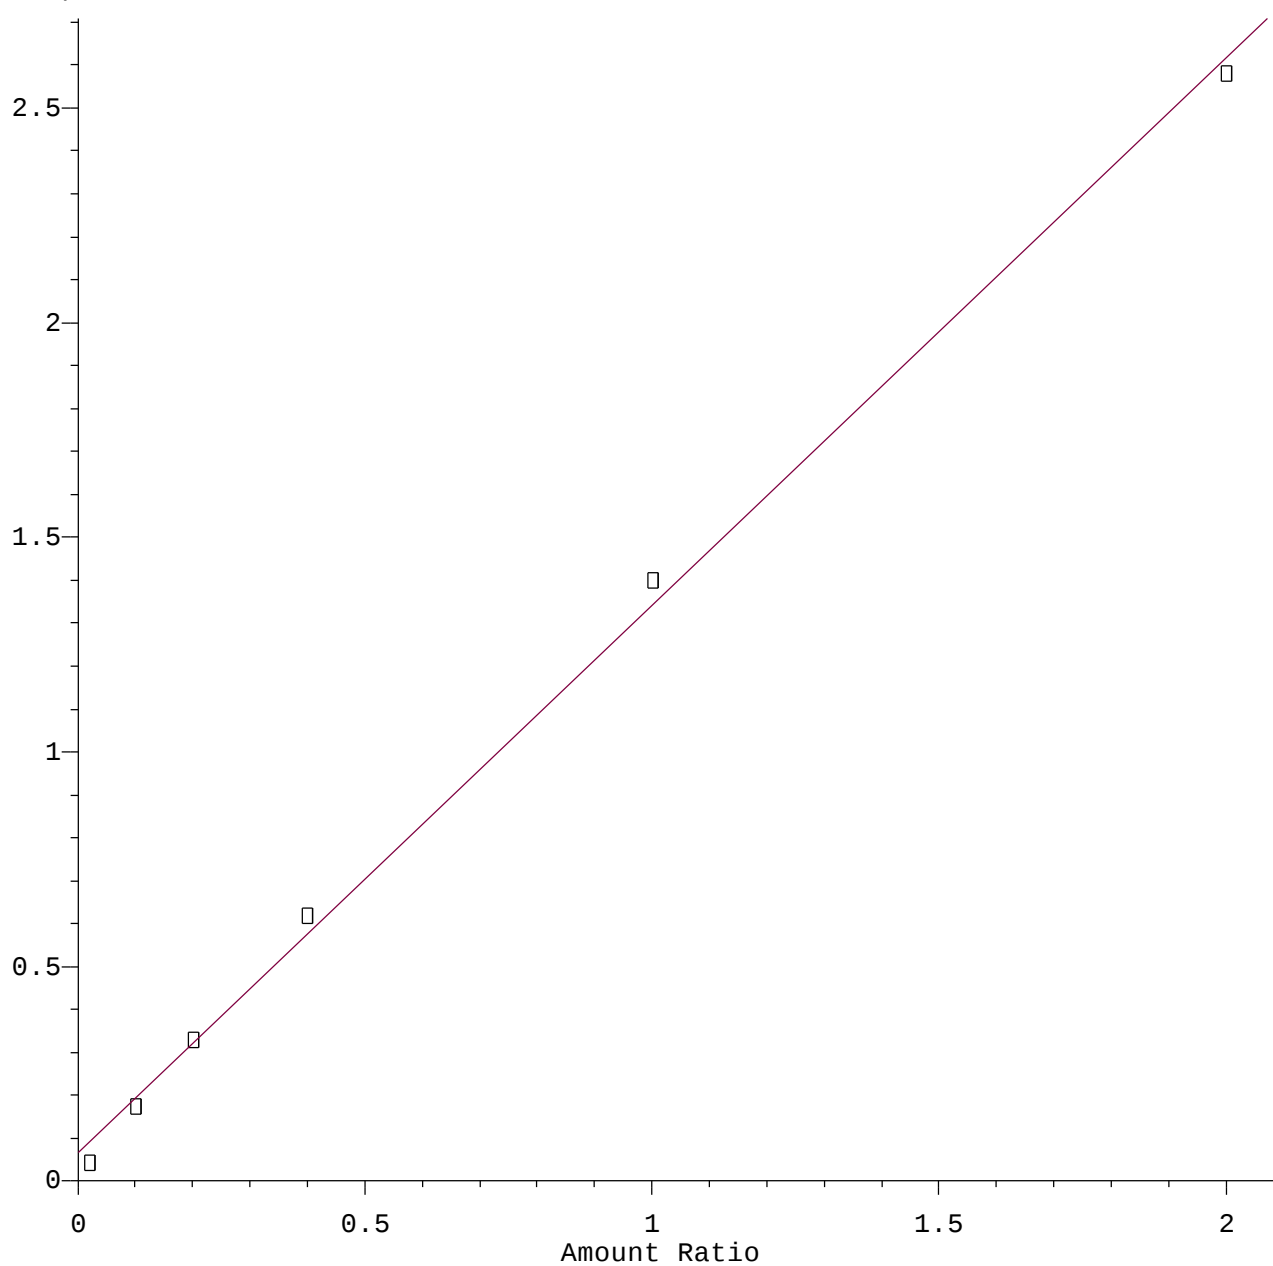


Resp Ratio = 1.27e+000 * Amt + 6.56e-002
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Calibration Table Last Updated: Fri May 10 06:48:32 2019


1,2,4-Trichlorobenzene

Response Ratio

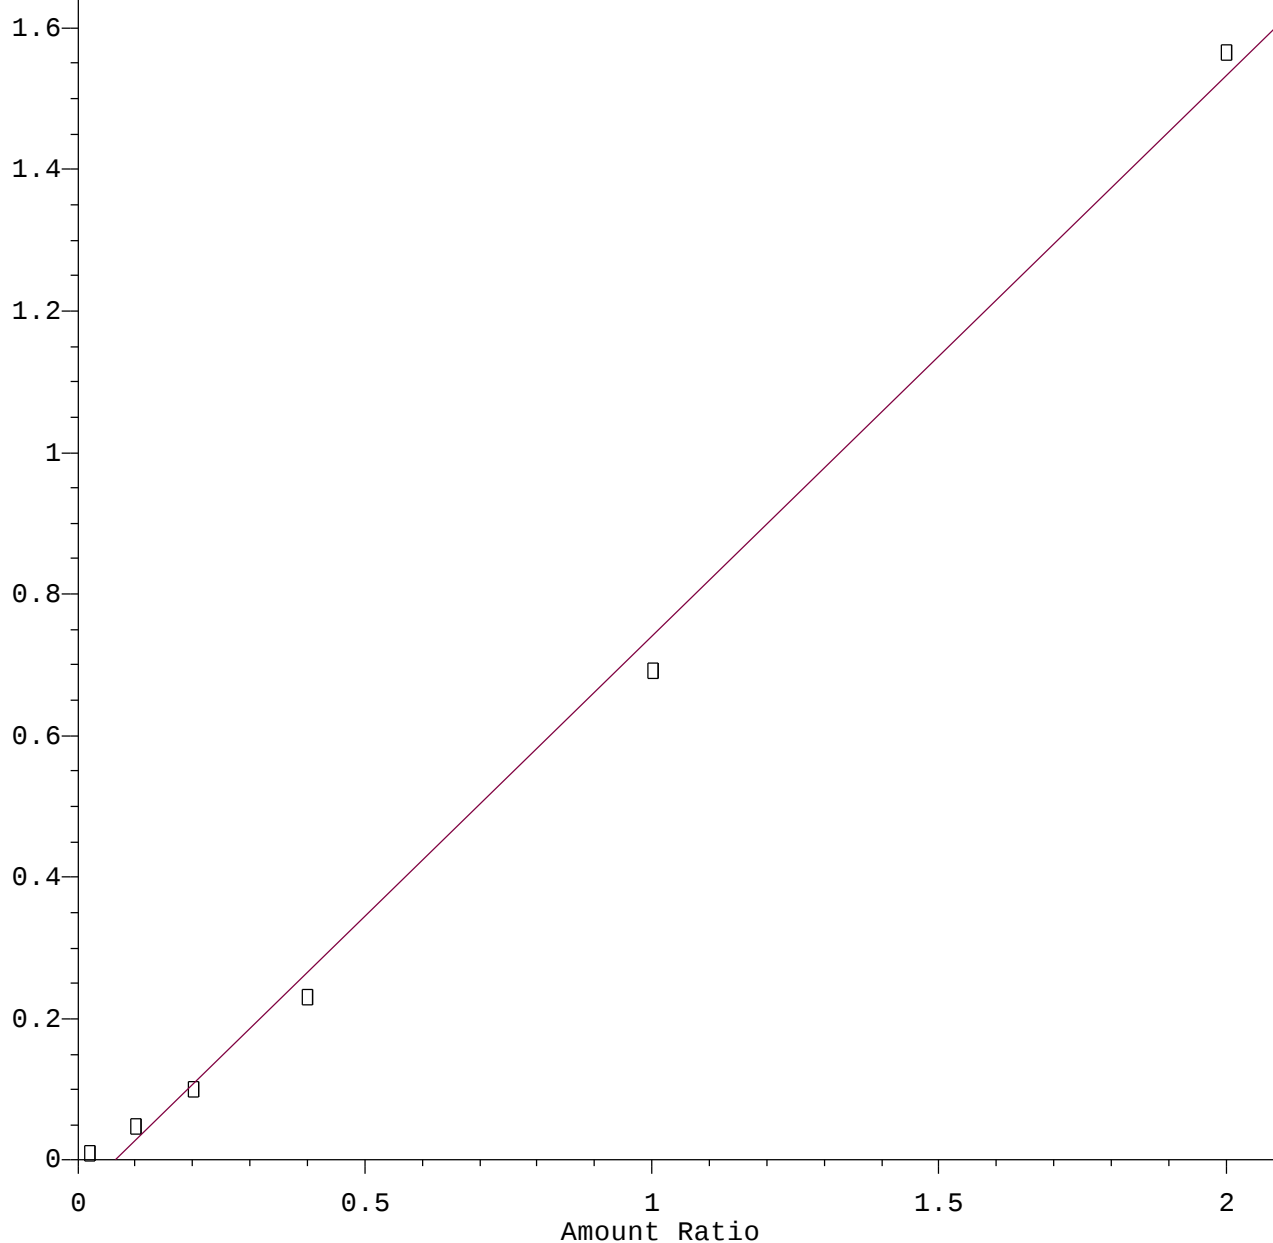


Resp Ratio = $7.92 \times 10^{-1} \times \text{Amt} - 5.08 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Calibration Table Last Updated: Fri May 10 06:48:32 2019

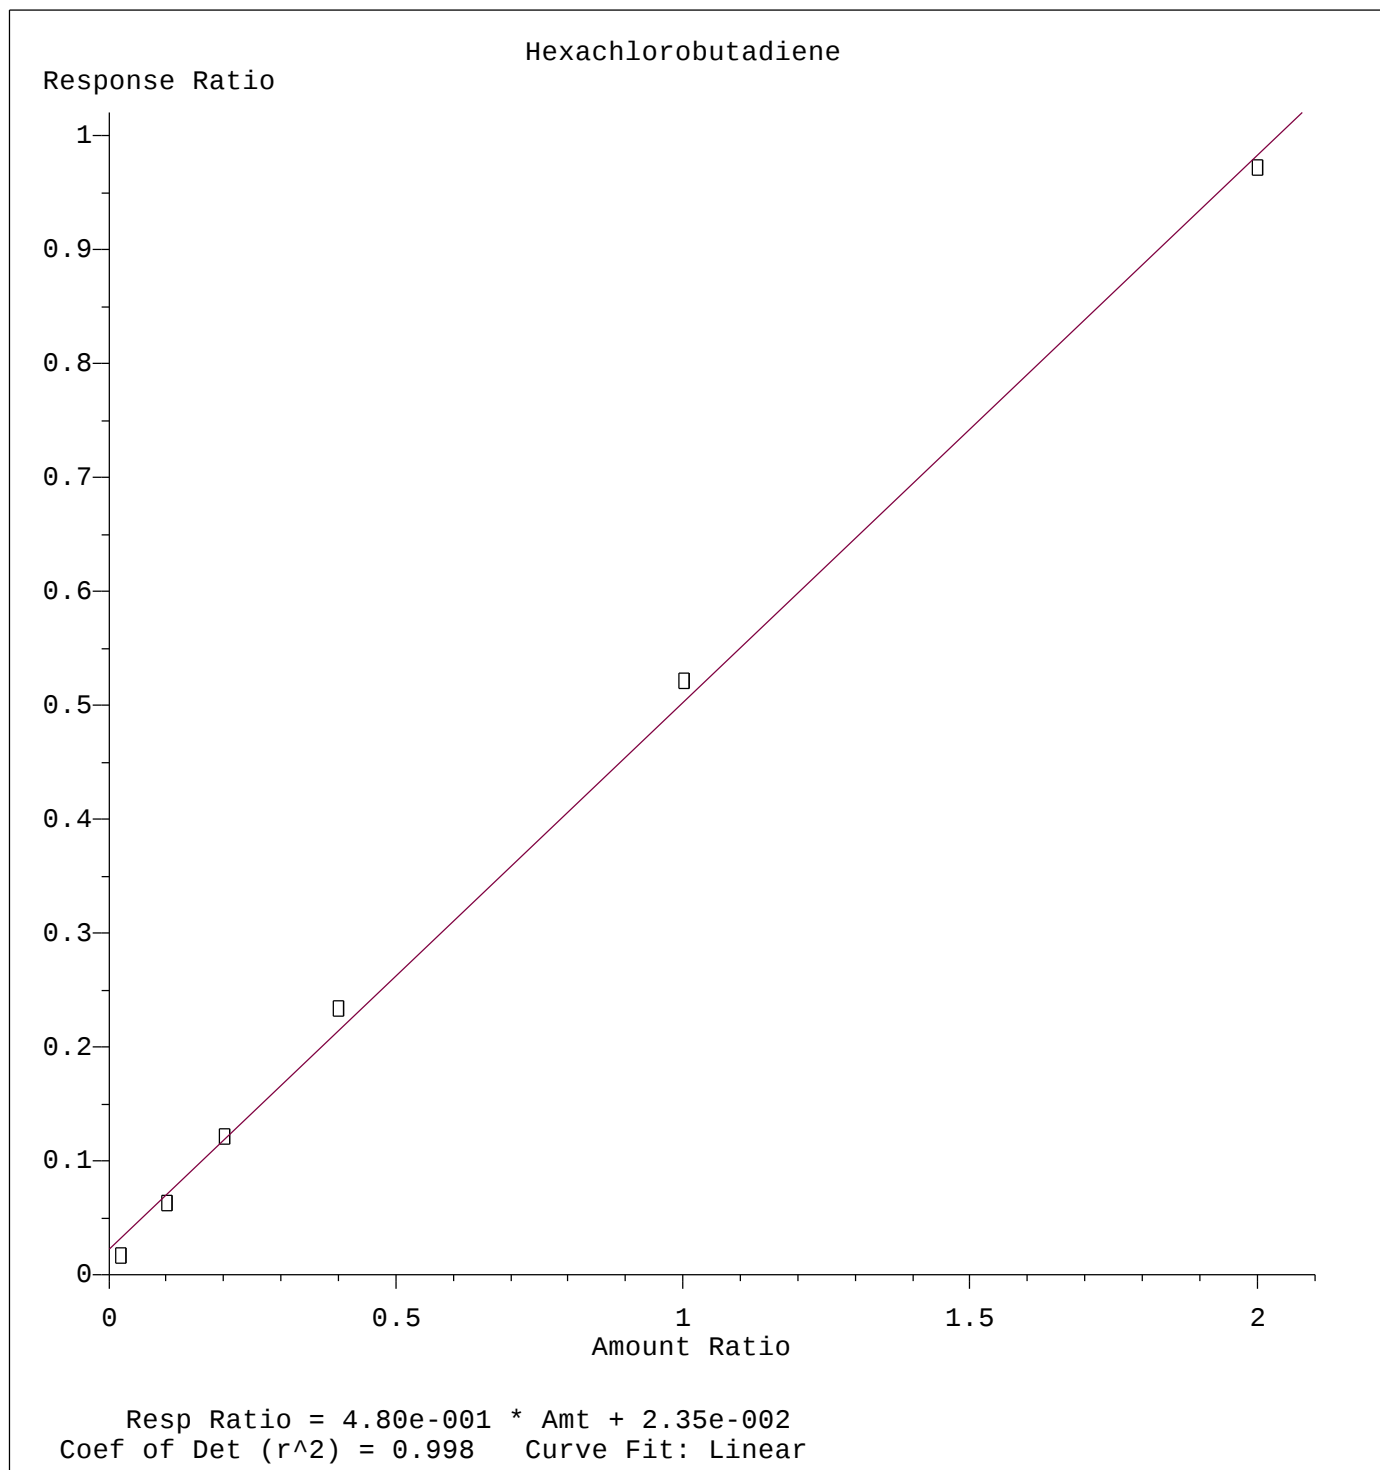


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Calibration Table Last Updated: Fri May 10 06:48:32 2019

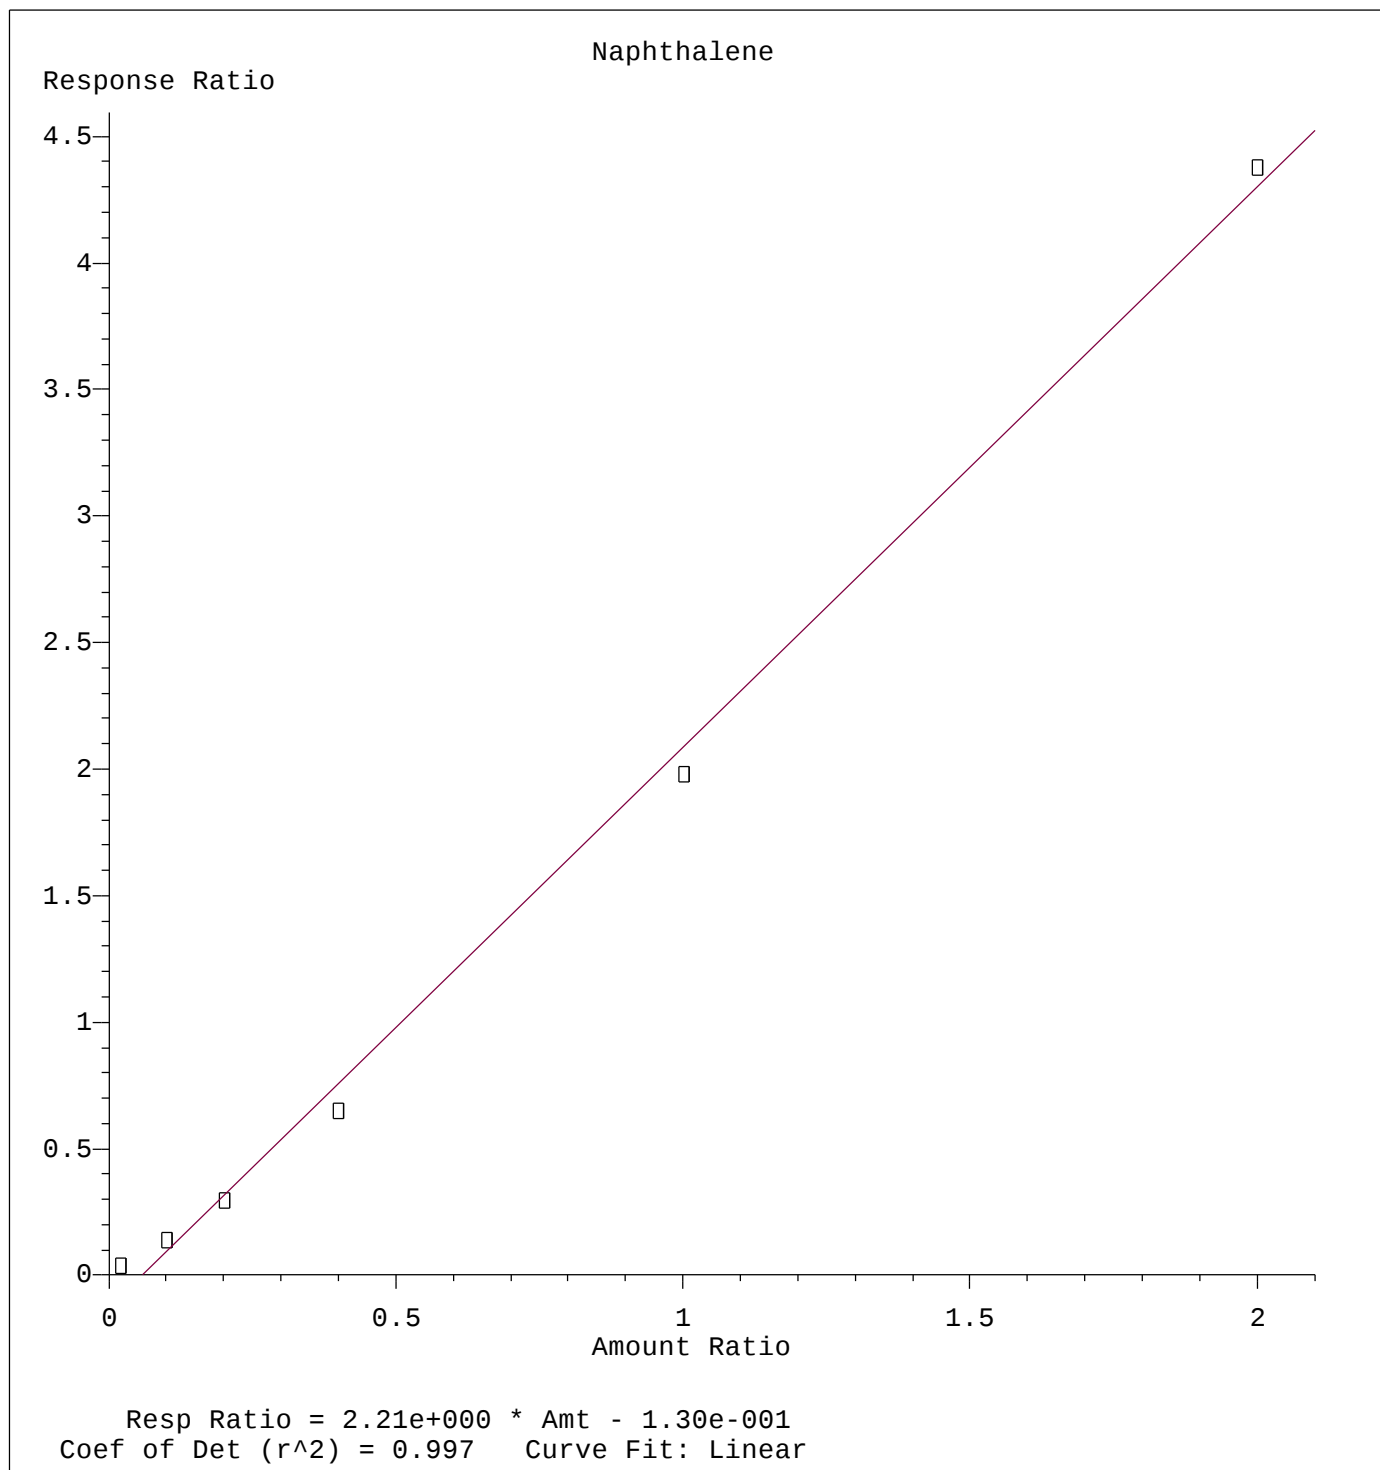

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Calibration Table Last Updated: Fri May 10 06:48:32 2019

1,2,3-Trichlorobenzene

Response Ratio

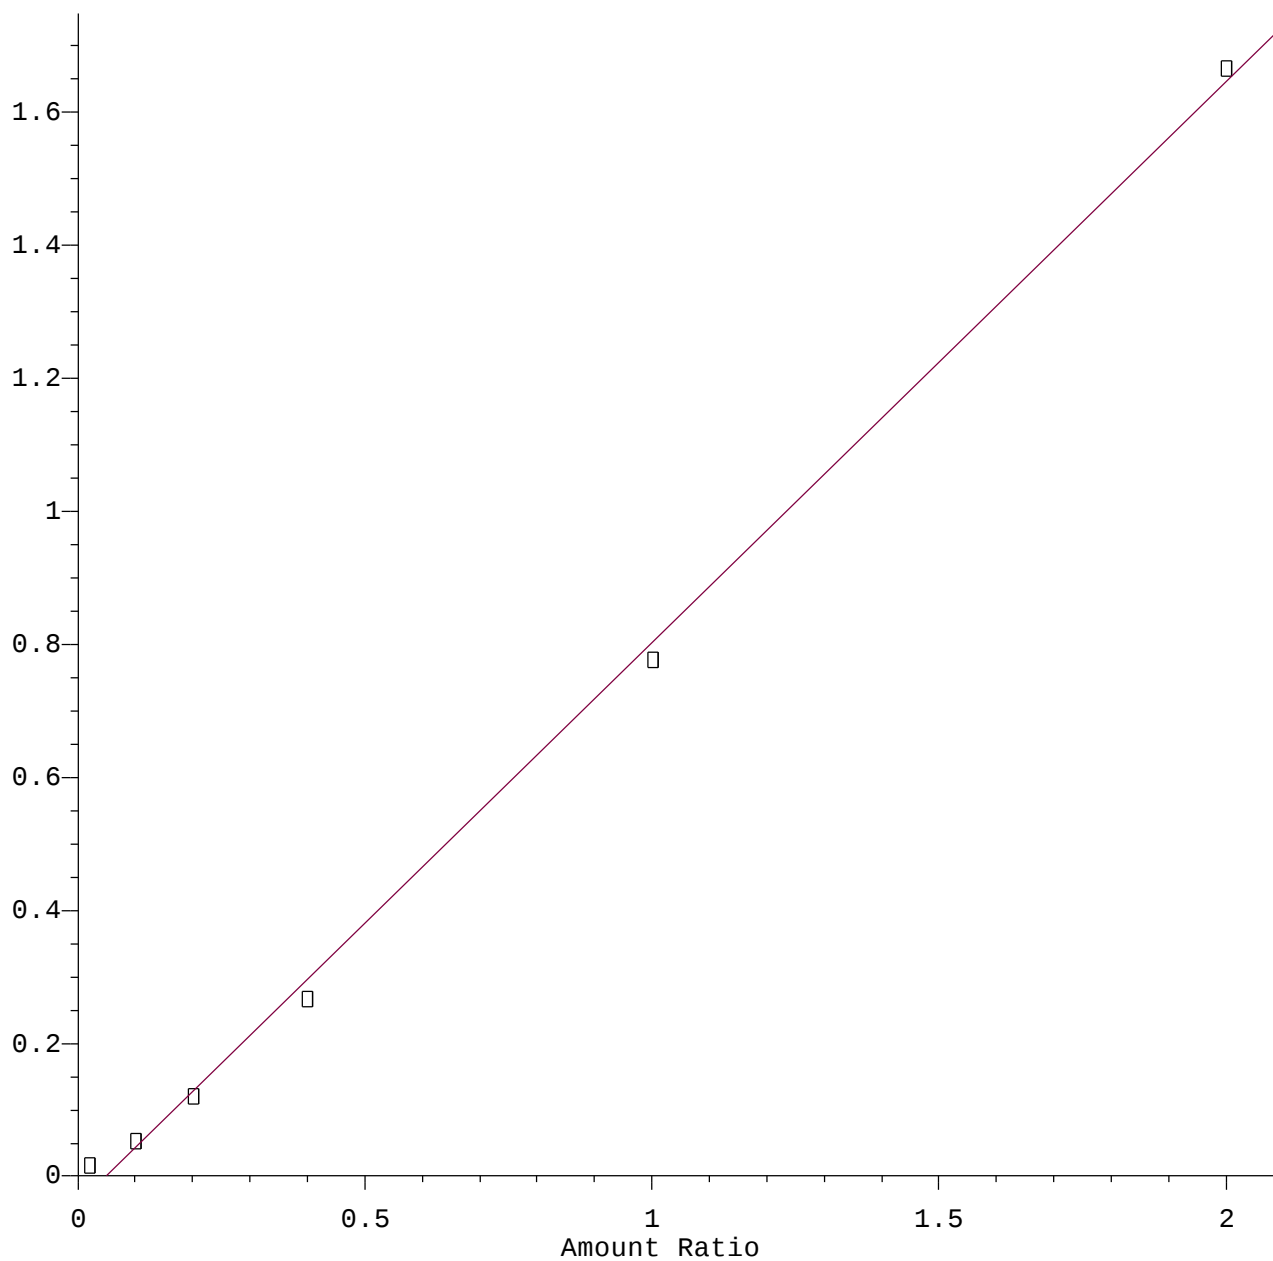

Resp Ratio = $8.43 \times 10^{-1} \times \text{Amt} - 4.09 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Calibration Table Last Updated: Fri May 10 06:48:32 2019