


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN050819\
Data File : VN055476.D
Acq On : 8 May 2019 15:02
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Title : SW846 8260
Last Update : Fri May 10 06:48:32 2019

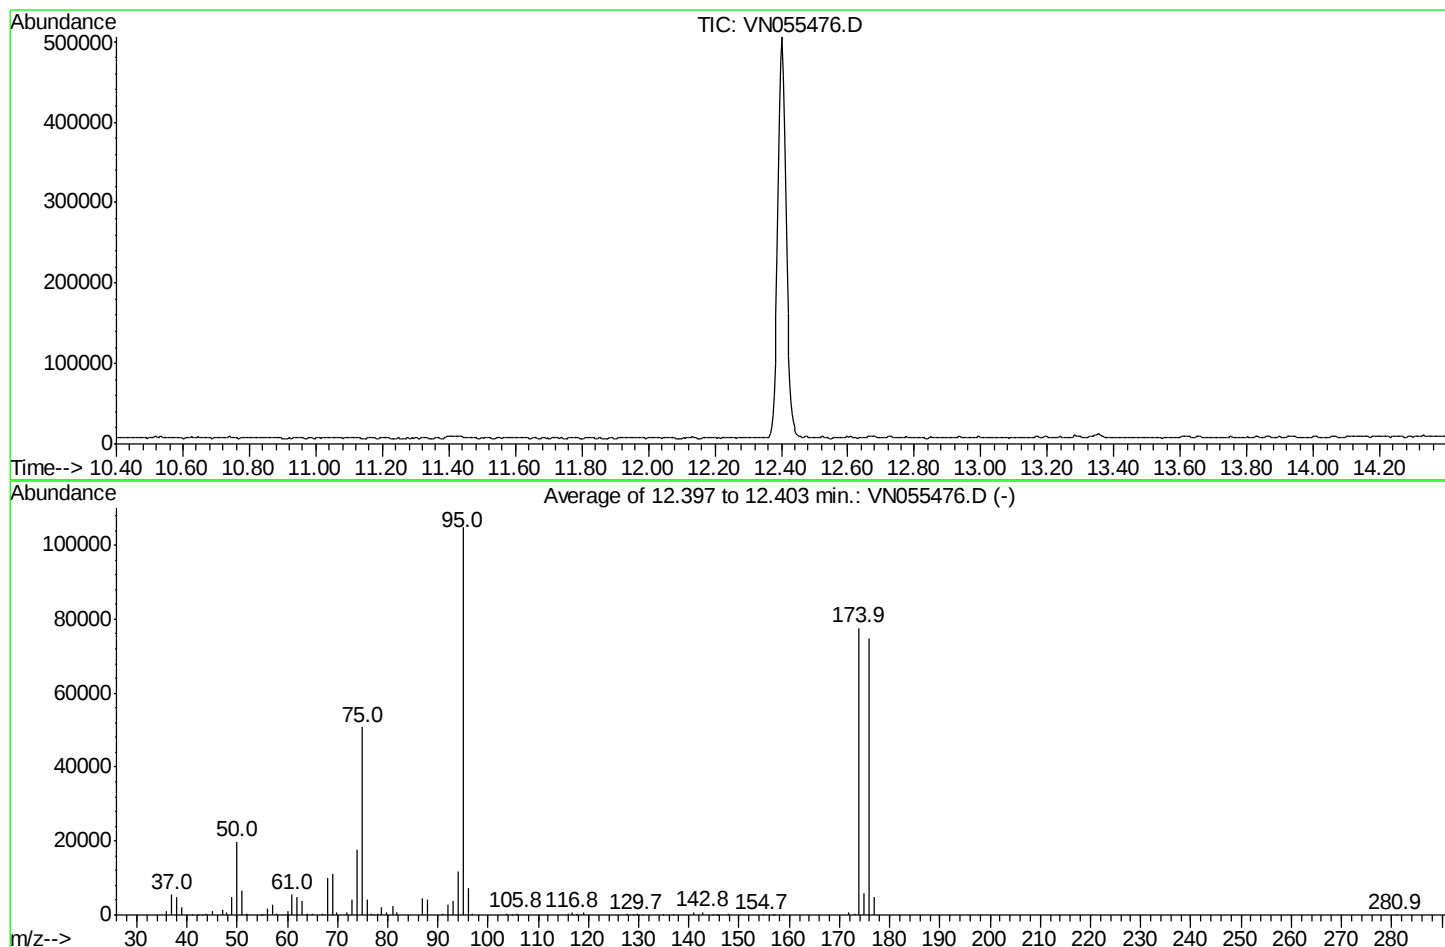

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	19749	PASS
75	95	30	60	48.4	50749	PASS
95	95	100	100	100.0	104810	PASS
96	95	5	9	7.0	7339	PASS
173	174	0.00	2	0.4	327	PASS
174	95	50	100	74.1	77629	PASS
175	174	5	9	7.6	5888	PASS
176	174	95	101	96.4	74826	PASS
177	176	5	9	6.7	4987	PASS