


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN050820\
 Data File : VN061349.D
 Acq On : 8 May 2020 9:34
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
 Title : SW846 8260
 Last Update : Tue May 05 07:01:08 2020

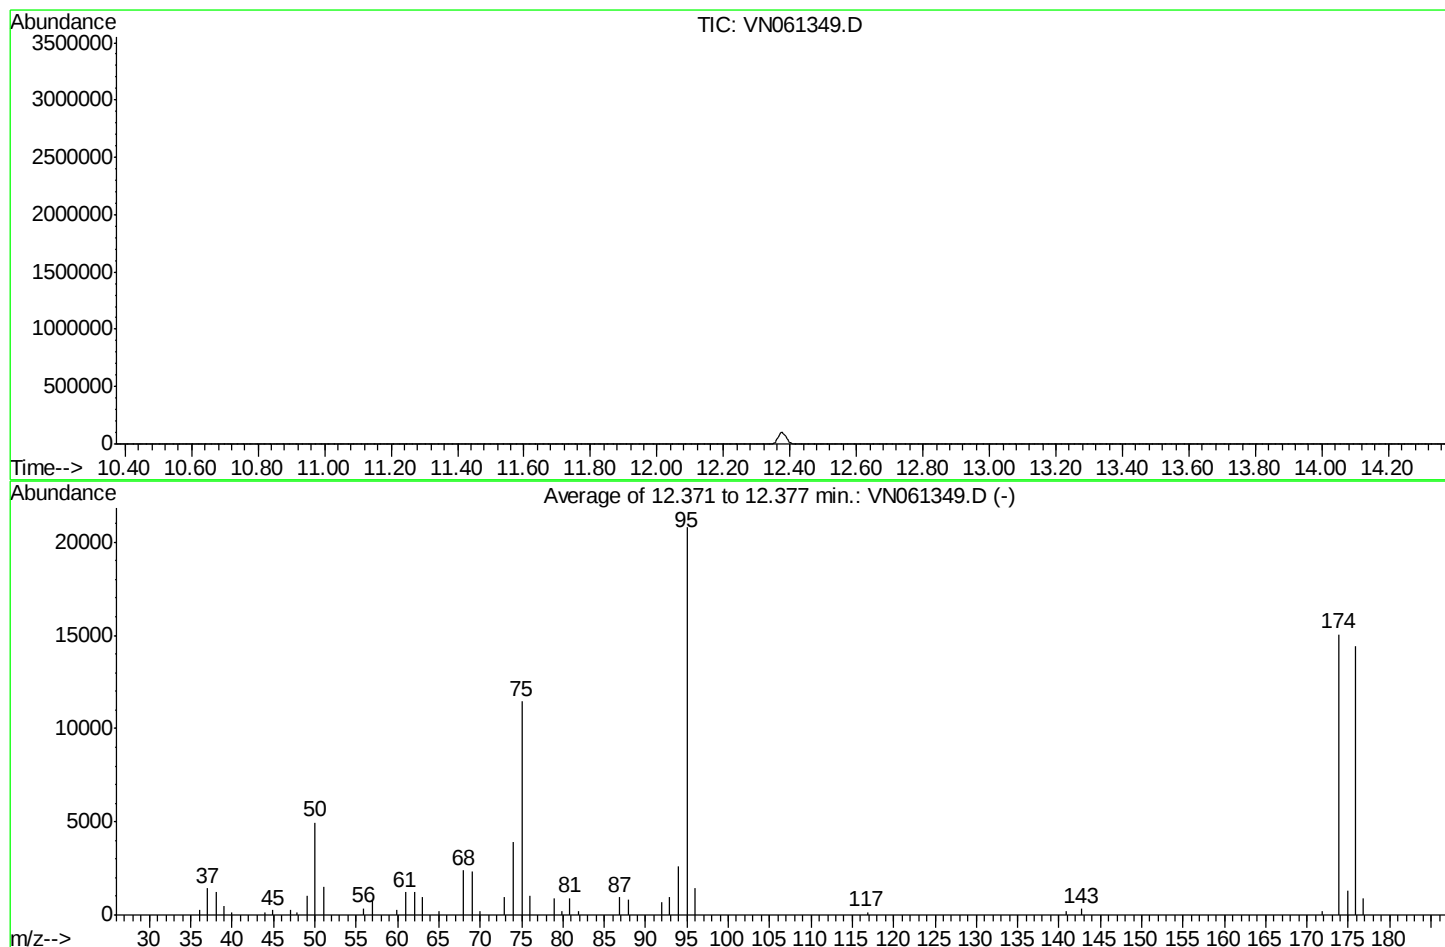

AutoFind: Scans 3353, 3354, 3355; Background Corrected with Scan 3341

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	4947	PASS
75	95	30	60	55.0	11441	PASS
95	95	100	100	100.0	20797	PASS
96	95	5	9	6.9	1430	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.4	15066	PASS
175	174	5	9	8.6	1291	PASS
176	174	95	101	95.7	14416	PASS
177	176	5	9	6.3	902	PASS