


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN050821\  
Data File : VN067046.D  
Acq On : 7 May 2021 9:09  
Operator : JC/MD  
Sample : BFB  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\624N050721W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Fri May 07 07:26:20 2021

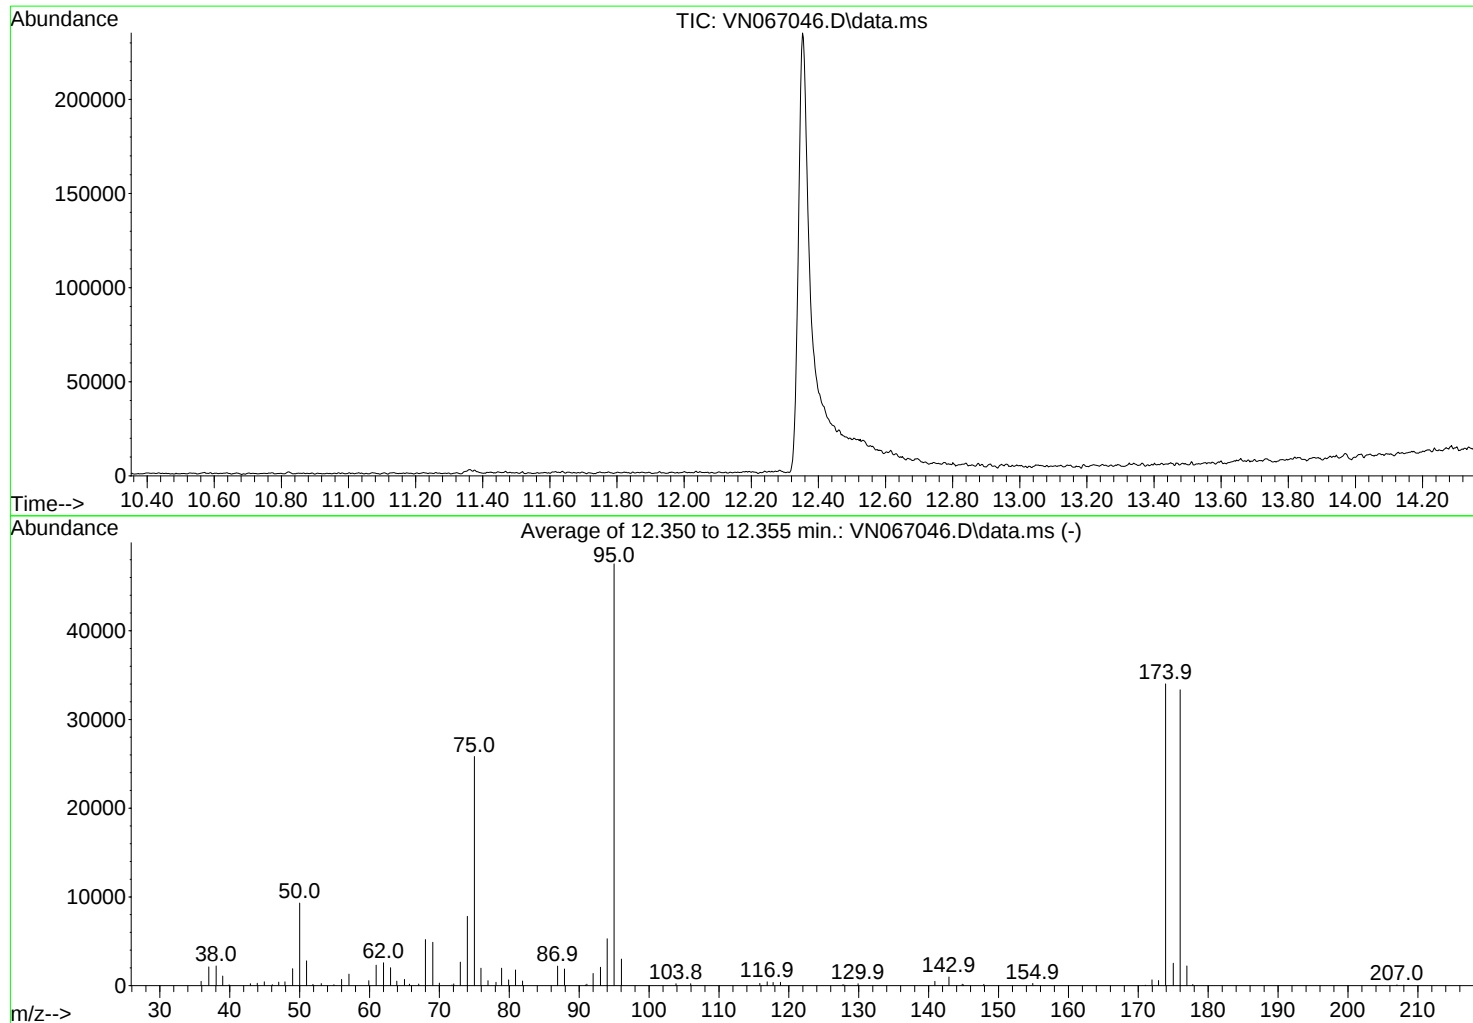

AutoFind: Scans 3950, 3951, 3952; Background Corrected with Scan 3936

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.6  | 9302  | PASS      |
| 75     | 95      | 30     | 60     | 54.3  | 25829 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 47544 | PASS      |
| 96     | 95      | 5      | 9      | 6.3   | 2989  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.7   | 586   | PASS      |
| 174    | 95      | 50     | 100    | 71.6  | 34019 | PASS      |
| 175    | 174     | 5      | 9      | 7.4   | 2522  | PASS      |
| 176    | 174     | 95     | 101    | 98.0  | 33355 | PASS      |
| 177    | 176     | 5      | 9      | 6.6   | 2213  | PASS      |