


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN050821\  
Data File : VN067046.D  
Acq On : 7 May 2021 9:09  
Operator : JC/MD  
Sample : BFB  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N050421W.M  
Title : SW846 8260  
Last Update : Wed May 05 07:24:52 2021

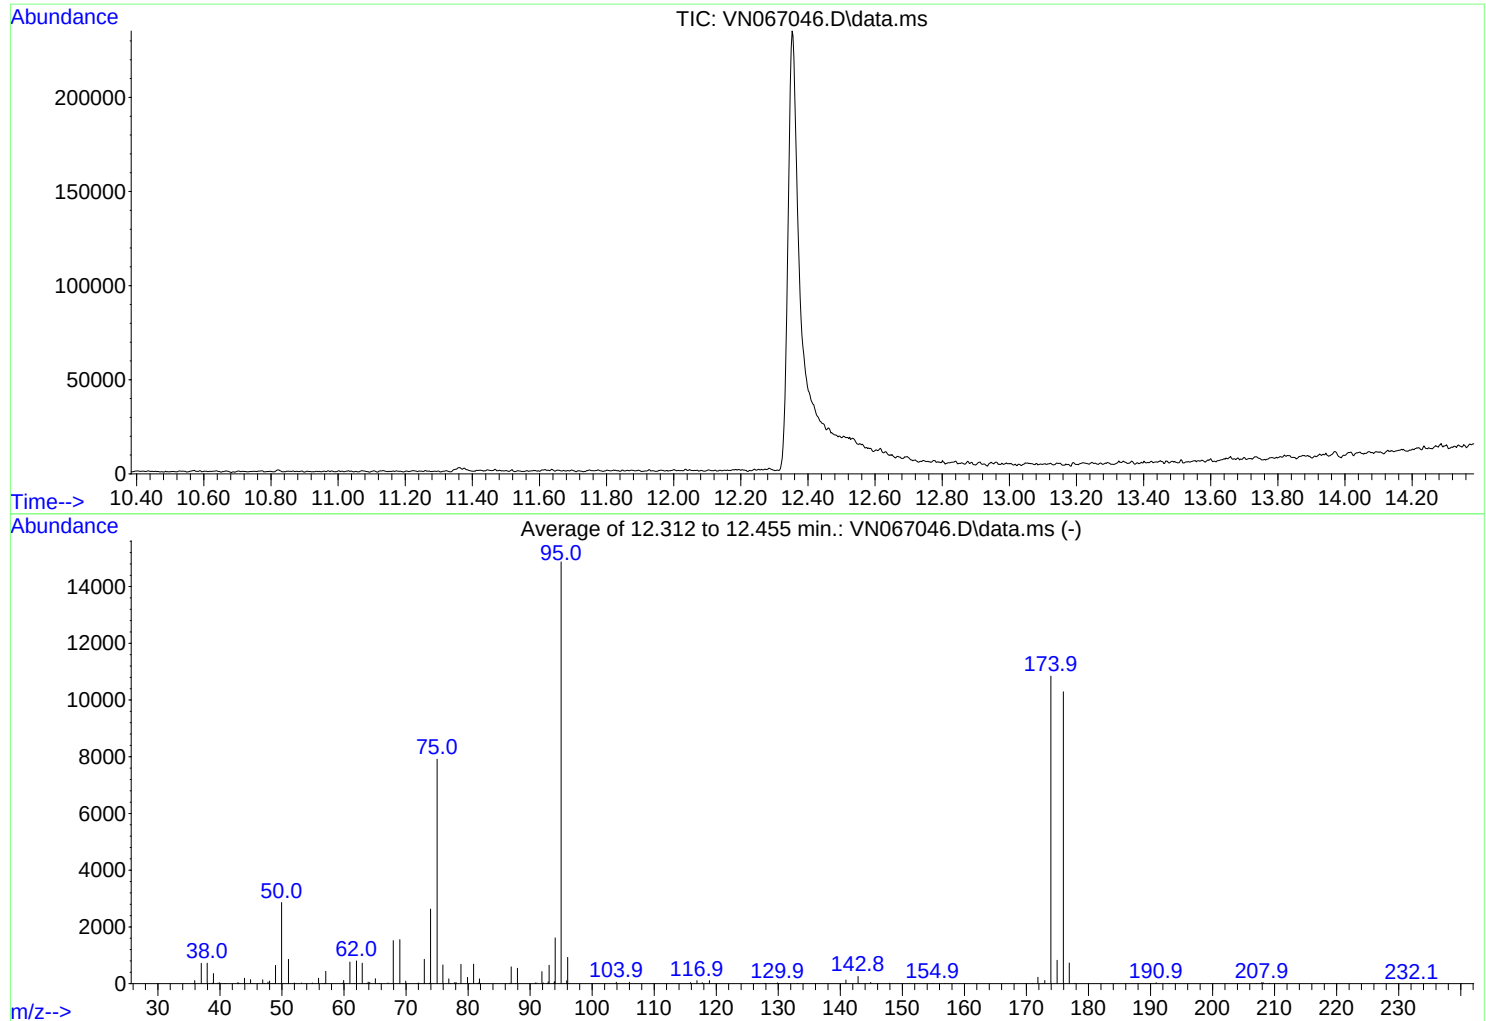

AutoFind: Averaged scan 3936 to 3989; Bkg corrected with scan 3935

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.2  | 2862  | PASS      |
| 75     | 95      | 30     | 60     | 53.2  | 7917  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 14872 | PASS      |
| 96     | 95      | 5      | 9      | 6.2   | 923   | PASS      |
| 173    | 174     | 0.00   | 2      | 1.0   | 113   | PASS      |
| 174    | 95      | 50     | 100    | 72.9  | 10844 | PASS      |
| 175    | 174     | 5      | 9      | 7.6   | 824   | PASS      |
| 176    | 174     | 95     | 101    | 94.9  | 10292 | PASS      |
| 177    | 176     | 5      | 9      | 7.1   | 726   | PASS      |