


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050821\
 Data File : VN067046.D
 Acq On : 7 May 2021 9:09
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050721W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri May 07 07:26:20 2021

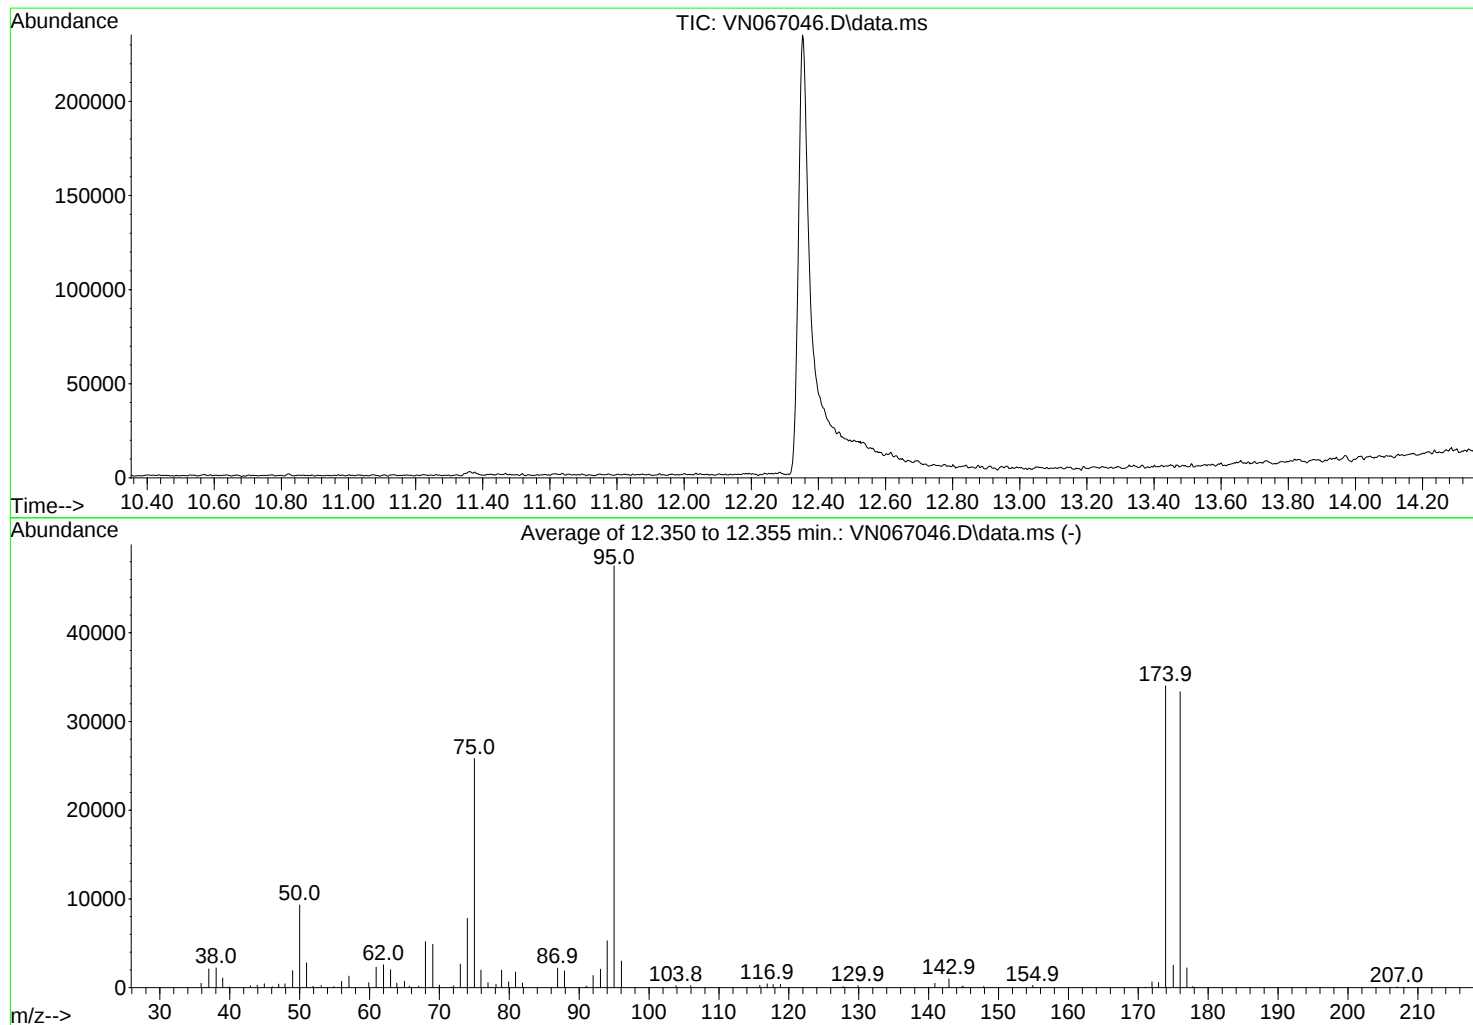

AutoFind: Scans 3950, 3951, 3952; Background Corrected with Scan 3936

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	9302	PASS
75	95	30	60	54.3	25829	PASS
95	95	100	100	100.0	47544	PASS
96	95	5	9	6.3	2989	PASS
173	174	0.00	2	1.7	586	PASS
174	95	50	100	71.6	34019	PASS
175	174	5	9	7.4	2522	PASS
176	174	95	101	98.0	33355	PASS
177	176	5	9	6.6	2213	PASS