

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050823\
 Data File : VN077620.D
 Acq On : 08 May 2023 16:32
 Operator : JC\MD
 Sample : 02642-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TT-052-IDWGW-20230504

Quant Time: May 09 06:03:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050823W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Tue May 09 05:58:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	7.819	128	114880	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.107	114	676727	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.865	117	562613	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.583	65	259220	31.377	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	104.600%
60) 4-Bromofluorobenzene	12.854	95	227209	25.398	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	84.667%
63) Toluene-d8	10.571	98	808570	31.116	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	103.733%
Target Compounds						
25) Chloroform	7.966	83	11196	0.829	ug/l	Qvalue # 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050823\
Data File : VN077620.D
Acq On : 08 May 2023 16:32
Operator : JC\MD
Sample : 02642-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TT-052-IDWGW-20230504

Quant Time: May 09 06:03:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050823W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Tue May 09 05:58:09 2023
Response via : Initial Calibration




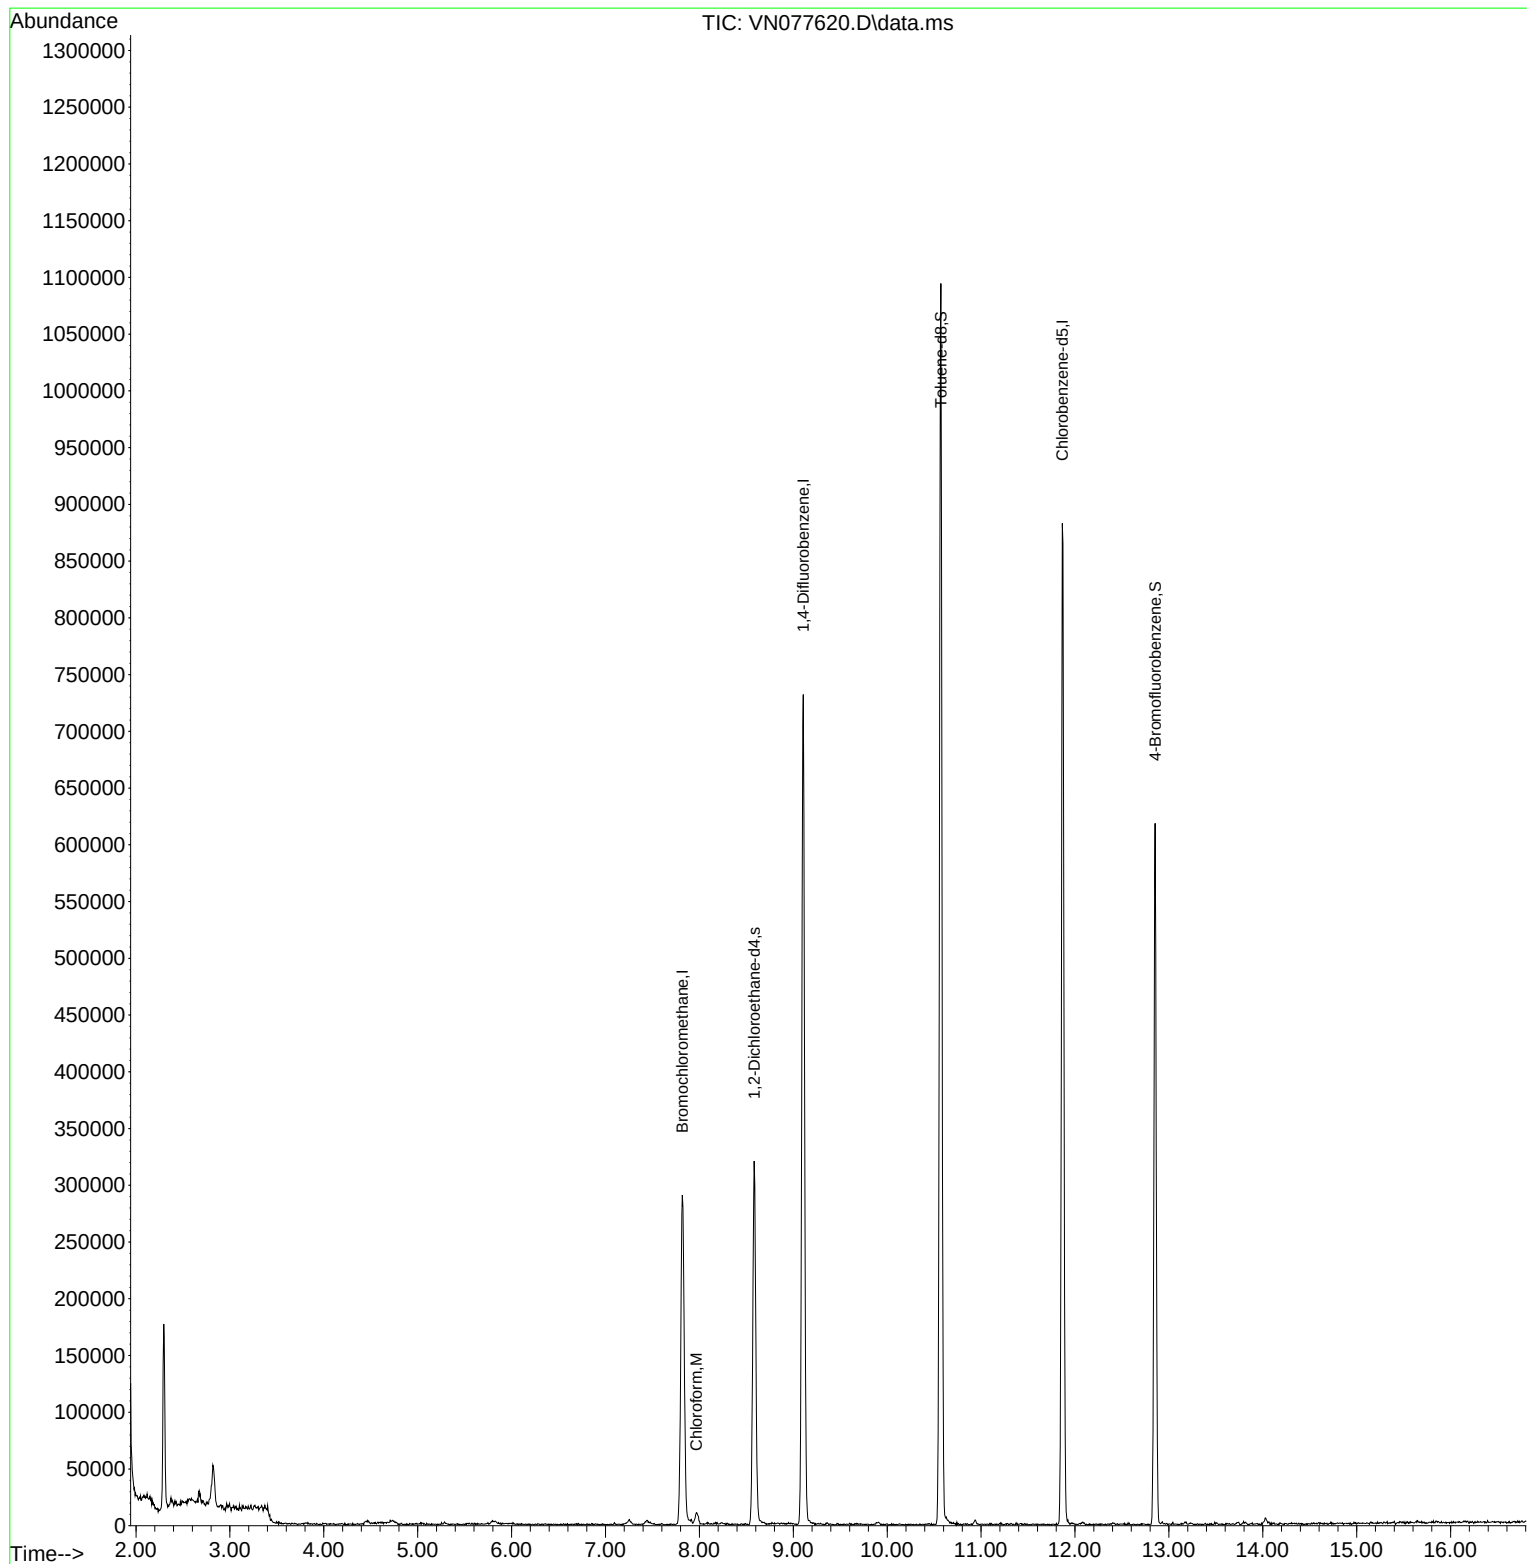


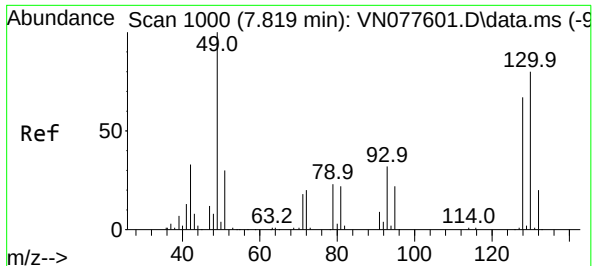

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.819 min Scan# 1000
Delta R.T. -0.000 min
Lab File: VN077620.D
Acq: 08 May 2023 16:32




Instrument :
MSVOA_N
ClientSampleId :
TT-052-IDWGW-20230504


Tgt Ion:128 Resp: 114880
Ion Ratio Lower Upper
128 100
49 122.2 0.0 369.8
130 128.2 0.0 317.8

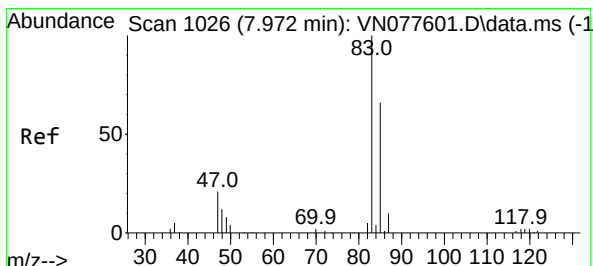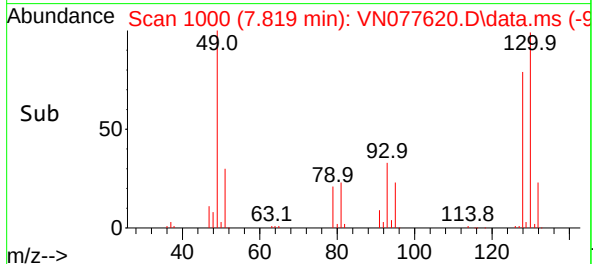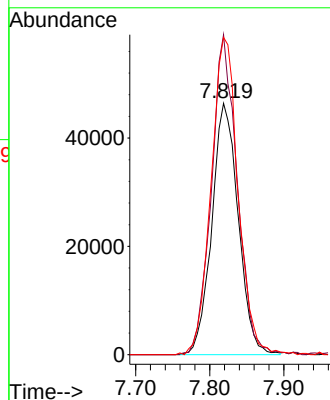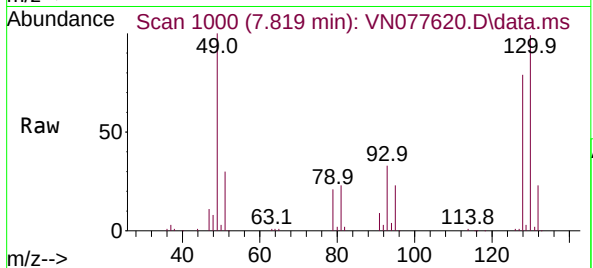

#25
Chloroform
Concen: 0.829 ug/l
RT: 7.966 min Scan# 1025
Delta R.T. -0.006 min
Lab File: VN077620.D
Acq: 08 May 2023 16:32

Tgt Ion: 83 Resp: 11196
Ion Ratio Lower Upper
83 100
85 48.5 53.0 79.6#

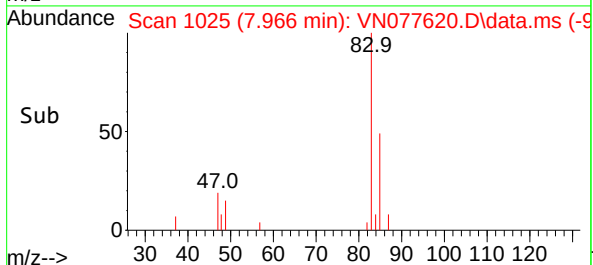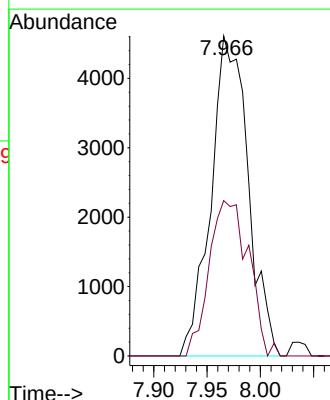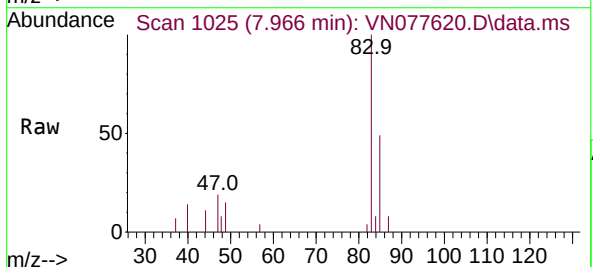

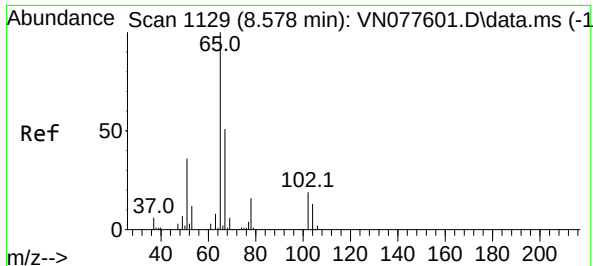

#27

1,2-Dichloroethane-d4

Concen: 31.377 ug/l

RT: 8.583 min Scan# 1129

Delta R.T. 0.005 min

Lab File: VN077620.D

Acq: 08 May 2023 16:32

Instrument :

MSVOA_N

ClientSampleId :





TT-052-IDWGW-20230504

Tgt Ion: 65 Resp: 259220

Ion Ratio Lower Upper

65 100

67 51.4 41.3 61.9

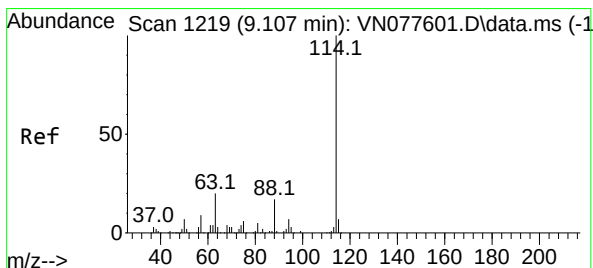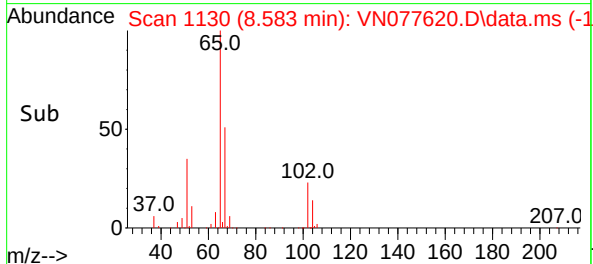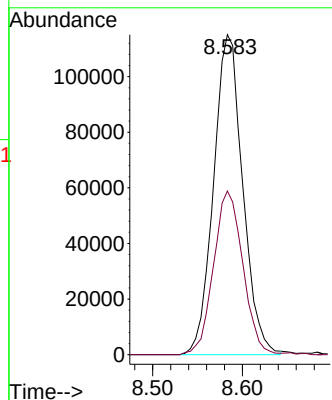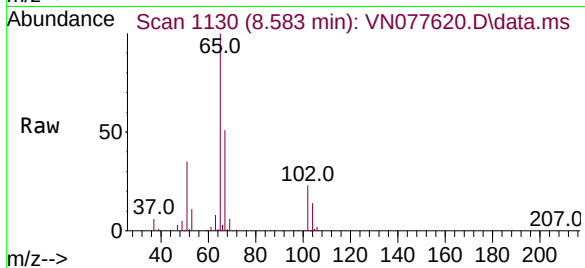

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 9.107 min Scan# 1219

Delta R.T. -0.000 min

Lab File: VN077620.D

Acq: 08 May 2023 16:32




Tgt Ion: 114 Resp: 676727


Ion Ratio Lower Upper

114 100

63 17.6 15.8 23.6

88 15.5 13.0 19.4

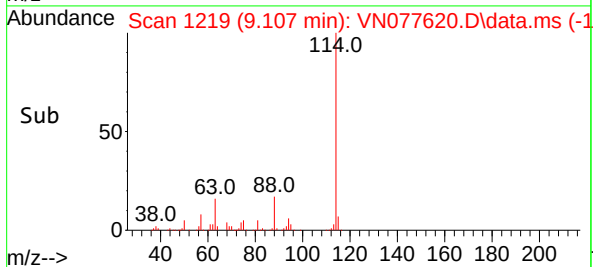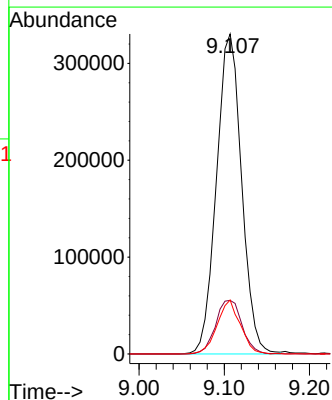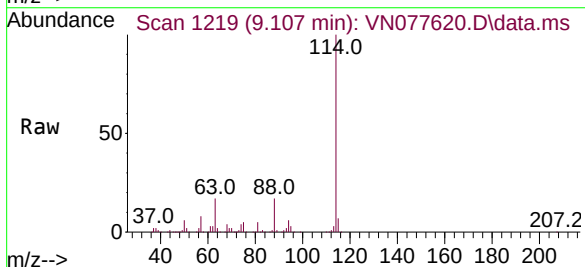

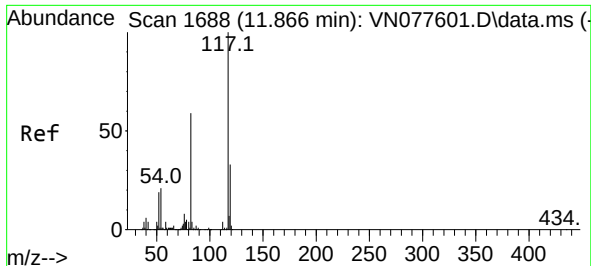

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.865 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN077620.D

Acq: 08 May 2023 16:32

Instrument :

MSVOA_N

ClientSampleId :

TT-052-IDWGW-20230504





Tgt Ion:117 Resp: 562613

Ion Ratio Lower Upper

117 100

82 53.9 47.4 71.2

119 31.3 26.6 39.8

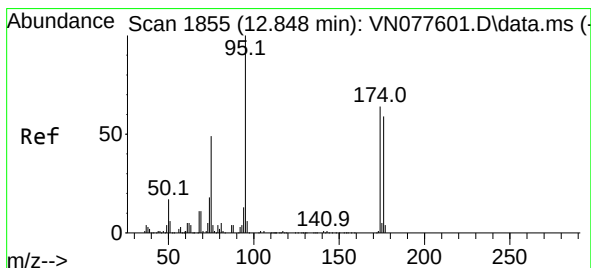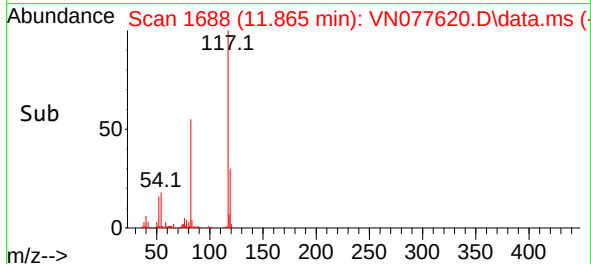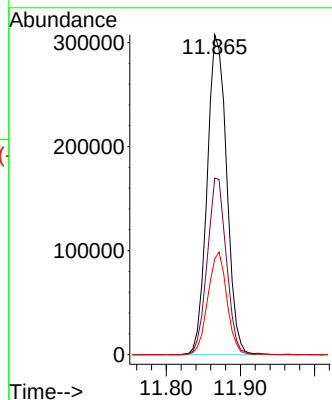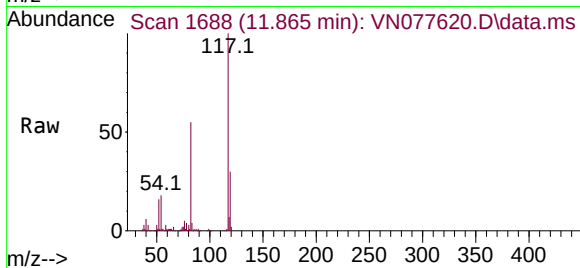

#60

4-Bromofluorobenzene

Concen: 25.398 ug/l

RT: 12.854 min Scan# 1856

Delta R.T. 0.006 min

Lab File: VN077620.D

Acq: 08 May 2023 16:32




Tgt Ion: 95 Resp: 227209


Ion Ratio Lower Upper

95 100

174 71.7 53.4 80.0

176 68.1 50.0 75.0

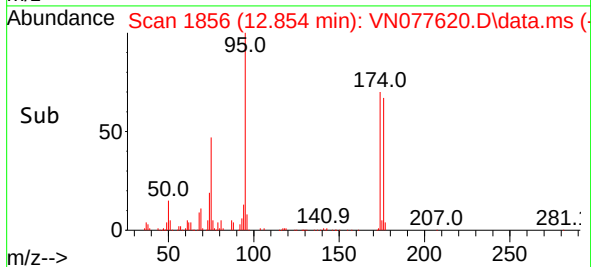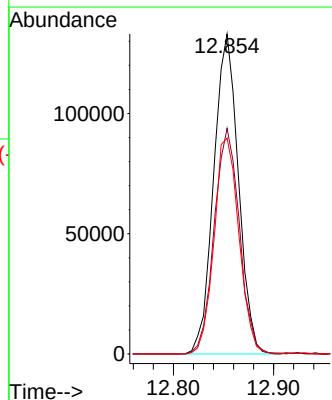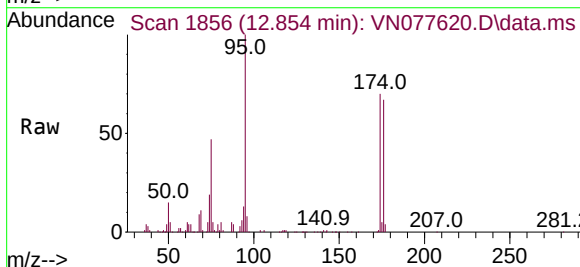

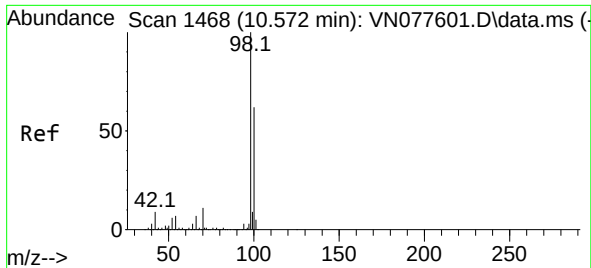

#63
Toluene-d8
Concen: 31.116 ug/l
RT: 10.571 min Scan# 14
Delta R.T. -0.001 min
Lab File: VN077620.D
Acq: 08 May 2023 16:32

Instrument :
MSVOA_N
ClientSampleId :
TT-052-IDWGW-20230504

Tgt Ion: 98 Resp: 808570
Ion Ratio Lower Upper
98 100
100 64.5 52.1 78.1

