
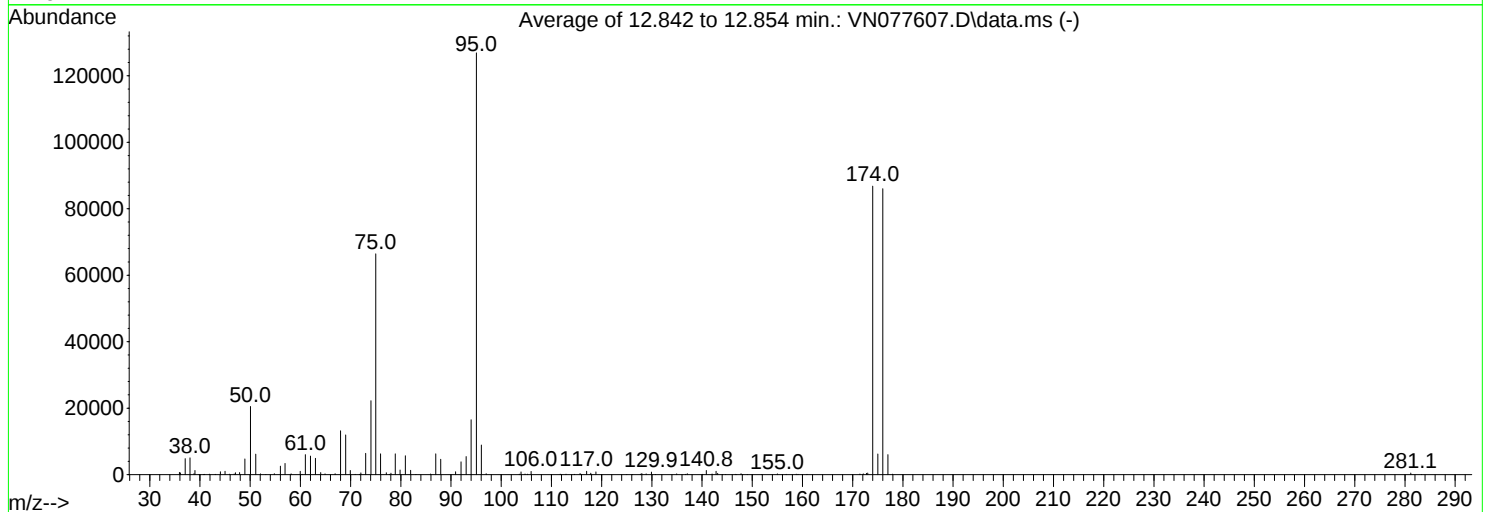


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050823\
Data File : VN077607.D
Acq On : 08 May 2023 09:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N050823W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue May 09 05:58:09 2023

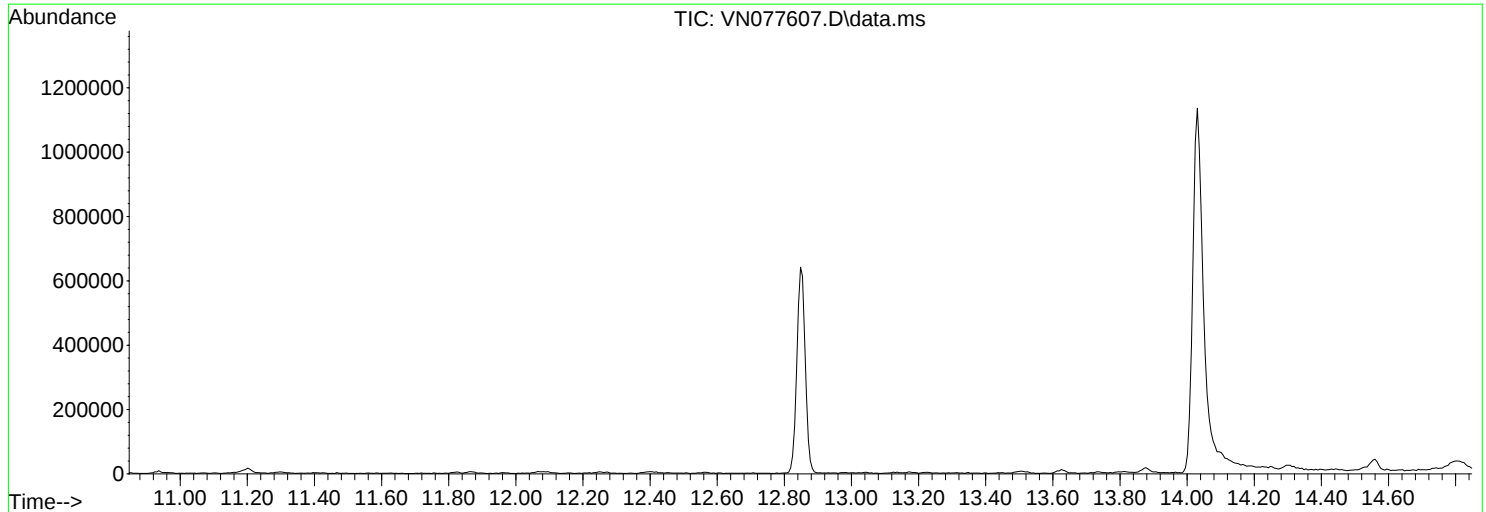

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	20501	PASS
75	95	30	60	52.4	66451	PASS
95	95	100	100	100.0	126909	PASS
96	95	5	9	7.0	8899	PASS
173	174	0.00	2	0.6	481	PASS
174	95	50	100	68.4	86787	PASS
175	174	5	9	7.2	6220	PASS
176	174	95	101	99.1	86013	PASS
177	176	5	9	7.0	6029	PASS