


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050825\
Data File : VN086537.D
Acq On : 08 May 2025 09:50
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

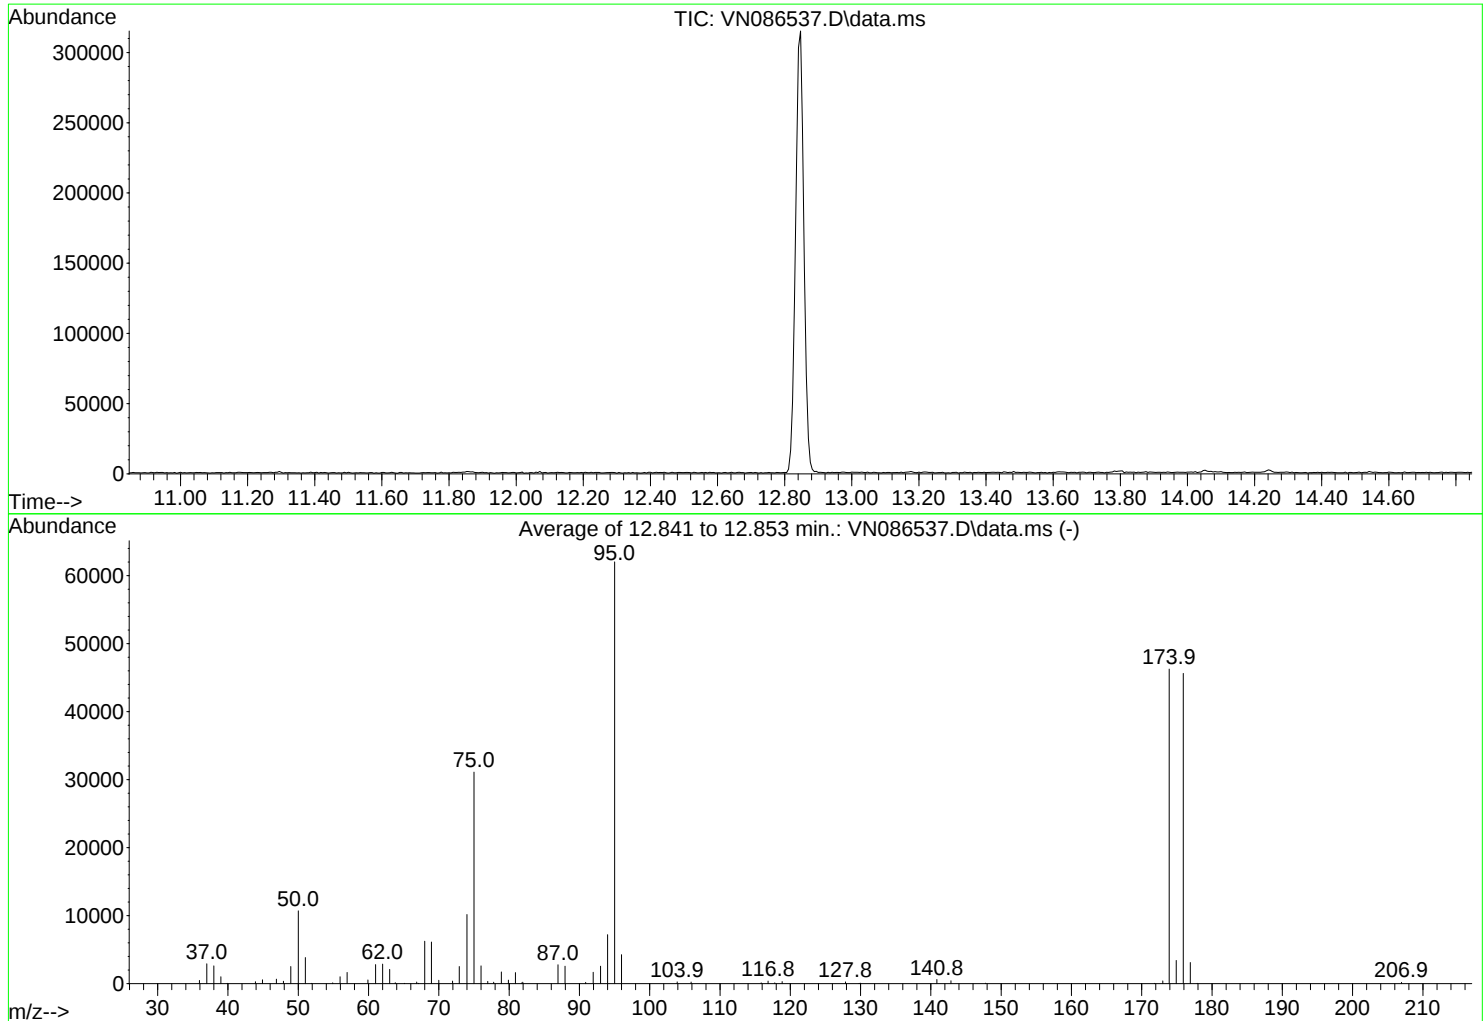

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	10716	PASS
75	95	30	60	50.1	31104	PASS
95	95	100	100	100.0	62037	PASS
96	95	5	9	6.9	4258	PASS
173	174	0.00	2	0.9	403	PASS
174	95	50	100	74.6	46272	PASS
175	174	5	9	7.4	3410	PASS
176	174	95	101	98.6	45621	PASS
177	176	5	9	6.8	3118	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	467	51.00	3836	66.85	229	77.80	211
37.00	2915	51.90	51	67.10	51	78.90	172
38.00	2603	54.90	111	68.00	6246	79.90	52
39.00	1015	55.95	1006	68.95	6130	80.90	161
39.90	41	56.95	1659	70.00	498	81.80	126
43.90	290	59.90	538	71.95	379	81.95	219
44.90	556	61.00	2796	72.90	2513	86.95	2785
46.90	651	62.00	2865	74.00	10178	87.95	2556
47.90	364	63.00	2085	75.00	31104	90.90	191
48.95	2524	63.80	144	76.00	2612	91.95	1671
50.00	10716	65.10	52	76.95	334	93.00	2576

Average of 12.841 to 12.853 min.: VN086537.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	7207	130.00	79	206.95	191		
95.00	62037	140.85	612				
96.00	4258	142.85	427				
103.90	248	147.80	63				
105.90	231	171.80	52				
115.85	128	173.00	403				
116.85	368	173.90	46272				
117.80	118	174.90	3410				
118.85	303	175.90	45621				
127.85	265	176.90	3118				
129.80	58	177.90	51				

Instrument :

MSVOA_N

ClientSampleId :

BFB