

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN050919\
 Data File : VN055493.D
 Acq On : 9 May 2019 13:33
 Operator : JC/SP
 Sample : K2672-17
 Misc : 5.01µ/10mL/100µL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SB-09-1.0-1.5

Quant Time: May 09 15:36:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 09 04:17:44 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.66	168	796659	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.58	114	1343253	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1129575	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	414527	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	553360	46.13	ug/l	0.00
Spiked Amount	50.000		Recovery	=	92.26%	
35) Dibromofluoromethane	7.59	113	413197	47.69	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.38%	
50) Toluene-d8	10.09	98	1619999	47.98	ug/l	0.00
Spiked Amount	50.000		Recovery	=	95.96%	
62) 4-Bromofluorobenzene	12.40	95	530747	46.62	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.24%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN050919\
Data File : VN055493.D
Acq On : 9 May 2019 13:33
Operator : JC/SP
Sample : K2672-17
Misc : 5.01µL/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SB-09-1.0-1.5

Quant Time: May 09 15:36:02 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Quant Title : SW846 8260
QLast Update : Thu May 09 04:17:44 2019
Response via : Initial Calibration

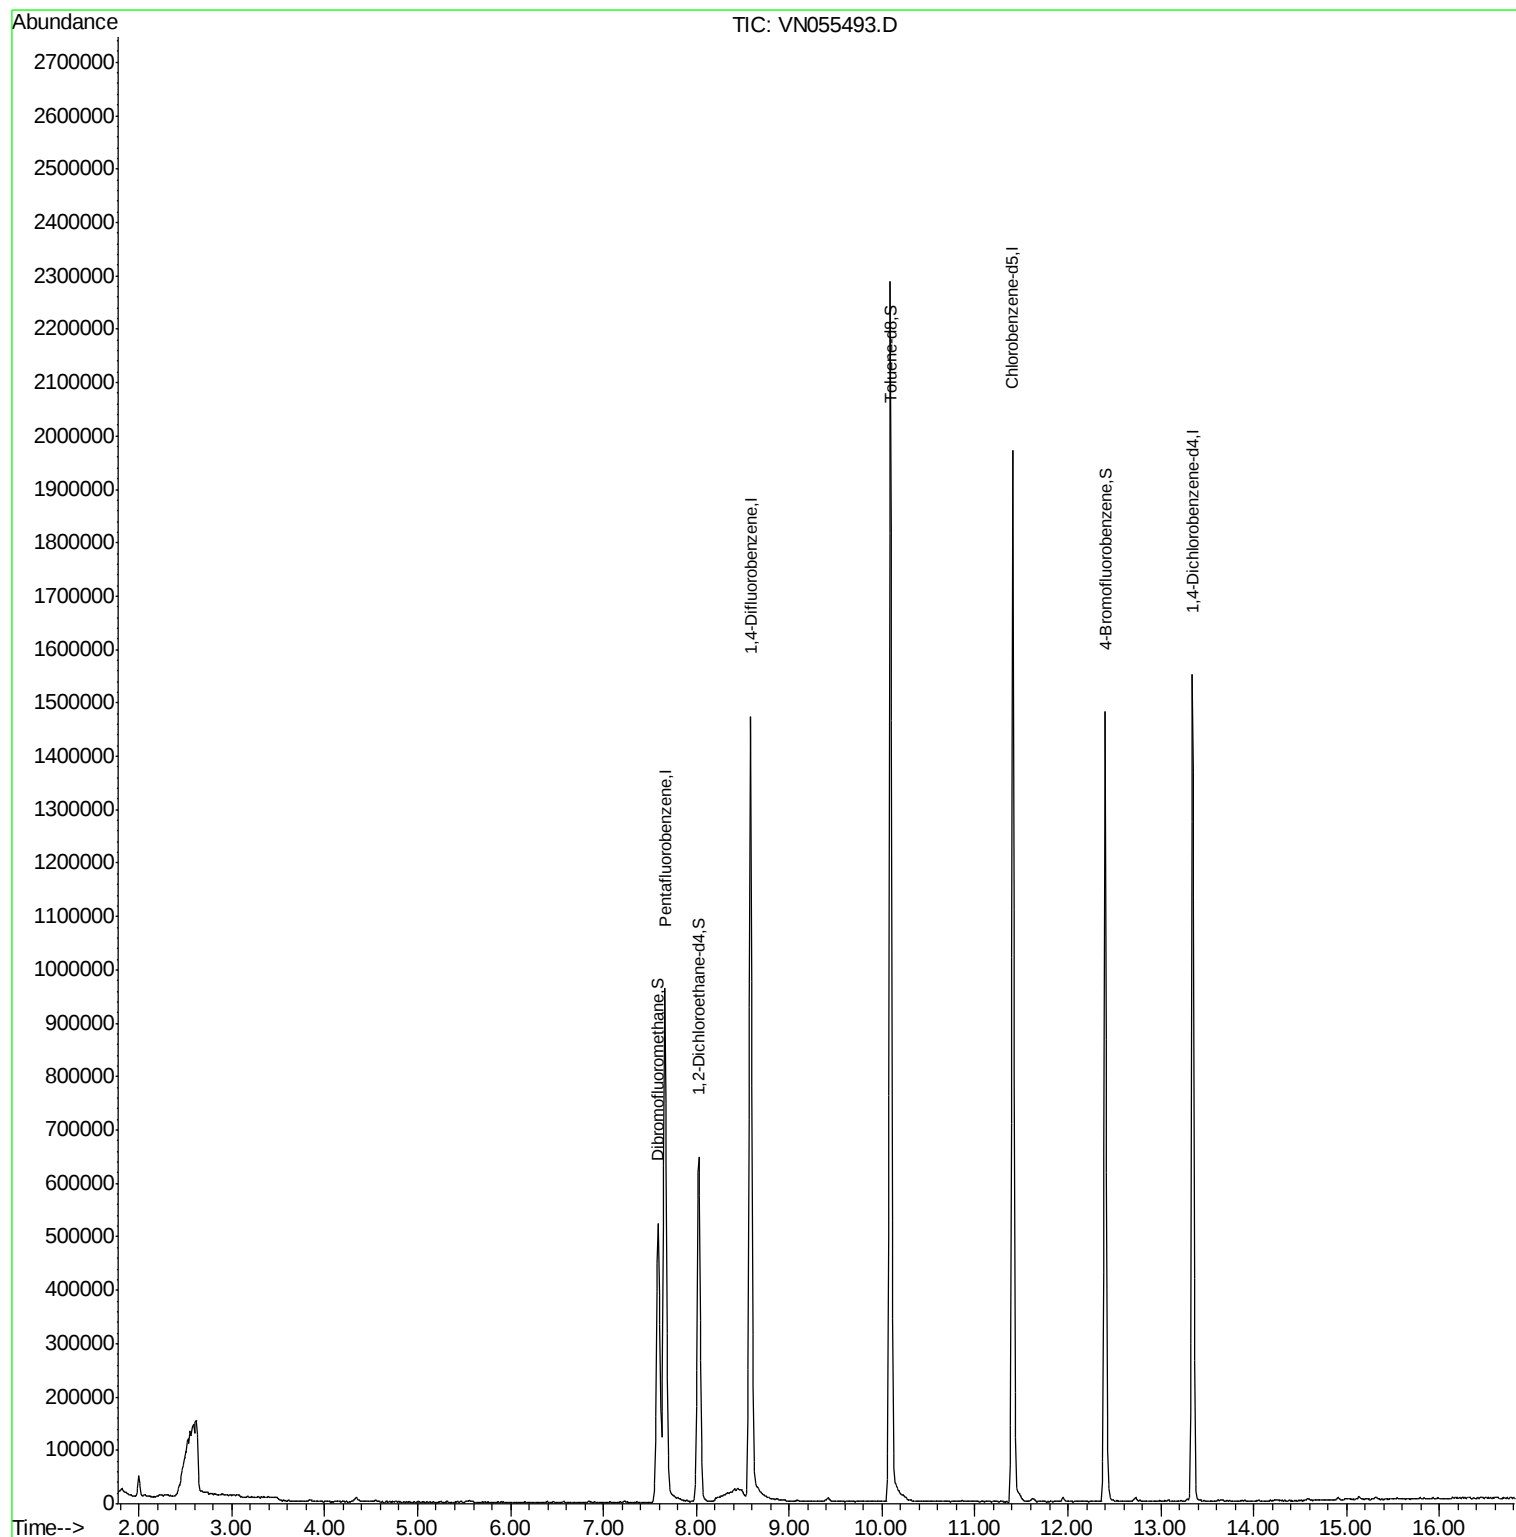

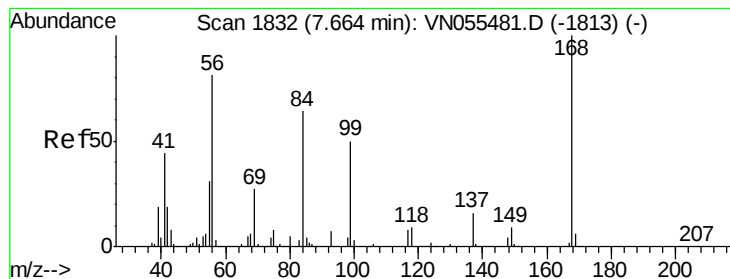

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.66 min Scan# 1832

Delta R.T. -0.00 min

Lab File: VN055493.D

Acq: 9 May 2019 13:33

Instrument :

MSVOA_N

ClientSampleId :


SB-09-1.0-1.5

Tot Ion:168 Resp: 796659

Ion Ratio Lower Upper




168 100

99 57.3 47.0 70.4

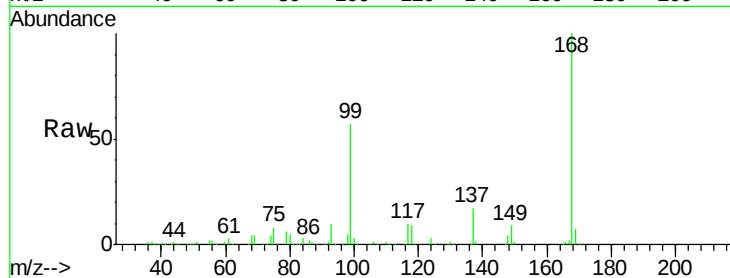

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

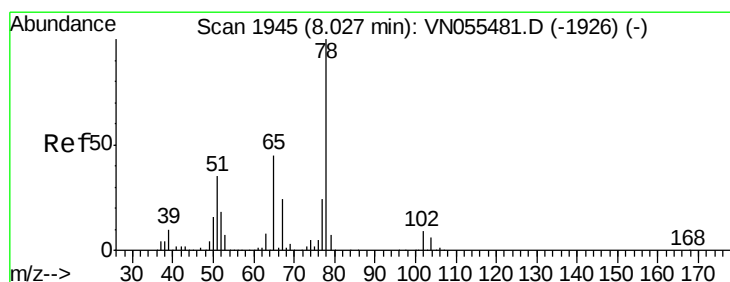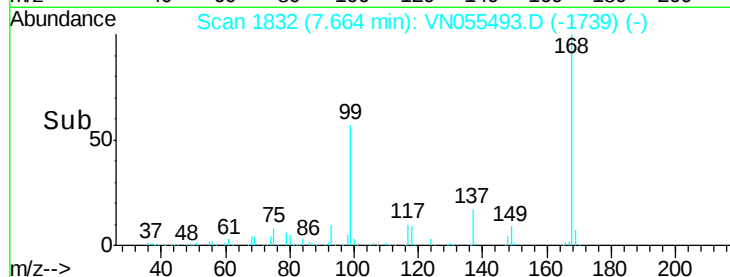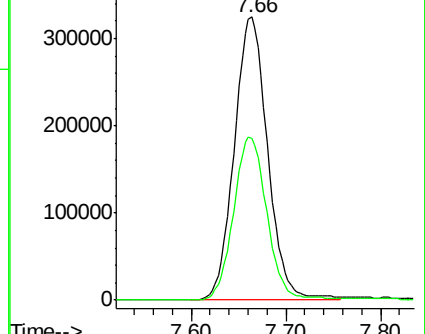

#33

1,2-Dichloroethane-d4

Concen: 46.133 ug/l

RT: 8.03 min Scan# 1945

Delta R.T. -0.00 min

Lab File: VN055493.D


Acq: 9 May 2019 13:33

Tgt Ion: 65 Resp: 553360

Ion Ratio Lower Upper



65 100


67 53.9 0.0 109.6

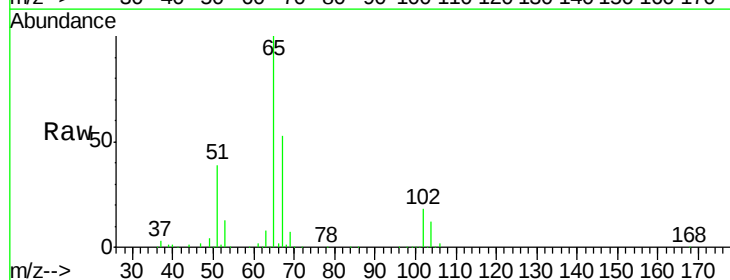

Abundance Ion 64.90 (64.60 to 65.60): VNO

Ion 66.90 (66.60 to 67.60): VNO

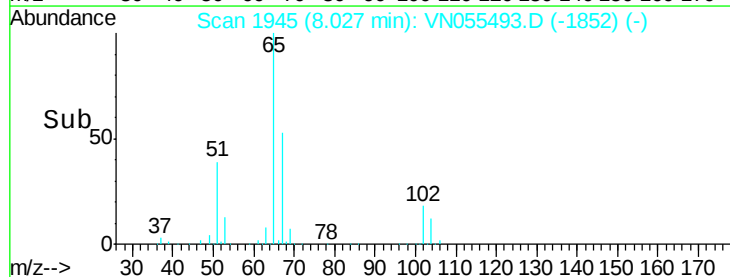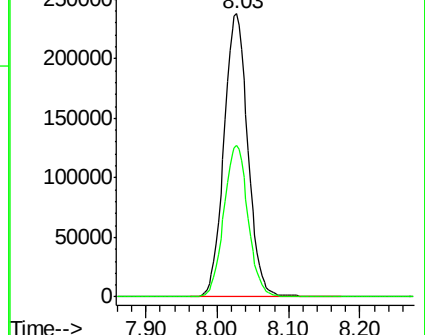

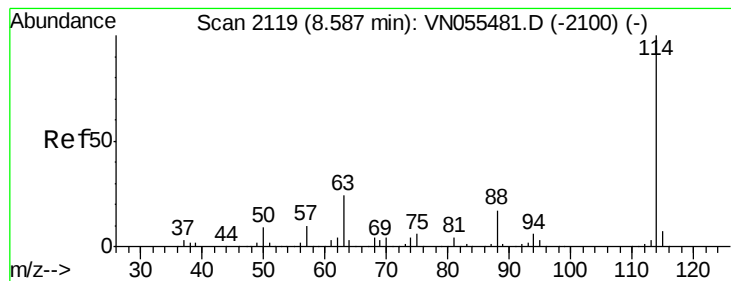

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.58 min Scan# 2118

Delta R.T. -0.00 min

Lab File: VN055493.D

Acq: 9 May 2019 13:33

Instrument :

MSVOA_N

ClientSampleId :

SB-09-1.0-1.5


Tot Ion:114 Resp: 1343253

Ion Ratio Lower Upper

114 100

63 22.7 0.0 47.4




88 16.2 0.0 34.0

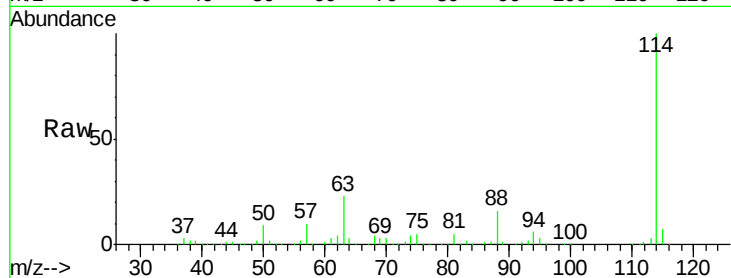

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

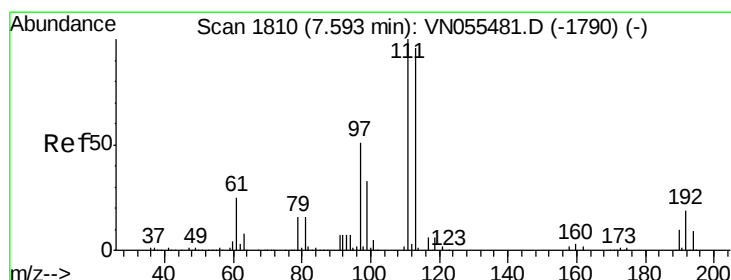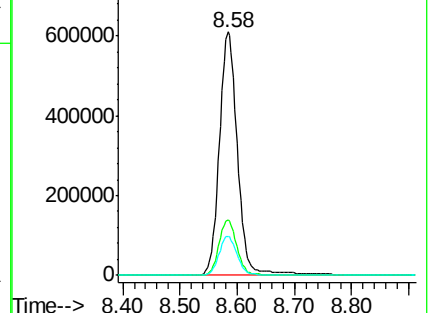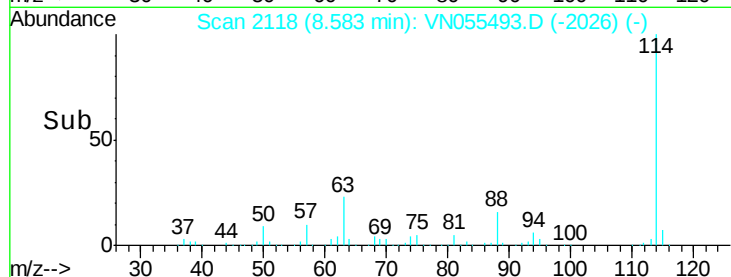

#35

Dibromofluoromethane

Concen: 47.686 ug/l

RT: 7.59 min Scan# 1809

Delta R.T. -0.00 min

Lab File: VN055493.D

Acq: 9 May 2019 13:33


Tgt Ion:113 Resp: 413197

Ion Ratio Lower Upper

113 100

111 102.1 82.9 124.3



192 18.9 15.6 23.4

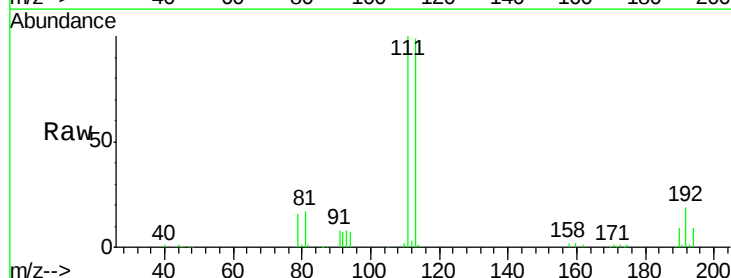


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

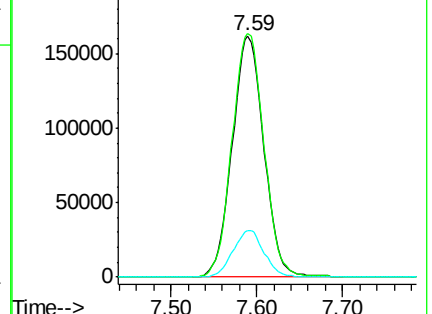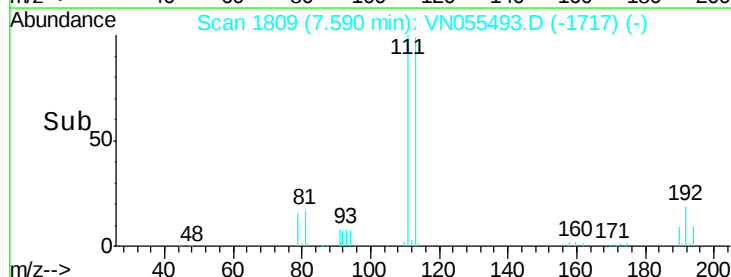

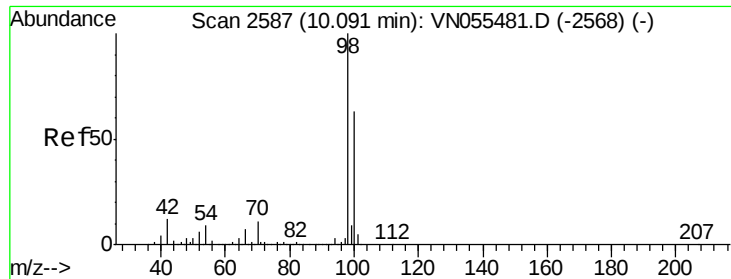

#50

Toluene-d8

Concen: 47.976 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN055493.D

Acq: 9 May 2019 13:33

Instrument :

MSVOA_N

ClientSampleId :





SB-09-1.0-1.5

Tot Ion: 98 Resp: 1619999

Ion Ratio Lower Upper

98 100

100 62.8 50.4 75.6

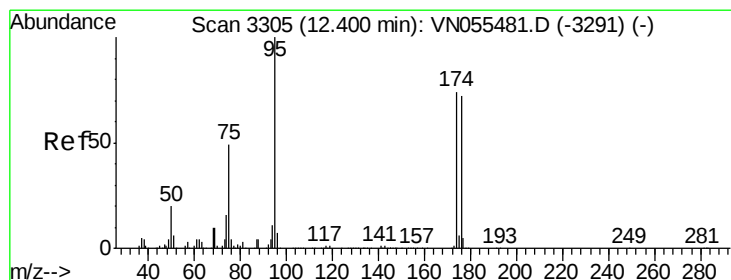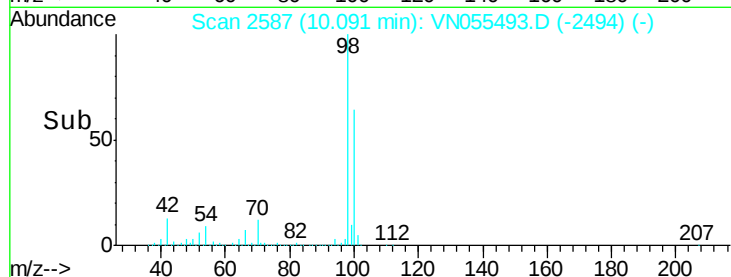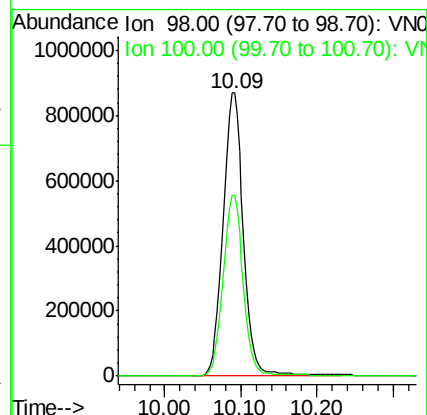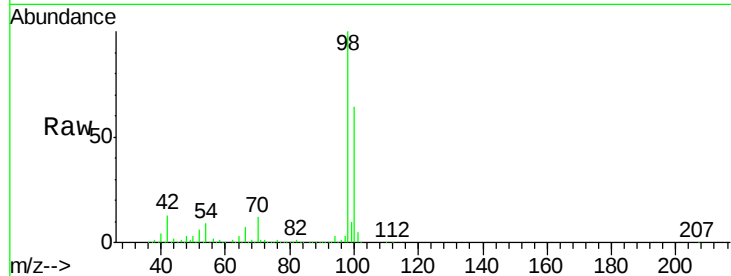

#62

4-Bromofluorobenzene

Concen: 46.615 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN055493.D

Acq: 9 May 2019 13:33




Tgt Ion: 95 Resp: 530747


Ion Ratio Lower Upper

95 100

174 77.2 0.0 152.2

176 75.0 0.0 147.8

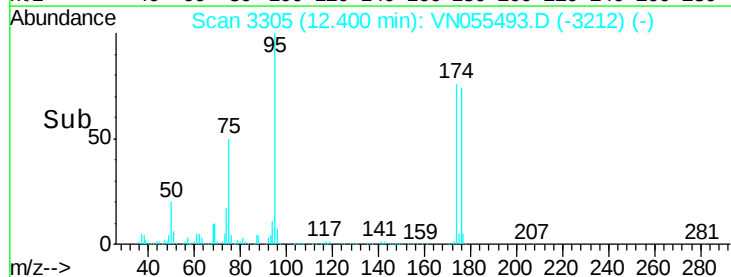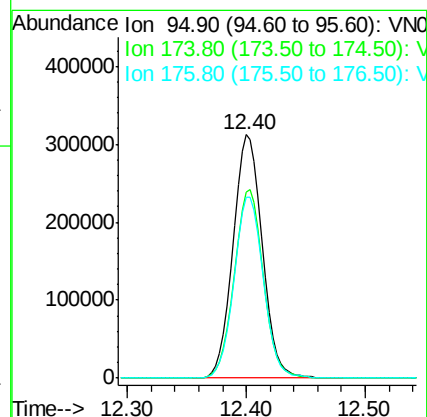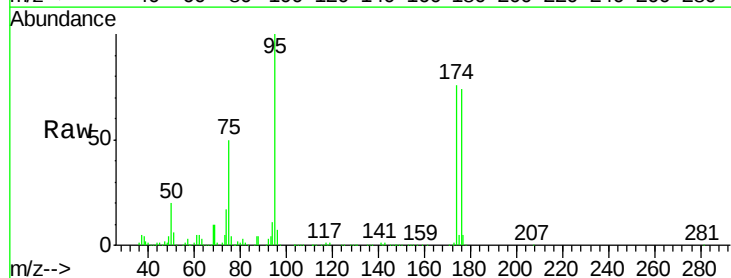


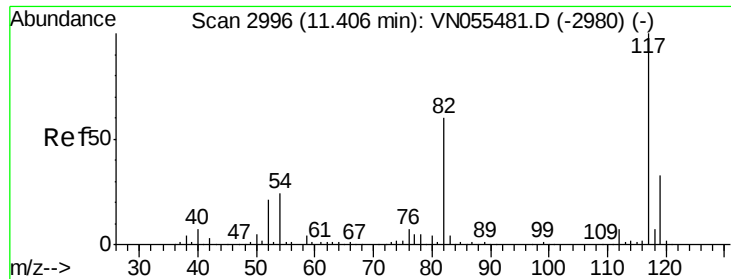




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. -0.00 min
Lab File: VN055493.D
Acq: 9 May 2019 13:33

Instrument :
MSVOA_N
ClientSampleId :
SB-09-1.0-1.5

Tot Ion:117 Resp: 1129575
Ion Ratio Lower Upper
117 100
82 59.4 48.0 72.0
119 31.8 26.0 39.0

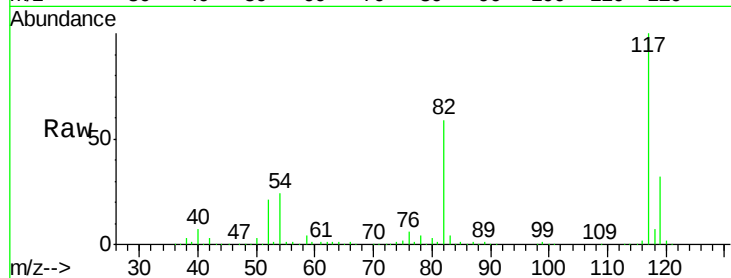


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

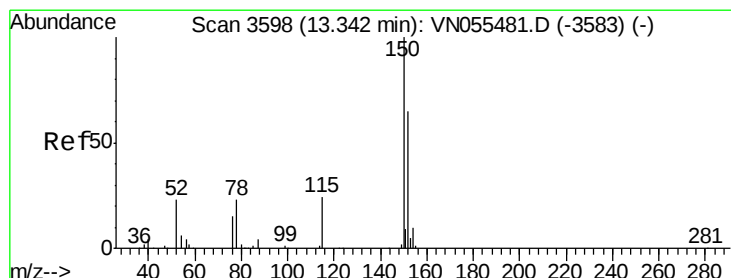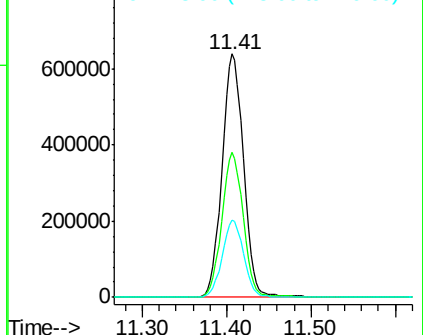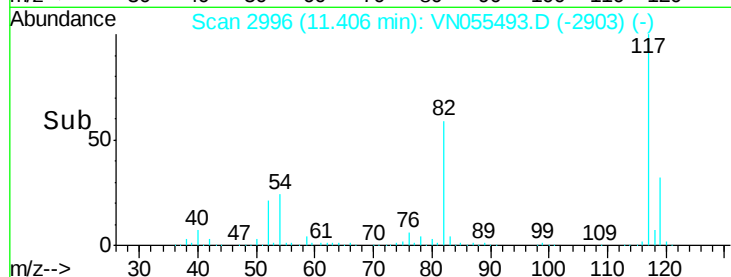

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. -0.00 min
Lab File: VN055493.D
Acq: 9 May 2019 13:33

Tgt Ion:152 Resp: 414527
Ion Ratio Lower Upper
152 100
115 61.5 30.1 90.5
150 158.5 0.0 355.0

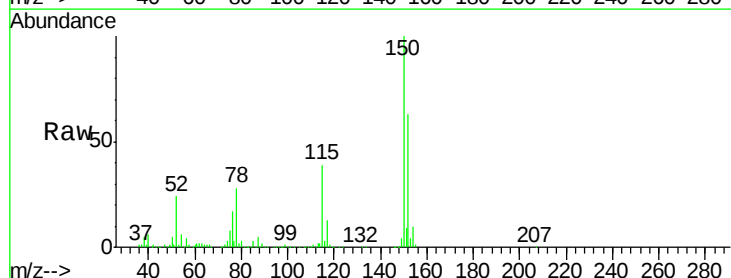

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

