


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN050919\
Data File : VN055510.D
Acq On : 9 May 2019 21:04
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N050819W.M
Title : SW846 8260
Last Update : Fri May 10 06:48:32 2019

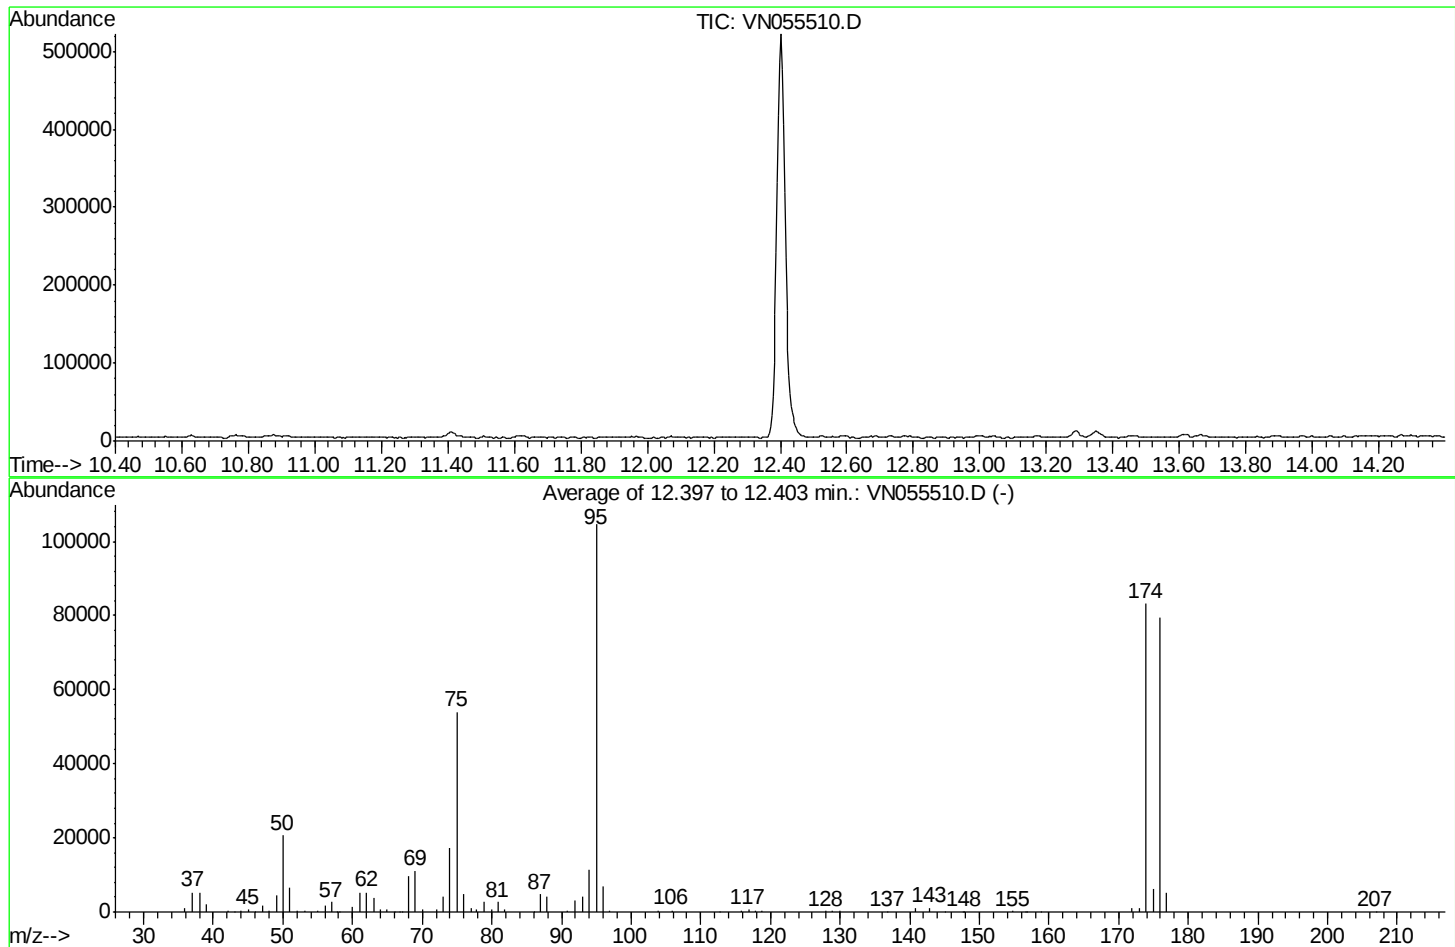

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	20677	PASS
75	95	30	60	51.6	53944	PASS
95	95	100	100	100.0	104613	PASS
96	95	5	9	6.7	6990	PASS
173	174	0.00	2	1.4	1199	PASS
174	95	50	100	79.5	83136	PASS
175	174	5	9	7.6	6326	PASS
176	174	95	101	95.4	79328	PASS
177	176	5	9	6.6	5228	PASS