

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050922\
 Data File : VN072377.D
 Acq On : 09 May 2022 14:21
 Operator : JC\MD
 Sample : N2740-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: May 10 06:45:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
 Quant Title : SW846 8260
 QLast Update : Tue Apr 26 18:50:11 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.080	168	289032	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	546812	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	585839	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	228722	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	202477	45.631	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	91.260%		
35) Dibromofluoromethane	8.016	113	164741	47.070	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	94.140%		
50) Toluene-d8	10.433	98	693294	50.412	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	100.820%		
62) 4-Bromofluorobenzene	12.727	95	271069	59.383	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	118.760%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.298	50	1774	Below Cal	#	67
5) Bromomethane	2.857	94	868	Below Cal	#	2
6) Chloroethane	3.022	64	534	Below Cal	#	42
10) Methyl Iodide	4.416	142	842	0.232	ug/l #	23
11) Tert butyl alcohol	5.345	59	521	0.714	ug/l #	72
13) Acrolein	4.045	56	266	0.362	ug/l #	63
15) Acrylonitrile	5.551	53	825	0.375	ug/l #	60
16) Acetone	4.292	43	4108	2.147	ug/l #	56
17) Carbon Disulfide	4.528	76	393	0.423	ug/l #	75
18) Methyl Acetate	4.875	43	1377	0.218	ug/l #	48
20) Methylene Chloride	5.098	84	2251	0.614	ug/l	90
25) 2-Butanone	7.333	43	1335	0.438	ug/l #	88
29) Tetrahydrofuran	7.686	42	646	0.323	ug/l #	50
31) Cyclohexane	8.080	56	6232	1.051	ug/l #	1
36) 1,1-Dichloropropene	8.086	75	23470	4.607	ug/l #	49
38) Carbon Tetrachloride	8.080	117	30622	5.612	ug/l #	15
43) Isopropyl Acetate	8.551	43	111	0.811	ug/l #	53
49) 1,4-Dioxane	9.569	88	66	0.841	ug/l #	25
51) 4-Methyl-2-Pentanone	10.321	43	2378	0.373	ug/l	88
56) Ethyl methacrylate	10.769	69	421	2.423	ug/l #	74
59) 2-Hexanone	11.086	43	5868	1.305	ug/l	89
74) N-amyl acetate	12.380	43	3580	0.473	ug/l #	87
75) 1,1,2,2-Tetrachloroethane	12.815	83	656	Below Cal	#	92
76) 1,2,3-Trichloropropane	12.727	75	136702	26.581	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	136702	69.107	ug/l #	10
87) 1,3-Dichlorobenzene	13.610	146	1833	0.237	ug/l	85
88) 1,4-Dichlorobenzene	13.610	146	1833	0.244	ug/l	84
89) n-Butylbenzene	13.933	91	3760	0.327	ug/l	98
91) 1,2-Dichlorobenzene	13.986	146	1899	0.249	ug/l	98
92) 1,2-Dibromo-3-Chloropr...	14.604	75	580	0.415	ug/l #	34
93) 1,2,4-Trichlorobenzene	15.262	180	2647	3.135	ug/l	94
95) Naphthalene	15.498	128	9454	5.029	ug/l #	89
96) 1,2,3-Trichlorobenzene	15.686	180	2737	3.411	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_N
ClientSampleId :

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050922\
Data File : VN072377.D
Acq On : 09 May 2022 14:21
Operator : JC\MD
Sample : N2740-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: May 10 06:45:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
Quant Title : SW846 8260
QLast Update : Tue Apr 26 18:50:11 2022
Response via : Initial Calibration




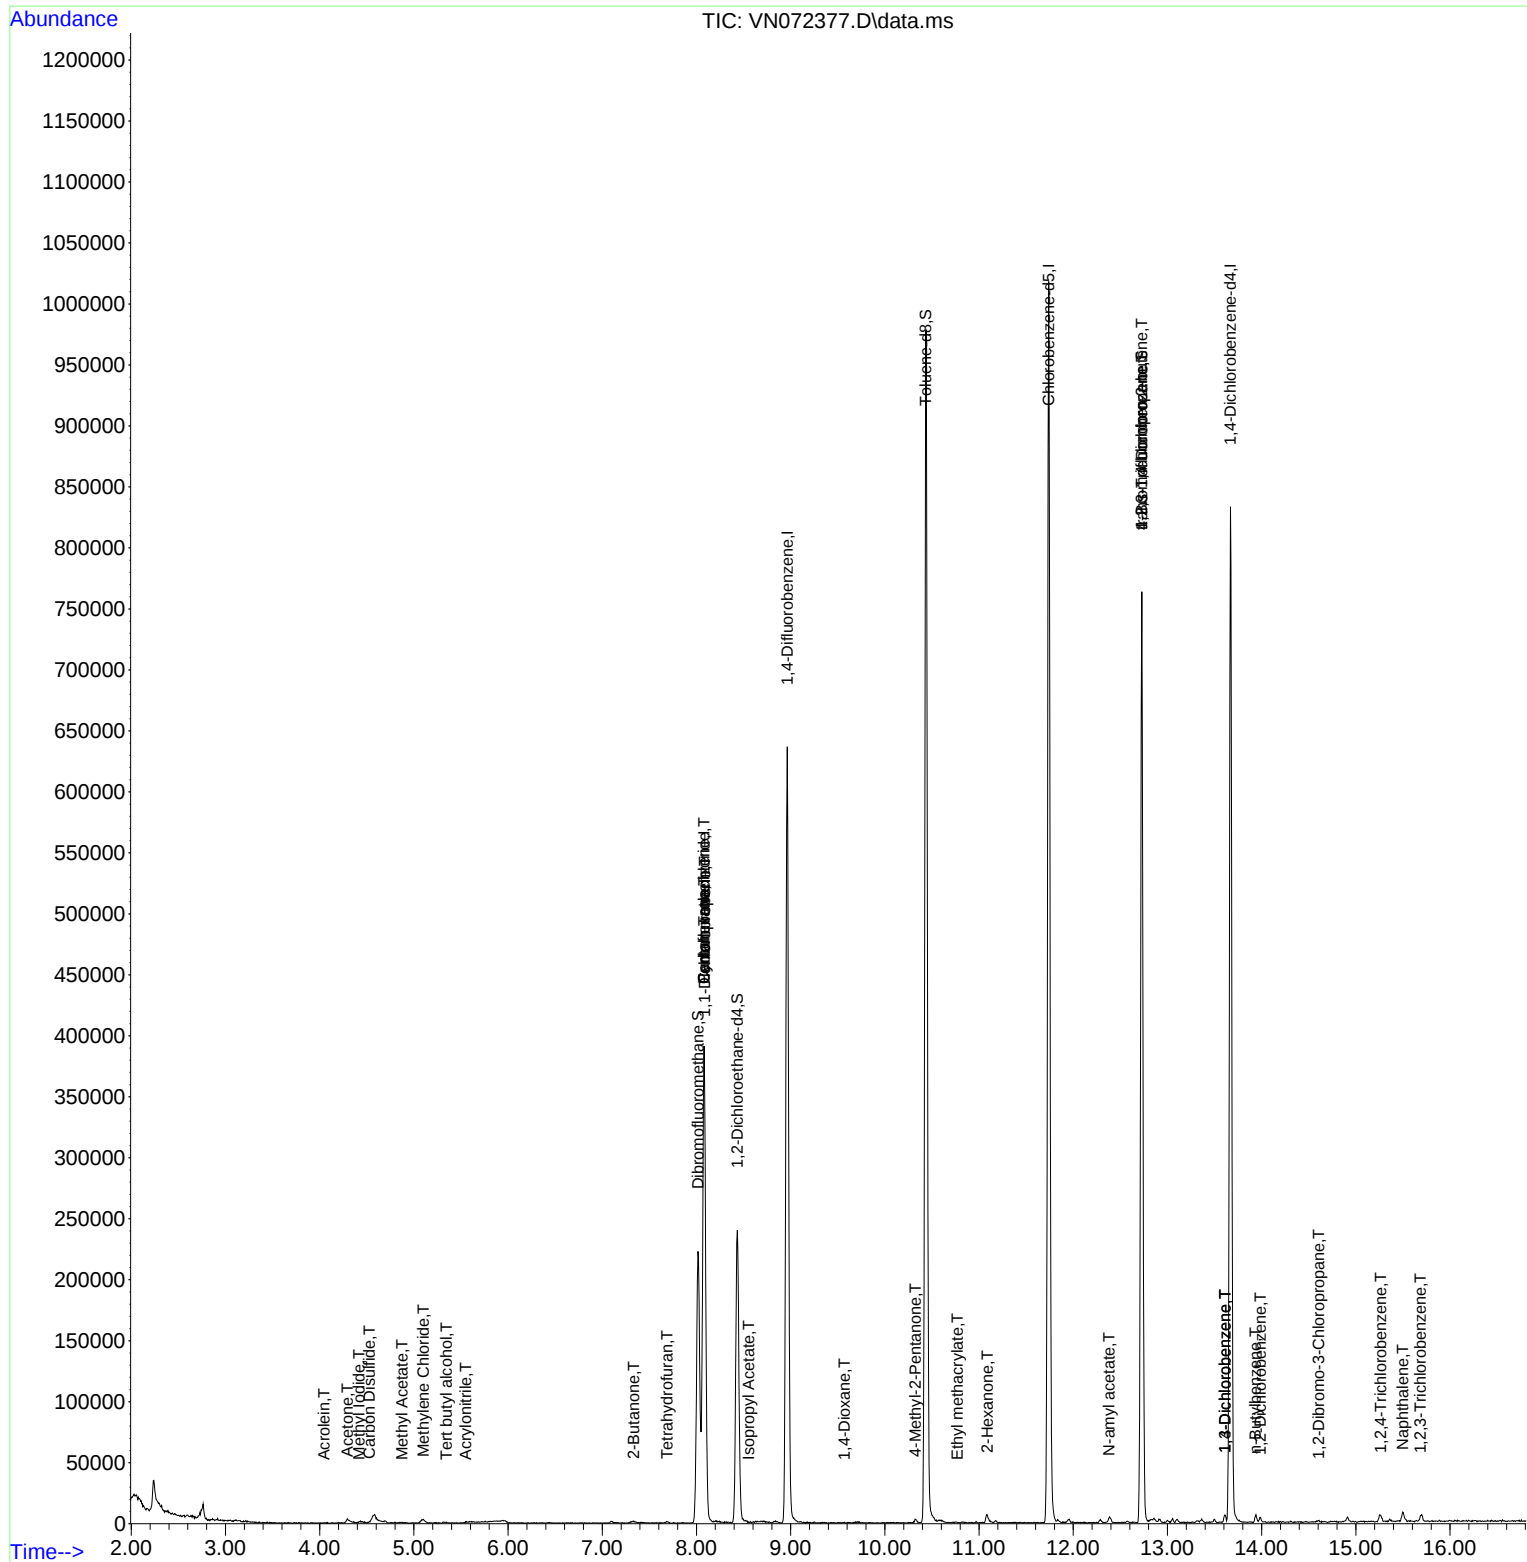




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.080 min Scan# 10
Delta R.T. -0.001 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 289032
Ion Ratio Lower Upper
168 100
99 59.9 42.3 63.5

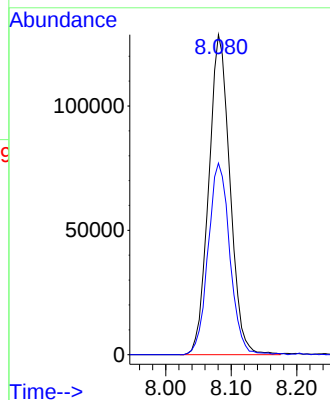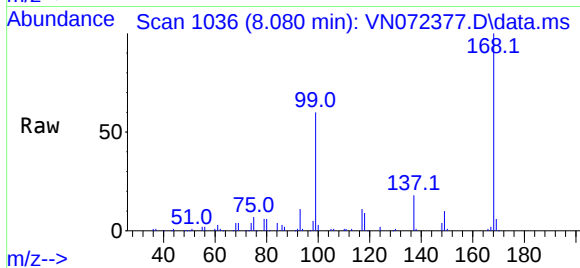

#3
Chloromethane
Concen: Below Cal
RT: 2.298 min Scan# 53
Delta R.T. -0.001 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

Tgt Ion: 50 Resp: 1774
Ion Ratio Lower Upper
50 100
52 13.9 25.7 38.5#


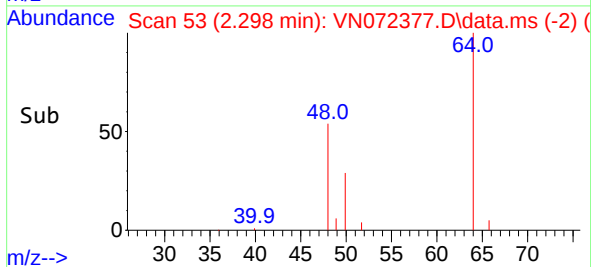
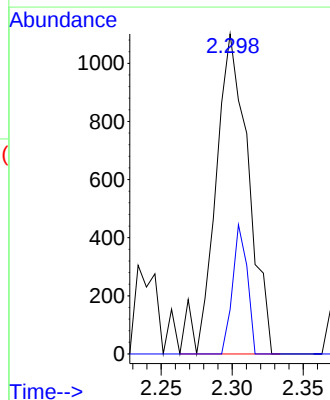
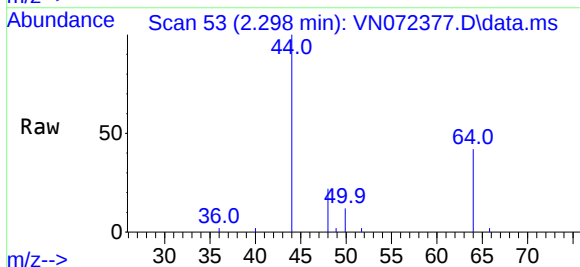


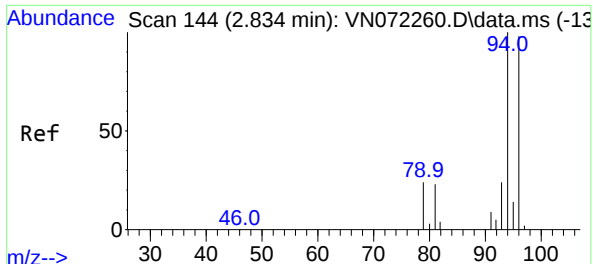

#5
Bromomethane
Concen: Below Cal
RT: 2.857 min Scan# 144
Delta R.T. 0.023 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21



Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 868
Ion Ratio Lower Upper
94 100
96 0.0 76.0 114.0#

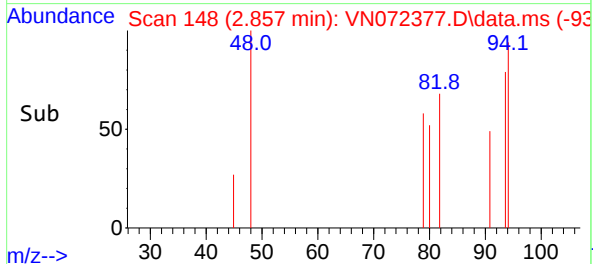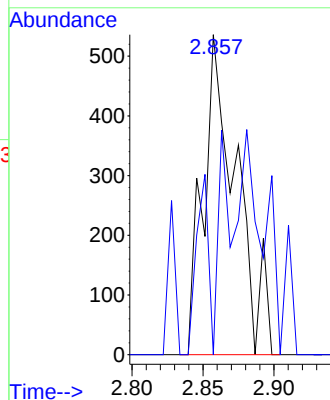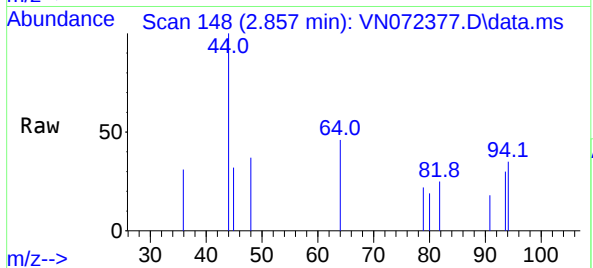

#6
Chloroethane
Concen: Below Cal
RT: 3.022 min Scan# 176
Delta R.T. 0.017 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21


Tgt Ion: 64 Resp: 534
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

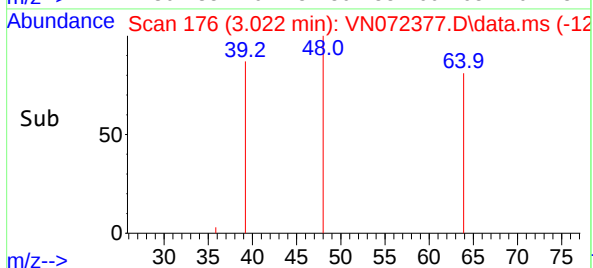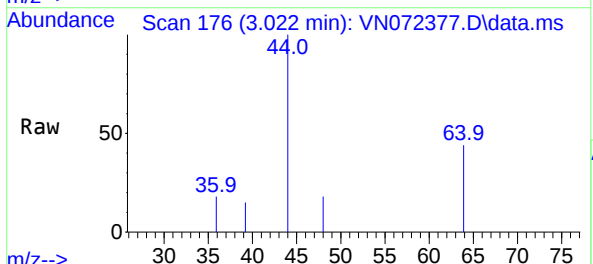






#10
Methyl Iodide
Concen: 0.232 ug/l
RT: 4.416 min Scan# 413
Delta R.T. -0.006 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:142 Resp: 842
Ion Ratio Lower Upper
142 100
127 95.2 31.3 46.9#
141 0.0 11.2 16.8#

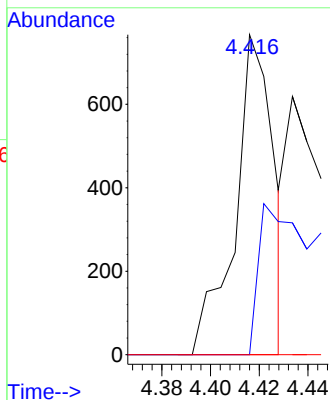


#11
Tert butyl alcohol
Concen: 0.714 ug/l
RT: 5.345 min Scan# 571
Delta R.T. -0.018 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21




Tgt Ion: 59 Resp: 521
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#

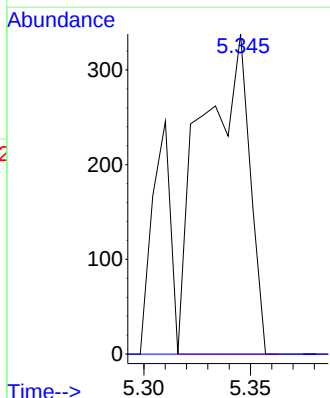






#13
Acrolein
Concen: 0.362 ug/l
RT: 4.045 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 266
Ion Ratio Lower Upper
56 100
55 38.7 54.8 82.2#



#15
Acrylonitrile
Concen: 0.375 ug/l
RT: 5.551 min Scan# 606
Delta R.T. 0.005 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

Tgt Ion: 53 Resp: 825
Ion Ratio Lower Upper
53 100
52 48.1 66.4 99.6#
51 10.4 28.5 42.7#


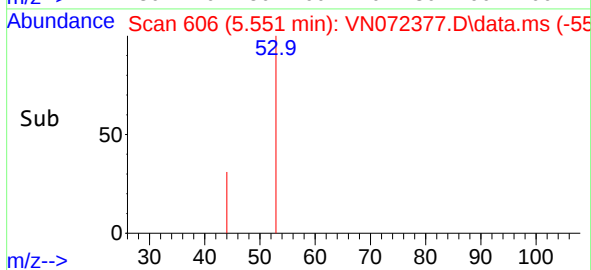






#16
Acetone
Concen: 2.147 ug/l
RT: 4.292 min Scan# 392
Delta R.T. 0.011 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 4108
Ion Ratio Lower Upper
43 100
58 57.1 26.0 39.0#



#17
Carbon Disulfide
Concen: 0.423 ug/l
RT: 4.528 min Scan# 432
Delta R.T. -0.006 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

Tgt Ion: 76 Resp: 393
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

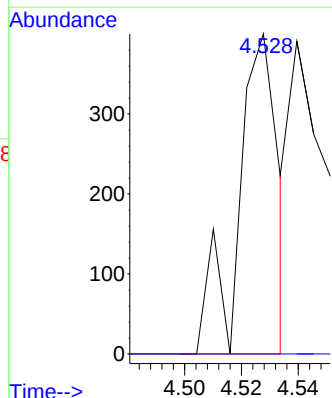



#18

Methyl Acetate

Concen: 0.218 ug/l

RT: 4.875 min Scan# 491

Delta R.T. 0.024 min


Lab File: VN072377.D

Acq: 09 May 2022 14:21

Instrument :

MSVOA_N

ClientSampleId :






Tgt Ion: 43 Resp: 1377

Ion Ratio Lower Upper

43 100

74 0.0 21.6 32.4#

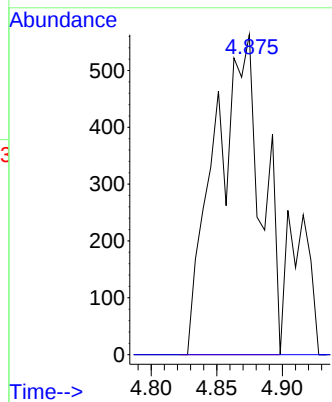

#20

Methylene Chloride

Concen: 0.614 ug/l

RT: 5.098 min Scan# 529

Delta R.T. 0.011 min

Lab File: VN072377.D

Acq: 09 May 2022 14:21

Tgt Ion: 84 Resp: 2251




Ion Ratio Lower Upper


84 100

49 119.8 88.3 132.5

51 31.2 28.2 42.2

86 52.9 50.6 76.0

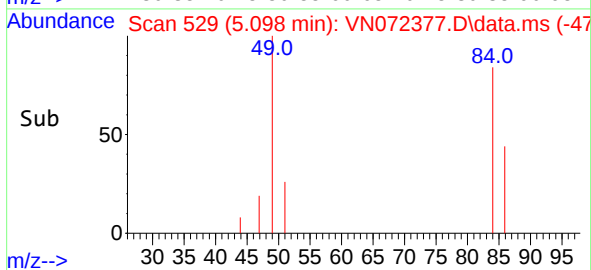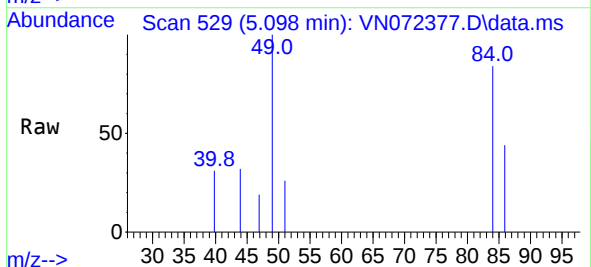



#25

2-Butanone

Concen: 0.438 ug/l

RT: 7.333 min Scan# 908

Delta R.T. 0.005 min

Lab File: VN072377.D

Acq: 09 May 2022 14:21

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 1335

Ion Ratio Lower Upper

43 100

72 23.2 23.7 35.5#

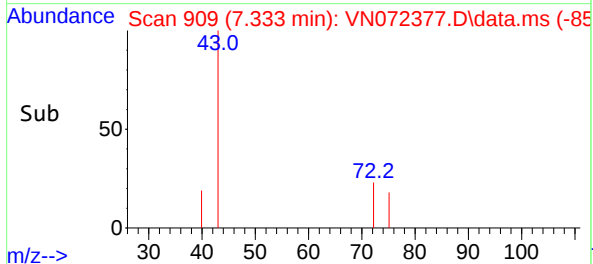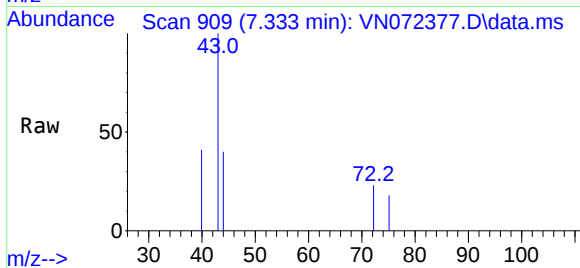

#29

Tetrahydrofuran

Concen: 0.323 ug/l

RT: 7.686 min Scan# 969

Delta R.T. 0.005 min

Lab File: VN072377.D

Acq: 09 May 2022 14:21




Tgt Ion: 42 Resp: 646


Ion Ratio Lower Upper

42 100

72 18.4 39.7 59.5#

71 9.6 36.6 55.0#

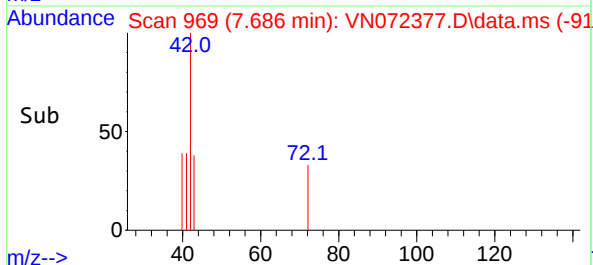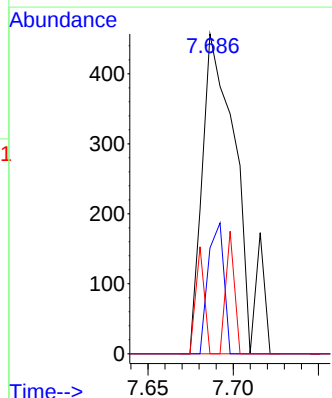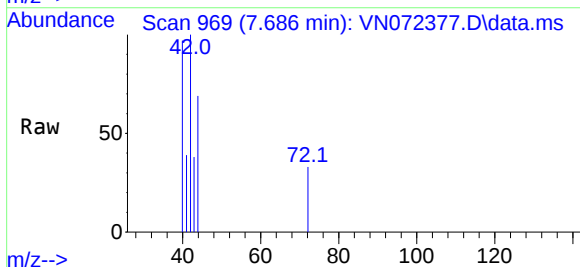



#31

Cyclohexane

Concen: 1.051 ug/l

RT: 8.080 min Scan# 1036

Delta R.T. -0.012 min


Lab File: VN072377.D

Acq: 09 May 2022 14:21

Instrument :

MSVOA_N

ClientSampleId :

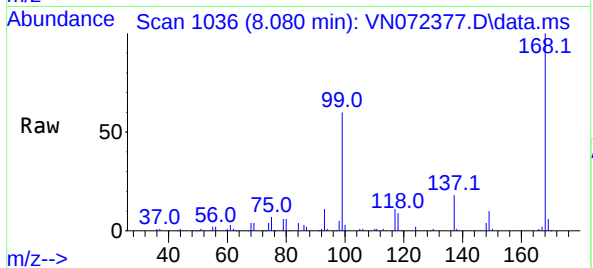




Tgt Ion: 56 Resp: 6232

Ion Ratio Lower Upper

56 100

69 166.1 27.8 41.8#

84 158.6 76.9 115.3#

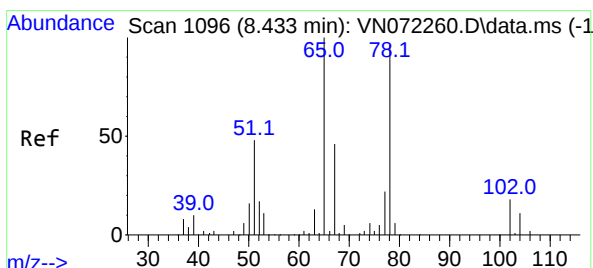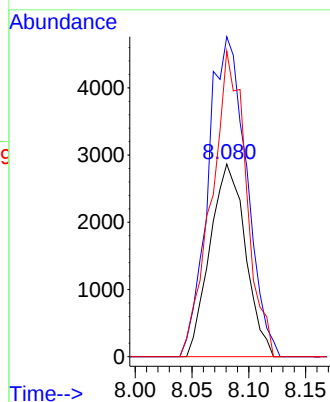

#33

1,2-Dichloroethane-d4

Concen: 45.631 ug/l

RT: 8.433 min Scan# 1096

Delta R.T. -0.001 min

Lab File: VN072377.D




Acq: 09 May 2022 14:21


Tgt Ion: 65 Resp: 202477

Ion Ratio Lower Upper

65 100

67 53.0 0.0 104.8

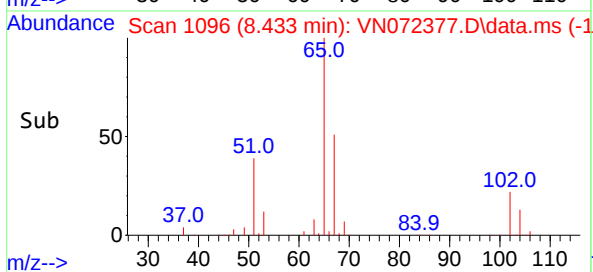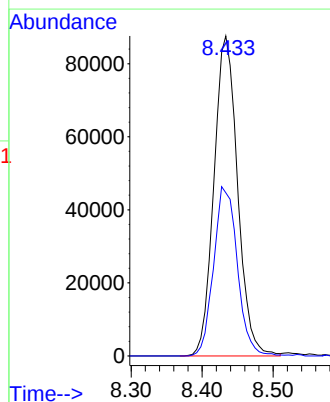



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072377.D

Acq: 09 May 2022 14:21

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 546812

Ion Ratio Lower Upper

114 100

63 20.7 0.0 40.0

88 16.2 0.0 32.6

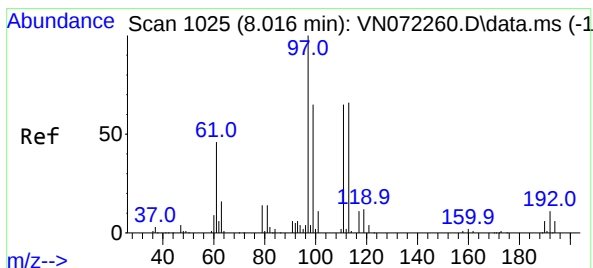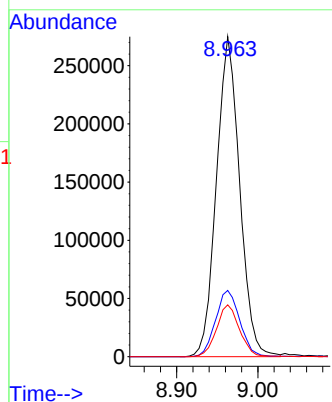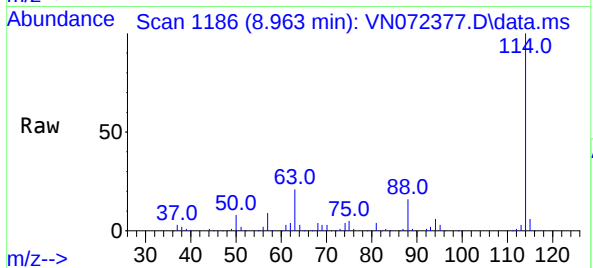

#35

Dibromofluoromethane

Concen: 47.070 ug/l

RT: 8.016 min Scan# 1025

Delta R.T. -0.000 min

Lab File: VN072377.D

Acq: 09 May 2022 14:21




Tgt Ion:113 Resp: 164741


Ion Ratio Lower Upper

113 100

111 101.8 81.4 122.0

192 19.3 17.0 25.6

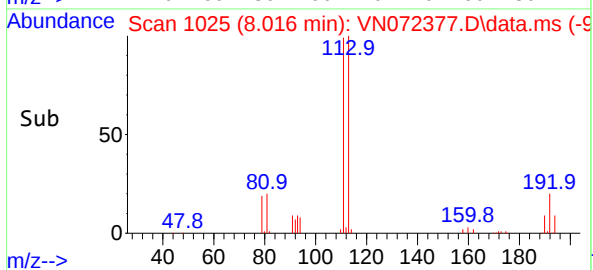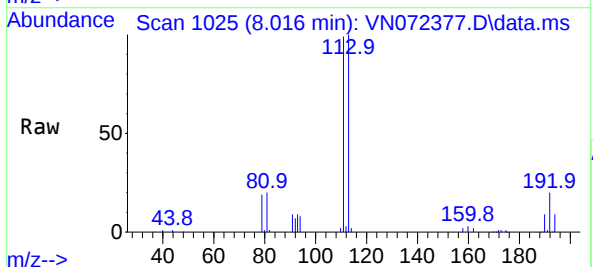

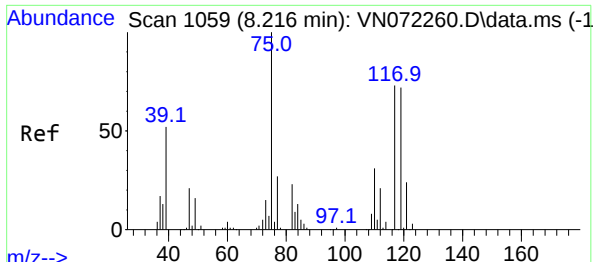

#36

1,1-Dichloropropene

Concen: 4.607 ug/l

RT: 8.086 min Scan# 1037

Delta R.T. -0.130 min


Lab File: VN072377.D

Acq: 09 May 2022 14:21

Instrument :

MSVOA_N

ClientSampleId :

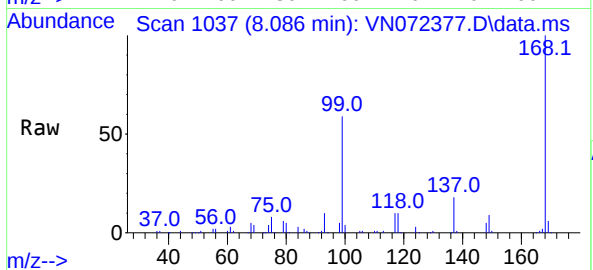




Tgt Ion: 75 Resp: 23470

Ion Ratio Lower Upper

75 100

110 9.3 18.3 54.8#

77 0.0 25.1 37.7#

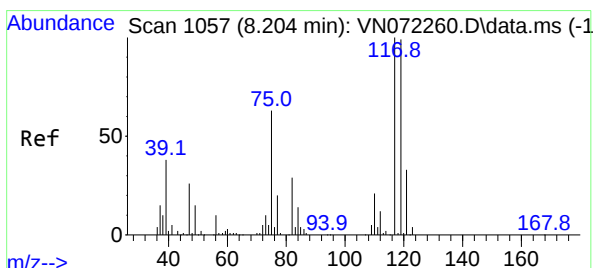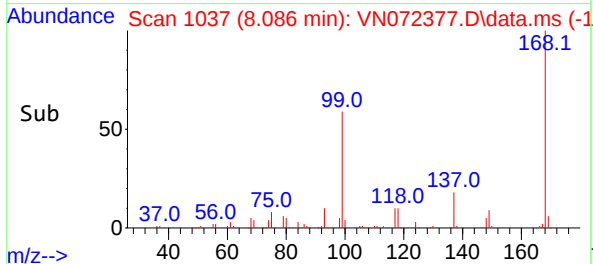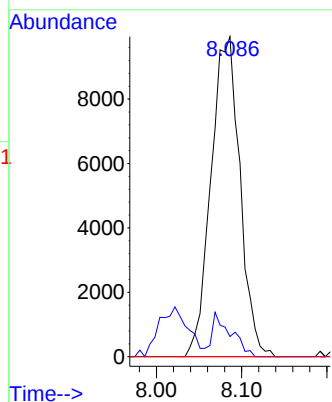

#38

Carbon Tetrachloride

Concen: 5.612 ug/l

RT: 8.080 min Scan# 1036

Delta R.T. -0.124 min

Lab File: VN072377.D

Acq: 09 May 2022 14:21




Tgt Ion: 117 Resp: 30622


Ion Ratio Lower Upper

117 100

119 3.6 75.8 113.8#


121 0.0 24.6 37.0#

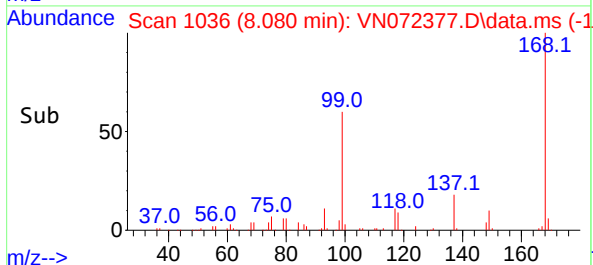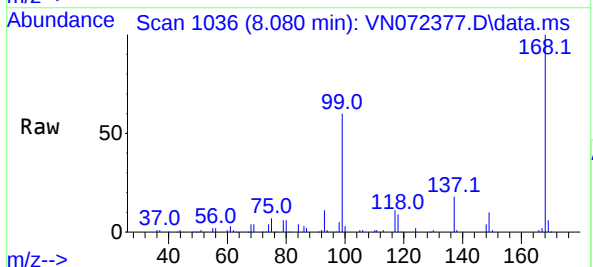






#43
Isopropyl Acetate
Concen: 0.811 ug/l
RT: 8.551 min Scan# 111
Delta R.T. -0.006 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21


Instrument :
MSVOA_N
ClientSampleId :

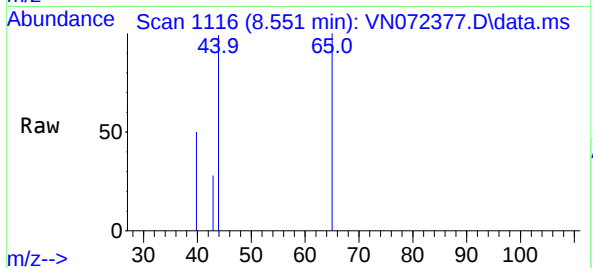



Tgt Ion: 43 Resp: 111
Ion Ratio Lower Upper
43 100
61 0.0 21.9 32.9#
87 0.0 12.0 18.0#

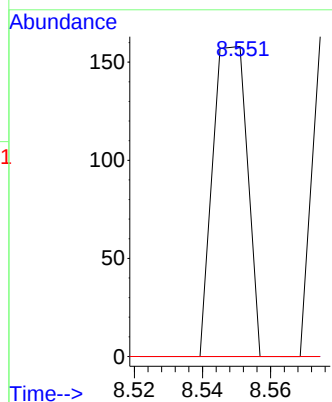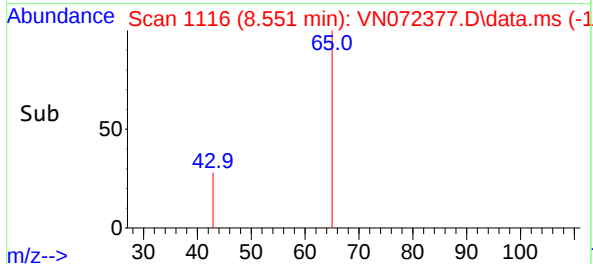


#49
1,4-Dioxane
Concen: 0.841 ug/l
RT: 9.569 min Scan# 1289
Delta R.T. 0.006 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

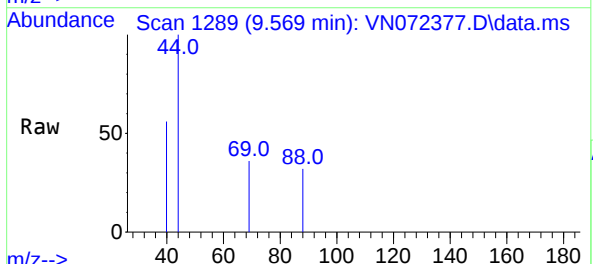

Tgt Ion: 88 Resp: 66
Ion Ratio Lower Upper
88 100
43 0.0 20.2 30.4#
58 0.0 54.2 81.4#




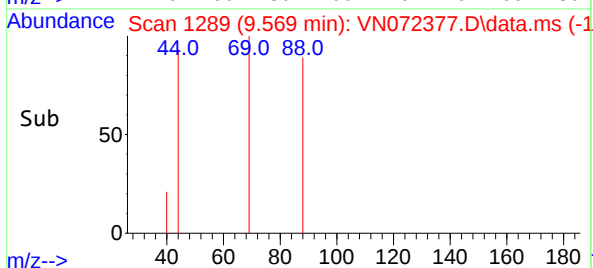




#50
Toluene-d8
Concen: 50.412 ug/l
RT: 10.433 min Scan# 1437
Delta R.T. -0.006 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 693294
Ion Ratio Lower Upper
98 100
100 64.2 52.6 78.8



#51
4-Methyl-2-Pentanone
Concen: 0.373 ug/l
RT: 10.321 min Scan# 1417
Delta R.T. -0.007 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21


Tgt Ion: 43 Resp: 2378
Ion Ratio Lower Upper
43 100
58 34.8 34.1 51.1

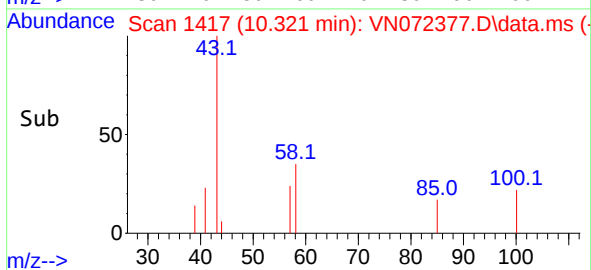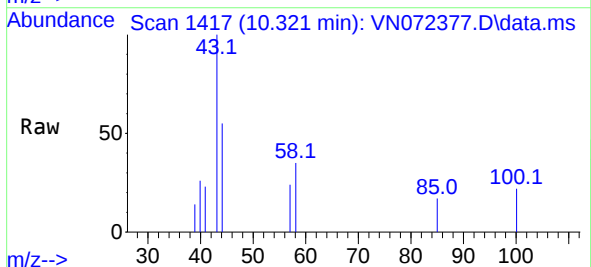






#56
Ethyl methacrylate
Concen: 2.423 ug/l
RT: 10.769 min Scan# 1493
Delta R.T. 0.012 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 69 Resp: 421
Ion Ratio Lower Upper
69 100
41 64.6 47.8 71.6
39 0.0 27.3 40.9#

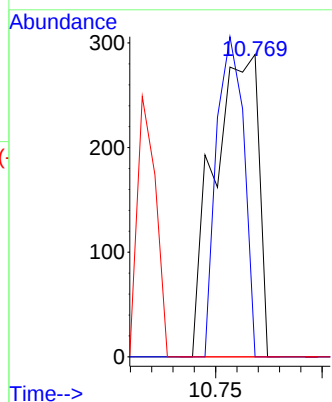

#59
2-Hexanone
Concen: 1.305 ug/l
RT: 11.086 min Scan# 1547
Delta R.T. 0.005 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

Tgt Ion: 43 Resp: 5868
Ion Ratio Lower Upper
43 100
58 51.0 29.7 89.1


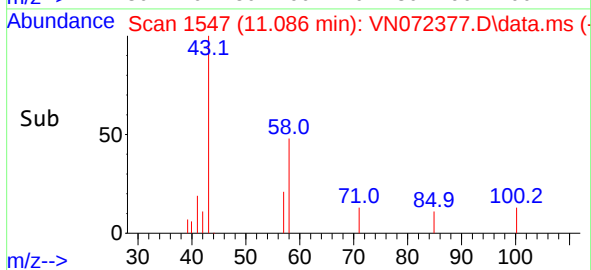






#62
4-Bromofluorobenzene
Concen: 59.383 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 271069
Ion Ratio Lower Upper
95 100
174 74.6 0.0 167.6
176 72.2 0.0 163.4



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

Tgt Ion: 117 Resp: 585839
Ion Ratio Lower Upper
117 100
82 57.9 44.2 66.2
119 32.8 25.4 38.0



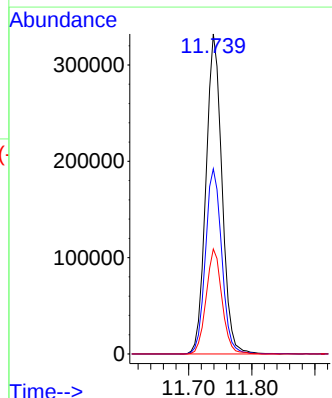



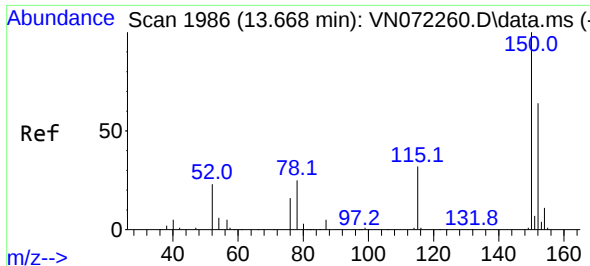

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. -0.001 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 228722
Ion Ratio Lower Upper
152 100
115 60.6 28.9 86.7
150 156.8 0.0 356.2

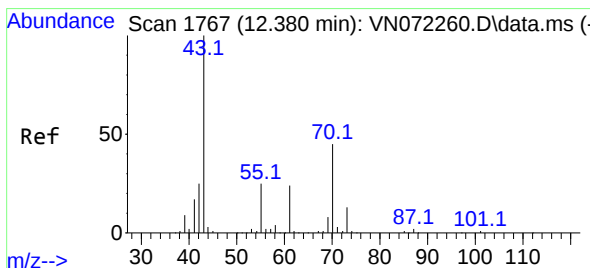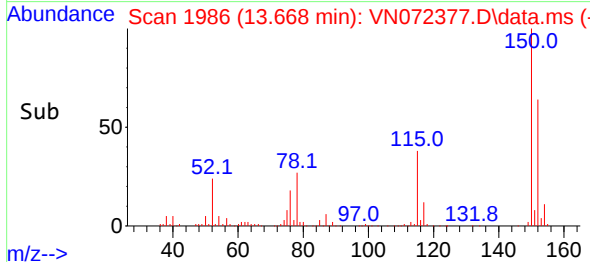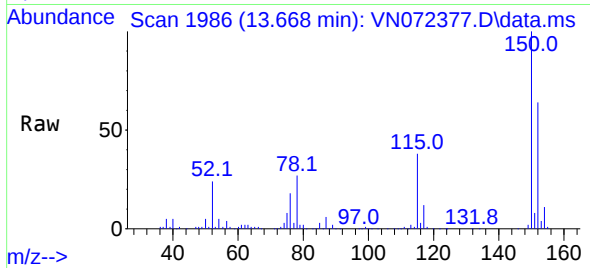

#74
N-ethyl acetate
Concen: 0.473 ug/l
RT: 12.380 min Scan# 1767
Delta R.T. 0.000 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21


Tgt Ion: 43 Resp: 3580
Ion Ratio Lower Upper
43 100
70 38.0 39.0 58.4#
55 23.8 21.1 31.7
61 18.5 21.1 31.7#

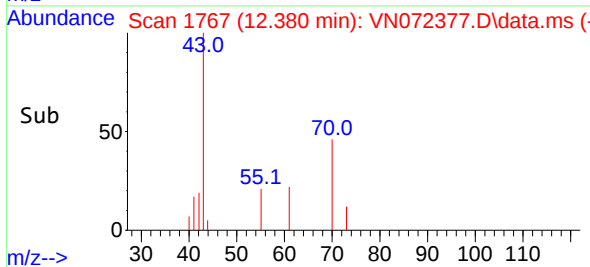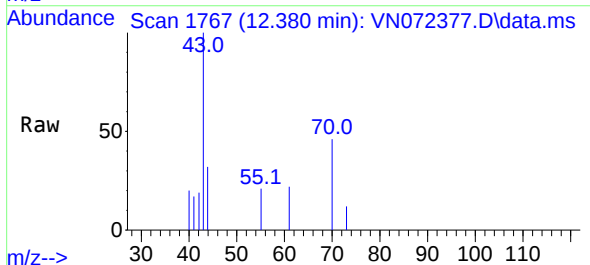






#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.815 min Scan# 1841
Delta R.T. -0.007 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21


Instrument :
MSVOA_N
ClientSampleId :

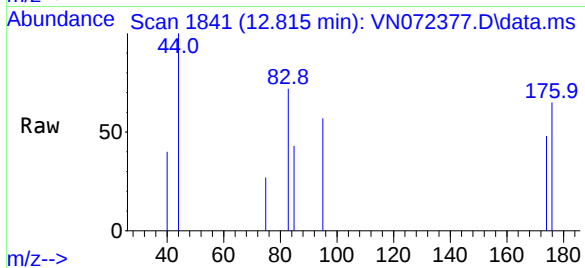



Tgt Ion: 83 Resp: 656
Ion Ratio Lower Upper
83 100
131 0.0 5.3 15.9#
85 68.6 32.3 96.9

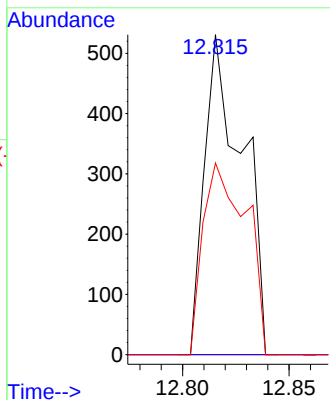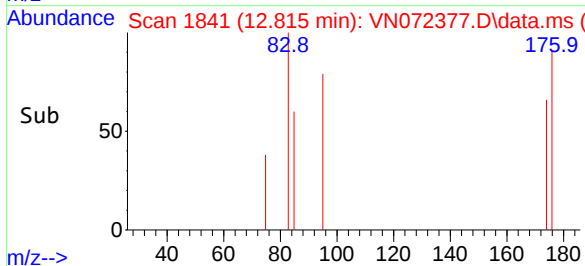


#76
1,2,3-Trichloropropane
Concen: 26.581 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

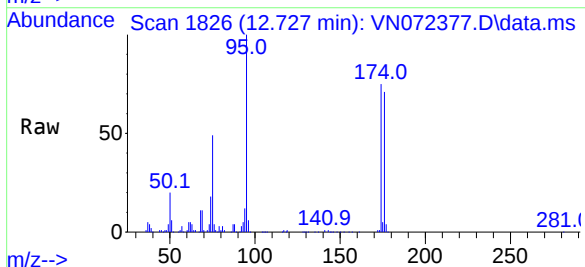


Tgt Ion: 75 Resp: 136702
Ion Ratio Lower Upper
75 100
77 1.2 98.5 295.5#

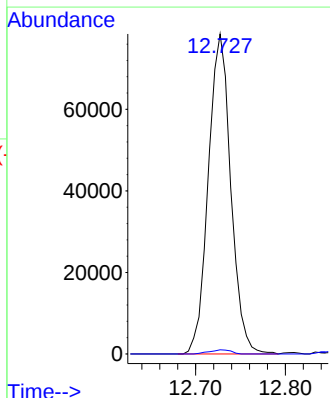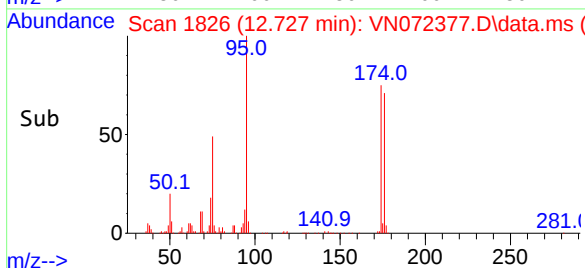






#81
trans-1,4-Dichloro-2-butene
Concen: 69.107 ug/l
RT: 12.727 min Scan# 1808
Delta R.T. 0.105 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 75 Resp: 136702
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#




#87
1,3-Dichlorobenzene
Concen: 0.237 ug/l
RT: 13.610 min Scan# 1976
Delta R.T. -0.000 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21




Tgt Ion:146 Resp: 1833
Ion Ratio Lower Upper
146 100
111 53.3 20.0 60.0
148 55.4 32.0 96.0








#88
1,4-Dichlorobenzene
Concen: 0.244 ug/l
RT: 13.610 min Scan# 1990
Delta R.T. -0.082 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:146 Resp: 1833
Ion Ratio Lower Upper
146 100
111 53.3 19.1 57.1
148 55.4 31.4 94.3



#89
n-Butylbenzene
Concen: 0.327 ug/l
RT: 13.933 min Scan# 2031
Delta R.T. -0.006 min
Lab File: VN072377.D
Acq: 09 May 2022 14:21

Tgt Ion: 91 Resp: 3760
Ion Ratio Lower Upper
91 100
92 55.7 26.9 80.7
134 26.2 13.6 40.8

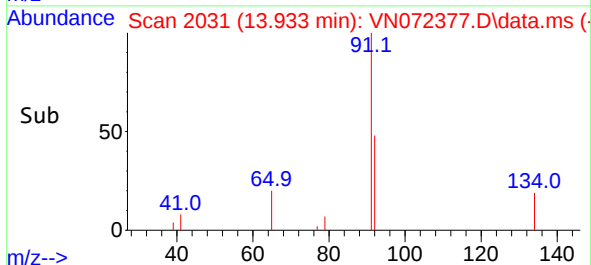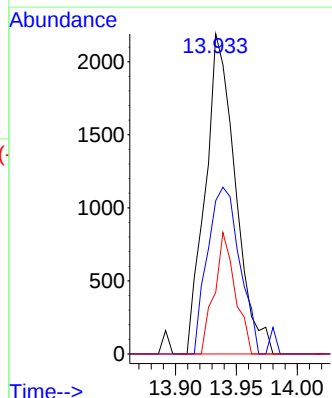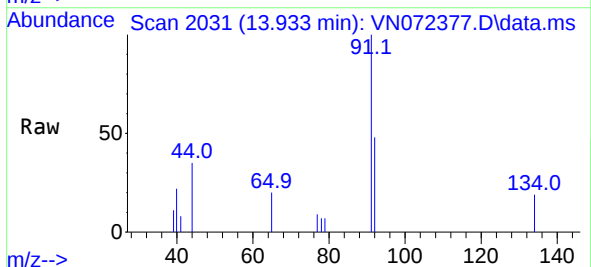



#91

1,2-Dichlorobenzene

Concen: 0.249 ug/l

RT: 13.986 min Scan# 2039

Delta R.T. -0.000 min

Lab File: VN072377.D

Acq: 09 May 2022 14:21

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:146 Resp: 1899

Ion Ratio Lower Upper

146 100

111 44.2 20.9 62.8

148 63.5 32.1 96.3

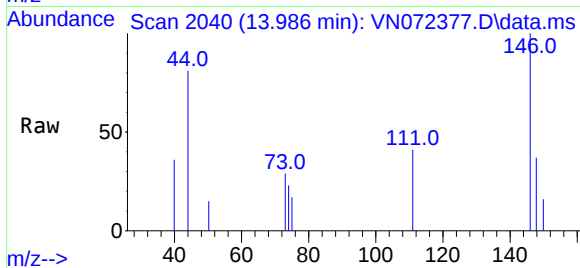

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.415 ug/l

RT: 14.604 min Scan# 2145

Delta R.T. 0.006 min

Lab File: VN072377.D

Acq: 09 May 2022 14:21




Tgt Ion: 75 Resp: 580


Ion Ratio Lower Upper

75 100

155 50.2 44.9 134.5


157 25.9 59.0 176.8#

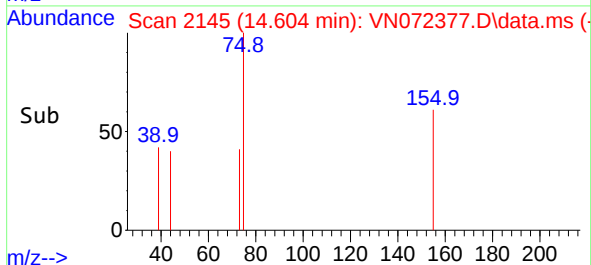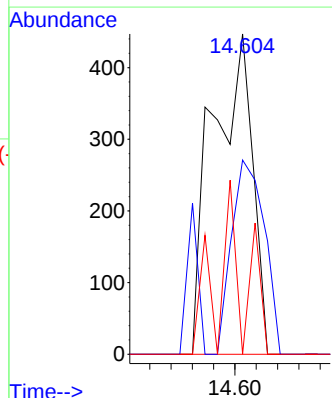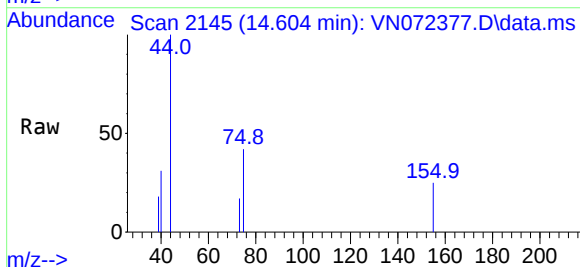






#93
 1,2,4-Trichlorobenzene
 Concen: 3.135 ug/l
 RT: 15.262 min Scan# 21
 Delta R.T. 0.005 min
 Lab File: VN072377.D
 Acq: 09 May 2022 14:21

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion:180 Resp: 2647




Ion	Ratio	Lower	Upper
180	100		
182	90.2	47.5	142.5
145	24.6	14.5	43.5

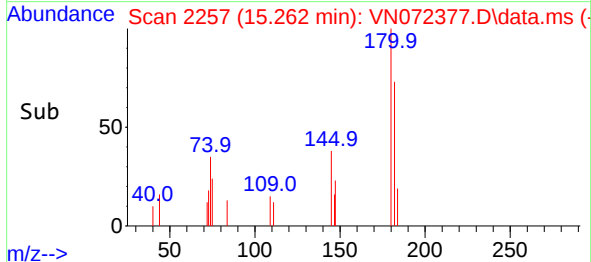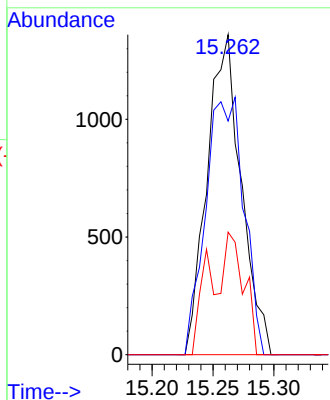


#95
 Naphthalene
 Concen: 5.029 ug/l
 RT: 15.498 min Scan# 2297
 Delta R.T. -0.000 min
 Lab File: VN072377.D
 Acq: 09 May 2022 14:21

Tgt Ion:128 Resp: 9454


Ion	Ratio	Lower	Upper
128	100		
127	9.0	10.3	15.5#
129	6.2	8.6	13.0#

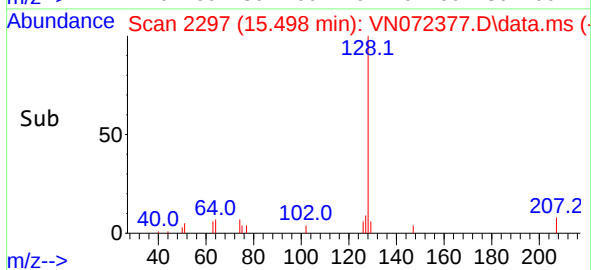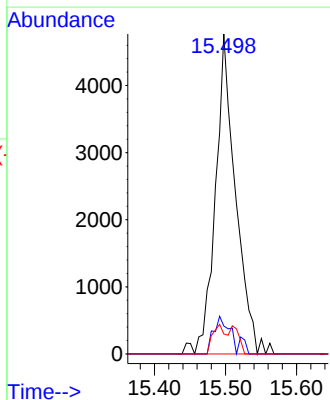



#96
 1,2,3-Trichlorobenzene
 Concen: 3.411 ug/l
 RT: 15.686 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VN072377.D
 Acq: 09 May 2022 14:21

Instrument :
 MSVOA_N
 ClientSampleId :

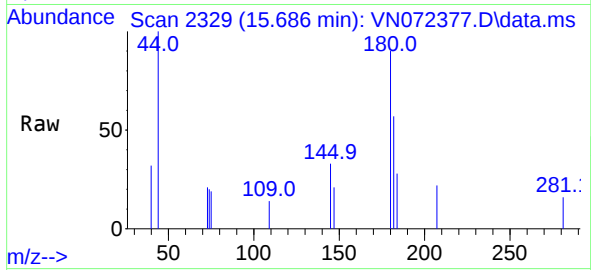

Tgt Ion:180 Resp: 2737

Ion	Ratio	Lower	Upper
180	100		
182	91.2	47.8	143.3
145	29.4	15.5	46.5

