


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050922\
 Data File : VN072371.D
 Acq On : 09 May 2022 09:17
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042622W.M
 Title : SW846 8260
 Last Update : Tue Apr 26 18:50:11 2022

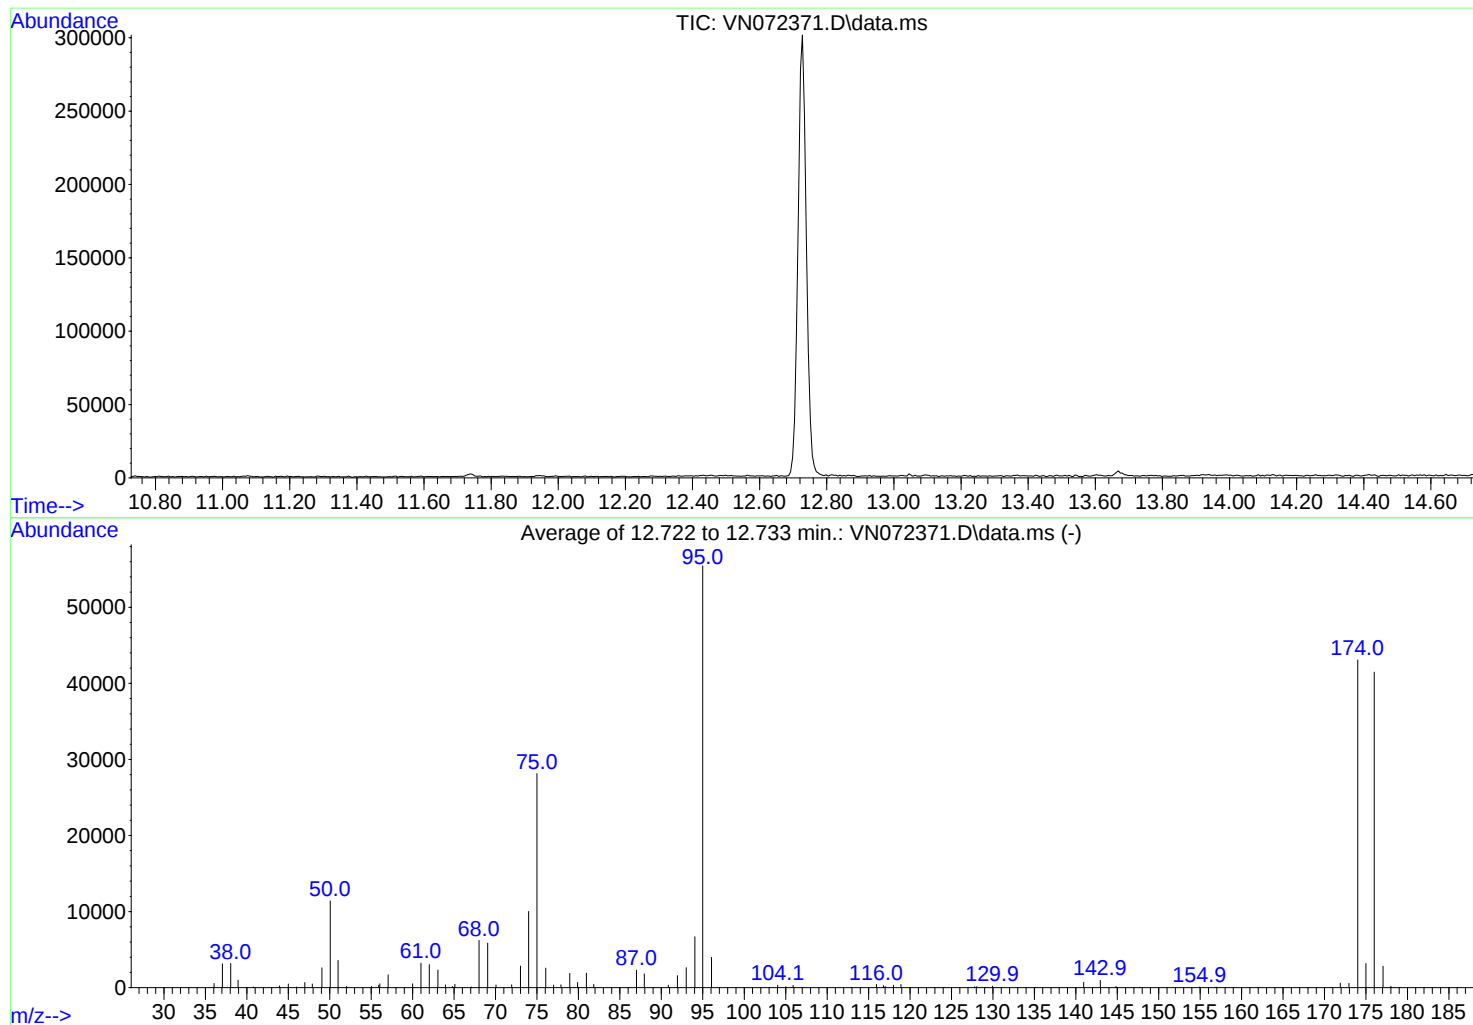

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	11400	PASS
75	95	30	60	50.8	28144	PASS
95	95	100	100	100.0	55451	PASS
96	95	5	9	7.2	3968	PASS
173	174	0.00	2	1.3	563	PASS
174	95	50	100	77.7	43088	PASS
175	174	5	9	7.4	3180	PASS
176	174	95	101	96.3	41477	PASS
177	176	5	9	6.8	2826	PASS