
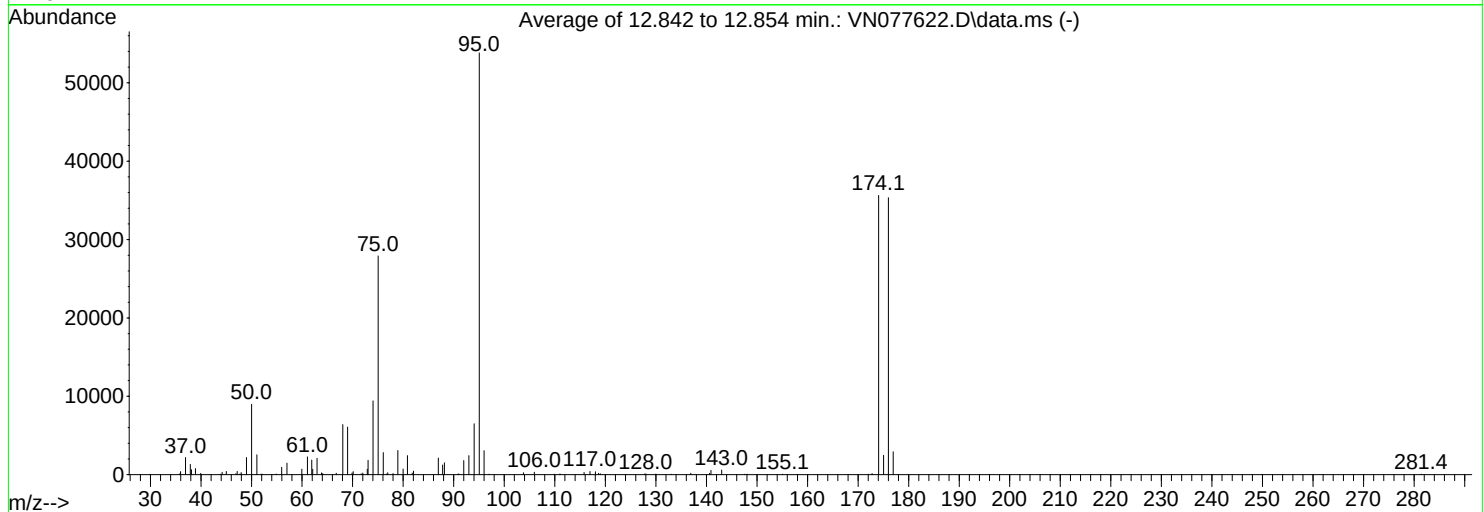


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050923\
Data File : VN077622.D
Acq On : 09 May 2023 09:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N050923W.M
Title : SW846 8260
Last Update : Wed May 10 13:06:57 2023

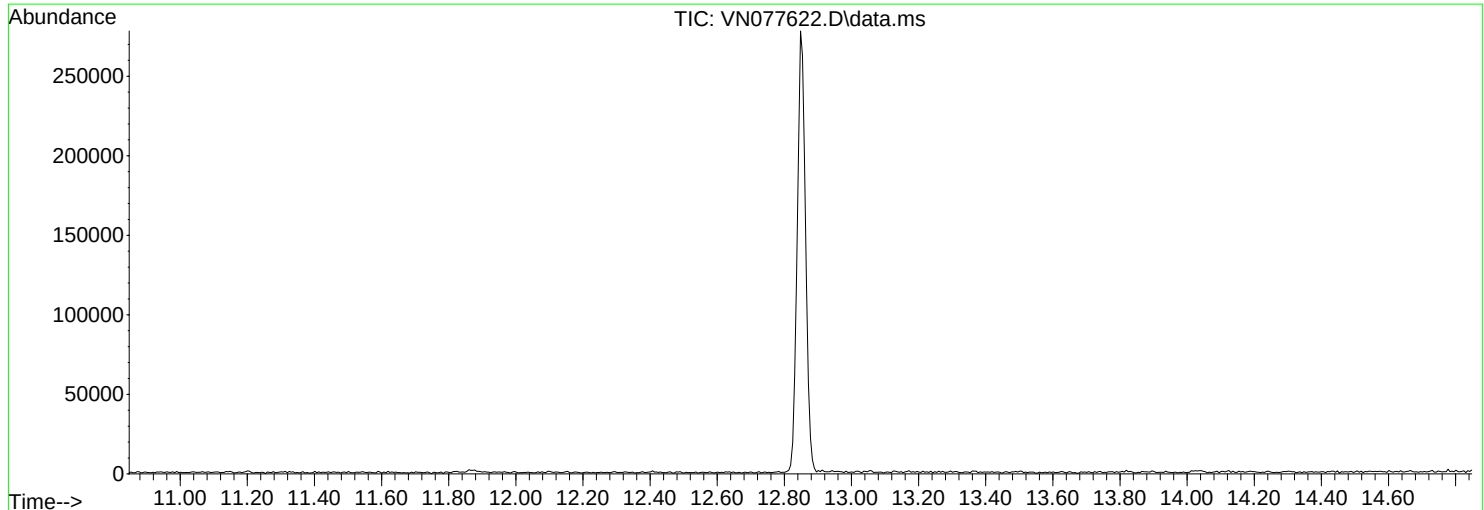

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	8988	PASS
75	95	30	60	51.8	27904	PASS
95	95	100	100	100.0	53829	PASS
96	95	5	9	5.7	3054	PASS
173	174	0.00	2	0.4	142	PASS
174	95	50	100	66.2	35635	PASS
175	174	5	9	7.0	2480	PASS
176	174	95	101	99.2	35341	PASS
177	176	5	9	8.3	2921	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	106	47.15	401	59.95	702	70.10	391
35.95	381	47.70	87	61.05	2270	71.70	107
36.95	2184	47.95	262	61.90	1860	72.00	21
37.90	1298	49.00	2189	62.10	689	72.90	69
38.10	631	50.00	8988	62.95	2079	73.05	1831
38.90	781	51.05	2543	63.85	234	74.05	9416
39.95	163	51.90	72	64.10	144	75.05	27904
43.90	64	52.10	52	66.75	195	76.05	2827
44.20	316	54.90	85	68.05	6400	76.70	92
45.00	417	55.95	948	69.00	6070	76.95	245
46.90	114	57.00	1472	69.90	229	78.00	145

Average of 12.842 to 12.854 min.: VN077622.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.95	3079	93.00	2432	116.95	415	143.00	601
80.00	724	94.05	6503	118.05	376	147.60	63
80.85	2436	95.05	53829	118.65	163	148.10	54
81.80	199	96.00	3054	119.00	118	155.10	56
82.05	444	97.00	57	127.80	86	172.00	64
86.95	2118	103.80	239	128.00	102	172.75	142
87.80	1227	105.95	302	130.00	75	174.05	35635
88.15	1517	109.90	67	133.00	73	175.05	2480
90.80	69	110.90	55	136.90	179	176.00	35341
91.00	94	111.10	62	140.60	172	176.95	2921
92.00	1807	115.80	287	140.90	544	281.40	63

Instrument :

MSVOA_N

ClientSampleId :

BFB