
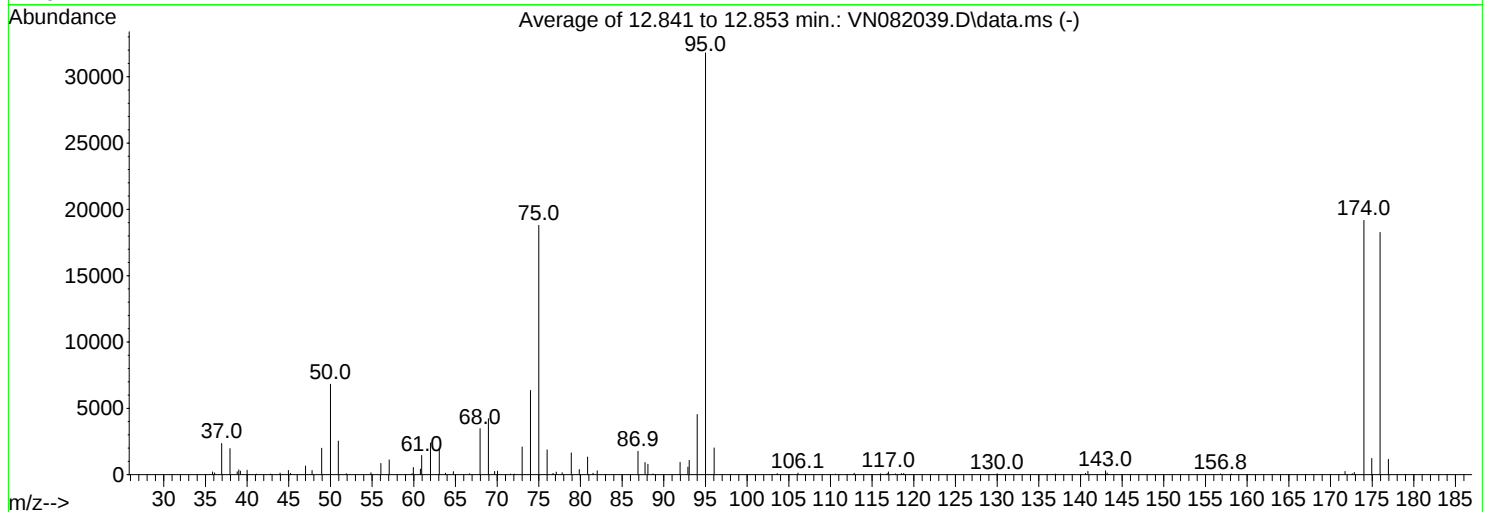


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050924\
Data File : VN082039.D
Acq On : 09 May 2024 09:28
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Title : SW846 8260
Last Update : Fri Apr 26 05:26:49 2024

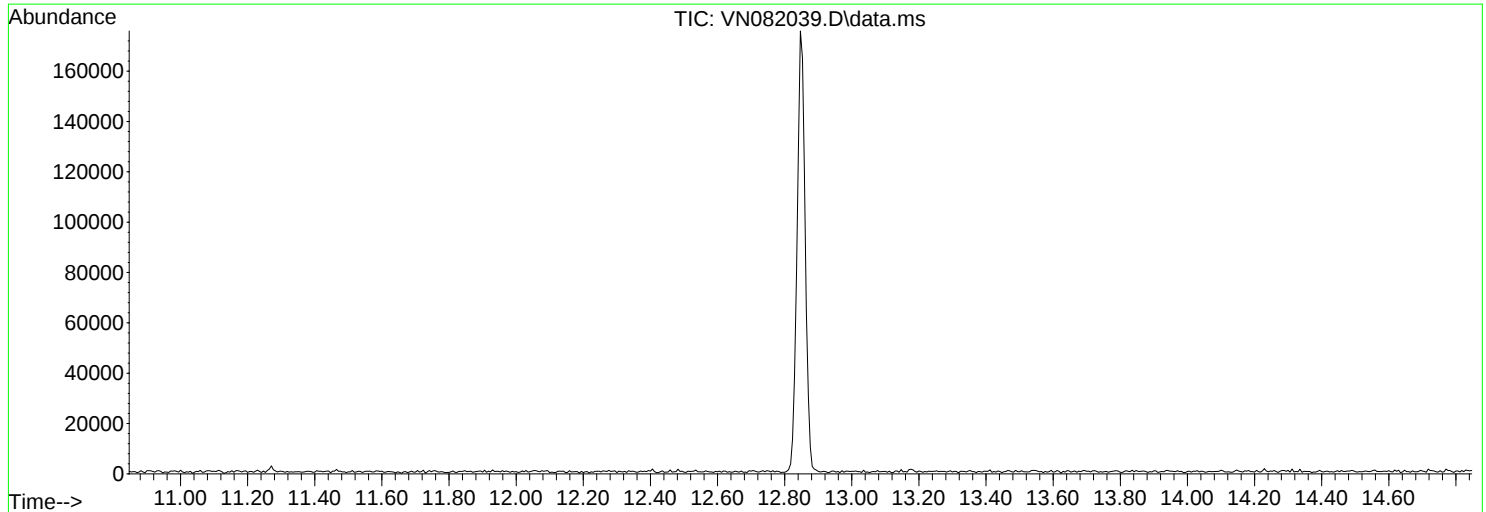

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	6818	PASS
75	95	30	60	59.1	18800	PASS
95	95	100	100	100.0	31800	PASS
96	95	5	9	6.3	2012	PASS
173	174	0.00	2	0.9	165	PASS
174	95	50	100	60.3	19170	PASS
175	174	5	9	6.4	1225	PASS
176	174	95	101	95.3	18262	PASS
177	176	5	9	6.3	1158	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	210	44.95	308	59.80	74	69.70	246
36.10	136	45.20	95	59.95	538	70.05	260
36.95	2357	47.00	650	60.80	419	71.60	51
37.95	1963	47.80	312	60.95	1447	72.10	51
38.80	223	48.95	1987	62.00	2394	73.00	2092
39.00	365	50.00	6818	63.05	1974	74.00	6342
39.20	267	50.95	2539	63.80	113	75.00	18800
40.00	341	51.90	77	64.75	234	76.00	1866
41.10	55	54.85	151	66.70	71	76.70	101
42.80	51	56.05	851	67.95	3475	77.10	192
43.95	116	57.05	1114	68.95	4228	77.80	147

Average of 12.841 to 12.853 min.: VN082039.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.90	1638	93.05	1077	117.80	56	171.75	246
79.85	384	94.00	4536	118.50	81	172.60	69
80.85	1332	95.00	31800	118.80	92	172.85	165
81.50	104	96.05	2012	130.00	74	174.00	19170
82.00	289	103.60	82	137.00	54	174.95	1225
86.90	1763	106.10	126	140.60	103	175.95	18262
87.75	918	110.60	50	140.90	248	176.95	1158
88.10	789	112.85	108	143.00	284		
88.70	58	116.00	68	143.20	122		
91.95	929	116.80	83	156.80	60		
92.90	566	116.95	210	158.10	55		

Instrument :

MSVOA_N

ClientSampleId :

BFB