

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050925\
 Data File : VN086554.D
 Acq On : 09 May 2025 11:34
 Operator : JC\MD
 Sample : VN0509MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0509MBL01

Quant Time: May 09 23:24:09 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
 Quant Title : SW846 8260
 QLast Update : Wed Apr 16 04:19:23 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.218	168	161578	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	304753	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	283891	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	123333	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.571	65	114071	48.685	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	97.380%		
35) Dibromofluoromethane	8.159	113	89742	63.449	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	126.900%#		
50) Toluene-d8	10.565	98	382413	50.589	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	101.180%		
62) 4-Bromofluorobenzene	12.847	95	133637	48.469	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery =	96.940%		
Target Compounds						Qvalue
3) Chloromethane	2.359	50	2863	1.028	ug/l #	82
5) Bromomethane	2.971	94	923	0.772	ug/l	96
10) Methyl Iodide	4.589	142	1079	0.551	ug/l #	42
13) Acrolein	4.165	56	57	Below Cal	#	13
15) Acrylonitrile	5.718	53	749	0.709	ug/l #	54
16) Acetone	4.430	43	1014	Below Cal	#	43
17) Carbon Disulfide	4.712	76	3305	0.580	ug/l #	74
20) Methylene Chloride	5.271	84	467	0.216	ug/l #	49
25) 2-Butanone	7.477	43	625	0.429	ug/l #	48
29) Tetrahydrofuran	7.841	42	592	0.607	ug/l #	41
31) Cyclohexane	8.224	56	3948	1.040	ug/l #	26
36) 1,1-Dichloropropene	8.224	75	13217	4.679	ug/l #	50
38) Carbon Tetrachloride	8.224	117	16180	6.014	ug/l #	15
43) Isopropyl Acetate	8.671	43	2914	Below Cal	#	55
51) 4-Methyl-2-Pentanone	10.441	43	686	0.225	ug/l #	35
59) 2-Hexanone	11.200	43	1354	0.599	ug/l	68
71) Bromoform	12.841	173	550	0.350	ug/l #	1
76) 1,2,3-Trichloropropane	12.847	75	68304	23.468	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	68304	56.362	ug/l #	10
85) sec-Butylbenzene	13.612	105	2536	0.256	ug/l	96
86) p-Isopropyltoluene	13.729	119	1993	0.244	ug/l	92
87) 1,3-Dichlorobenzene	13.735	146	1223	0.291	ug/l	94
88) 1,4-Dichlorobenzene	13.735	146	1223	0.289	ug/l	95
89) n-Butylbenzene	14.053	91	3378	0.466	ug/l	97
91) 1,2-Dichlorobenzene	14.106	146	1313	0.322	ug/l	87
93) 1,2,4-Trichlorobenzene	15.388	180	1979	1.014	ug/l	85
94) Hexachlorobutadiene	15.500	225	1083	1.471	ug/l	94
95) Naphthalene	15.635	128	9157	1.324	ug/l	97
96) 1,2,3-Trichlorobenzene	15.835	180	2206	1.194	ug/l	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050925\
Data File : VN086554.D
Acq On : 09 May 2025 11:34
Operator : JC\MD
Sample : VN0509MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01

Quant Time: May 09 23:24:09 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Quant Title : SW846 8260
QLast Update : Wed Apr 16 04:19:23 2025
Response via : Initial Calibration




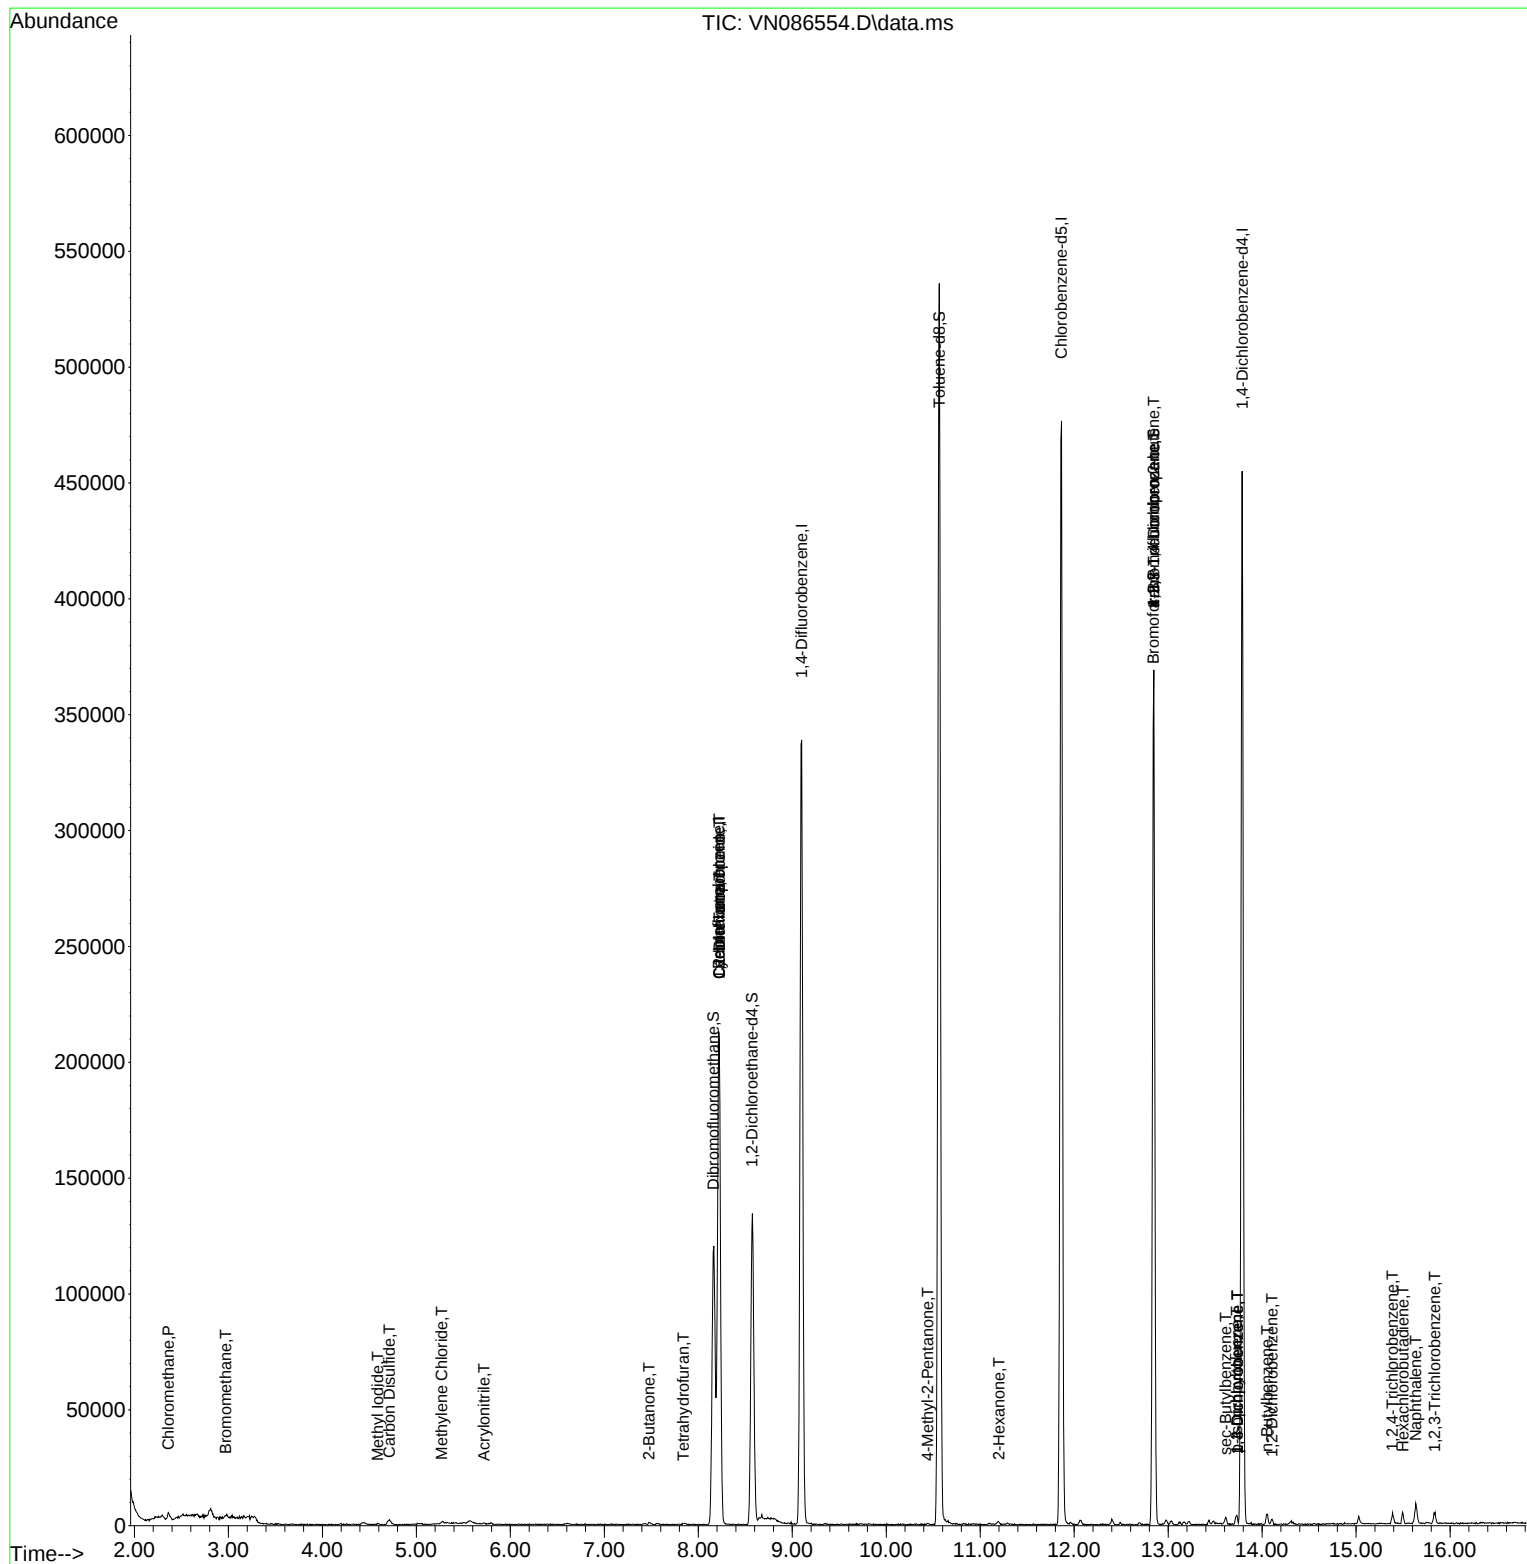




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34




Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01

Tgt Ion:168 Resp: 161578
Ion Ratio Lower Upper
168 100
99 59.1 52.5 78.7



#3
Chloromethane
Concen: 1.028 ug/l
RT: 2.359 min Scan# 69
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion: 50 Resp: 2863
Ion Ratio Lower Upper
50 100
52 43.2 26.5 39.7#


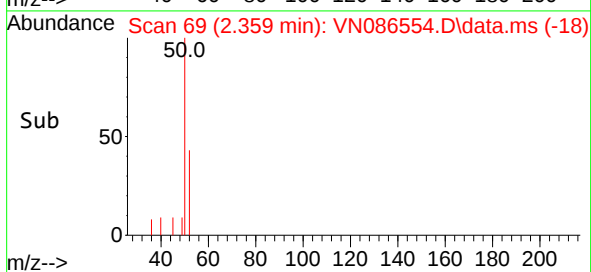

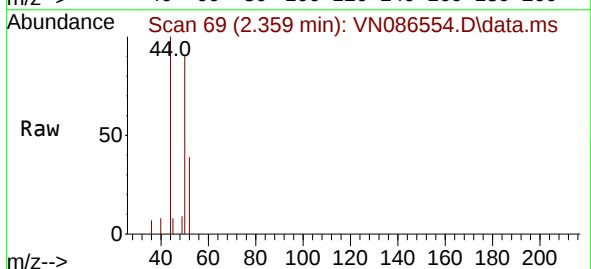




#5
Bromomethane
Concen: 0.772 ug/l
RT: 2.971 min Scan# 11
Delta R.T. 0.018 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34




Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01


Tgt Ion: 94 Resp: 923
Ion Ratio Lower Upper
94 100
96 97.6 75.2 112.8

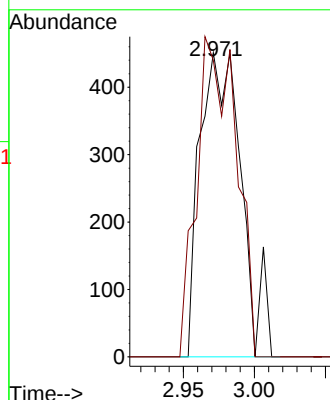

#10
Methyl Iodide
Concen: 0.551 ug/l
RT: 4.589 min Scan# 448
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion: 142 Resp: 1079
Ion Ratio Lower Upper
142 100
127 0.0 32.7 49.1#
141 0.0 11.7 17.5#



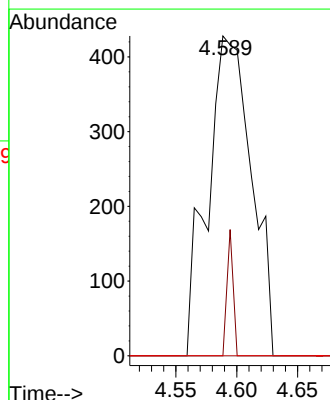





#13
Acrolein
Concen: Below Cal
RT: 4.165 min Scan# 31
Delta R.T. -0.012 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34




Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01


Tgt Ion: 56 Resp: 57
Ion Ratio Lower Upper
56 100
55 0.0 58.5 87.7#



#15
Acrylonitrile
Concen: 0.709 ug/l
RT: 5.718 min Scan# 640
Delta R.T. 0.006 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion: 53 Resp: 749
Ion Ratio Lower Upper
53 100
52 46.5 65.5 98.3#
51 0.0 28.6 42.8#









#16
Acetone
Concen: Below Cal
RT: 4.430 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34




Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01


Tgt Ion: 43 Resp: 1014
Ion Ratio Lower Upper
43 100
58 0.0 25.3 37.9#



#17
Carbon Disulfide
Concen: 0.580 ug/l
RT: 4.712 min Scan# 469
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion: 76 Resp: 3305
Ion Ratio Lower Upper
76 100
78 0.0 7.6 11.4#


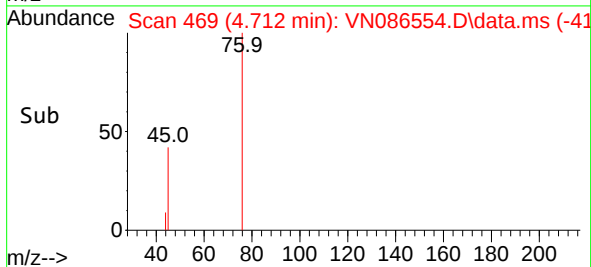

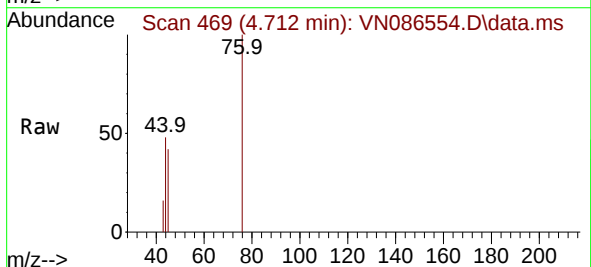




#20
Methylene Chloride
Concen: 0.216 ug/l
RT: 5.271 min Scan# 50
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34




Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01


Tgt Ion: 84	Resp:	467
Ion	Ratio	Lower Upper
84	100	
49	87.1	98.2 147.2#
51	0.0	29.8 44.6#
86	0.0	52.0 78.0#

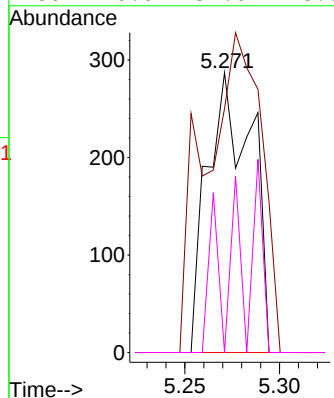

#25
2-Butanone
Concen: 0.429 ug/l
RT: 7.477 min Scan# 939
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion: 43	Resp:	625
Ion	Ratio	Lower Upper
43	100	
72	0.0	21.7 32.5#

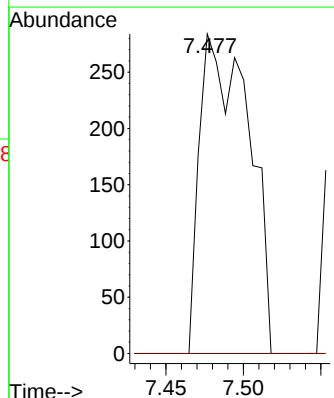



#29

Tetrahydrofuran

Concen: 0.607 ug/l

RT: 7.841 min Scan# 1066

Delta R.T. 0.006 min

Lab File: VN086554.D

Acq: 09 May 2025 11:34





Instrument :

MSVOA_N

ClientSampleId :

VN0509MBL01

Tgt Ion:	42	Resp:	592
Ion	Ratio	Lower	Upper
42	100		
72	11.5	36.2	54.4#
71	0.0	34.0	51.0#

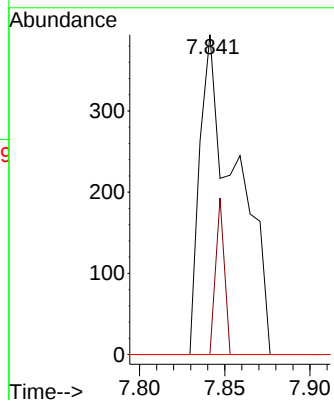

#31

Cyclohexane

Concen: 1.040 ug/l




RT: 8.224 min Scan# 1066


Delta R.T. -0.030 min

Lab File: VN086554.D

Acq: 09 May 2025 11:34

Tgt Ion:	56	Resp:	3948
Ion	Ratio	Lower	Upper
56	100		
69	134.9	24.2	36.2#
84	118.9	70.3	105.5#


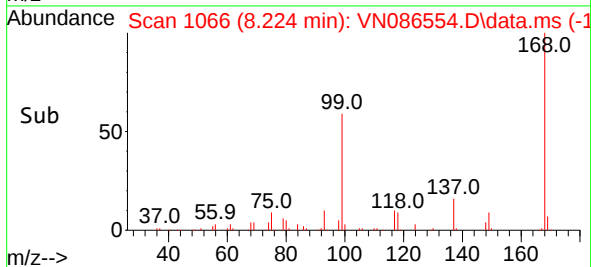
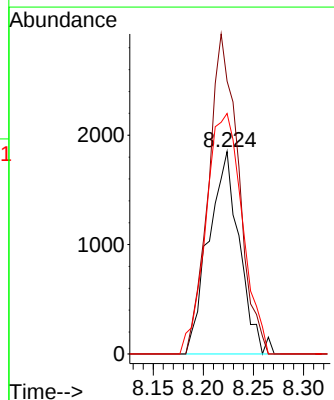
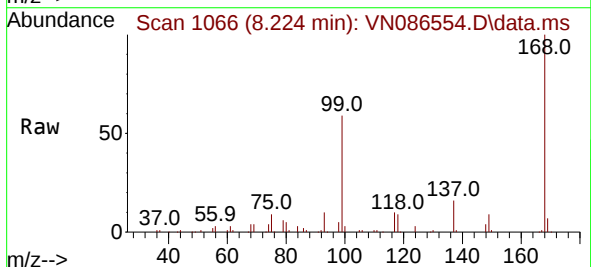


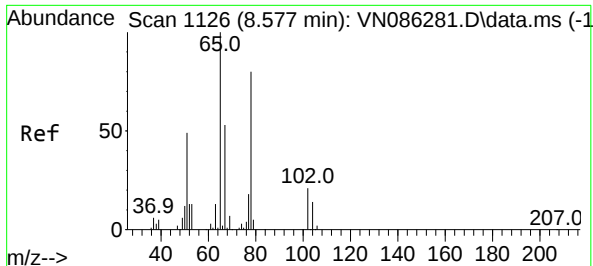

#33
 1,2-Dichloroethane-d4
 Concen: 48.685 ug/l
 RT: 8.571 min Scan# 1126
 Delta R.T. -0.006 min
 Lab File: VN086554.D
 Acq: 09 May 2025 11:34




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0509MBL01


Tgt Ion: 65 Resp: 114071
 Ion Ratio Lower Upper
 65 100
 67 51.6 0.0 106.0

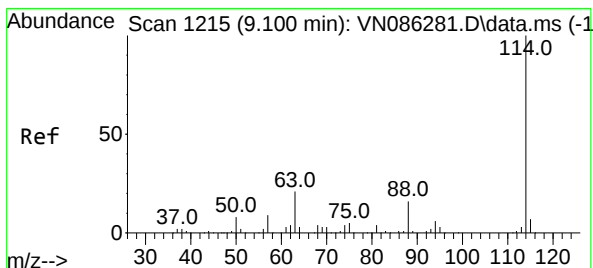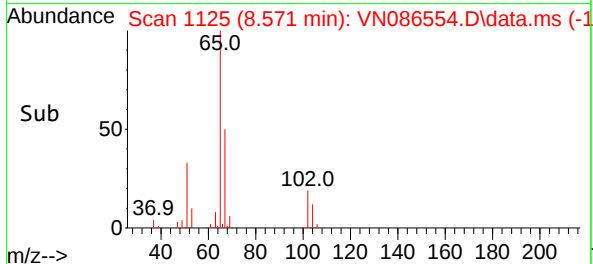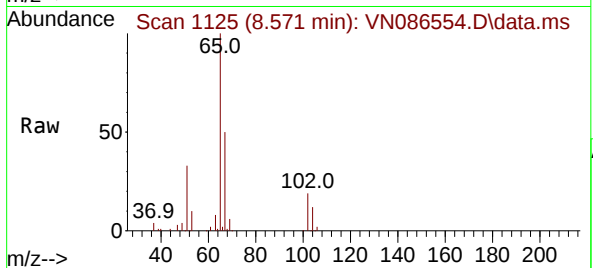

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 9.100 min Scan# 1215
 Delta R.T. -0.000 min
 Lab File: VN086554.D
 Acq: 09 May 2025 11:34

Tgt Ion: 114 Resp: 304753
 Ion Ratio Lower Upper
 114 100
 63 19.8 0.0 42.6
 88 15.2 0.0 31.8

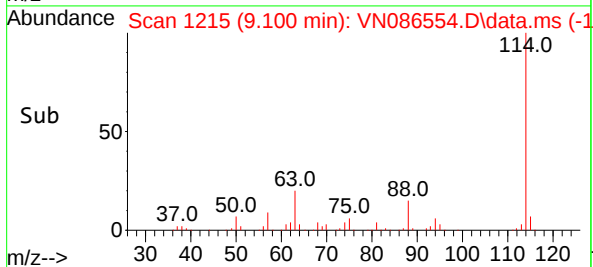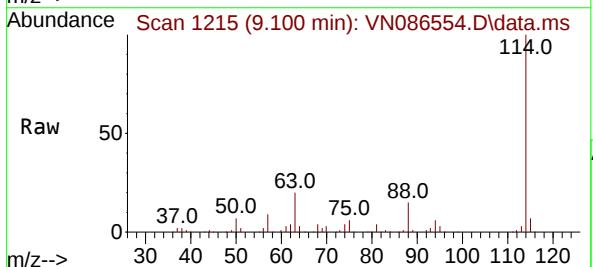

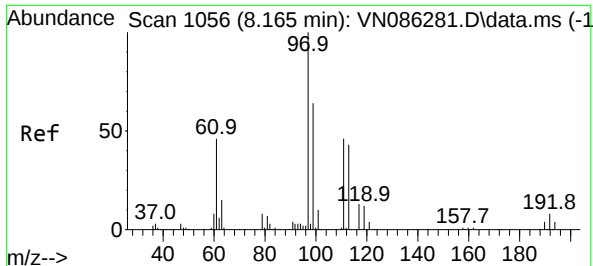

#35

Dibromofluoromethane

Concen: 63.449 ug/l

RT: 8.159 min Scan# 1055

Delta R.T. -0.006 min

Lab File: VN086554.D

Acq: 09 May 2025 11:34

Instrument :

MSVOA_N

ClientSampleId :

VN0509MBL01





Tgt Ion:113 Resp: 89742

Ion Ratio Lower Upper

113 100

111 103.9 83.4 125.0

192 17.8 13.7 20.5

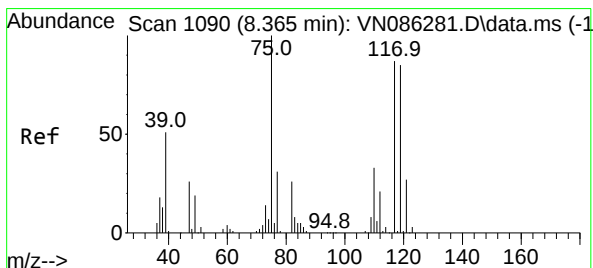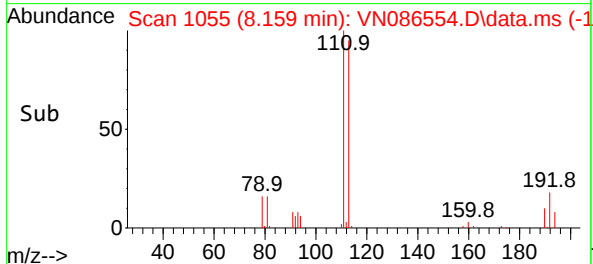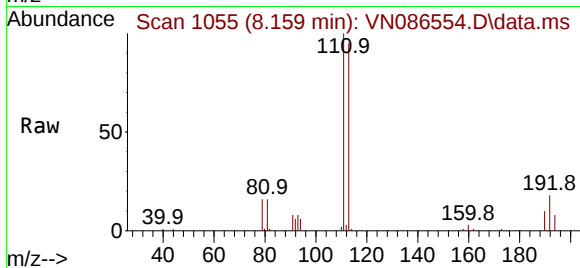

#36

1,1-Dichloropropene

Concen: 4.679 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.141 min

Lab File: VN086554.D

Acq: 09 May 2025 11:34




Tgt Ion: 75 Resp: 13217


Ion Ratio Lower Upper

75 100

110 8.8 16.8 50.4#


77 0.0 24.9 37.3#

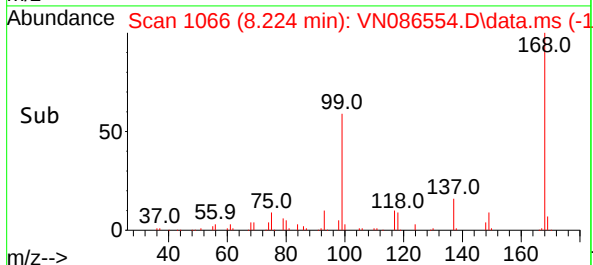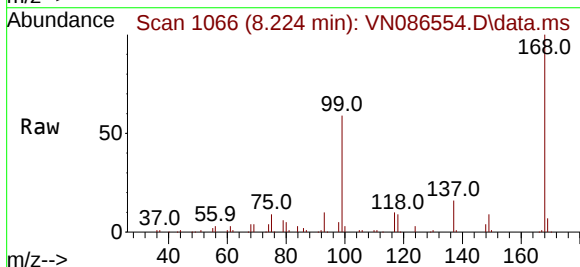



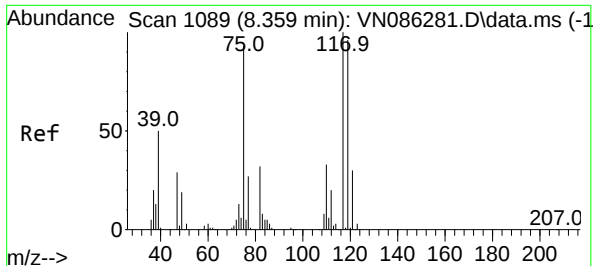


#38
Carbon Tetrachloride
Concen: 6.014 ug/l
RT: 8.224 min Scan# 1106
Delta R.T. -0.135 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01



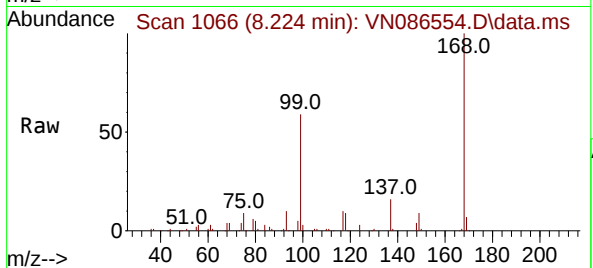



Tgt Ion:117 Resp: 16180
Ion Ratio Lower Upper
117 100
119 4.0 76.8 115.2#
121 0.0 23.8 35.8#

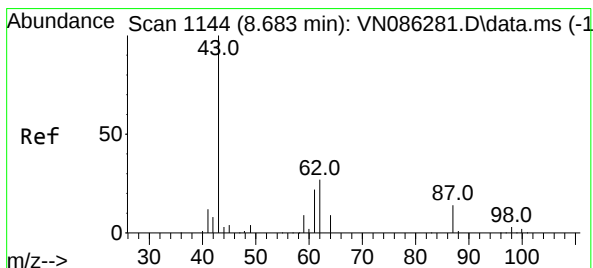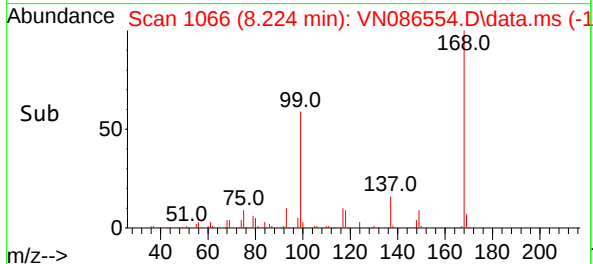

#43
Isopropyl Acetate
Concen: Below Cal
RT: 8.671 min Scan# 1142
Delta R.T. -0.012 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion: 43 Resp: 2914
Ion Ratio Lower Upper
43 100
61 0.0 20.5 30.7#
87 0.0 10.5 15.7#


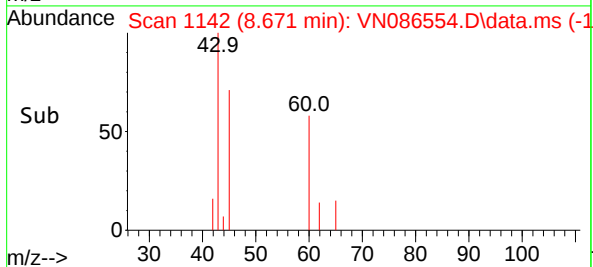

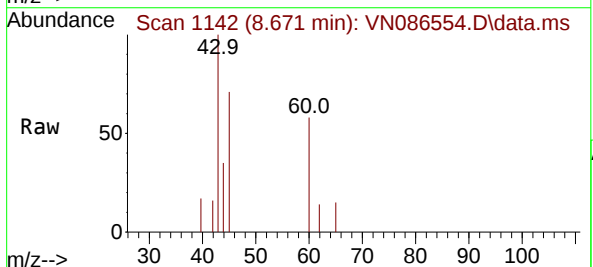




#50
Toluene-d8
Concen: 50.589 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34




Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01


Tgt Ion: 98 Resp: 382413
Ion Ratio Lower Upper
98 100
100 65.6 52.5 78.7



#51
4-Methyl-2-Pentanone
Concen: 0.225 ug/l
RT: 10.441 min Scan# 1443
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion: 43 Resp: 686
Ion Ratio Lower Upper
43 100
58 0.0 32.2 48.4#




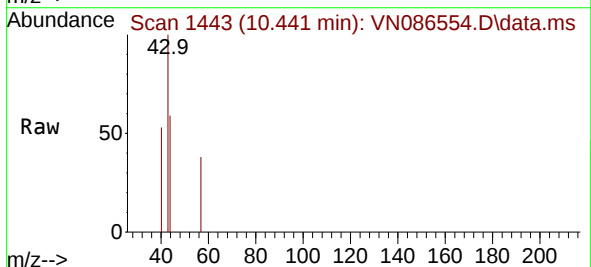


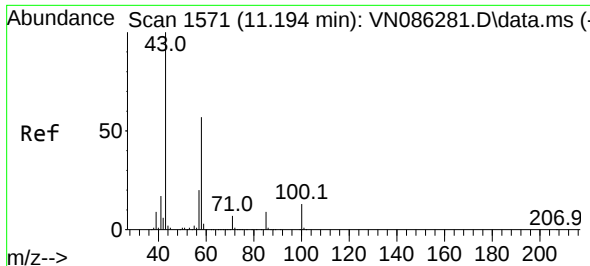

#59
2-Hexanone
Concen: 0.599 ug/l
RT: 11.200 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34




Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01


Tgt Ion: 43 Resp: 1354
Ion Ratio Lower Upper
43 100
58 33.4 28.3 85.0

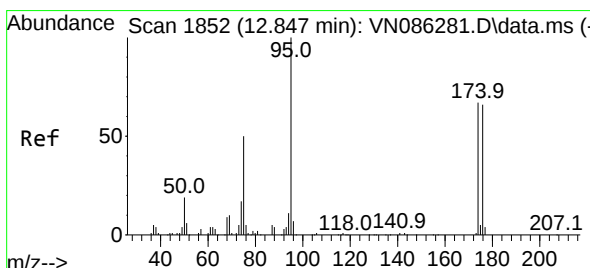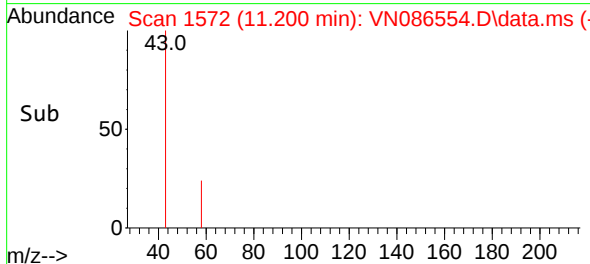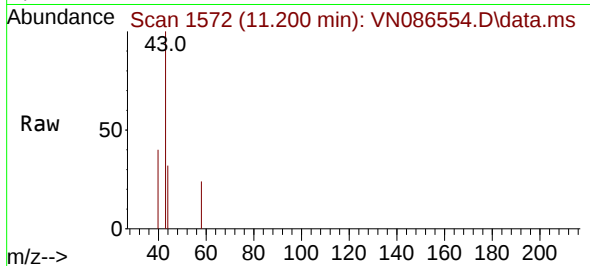

#62
4-Bromofluorobenzene
Concen: 48.469 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion: 95 Resp: 133637
Ion Ratio Lower Upper
95 100
174 73.6 0.0 133.4
176 70.7 0.0 129.2


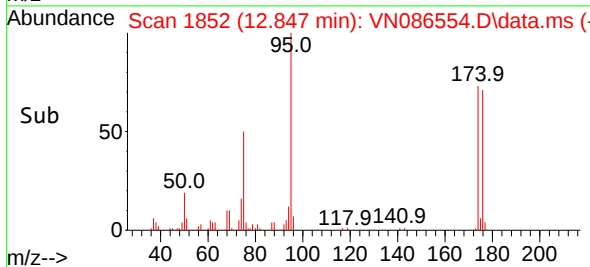

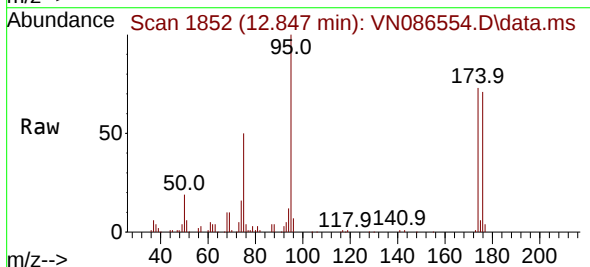




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34




Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01


Tgt Ion:117 Resp: 283891
Ion Ratio Lower Upper
117 100
82 52.8 44.7 67.1
119 32.0 26.4 39.6

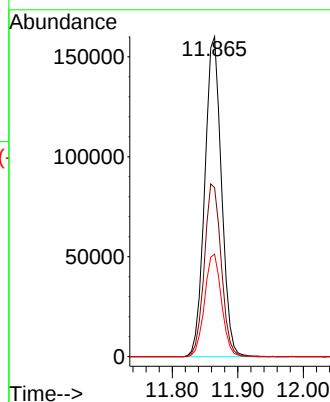

#71
Bromoform
Concen: 0.350 ug/l
RT: 12.841 min Scan# 1851
Delta R.T. 0.265 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion:173 Resp: 550
Ion Ratio Lower Upper
173 100
175 1110.7 24.6 73.6#
254 0.0 0.0 0.0

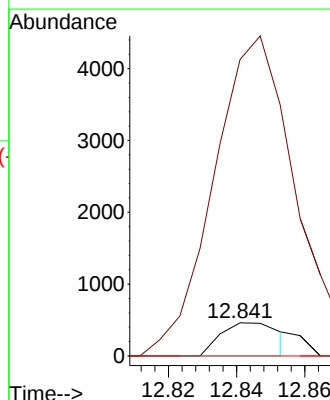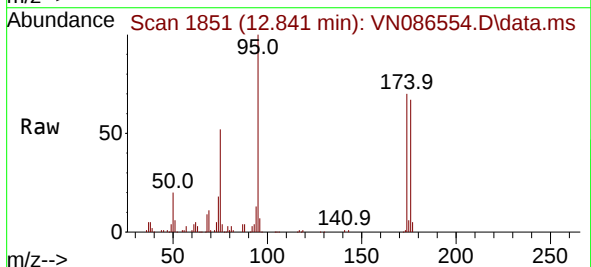

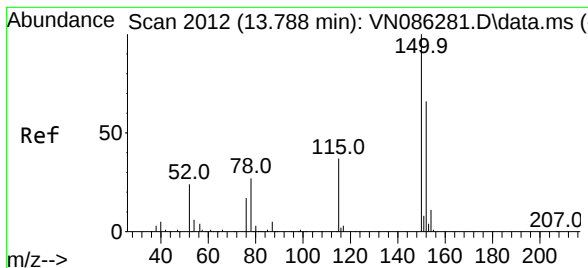

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.788 min Scan# 2012

Delta R.T. -0.000 min

Lab File: VN086554.D

Acq: 09 May 2025 11:34

Instrument :

MSVOA_N

ClientSampleId :

VN0509MBL01





Tgt Ion:152 Resp: 123333

Ion Ratio Lower Upper

152 100

115 61.4 31.9 95.9

150 156.6 0.0 352.0

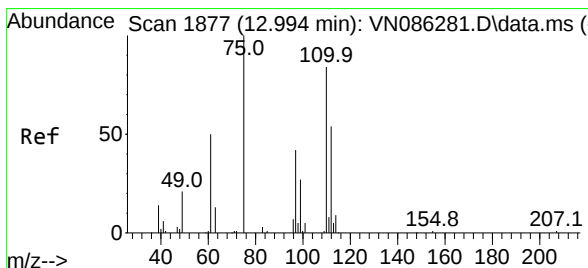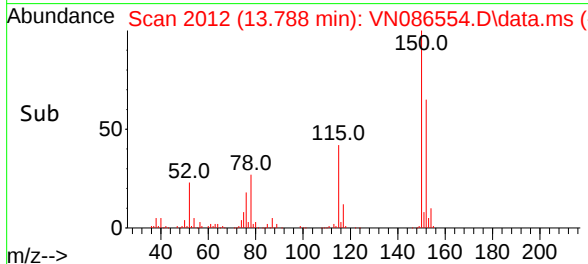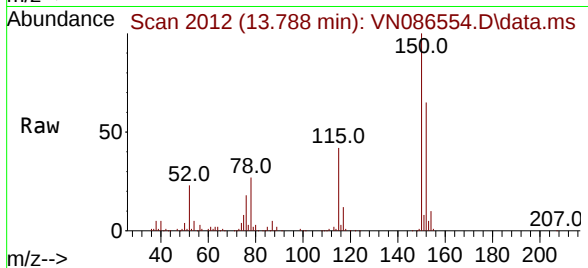

#76

1,2,3-Trichloropropane

Concen: 23.468 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.147 min

Lab File: VN086554.D




Acq: 09 May 2025 11:34


Tgt Ion: 75 Resp: 68304

Ion Ratio Lower Upper

75 100

77 1.2 98.8 296.4#


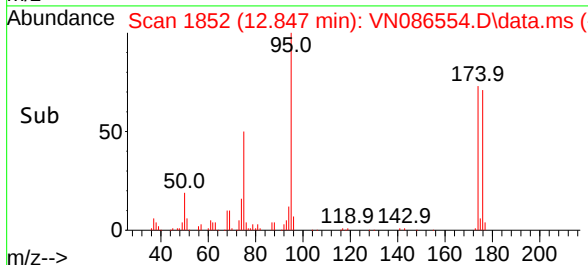

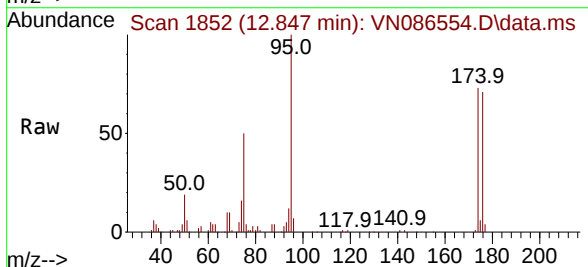




#81
trans-1,4-Dichloro-2-butene
Concen: 56.362 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.112 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34




Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01


Tgt Ion: 75 Resp: 68304
Ion Ratio Lower Upper
75 100
53 0.0 79.2 118.8#
89 0.0 35.7 53.5#



#85
sec-Butylbenzene
Concen: 0.256 ug/l
RT: 13.612 min Scan# 1982
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion: 105 Resp: 2536
Ion Ratio Lower Upper
105 100
134 21.1 9.7 29.1

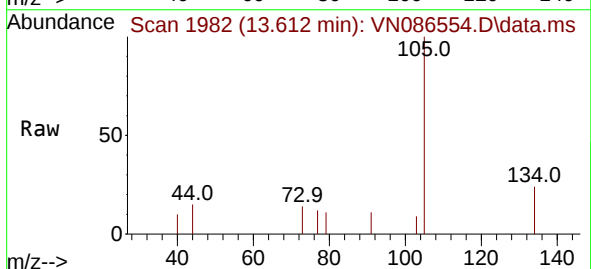



#86

p-Isopropyltoluene

Concen: 0.244 ug/l

RT: 13.729 min Scan# 2000

Delta R.T. 0.006 min

Lab File: VN086554.D

Acq: 09 May 2025 11:34

Instrument :

MSVOA_N

ClientSampleId :

VN0509MBL01





Tgt Ion:119 Resp: 1993

Ion Ratio Lower Upper

119 100

134 22.0 13.1 39.1

91 19.9 11.9 35.9



#87

1,3-Dichlorobenzene

Concen: 0.291 ug/l

RT: 13.735 min Scan# 2003

Delta R.T. 0.006 min

Lab File: VN086554.D

Acq: 09 May 2025 11:34




Tgt Ion:146 Resp: 1223


Ion Ratio Lower Upper

146 100

111 39.2 21.9 65.7


148 67.3 31.9 95.5

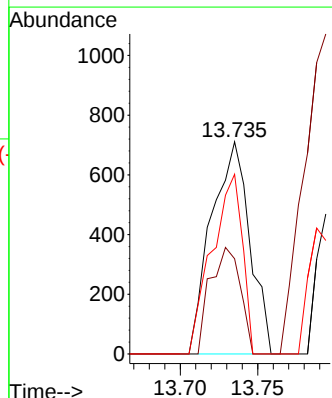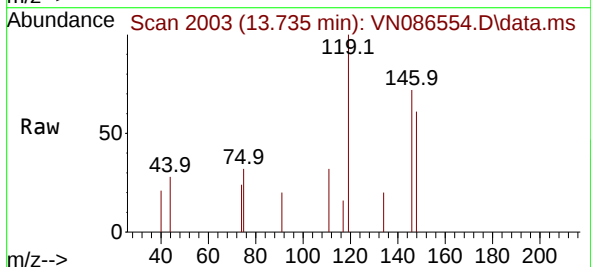






#88
1,4-Dichlorobenzene
Concen: 0.289 ug/l
RT: 13.735 min Scan# 2016
Delta R.T. -0.077 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01







Tgt Ion:146 Resp: 1223
Ion Ratio Lower Upper
146 100
111 39.2 21.3 63.9
148 67.3 31.9 95.9



#89
n-Butylbenzene
Concen: 0.466 ug/l
RT: 14.053 min Scan# 2057
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Tgt Ion: 91 Resp: 3378
Ion Ratio Lower Upper
91 100
92 57.1 26.8 80.4
134 24.5 12.2 36.6


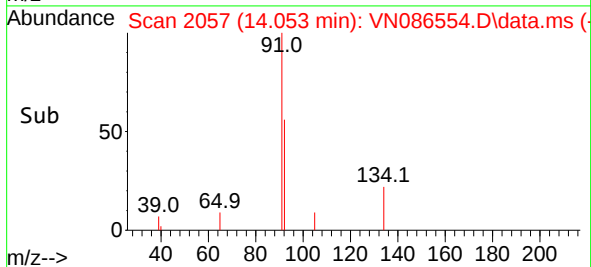

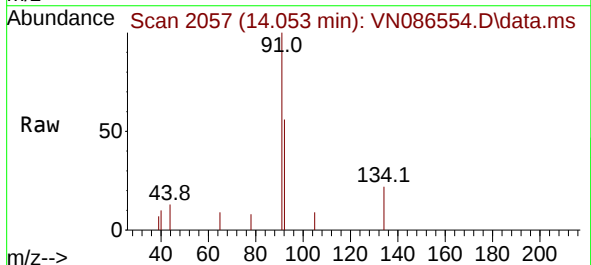




#91
1,2-Dichlorobenzene
Concen: 0.322 ug/l
RT: 14.106 min Scan# 2066
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34




Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01


Tgt Ion:146	Resp:	1313
Ion	Ratio	Lower Upper
146	100	
111	32.7	22.4 67.0
148	56.3	31.8 95.4

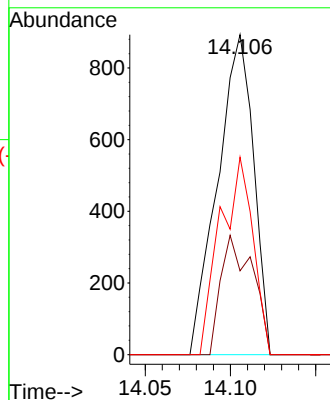

#93
1,2,4-Trichlorobenzene
Concen: 1.014 ug/l
RT: 15.388 min Scan# 2284
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34


Tgt Ion:180	Resp:	1979
Ion	Ratio	Lower Upper
180	100	
182	81.9	47.0 141.0
145	21.0	16.4 49.1

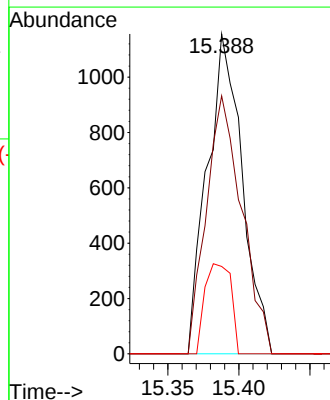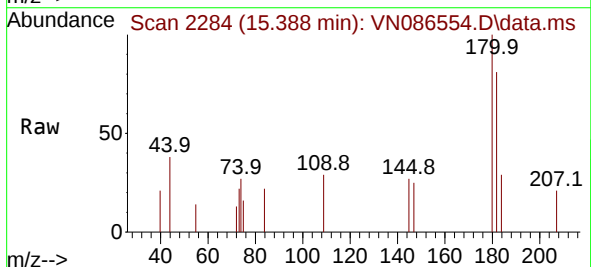






#94
Hexachlorobutadiene
Concen: 1.471 ug/l
RT: 15.500 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34

Instrument :
MSVOA_N
ClientSampleId :
VN0509MBL01



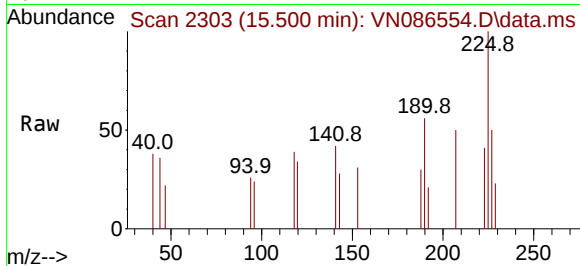



Tgt Ion	225	Resp:	1083
Ion Ratio	100	Lower	Upper
225	100		
223	62.6	32.8	98.3
227	56.8	31.4	94.0

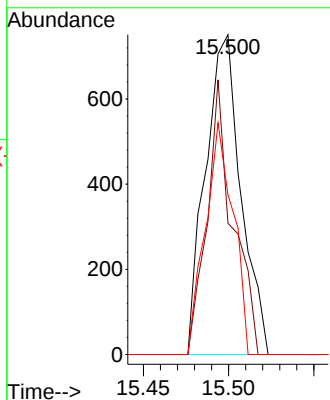

#95
Naphthalene
Concen: 1.324 ug/l
RT: 15.635 min Scan# 2326
Delta R.T. -0.000 min
Lab File: VN086554.D
Acq: 09 May 2025 11:34


Tgt Ion	128	Resp:	9157
Ion Ratio	100	Lower	Upper
128	100		
127	10.7	10.2	15.4
129	11.3	8.6	13.0

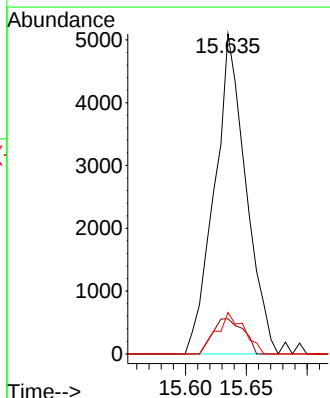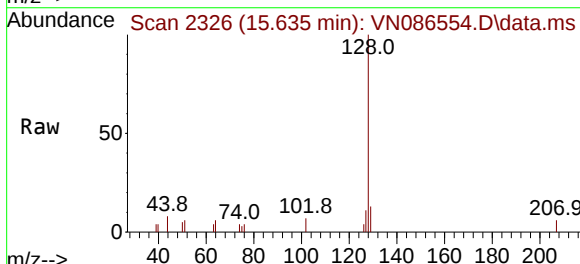



#96
 1,2,3-Trichlorobenzene
 Concen: 1.194 ug/l
 RT: 15.835 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN086554.D
 Acq: 09 May 2025 11:34

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0509MBL01



Tgt Ion:	180	Resp:	2206
Ion	Ratio	Lower	Upper
180	100		
182	93.3	47.3	142.0
145	25.7	17.2	51.5

