
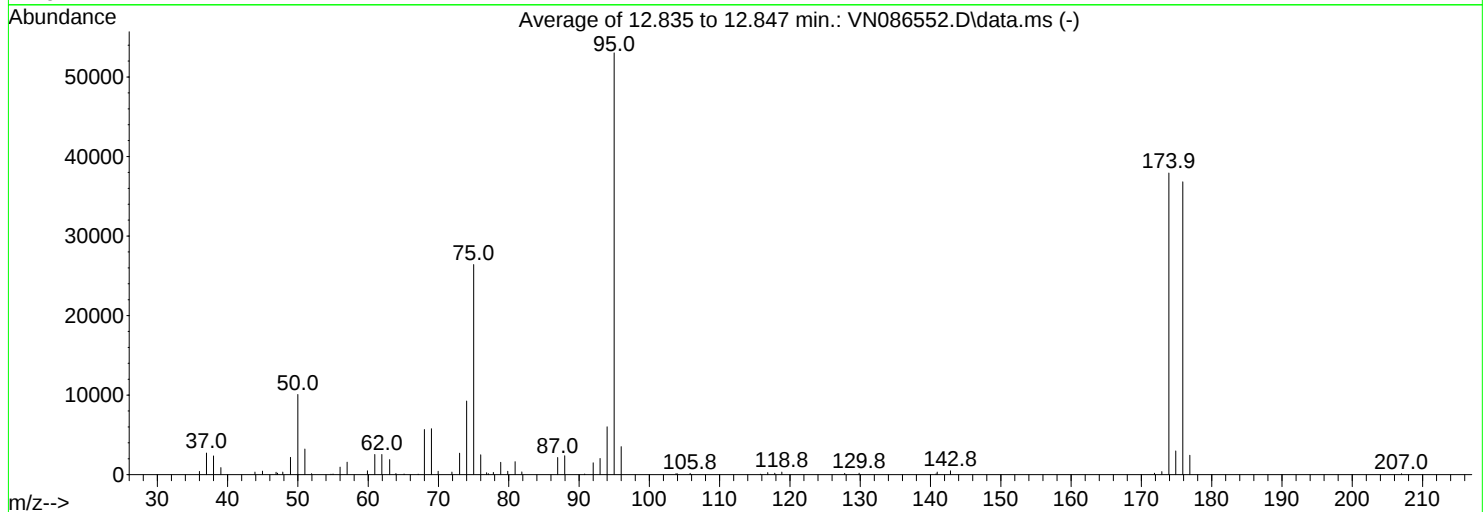


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN050925\
Data File : VN086552.D
Acq On : 09 May 2025 09:49
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041525W.M
Title : SW846 8260
Last Update : Wed Apr 16 04:19:23 2025

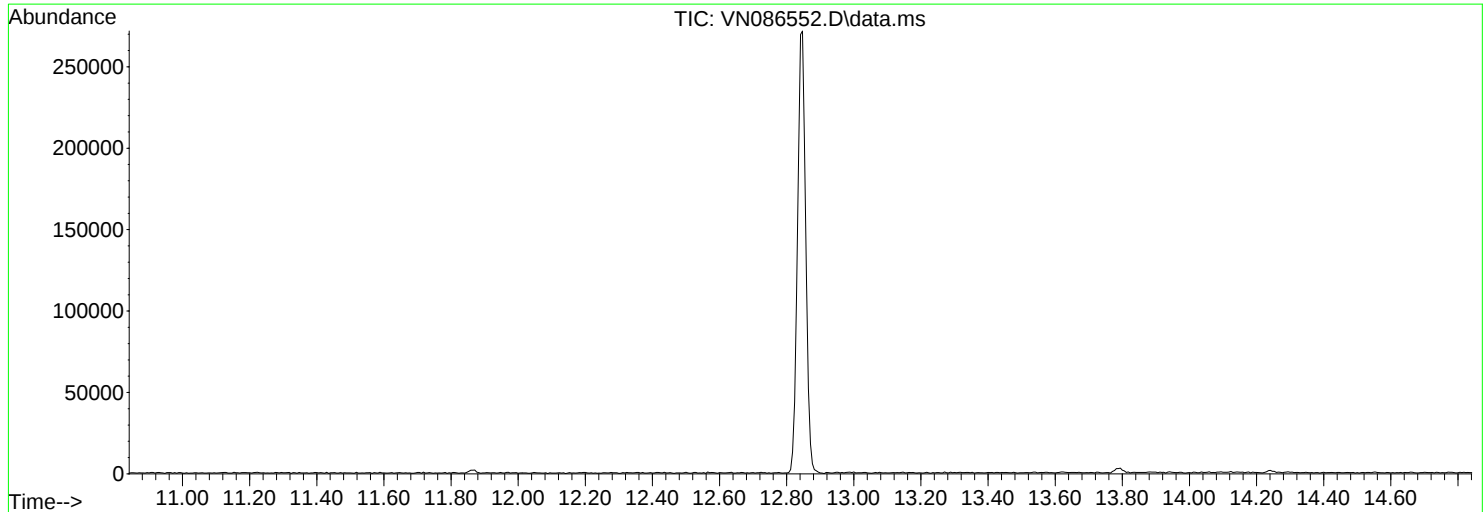

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	10073	PASS
75	95	30	60	49.8	26408	PASS
95	95	100	100	100.0	53037	PASS
96	95	5	9	6.7	3528	PASS
173	174	0.00	2	1.0	383	PASS
174	95	50	100	71.5	37923	PASS
175	174	5	9	7.9	2983	PASS
176	174	95	101	97.1	36827	PASS
177	176	5	9	6.6	2445	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	410	51.00	3219	65.10	77	77.10	111
37.00	2720	51.95	115	67.10	61	77.80	28
38.00	2349	54.70	55	68.00	5679	78.85	155
39.05	892	55.00	74	69.00	5774	79.85	43
43.90	314	56.00	946	69.95	426	80.90	1628
44.95	447	57.00	1564	71.90	324	81.85	334
46.90	309	59.90	484	73.00	2706	86.95	2157
47.10	191	60.95	2528	74.00	9264	87.95	2368
47.85	328	61.95	2542	75.00	26408	90.80	76
48.95	2181	63.05	1894	76.00	2488	92.00	1480
50.00	10073	63.95	148	76.85	239	93.00	2027

Average of 12.835 to 12.847 min.: VN086552.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.00	6027	129.85	180				
95.00	53037	140.80	92				
96.00	3528	140.95	332				
103.80	145	142.85	474				
104.00	98	171.85	175				
105.80	161	172.90	383				
115.80	58	173.90	37923				
116.85	261	174.90	2983				
117.85	186	175.90	36827				
118.85	315	176.90	2445				
127.80	159	207.00	120				

Instrument :

MSVOA_N

ClientSampleId :

BFB