


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051021\
 Data File : VN067065.D
 Acq On : 10 May 2021 12:02
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N050421W.M
 Title : SW846 8260
 Last Update : Wed May 05 07:24:52 2021

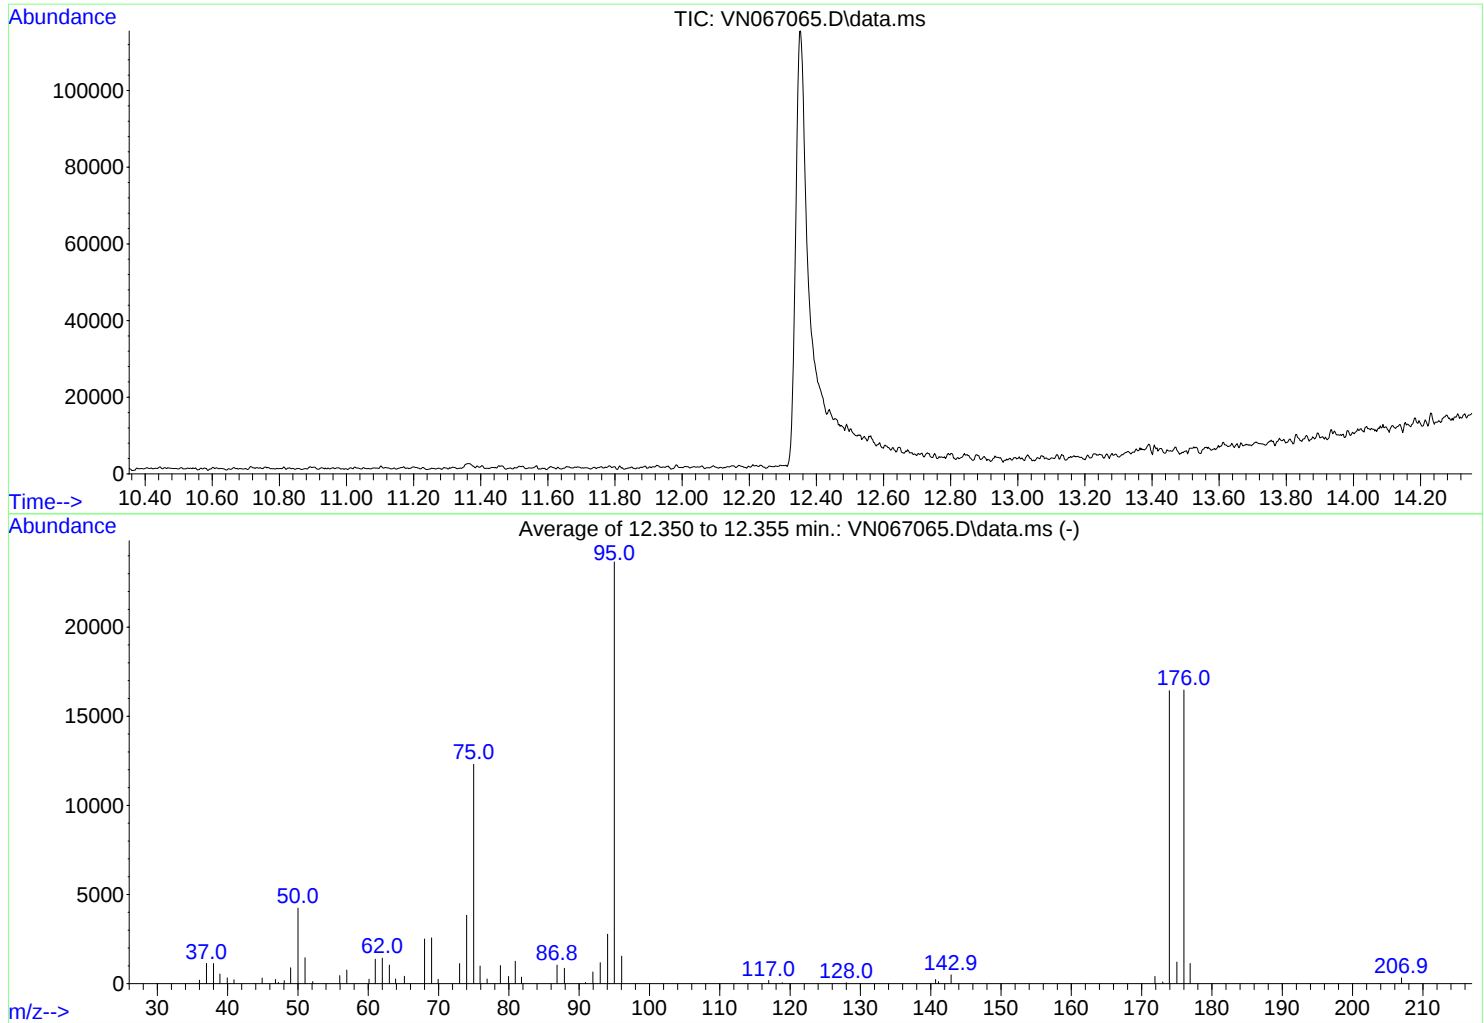

AutoFind: Scans 3950, 3951, 3952; Background Corrected with Scan 3934

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	4234	PASS
75	95	30	60	52.0	12305	PASS
95	95	100	100	100.0	23664	PASS
96	95	5	9	6.5	1543	PASS
173	174	0.00	2	0.6	100	PASS
174	95	50	100	69.5	16439	PASS
175	174	5	9	7.4	1216	PASS
176	174	95	101	100.2	16476	PASS
177	176	5	9	6.9	1135	PASS