

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051024\
 Data File : VN082068.D
 Acq On : 10 May 2024 14:34
 Operator : JC\MD
 Sample : PB160834TB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: May 10 23:22:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 26 05:26:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	119929	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	265271	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	239263	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	84752	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	106178	52.457	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 104.920%	
35) Dibromofluoromethane	8.171	113	78052	48.869	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 97.740%	
50) Toluene-d8	10.571	98	335961	53.559	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 107.120%	
62) 4-Bromofluorobenzene	12.847	95	107570	43.381	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	= 86.760%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.371	50	750	0.427	ug/l #	43
5) Bromomethane	2.966	94	405	Below Cal		97
10) Methyl Iodide	4.589	142	363	0.290	ug/l #	40
11) Tert butyl alcohol	5.507	59	4686	12.735	ug/l #	89
13) Acrolein	4.189	56	440	Below Cal	#	70
16) Acetone	4.424	43	22799	33.353	ug/l	89
17) Carbon Disulfide	4.707	76	1575	0.361	ug/l #	74
18) Methyl Acetate	5.024	43	1475	0.719	ug/l #	61
20) Methylene Chloride	5.283	84	8575	4.943	ug/l #	85
25) 2-Butanone	7.477	43	23938	20.837	ug/l #	66
29) Tetrahydrofuran	7.836	42	606	0.736	ug/l #	29
31) Cyclohexane	8.230	56	3974	1.303	ug/l #	46
37) Ethyl Acetate	7.553	43	4605	1.639	ug/l #	69
38) Carbon Tetrachloride	8.224	117	13959	5.497	ug/l #	18
43) Isopropyl Acetate	8.689	43	194853	36.887	ug/l #	80
45) 1,2-Dichloropropane	9.747	63	2214	1.085	ug/l #	45
48) Methyl methacrylate	9.659	41	6995	2.774	ug/l #	38
49) 1,4-Dioxane	9.677	88	185	4.827	ug/l #	1
51) 4-Methyl-2-Pentanone	10.442	43	6874	2.312	ug/l	90
52) Toluene	10.630	92	2490	0.533	ug/l	80
54) cis-1,3-Dichloropropene	10.359	75	50352	15.089	ug/l #	76
57) 1,3-Dichloropropane	11.206	76	6116	1.873	ug/l #	42
59) 2-Hexanone	11.171	43	130343	58.897	ug/l #	23
74) N-amyl acetate	12.465	43	6785	1.617	ug/l #	42
75) 1,1,2,2-Tetrachloroethane	12.965	83	533	0.236	ug/l #	37
76) 1,2,3-Trichloropropane	12.847	75	62335	28.367	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	62335	58.128	ug/l #	12
94) Hexachlorobutadiene	15.512	225	174	0.299	ug/l #	20
95) Naphthalene	15.641	128	2482	0.416	ug/l #	82
96) 1,2,3-Trichlorobenzene	15.841	180	623	0.411	ug/l	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051024\
Data File : VN082068.D
Acq On : 10 May 2024 14:34
Operator : JC\MD
Sample : PB160834TB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: May 10 23:22:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 26 05:26:49 2024
Response via : Initial Calibration

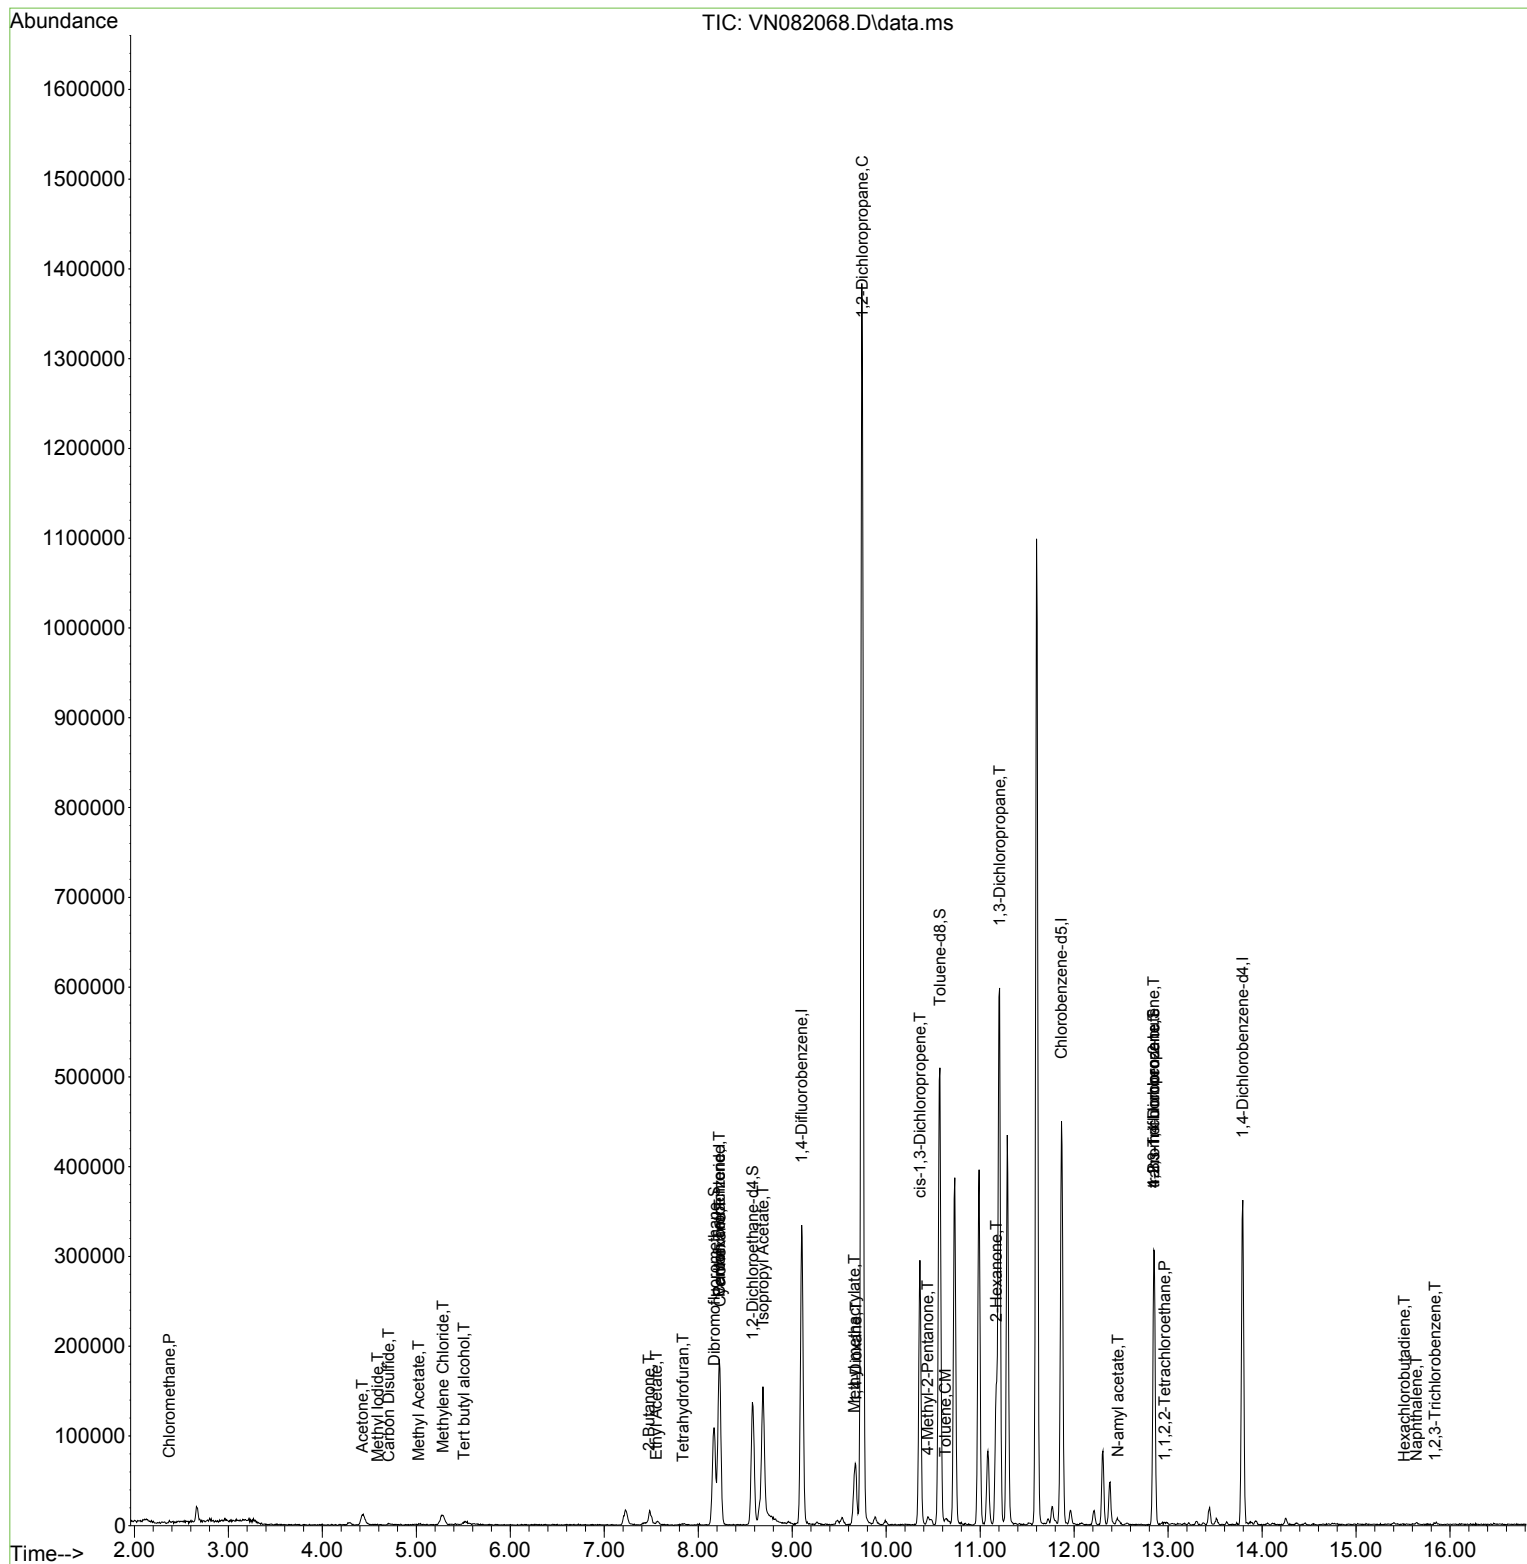



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.224 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN082068.D

Acq: 10 May 2024 14:34

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:168 Resp: 119929

Ion Ratio Lower Upper

168 100

99 63.4 48.2 72.4

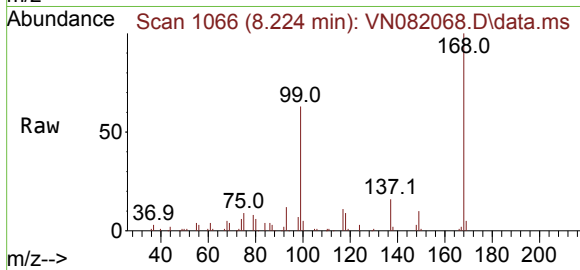

#3

Chloromethane

Concen: 0.427 ug/l

RT: 2.371 min Scan# 71

Delta R.T. 0.012 min

Lab File: VN082068.D




Acq: 10 May 2024 14:34


Tgt Ion: 50 Resp: 750

Ion Ratio Lower Upper

50 100

52 0.0 25.5 38.3#




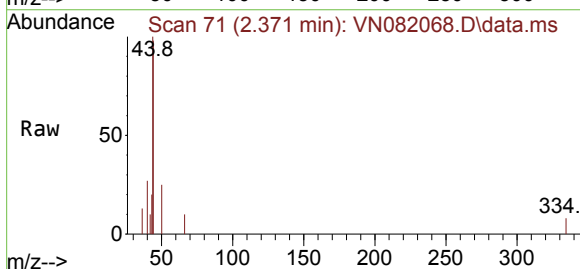




#5
Bromomethane
Concen: Below Cal
RT: 2.966 min Scan# 1
Delta R.T. 0.018 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 94 Resp: 405
Ion Ratio Lower Upper
94 100
96 96.2 74.8 112.2

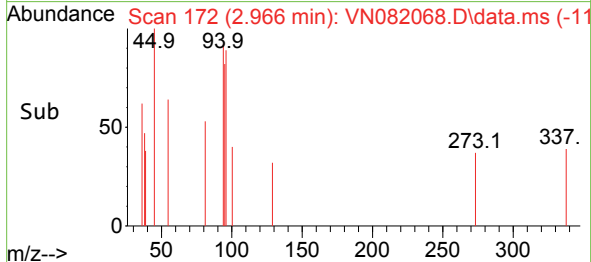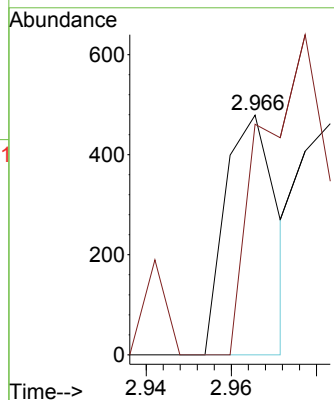

#10
Methyl Iodide
Concen: 0.290 ug/l
RT: 4.589 min Scan# 448
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34


Tgt Ion:142 Resp: 363
Ion Ratio Lower Upper
142 100
127 0.0 35.8 53.6#
141 0.0 11.4 17.2#

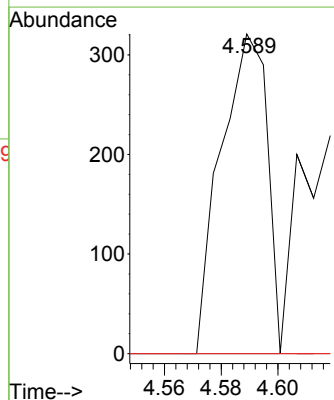






#11
Tert butyl alcohol
Concen: 12.735 ug/l
RT: 5.507 min Scan# 606
Delta R.T. -0.011 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 59 Resp: 4686
Ion Ratio Lower Upper
59 100
57 6.9 8.9 13.3#

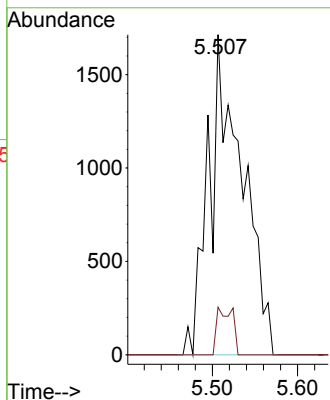

#13
Acrolein
Concen: Below Cal
RT: 4.189 min Scan# 380
Delta R.T. 0.012 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Tgt Ion: 56 Resp: 440
Ion Ratio Lower Upper
56 100
55 45.5 55.8 83.8#



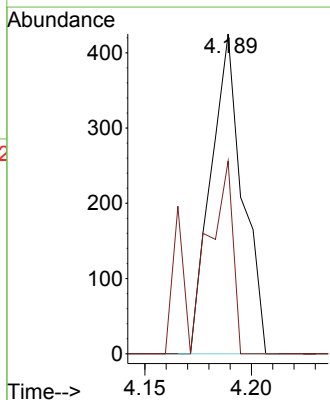





#16
Acetone
Concen: 33.353 ug/l
RT: 4.424 min Scan# 41
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 22799
Ion Ratio Lower Upper
43 100
58 25.7 25.2 37.8

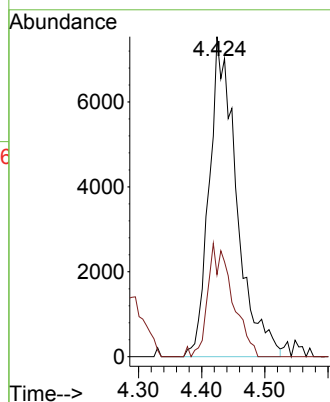

#17
Carbon Disulfide
Concen: 0.361 ug/l
RT: 4.707 min Scan# 468
Delta R.T. -0.006 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34


Tgt Ion: 76 Resp: 1575
Ion Ratio Lower Upper
76 100
78 0.0 7.5 11.3#

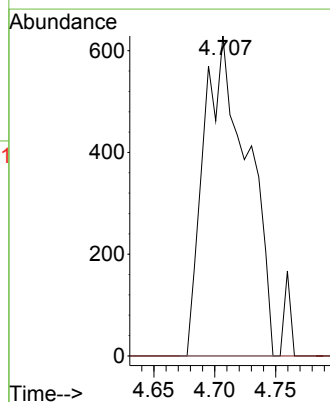






#18
Methyl Acetate
Concen: 0.719 ug/l
RT: 5.024 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 1475
Ion Ratio Lower Upper
43 100
74 7.5 22.2 33.2#



#20
Methylene Chloride
Concen: 4.943 ug/l
RT: 5.283 min Scan# 566
Delta R.T. 0.006 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34


Tgt Ion: 84 Resp: 8575
Ion Ratio Lower Upper
84 100
49 121.2 84.9 127.3
51 21.3 27.0 40.6#
86 55.0 52.3 78.5








#25
2-Butanone
Concen: 20.837 ug/l
RT: 7.477 min Scan# 91
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 43 Resp: 23938
Ion Ratio Lower Upper
43 100
72 12.8 25.3 37.9#




#29
Tetrahydrofuran
Concen: 0.736 ug/l
RT: 7.836 min Scan# 1000
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34




Tgt Ion: 42 Resp: 606
Ion Ratio Lower Upper
42 100
72 0.0 39.3 58.9#
71 0.0 37.4 56.0#








#31
Cyclohexane
Concen: 1.303 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.029 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 3974
Ion Ratio Lower Upper
56 100
69 137.7 24.4 36.6#
84 104.6 77.0 115.4



#33
1,2-Dichloroethane-d4
Concen: 52.457 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Tgt Ion: 65 Resp: 106178
Ion Ratio Lower Upper
65 100
67 54.1 0.0 103.0





#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. 0.000 min

Lab File: VN082068.D

Acq: 10 May 2024 14:34

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion:114 Resp: 265271

Ion Ratio Lower Upper

114 100

63 23.4 0.0 41.0

88 15.5 0.0 31.4



#35

Dibromofluoromethane

Concen: 48.869 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN082068.D

Acq: 10 May 2024 14:34




Tgt Ion:113 Resp: 78052


Ion Ratio Lower Upper

113 100

111 106.0 83.4 125.2


192 15.1 14.0 21.0








#37
Ethyl Acetate
Concen: 1.639 ug/l
RT: 7.553 min Scan# 91
Delta R.T. -0.005 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 43 Resp: 4605
Ion Ratio Lower Upper
43 100
61 0.0 11.3 16.9#
70 1.3 8.7 13.1#

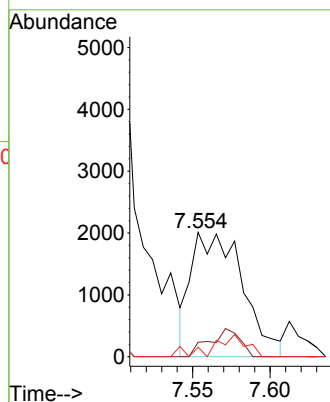


#38
Carbon Tetrachloride
Concen: 5.497 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.135 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34




Tgt Ion: 117 Resp: 13959
Ion Ratio Lower Upper
117 100
119 7.0 76.5 114.7#
121 0.0 23.9 35.9#

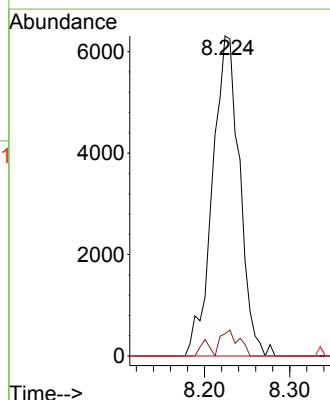






#43
Isopropyl Acetate
Concen: 36.887 ug/l
RT: 8.689 min Scan# 1145
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 194853
Ion Ratio Lower Upper
43 100
61 16.0 22.8 34.2#
87 9.5 12.0 18.0#



#45
1,2-Dichloropropane
Concen: 1.085 ug/l
RT: 9.747 min Scan# 1325
Delta R.T. 0.124 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34


Tgt Ion: 63 Resp: 2214
Ion Ratio Lower Upper
63 100
65 0.0 24.1 36.1#

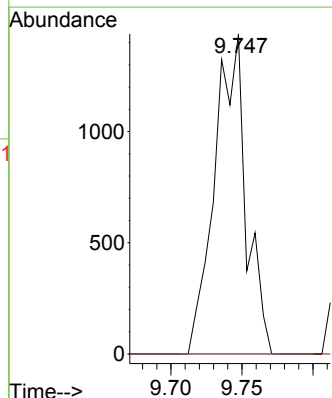






#48
Methyl methacrylate
Concen: 2.774 ug/l
RT: 9.659 min Scan# 11
Delta R.T. -0.023 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 41 Resp: 6995
Ion Ratio Lower Upper
41 100
69 0.0 77.9 116.9#
39 58.6 50.9 76.3



#49
1,4-Dioxane
Concen: 4.827 ug/l
RT: 9.677 min Scan# 1313
Delta R.T. -0.017 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Tgt Ion: 88 Resp: 185
Ion Ratio Lower Upper
88 100
43 0.0 19.0 28.6#
58 2771.4 50.6 76.0#









#50
Toluene-d8
Concen: 53.559 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.006 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 335961
Ion Ratio Lower Upper
98 100
100 66.3 51.8 77.6

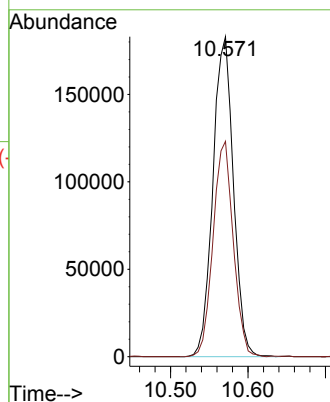

#51
4-Methyl-2-Pentanone
Concen: 2.312 ug/l
RT: 10.442 min Scan# 1443
Delta R.T. -0.005 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Tgt Ion: 43 Resp: 6874
Ion Ratio Lower Upper
43 100
58 34.9 33.2 49.8



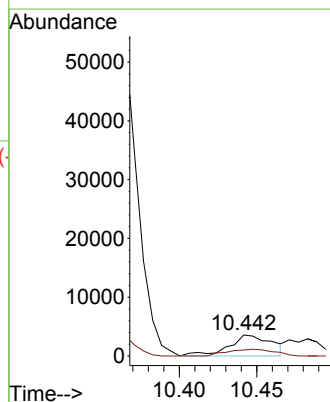



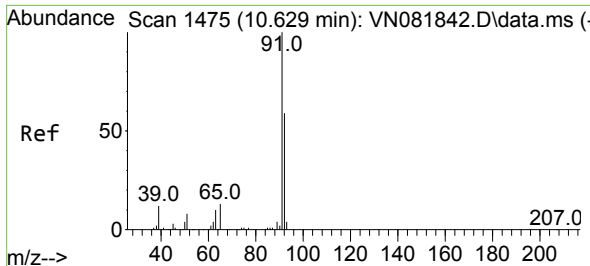

#52
Toluene
Concen: 0.533 ug/l
RT: 10.630 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 92 Resp: 2490
Ion Ratio Lower Upper
92 100
91 142.8 136.7 205.1

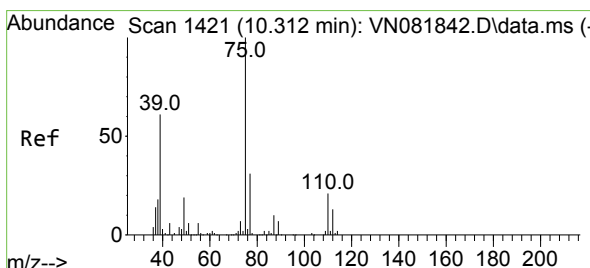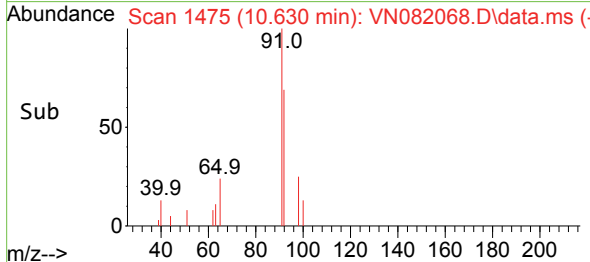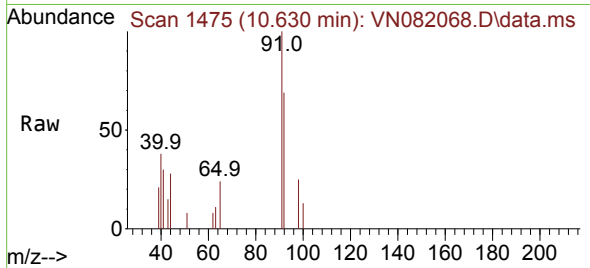

#54
cis-1,3-Dichloropropene
Concen: 15.089 ug/l
RT: 10.359 min Scan# 1429
Delta R.T. 0.047 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Tgt Ion: 75 Resp: 50352
Ion Ratio Lower Upper
75 100
77 0.9 25.0 37.4#
39 42.2 34.8 52.2

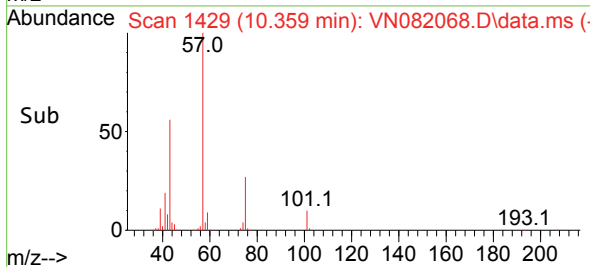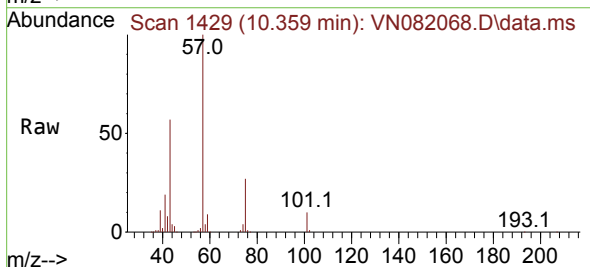

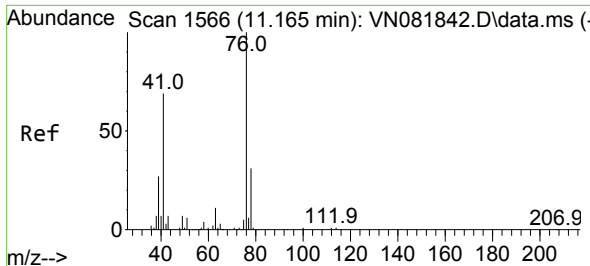

#57

1,3-Dichloropropane

Concen: 1.873 ug/l

RT: 11.206 min Scan# 11

Delta R.T. 0.042 min

Lab File: VN082068.D

Acq: 10 May 2024 14:34

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 76 Resp: 6116

Ion Ratio Lower Upper

76 100

78 0.0 25.8 38.6#

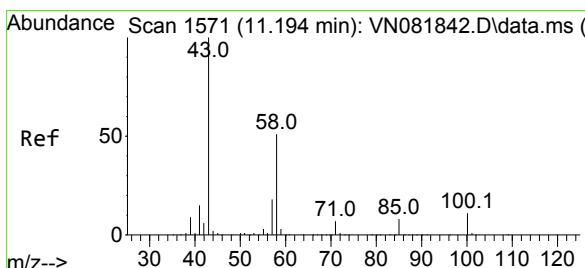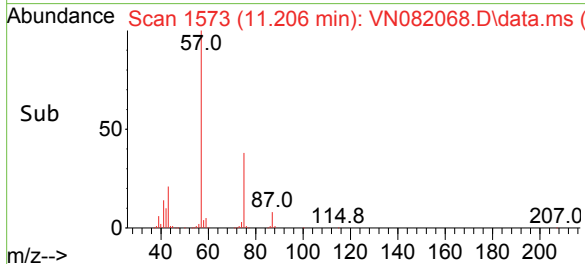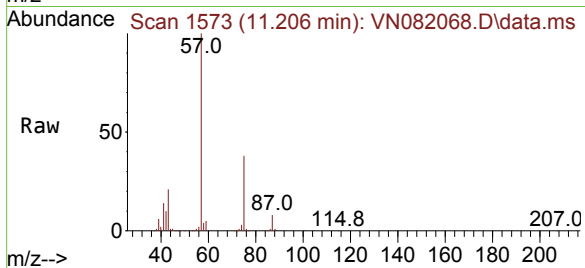

#59

2-Hexanone

Concen: 58.897 ug/l

RT: 11.171 min Scan# 1567

Delta R.T. -0.023 min

Lab File: VN082068.D




Acq: 10 May 2024 14:34


Tgt Ion: 43 Resp: 130343

Ion Ratio Lower Upper

43 100

58 0.0 28.3 84.9#


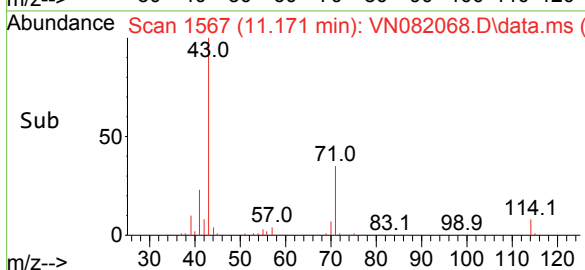

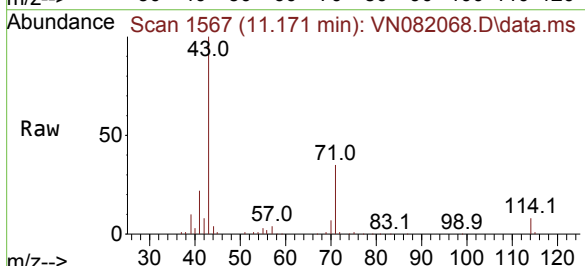




#62
4-Bromofluorobenzene
Concen: 43.381 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 107570
Ion Ratio Lower Upper
95 100
174 61.8 0.0 160.6
176 58.0 0.0 152.8



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Tgt Ion: 117 Resp: 239263
Ion Ratio Lower Upper
117 100
82 63.3 44.6 66.8
119 31.9 25.9 38.9

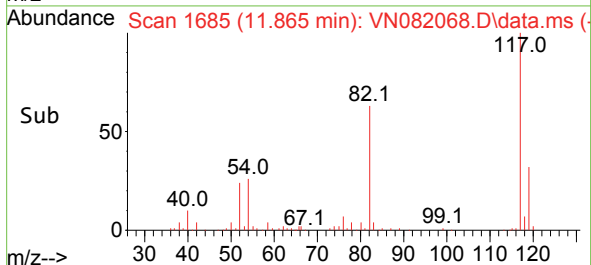

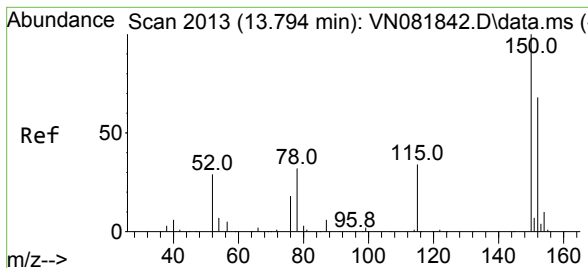

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. 0.000 min


Lab File: VN082068.D

Acq: 10 May 2024 14:34

Instrument :

MSVOA_N

ClientSampleId :

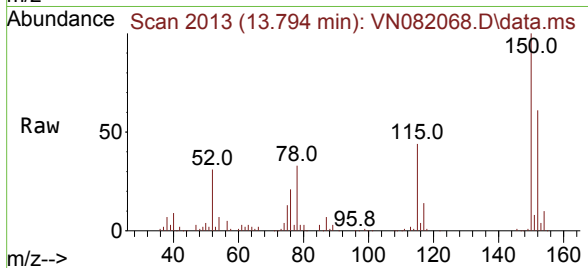




Tgt Ion:152 Resp: 84752

Ion Ratio Lower Upper

152 100

115 63.8 30.4 91.3

150 161.0 0.0 353.2

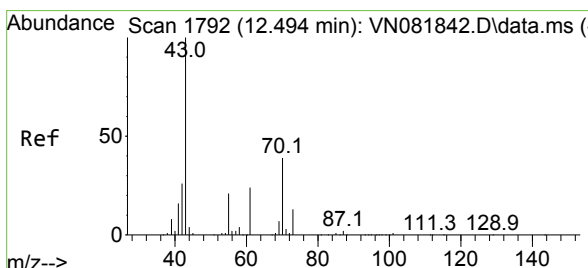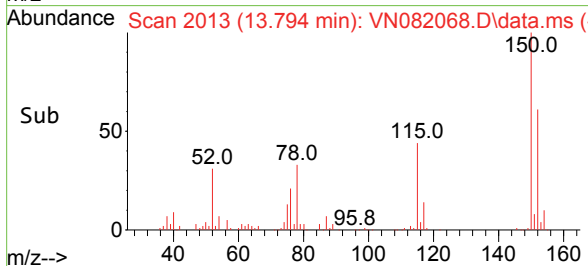

#74

N-ethyl acetate

Concen: 1.617 ug/l

RT: 12.465 min Scan# 1787

Delta R.T. -0.029 min

Lab File: VN082068.D

Acq: 10 May 2024 14:34

Tgt Ion: 43 Resp: 6785




Ion Ratio Lower Upper


43 100

70 1.0 39.0 58.4#

55 5.4 21.3 31.9#

61 0.0 20.5 30.7#

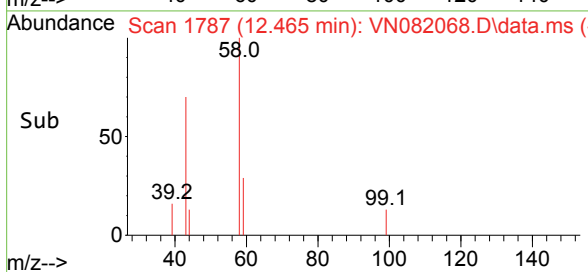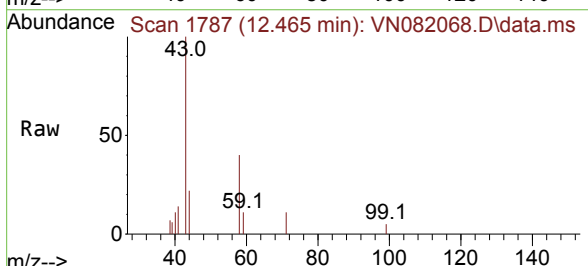

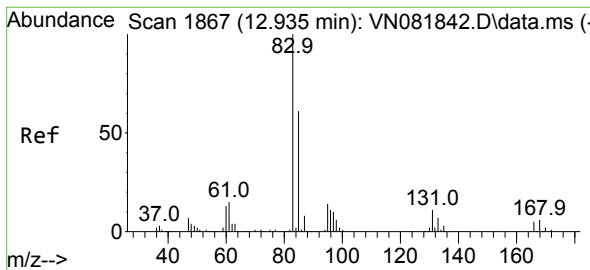

#75

1,1,2,2-Tetrachloroethane

Concen: 0.236 ug/l

RT: 12.965 min Scan# 1872

Delta R.T. 0.030 min

Lab File: VN082068.D

Acq: 10 May 2024 14:34

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 83 Resp: 533

Ion Ratio Lower Upper

83 100

131 0.0 5.5 16.4#

85 10.9 32.9 98.6#

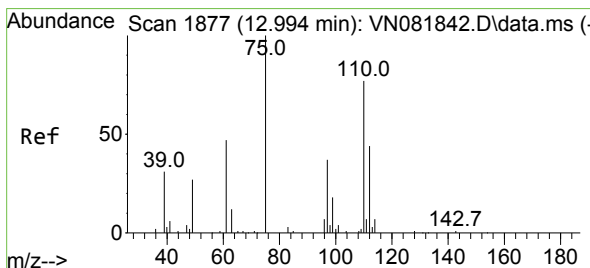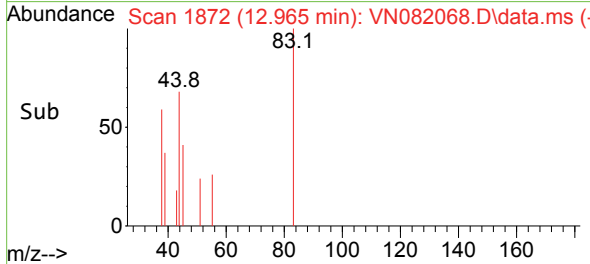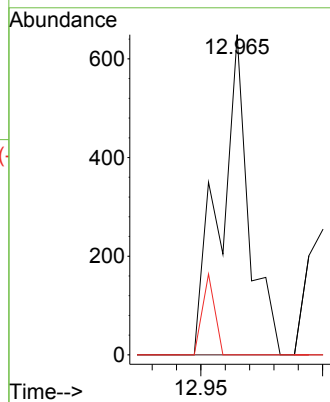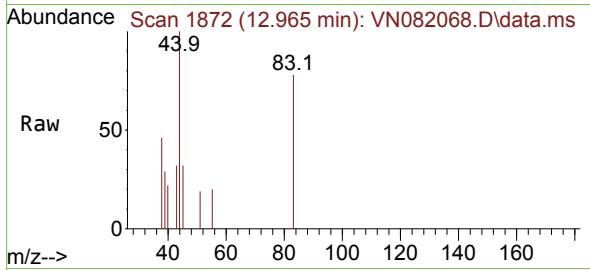

#76

1,2,3-Trichloropropane

Concen: 28.367 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.147 min

Lab File: VN082068.D




Acq: 10 May 2024 14:34


Tgt Ion: 75 Resp: 62335

Ion Ratio Lower Upper

75 100


77 1.6 90.5 271.3#

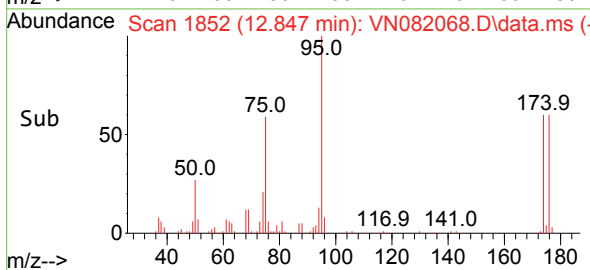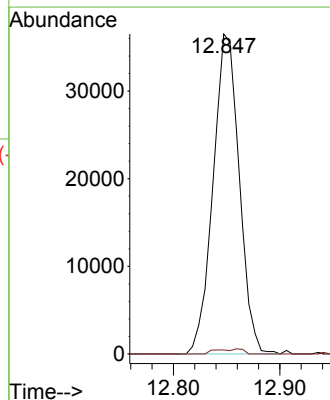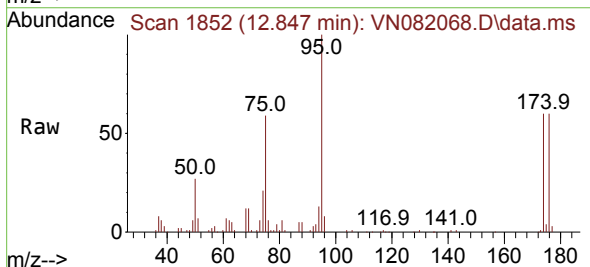






#81
trans-1,4-Dichloro-2-butene
Concen: 58.128 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.106 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 75 Resp: 62335
Ion Ratio Lower Upper
75 100
53 0.0 72.9 109.3#
89 0.0 39.1 58.7#




#94
Hexachlorobutadiene
Concen: 0.299 ug/l
RT: 15.512 min Scan# 2305
Delta R.T. 0.012 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34



Tgt Ion: 225 Resp: 174
Ion Ratio Lower Upper
225 100
223 0.0 31.1 93.2#
227 0.0 30.6 91.6#









#95
Naphthalene
Concen: 0.416 ug/l
RT: 15.641 min Scan# 2327
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion:128 Resp: 2482
Ion Ratio Lower Upper
128 100
127 2.3 10.1 15.1#
129 7.7 8.9 13.3#



#96
1,2,3-Trichlorobenzene
Concen: 0.411 ug/l
RT: 15.841 min Scan# 2361
Delta R.T. 0.000 min
Lab File: VN082068.D
Acq: 10 May 2024 14:34

Tgt Ion:180 Resp: 623
Ion Ratio Lower Upper
180 100
182 57.3 46.0 137.8
145 25.4 17.1 51.3

