
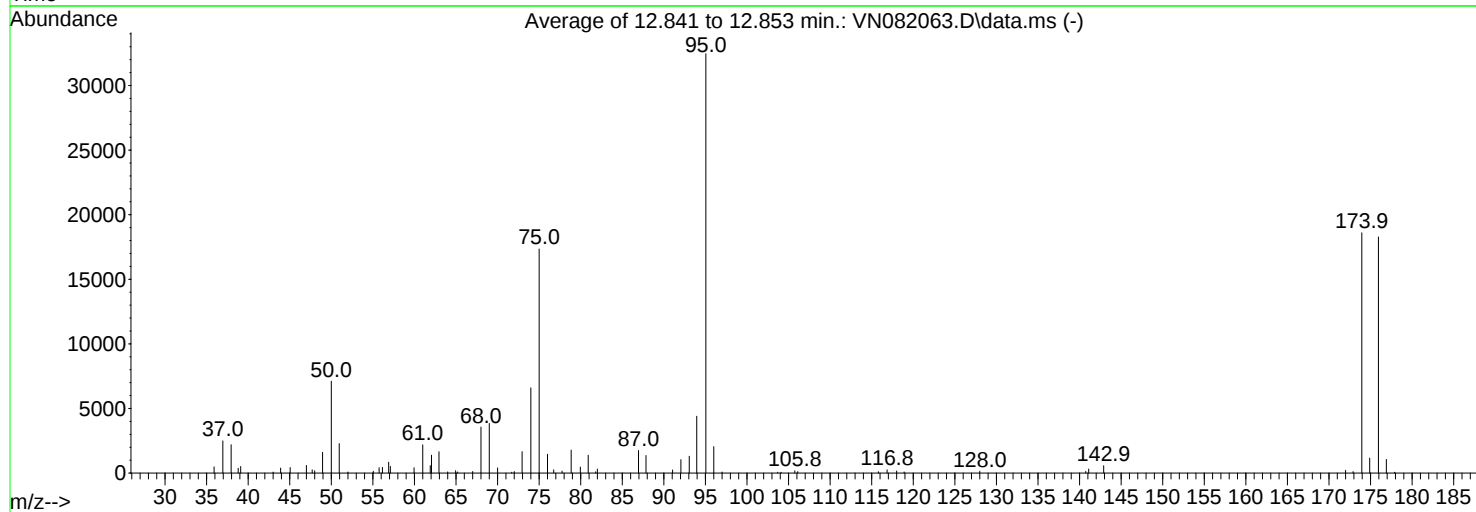


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051024\
Data File : VN082063.D
Acq On : 10 May 2024 09:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N042524W.M
Title : SW846 8260
Last Update : Fri Apr 26 05:26:49 2024

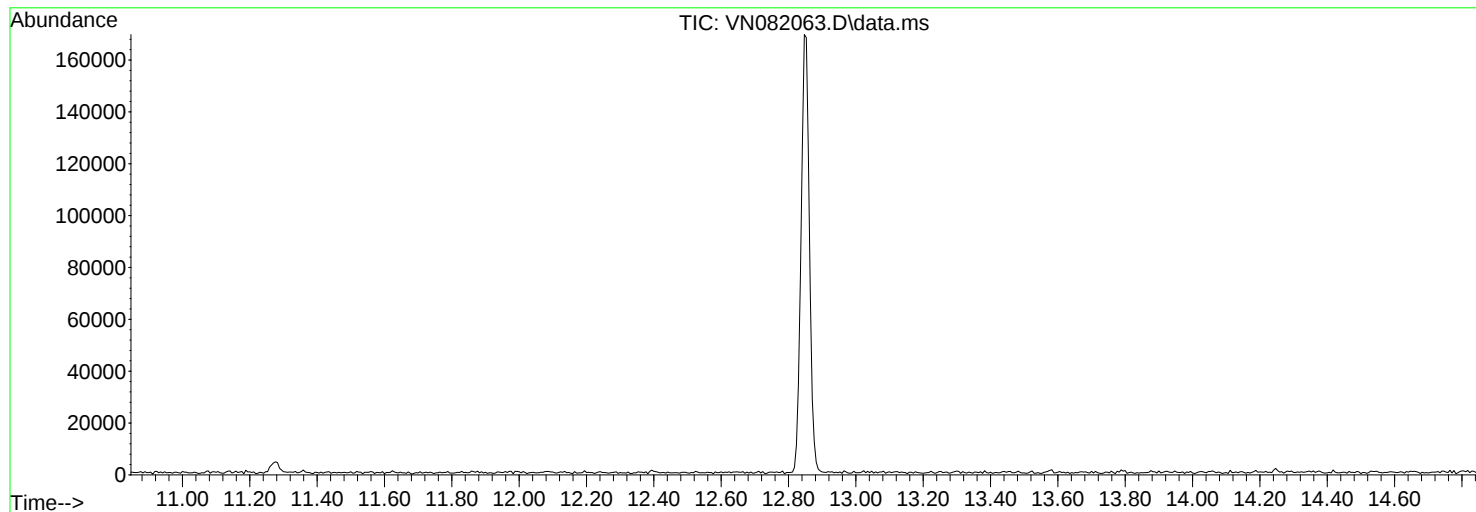

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	7117	PASS
75	95	30	60	53.4	17347	PASS
95	95	100	100	100.0	32461	PASS
96	95	5	9	6.3	2048	PASS
173	174	0.00	2	0.6	116	PASS
174	95	50	100	57.3	18603	PASS
175	174	5	9	6.3	1165	PASS
176	174	95	101	98.3	18281	PASS
177	176	5	9	5.8	1058	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	485	48.95	1612	61.90	577	72.00	120
36.95	2492	50.00	7117	62.05	1386	72.95	1658
37.95	2196	50.95	2285	62.95	1652	74.00	6598
38.80	376	52.00	85	64.00	93	75.00	17347
39.10	511	55.05	142	64.95	188	76.00	1456
43.00	78	55.75	421	65.20	88	76.75	250
43.90	388	56.15	443	67.00	125	77.75	158
45.05	433	56.90	845	68.00	3558	78.85	1781
47.00	593	57.10	519	69.00	3842	79.95	466
47.70	253	59.95	415	70.00	400	80.90	1387
48.00	183	61.00	2185	71.70	66	81.80	101

Average of 12.841 to 12.853 min.: VN082063.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
82.00	312	104.10	52	172.00	217		
86.95	1750	105.75	180	172.90	116		
87.85	1362	106.10	116	173.95	18603		
91.05	243	115.80	109	174.90	1165		
92.05	1041	116.85	253	175.95	18281		
93.05	1304	118.00	169	176.90	1058		
93.95	4400	118.90	89	177.90	68		
95.05	32461	128.00	145				
96.00	2048	140.75	135				
97.00	84	141.10	317				
103.70	67	142.90	571				

Instrument :

MSVOA_N

ClientSampleId :

BFB