


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN051120\
 Data File : VN061378.D
 Acq On : 11 May 2020 9:54
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N042720W.M
 Title : SW846 8260
 Last Update : Tue May 05 07:01:08 2020

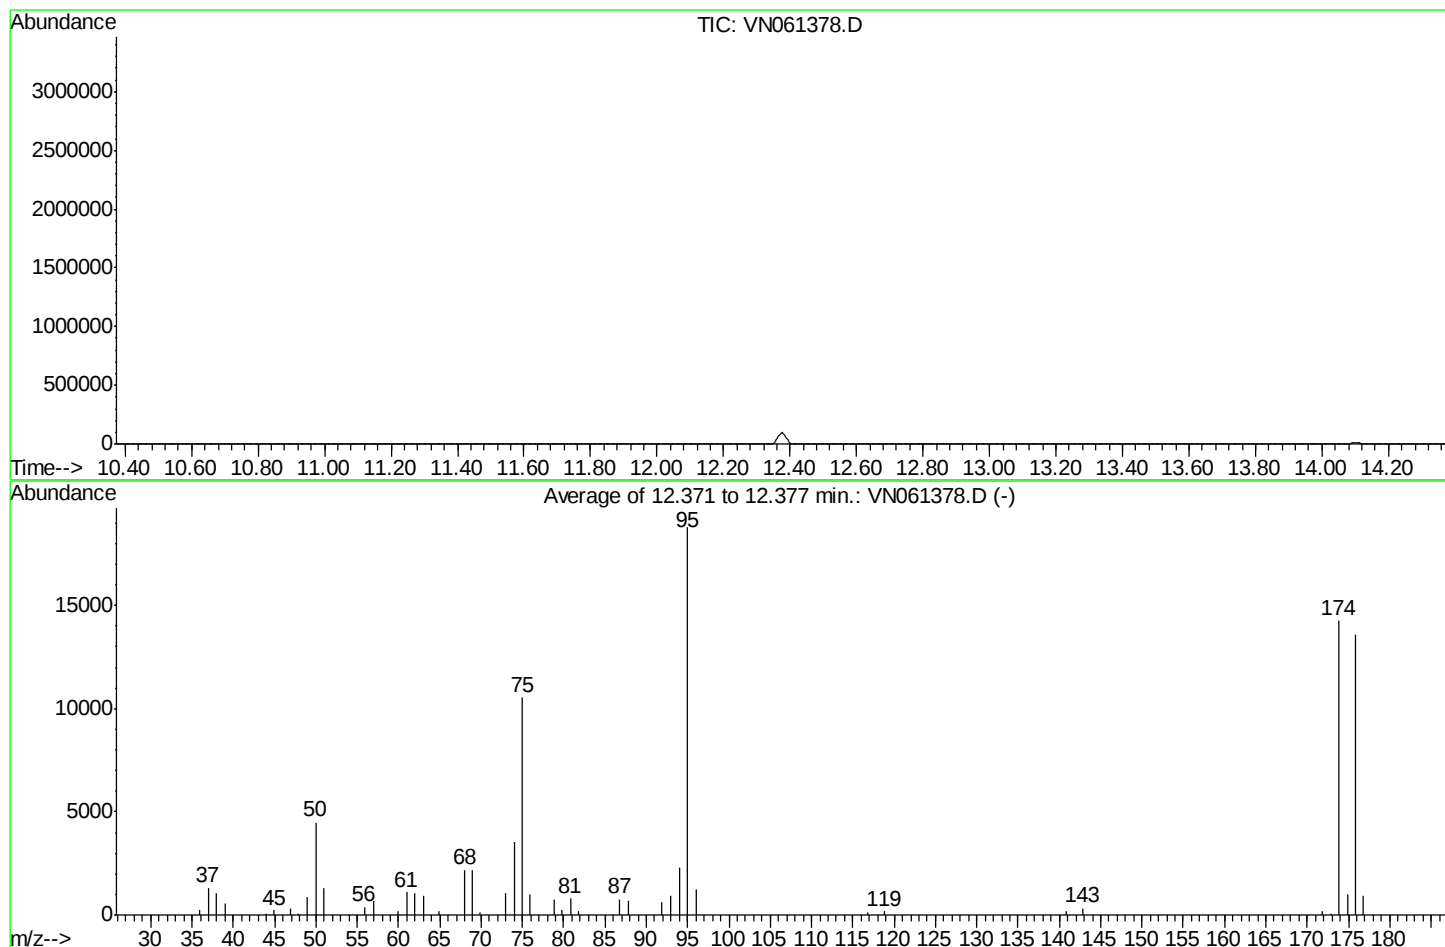

AutoFind: Scans 3353, 3354, 3355; Background Corrected with Scan 3341

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.9	4486	PASS
75	95	30	60	56.1	10534	PASS
95	95	100	100	100.0	18786	PASS
96	95	5	9	6.7	1263	PASS
173	174	0.00	2	0.5	71	PASS
174	95	50	100	75.9	14252	PASS
175	174	5	9	7.2	1023	PASS
176	174	95	101	95.2	13568	PASS
177	176	5	9	6.7	914	PASS