

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051122\
 Data File : VN072440.D
 Acq On : 12 May 2022 01:43
 Operator : JC\MD
 Sample : N2800-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-14D

Quant Time: May 12 02:19:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051022W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 10 15:43:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	200537	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	374820	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	416274	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	185627	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	161881	52.703	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 105.400%			
35) Dibromofluoromethane	8.022	113	118874	47.670	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 95.340%			
50) Toluene-d8	10.440	98	472754	49.778	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 99.560%			
62) 4-Bromofluorobenzene	12.728	95	203121	64.400	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 128.800%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.305	50	564	Below Cal	#	54
5) Bromomethane	2.864	94	349	0.275	ug/l #	66
6) Chloroethane	2.993	64	144	Below Cal	#	42
11) Tert butyl alcohol	5.381	59	1229	2.447	ug/l #	72
13) Acrolein	4.246	56	3556	7.237	ug/l	100
14) Allyl chloride	5.081	41	21999	5.855	ug/l #	65
15) Acrylonitrile	5.622	53	3188	2.336	ug/l #	22
16) Acetone	4.275	43	13044	10.723	ug/l #	64
18) Methyl Acetate	5.075	43	46112	12.875	ug/l #	48
19) Methyl tert-butyl Ether	5.616	73	10479	1.437	ug/l #	1
20) Methylene Chloride	5.087	84	1870	0.750	ug/l #	50
25) 2-Butanone	7.334	43	1494	0.778	ug/l #	45
30) Chloroform	7.810	83	6478	1.478	ug/l	85
31) Cyclohexane	8.093	56	7122	1.750	ug/l #	57
36) 1,1-Dichloropropene	8.081	75	16615	4.639	ug/l #	50
37) Ethyl Acetate	7.334	43	1494	0.348	ug/l #	67
38) Carbon Tetrachloride	8.081	117	21838	5.448	ug/l #	18
39) Methylcyclohexane	9.457	83	2779	0.690	ug/l #	82
40) Benzene	8.457	78	14924	1.395	ug/l #	89
41) Methacrylonitrile	7.834	41	1417	0.666	ug/l #	31
43) Isopropyl Acetate	8.563	43	4842	0.734	ug/l #	53
48) Methyl methacrylate	9.581	41	653	0.212	ug/l #	15
55) 1,1,2-Trichloroethane	10.875	97	2340	0.851	ug/l #	16
58) 2-Chloroethyl Vinyl ether	9.975	63	55	17.389	ug/l #	44
73) Isopropylbenzene	12.575	105	36843	2.396	ug/l	96
76) 1,2,3-Trichloropropane	12.728	75	114397	23.628	ug/l #	1
78) n-propylbenzene	12.922	91	4886	0.297	ug/l	92
81) trans-1,4-Dichloro-2-b...	12.728	75	114397	78.825	ug/l #	11
85) sec-Butylbenzene	13.492	105	6752	0.459	ug/l #	58
89) n-Butylbenzene	13.933	91	4236	0.484	ug/l	87
90) Hexachloroethane	14.210	117	2163	0.945	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	14.322	75	1029	1.060	ug/l #	1
95) Naphthalene	15.498	128	22532	5.555	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_N
ClientSampleId :
MW-14D

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051122\
Data File : VN072440.D
Acq On : 12 May 2022 01:43
Operator : JC\MD
Sample : N2800-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-14D

Quant Time: May 12 02:19:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051022W.M
Quant Title : SW846 8260
QLast Update : Tue May 10 15:43:28 2022
Response via : Initial Calibration




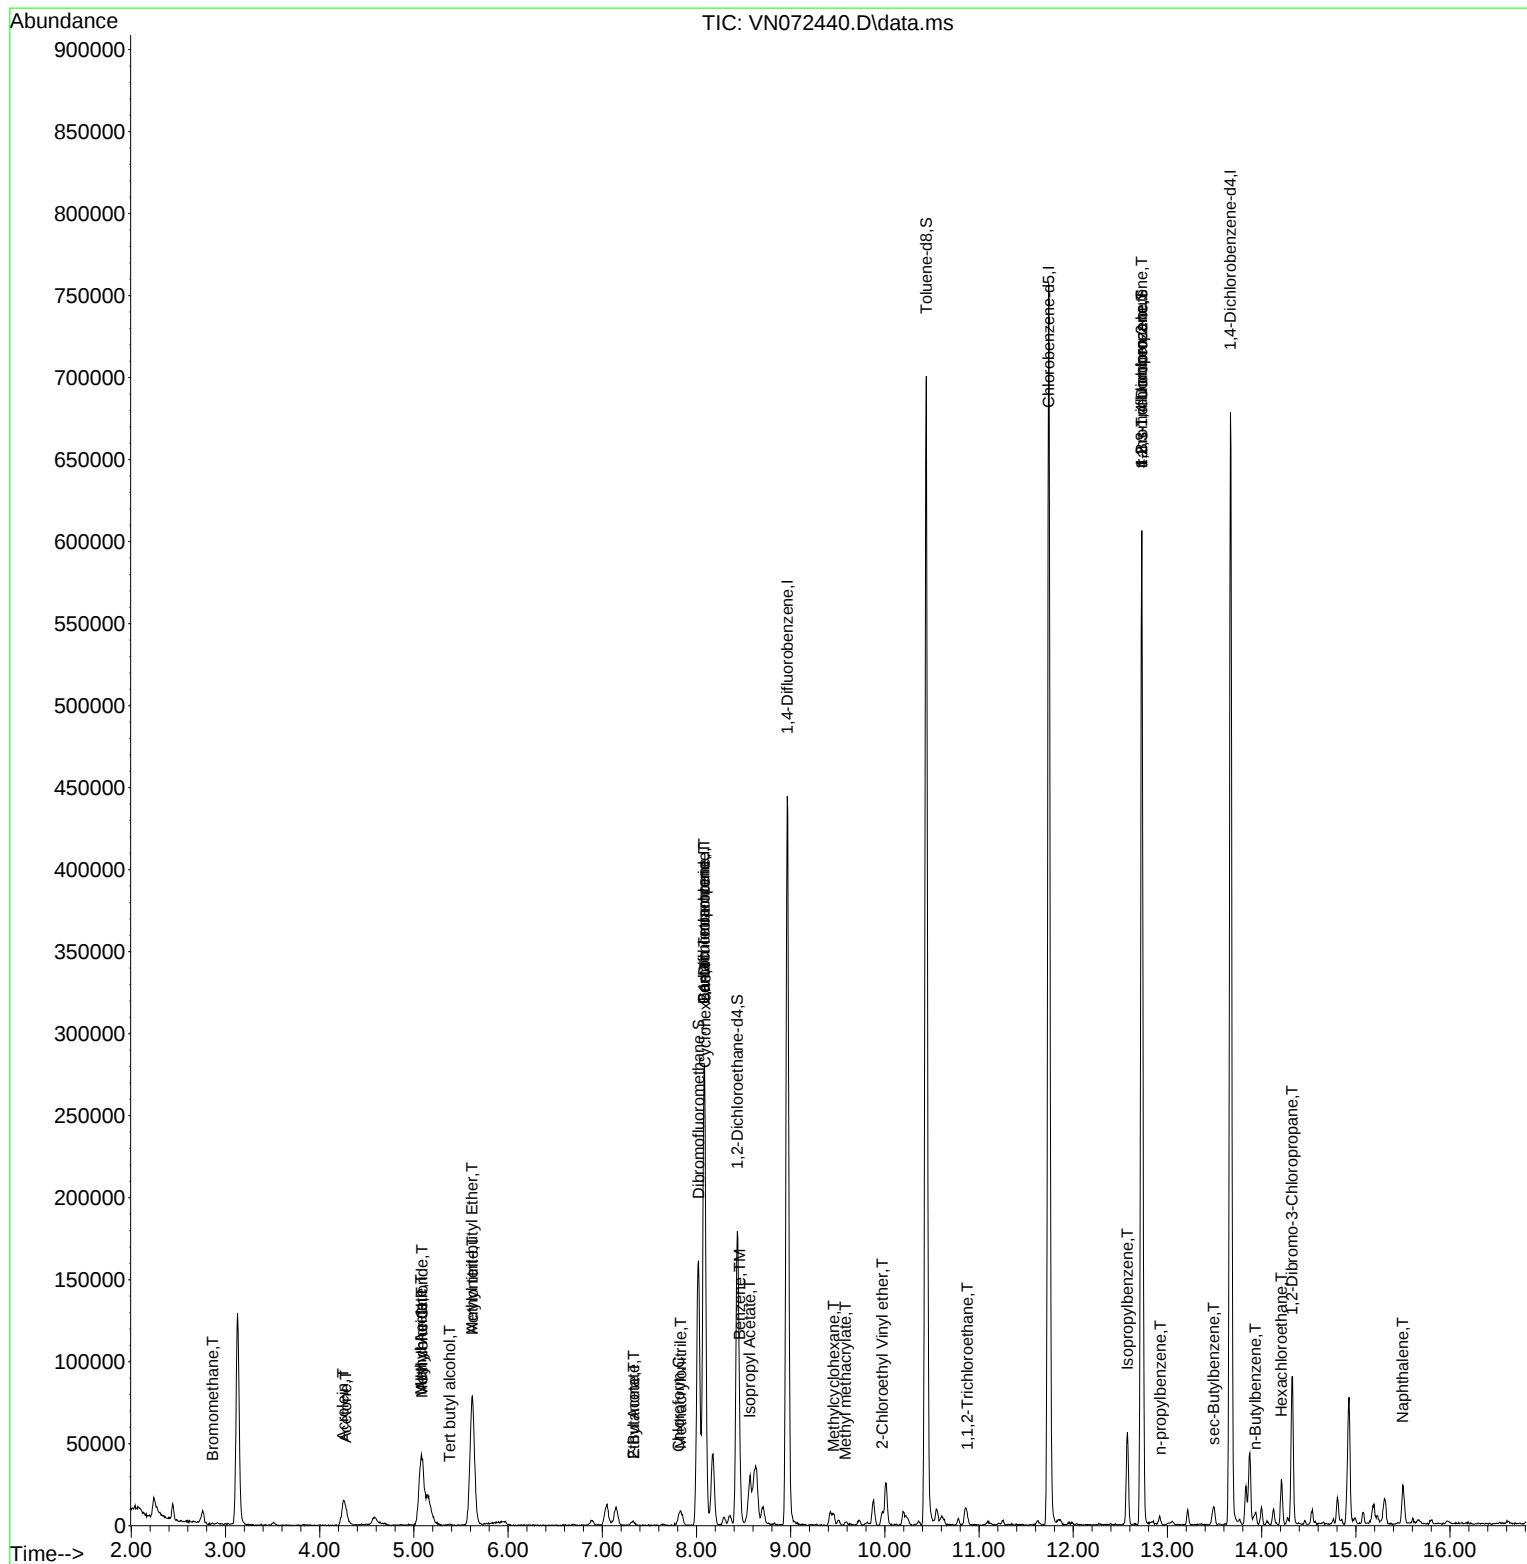




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion:168 Resp: 200537
Ion Ratio Lower Upper
168 100
99 63.0 42.3 63.5

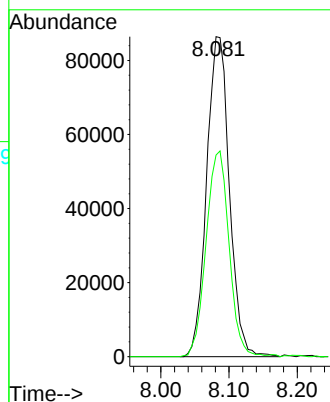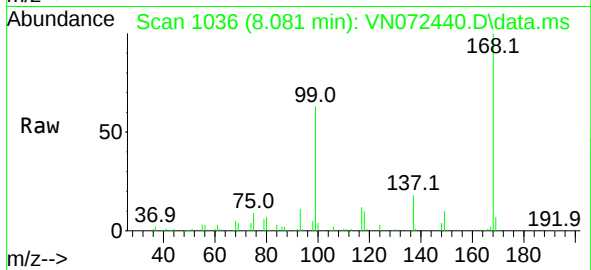

#3
Chloromethane
Concen: Below Cal
RT: 2.305 min Scan# 54
Delta R.T. 0.006 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion: 50 Resp: 564
Ion Ratio Lower Upper
50 100
52 57.8 25.7 38.5#



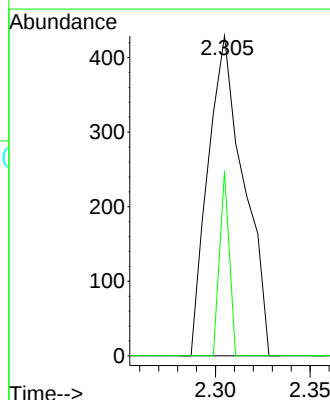
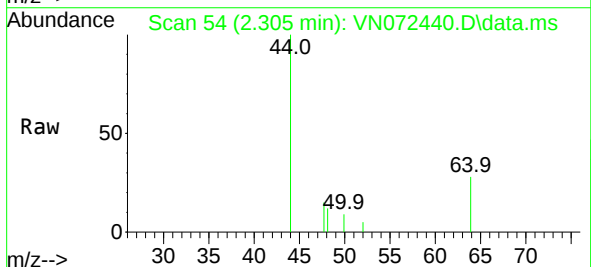




#5
Bromomethane
Concen: 0.275 ug/l
RT: 2.864 min Scan# 149
Delta R.T. 0.036 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion: 94 Resp: 349
Ion Ratio Lower Upper
94 100
96 62.1 76.0 114.0#

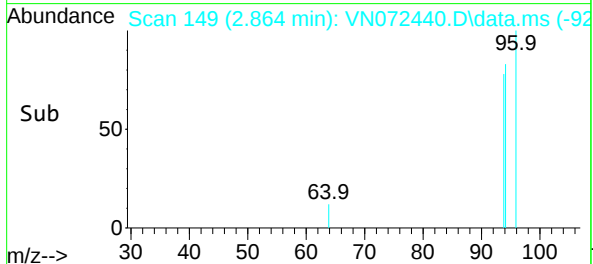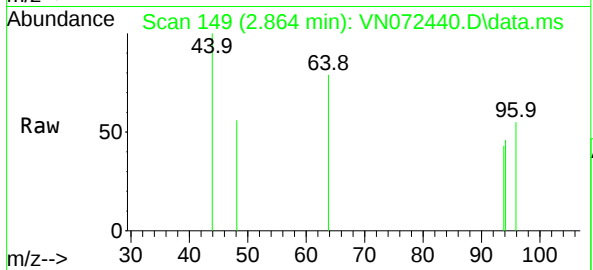

#6
Chloroethane
Concen: Below Cal
RT: 2.993 min Scan# 171
Delta R.T. -0.012 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion: 64 Resp: 144
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#


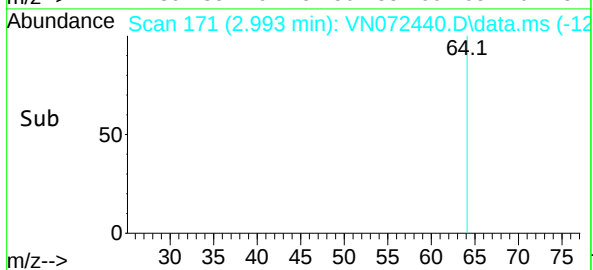

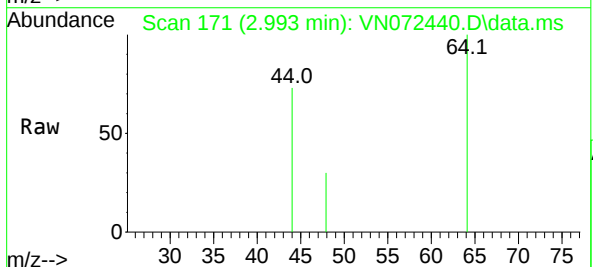




#11
Tert butyl alcohol
Concen: 2.447 ug/l
RT: 5.381 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion: 59 Resp: 1229
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#



#13
Acrolein
Concen: 7.237 ug/l
RT: 4.246 min Scan# 384
Delta R.T. 0.212 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion: 56 Resp: 3556
Ion Ratio Lower Upper
56 100
55 68.8 54.8 82.2



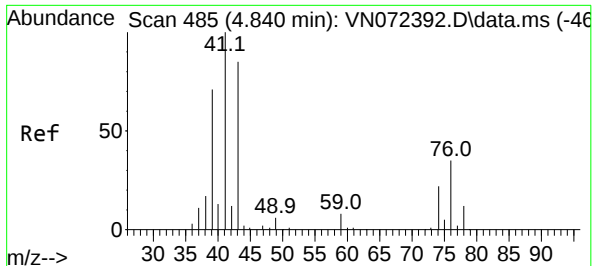

#14

Allyl chloride

Concen: 5.855 ug/l

RT: 5.081 min Scan# 51

Delta R.T. 0.241 min

Lab File: VN072440.D

Acq: 12 May 2022 01:43

Instrument :

MSVOA_N

ClientSampleId :

MW-14D





Tgt Ion: 41 Resp: 21999

Ion Ratio Lower Upper

41 100

39 50.3 53.2 79.8#

76 0.0 29.9 44.9#

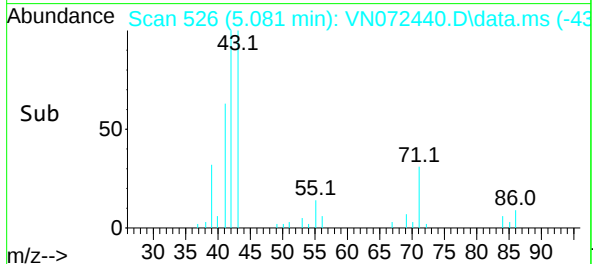

#15

Acrylonitrile

Concen: 2.336 ug/l

RT: 5.622 min Scan# 618

Delta R.T. 0.070 min

Lab File: VN072440.D

Acq: 12 May 2022 01:43




Tgt Ion: 53 Resp: 3188


Ion Ratio Lower Upper

53 100

52 5.0 66.4 99.6#

51 70.3 28.5 42.7#


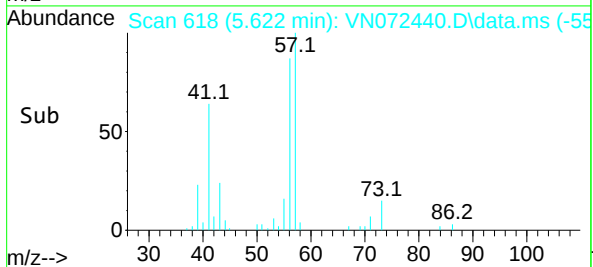

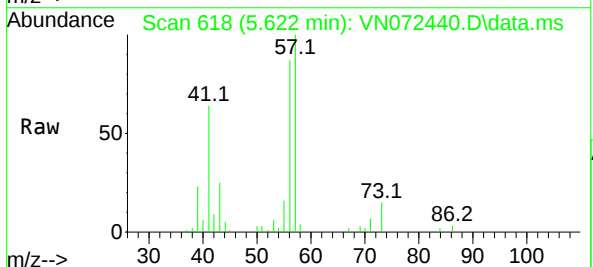




#16
Acetone
Concen: 10.723 ug/l
RT: 4.275 min Scan# 31
Delta R.T. -0.006 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion: 43 Resp: 13044
Ion Ratio Lower Upper
43 100
58 12.3 26.0 39.0#

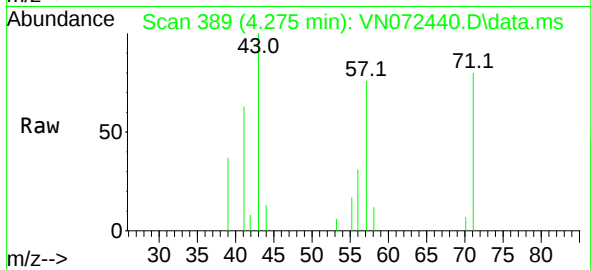

#18
Methyl Acetate
Concen: 12.875 ug/l
RT: 5.075 min Scan# 525
Delta R.T. 0.229 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion: 43 Resp: 46112
Ion Ratio Lower Upper
43 100
74 0.0 21.6 32.4#




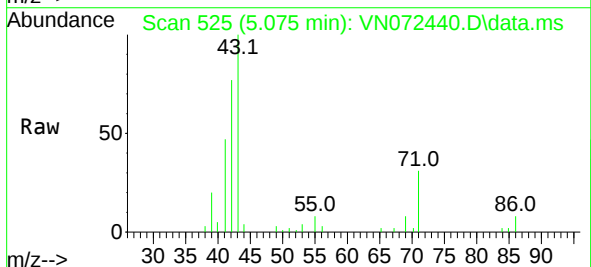




#19
Methyl tert-butyl Ether
Concen: 1.437 ug/l
RT: 5.616 min Scan# 616
Delta R.T. 0.006 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion: 73 Resp: 10479
Ion Ratio Lower Upper
73 100
57 595.4 17.6 26.4#

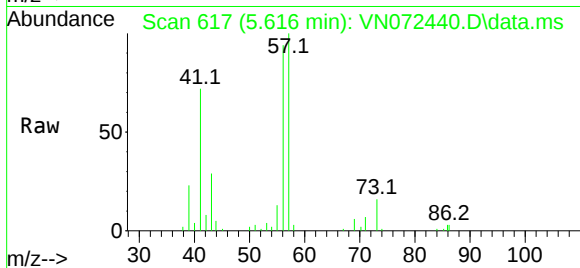

#20
Methylene Chloride
Concen: 0.750 ug/l
RT: 5.087 min Scan# 527
Delta R.T. -0.006 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion: 84 Resp: 1870
Ion Ratio Lower Upper
84 100
49 38.3 88.3 132.5#
51 44.5 28.2 42.2#
86 92.7 50.6 76.0#


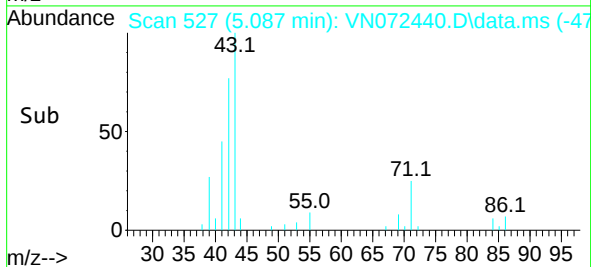

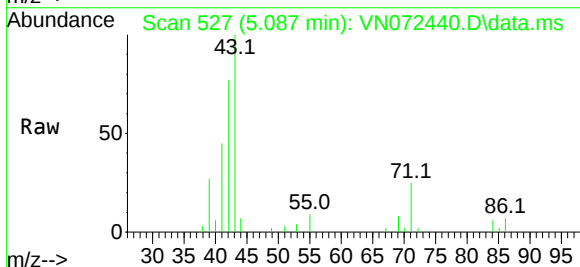




#25
2-Butanone
Concen: 0.778 ug/l
RT: 7.334 min Scan# 909
Delta R.T. 0.006 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion: 43 Resp: 1494
Ion Ratio Lower Upper
43 100
72 0.0 23.7 35.5#

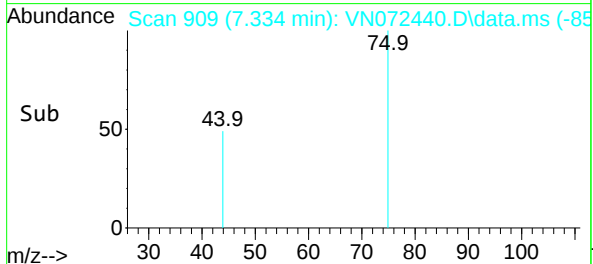

#30
Chloroform
Concen: 1.478 ug/l
RT: 7.810 min Scan# 990
Delta R.T. -0.006 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43


Tgt Ion: 83 Resp: 6478
Ion Ratio Lower Upper
83 100
85 53.3 51.8 77.8

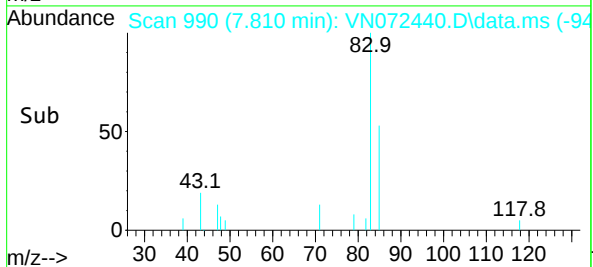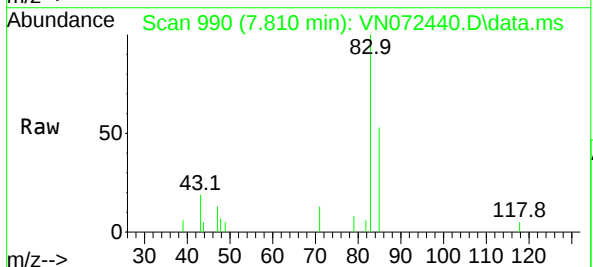



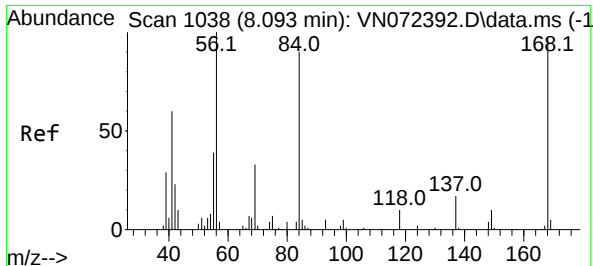


#31
Cyclohexane
Concen: 1.750 ug/l
RT: 8.093 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Instrument :
MSVOA_N
ClientSampleId :
MW-14D







Tgt Ion: 56 Resp: 7122
Ion Ratio Lower Upper
56 100
69 110.7 27.8 41.8#
84 106.9 76.9 115.3

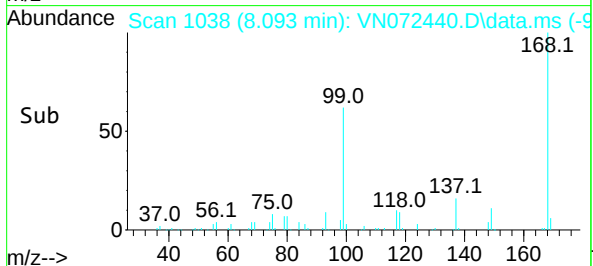

#33
1,2-Dichloroethane-d4
Concen: 52.703 ug/l
RT: 8.434 min Scan# 1096
Delta R.T. -0.000 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion: 65 Resp: 161881
Ion Ratio Lower Upper
65 100
67 47.7 0.0 104.8

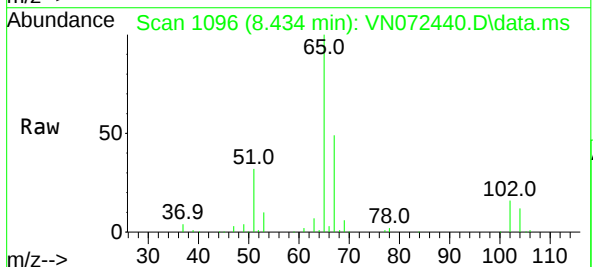

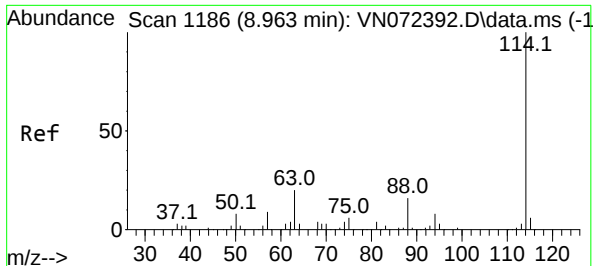

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. 0.000 min

Lab File: VN072440.D

Acq: 12 May 2022 01:43

Instrument :

MSVOA_N

ClientSampleId :

MW-14D





Tgt Ion:114 Resp: 374820

Ion Ratio Lower Upper

114 100

63 20.3 0.0 40.0

88 16.3 0.0 32.6

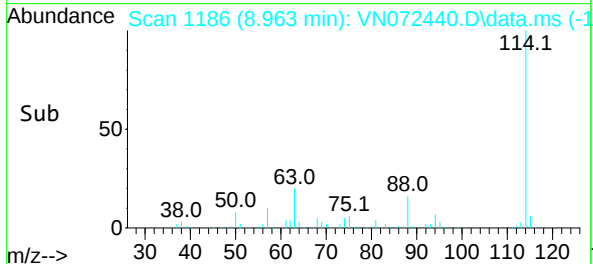

#35

Dibromofluoromethane

Concen: 47.670 ug/l

RT: 8.022 min Scan# 1026

Delta R.T. 0.006 min

Lab File: VN072440.D

Acq: 12 May 2022 01:43




Tgt Ion:113 Resp: 118874


Ion Ratio Lower Upper

113 100

111 102.8 81.4 122.0

192 20.1 17.0 25.6

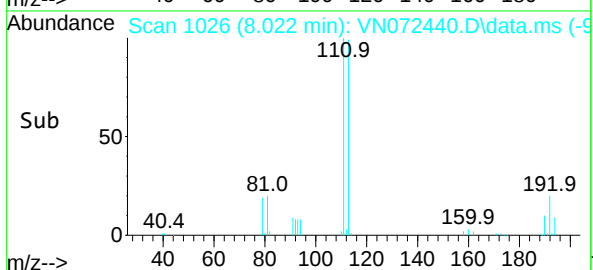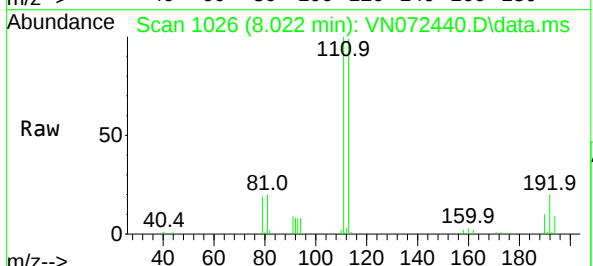

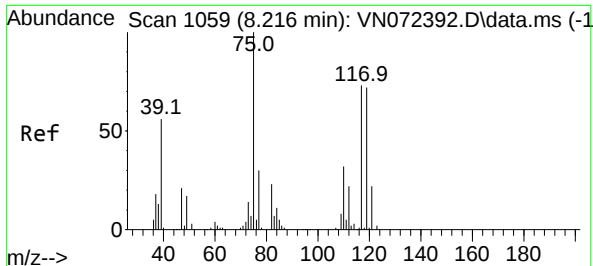

#36

1,1-Dichloropropene

Concen: 4.639 ug/l

RT: 8.081 min Scan# 1

Delta R.T. -0.135 min

Lab File: VN072440.D

Acq: 12 May 2022 01:43

Instrument :

MSVOA_N

ClientSampleId :

MW-14D





Tgt Ion: 75 Resp: 16615

Ion Ratio Lower Upper

75 100

110 10.6 18.3 54.8#

77 0.0 25.1 37.7#

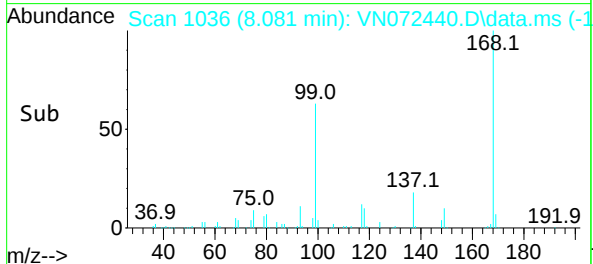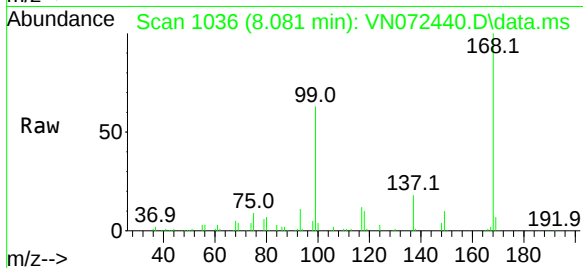

#37

Ethyl Acetate

Concen: 0.348 ug/l

RT: 7.334 min Scan# 909

Delta R.T. -0.070 min

Lab File: VN072440.D

Acq: 12 May 2022 01:43




Tgt Ion: 43 Resp: 1494


Ion Ratio Lower Upper

43 100

61 0.0 11.8 17.6#

70 0.0 9.3 13.9#


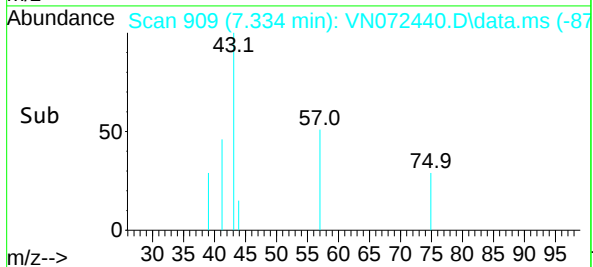

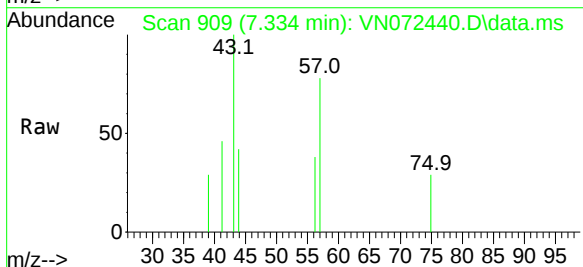




#38
Carbon Tetrachloride
Concen: 5.448 ug/l
RT: 8.081 min Scan# 1057
Delta R.T. -0.123 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion:117 Resp: 21838
Ion Ratio Lower Upper
117 100
119 7.1 75.8 113.8#
121 0.0 24.6 37.0#

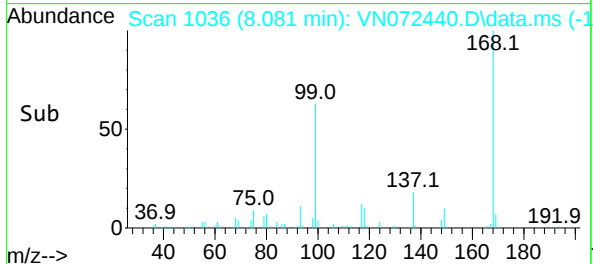

#39
Methylcyclohexane
Concen: 0.690 ug/l
RT: 9.457 min Scan# 1270
Delta R.T. 0.000 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion: 83 Resp: 2779
Ion Ratio Lower Upper
83 100
55 49.3 57.8 86.8#
98 46.1 39.4 59.2


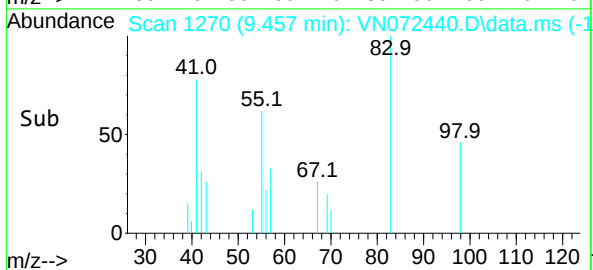

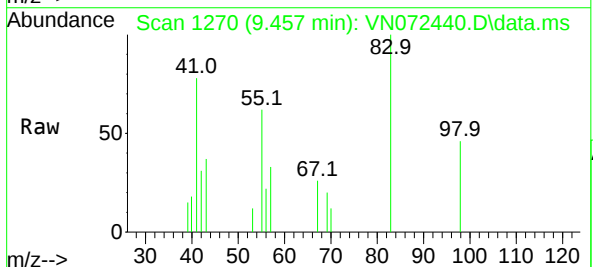




#40
Benzene
Concen: 1.395 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. 0.000 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion: 78 Resp: 14924
Ion Ratio Lower Upper
78 100
77 29.8 19.4 29.0#

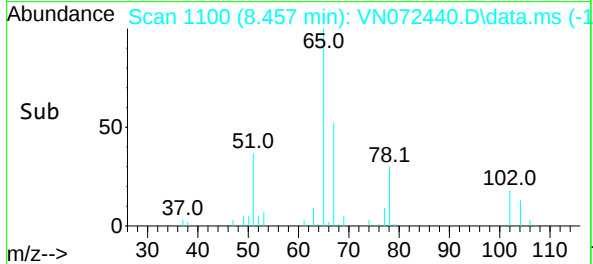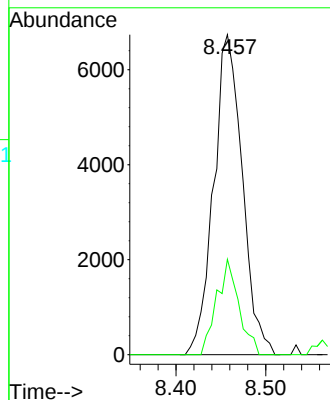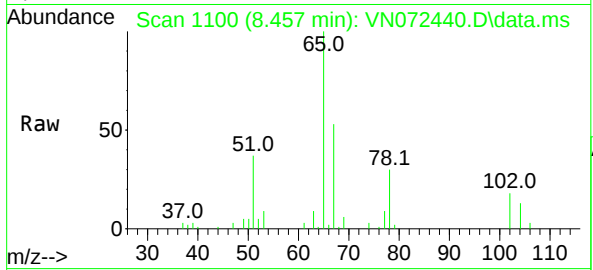

#41
Methacrylonitrile
Concen: 0.666 ug/l
RT: 7.834 min Scan# 994
Delta R.T. 0.206 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion: 41 Resp: 1417
Ion Ratio Lower Upper
41 100
39 35.6 48.6 73.0#
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#

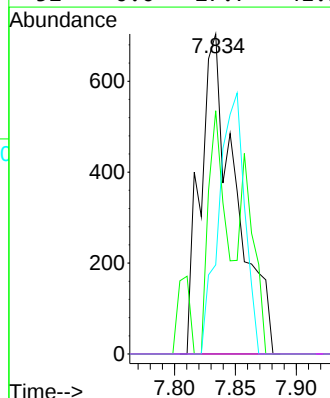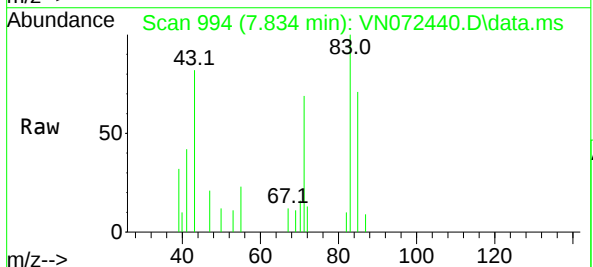

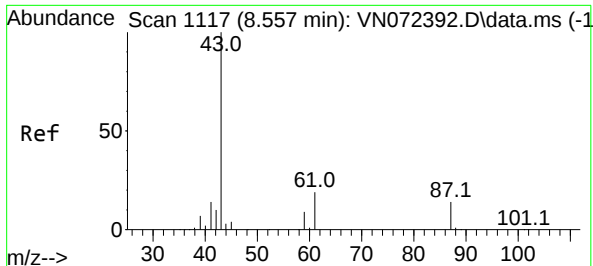

#43

Isopropyl Acetate

Concen: 0.734 ug/l

RT: 8.563 min Scan# 1118

Delta R.T. 0.006 min

Lab File: VN072440.D

Acq: 12 May 2022 01:43

Instrument :

MSVOA_N

ClientSampleId :

MW-14D





Tgt Ion: 43 Resp: 4842

Ion Ratio Lower Upper

43 100

61 0.0 21.9 32.9#

87 0.0 12.0 18.0#

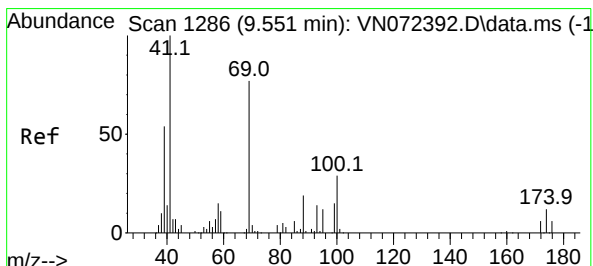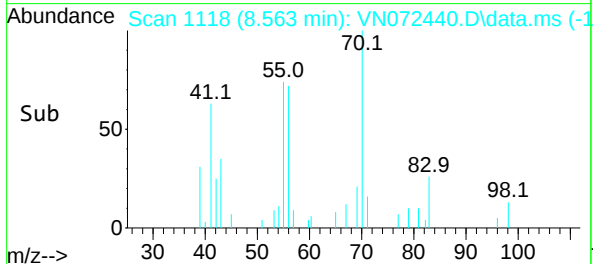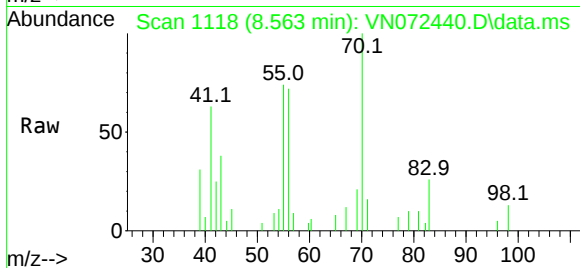

#48

Methyl methacrylate

Concen: 0.212 ug/l

RT: 9.581 min Scan# 1291

Delta R.T. 0.030 min

Lab File: VN072440.D

Acq: 12 May 2022 01:43




Tgt Ion: 41 Resp: 653


Ion Ratio Lower Upper

41 100

69 0.0 74.7 112.1#

39 8.3 45.6 68.4#


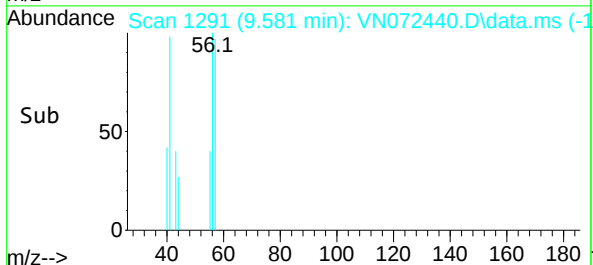

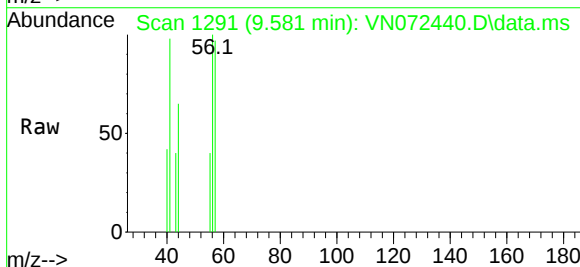




#50
Toluene-d8
Concen: 49.778 ug/l
RT: 10.440 min Scan# 1437
Delta R.T. 0.001 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion: 98 Resp: 472754
Ion Ratio Lower Upper
98 100
100 65.1 52.6 78.8

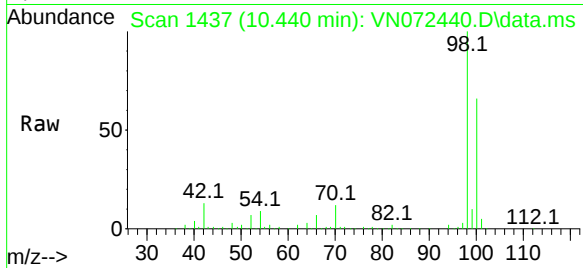

#55
1,1,2-Trichloroethane
Concen: 0.851 ug/l
RT: 10.875 min Scan# 1511
Delta R.T. -0.017 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion: 97 Resp: 2340
Ion Ratio Lower Upper
97 100
83 0.0 66.2 99.4#
85 0.0 43.9 65.9#
99 0.0 50.6 76.0#


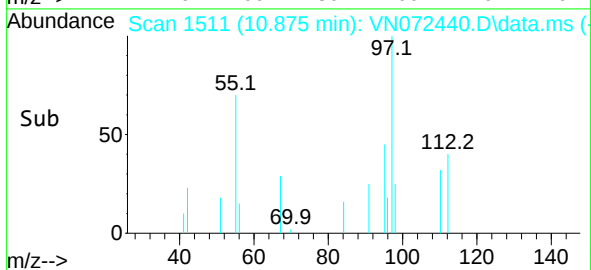

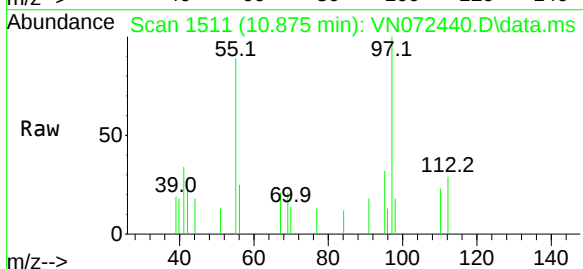




#58
 2-Chloroethyl Vinyl ether
 Concen: 17.389 ug/l
 RT: 9.975 min Scan# 11
 Delta R.T. -0.065 min
 Lab File: VN072440.D
 Acq: 12 May 2022 01:43




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-14D


Tgt Ion: 63 Resp: 55
 Ion Ratio Lower Upper
 63 100
 106 0.0 24.6 36.8#

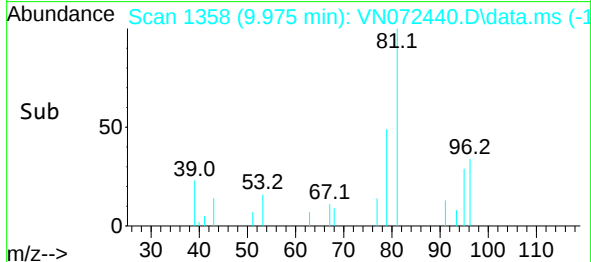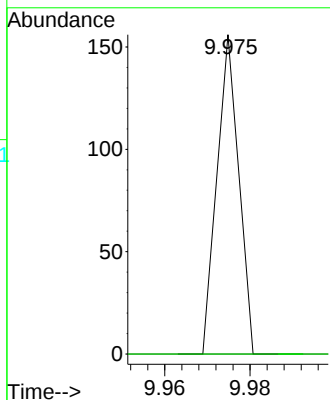

#62
 4-Bromofluorobenzene
 Concen: 64.400 ug/l
 RT: 12.728 min Scan# 1826
 Delta R.T. 0.006 min
 Lab File: VN072440.D
 Acq: 12 May 2022 01:43

Tgt Ion: 95 Resp: 203121
 Ion Ratio Lower Upper
 95 100
 174 78.2 0.0 167.6
 176 76.2 0.0 163.4


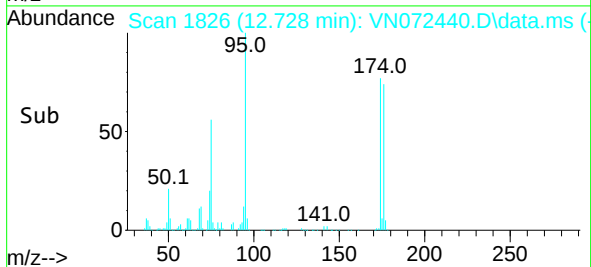
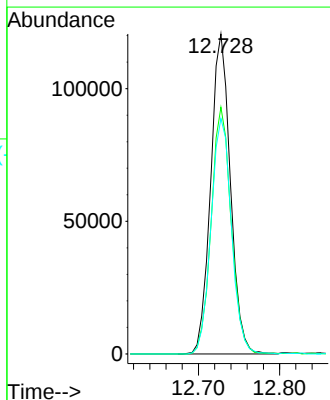
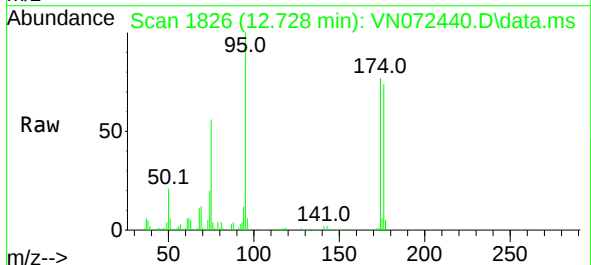




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion:117 Resp: 416274
Ion Ratio Lower Upper
117 100
82 56.7 44.2 66.2
119 33.2 25.4 38.0

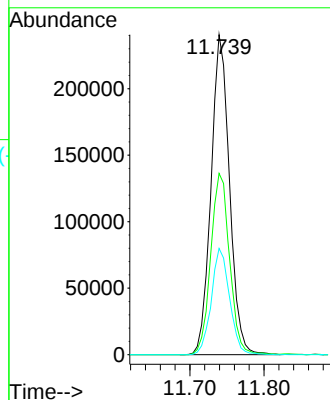

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. -0.000 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion:152 Resp: 185627
Ion Ratio Lower Upper
152 100
115 60.9 28.9 86.7
150 157.1 0.0 356.2

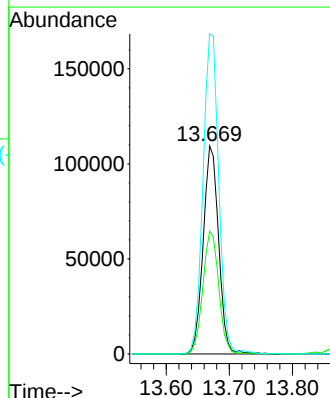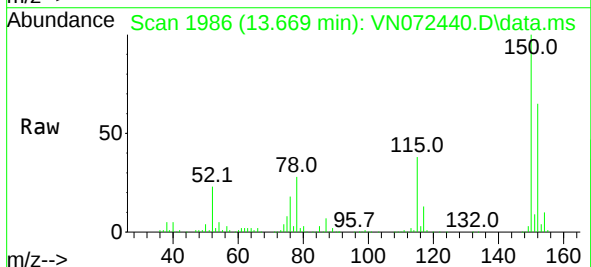



#73

Isopropylbenzene

Concen: 2.396 ug/l

RT: 12.575 min Scan# 1800

Delta R.T. -0.000 min

Lab File: VN072440.D

Acq: 12 May 2022 01:43

Instrument :

MSVOA_N

ClientSampleId :





MW-14D

Tgt Ion:105 Resp: 36843

Ion Ratio Lower Upper

105 100

120 25.0 13.5 40.4

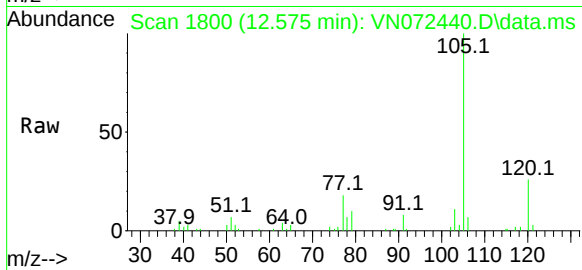

#76

1,2,3-Trichloropropane

Concen: 23.628 ug/l

RT: 12.728 min Scan# 1826

Delta R.T. -0.147 min

Lab File: VN072440.D




Acq: 12 May 2022 01:43


Tgt Ion: 75 Resp: 114397

Ion Ratio Lower Upper

75 100

77 1.3 98.5 295.5#


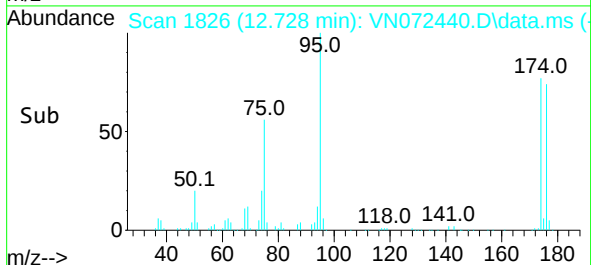

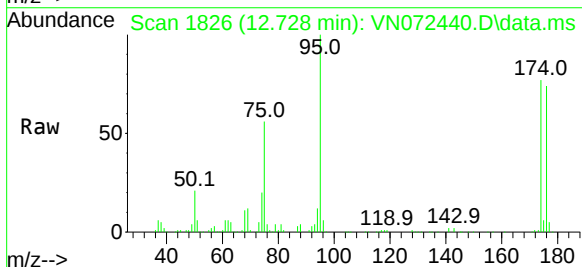




#78
n-propylbenzene
Concen: 0.297 ug/l
RT: 12.922 min Scan# 1859
Delta R.T. 0.006 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43




Instrument :
MSVOA_N
ClientSampleId :
MW-14D


Tgt Ion: 91 Resp: 4886
Ion Ratio Lower Upper
91 100
120 19.9 11.9 35.5

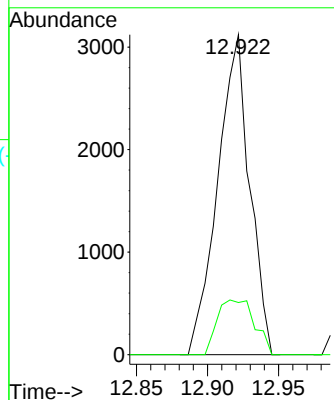

#81
trans-1,4-Dichloro-2-butene
Concen: 78.825 ug/l
RT: 12.728 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Tgt Ion: 75 Resp: 114397
Ion Ratio Lower Upper
75 100
53 0.1 78.0 117.0#
89 0.0 37.2 55.8#


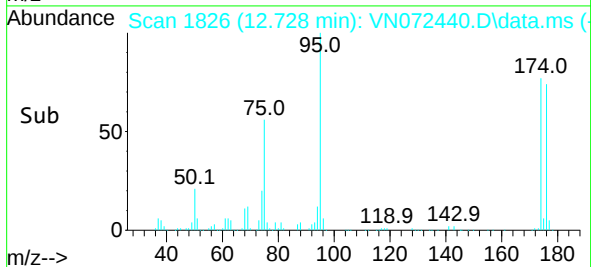
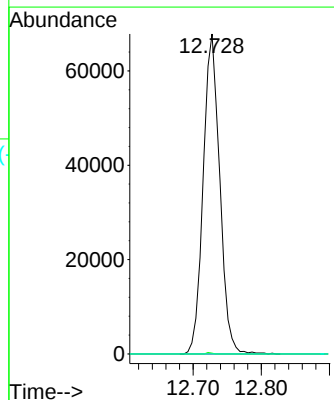
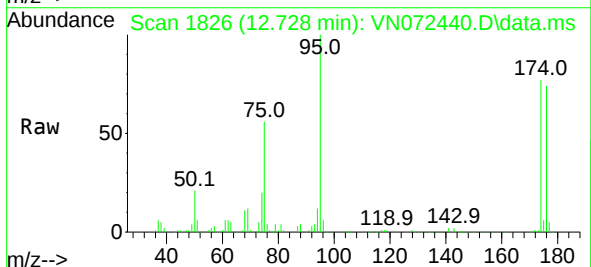




#85
 sec-Butylbenzene
 Concen: 0.459 ug/l
 RT: 13.492 min Scan# 1957
 Delta R.T. -0.006 min
 Lab File: VN072440.D
 Acq: 12 May 2022 01:43




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-14D


Tgt Ion:105 Resp: 6752
 Ion Ratio Lower Upper
 105 100
 134 40.4 10.4 31.1#

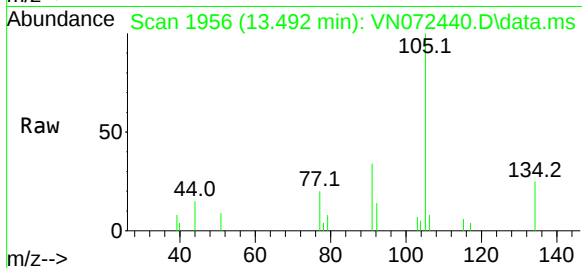

#89
 n-Butylbenzene
 Concen: 0.484 ug/l
 RT: 13.933 min Scan# 2031
 Delta R.T. -0.006 min
 Lab File: VN072440.D
 Acq: 12 May 2022 01:43

Tgt Ion: 91 Resp: 4236
 Ion Ratio Lower Upper
 91 100
 92 46.0 26.9 80.7
 134 17.7 13.6 40.8


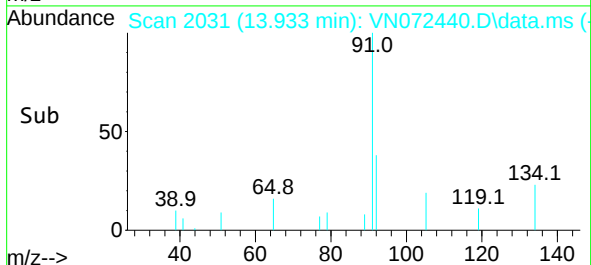

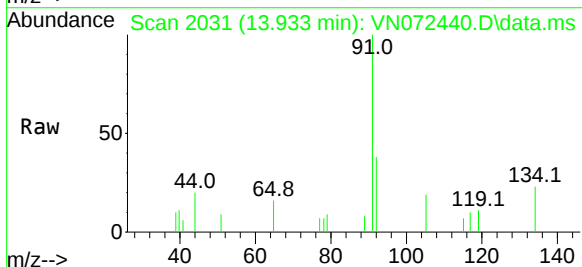




#90
 Hexachloroethane
 Concen: 0.945 ug/l
 RT: 14.210 min Scan# 2077
 Delta R.T. 0.006 min
 Lab File: VN072440.D
 Acq: 12 May 2022 01:43




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-14D


Tgt Ion:117 Resp: 2163
 Ion Ratio Lower Upper
 117 100
 201 0.0 40.6 122.0#

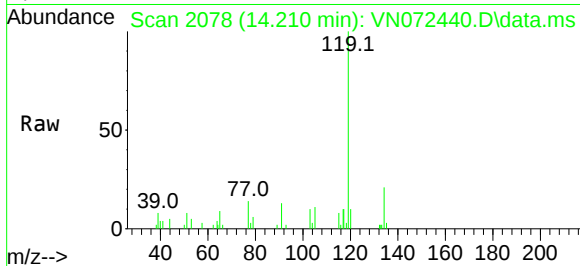

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 1.060 ug/l
 RT: 14.322 min Scan# 2097
 Delta R.T. -0.276 min
 Lab File: VN072440.D
 Acq: 12 May 2022 01:43

Tgt Ion: 75 Resp: 1029
 Ion Ratio Lower Upper
 75 100
 155 0.0 44.9 134.5#
 157 0.0 59.0 176.8#

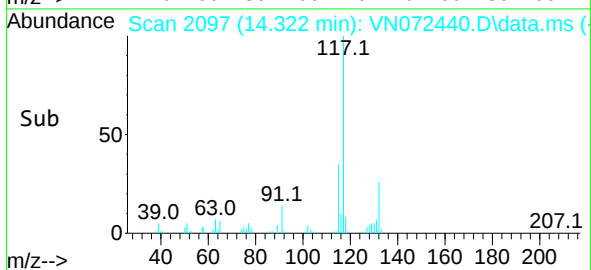

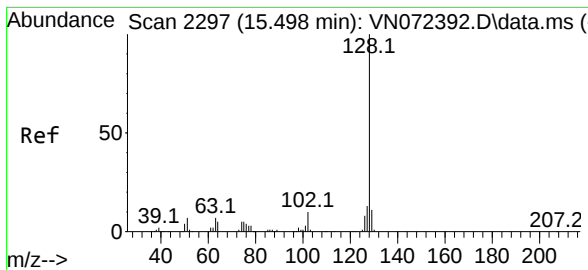

#95
Naphthalene
Concen: 5.555 ug/l
RT: 15.498 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN072440.D
Acq: 12 May 2022 01:43

Instrument :
MSVOA_N
ClientSampleId :
MW-14D

Tgt Ion:	128	Resp:	22532
Ion	Ratio	Lower	Upper
128	100		
127	13.9	10.3	15.5
129	12.4	8.6	13.0

