


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN051122\
Data File : VN072432.D
Acq On : 11 May 2022 21:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051022W.M
Title : SW846 8260
Last Update : Tue May 10 15:43:28 2022

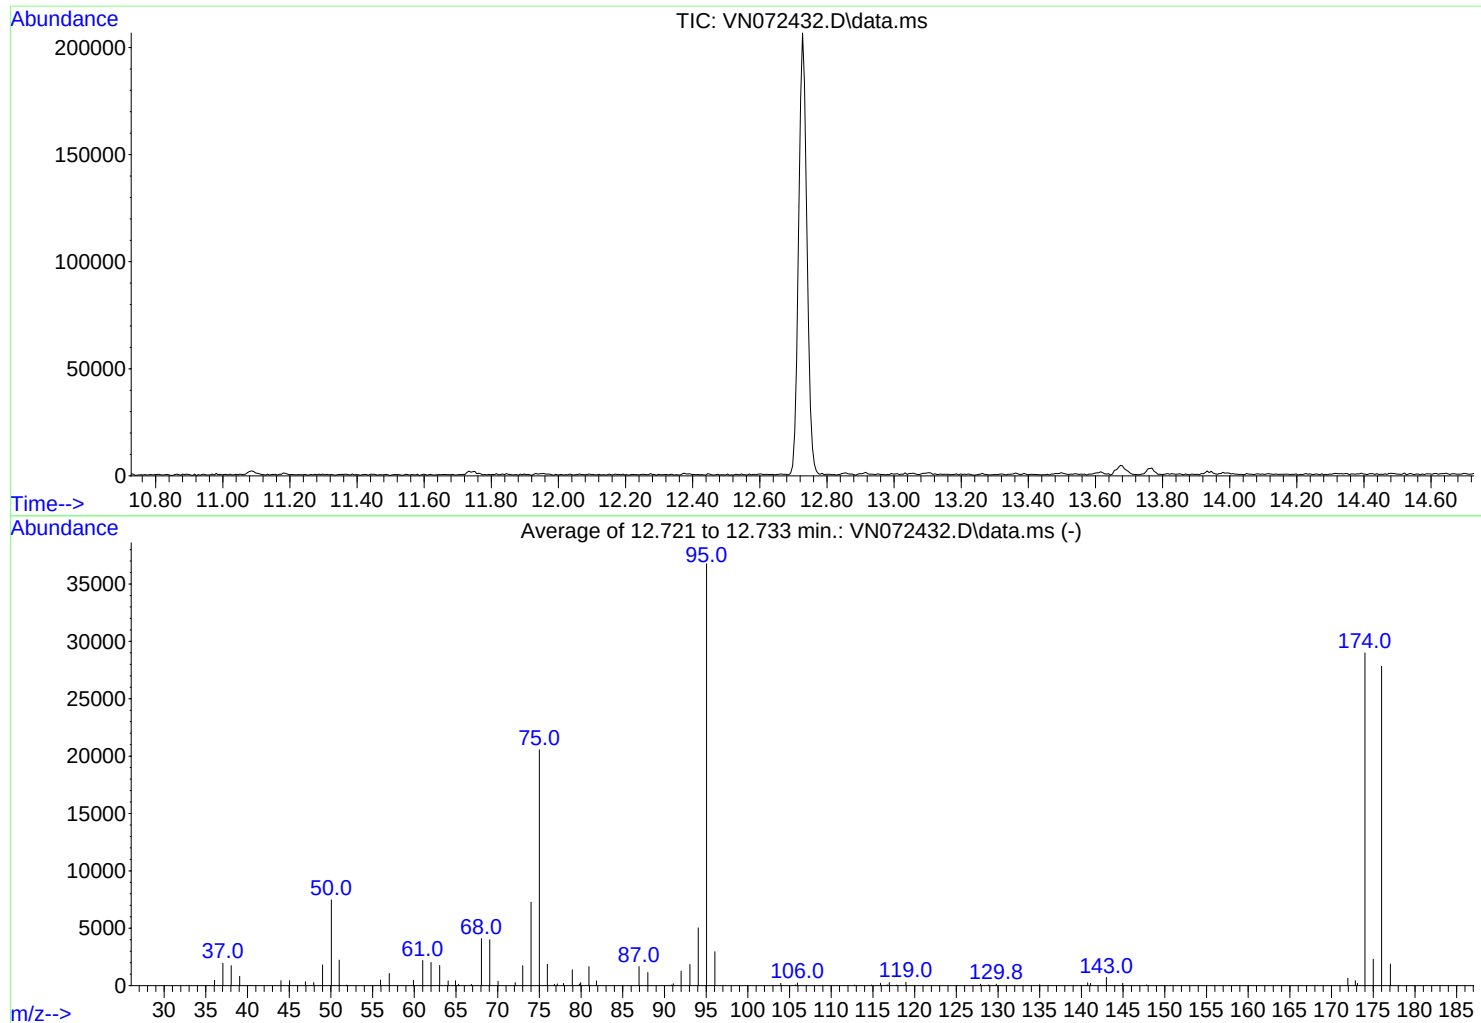

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	7481	PASS
75	95	30	60	55.9	20547	PASS
95	95	100	100	100.0	36757	PASS
96	95	5	9	8.0	2953	PASS
173	174	0.00	2	1.5	432	PASS
174	95	50	100	78.9	29008	PASS
175	174	5	9	7.9	2305	PASS
176	174	95	101	96.0	27837	PASS
177	176	5	9	6.7	1878	PASS